

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051322\
 Data File : VX028712.D
 Acq On : 14 May 2022 05:17
 Operator : JC/MD
 Sample : PB144804TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB144804TB

Quant Time: May 16 02:34:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	241313	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	450675	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	500556	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	190172	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	178116	53.847	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 107.700%	
35) Dibromofluoromethane	5.391	113	147704	50.022	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 100.040%	
50) Toluene-d8	8.653	98	552744	49.652	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 99.300%	
62) 4-Bromofluorobenzene	11.079	95	220208	52.960	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 105.920%	
Target Compounds						
						Qvalue
16) Acetone	2.373	43	40425	28.475	ug/l	95
20) Methylene Chloride	2.788	84	10984	3.688	ug/l #	82
43) Isopropyl Acetate	6.348	43	22905	3.161	ug/l #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051322\
Data File : VX028712.D
Acq On : 14 May 2022 05:17
Operator : JC/MD
Sample : PB144804TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB144804TB

Quant Time: May 16 02:34:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration



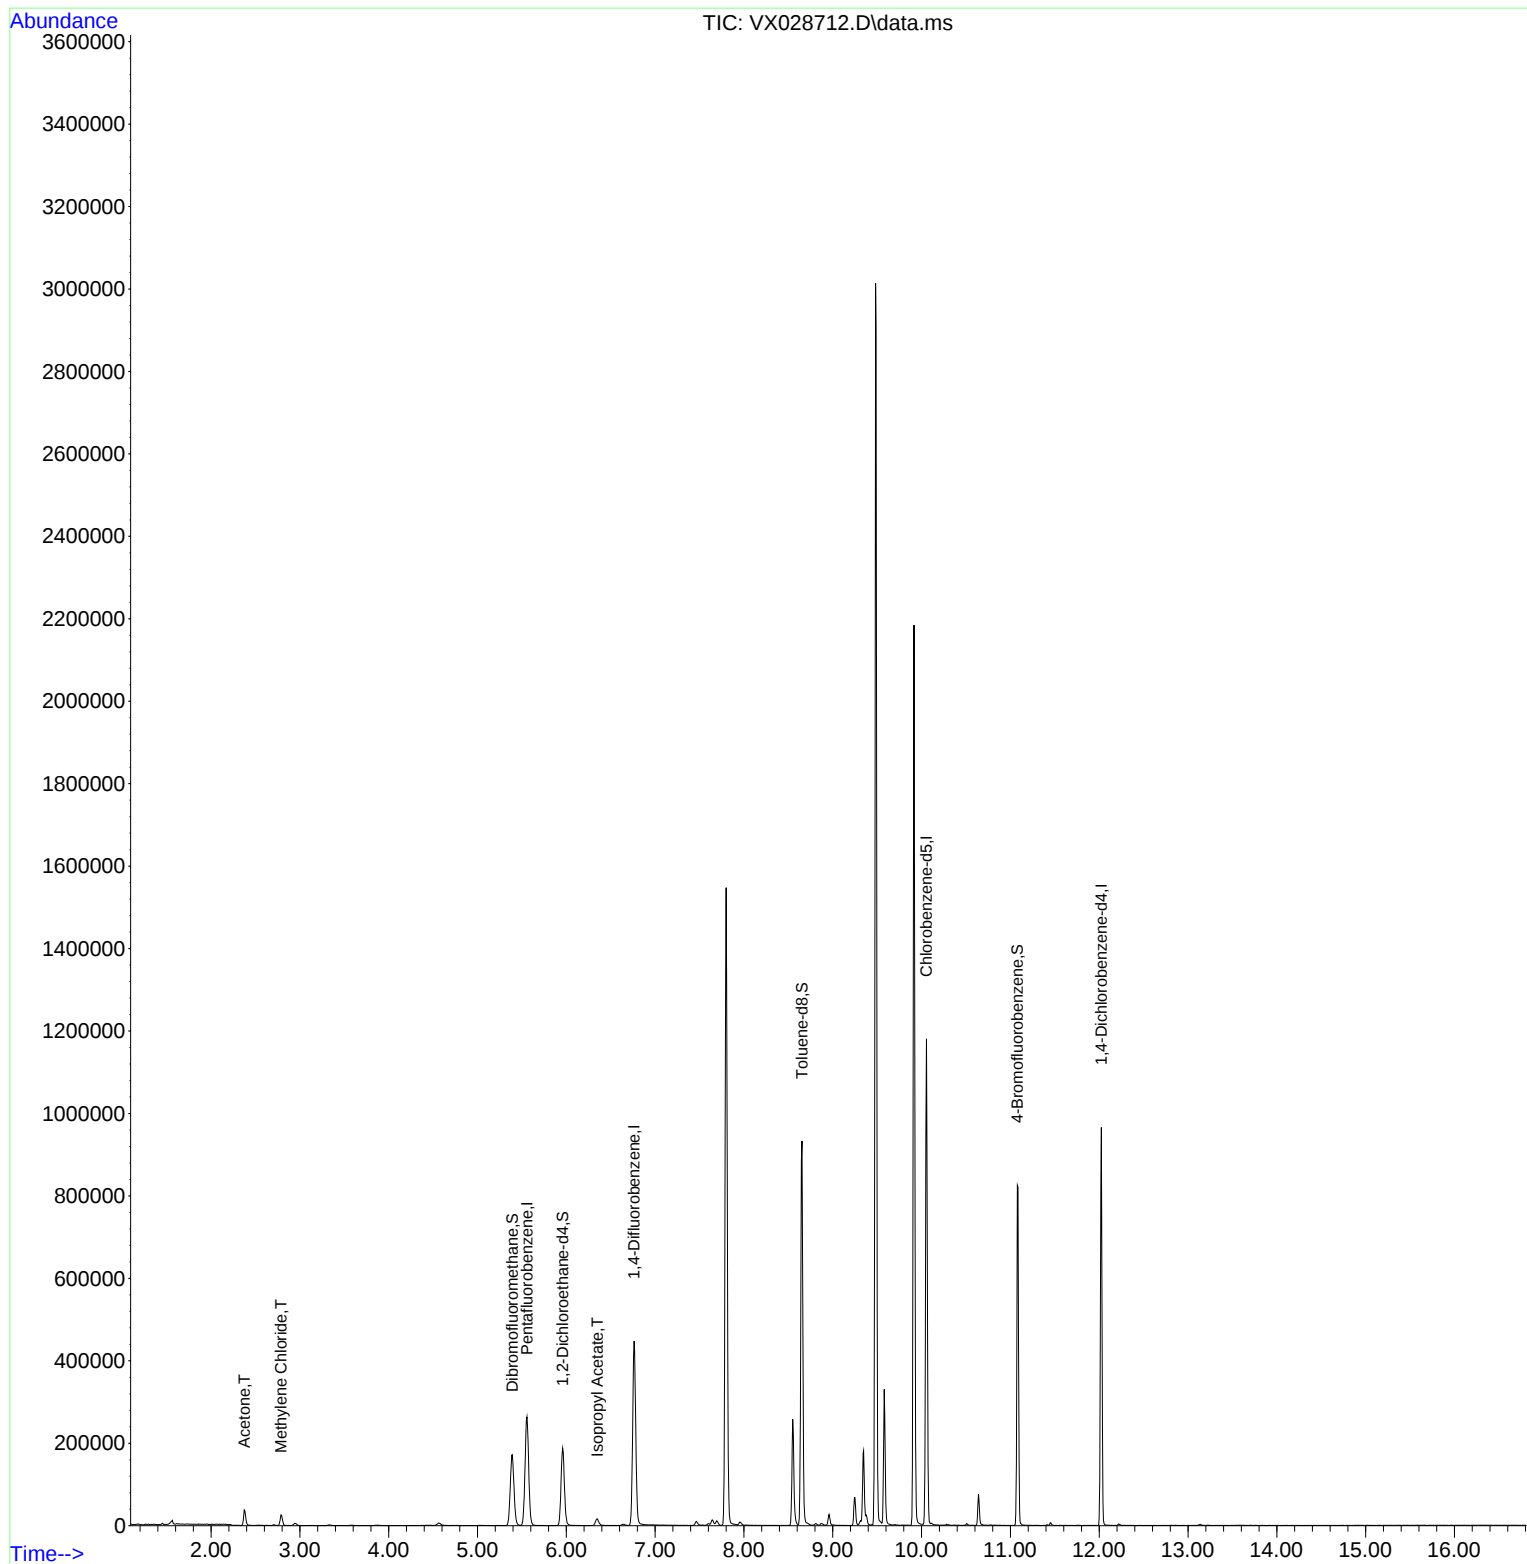




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17




Instrument :
MSVOA_X
ClientSampleId :
PB144804TB


Tgt Ion:168 Resp: 241313
Ion Ratio Lower Upper
168 100
99 61.7 41.7 62.5

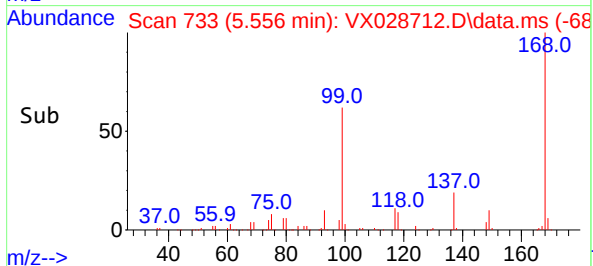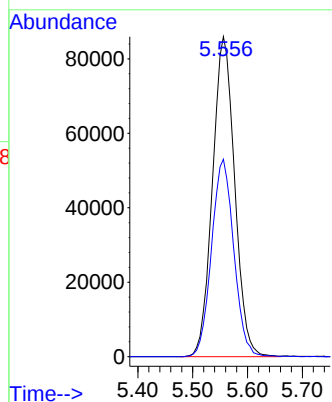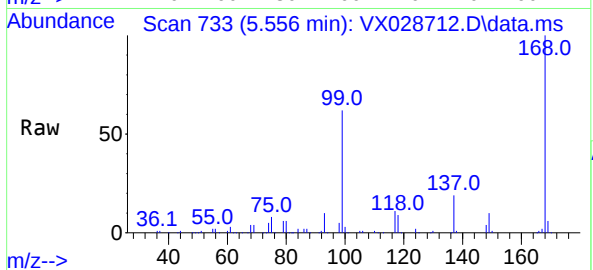

#16
Acetone
Concen: 28.475 ug/l
RT: 2.373 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17

Tgt Ion: 43 Resp: 40425
Ion Ratio Lower Upper
43 100
58 33.3 28.8 43.2

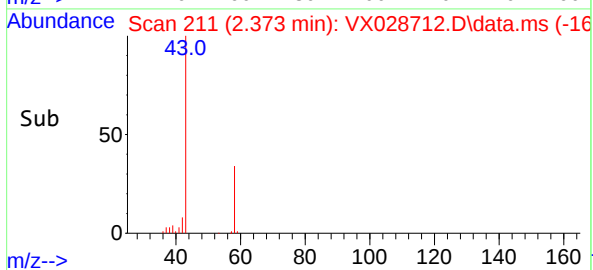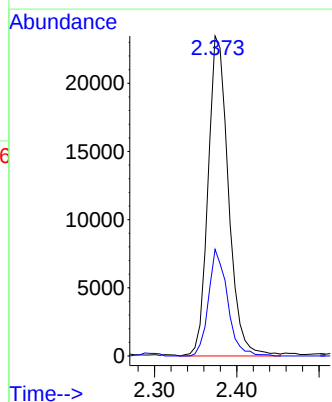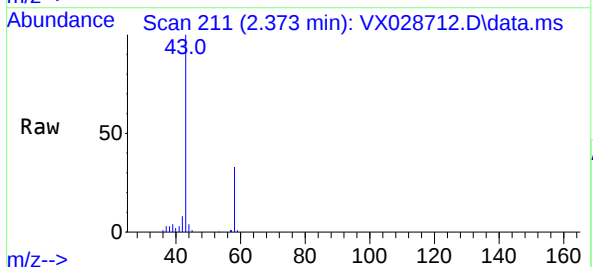




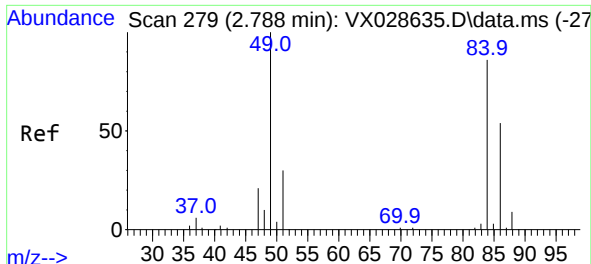


#20
Methylene Chloride
Concen: 3.688 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17

Instrument :
MSVOA_X
ClientSampleId :
PB144804TB

Tgt Ion: 84 Resp: 10984




Ion	Ratio	Lower	Upper
84	100		
49	136.4	85.5	128.3#
51	38.9	26.6	39.8
86	60.1	51.5	77.3

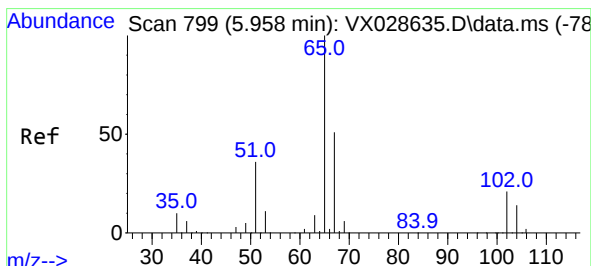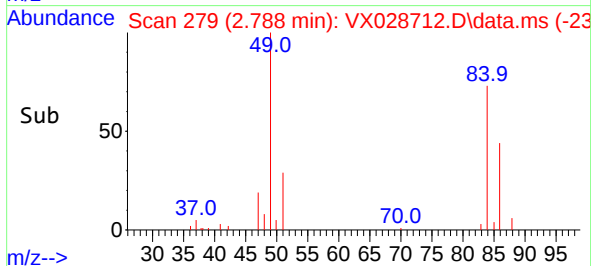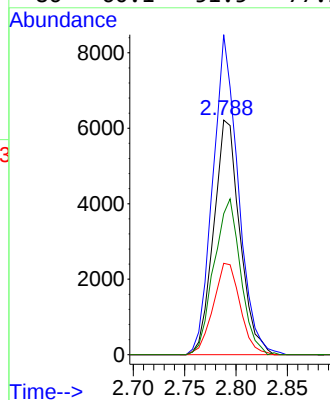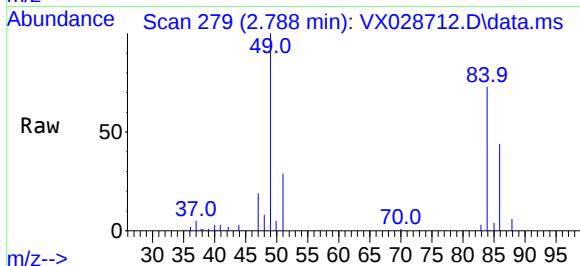


#33
1,2-Dichloroethane-d4
Concen: 53.847 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17

Tgt Ion: 65 Resp: 178116

Ion	Ratio	Lower	Upper
65	100		
67	52.2	0.0	107.4


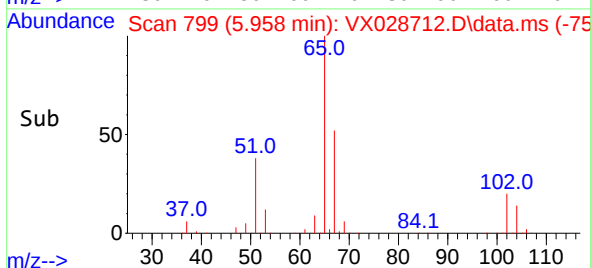
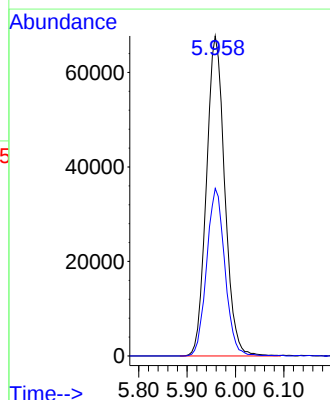
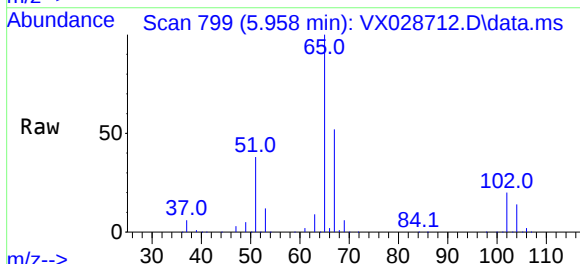


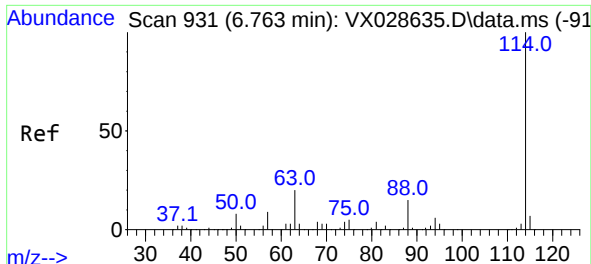

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17




Instrument :
MSVOA_X
ClientSampleId :
PB144804TB


Tgt Ion:114 Resp: 450675
Ion Ratio Lower Upper
114 100
63 20.2 0.0 36.8
88 16.3 0.0 32.4

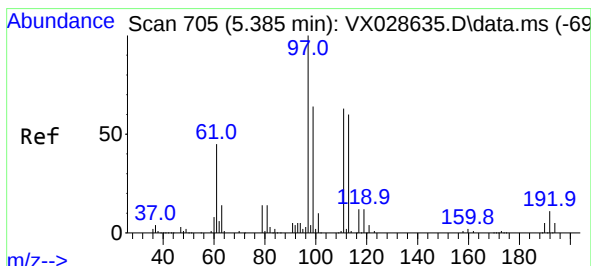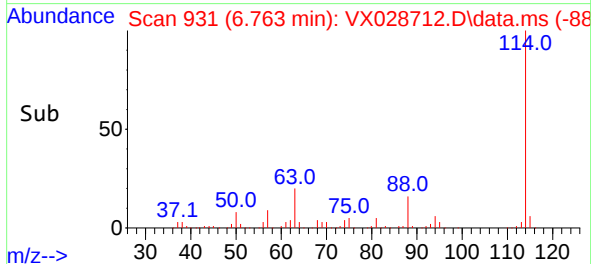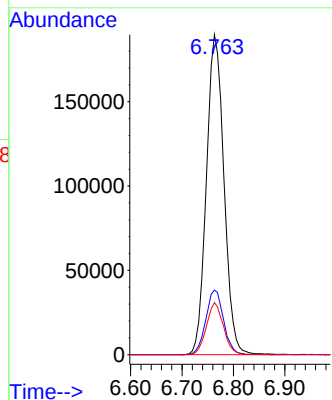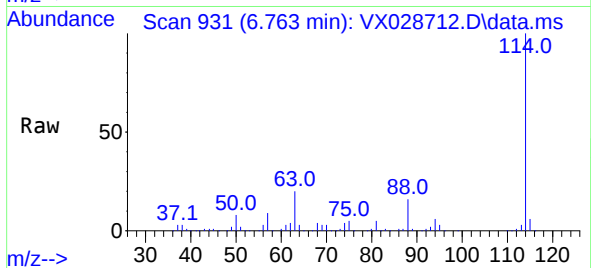

#35
Dibromofluoromethane
Concen: 50.022 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17

Tgt Ion:113 Resp: 147704
Ion Ratio Lower Upper
113 100
111 103.9 82.8 124.2
192 18.1 16.9 25.3


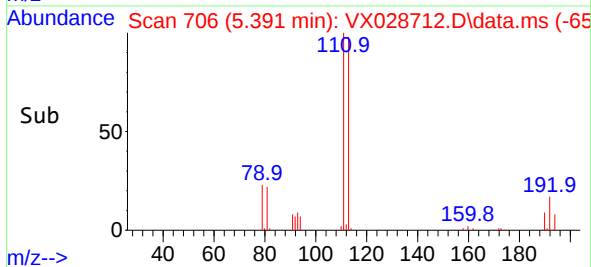
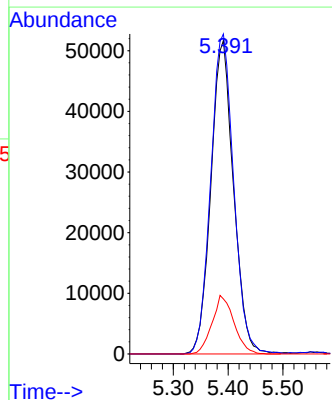
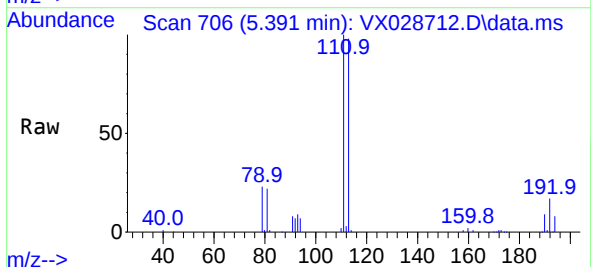


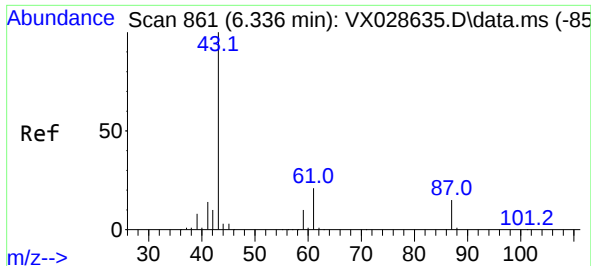

#43
Isopropyl Acetate
Concen: 3.161 ug/l
RT: 6.348 min Scan# 80
Delta R.T. 0.012 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17




Instrument :
MSVOA_X
ClientSampleId :
PB144804TB

Tgt Ion: 43 Resp: 22905
Ion Ratio Lower Upper
43 100
61 17.0 18.5 27.7#
87 14.4 13.0 19.6

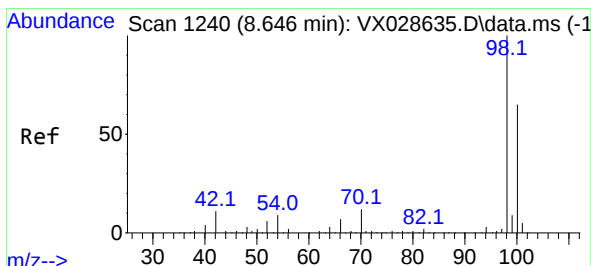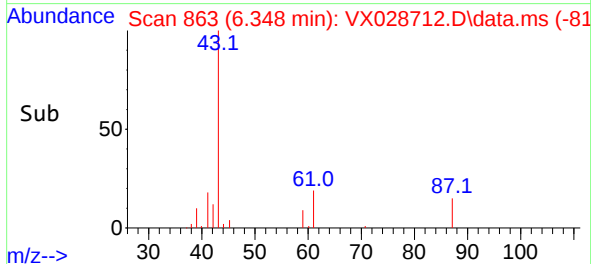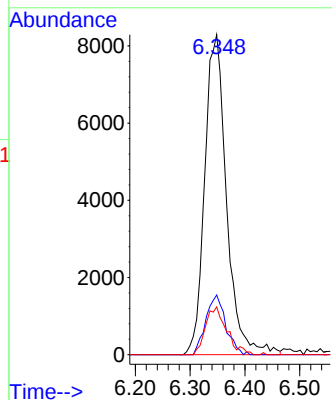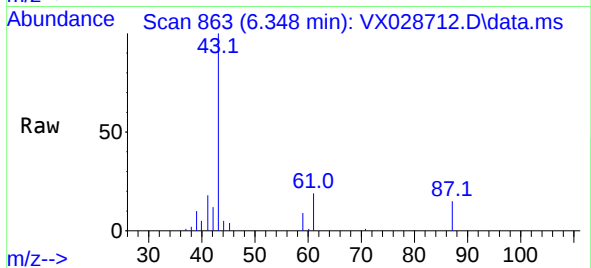

#50
Toluene-d8
Concen: 49.652 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.007 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17

Tgt Ion: 98 Resp: 552744
Ion Ratio Lower Upper
98 100
100 65.9 52.6 78.8


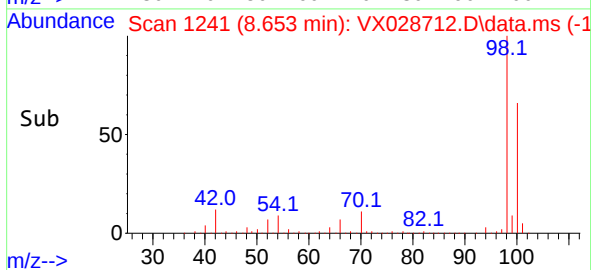
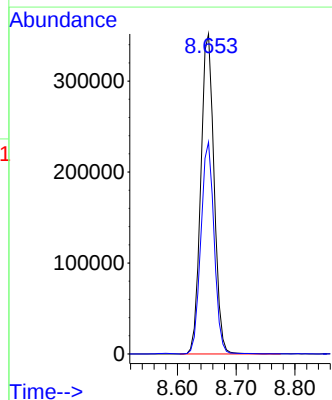
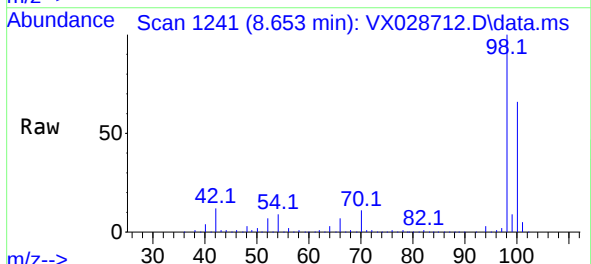




#62
4-Bromofluorobenzene
Concen: 52.960 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17




Instrument :
MSVOA_X
ClientSampleId :
PB144804TB


Tgt Ion: 95 Resp: 220208
Ion Ratio Lower Upper
95 100
174 75.6 0.0 163.0
176 73.2 0.0 155.0

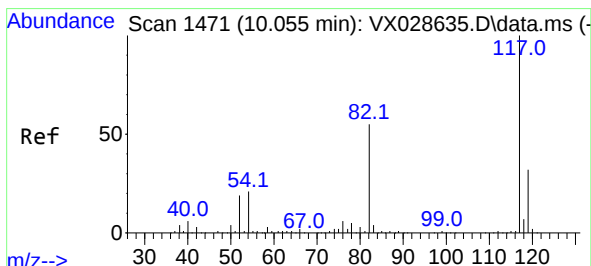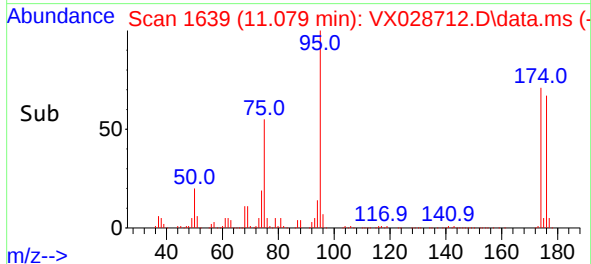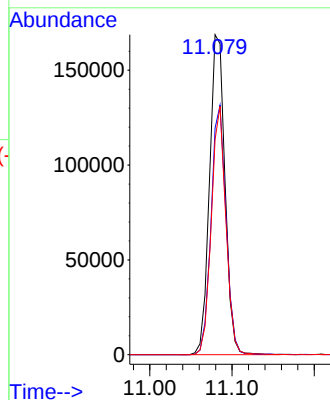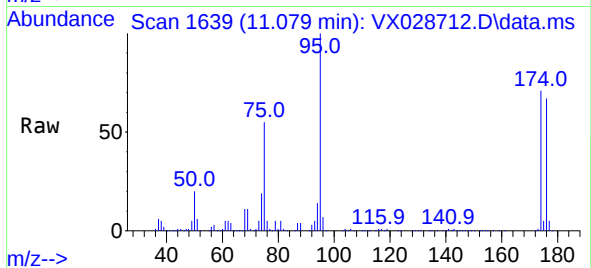

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028712.D
Acq: 14 May 2022 05:17

Tgt Ion: 117 Resp: 500556
Ion Ratio Lower Upper
117 100
82 56.3 41.8 62.8
119 31.6 24.8 37.2

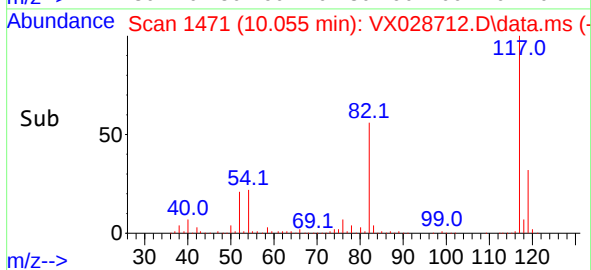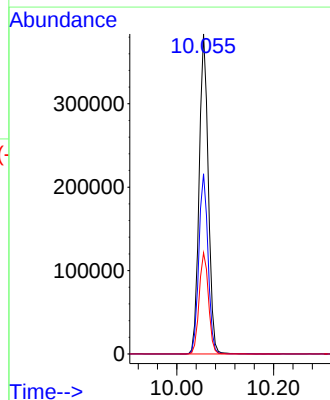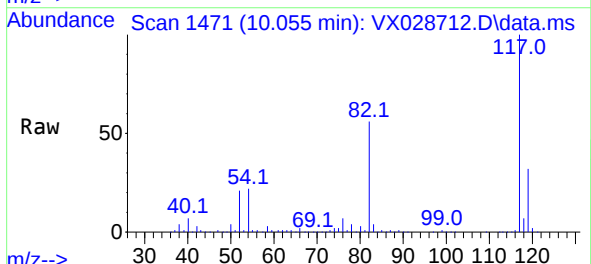

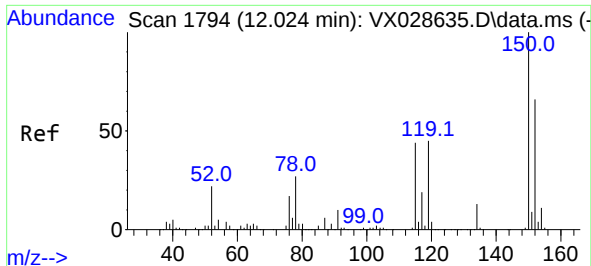

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX028712.D
 Acq: 14 May 2022 05:17

Instrument :
 MSVOA_X
 ClientSampleId :
 PB144804TB

Tgt Ion:152 Resp: 190172
 Ion Ratio Lower Upper
 152 100
 115 61.3 37.5 112.7
 150 156.6 0.0 338.2

