
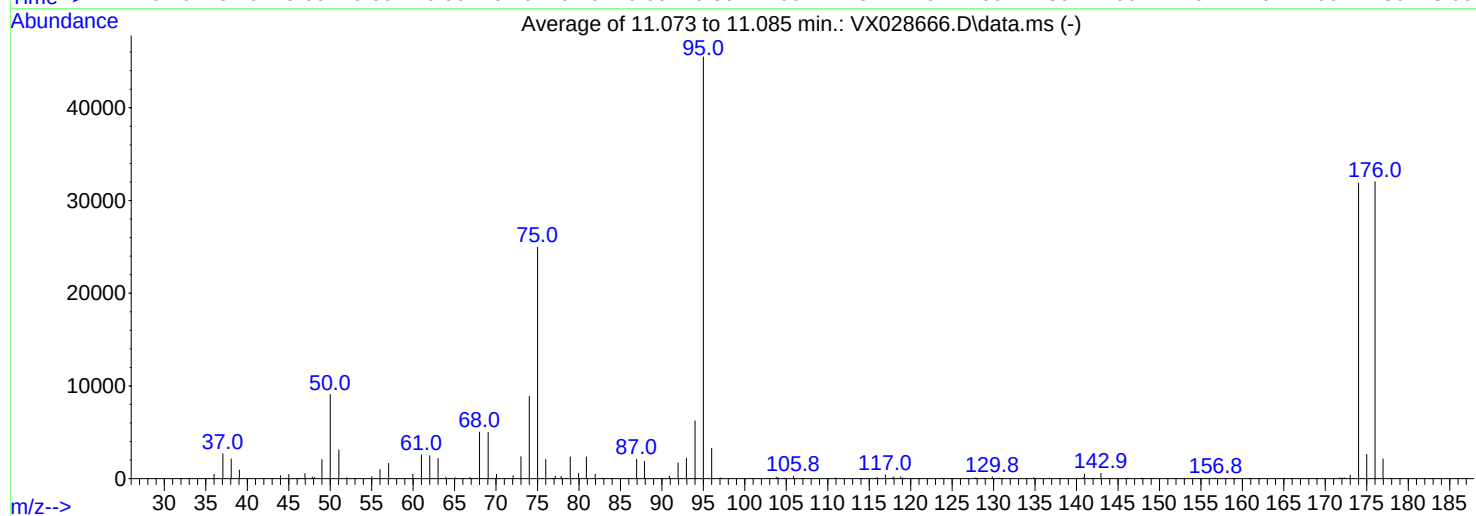


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051322\
 Data File : VX028666.D
 Acq On : 13 May 2022 09:40
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260
 Last Update : Thu May 12 14:58:53 2022

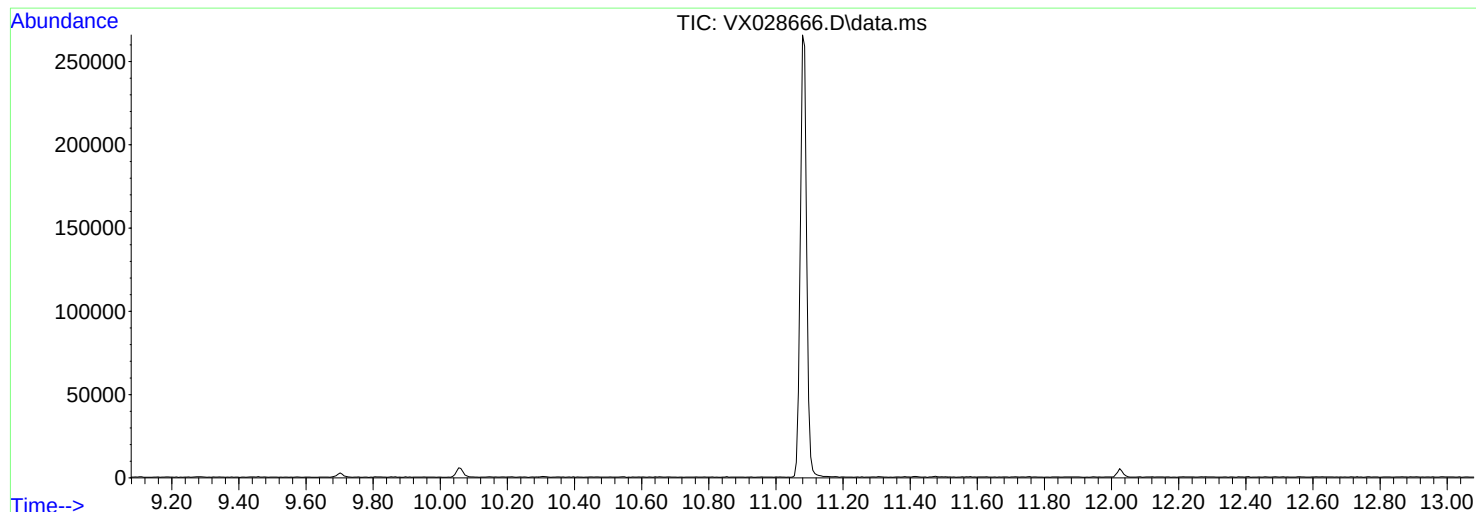

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	9080	PASS
75	95	30	60	54.9	24979	PASS
95	95	100	100	100.0	45491	PASS
96	95	5	9	7.2	3258	PASS
173	174	0.00	2	1.2	377	PASS
174	95	50	100	70.1	31872	PASS
175	174	5	9	8.2	2616	PASS
176	174	95	101	100.5	32032	PASS
177	176	5	9	6.7	2147	PASS