

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
 Data File : VX021987.D
 Acq On : 14 May 2021 12:01
 Operator : JC/MD
 Sample : M2383-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KTW-02DL

Quant Time: May 15 01:03:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
 Quant Title : SW846 8260
 QLast Update : Sat May 08 05:38:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	78662	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	170653	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	182030	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	85533	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	66118	51.07	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.14%			
35) Dibromofluoromethane	5.391	113	57713	49.35	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 98.70%			
50) Toluene-d8	8.653	98	225400	50.50	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 101.00%			
62) 4-Bromofluorobenzene	11.085	95	101319	57.52	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 115.04%			
Target Compounds						Qvalue
5) Bromomethane	1.611	94	274	0.52	ug/l	81
6) Chloroethane	1.721	64	1432	1.92	ug/l #	60
10) Methyl Iodide	2.453	142	1052	0.88	ug/l #	90
11) Tert butyl alcohol	2.941	59	846	2.45	ug/l #	80
13) Acrolein	2.209	56	116	Below Cal	#	14
16) Acetone	2.386	43	1277	2.20	ug/l	90
17) Carbon Disulfide	2.514	76	272087	91.72	ug/l	99
18) Methyl Acetate	2.709	43	535	0.33	ug/l #	47
20) Methylene Chloride	2.794	84	928	0.92	ug/l #	88
25) 2-Butanone	4.574	43	662	0.66	ug/l #	45
30) Chloroform	5.093	83	675	0.32	ug/l #	76
31) Cyclohexane	5.562	56	2012	1.18	ug/l #	1
36) 1,1-Dichloropropene	5.562	75	7120	3.94	ug/l #	49
38) Carbon Tetrachloride	5.556	117	8749	4.84	ug/l #	16
40) Benzene	6.050	78	19094	3.51	ug/l #	88
52) Toluene	8.726	92	3814	1.10	ug/l	98
55) 1,1,2-Trichloroethane	9.019	97	281	0.20	ug/l #	15
67) Ethyl Benzene	10.195	91	27382	3.52	ug/l	98
68) m/p-Xylenes	10.305	106	18117	6.10	ug/l	99
69) o-Xylene	10.646	106	6907	2.33	ug/l	94
73) Isopropylbenzene	10.963	105	1957	0.25	ug/l	93
76) 1,2,3-Trichloropropane	11.085	75	51544	21.20	ug/l #	39
78) n-propylbenzene	11.311	91	8004	0.87	ug/l	96
79) 2-Chlorotoluene	11.616	91	1842	0.33	ug/l	81
80) 1,3,5-Trimethylbenzene	11.457	105	15373	2.31	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.085	75	51544	49.17	ug/l #	12
82) 4-Chlorotoluene	11.457	91	2164	0.34	ug/l #	45
84) 1,2,4-Trimethylbenzene	11.756	105	55689	8.35	ug/l	100
85) sec-Butylbenzene	11.756	105	55689	7.04	ug/l #	57
89) n-Butylbenzene	12.335	91	1633	0.26	ug/l #	59
90) Hexachloroethane	12.616	117	551	0.45	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.957	75	58	Below Cal	#	1
94) Hexachlorobutadiene	13.725	225	158	0.22	ug/l #	39
95) Naphthalene	13.780	128	444088	57.92	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
Data File : VX021987.D
Acq On : 14 May 2021 12:01
Operator : JC/MD
Sample : M2383-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL

Quant Time: May 15 01:03:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260
QLast Update : Sat May 08 05:38:18 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
Data File : VX021987.D
Acq On : 14 May 2021 12:01
Operator : JC/MD
Sample : M2383-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL

Quant Time: May 15 01:03:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260
QLast Update : Sat May 08 05:38:18 2021
Response via : Initial Calibration




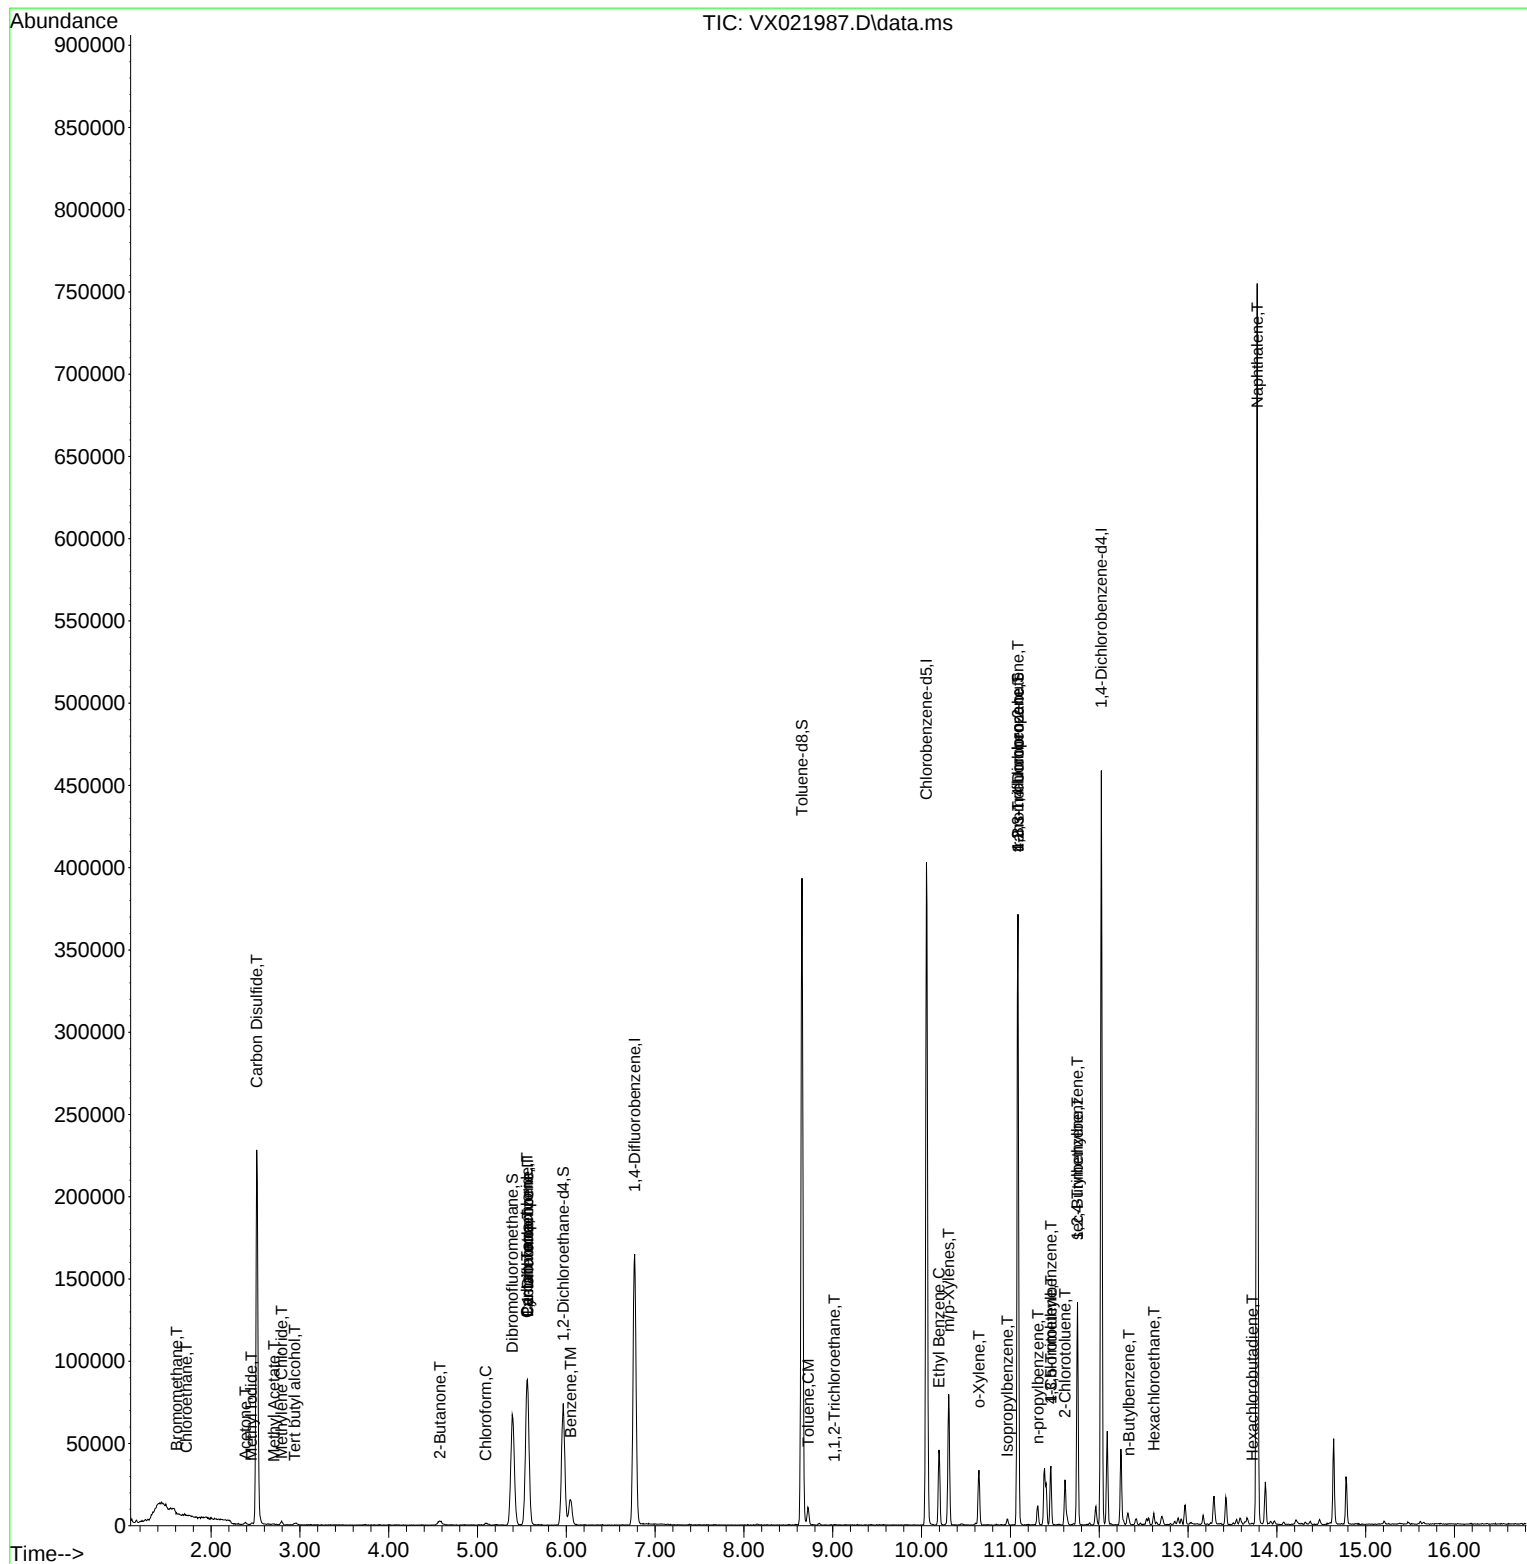




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion:168 Resp: 78662
Ion Ratio Lower Upper
168 100
99 65.1 45.8 68.6



#5
Bromomethane
Concen: 0.52 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 94 Resp: 274
Ion Ratio Lower Upper
94 100
96 77.0 76.4 114.6


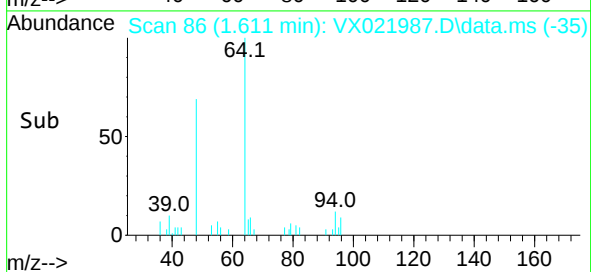

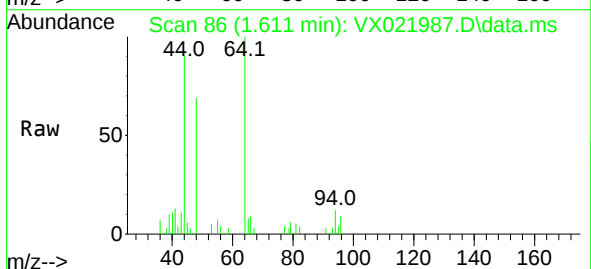


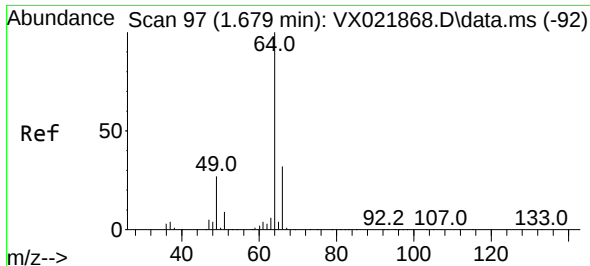

#6
Chloroethane
Concen: 1.92 ug/l
RT: 1.721 min Scan# 104
Delta R.T. 0.042 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion: 64 Resp: 1432
Ion Ratio Lower Upper
64 100
66 9.3 25.4 38.0#

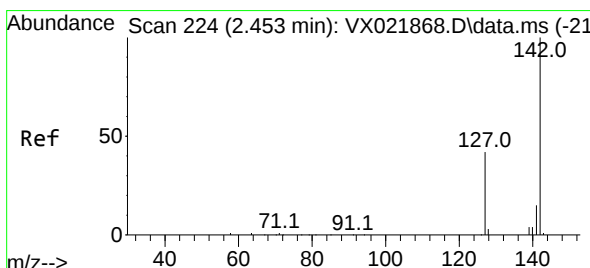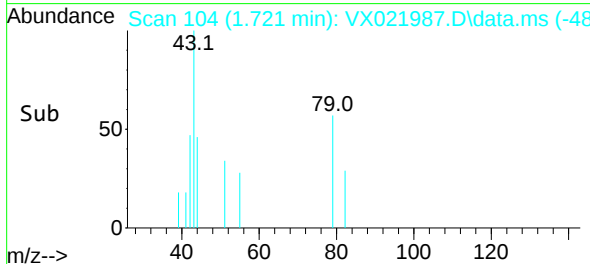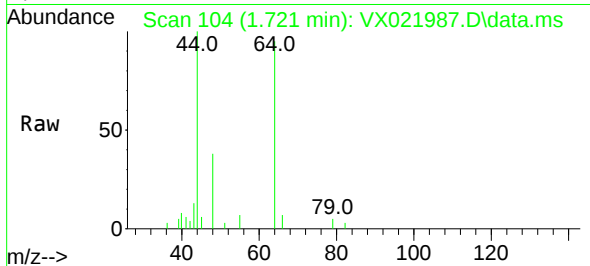

#10
Methyl Iodide
Concen: 0.88 ug/l
RT: 2.453 min Scan# 224
Delta R.T. -0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 142 Resp: 1052
Ion Ratio Lower Upper
142 100
127 46.3 33.3 49.9
141 7.1 11.4 17.0#

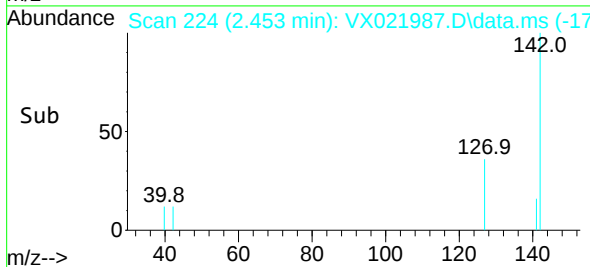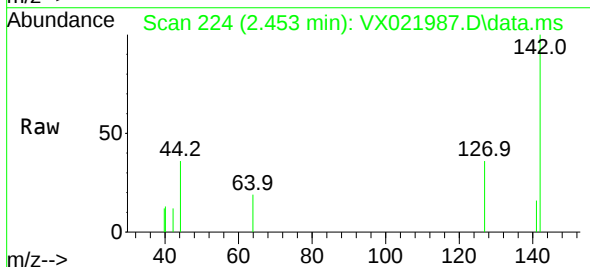




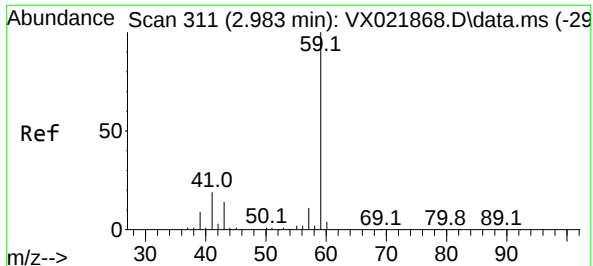


#11

Tert butyl alcohol
Concen: 2.45 ug/l
RT: 2.941 min Scan# 304
Delta R.T. -0.042 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL




Tgt Ion: 59 Resp: 846
Ion Ratio Lower Upper
59 100
57 2.2 7.8 11.8#

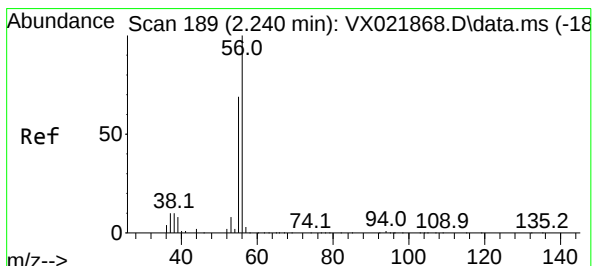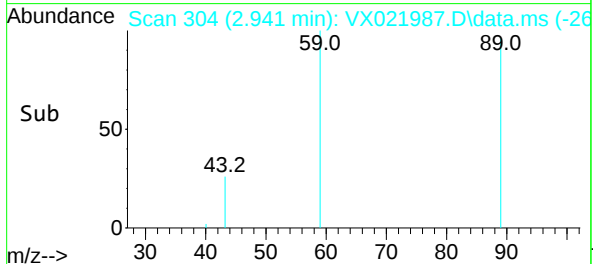


#13

Acrolein
Concen: Below Cal
RT: 2.209 min Scan# 184
Delta R.T. -0.031 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 56 Resp: 116
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#


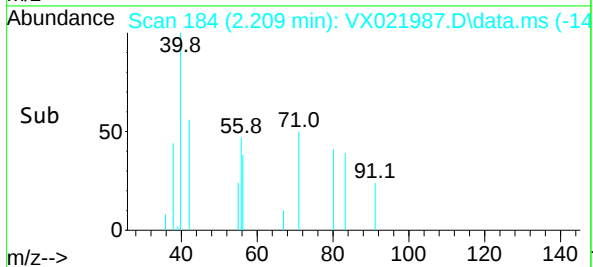

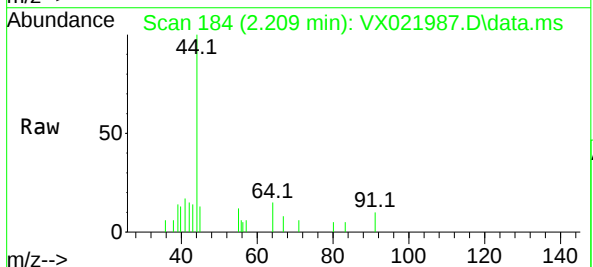




#16
Acetone
Concen: 2.20 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion: 43 Resp: 1277
Ion Ratio Lower Upper
43 100
58 40.5 27.8 41.8

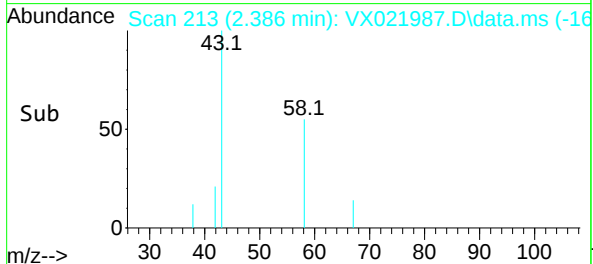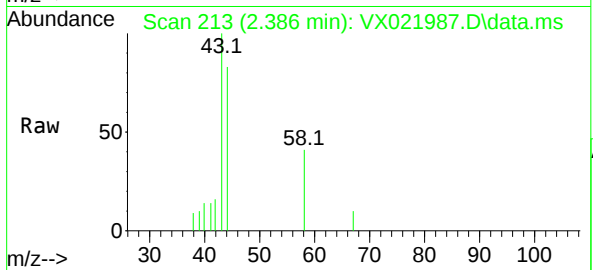

#17
Carbon Disulfide
Concen: 91.72 ug/l
RT: 2.514 min Scan# 234
Delta R.T. 0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 76 Resp: 272087
Ion Ratio Lower Upper
76 100
78 9.3 7.2 10.8


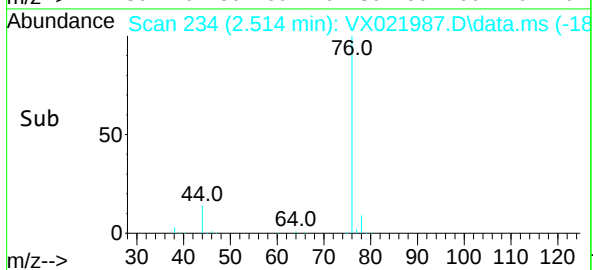

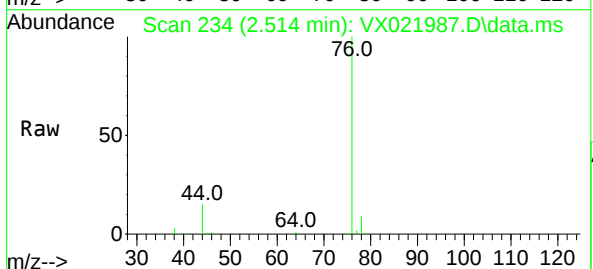




#18
Methyl Acetate
Concen: 0.33 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleID :
KTW-02DL


Tgt Ion: 43 Resp: 535
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#



#20
Methylene Chloride
Concen: 0.92 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 84 Resp: 928
Ion Ratio Lower Upper
84 100
49 119.8 88.6 132.8
51 48.3 27.0 40.6#
86 54.7 50.3 75.5


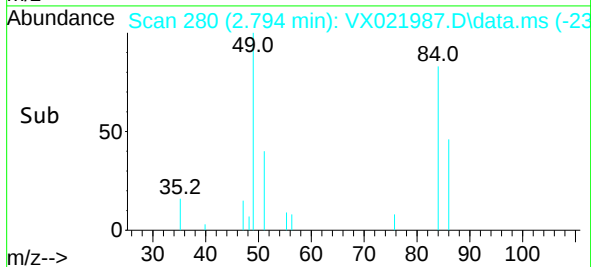

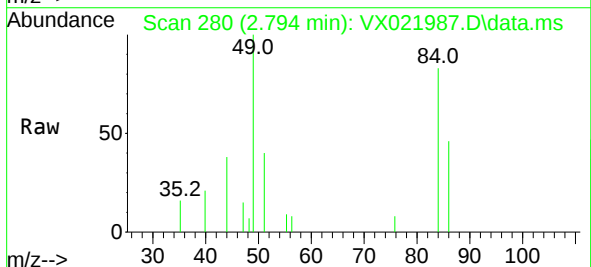




#25
2-Butanone
Concen: 0.66 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampled :
KTW-02DL


Tgt Ion: 43 Resp: 662
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#

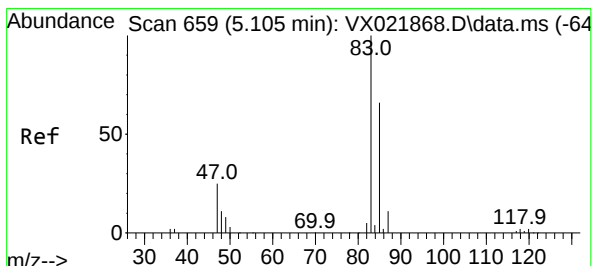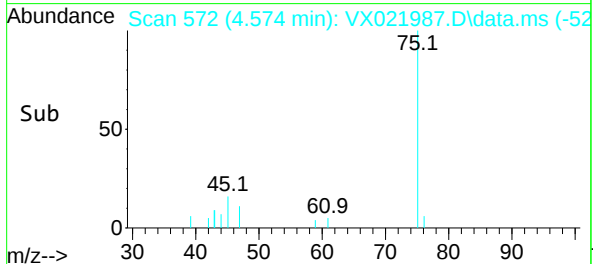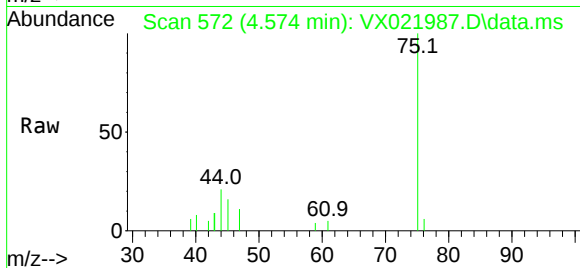

#30
Chloroform
Concen: 0.32 ug/l
RT: 5.093 min Scan# 657
Delta R.T. -0.012 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01


Tgt Ion: 83 Resp: 675
Ion Ratio Lower Upper
83 100
85 46.4 52.0 78.0#

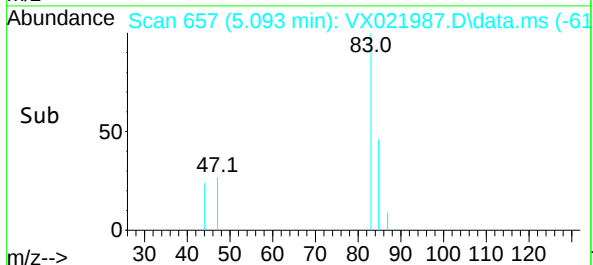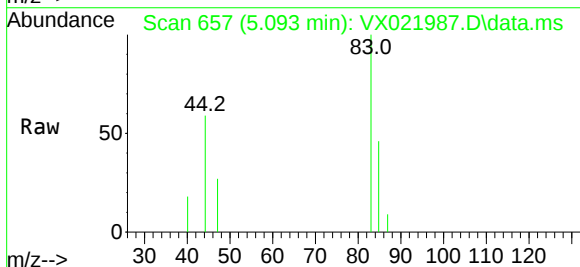



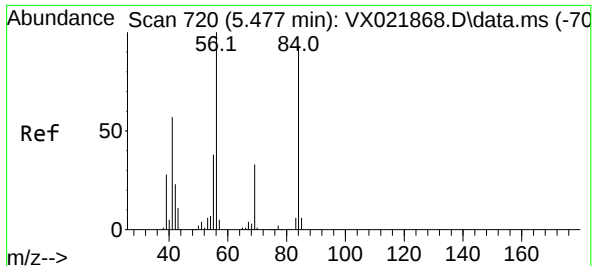


#31
Cyclohexane
Concen: 1.18 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.085 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL



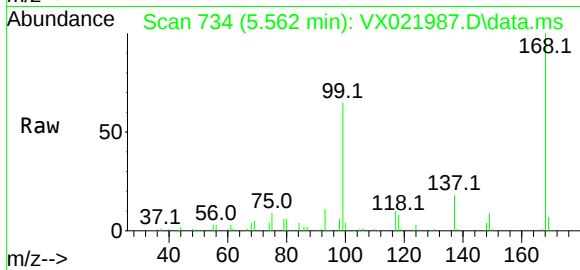



Tgt Ion: 56 Resp: 2012
Ion Ratio Lower Upper
56 100
69 187.1 25.3 37.9#
84 146.0 71.4 107.0#

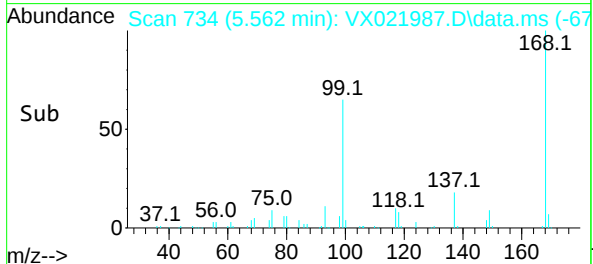

#33
1,2-Dichloroethane-d4
Concen: 51.07 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.007 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 65 Resp: 66118
Ion Ratio Lower Upper
65 100
67 51.9 0.0 105.4


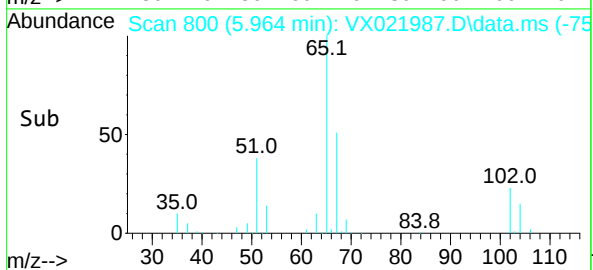

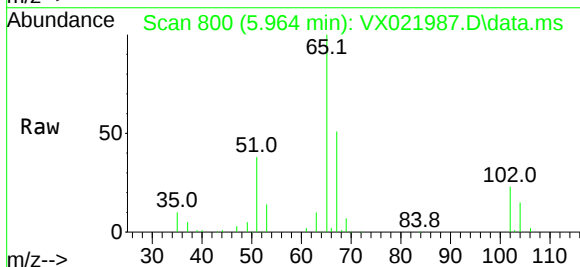


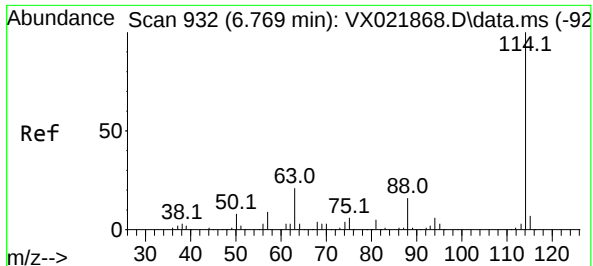

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion:114 Resp: 170653
Ion Ratio Lower Upper
114 100
63 21.5 0.0 40.8
88 17.1 0.0 32.8

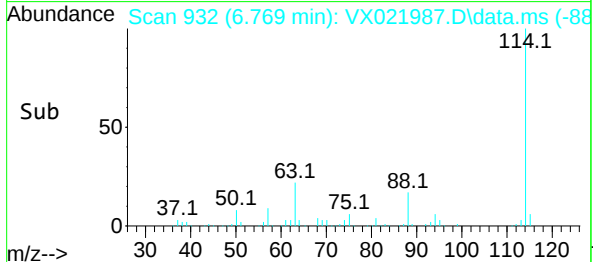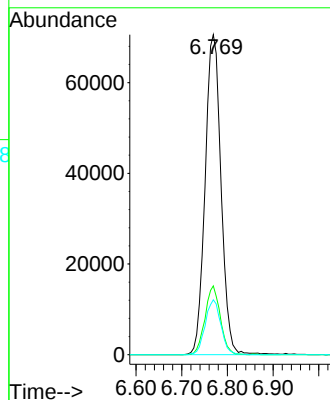

#35
Dibromofluoromethane
Concen: 49.35 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion:113 Resp: 57713
Ion Ratio Lower Upper
113 100
111 102.1 81.9 122.9
192 16.1 16.7 25.1#

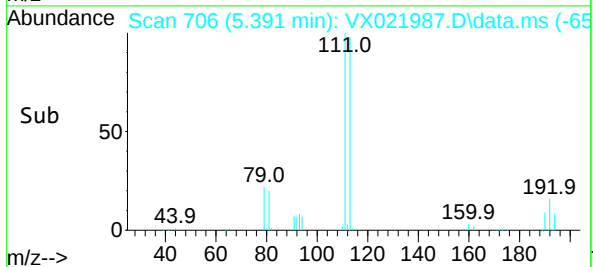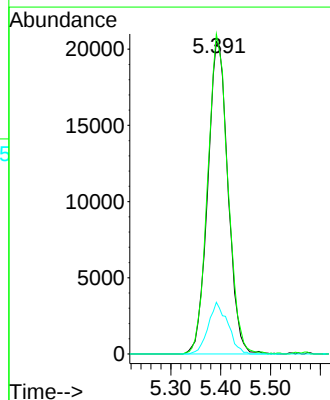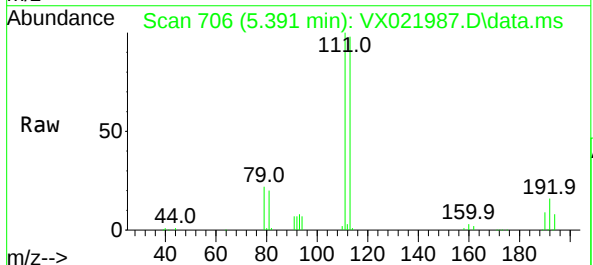



#36

1,1-Dichloropropene

Concen: 3.94 ug/l

RT: 5.562 min Scan# 734





Delta R.T. -0.140 min

Lab File: VX021987.D

Acq: 14 May 2021 12:01

Tgt Ion:	75	Resp:	7120
Ion	Ratio	Lower	Upper
75	100		
110	9.0	18.1	54.4#
77	0.0	25.3	37.9#

Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL

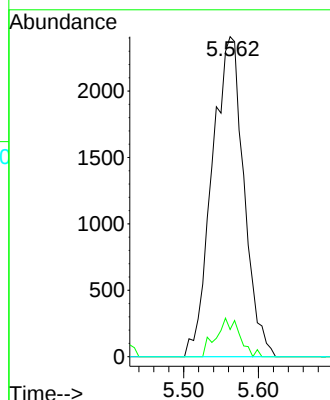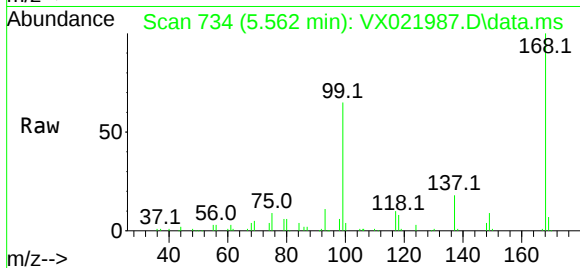

#38

Carbon Tetrachloride

Concen: 4.84 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.134 min

Lab File: VX021987.D

Acq: 14 May 2021 12:01

Tgt Ion:	117	Resp:	8749
Ion	Ratio	Lower	Upper
117	100		
119	4.6	76.2	114.2#
121	0.0	24.8	37.2#


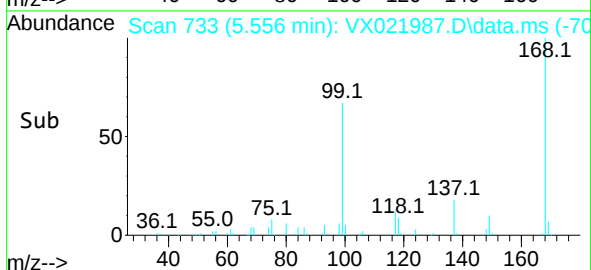
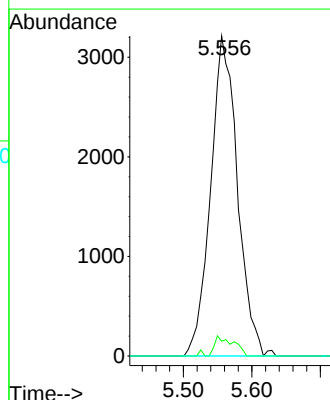
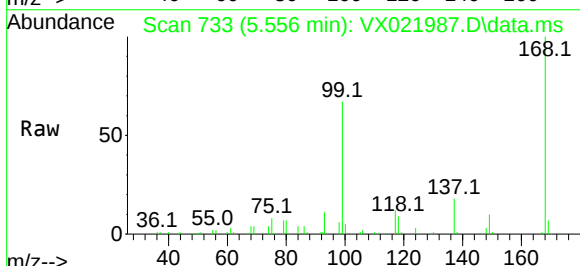




#40
Benzene
Concen: 3.51 ug/l
RT: 6.050 min Scan# 814
Delta R.T. 0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion: 78 Resp: 19094
Ion Ratio Lower Upper
78 100
77 17.6 18.9 28.3#



#50
Toluene-d8
Concen: 50.50 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 98 Resp: 225400
Ion Ratio Lower Upper
98 100
100 67.1 51.9 77.9


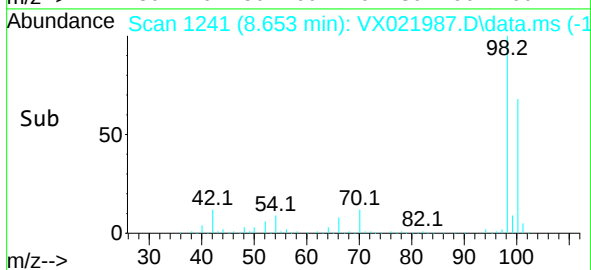

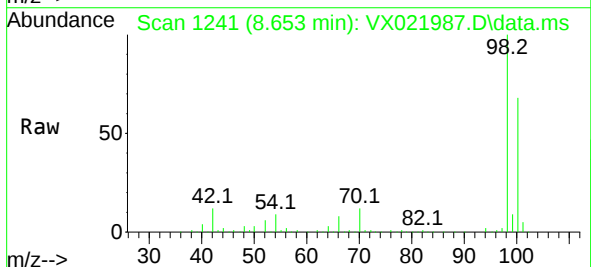




#52
Toluene
Concen: 1.10 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion: 92 Resp: 3814
Ion Ratio Lower Upper
92 100
91 168.3 137.1 205.7

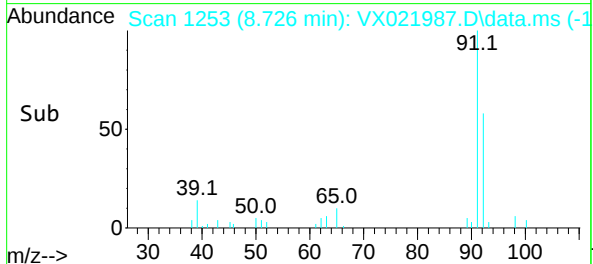

#55
1,1,2-Trichloroethane
Concen: 0.20 ug/l
RT: 9.019 min Scan# 1301
Delta R.T. -0.140 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 97 Resp: 281
Ion Ratio Lower Upper
97 100
83 0.0 69.3 103.9#
85 0.0 44.3 66.5#
99 0.0 50.3 75.5#



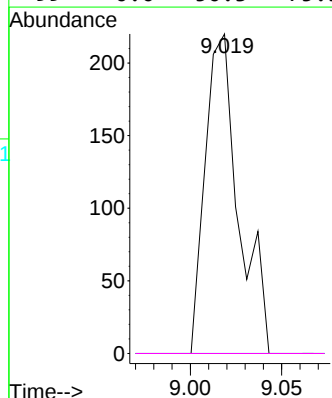
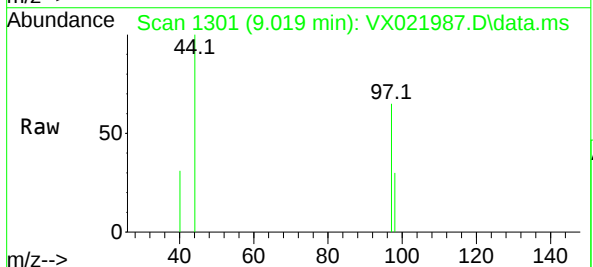




#62
4-Bromofluorobenzene
Concen: 57.52 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampled :
KTW-02DL


Tgt Ion: 95 Resp: 101319
Ion Ratio Lower Upper
95 100
174 64.6 0.0 154.6
176 61.8 0.0 155.8

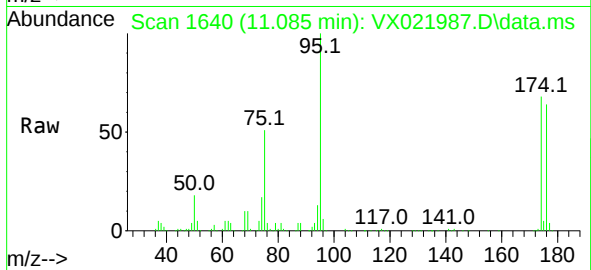

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 117 Resp: 182030
Ion Ratio Lower Upper
117 100
82 58.3 47.4 71.2
119 31.2 26.6 39.8


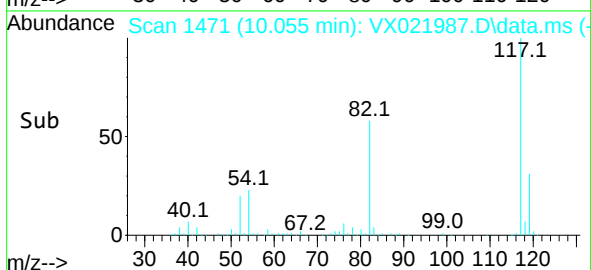

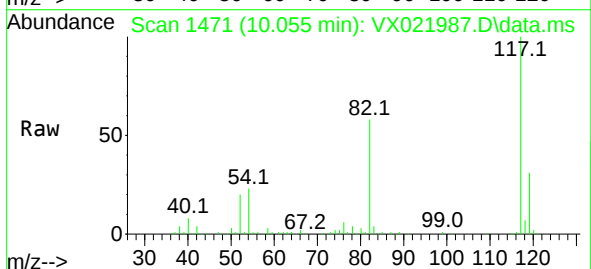




#67
Ethyl Benzene
Concen: 3.52 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampled :
KTW-02DL


Tgt Ion: 91 Resp: 27382
Ion Ratio Lower Upper
91 100
106 29.7 24.6 37.0



#68
m/p-Xylenes
Concen: 6.10 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 106 Resp: 18117
Ion Ratio Lower Upper
106 100
91 204.6 162.8 244.2









#69
o-Xylene
Concen: 2.33 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampled :
KTW-02DL


Tgt Ion:106 Resp: 6907
Ion Ratio Lower Upper
106 100
91 225.9 108.1 324.2

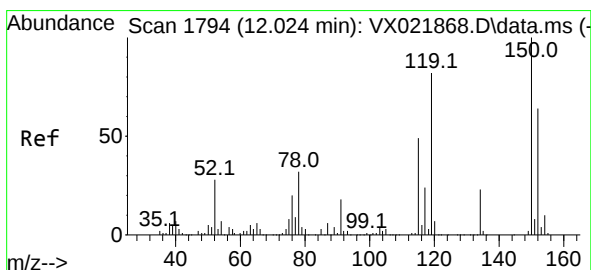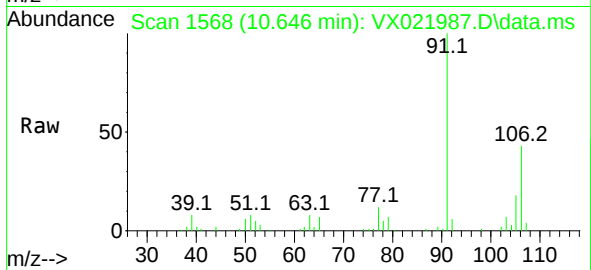

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion:152 Resp: 85533
Ion Ratio Lower Upper
152 100
115 66.4 41.1 123.3
150 156.3 0.0 349.0


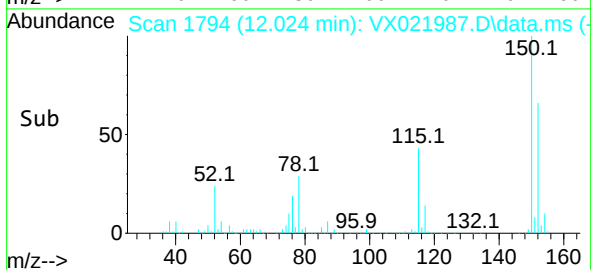

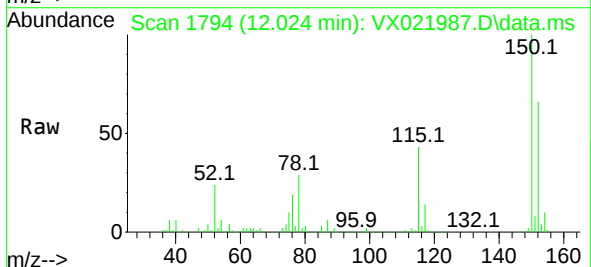


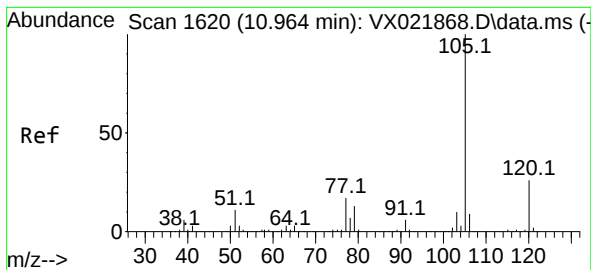

#73
Isopropylbenzene
Concen: 0.25 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampled :
KTW-02DL


Tgt Ion:105 Resp: 1957
Ion Ratio Lower Upper
105 100
120 22.8 13.2 39.6

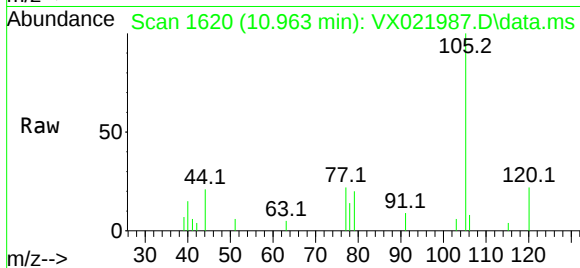

#76
1,2,3-Trichloropropane
Concen: 21.20 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 75 Resp: 51544
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#


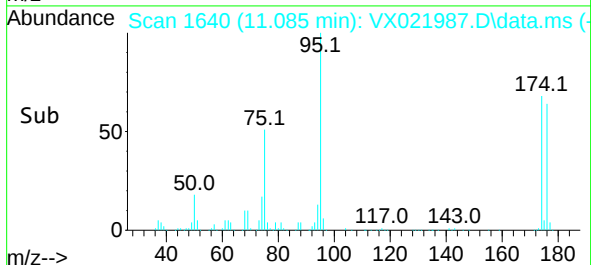

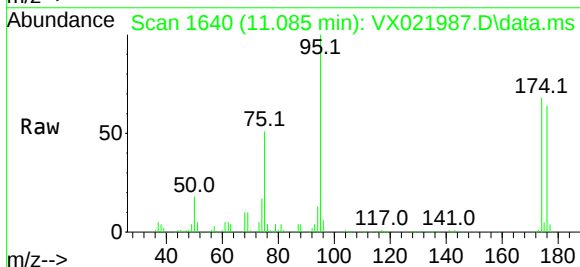




#78
n-propylbenzene
Concen: 0.87 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion: 91 Resp: 8004
Ion Ratio Lower Upper
91 100
120 21.1 11.5 34.5



#79
2-Chlorotoluene
Concen: 0.33 ug/l
RT: 11.616 min Scan# 1727
Delta R.T. 0.250 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 91 Resp: 1842
Ion Ratio Lower Upper
91 100
126 44.1 16.6 49.8


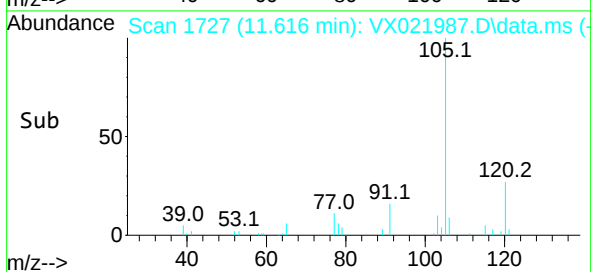

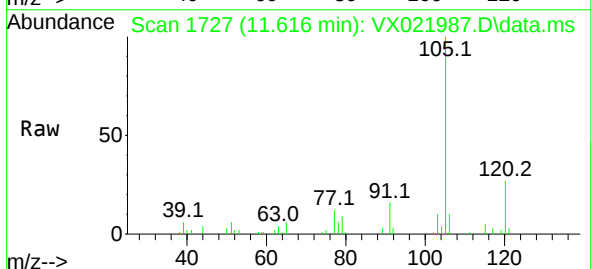




#80
1,3,5-Trimethylbenzene
Concen: 2.31 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampled :
KTW-02DL


Tgt Ion:105 Resp: 15373
Ion Ratio Lower Upper
105 100
120 49.2 23.8 71.5

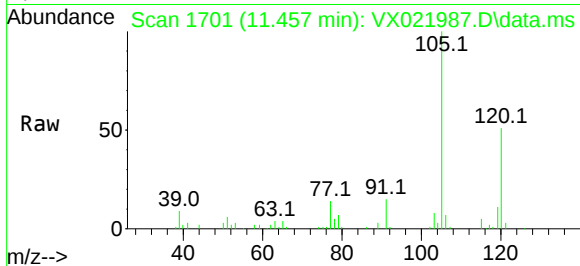

#81
trans-1,4-Dichloro-2-butene
Concen: 49.17 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 75 Resp: 51544
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


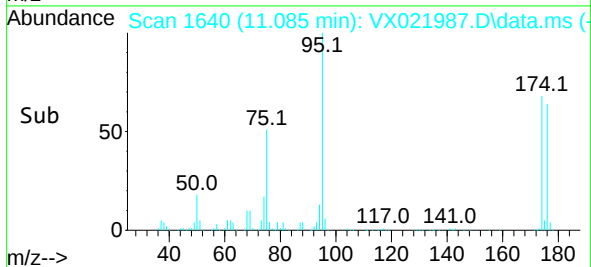

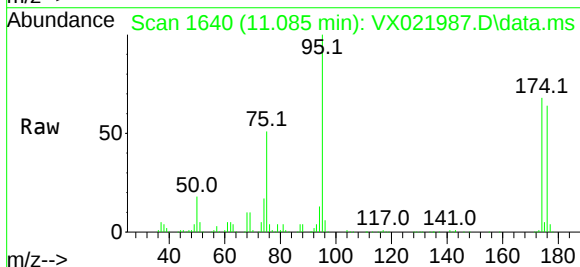




#82
4-Chlorotoluene
Concen: 0.34 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampled :
KTW-02DL


Tgt Ion: 91 Resp: 2164
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

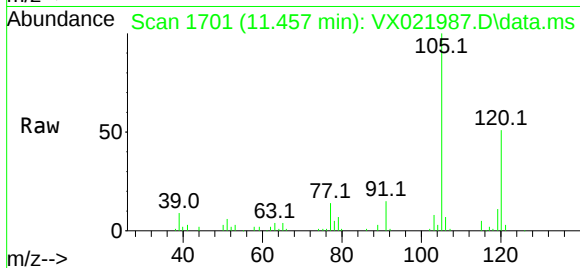

#84
1,2,4-Trimethylbenzene
Concen: 8.35 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 105 Resp: 55689
Ion Ratio Lower Upper
105 100
120 44.9 22.4 67.3


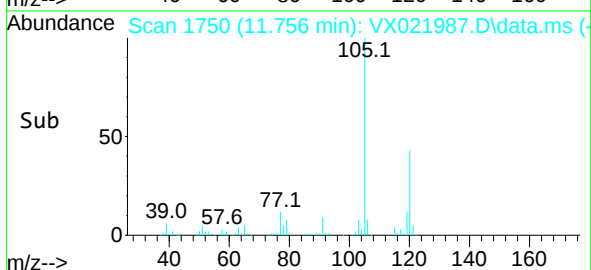

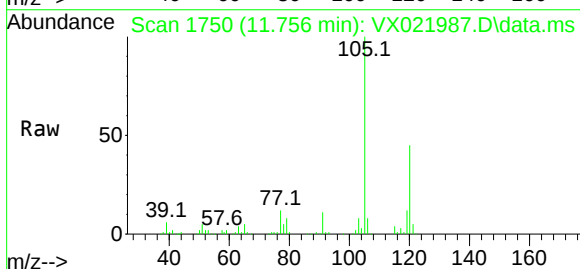




#85
 sec-Butylbenzene
 Concen: 7.04 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.140 min
 Lab File: VX021987.D
 Acq: 14 May 2021 12:01




Instrument :
 MSVOA_X
 ClientSampleId :
 KTW-02DL


Tgt Ion:105 Resp: 55689
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 29.8#

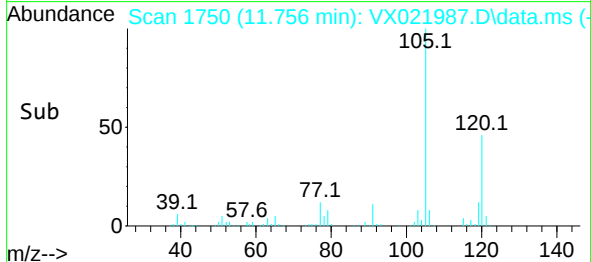

#89
 n-Butylbenzene
 Concen: 0.26 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.000 min
 Lab File: VX021987.D
 Acq: 14 May 2021 12:01

Tgt Ion: 91 Resp: 1633
 Ion Ratio Lower Upper
 91 100
 92 42.6 27.4 82.0
 134 73.7 13.2 39.5#


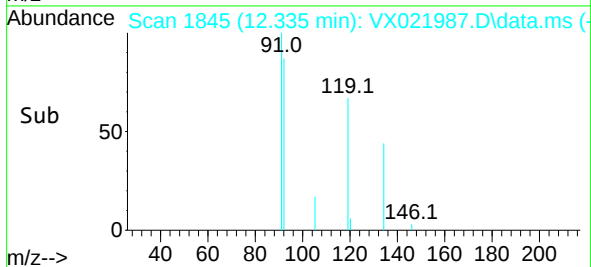

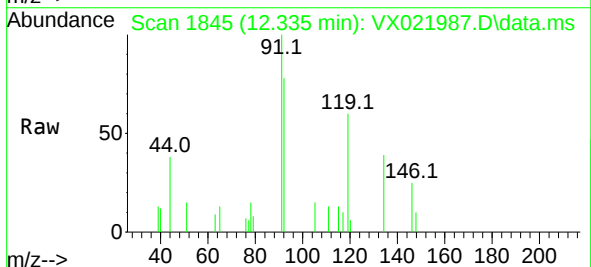




#90
Hexachloroethane
Concen: 0.45 ug/l
RT: 12.616 min Scan# 1891
Delta R.T. 0.073 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01




Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL


Tgt Ion:117 Resp: 551
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

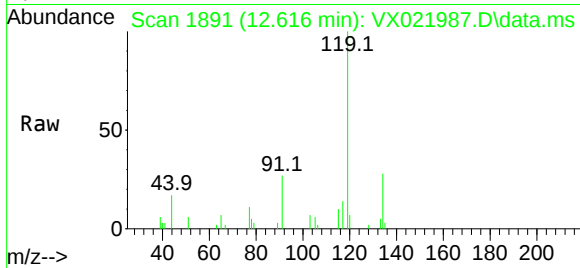

#92
1,2-Dibromo-3-Chloropropane
Concen: Below Cal
RT: 12.957 min Scan# 1947
Delta R.T. 0.012 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion: 75 Resp: 58
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#


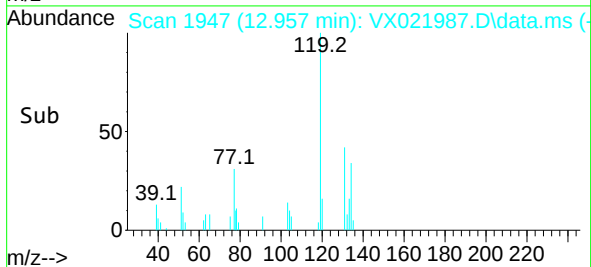

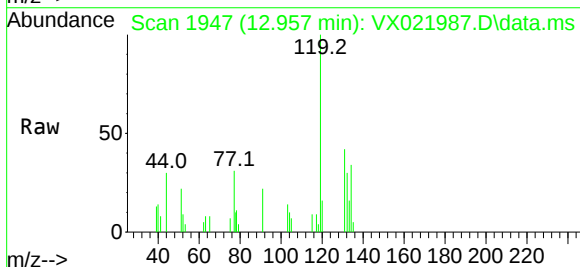




#94
Hexachlorobutadiene
Concen: 0.22 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.006 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Instrument :
MSVOA_X
ClientSampleId :
KTW-02DL

Tgt Ion:225 Resp: 158
Ion Ratio Lower Upper
225 100
223 31.0 31.1 93.2#
227 0.0 31.6 95.0#

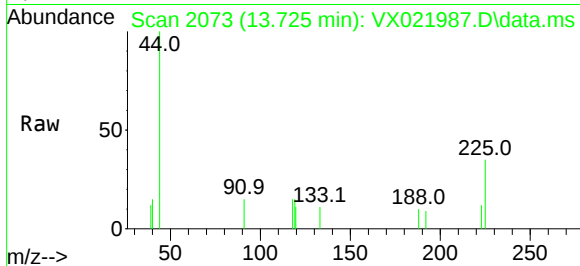

#95
Naphthalene
Concen: 57.92 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX021987.D
Acq: 14 May 2021 12:01

Tgt Ion:128 Resp: 444088
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 10.7 8.8 13.2

