

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
 Data File : VX021989.D
 Acq On : 14 May 2021 12:47
 Operator : JC/MD
 Sample : M2383-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB-01-05112021

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M

Title : SW846 8260

Signal : TIC: VX021989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.380	207	212	222	rVB	11127	18365	2.99%	0.538%
2	2.532	230	237	247	rBV2	5942	12125	1.97%	0.355%
3	2.947	297	305	317	rBV2	11698	27511	4.47%	0.806%
4	4.568	560	571	585	rBV2	23499	80032	13.02%	2.345%
5	5.397	695	707	722	rBV	67580	193663	31.50%	5.675%
6	5.562	722	734	747	rVB	90353	255538	41.57%	7.488%
7	5.964	788	800	812	rBV2	74174	198819	32.34%	5.826%
8	6.769	920	932	950	rBV	169535	412238	67.05%	12.080%
9	8.653	1234	1241	1256	rBV	400326	614787	100.00%	18.015%
10	10.055	1465	1471	1481	rBV	426834	575421	93.60%	16.861%
11	11.085	1634	1640	1651	rVB	363653	458222	74.53%	13.427%
12	12.024	1789	1794	1803	rVB	470970	565928	92.05%	16.583%




Sum of corrected areas: 3412649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
Data File : VX021989.D
Acq On : 14 May 2021 12:47
Operator : JC/MD
Sample : M2383-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-01-05112021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

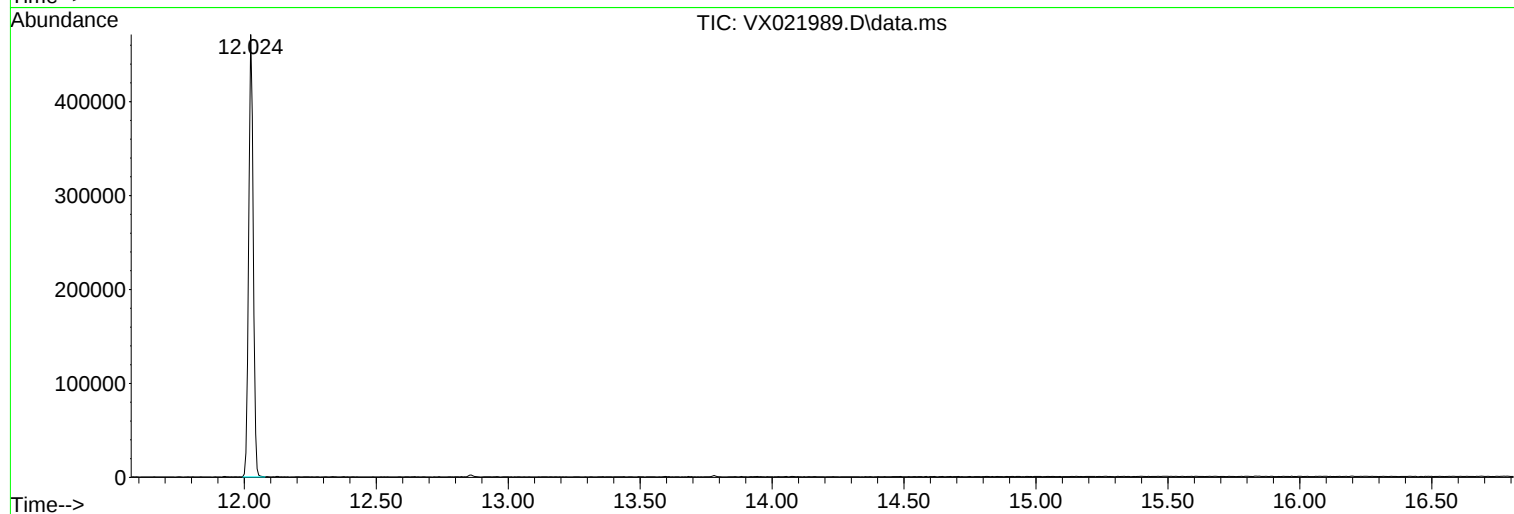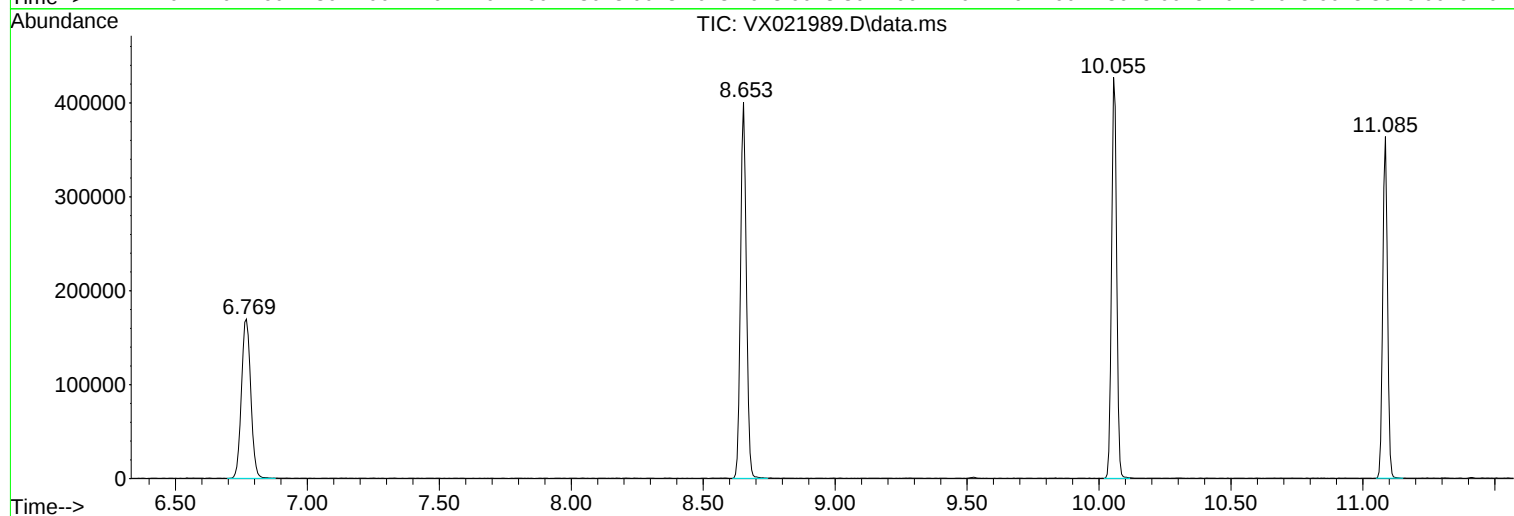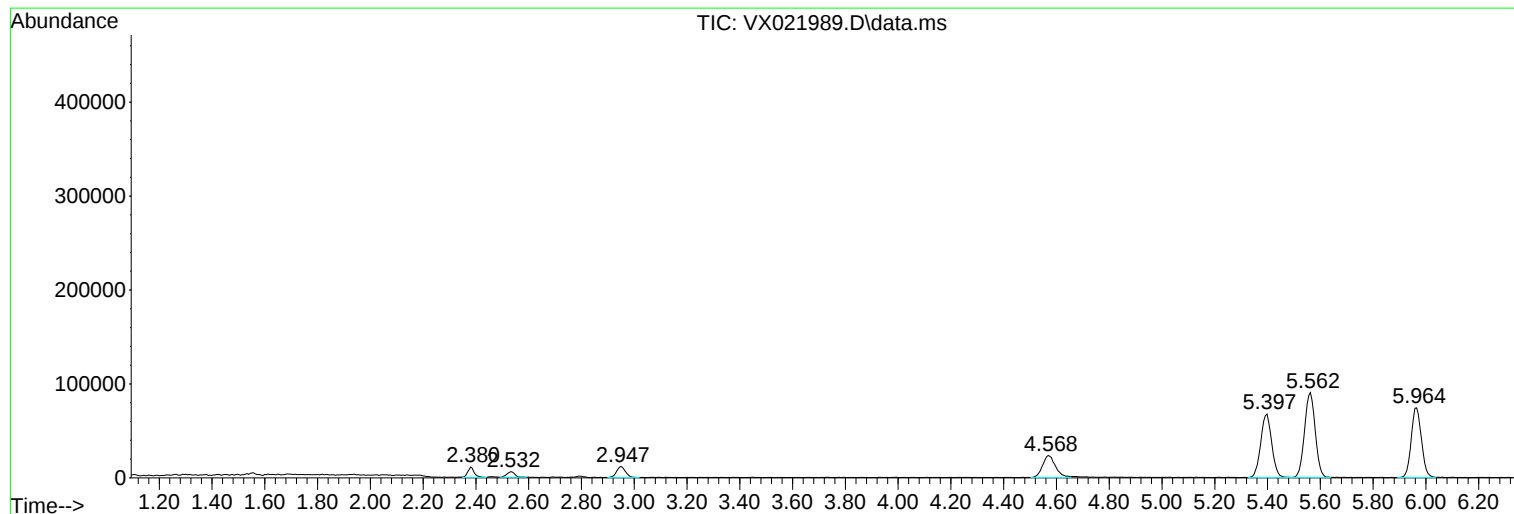

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
Data File : VX021989.D
Acq On : 14 May 2021 12:47
Operator : JC/MD
Sample : M2383-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-01-05112021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
Data File : VX021989.D
Acq On : 14 May 2021 12:47
Operator : JC/MD
Sample : M2383-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-01-05112021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
