
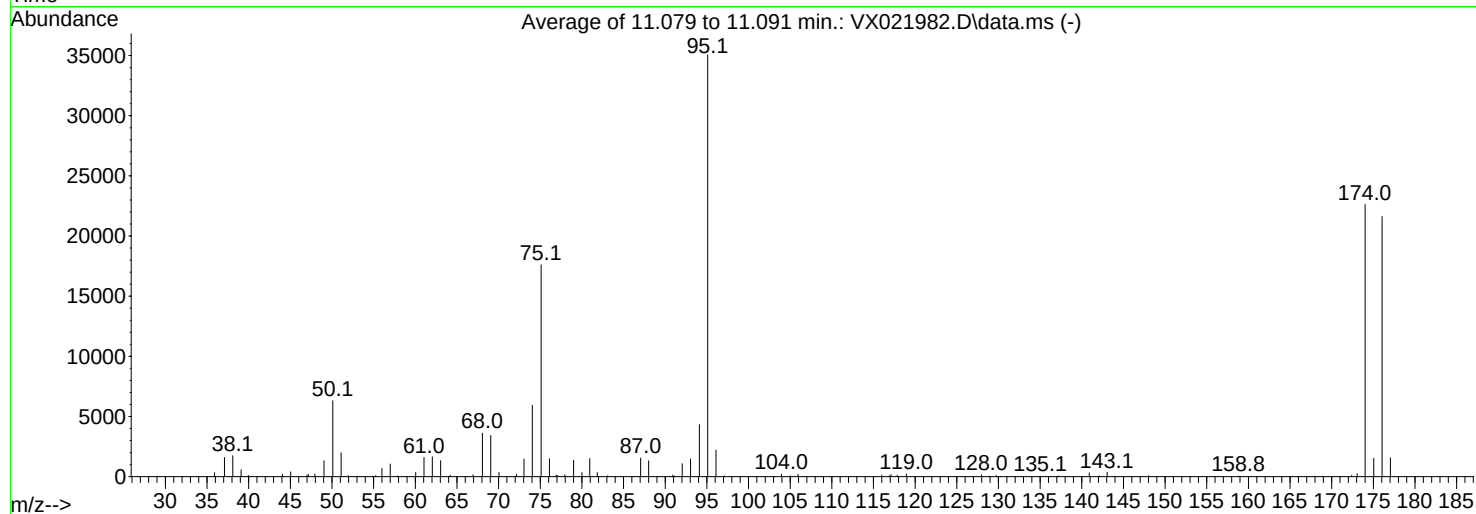


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051421\
 Data File : VX021982.D
 Acq On : 14 May 2021 09:20
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
 Title : SW846 8260
 Last Update : Sat May 08 05:38:18 2021

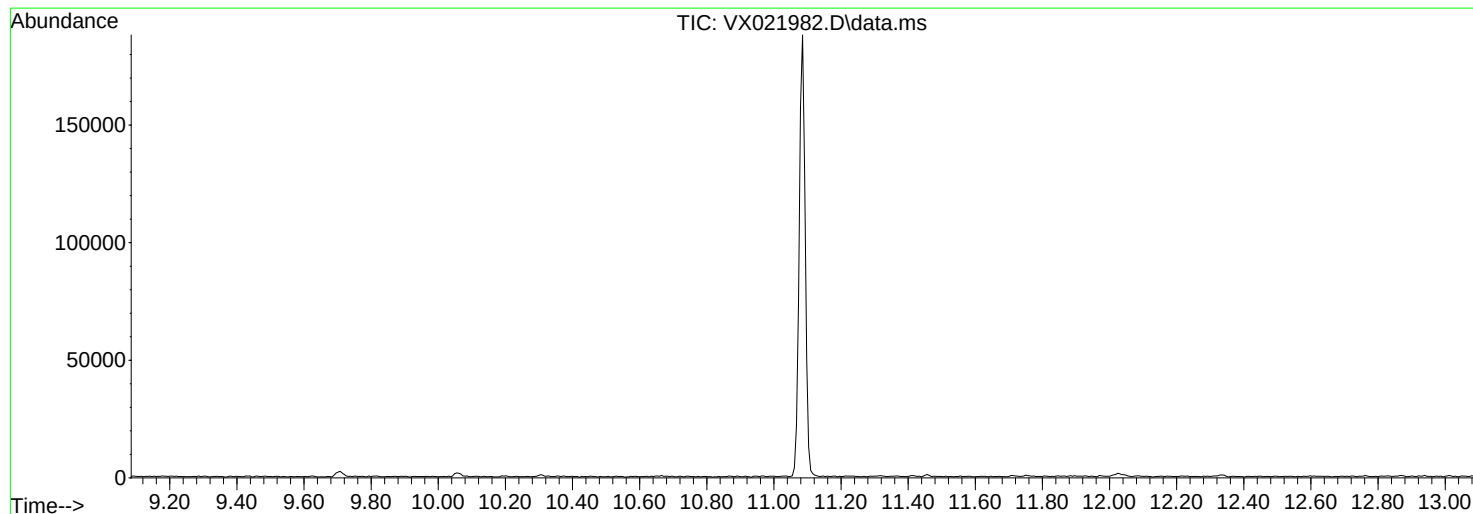

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	6314	PASS
75	95	30	60	50.2	17614	PASS
95	95	100	100	100.0	35061	PASS
96	95	5	9	6.3	2202	PASS
173	174	0.00	2	1.1	255	PASS
174	95	50	100	64.5	22619	PASS
175	174	5	9	6.8	1534	PASS
176	174	95	101	95.6	21627	PASS
177	176	5	9	7.2	1557	PASS