

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051425\
 Data File : VX046185.D
 Acq On : 14 May 2025 11:37
 Operator : JC/MD
 Sample : Q2018-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB

Quant Time: May 15 01:19:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	69447	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	142077	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	132653	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	56930	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	69480	53.664	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.320%
35) Dibromofluoromethane	5.379	113	50895	49.746	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.500%
50) Toluene-d8	8.647	98	177500	50.126	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.260%
62) 4-Bromofluorobenzene	11.079	95	69701	51.314	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	102.620%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051425\
Data File : VX046185.D
Acq On : 14 May 2025 11:37
Operator : JC/MD
Sample : Q2018-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB

Quant Time: May 15 01:19:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




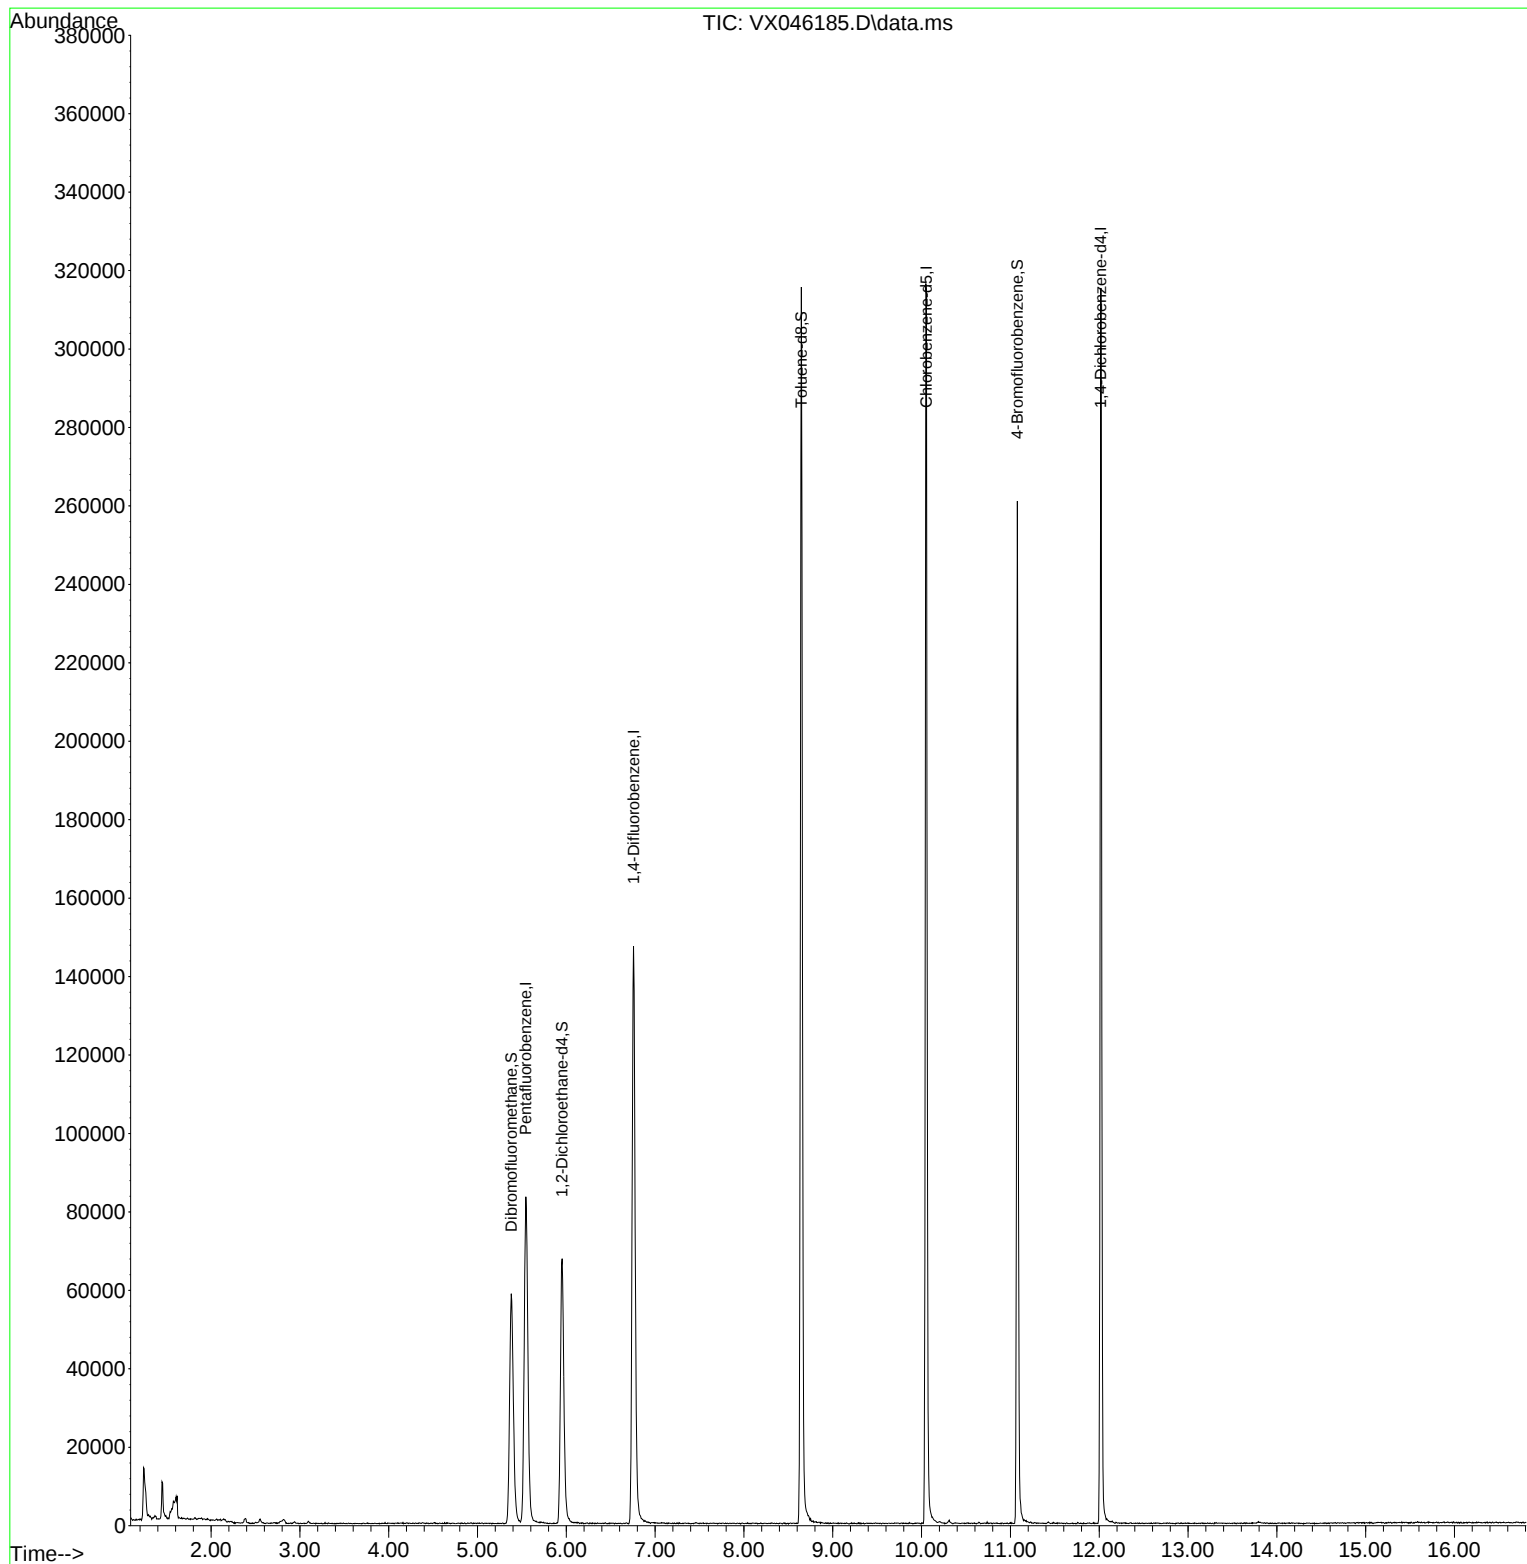




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.000 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37




Instrument :
MSVOA_X
ClientSampleId :
FB

Tgt Ion:168 Resp: 69447
Ion Ratio Lower Upper
168 100
99 73.8 54.9 82.3

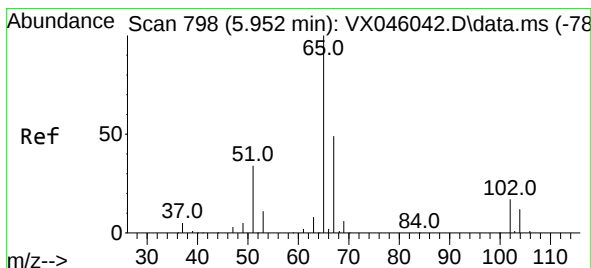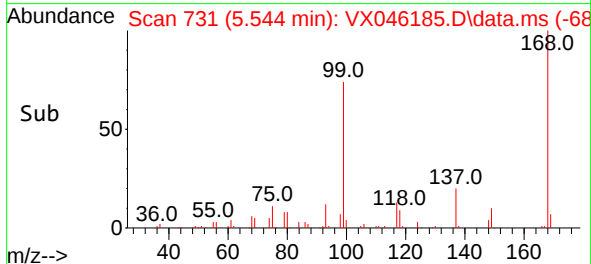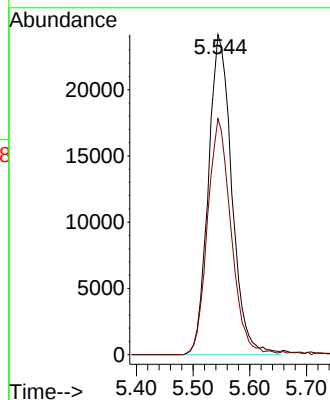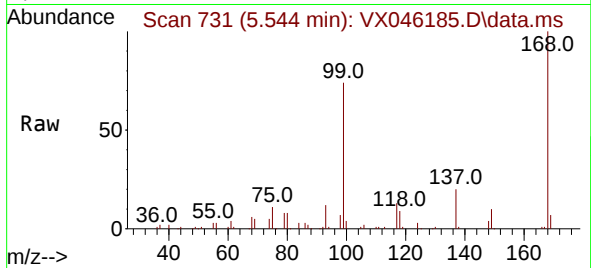

#33
1,2-Dichloroethane-d4
Concen: 53.664 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37

Tgt Ion: 65 Resp: 69480
Ion Ratio Lower Upper
65 100
67 50.3 0.0 99.0

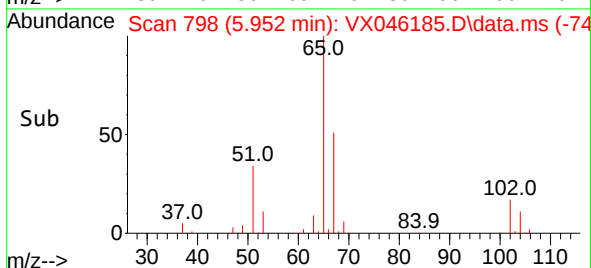
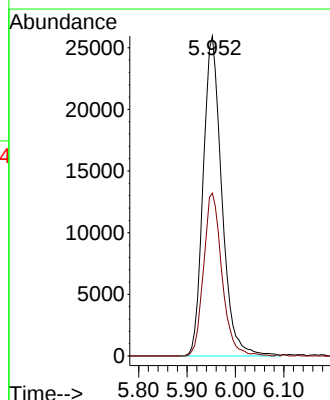
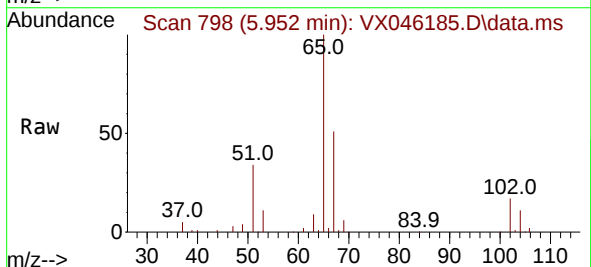




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37




Instrument :
MSVOA_X
ClientSampleId :
FB

Tgt Ion:114 Resp: 142077
Ion Ratio Lower Upper
114 100
63 21.9 0.0 49.2
88 16.8 0.0 33.6

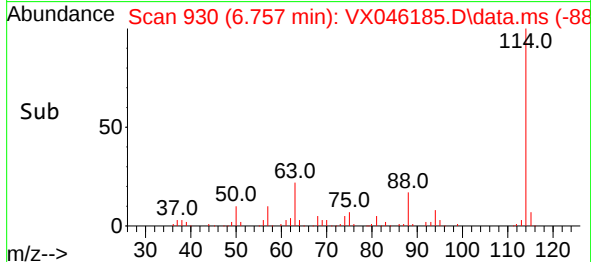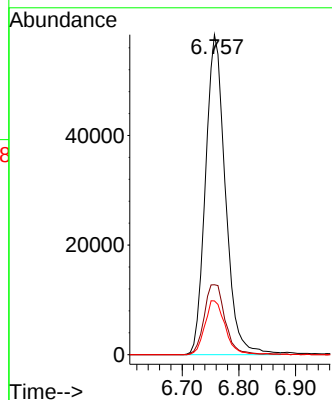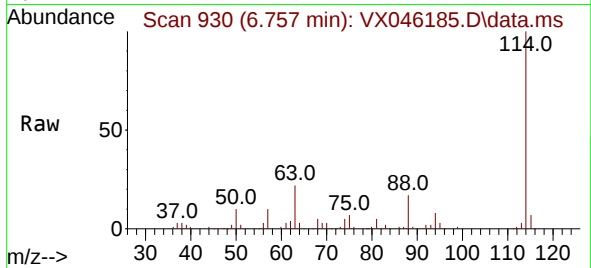

#35
Dibromofluoromethane
Concen: 49.746 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37

Tgt Ion:113 Resp: 50895
Ion Ratio Lower Upper
113 100
111 103.8 83.1 124.7
192 17.0 13.3 19.9


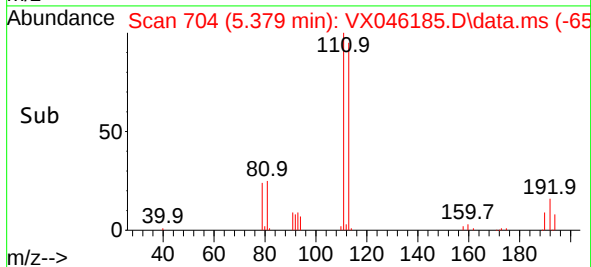
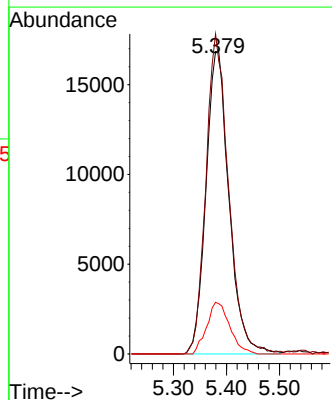
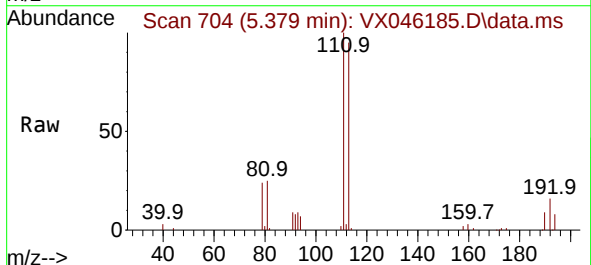




#50
Toluene-d8
Concen: 50.126 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37




Instrument :
MSVOA_X
ClientSampleId :
FB


Tgt Ion: 98 Resp: 177500
Ion Ratio Lower Upper
98 100
100 64.9 53.5 80.3

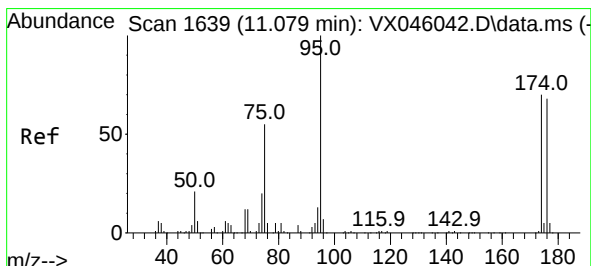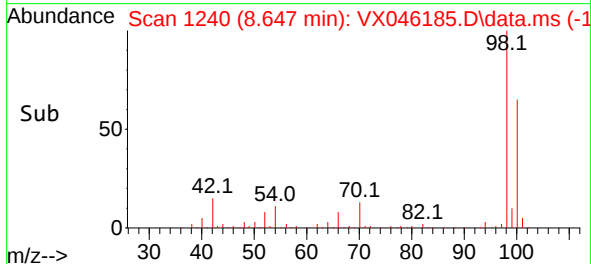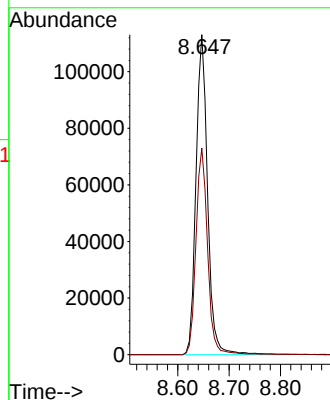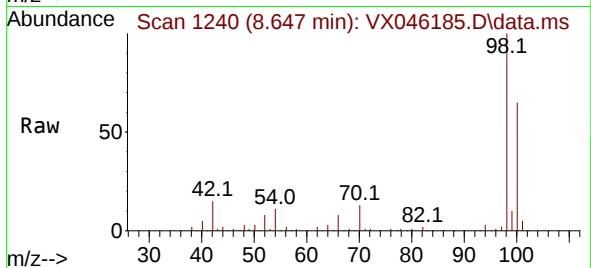

#62
4-Bromofluorobenzene
Concen: 51.314 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37

Tgt Ion: 95 Resp: 69701
Ion Ratio Lower Upper
95 100
174 65.8 0.0 135.8
176 63.4 0.0 131.4

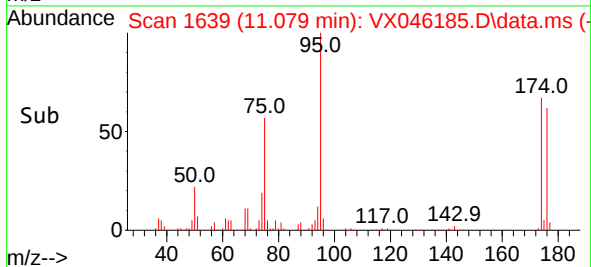
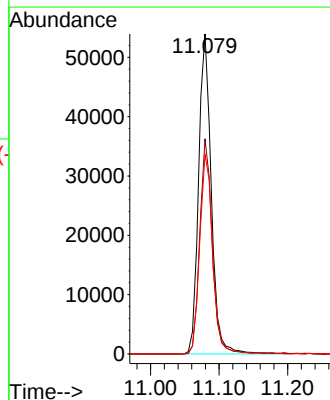
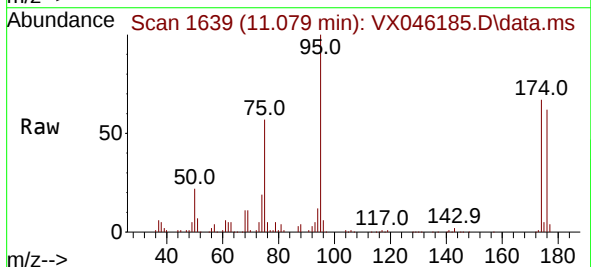


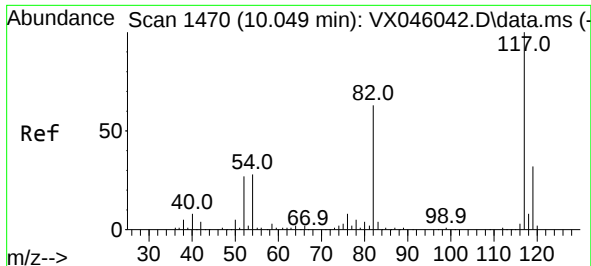

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37

Instrument :
MSVOA_X
ClientSampleId :
FB

Tgt Ion:117 Resp: 132653
Ion Ratio Lower Upper
117 100
82 60.0 50.6 76.0
119 32.9 25.8 38.6

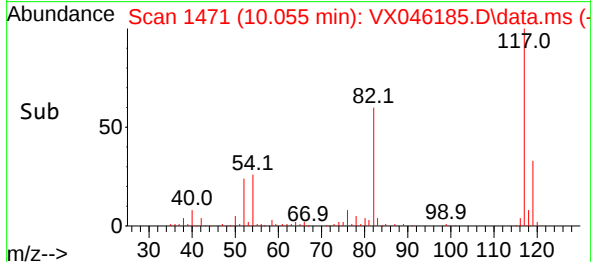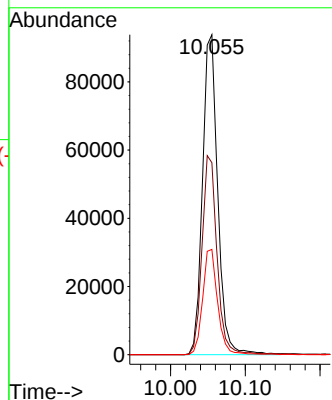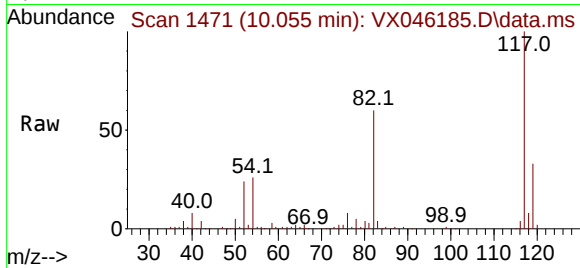

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX046185.D
Acq: 14 May 2025 11:37

Tgt Ion:152 Resp: 56930
Ion Ratio Lower Upper
152 100
115 66.8 46.9 140.7
150 161.0 0.0 351.0

