


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX051520\
Data File : VX016268.D
Acq On : 15 May 2020 09:21
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X050420W.M
Title : SW846 8260
Last Update : Wed May 06 06:43:32 2020

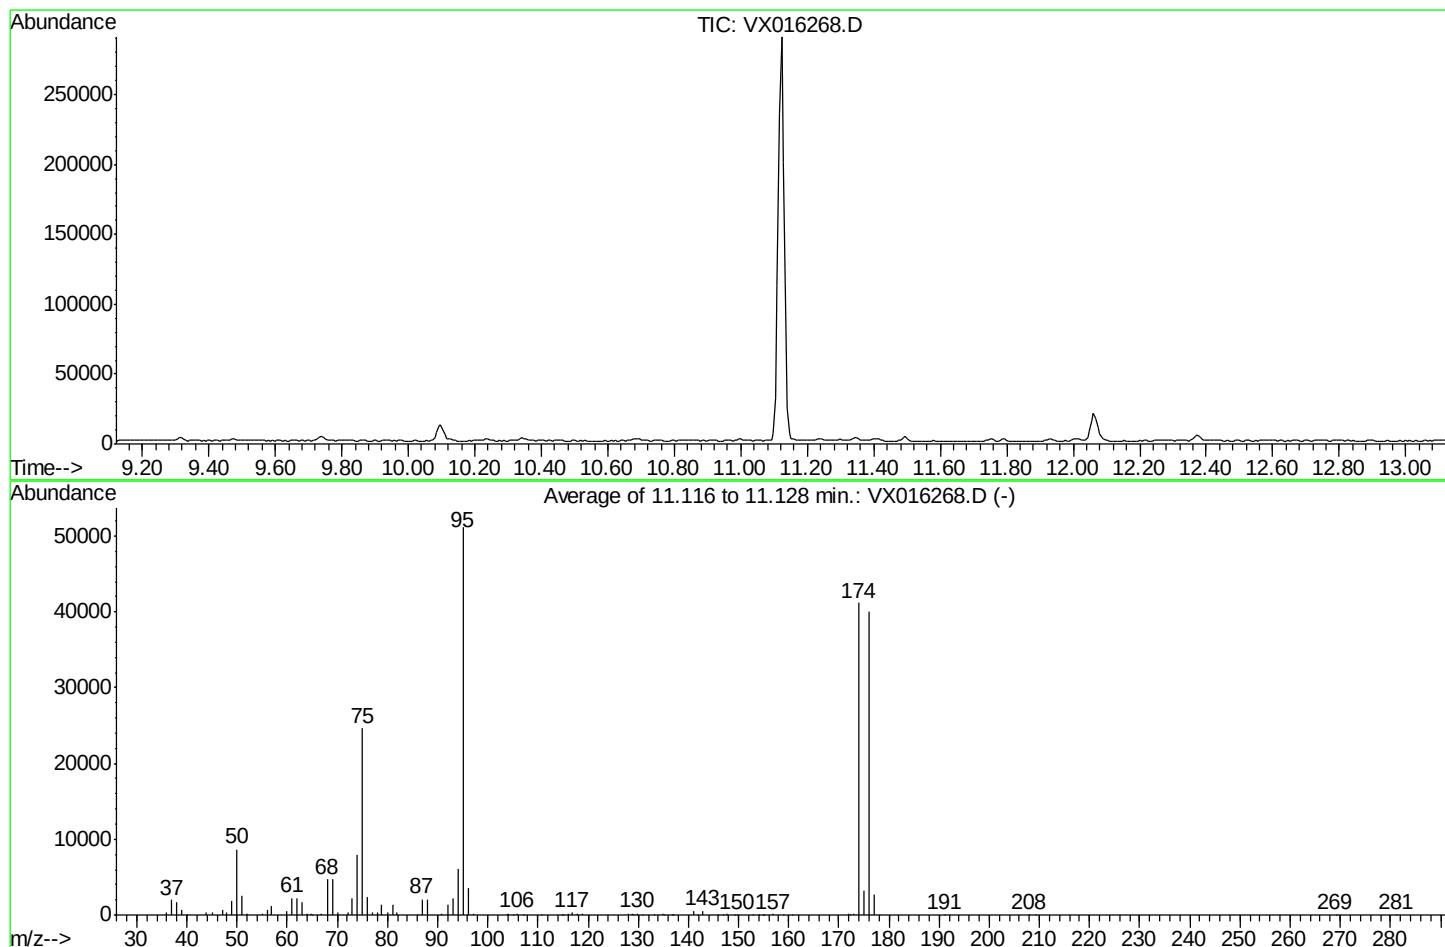

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8704	PASS
75	95	30	60	48.2	24645	PASS
95	95	100	100	100.0	51165	PASS
96	95	5	9	6.9	3532	PASS
173	174	0.00	2	0.6	254	PASS
174	95	50	100	80.4	41149	PASS
175	174	5	9	7.6	3140	PASS
176	174	95	101	97.4	40090	PASS
177	176	5	9	6.9	2761	PASS