

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX051521\  
 Data File : VX022004.D  
 Acq On : 14 May 2021 19:04  
 Operator : JC/MD  
 Sample : M2410-01  
 Misc : 25.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BG6M6

Quant Time: May 14 23:40:42 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR051021WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri May 14 23:38:54 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min)     |
|-------------------------------|--------|-------|----------|----------|-------|--------------|
| -----                         |        |       |          |          |       |              |
| Internal Standards            |        |       |          |          |       |              |
| 1) 1,4-Difluorobenzene        | 6.769  | 114   | 71055    | 5.00     | ug/L  | 0.00         |
| 28) Chlorobenzene-d5          | 10.055 | 117   | 65824    | 5.00     | ug/L  | 0.00         |
| 58) 1,4-Dichlorobenzene-d4    | 12.024 | 152   | 29725    | 5.00     | ug/L  | 0.00         |
| System Monitoring Compounds   |        |       |          |          |       |              |
| 4) Vinyl Chloride-d3          | 1.368  | 65    | 25438    | 4.17     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 83.40%       |
| 7) Chloroethane-d5            | 1.672  | 69    | 20526    | 4.20     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 84.00%       |
| 11) 1,1-Dichloroethene-d2     | 2.306  | 63    | 36465    | 3.60     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 72.00%       |
| 20) 2-Butanone-d5             | 4.471  | 46    | 60104    | 43.23    | ug/L  | 0.00         |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 86.46%       |
| 24) Chloroform-d              | 5.062  | 84    | 46025    | 4.39     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 87.80%       |
| 26) 1,2-Dichloroethane-d4     | 5.958  | 65    | 24436    | 4.54     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 90.80%       |
| 32) Benzene-d6                | 5.983  | 84    | 102530   | 4.70     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 94.00%       |
| 36) 1,2-Dichloropropane-d6    | 7.312  | 67    | 30187    | 4.51     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 90.20%       |
| 41) Toluene-d8                | 8.653  | 98    | 93913    | 4.74     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 94.80%       |
| 43) trans-1,3-Dichloroprop... | 8.952  | 79    | 12155    | 4.02     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 80.40%       |
| 46) 2-Hexanone-d5             | 9.390  | 63    | 53236    | 41.46    | ug/L  | 0.00         |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 82.92%       |
| 56) 1,1,2,2-Tetrachloroeth... | 11.195 | 84    | 20972    | 4.06     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 81.20%       |
| 66) 1,2-Dichlorobenzene-d4    | 12.323 | 152   | 29413    | 4.72     | ug/L  | 0.00         |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 94.40%       |
| Target Compounds              |        |       |          |          |       |              |
| 13) Acetone                   | 2.398  | 43    | 1592     | 2.24     | ug/L  | Qvalue<br>95 |
| -----                         |        |       |          |          |       |              |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX051521\  
Data File : VX022004.D  
Acq On : 14 May 2021 19:04  
Operator : JC/MD  
Sample : M2410-01  
Misc : 25.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BG6M6


Quant Time: May 14 23:40:42 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXTR051021WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri May 14 23:38:54 2021  
Response via : Initial Calibration

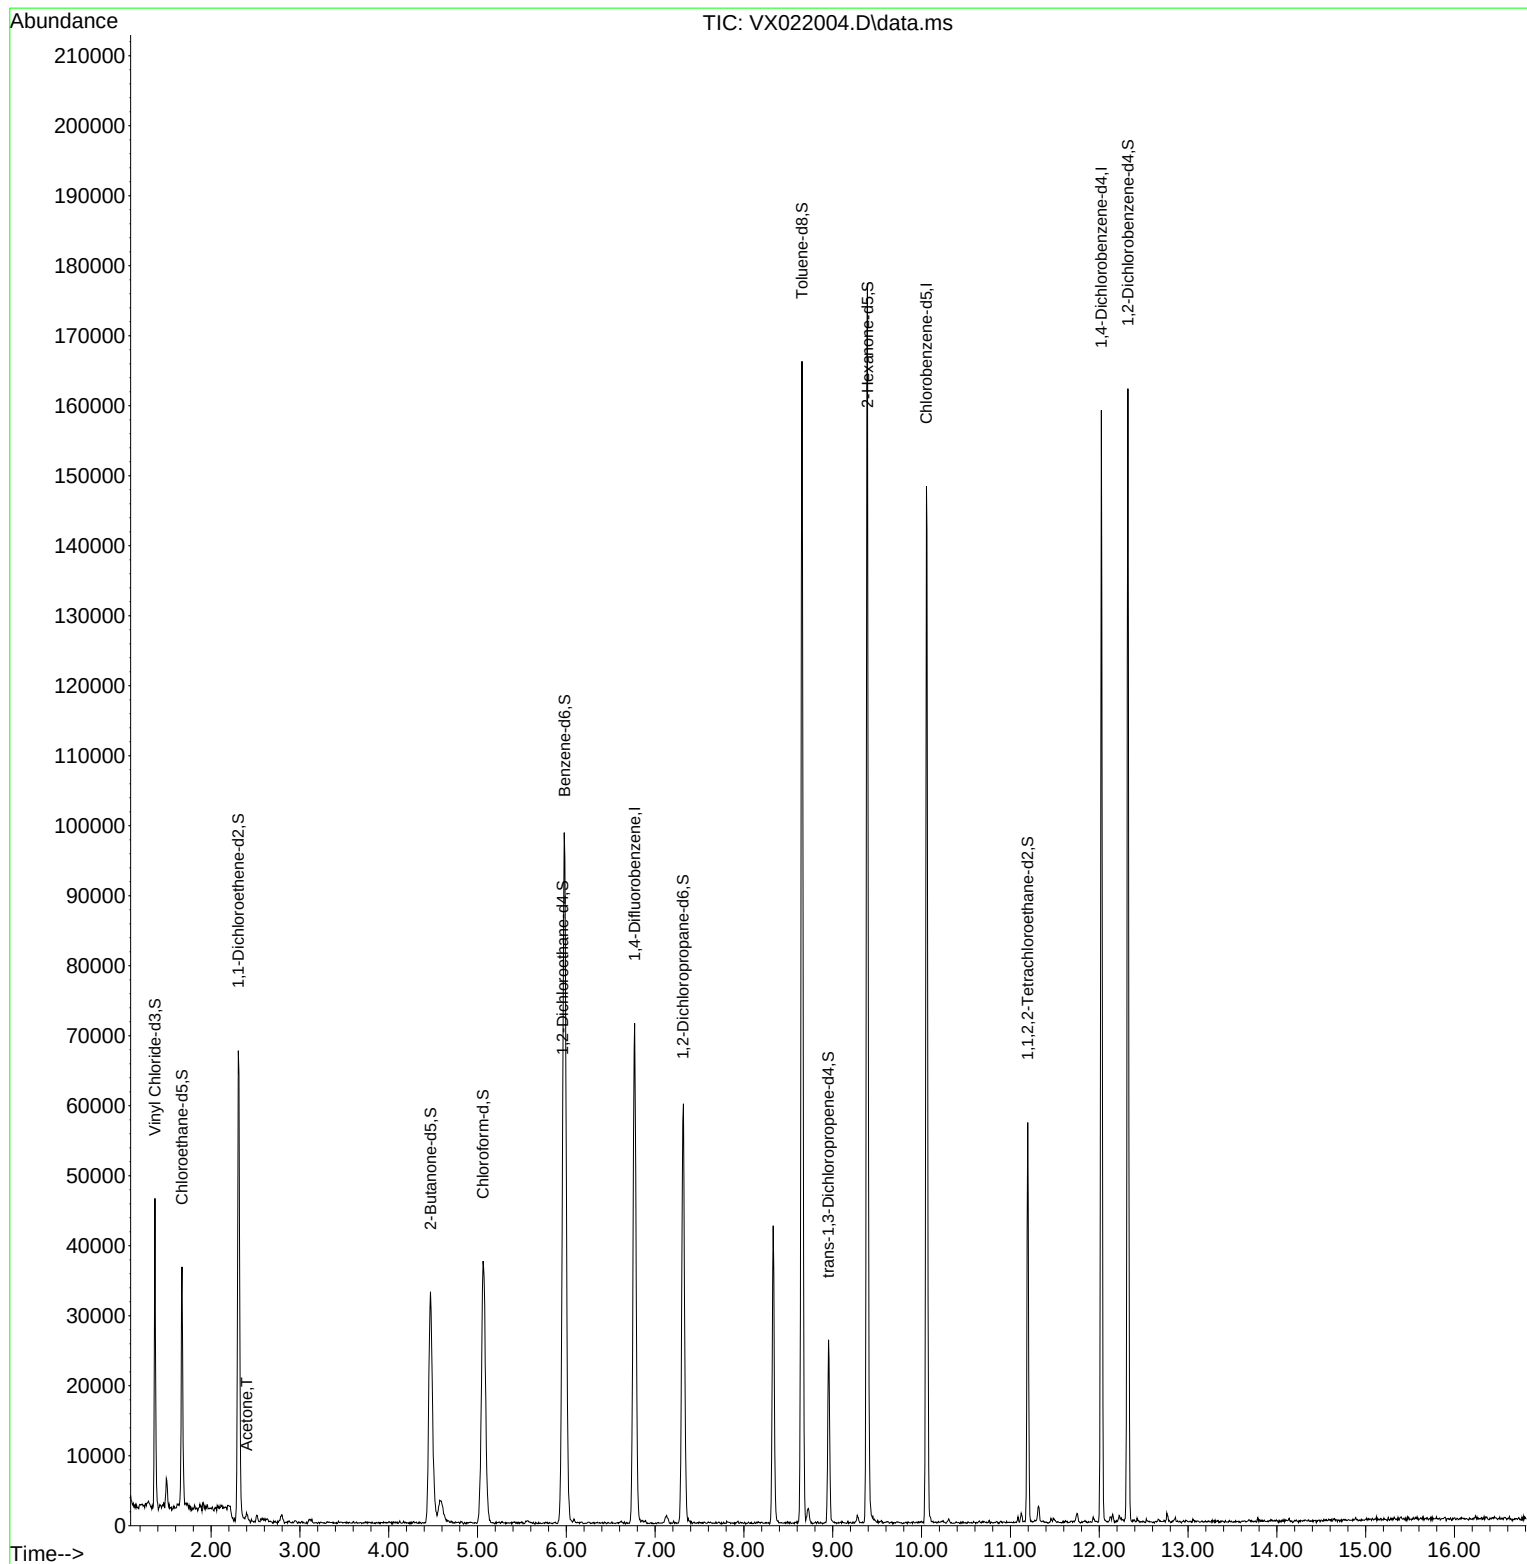

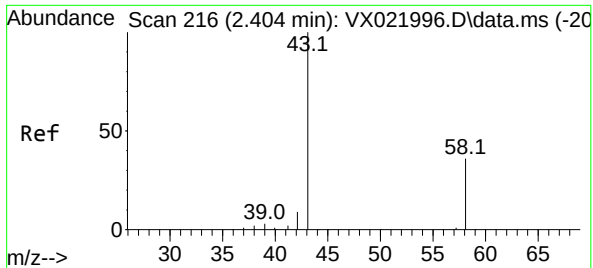

#13  
 Acetone  
 Concen: 2.24 ug/L  
 RT: 2.398 min Scan# 215  
 Delta R.T. -0.006 min  
 Lab File: VX022004.D  
 Acq: 14 May 2021 19:04

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BG6M6

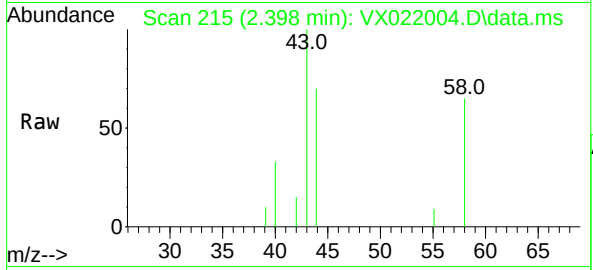

Tgt Ion: 43 Resp: 1592

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 43  | 100   |       |       |
| 58  | 30.5  | 0.0   | 66.4  |

