

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
 Data File : VX021999.D
 Acq On : 14 May 2021 17:09
 Operator : JC/MD
 Sample : M2410-12
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6N7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX021999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	47300	44826	15.31%	1.793%
2	1.672	91	96	106	rVB	33946	44337	15.15%	1.774%
3	2.312	195	201	210	rBV	66544	108010	36.90%	4.321%
4	2.404	210	216	224	rVB	4562	10362	3.54%	0.415%
5	2.788	275	279	286	rBV3	1946	3521	1.20%	0.141%
6	4.477	544	556	566	rBV2	31221	98640	33.70%	3.946%
7	4.593	566	575	591	rVB	16399	62186	21.24%	2.488%
8	5.062	638	652	666	rBV2	41902	139694	47.72%	5.588%
9	5.976	790	802	815	rBV3	99882	292739	100.00%	11.710%
10	6.769	923	932	942	rBV	72976	170202	58.14%	6.809%
11	7.135	986	992	1000	rVB4	8463	18783	6.42%	0.751%
12	7.312	1012	1021	1032	rBV2	59418	134630	45.99%	5.386%
13	8.330	1181	1188	1198	rBV	43672	71330	24.37%	2.853%
14	8.653	1234	1241	1248	rBV	178308	266233	90.95%	10.650%
15	8.720	1248	1252	1258	rVB2	5218	7759	2.65%	0.310%
16	8.952	1284	1290	1300	rVB	27184	41200	14.07%	1.648%
17	9.390	1356	1362	1374	rBV	180416	261949	89.48%	10.479%
18	10.055	1466	1471	1480	rVB	146782	200358	68.44%	8.015%
19	10.305	1505	1512	1516	rVB3	2619	3887	1.33%	0.155%
20	11.195	1653	1658	1664	rBV	57253	72409	24.74%	2.897%
21	11.317	1673	1678	1683	rVB4	2305	3963	1.35%	0.159%
22	11.756	1746	1750	1754	rVB2	2348	3167	1.08%	0.127%
23	12.024	1789	1794	1801	rBV	164268	196603	67.16%	7.865%
24	12.225	1822	1827	1833	rBV4	2550	5338	1.82%	0.214%
25	12.323	1836	1843	1849	rVV	167350	207033	70.72%	8.282%
26	13.250	1990	1995	2001	rBV3	2170	3387	1.16%	0.135%
27	14.134	2134	2140	2147	rBV	15606	20386	6.96%	0.816%
28	15.396	2339	2347	2353	rVB2	3892	6880	2.35%	0.275%


Sum of corrected areas: 2499812

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX021999.D
Acq On : 14 May 2021 17:09
Operator : JC/MD
Sample : M2410-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

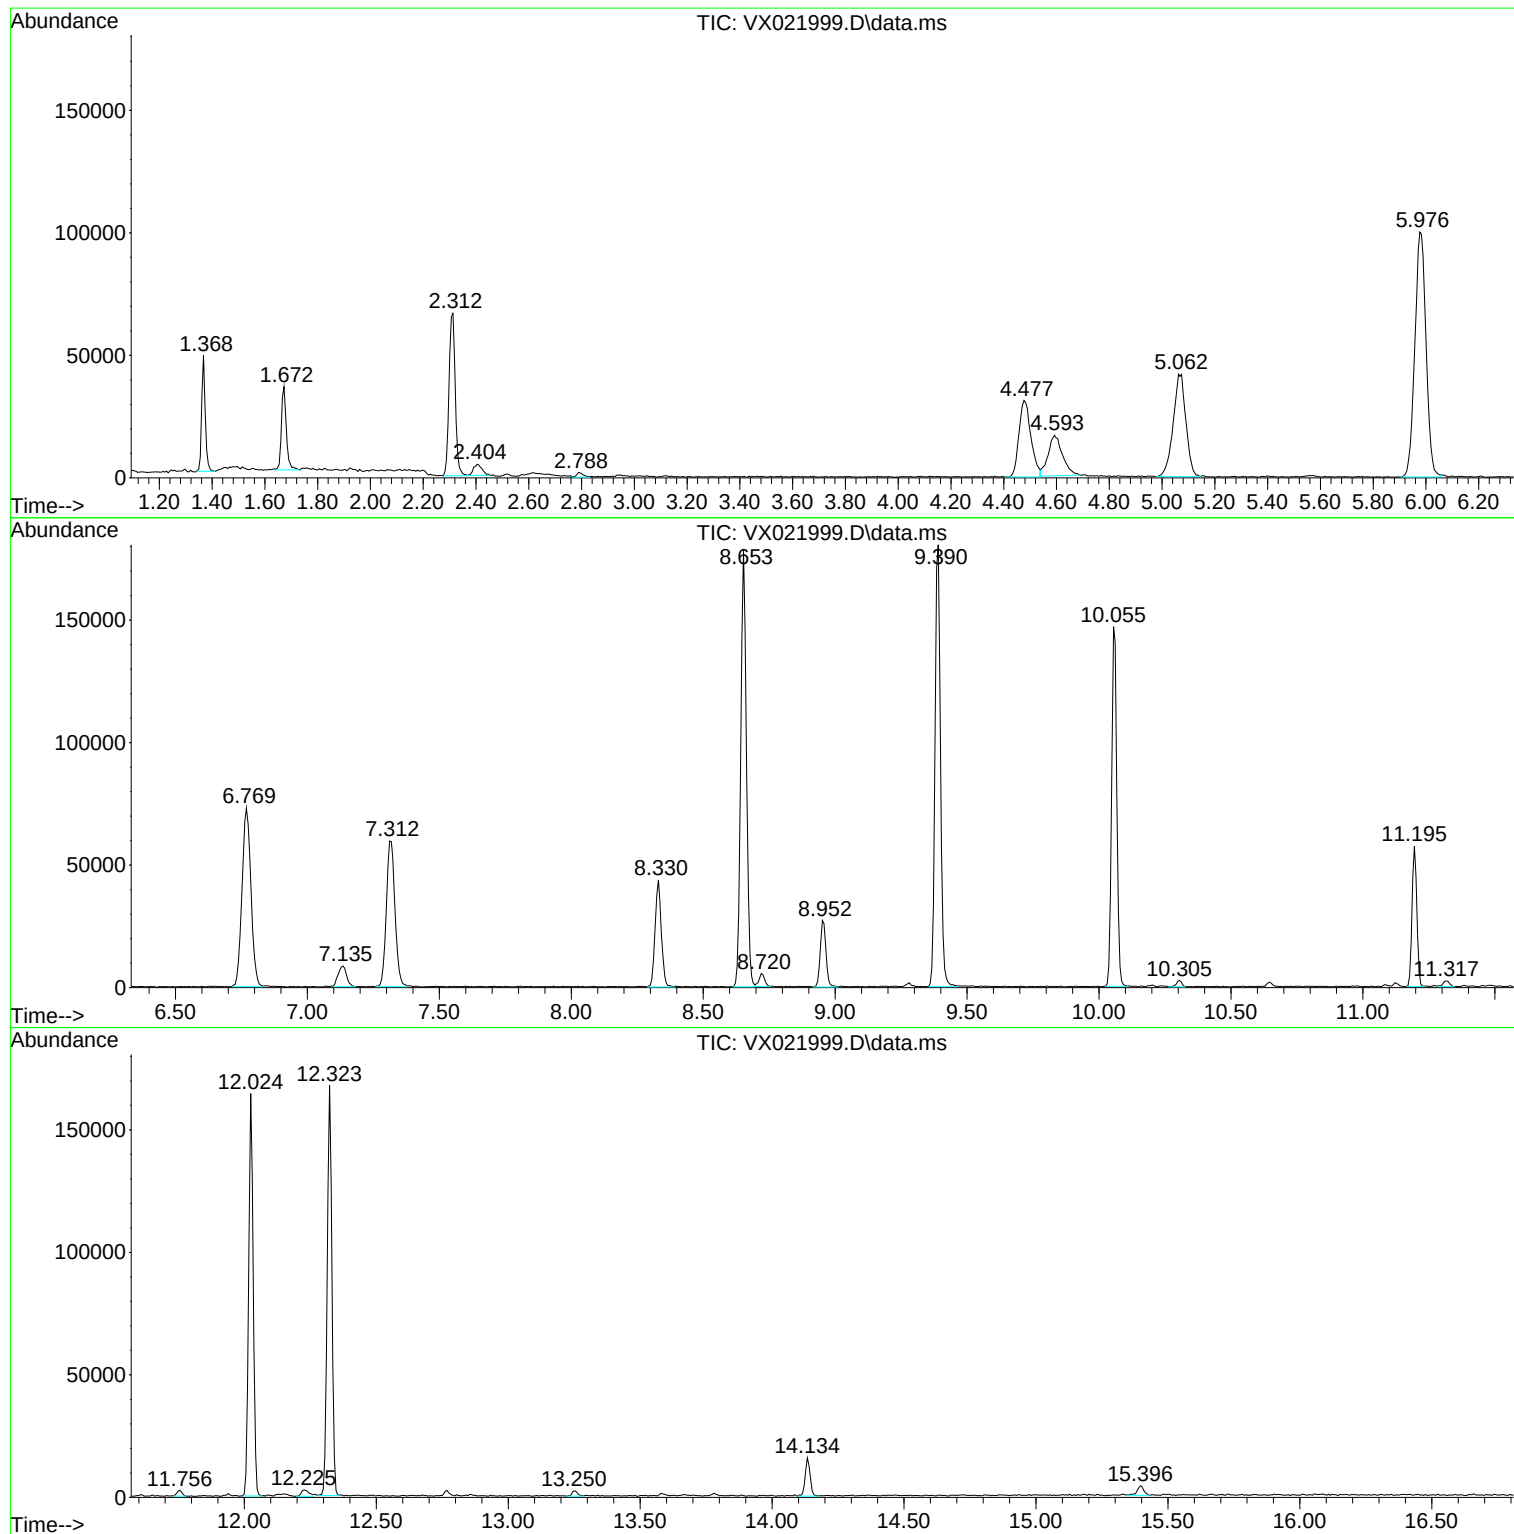

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX021999.D
Acq On : 14 May 2021 17:09
Operator : JC/MD
Sample : M2410-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX021999.D
Acq On : 14 May 2021 17:09
Operator : JC/MD
Sample : M2410-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
