

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
 Data File : VX022001.D
 Acq On : 14 May 2021 17:54
 Operator : JC/MD
 Sample : M2395-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW6E6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX022001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	52	rBV	44360	43963	14.83%	1.833%
2	1.440	52	58	59	rBV4	1743	3217	1.09%	0.134%
3	1.672	91	96	102	rVB	35935	41754	14.08%	1.741%
4	2.312	193	201	211	rVB	65435	107045	36.11%	4.464%
5	2.794	275	280	286	rBV2	2980	4877	1.65%	0.203%
6	4.470	544	555	567	rBV	35353	103136	34.79%	4.301%
7	5.068	642	653	667	rBV	41052	121664	41.04%	5.074%
8	5.982	789	803	815	rBV3	103640	296459	100.00%	12.363%
9	6.769	923	932	943	rBV	76360	178016	60.05%	7.424%
10	7.317	1011	1022	1036	rBV2	62561	138583	46.75%	5.779%
11	8.329	1181	1188	1196	rBV2	45168	70952	23.93%	2.959%
12	8.652	1235	1241	1248	rBV	174081	267153	90.11%	11.141%
13	8.720	1249	1252	1258	rVB3	2628	4161	1.40%	0.174%
14	8.951	1285	1290	1300	rVB	26784	40788	13.76%	1.701%
15	9.390	1355	1362	1372	rBV	182553	264767	89.31%	11.042%
16	10.055	1466	1471	1480	rBV	152487	210332	70.95%	8.772%
17	10.244	1498	1502	1507	rVB2	5464	7443	2.51%	0.310%
18	11.195	1653	1658	1665	rVB	56892	74667	25.19%	3.114%
19	11.317	1674	1678	1683	rVB2	2464	3645	1.23%	0.152%
20	12.024	1789	1794	1800	rBV	172205	207026	69.83%	8.634%
21	12.323	1836	1843	1849	rVB	166970	208243	70.24%	8.684%




Sum of corrected areas: 2397891

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022001.D
Acq On : 14 May 2021 17:54
Operator : JC/MD
Sample : M2395-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

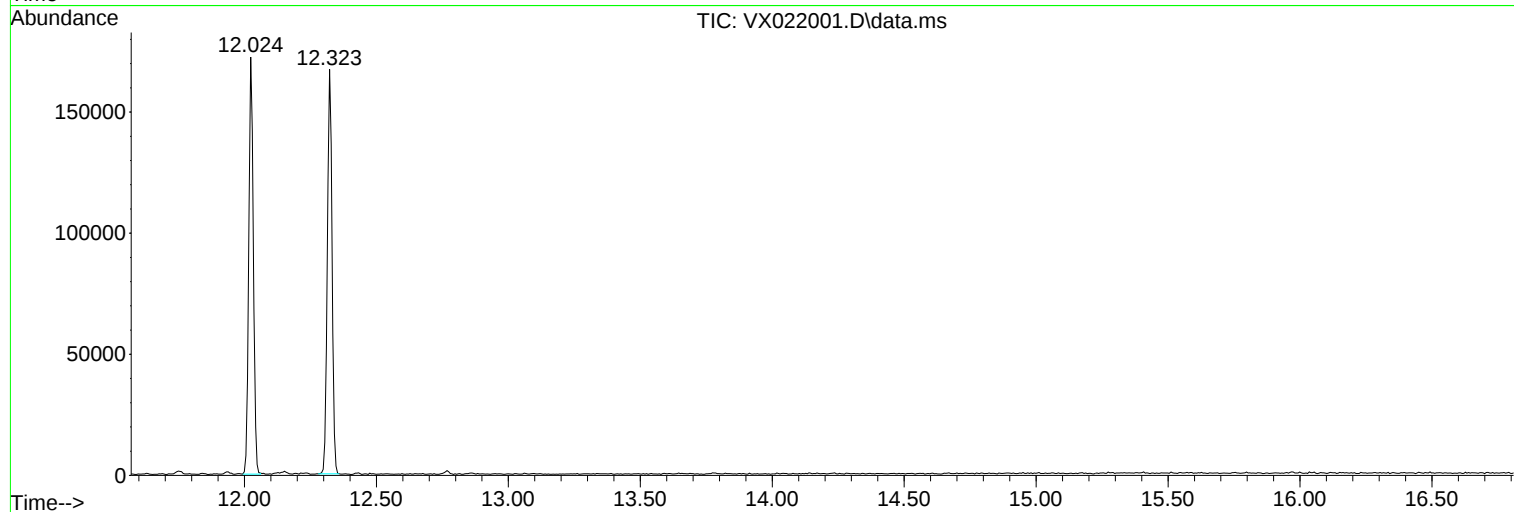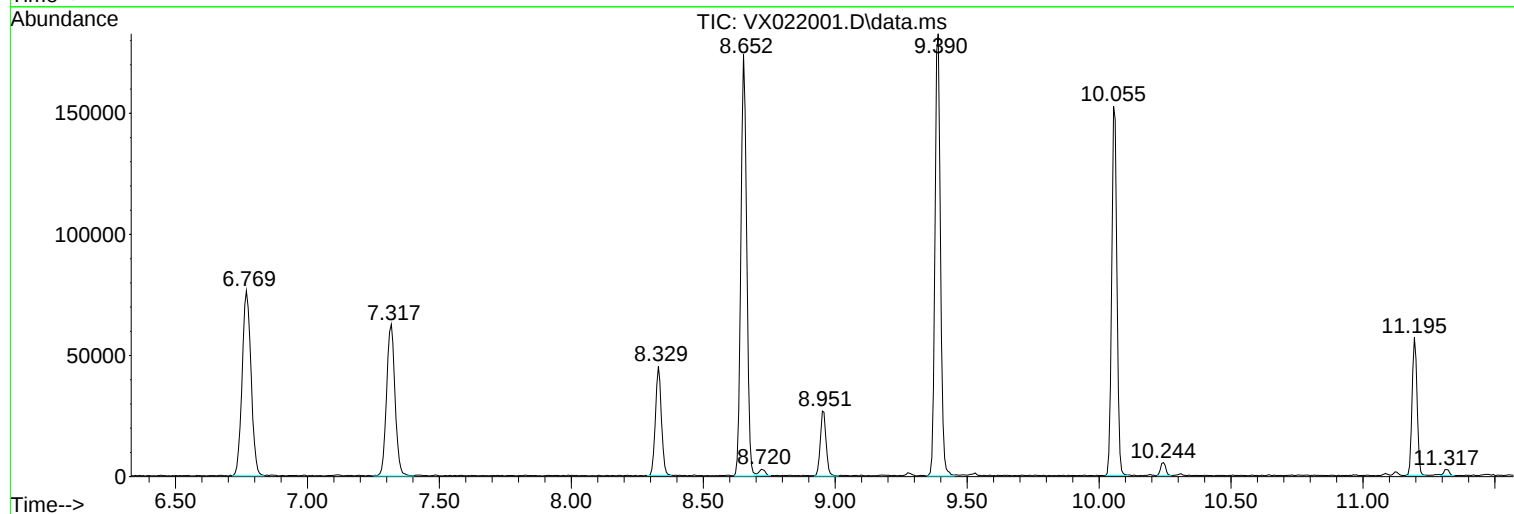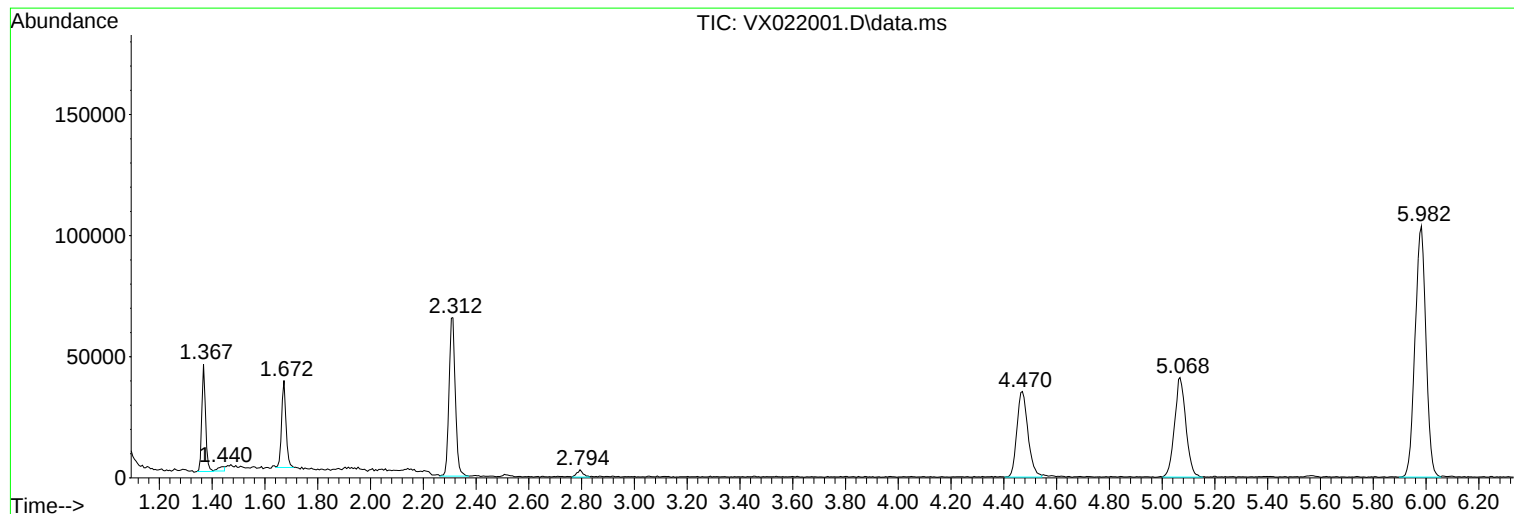

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022001.D
Acq On : 14 May 2021 17:54
Operator : JC/MD
Sample : M2395-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022001.D
Acq On : 14 May 2021 17:54
Operator : JC/MD
Sample : M2395-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
