

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
 Data File : VX022003.D
 Acq On : 14 May 2021 18:41
 Operator : JC/MD
 Sample : M2395-13
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW6E8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX022003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	51	rBV	43967	42801	14.95%	1.841%
2	1.672	92	96	104	rBV	35576	43075	15.04%	1.853%
3	2.306	194	200	210	rBV	67615	106072	37.04%	4.563%
4	2.794	274	280	286	rBV4	2997	5849	2.04%	0.252%
5	4.470	546	555	570	rBV	31368	98530	34.41%	4.238%
6	5.062	641	652	665	rBV	39621	121396	42.39%	5.222%
7	5.976	790	802	817	rBV3	97371	286374	100.00%	12.318%
8	6.769	922	932	944	rBV	73890	175465	61.27%	7.548%
9	7.317	1013	1022	1031	rBV	59740	133087	46.47%	5.725%
10	8.329	1181	1188	1200	rBV	42363	69487	24.26%	2.989%
11	8.653	1235	1241	1249	rBV	168456	257170	89.80%	11.062%
12	8.720	1249	1252	1257	rVB2	2825	4061	1.42%	0.175%
13	8.951	1285	1290	1299	rBV	26650	39454	13.78%	1.697%
14	9.390	1356	1362	1372	rBV	177386	256565	89.59%	11.036%
15	10.055	1466	1471	1481	rVB	147431	204193	71.30%	8.783%
16	10.244	1498	1502	1506	rVB2	2935	3864	1.35%	0.166%
17	11.195	1653	1658	1666	rVB	61207	73180	25.55%	3.148%
18	11.311	1674	1677	1682	rVB3	2206	3011	1.05%	0.130%
19	12.024	1788	1794	1800	rBV	163064	200377	69.97%	8.619%
20	12.323	1836	1843	1850	rBV	166299	200788	70.11%	8.637%




Sum of corrected areas: 2324799

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022003.D
Acq On : 14 May 2021 18:41
Operator : JC/MD
Sample : M2395-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

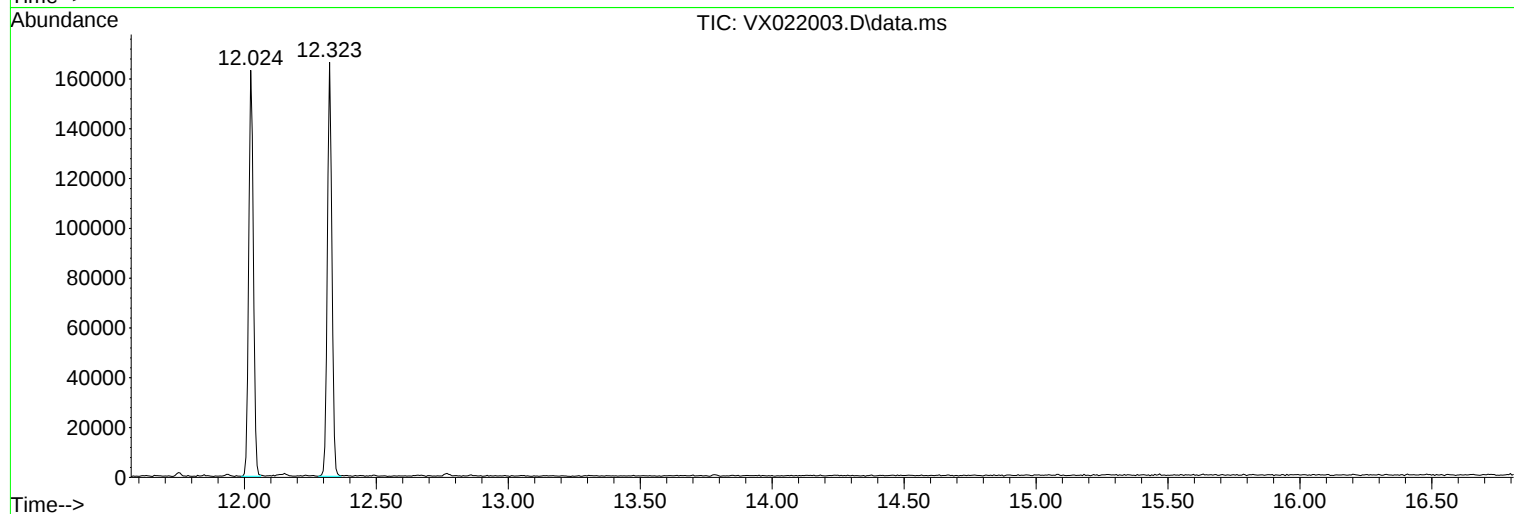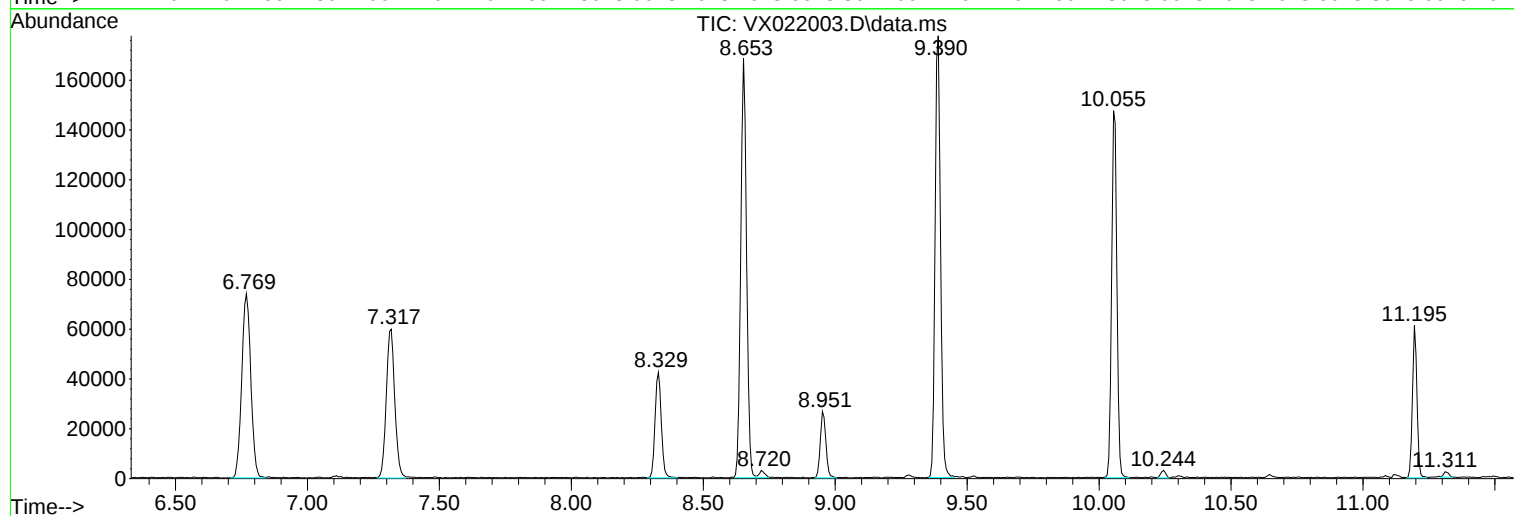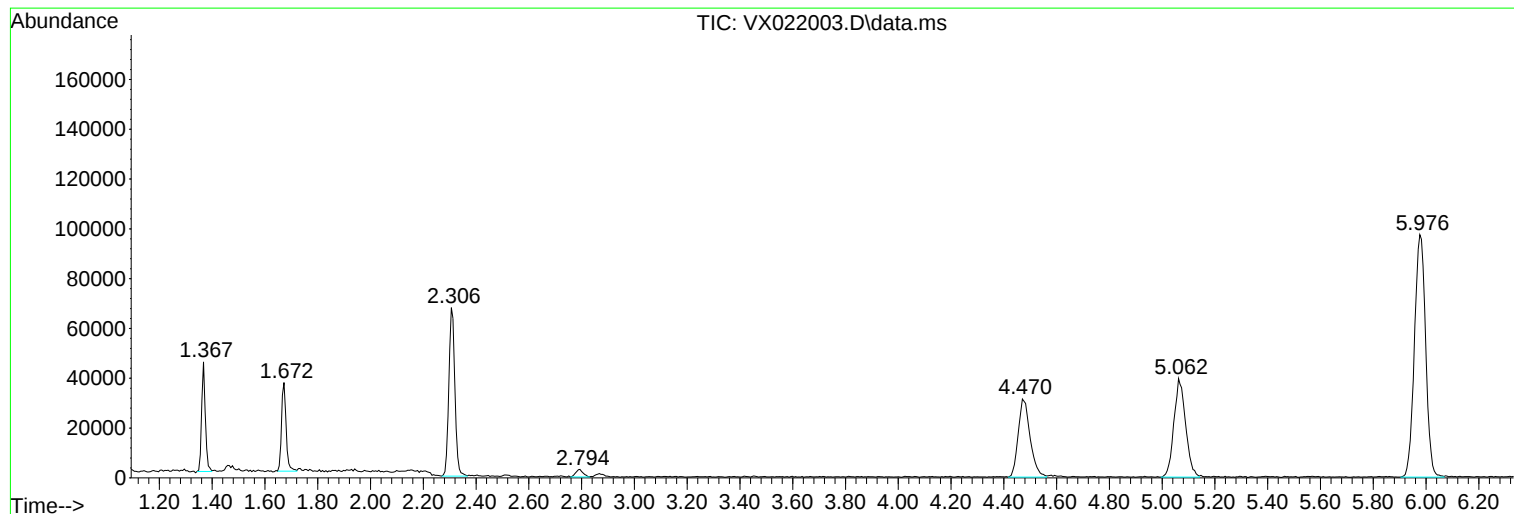

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022003.D
Acq On : 14 May 2021 18:41
Operator : JC/MD
Sample : M2395-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022003.D
Acq On : 14 May 2021 18:41
Operator : JC/MD
Sample : M2395-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
