

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
 Data File : VX022004.D
 Acq On : 14 May 2021 19:04
 Operator : JC/MD
 Sample : M2410-01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6M6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX022004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	44509	43501	15.33%	1.893%
2	1.496	64	67	73	rVB3	4329	6171	2.17%	0.268%
3	1.672	91	96	101	rBV	34026	41566	14.65%	1.808%
4	2.306	194	200	210	rBV	67263	105980	37.34%	4.611%
5	4.471	545	555	567	rBV	33031	96939	34.16%	4.217%
6	4.574	567	572	574	rBV3	2165	3712	1.31%	0.161%
7	5.062	640	652	669	rBV	37492	118795	41.86%	5.168%
8	5.976	789	802	817	rBV3	98733	283802	100.00%	12.347%
9	6.769	922	932	943	rBV	71452	168845	59.49%	7.346%
10	7.129	983	991	998	rVB3	1196	2898	1.02%	0.126%
11	7.318	1012	1022	1030	rBV	59889	129202	45.53%	5.621%
12	8.330	1181	1188	1196	rBV	42629	69565	24.51%	3.026%
13	8.653	1233	1241	1248	rBV	166041	255154	89.91%	11.100%
14	8.726	1248	1253	1258	rVB	2117	4076	1.44%	0.177%
15	8.952	1285	1290	1296	rBV	26113	37707	13.29%	1.640%
16	9.390	1354	1362	1374	rBV	177078	254236	89.58%	11.060%
17	10.055	1466	1471	1480	rBV	148062	202507	71.36%	8.810%
18	11.195	1653	1658	1663	rBV	57024	70586	24.87%	3.071%
19	11.317	1673	1678	1684	rVB3	2221	3398	1.20%	0.148%
20	12.024	1789	1794	1804	rVB	158810	196938	69.39%	8.568%
21	12.323	1836	1843	1851	rVB	161894	203019	71.54%	8.832%


Sum of corrected areas: 2298597

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022004.D
Acq On : 14 May 2021 19:04
Operator : JC/MD
Sample : M2410-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

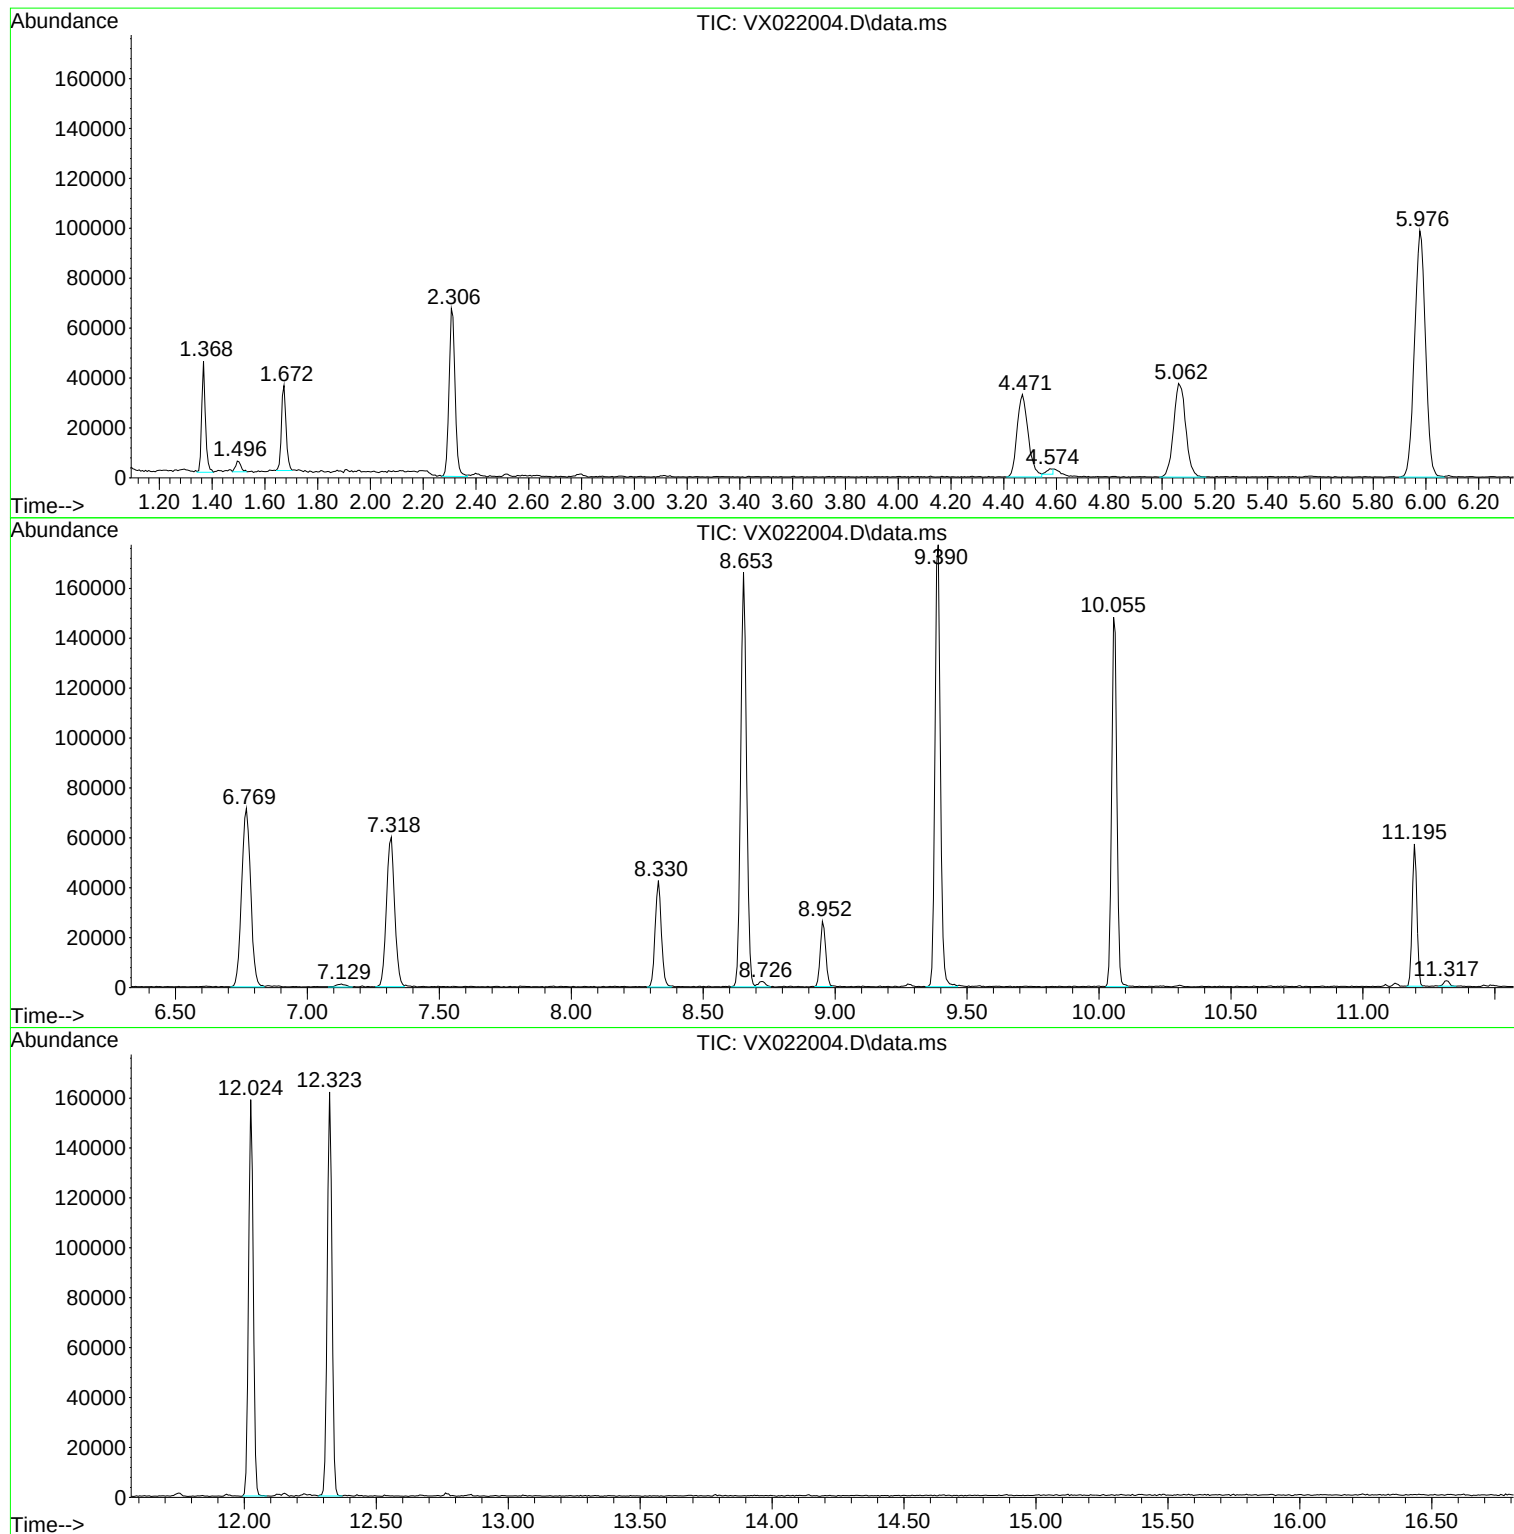

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022004.D
Acq On : 14 May 2021 19:04
Operator : JC/MD
Sample : M2410-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022004.D
Acq On : 14 May 2021 19:04
Operator : JC/MD
Sample : M2410-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
