

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
 Data File : VX022011.D
 Acq On : 14 May 2021 21:48
 Operator : JC/MD
 Sample : M2410-08
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6N3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX022011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rVB	41416	40807	2.21%	0.960%
2	1.672	92	96	101	rBV	32171	38545	2.09%	0.907%
3	2.306	194	200	211	rVB2	64338	112007	6.07%	2.635%
4	3.617	407	415	425	rVB2	13105	30831	1.67%	0.725%
5	4.483	546	557	570	rBV	33465	114471	6.20%	2.693%
6	5.068	639	653	670	rBV5	38019	136209	7.38%	3.204%
7	5.385	696	705	717	rBV3	7067	21289	1.15%	0.501%
8	5.976	788	802	815	rBV4	96726	278419	15.09%	6.550%
9	6.769	921	932	948	rBV	69379	165886	8.99%	3.903%
10	7.129	981	991	1008	rBV	845371	1844840	100.00%	43.401%
11	7.312	1013	1021	1033	rVB	57698	130917	7.10%	3.080%
12	8.330	1182	1188	1202	rBV2	39988	66580	3.61%	1.566%
13	8.653	1233	1241	1249	rBV	163999	254093	13.77%	5.978%
14	8.952	1284	1290	1297	rBV	25017	36708	1.99%	0.864%
15	9.275	1337	1343	1352	rVB	45733	69737	3.78%	1.641%
16	9.390	1356	1362	1373	rVV	179920	251958	13.66%	5.927%
17	10.055	1466	1471	1480	rBV	143695	196830	10.67%	4.631%
18	11.195	1653	1658	1663	rBV	56262	70440	3.82%	1.657%
19	12.024	1789	1794	1800	rBV	155601	192141	10.42%	4.520%
20	12.323	1838	1843	1850	rVB	157318	198020	10.73%	4.658%




Sum of corrected areas: 4250728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022011.D
Acq On : 14 May 2021 21:48
Operator : JC/MD
Sample : M2410-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

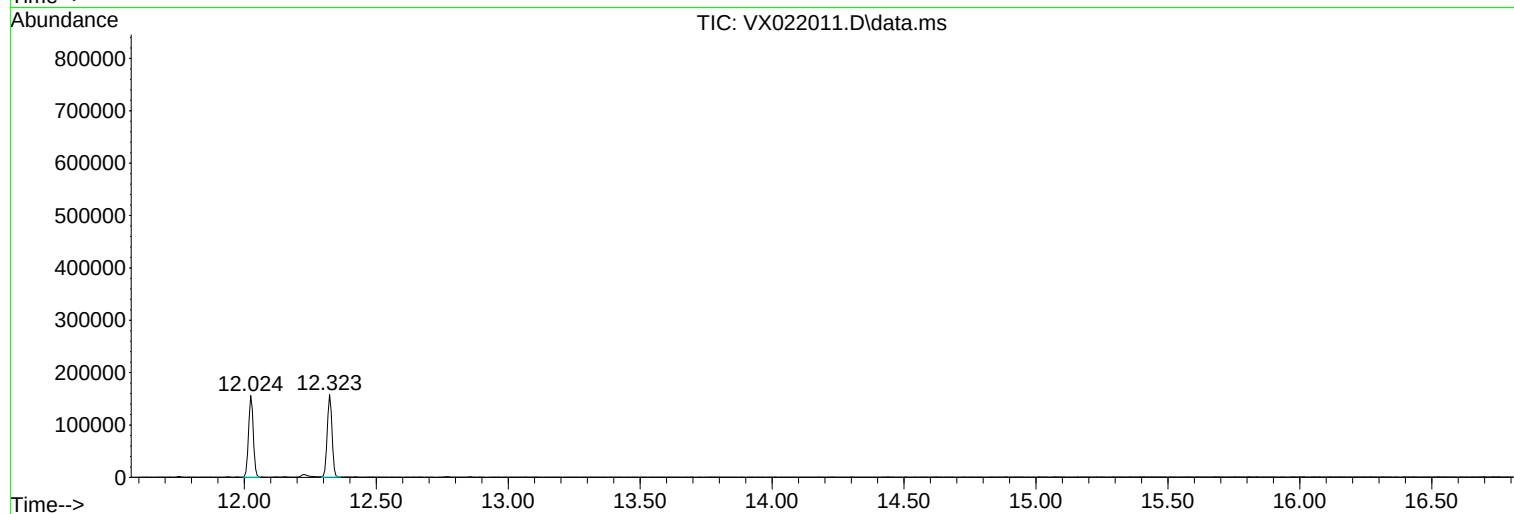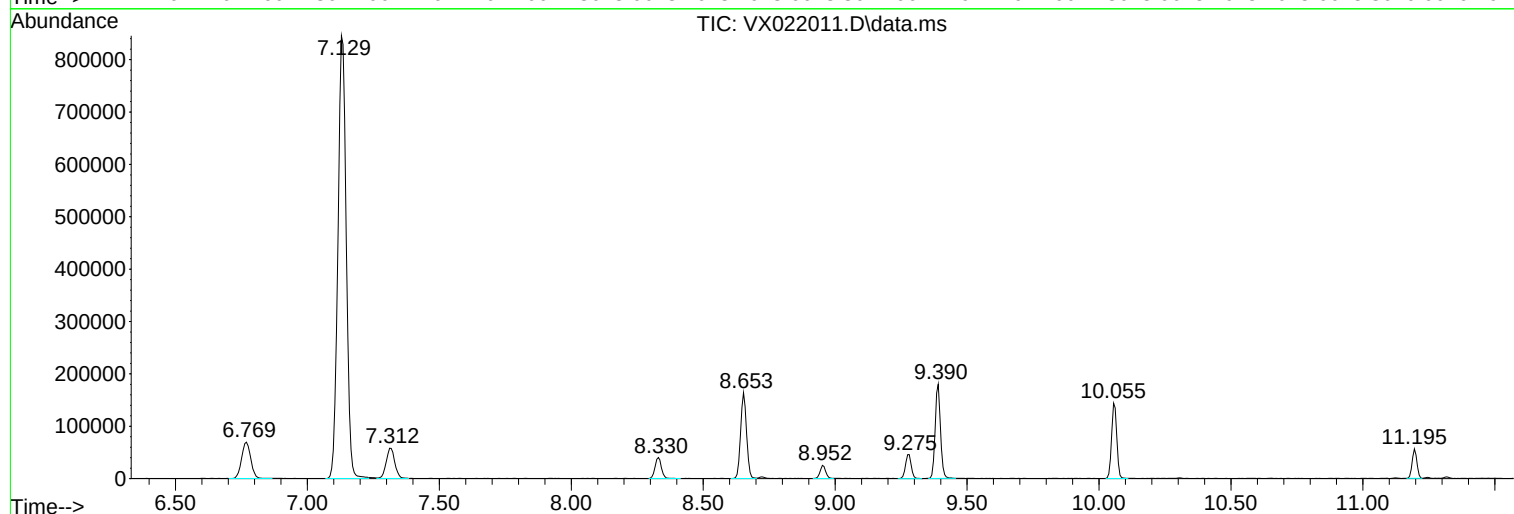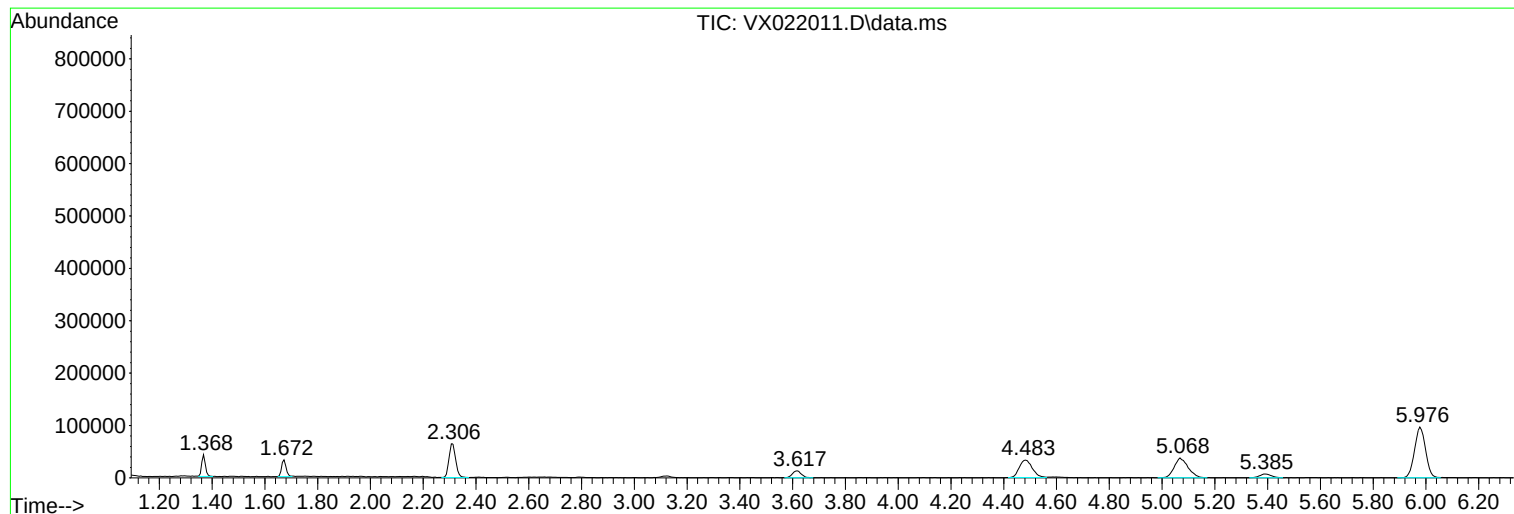

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022011.D
Acq On : 14 May 2021 21:48
Operator : JC/MD
Sample : M2410-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
Data File : VX022011.D
Acq On : 14 May 2021 21:48
Operator : JC/MD
Sample : M2410-08
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------