
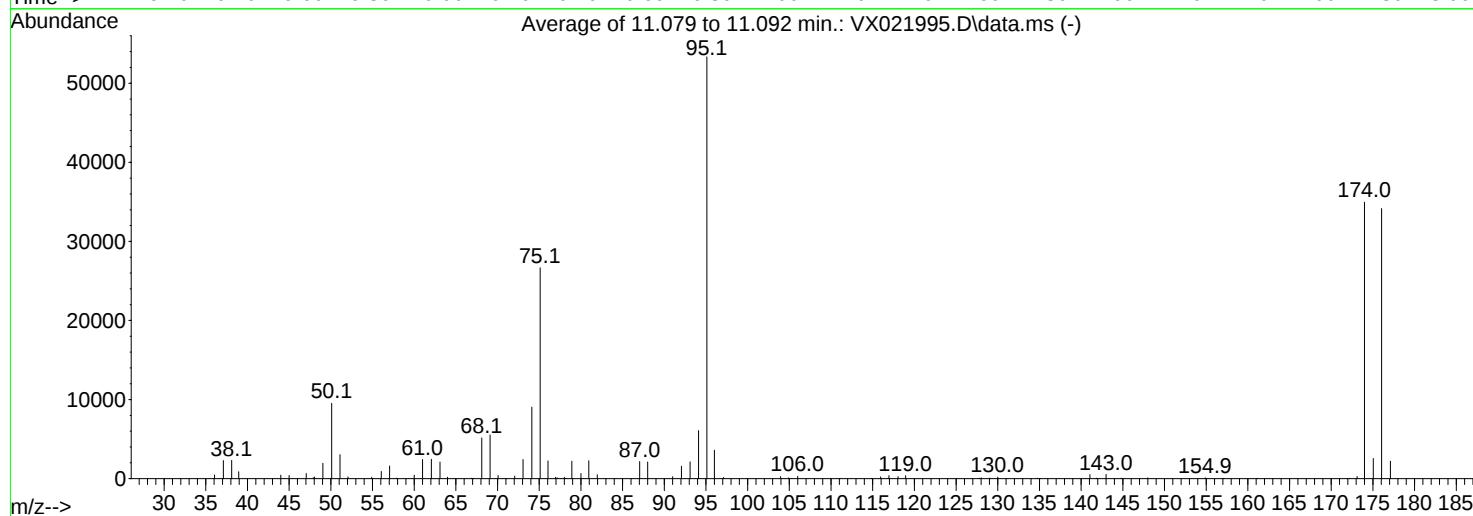


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051521\
 Data File : VX021995.D
 Acq On : 14 May 2021 15:11
 Operator : JC/MD
 Sample : BFB72
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB172

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri May 14 23:38:54 2021

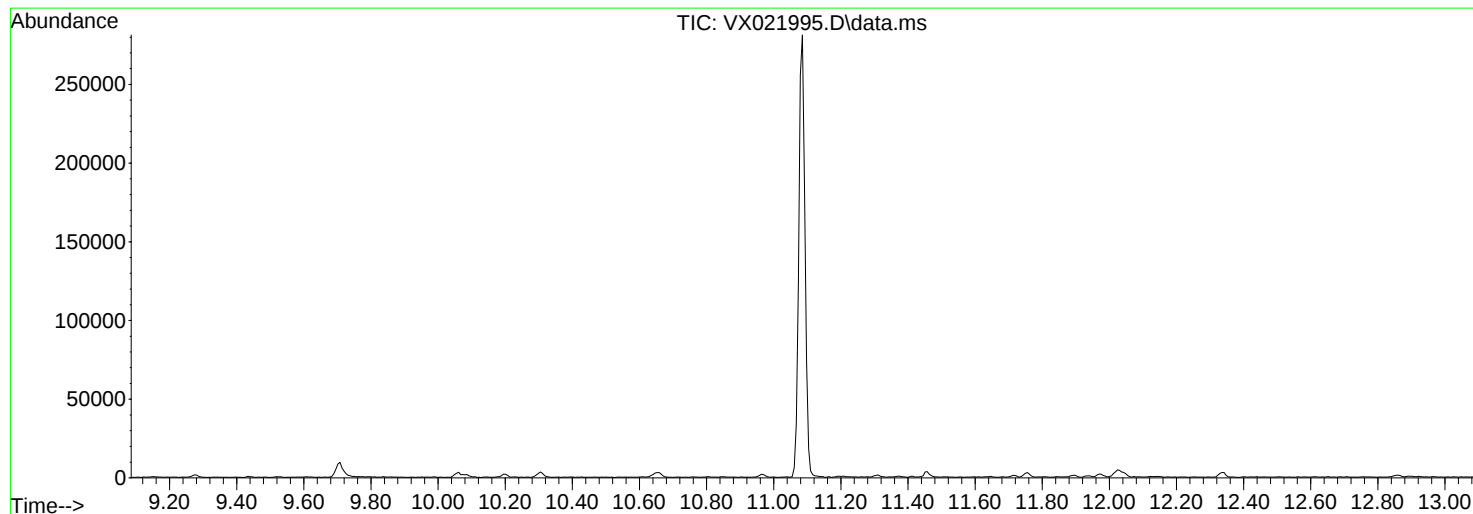

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9526	PASS
75	95	30	80	50.0	26675	PASS
95	95	100	100	100.0	53336	PASS
96	95	5	9	6.8	3604	PASS
173	174	0.00	2	0.8	280	PASS
174	95	50	120	65.5	34955	PASS
175	174	5	9	7.3	2550	PASS
176	174	95	105	97.7	34160	PASS
177	176	5	10	6.4	2198	PASS

m/z	Abundance
38.90	52.0
39.90	94.0
40.90	63.0
43.10	59.0
43.90	314.0

Instrument :
MSVOA_X
ClientSampleId :
BFB172

m/z	Abundance
36.00	559.0
37.10	2886.0
38.10	2893.0
39.00	1066.0
40.10	114.0
44.10	976.0
45.00	497.0
47.10	917.0
47.90	359.0
49.10	2173.0
50.10	11120.0
51.10	3729.0
52.10	315.0
55.00	176.0
56.10	1257.0
57.10	1646.0
57.90	117.0
60.00	471.0
61.00	2753.0
62.00	2845.0
63.10	2787.0
64.00	250.0
67.00	125.0
68.10	5931.0
69.10	6415.0
70.10	526.0
72.00	349.0
73.10	2862.0
74.10	9906.0
75.10	29848.0
76.10	2750.0
77.00	233.0
78.00	243.0
78.90	2402.0
80.00	722.0
81.00	2459.0
81.90	471.0
83.00	63.0
87.10	2039.0
88.00	2483.0
91.00	277.0
92.10	1600.0
93.10	2494.0
94.10	6553.0
95.10	58248.0
96.00	4286.0
97.10	170.0
103.90	328.0
104.90	115.0
106.00	302.0
111.10	64.0
114.80	60.0
116.00	163.0
117.00	356.0
118.00	251.0
118.90	443.0
127.80	166.0
129.10	59.0
130.00	227.0
135.10	64.0
141.10	507.0
141.90	109.0
143.00	537.0
144.80	99.0
147.90	76.0
154.90	159.0
157.10	81.0
161.20	55.0
171.90	73.0
173.10	262.0
174.00	32072.0
175.10	2522.0
176.00	31008.0
177.10	2138.0

Instrument :
MSVOA_X
ClientSampleId :
BFB172

m/z	Abundance
36.10	514.0
37.10	2605.0
38.10	2503.0
39.00	1090.0
39.90	131.0
42.90	65.0
44.10	841.0
45.00	355.0
47.00	700.0
48.10	380.0
49.00	2316.0
50.10	10814.0
51.10	3391.0
52.00	302.0
54.90	181.0
56.00	894.0
57.00	1862.0
57.90	54.0
60.00	617.0
61.00	2828.0
62.10	2940.0
63.10	2204.0
64.10	182.0
66.80	86.0
68.10	5792.0
69.10	6876.0
70.10	397.0
71.10	54.0
72.10	391.0
73.00	2531.0
74.10	10706.0
75.10	31248.0
76.00	2660.0
76.90	229.0
77.20	211.0
78.00	317.0
78.90	2634.0
80.00	758.0
80.90	2698.0
82.00	575.0
87.00	2621.0
88.00	2343.0
91.00	291.0
92.00	1745.0
93.10	2534.0
94.10	7037.0
95.10	61488.0
96.00	3924.0
97.10	181.0
104.00	340.0
104.90	166.0
106.00	343.0
111.10	65.0
114.90	63.0
115.90	242.0
116.90	394.0
118.10	252.0
119.00	423.0
128.10	161.0
129.00	70.0
130.00	229.0
131.10	75.0
134.80	101.0
141.00	559.0
141.80	82.0
143.00	538.0
144.80	56.0
148.00	137.0
154.90	88.0
157.10	63.0
161.10	74.0
172.20	104.0
173.10	386.0
174.00	41904.0
175.10	2975.0
176.10	40776.0
177.10	2627.0

Instrument :
MSVOA_X
ClientSampleId :
BFB172

m/z	Abundance
36.00	342.0
37.10	1351.0
38.00	1525.0
39.10	623.0
40.10	125.0
44.10	450.0
45.00	375.0
47.10	352.0
48.00	223.0
49.10	1324.0
50.10	6645.0
51.10	1981.0
51.90	73.0
54.80	110.0
56.00	594.0
57.10	1312.0
60.10	247.0
61.00	1684.0
62.10	1569.0
63.10	1344.0
63.90	119.0
67.10	124.0
68.10	3703.0
69.00	3297.0
70.00	320.0
72.10	215.0
73.00	1912.0
74.10	6538.0
75.10	18928.0
76.00	1357.0
77.10	145.0
77.60	132.0
78.20	131.0
79.00	1551.0
80.00	483.0
80.90	1663.0
81.90	446.0
87.00	1843.0
88.00	1512.0
91.10	188.0
92.10	1314.0
93.00	1369.0
94.10	4598.0
95.10	40272.0
96.10	2603.0
97.00	63.0
104.00	151.0
106.00	249.0
115.90	253.0
117.00	396.0
118.00	263.0
119.00	314.0
128.00	121.0
129.00	99.0
130.00	145.0
134.80	71.0
141.00	456.0
143.00	563.0
148.10	96.0
154.90	59.0
173.00	192.0
174.00	30888.0
175.00	2152.0
176.10	30696.0
177.10	1828.0

Instrument :
MSVOA_X
ClientSampleId :
BFB172