

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051523\
 Data File : VX035653.D
 Acq On : 15 May 2023 10:21
 Operator : JC/MD
 Sample : VX0515MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0515MBL01

Quant Time: May 16 04:54:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.549	168	206102	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	377365	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	344239	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	156932	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	168830	46.956	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	93.920%		
35) Dibromofluoromethane	5.379	113	124484	48.914	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.820%		
50) Toluene-d8	8.646	98	457820	48.696	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.400%		
62) 4-Bromofluorobenzene	11.079	95	187891	49.634	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.260%		
Target Compounds						Qvalue
3) Chloromethane	1.294	50	677	0.208	ug/l	99
5) Bromomethane	1.611	94	313	0.209	ug/l #	43
11) Tert butyl alcohol	2.934	59	170	0.268	ug/l #	73
13) Acrolein	2.245	56	618	0.821	ug/l	91
15) Acrylonitrile	3.074	53	629	0.450	ug/l #	75
16) Acetone	2.404	43	1106	0.716	ug/l	99
17) Carbon Disulfide	2.513	76	2299	0.415	ug/l #	85
20) Methylene Chloride	2.782	84	618	0.221	ug/l	86
31) Cyclohexane	5.543	56	5879	1.294	ug/l #	27
36) 1,1-Dichloropropene	5.543	75	19696	4.903	ug/l #	50
38) Carbon Tetrachloride	5.543	117	23430	6.157	ug/l #	16
49) 1,4-Dioxane	7.744	88	411	7.138	ug/l #	61
68) m/p-Xylenes	10.305	106	1136	0.217	ug/l	83
76) 1,2,3-Trichloropropane	11.079	75	101161	26.354	ug/l #	34
80) 1,3,5-Trimethylbenzene	11.451	105	2346	0.209	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.079	75	101161	84.934	ug/l #	8
82) 4-Chlorotoluene	11.457	91	2326	0.208	ug/l	98
83) tert-Butylbenzene	11.713	119	2226	0.204	ug/l	93
84) 1,2,4-Trimethylbenzene	11.749	105	2606	0.231	ug/l	92
85) sec-Butylbenzene	11.890	105	2966	0.216	ug/l	97
86) p-Isopropyltoluene	12.006	119	2672	0.237	ug/l #	75
87) 1,3-Dichlorobenzene	11.969	146	1548	0.271	ug/l	90
88) 1,4-Dichlorobenzene	11.969	146	1548	0.269	ug/l	90
89) n-Butylbenzene	12.329	91	2795	0.272	ug/l	97
90) Hexachloroethane	12.542	117	349	0.204	ug/l	87
91) 1,2-Dichlorobenzene	12.335	146	1462	0.262	ug/l	95
93) 1,2,4-Trichlorobenzene	13.585	180	1978	0.588	ug/l	94
94) Hexachlorobutadiene	13.719	225	1181	0.885	ug/l	88
95) Naphthalene	13.774	128	6023	0.523	ug/l	98
96) 1,2,3-Trichlorobenzene	13.956	180	2161	0.654	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051523\
Data File : VX035653.D
Acq On : 15 May 2023 10:21
Operator : JC/MD
Sample : VX0515MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01

Quant Time: May 16 04:54:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260
QLast Update : Thu May 11 13:57:54 2023
Response via : Initial Calibration




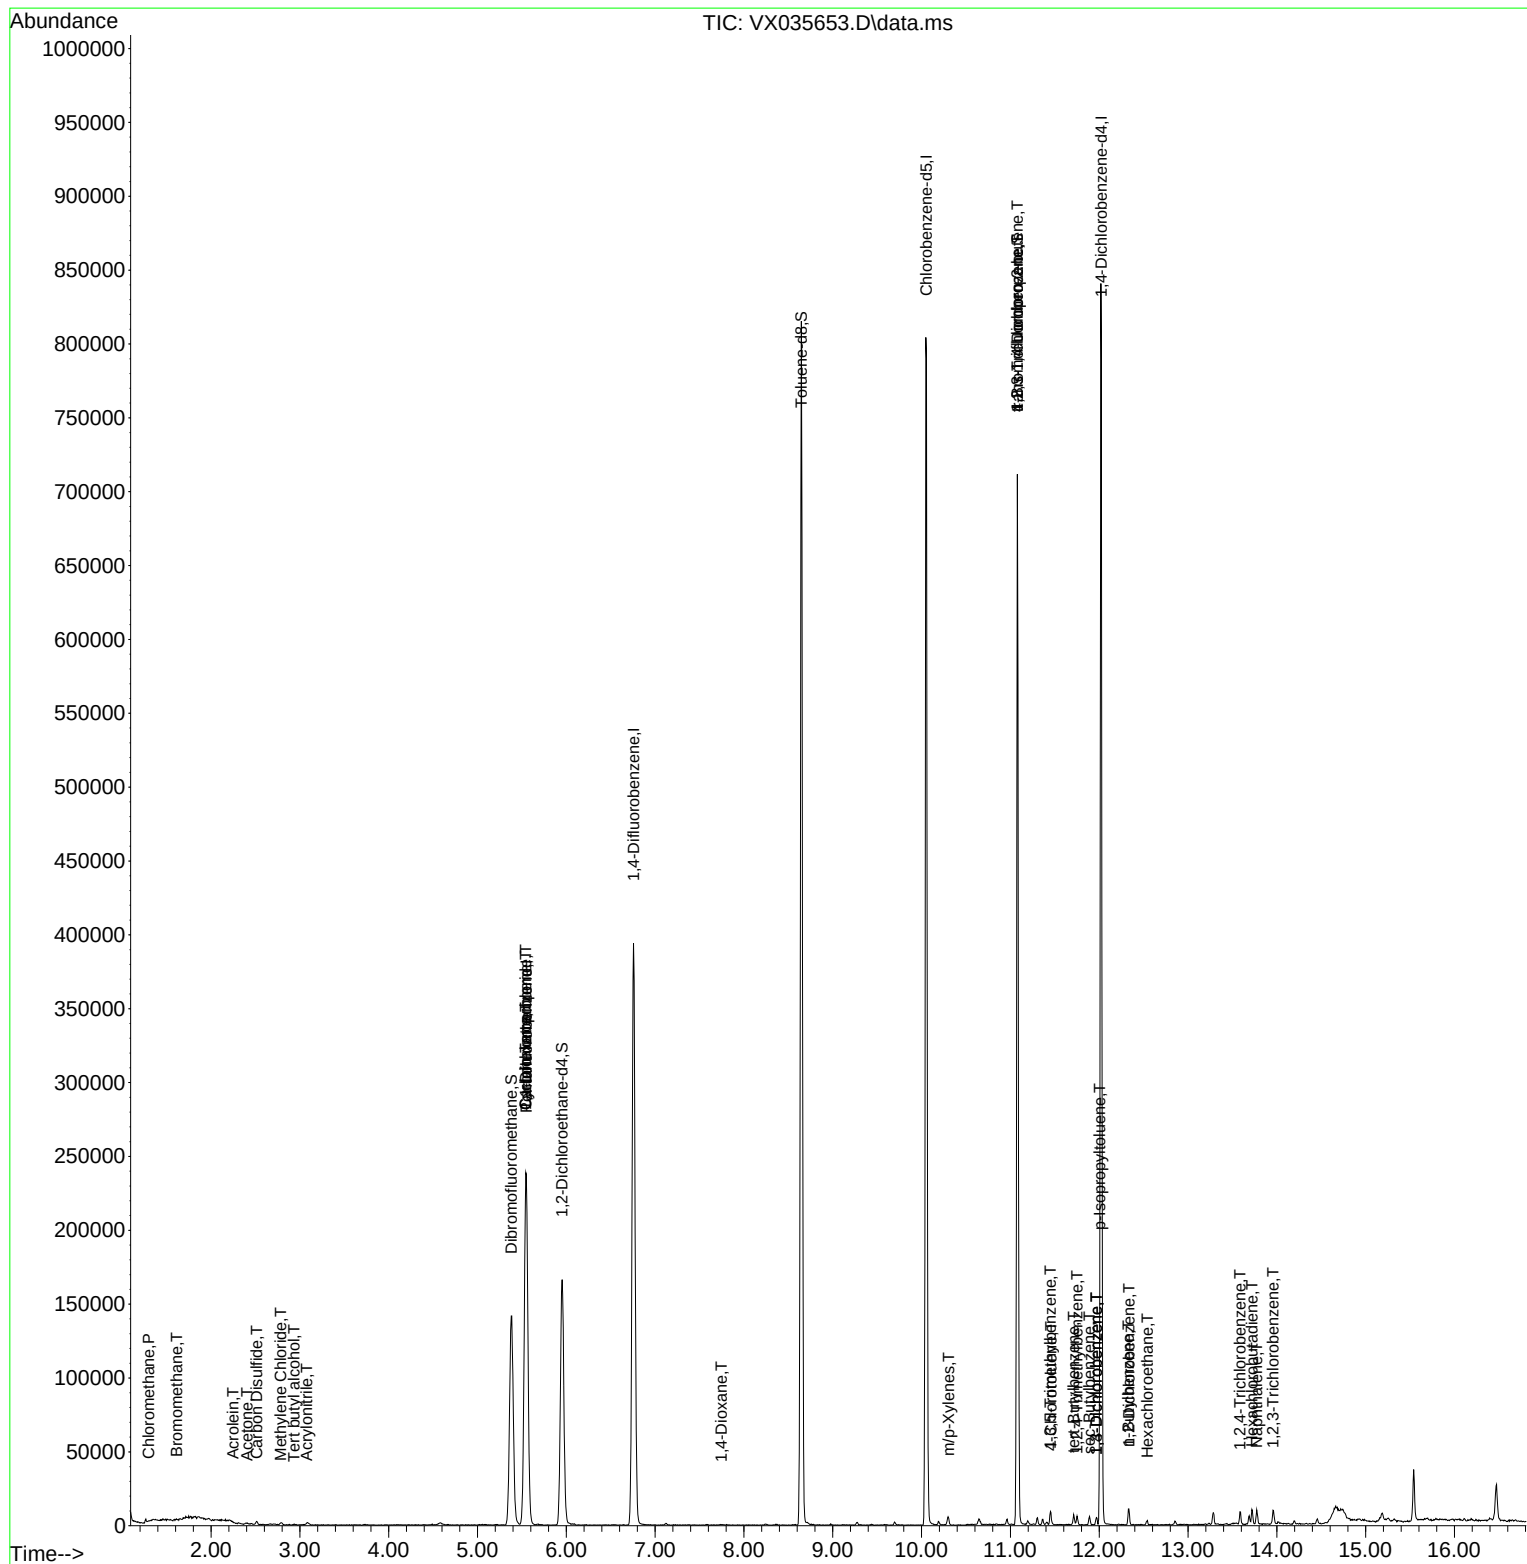




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.549 min Scan# 71
Delta R.T. -0.001 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion:168 Resp: 206102
Ion Ratio Lower Upper
168 100
99 68.3 45.7 68.5

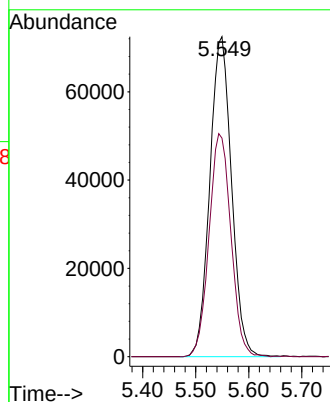

#3
Chloromethane
Concen: 0.208 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion: 50 Resp: 677
Ion Ratio Lower Upper
50 100
52 31.6 25.9 38.9


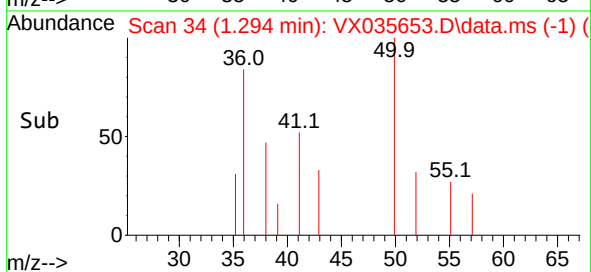
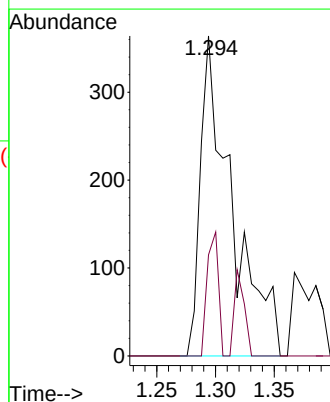



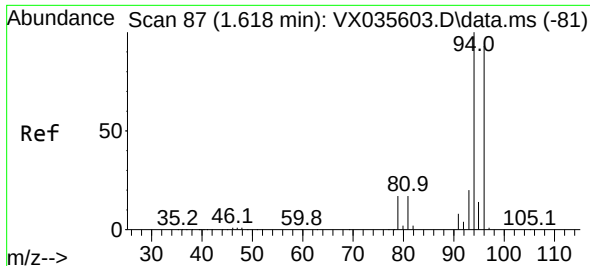

#5
Bromomethane
Concen: 0.209 ug/l
RT: 1.611 min Scan# 80
Delta R.T. -0.007 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion: 94 Resp: 313
Ion Ratio Lower Upper
94 100
96 40.6 77.0 115.6#

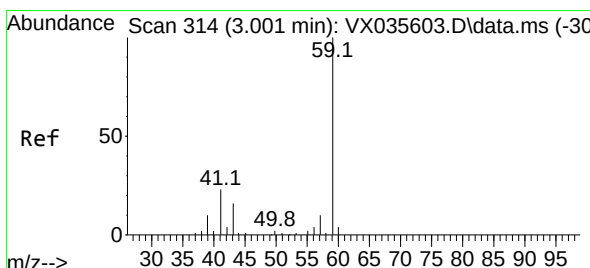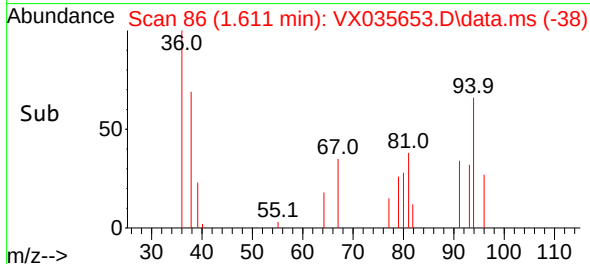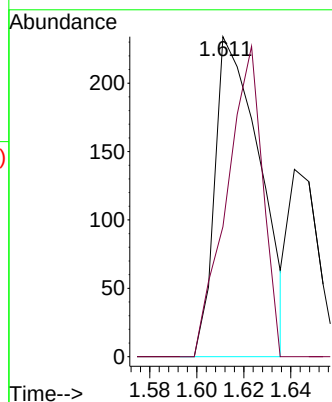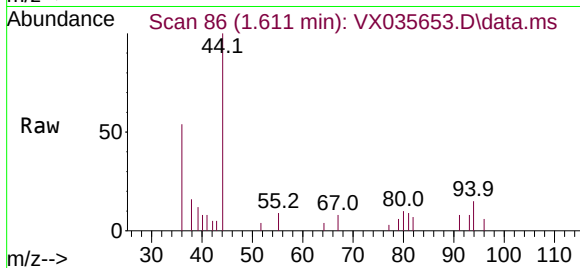

#11
Tert butyl alcohol
Concen: 0.268 ug/l
RT: 2.934 min Scan# 303
Delta R.T. -0.067 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion: 59 Resp: 170
Ion Ratio Lower Upper
59 100
57 0.0 8.1 12.1#


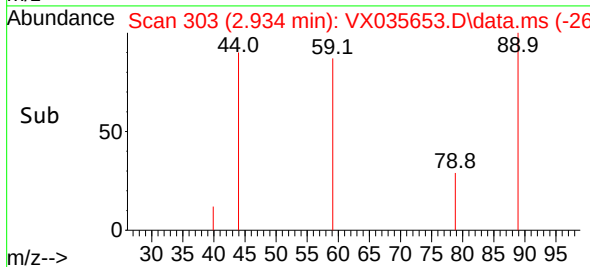
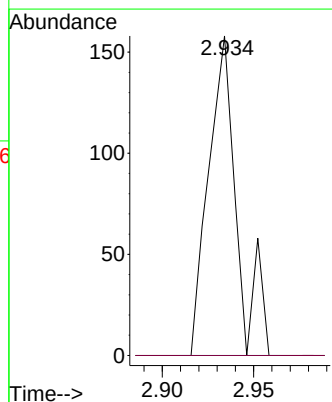
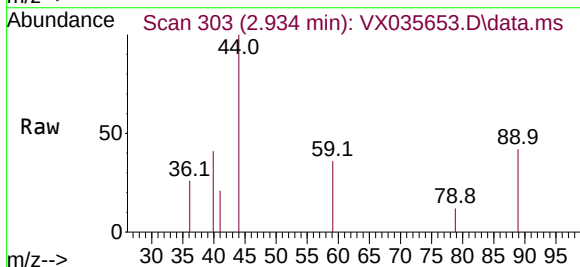




#13
Acrolein
Concen: 0.821 ug/l
RT: 2.245 min Scan# 19
Delta R.T. 0.006 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion: 56 Resp: 618
Ion Ratio Lower Upper
56 100
55 78.3 56.6 85.0

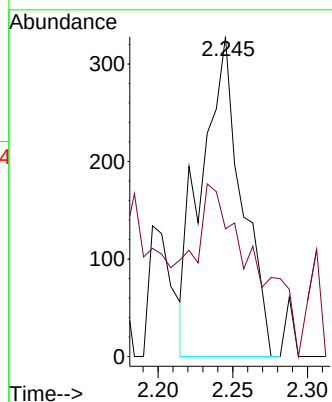

#15
Acrylonitrile
Concen: 0.450 ug/l
RT: 3.074 min Scan# 326
Delta R.T. 0.006 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion: 53 Resp: 629
Ion Ratio Lower Upper
53 100
52 93.8 66.2 99.2
51 4.0 28.3 42.5#

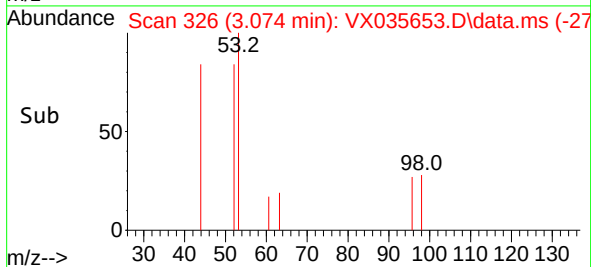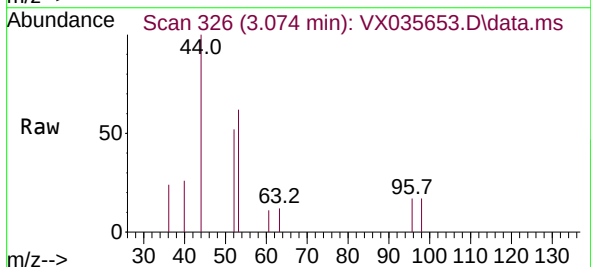



#16

Acetone

Concen: 0.716 ug/l

RT: 2.404 min Scan# 216

Delta R.T. 0.012 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21

Instrument :

MSVOA_X

ClientSampleId :





VX0515MBL01

Tgt Ion: 43 Resp: 1106

Ion Ratio Lower Upper

43 100

58 30.1 24.7 37.1

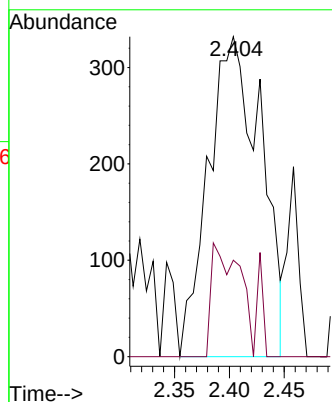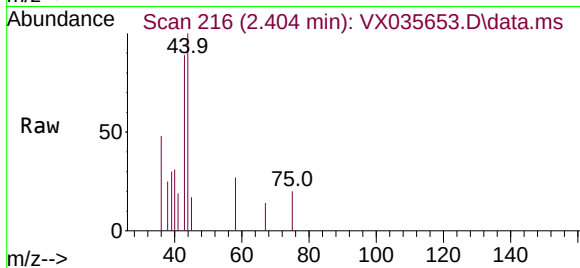

#17

Carbon Disulfide

Concen: 0.415 ug/l

RT: 2.513 min Scan# 234

Delta R.T. -0.001 min

Lab File: VX035653.D




Acq: 15 May 2023 10:21


Tgt Ion: 76 Resp: 2299

Ion Ratio Lower Upper

76 100

78 14.3 7.2 10.8#


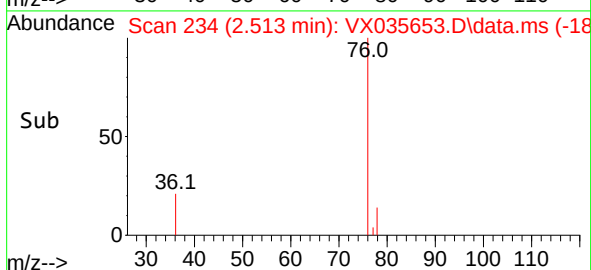

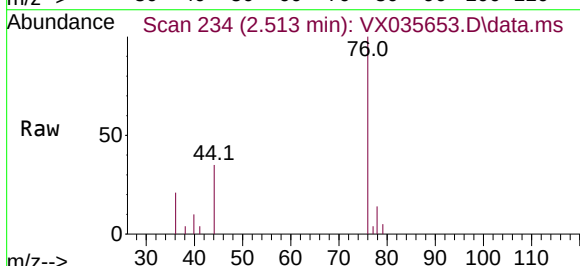




#20
Methylene Chloride
Concen: 0.221 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion:	84	Resp:	618
Ion	Ratio	Lower	Upper
84	100		
49	107.5	103.8	155.8
51	42.5	31.8	47.8
86	55.7	51.4	77.2

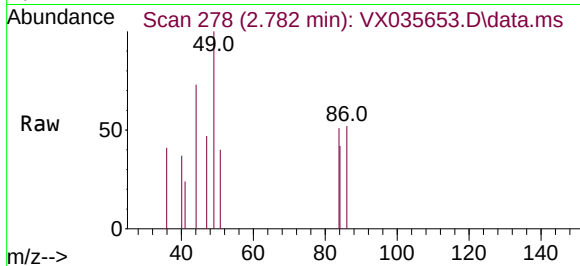

#31
Cyclohexane
Concen: 1.294 ug/l
RT: 5.543 min Scan# 731
Delta R.T. 0.072 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion:	56	Resp:	5879
Ion	Ratio	Lower	Upper
56	100		
69	168.1	23.7	35.5#
84	94.6	68.5	102.7

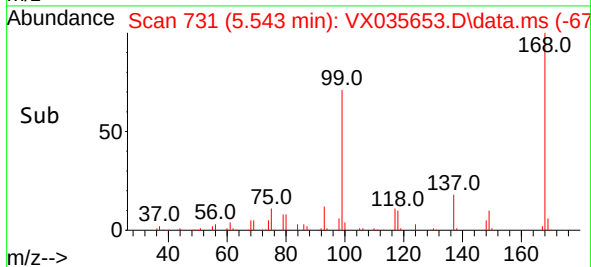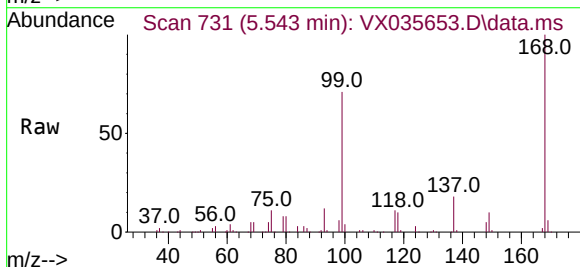



#33

1,2-Dichloroethane-d4

Concen: 46.956 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21

Instrument :

MSVOA_X

ClientSampleId :





VX0515MBL01

Tgt Ion: 65 Resp: 168830

Ion Ratio Lower Upper

65 100

67 49.9 0.0 104.0

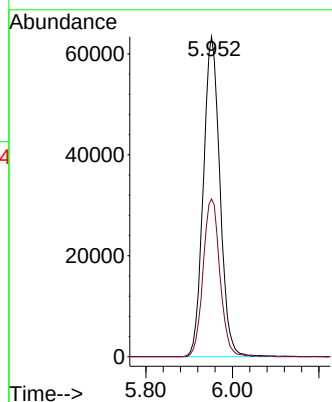

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.006 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21




Tgt Ion: 114 Resp: 377365


Ion Ratio Lower Upper

114 100

63 23.9 0.0 42.2

88 18.4 0.0 33.2

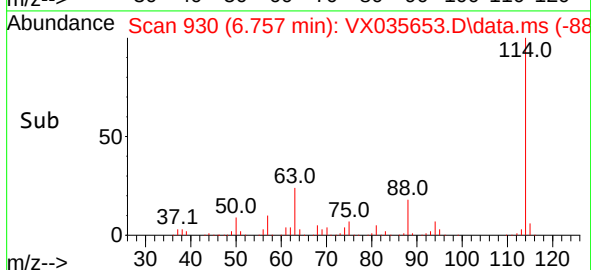

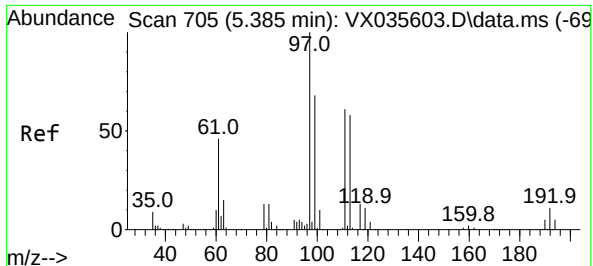

#35

Dibromofluoromethane

Concen: 48.914 ug/l

RT: 5.379 min Scan# 705

Delta R.T. -0.006 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21

Instrument :

MSVOA_X

ClientSampleId :

VX0515MBL01





Tgt Ion:113 Resp: 124484

Ion Ratio Lower Upper

113 100

111 102.5 83.7 125.5

192 16.9 15.4 23.2

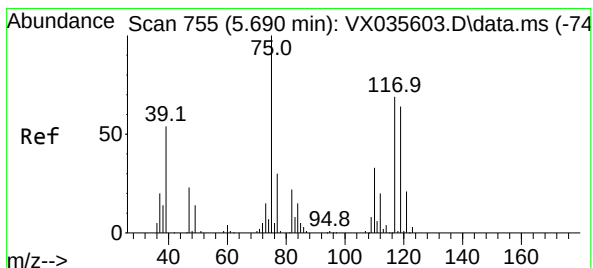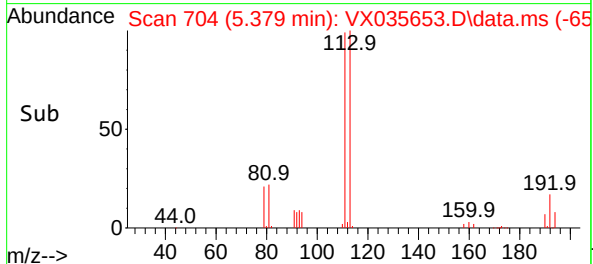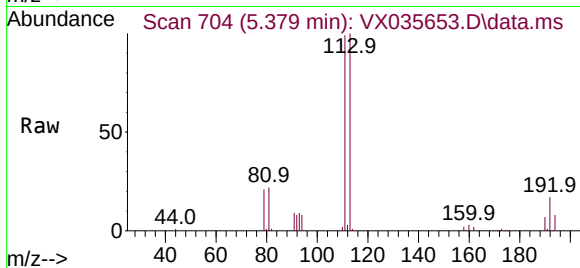

#36

1,1-Dichloropropene

Concen: 4.903 ug/l

RT: 5.543 min Scan# 731

Delta R.T. -0.147 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21




Tgt Ion: 75 Resp: 19696


Ion Ratio Lower Upper

75 100

110 9.1 17.5 52.5#


77 0.0 24.3 36.5#

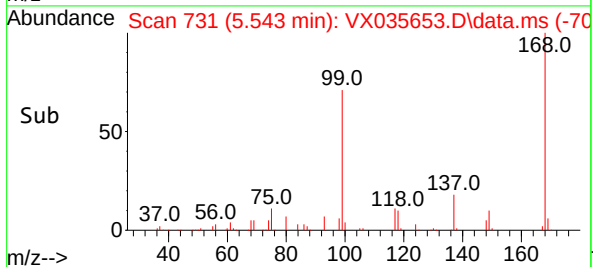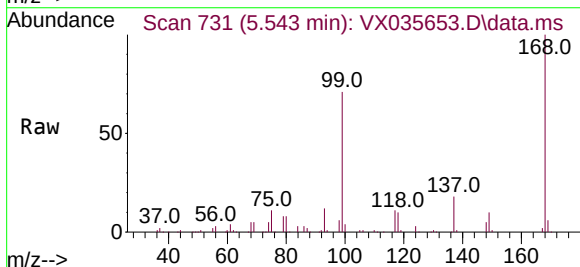






#38
Carbon Tetrachloride
Concen: 6.157 ug/l
RT: 5.543 min Scan# 71
Delta R.T. -0.135 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01



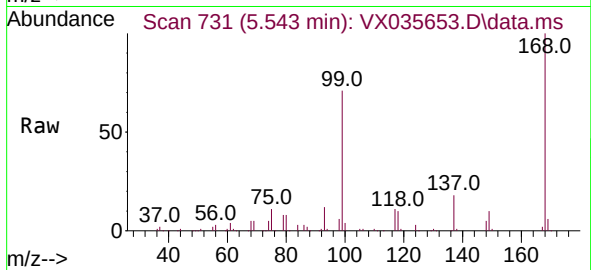



Tgt Ion:117 Resp: 23430
Ion Ratio Lower Upper
117 100
119 4.8 76.6 114.8#
121 0.0 23.8 35.6#



#49
1,4-Dioxane
Concen: 7.138 ug/l
RT: 7.744 min Scan# 1092
Delta R.T. 0.036 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion: 88 Resp: 411
Ion Ratio Lower Upper
88 100
43 23.1 27.7 41.5#
58 30.7 56.8 85.2#


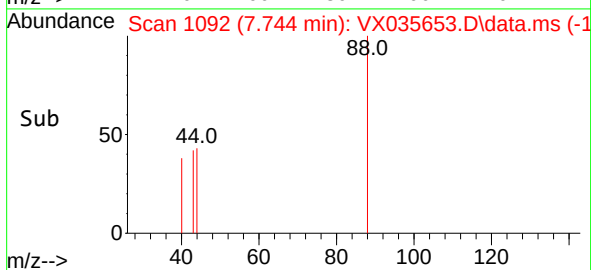

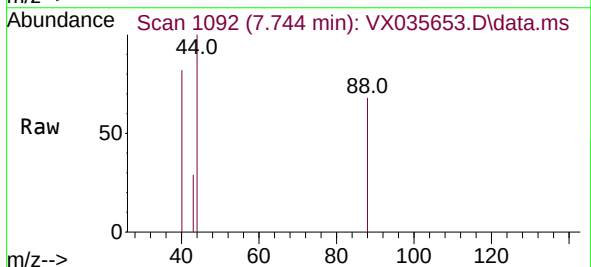




#50
Toluene-d8
Concen: 48.696 ug/l
RT: 8.646 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion: 98 Resp: 457820
Ion Ratio Lower Upper
98 100
100 65.1 52.5 78.7

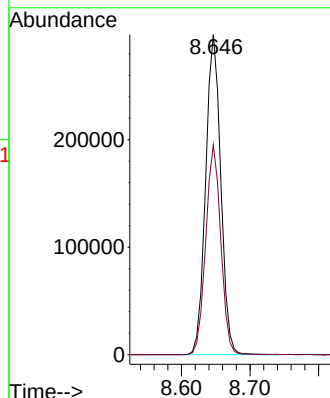

#62
4-Bromofluorobenzene
Concen: 49.634 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion: 95 Resp: 187891
Ion Ratio Lower Upper
95 100
174 65.4 0.0 147.4
176 62.7 0.0 140.6


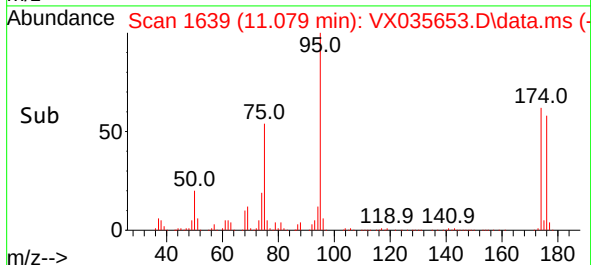
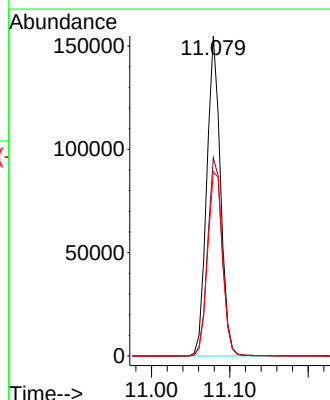
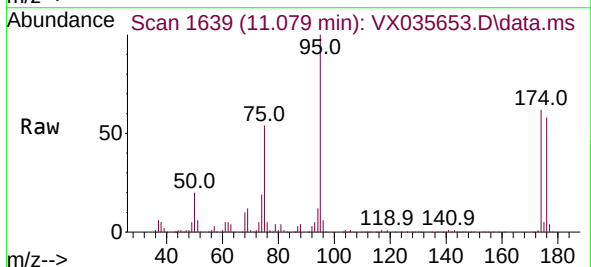




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion:117 Resp: 344239
Ion Ratio Lower Upper
117 100
82 59.2 45.0 67.4
119 32.3 26.0 39.0

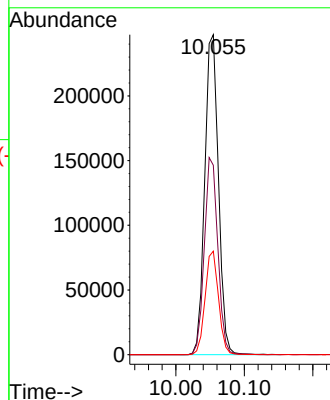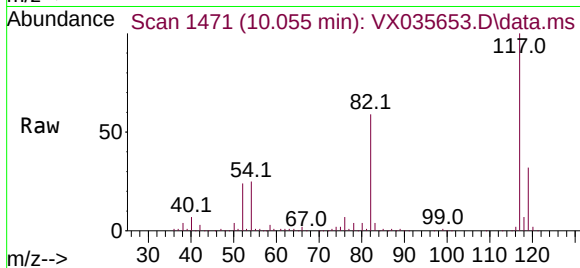

#68
m/p-Xylenes
Concen: 0.217 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion:106 Resp: 1136
Ion Ratio Lower Upper
106 100
91 230.6 164.0 246.0


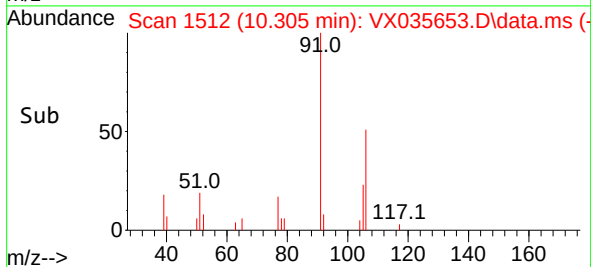
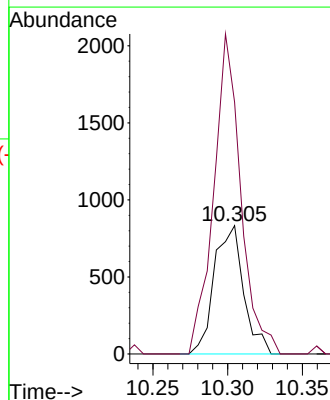
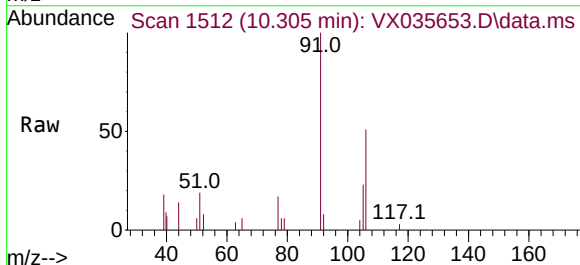




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX035653.D
 Acq: 15 May 2023 10:21




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0515MBL01


Tgt Ion:152 Resp: 156932
 Ion Ratio Lower Upper
 152 100
 115 66.5 45.0 135.0
 150 156.1 0.0 352.4

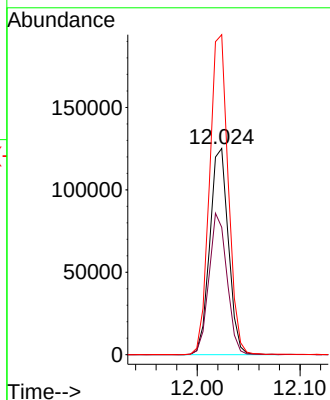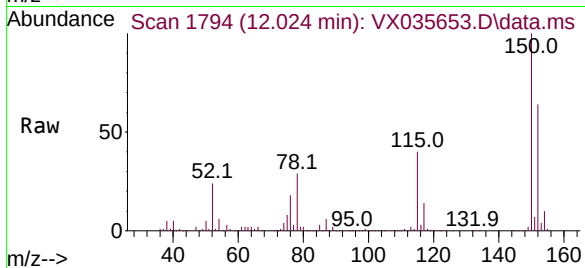

#76
 1,2,3-Trichloropropane
 Concen: 26.354 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX035653.D
 Acq: 15 May 2023 10:21

Tgt Ion: 75 Resp: 101161
 Ion Ratio Lower Upper
 75 100
 77 1.1 21.6 64.8#

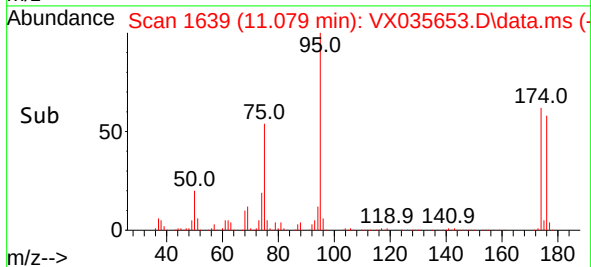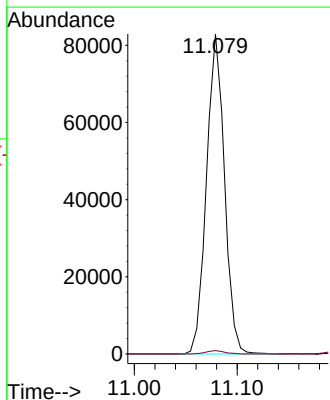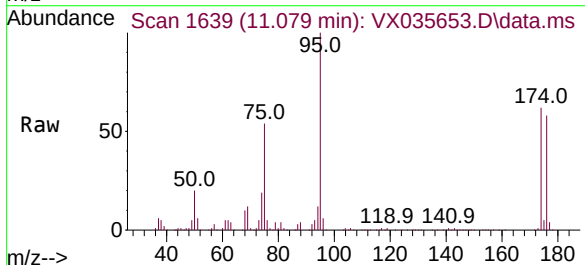



#80

1,3,5-Trimethylbenzene

Concen: 0.209 ug/l

RT: 11.451 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21

Instrument :

MSVOA_X

ClientSampleId :





VX0515MBL01

Tgt Ion:105 Resp: 2346

Ion Ratio Lower Upper

105 100

120 43.1 23.7 71.1

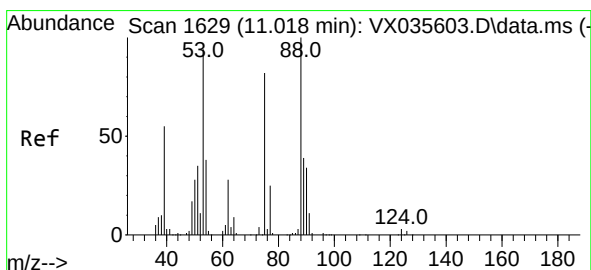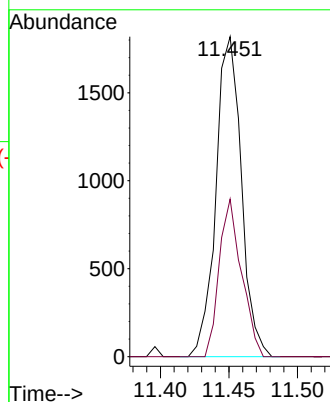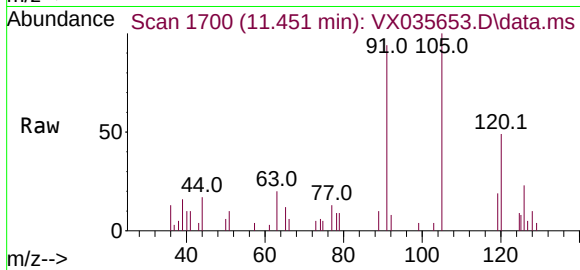

#81

trans-1,4-Dichloro-2-butene

Concen: 84.934 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21




Tgt Ion: 75 Resp: 101161


Ion Ratio Lower Upper

75 100

53 0.0 82.6 124.0#

89 0.0 36.9 55.3#



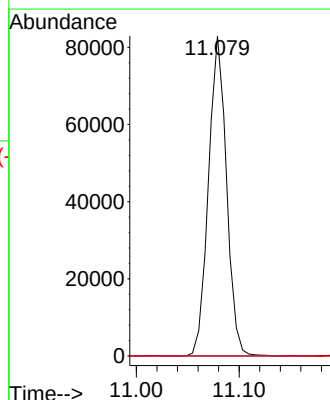
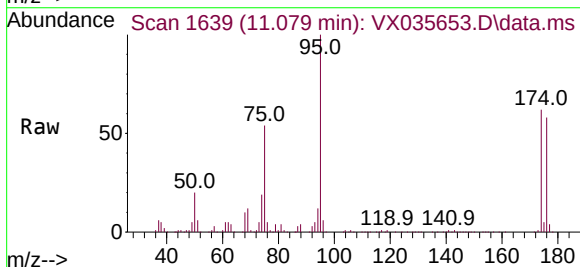




#82
4-Chlorotoluene
Concen: 0.208 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion: 91 Resp: 2326
Ion Ratio Lower Upper
91 100
126 29.3 14.2 42.6

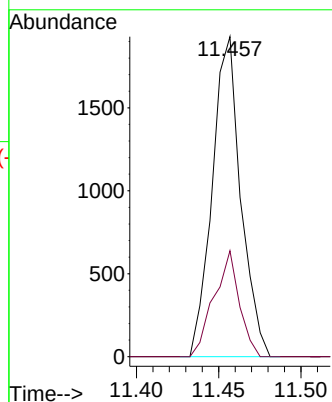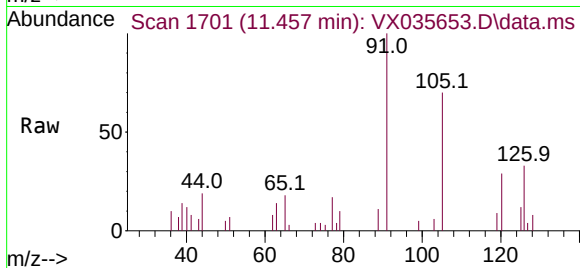

#83
tert-Butylbenzene
Concen: 0.204 ug/l
RT: 11.713 min Scan# 1743
Delta R.T. -0.000 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion: 119 Resp: 2226
Ion Ratio Lower Upper
119 100
91 67.3 30.6 92.0
134 25.8 11.8 35.4


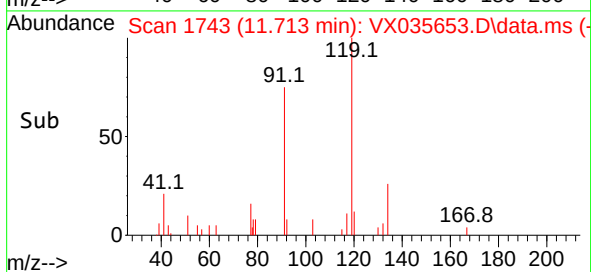
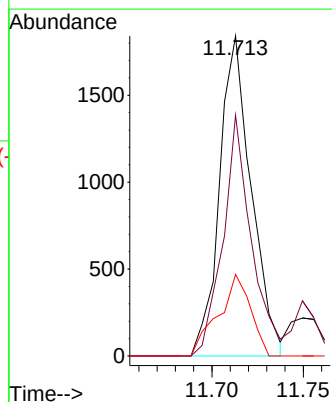
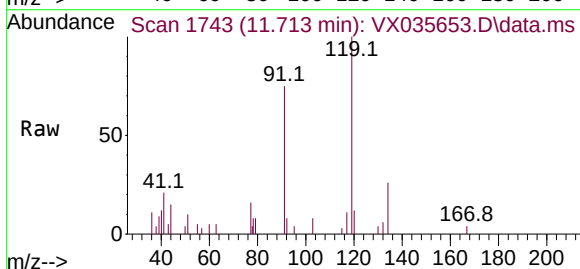




#84
1,2,4-Trimethylbenzene
Concen: 0.231 ug/l
RT: 11.749 min Scan# 1749
Delta R.T. -0.001 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion:105 Resp: 2606
Ion Ratio Lower Upper
105 100
120 39.2 22.4 67.0

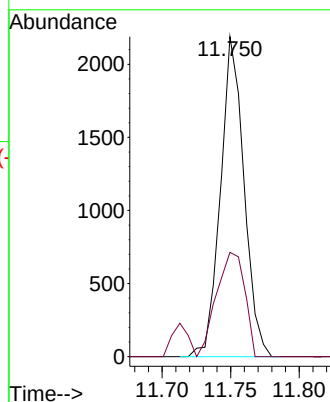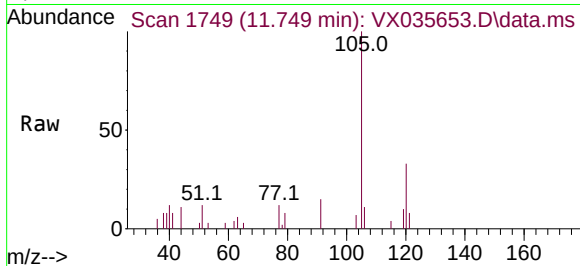

#85
sec-Butylbenzene
Concen: 0.216 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.000 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion:105 Resp: 2966
Ion Ratio Lower Upper
105 100
134 21.8 10.2 30.4


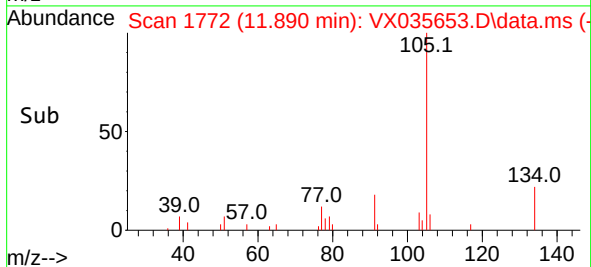
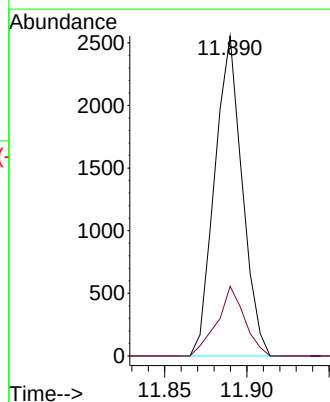
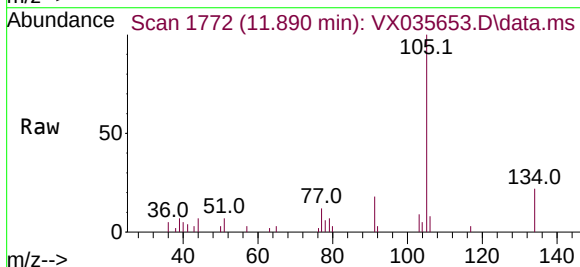




#86
 p-Isopropyltoluene
 Concen: 0.237 ug/l
 RT: 12.006 min Scan# 1791
 Delta R.T. -0.000 min
 Lab File: VX035653.D
 Acq: 15 May 2023 10:21




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0515MBL01


Tgt Ion:119 Resp: 2672
 Ion Ratio Lower Upper
 119 100
 134 34.0 13.2 39.5
 91 43.9 12.9 38.7#

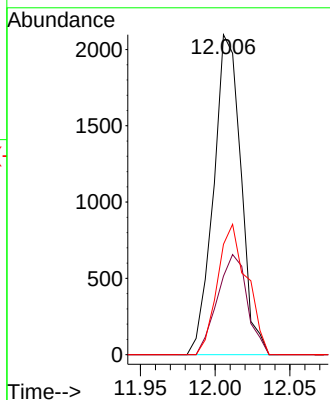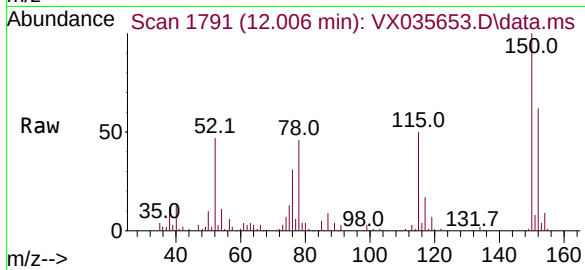

#87
 1,3-Dichlorobenzene
 Concen: 0.271 ug/l
 RT: 11.969 min Scan# 1785
 Delta R.T. -0.000 min
 Lab File: VX035653.D
 Acq: 15 May 2023 10:21

Tgt Ion:146 Resp: 1548
 Ion Ratio Lower Upper
 146 100
 111 52.1 20.9 62.8
 148 67.4 31.6 95.0

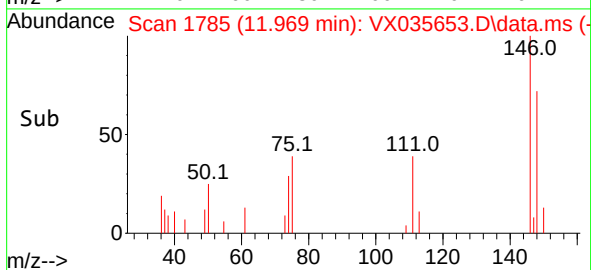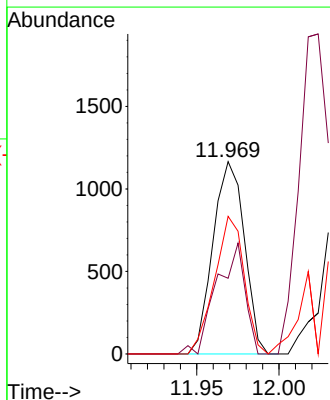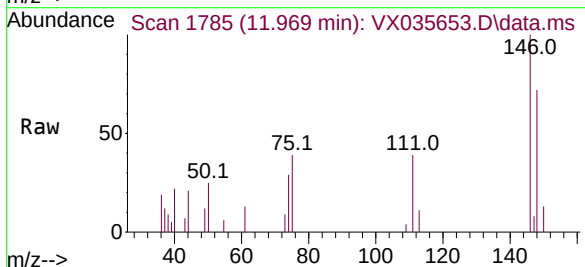



#88

1,4-Dichlorobenzene

Concen: 0.269 ug/l

RT: 11.969 min Scan# 1797

Delta R.T. -0.073 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21

Instrument :

MSVOA_X

ClientSampleId :

VX0515MBL01





Tgt Ion:146 Resp: 1548

Ion Ratio Lower Upper

146 100

111 52.1 20.6 61.9

148 67.4 31.8 95.4

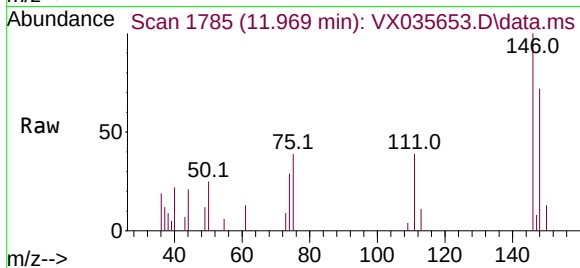

#89

n-Butylbenzene

Concen: 0.272 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21




Tgt Ion: 91 Resp: 2795


Ion Ratio Lower Upper

91 100

92 55.5 27.7 83.0

134 30.7 13.0 38.9

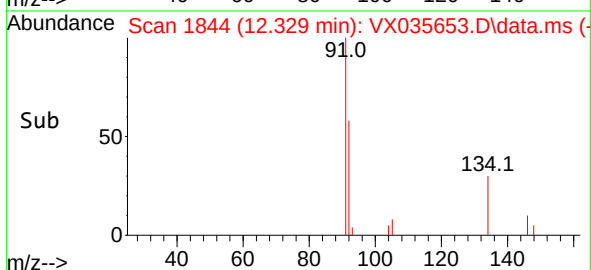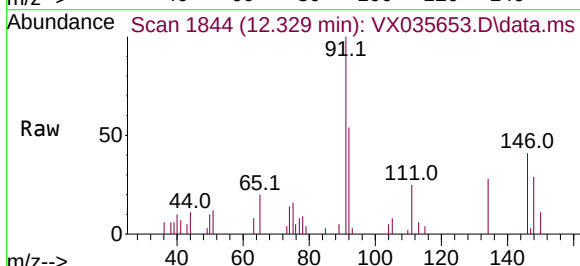



#90

Hexachloroethane

Concen: 0.204 ug/l

RT: 12.542 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21

Instrument :

MSVOA_X

ClientSampleId :





VX0515MBL01

Tgt Ion:117 Resp: 349

Ion Ratio Lower Upper

117 100

201 58.5 34.4 103.1

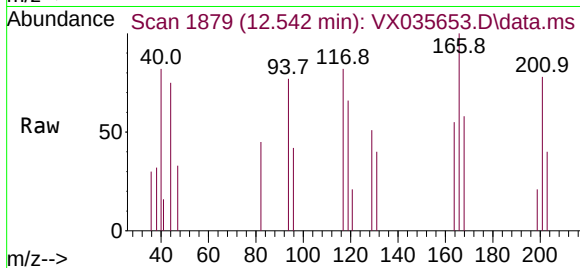

#91

1,2-Dichlorobenzene

Concen: 0.262 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. -0.000 min

Lab File: VX035653.D

Acq: 15 May 2023 10:21




Tgt Ion:146 Resp: 1462


Ion Ratio Lower Upper

146 100

111 39.7 22.0 66.0

148 66.6 32.0 96.0


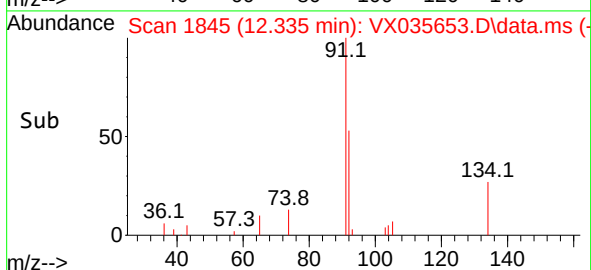

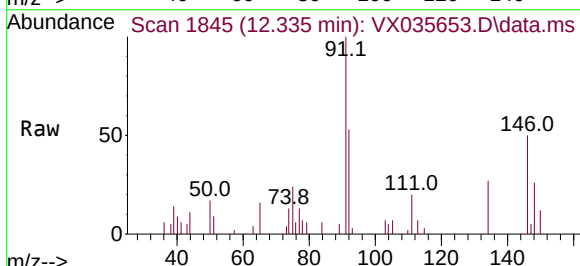




#93
1,2,4-Trichlorobenzene
Concen: 0.588 ug/l
RT: 13.585 min Scan# 2050
Delta R.T. -0.000 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21




Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01


Tgt Ion:180 Resp: 1978
Ion Ratio Lower Upper
180 100
182 102.0 47.0 141.0
145 32.2 15.9 47.7

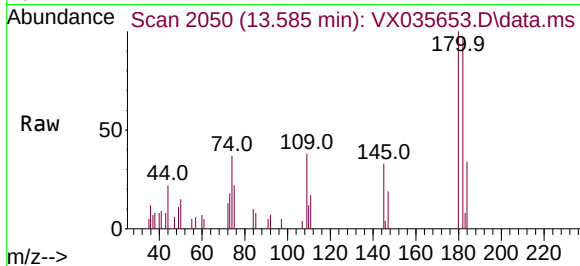

#94
Hexachlorobutadiene
Concen: 0.885 ug/l
RT: 13.719 min Scan# 2072
Delta R.T. -0.006 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion:225 Resp: 1181
Ion Ratio Lower Upper
225 100
223 49.4 32.1 96.5
227 59.3 31.8 95.4


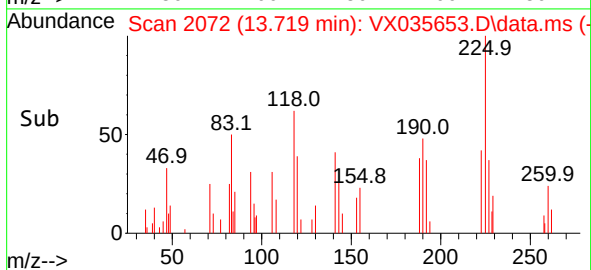

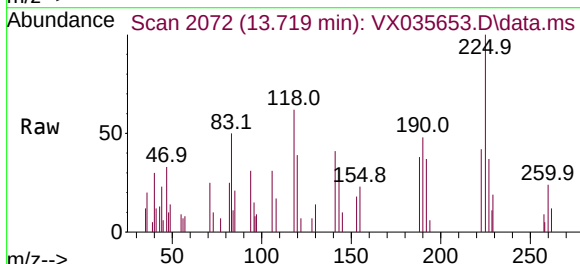


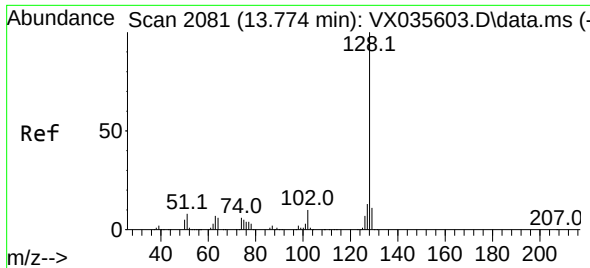

#95
Naphthalene
Concen: 0.523 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Instrument :
MSVOA_X
ClientSampleId :
VX0515MBL01

Tgt Ion:	128	Resp:	6023
Ion	Ratio	Lower	Upper
128	100		
127	14.4	10.2	15.4
129	10.7	8.6	13.0

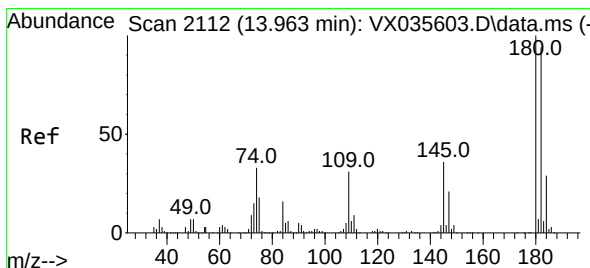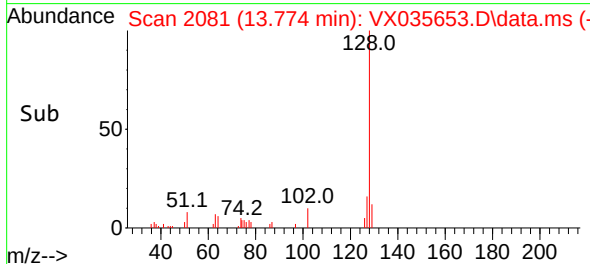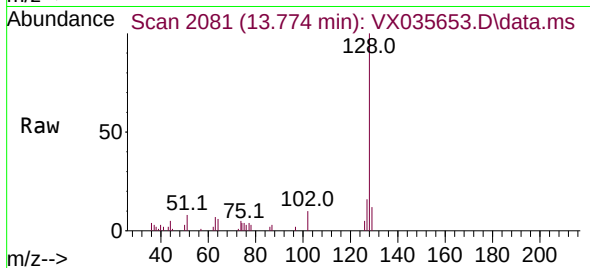

#96
1,2,3-Trichlorobenzene
Concen: 0.654 ug/l
RT: 13.956 min Scan# 2111
Delta R.T. -0.007 min
Lab File: VX035653.D
Acq: 15 May 2023 10:21

Tgt Ion:	180	Resp:	2161
Ion	Ratio	Lower	Upper
180	100		
182	88.8	48.0	144.2
145	32.7	17.7	53.1

