

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051523\
 Data File : VX035674.D
 Acq On : 15 May 2023 18:42
 Operator : JC/MD
 Sample : 02643-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-IDW-S-05042023

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Title : SW846 8260

Signal : TIC: VX035674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	57	60	67	rBV	26004	33815	1.17%	0.211%
2	2.392	206	214	228	rVB	21406	50524	1.74%	0.315%
3	2.788	272	279	295	rVB	24593	47450	1.64%	0.296%
4	4.233	506	516	524	rBV3	17035	48271	1.67%	0.301%
5	4.574	563	572	586	rBV2	11612	37639	1.30%	0.235%
6	4.714	586	595	608	rBV	26649	76326	2.64%	0.476%
7	5.385	692	705	719	rBV	122923	361463	12.48%	2.253%
8	5.550	719	732	749	rVB2	208573	599118	20.69%	3.734%
9	5.952	787	798	812	rBV	148394	398572	13.76%	2.484%
10	6.336	850	861	876	rBV	128714	332195	11.47%	2.070%
11	6.763	920	931	941	rBV	345495	829875	28.66%	5.172%
12	7.129	984	991	1002	rVB2	25515	57788	2.00%	0.360%
13	7.580	1059	1065	1069	rBV2	14677	29707	1.03%	0.185%
14	7.641	1069	1075	1080	rVV	74848	140672	4.86%	0.877%
15	7.690	1080	1083	1091	rVB	22346	39856	1.38%	0.248%
16	7.799	1093	1101	1121	rBV	1659158	2895608	100.00%	18.047%
17	8.549	1214	1224	1233	rBV	363660	562617	19.43%	3.507%
18	8.647	1233	1240	1249	rBV	716202	1133964	39.16%	7.067%
19	8.951	1283	1290	1303	rBV	480367	685893	23.69%	4.275%
20	9.244	1332	1338	1344	rBV	467001	642629	22.19%	4.005%
21	9.305	1344	1348	1351	rVV	55162	77860	2.69%	0.485%
22	9.342	1351	1354	1356	rVV	72046	94517	3.26%	0.589%
23	9.378	1356	1360	1365	rVV	202400	289268	9.99%	1.803%
24	9.482	1372	1377	1381	rVV	770625	1005257	34.72%	6.265%
25	9.518	1381	1383	1388	rVV	94956	116139	4.01%	0.724%
26	9.579	1388	1393	1411	rVB	546505	703334	24.29%	4.384%
27	9.915	1442	1448	1460	rBV	1375501	1727357	59.65%	10.766%
28	10.055	1463	1471	1477	rBV	754449	1049347	36.24%	6.540%
29	10.640	1562	1567	1571	rBV	105748	130403	4.50%	0.813%
30	10.683	1571	1574	1582	rVB	44155	54395	1.88%	0.339%
31	11.079	1634	1639	1650	rBV	628715	788398	27.23%	4.914%
32	12.024	1788	1794	1801	rBV	716955	934295	32.27%	5.823%
33	15.542	2365	2371	2383	rBV2	23324	38589	1.33%	0.241%
34	16.475	2517	2524	2531	rBV4	15813	31815	1.10%	0.198%

Sum of corrected areas: 16044956

Instrument :

MSVOA_X

ClientSampleId :




FSND-IDW-S-05042023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051523\
Data File : VX035674.D
Acq On : 15 May 2023 18:42
Operator : JC/MD
Sample : 02643-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-IDW-S-05042023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

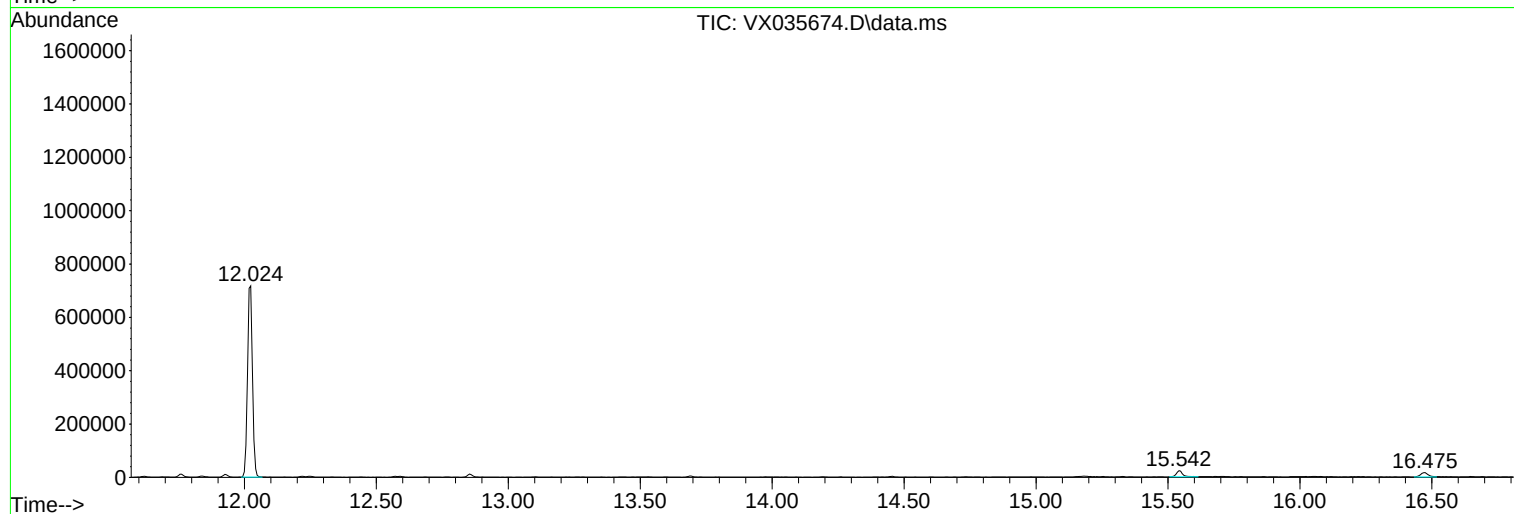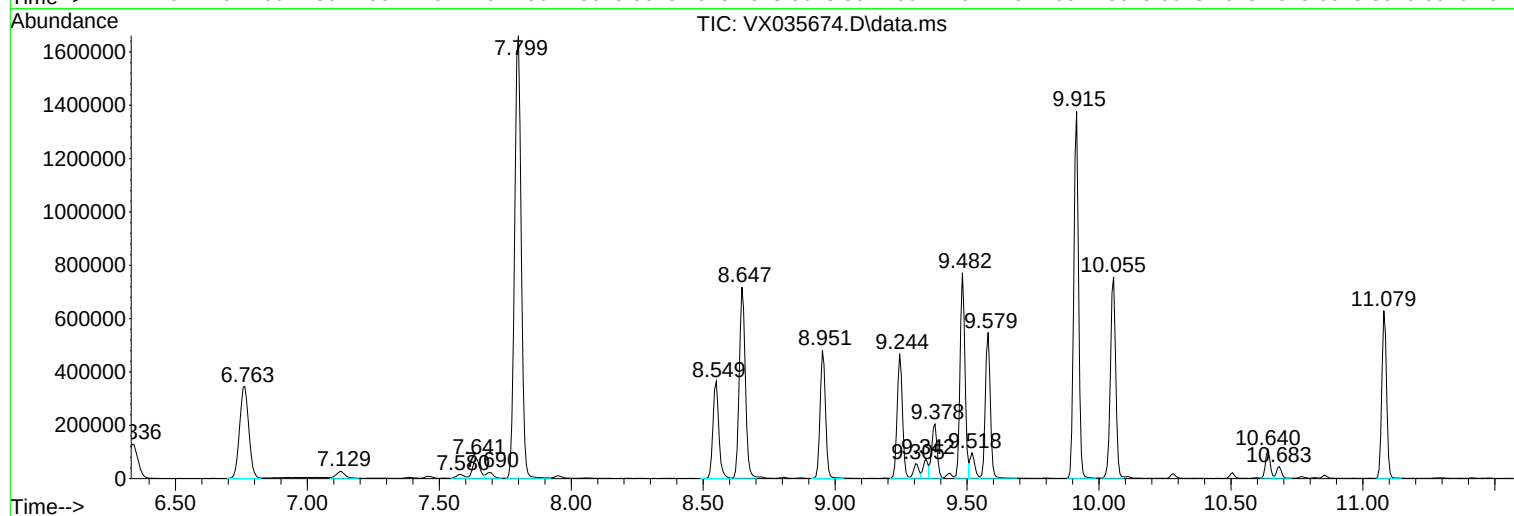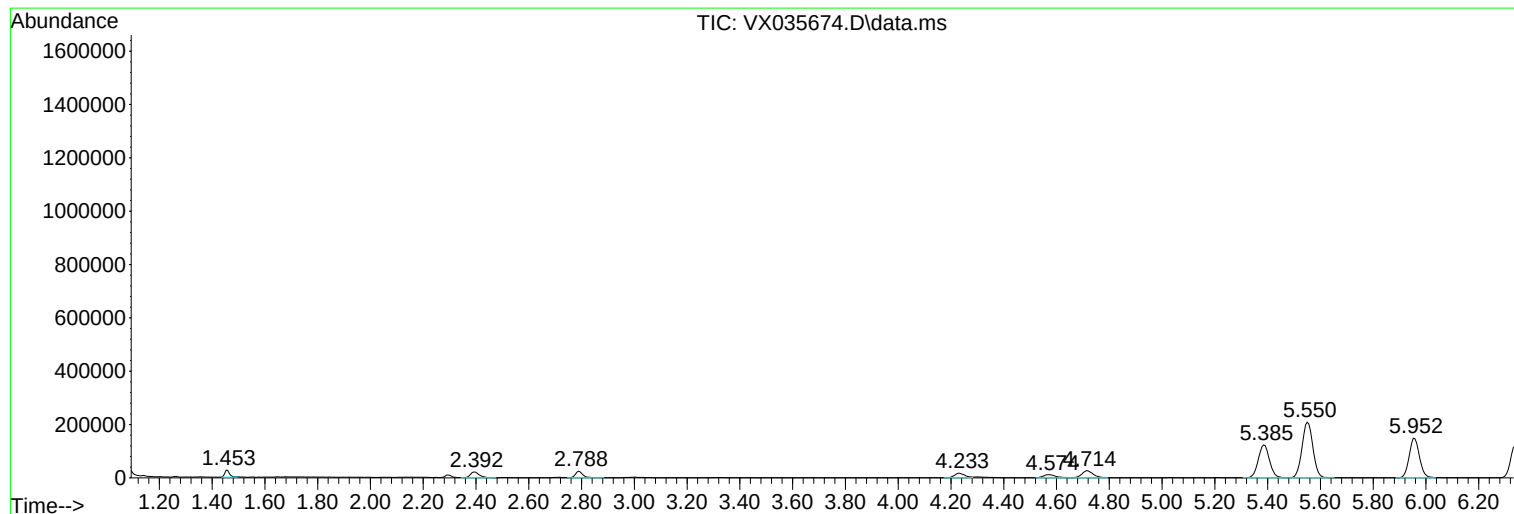

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051523\
Data File : VX035674.D
Acq On : 15 May 2023 18:42
Operator : JC/MD
Sample : 02643-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-IDW-S-05042023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051523\
Data File : VX035674.D
Acq On : 15 May 2023 18:42
Operator : JC/MD
Sample : 02643-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-IDW-S-05042023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc