



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051523\
Data File : VX035651.D
Acq On : 15 May 2023 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Title : SW846 8260
Last Update : Thu May 11 13:57:54 2023

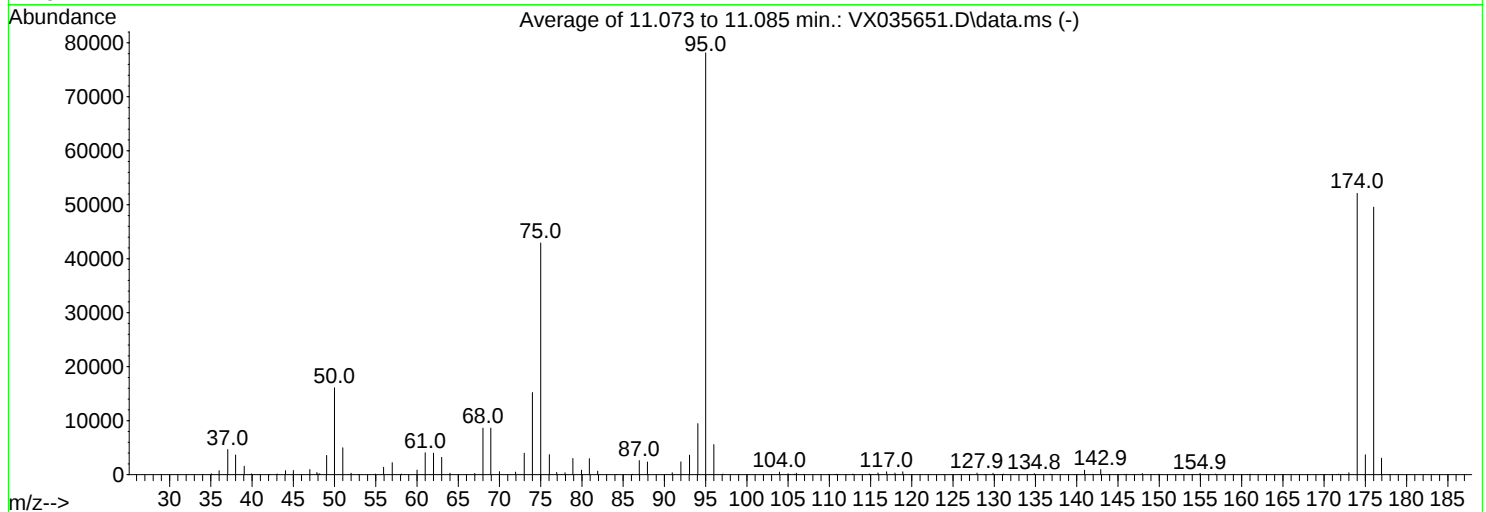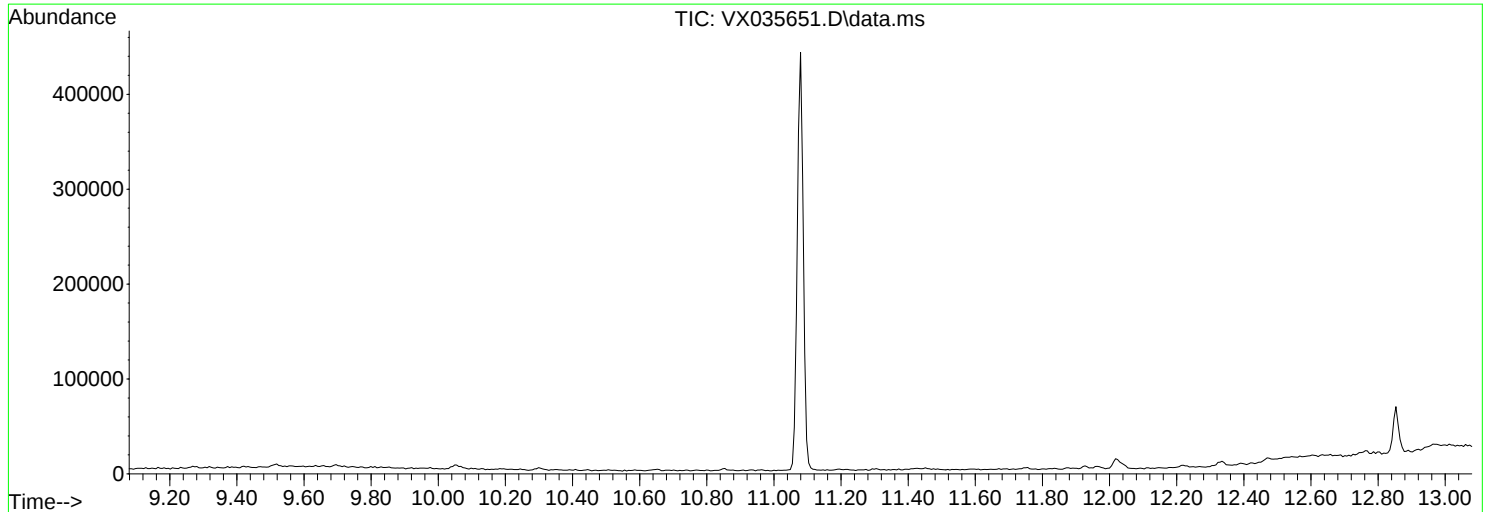

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1630

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	16097	PASS
75	95	30	60	54.9	42909	PASS
95	95	100	100	100.0	78141	PASS
96	95	5	9	7.1	5565	PASS
173	174	0.00	2	0.7	355	PASS
174	95	50	100	66.7	52125	PASS
175	174	5	9	7.1	3684	PASS
176	174	95	101	95.1	49579	PASS
177	176	5	9	6.2	3065	PASS