

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX051619\
 Data File : VX009617.D
 Acq On : 16 May 2019 19:05
 Operator : JC/SP
 Sample : K2644-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EO-01-051519-B

Quant Time: May 17 06:40:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 09 07:31:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	169890	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	269075	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	242329	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	103429	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	112689	48.59	ug/l	0.00
Spiked Amount			Recovery	=	97.18%	
35) Dibromofluoromethane	5.50	113	82617	48.84	ug/l	0.00
Spiked Amount			Recovery	=	97.68%	
50) Toluene-d8	8.71	98	344960	50.51	ug/l	0.00
Spiked Amount			Recovery	=	101.02%	
62) 4-Bromofluorobenzene	11.13	95	112525	45.35	ug/l	0.00
Spiked Amount			Recovery	=	90.70%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Methyl Iodide	2.52	142	20	4.604	ug/l #	42
11) Tert butyl alcohol	3.04	59	409	0.762	ug/l #	73
13) Acrolein	2.29	56	243	0.500	ug/l	94
16) Acetone	2.44	43	16991	13.644	ug/l	96
18) Methyl Acetate	2.78	43	5107	1.724	ug/l	96
20) Methylene Chloride	2.86	84	50429	25.010	ug/l	98
25) 2-Butanone	4.69	43	3278	1.694	ug/l #	88
28) Bromochloromethane	5.12	49	19	Below Cal	#	20
29) Tetrahydrofuran	5.15	42	1722	1.383	ug/l	97
31) Cyclohexane	5.67	56	4004	1.168	ug/l #	1
36) 1,1-Dichloropropene	5.67	75	12967	5.186	ug/l #	52
38) Carbon Tetrachloride	5.67	117	15864	6.983	ug/l #	15
43) Isopropyl Acetate	6.45	43	12432	2.231	ug/l	100
48) Methyl methacrylate	7.68	41	7593	2.746	ug/l #	18
49) 1,4-Dioxane	7.82	88	19	0.339	ug/l #	20
51) 4-Methyl-2-Pentanone	8.61	43	86082	23.632	ug/l #	51
54) cis-1,3-Dichloropropene	8.62	75	35816	11.291	ug/l #	60
57) 1,3-Dichloropropane	9.54	76	8531	2.526	ug/l #	44
59) 2-Hexanone	9.44	43	12105	4.231	ug/l #	26
74) N-amyl acetate	10.69	43	13917	3.174	ug/l #	56
76) 1,2,3-Trichloropropane	11.13	75	58179	24.250	ug/l #	34
80) 1,3,5-Trimethylbenzene	11.51	105	2927	0.462	ug/l	97
81) trans-1,4-Dichloro-2-buten	11.13	75	58179	62.046	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	2356	0.371	ug/l	95
95) Naphthalene	13.83	128	8001	1.061	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :


EO-01-051519-B

Tot Ion:168 Resp: 169890

Ion Ratio Lower Upper

168 100

99 53.2 42.3 63.5

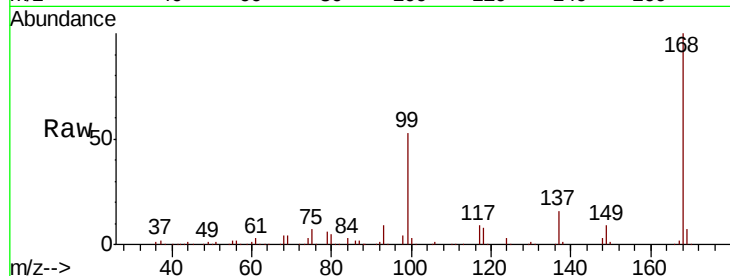

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#10

Methyl Iodide

Concen: 4.604 ug/l

RT: 2.52 min Scan# 224

Delta R.T. 0.01 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05


Tgt Ion:142 Resp: 20

Ion Ratio Lower Upper

142 100

127 0.0 32.7 49.1#

141 0.0 11.5 17.3#



Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

2.52


60


40

20

0

Time--> 2.50 2.51 2.52 2.53 2.54









#11
Tert butyl alcohol
Concen: 0.762 ug/l
RT: 3.04 min Scan# 310
Delta R.T. -0.01 min
Lab File: VX009617.D
Acq: 16 May 2019 19:05




Instrument :
MSVOA_X
ClientSampleId :
EO-01-051519-B

Tot Ion: 59 Resp: 409
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

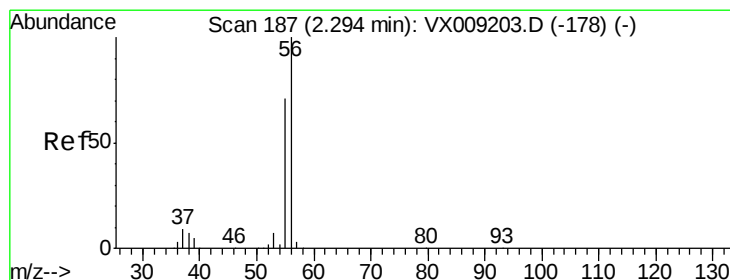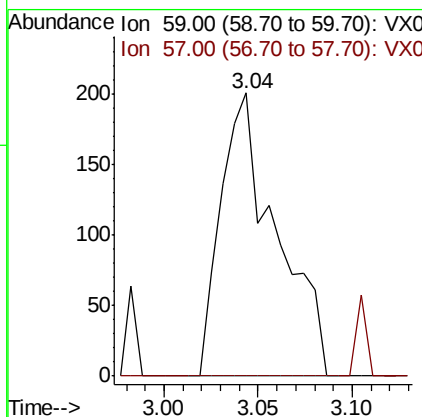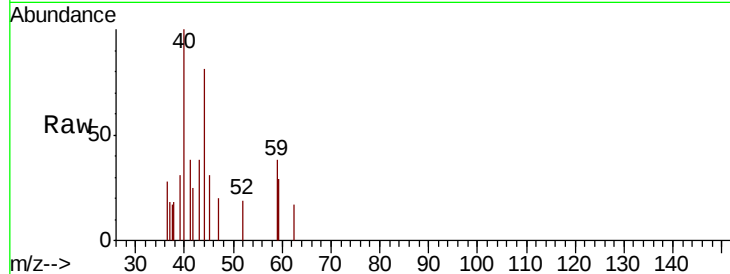

#13
Acrolein
Concen: 0.500 ug/l
RT: 2.29 min Scan# 187
Delta R.T. -0.00 min
Lab File: VX009617.D
Acq: 16 May 2019 19:05

Tgt Ion: 56 Resp: 243
Ion Ratio Lower Upper
56 100
55 65.8 56.6 85.0

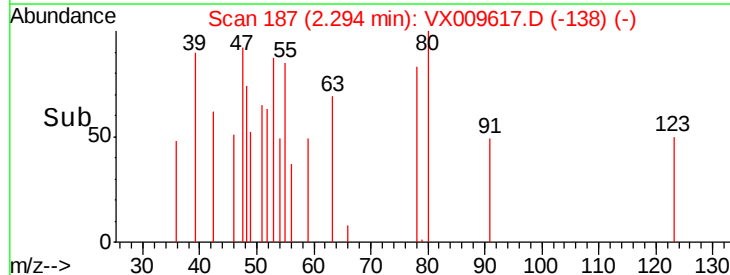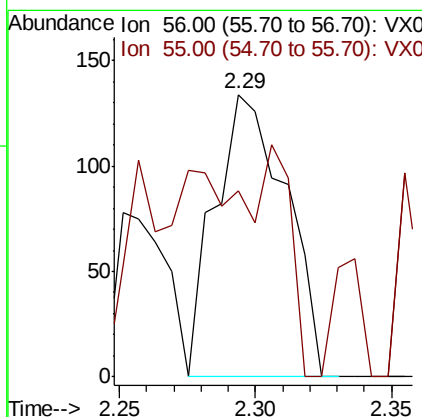



#16

Acetone

Concen: 13.644 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :


EO-01-051519-B

Tot Ion: 43 Resp: 16991

Ion Ratio Lower Upper

43 100

58 28.7 24.9 37.3



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

10000

8000



6000

4000

2000

0

Time--> 2.30 2.40 2.50 2.60

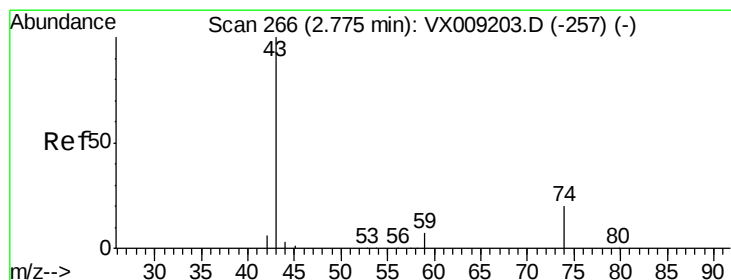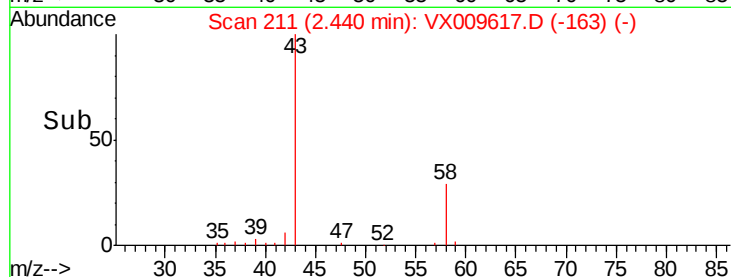

#18

Methyl Acetate

Concen: 1.724 ug/l

RT: 2.78 min Scan# 266

Delta R.T. -0.00 min

Lab File: VX009617.D


Acq: 16 May 2019 19:05

Tgt Ion: 43 Resp: 5107

Ion Ratio Lower Upper

43 100

74 22.1 16.2 24.4

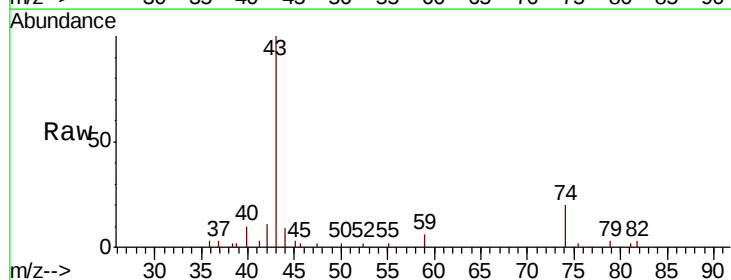

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

3000

2500

2000


1500


1000

500

0

Time--> 2.70 2.75 2.80 2.85

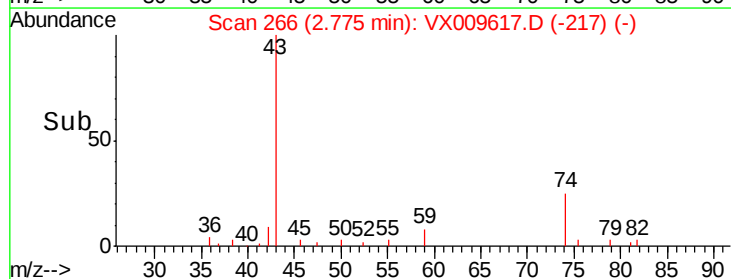



#20

Methvlene Chloride

Concen: 25.010 ug/l

RT: 2.86 min Scan# 280

Delta R.T. 0.01 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :

EO-01-051519-B

Tot Ion: 84 Resp: 50429



Ion Ratio Lower Upper

84 100

49 135.7 109.9 164.9

51 42.3 32.7 49.1

86 63.9 52.0 78.0





Abundance

Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

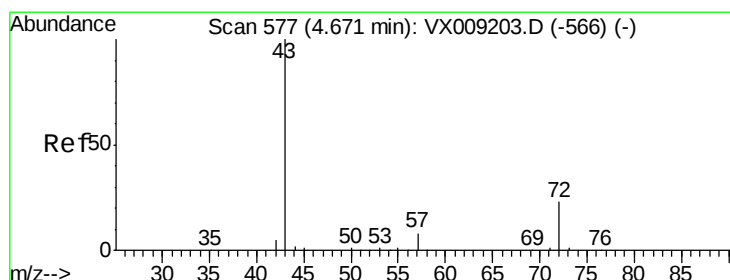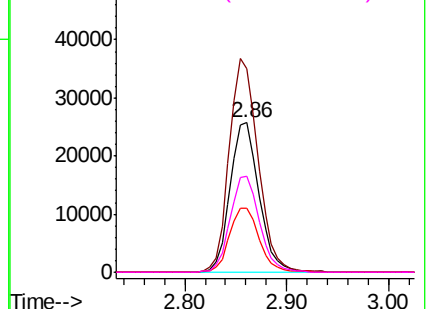

#25

2-Butanone

Concen: 1.694 ug/l

RT: 4.69 min Scan# 580

Delta R.T. 0.02 min

Lab File: VX009617.D



Acq: 16 May 2019 19:05

Tgt Ion: 43 Resp: 3278

Ion Ratio Lower Upper

43 100


72 28.7 18.2 27.2#




Abundance

Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

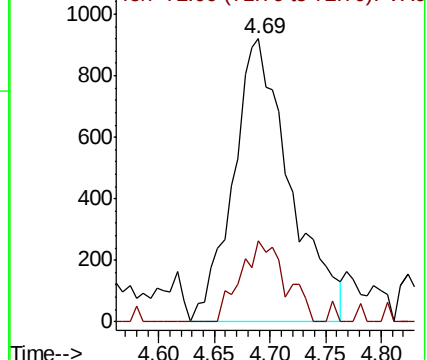

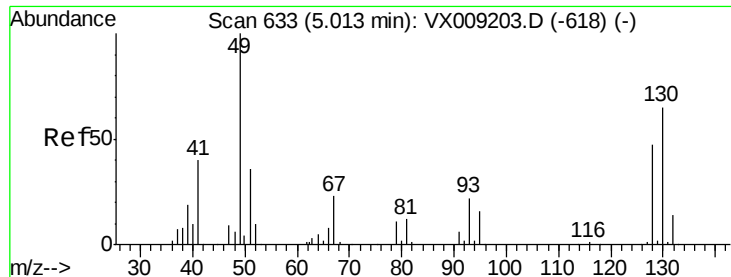

#28

Bromochloromethane

Concen: Below Cal

RT: 5.12 min Scan# 650

Delta R.T. 0.10 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :

EO-01-051519-B


Tot Ion: 49 Resp: 19

Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.8




130 0.0 51.2 76.8#



Abundance Ion 48.90 (48.60 to 49.60): VX0

Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V

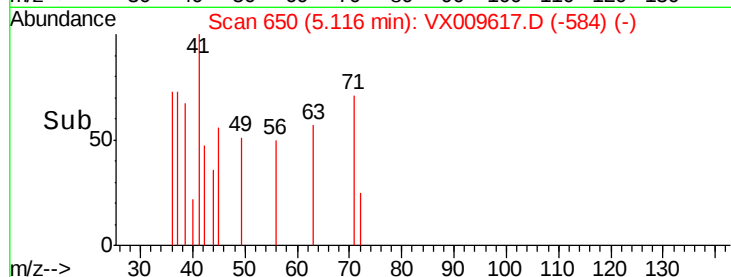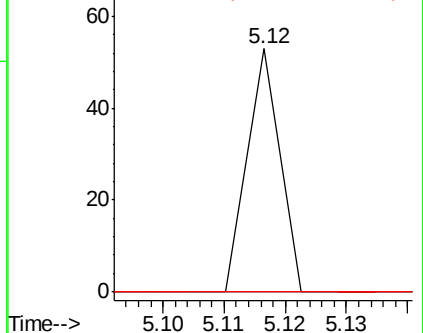

#29

Tetrahydrofuran

Concen: 1.383 ug/l

RT: 5.15 min Scan# 656

Delta R.T. 0.02 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05


Tgt Ion: 42 Resp: 1722

Ion Ratio Lower Upper

42 100

72 36.0 30.4 45.6



71 37.2 28.6 43.0




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0



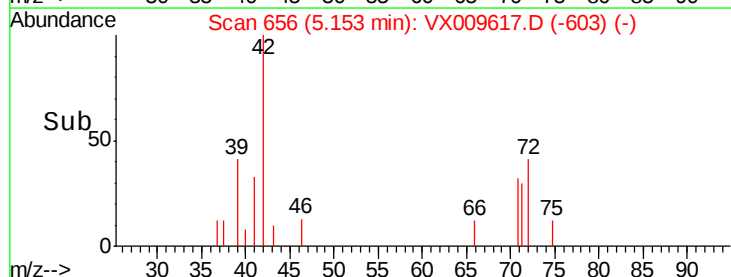
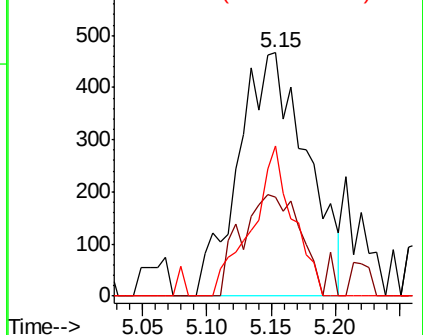




#31
Cvclohexane
Concen: 1.168 ug/l
RT: 5.67 min Scan# 740
Delta R.T. 0.09 min
Lab File: VX009617.D
Acq: 16 May 2019 19:05




Instrument :
MSVOA_X
ClientSampleId :
EO-01-051519-B


Tot Ion: 56 Resp: 4004
Ion Ratio Lower Upper
56 100
69 162.5 23.4 35.0#
84 145.9 61.9 92.9#

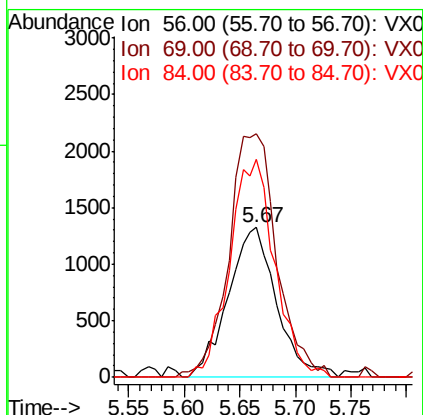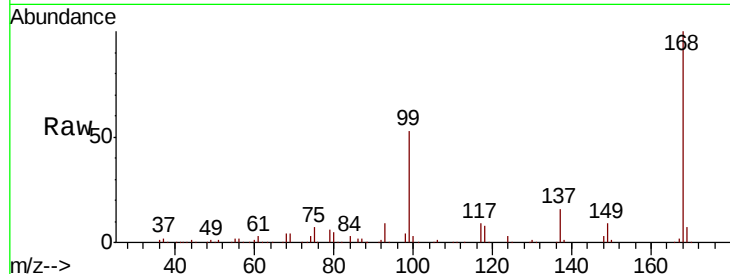

#33
1,2-Dichloroethane-d4
Concen: 48.590 ug/l
RT: 6.06 min Scan# 805
Delta R.T. -0.00 min
Lab File: VX009617.D
Acq: 16 May 2019 19:05

Tgt Ion: 65 Resp: 112689
Ion Ratio Lower Upper
65 100
67 53.7 0.0 106.6


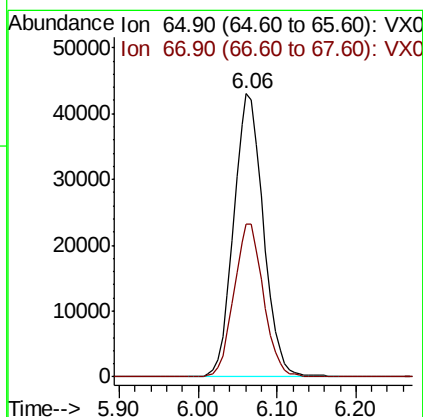

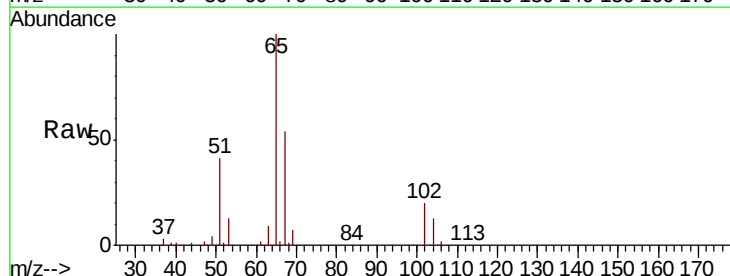


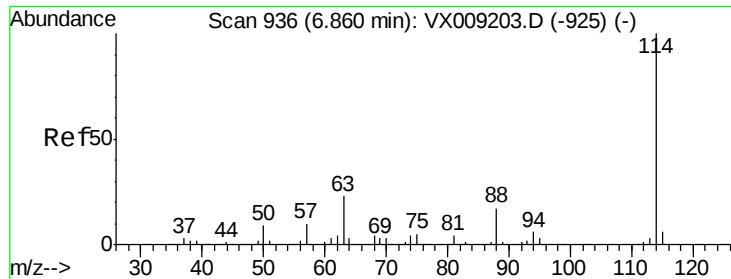

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX009617.D
 Acq: 16 May 2019 19:05




Instrument :
 MSVOA_X
 ClientSampleId :
 EO-01-051519-B


Tot Ion	Ratio	Lower	Upper
114	100		
63	23.2	0.0	45.6
88	16.7	0.0	33.2

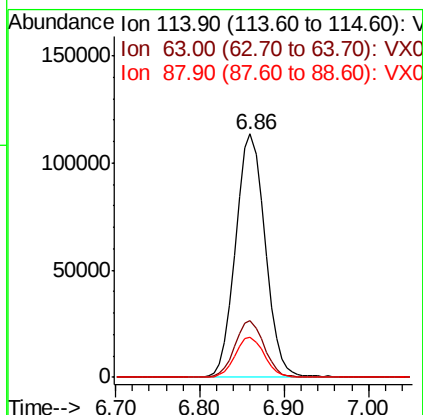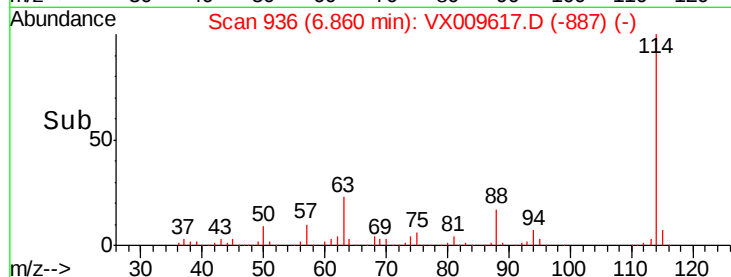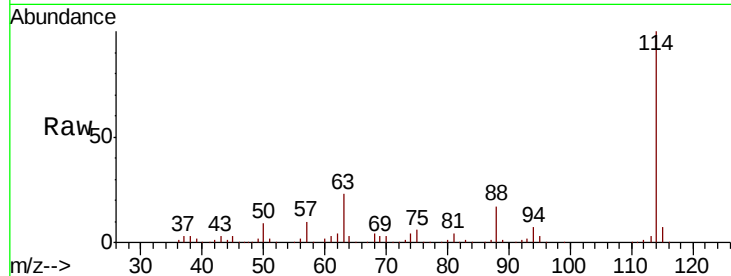

#35
 Dibromofluoromethane
 Concen: 48.842 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX009617.D
 Acq: 16 May 2019 19:05

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.8	82.8	124.2
192	21.5	17.0	25.6

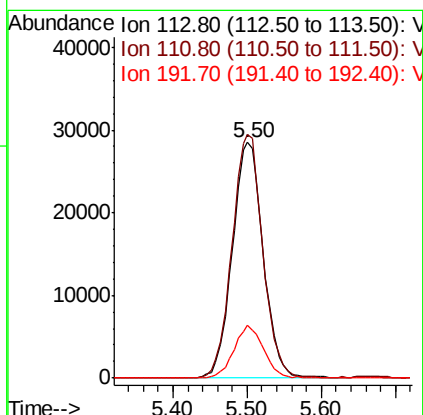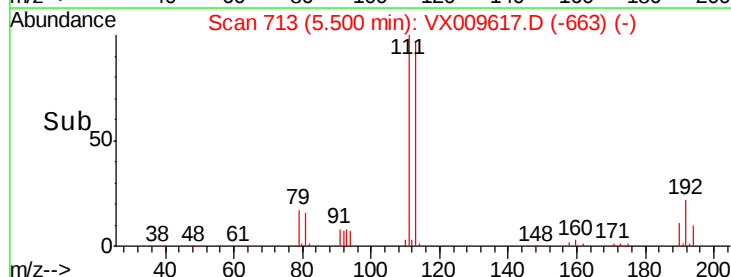



#36

1,1-Dichloropropene

Concen: 5.186 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.13 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :

EO-01-051519-B


Tot Ion: 75 Resp: 12967

Ion Ratio Lower Upper

75 100

110 10.3 16.9 50.6#




77 0.0 24.8 37.2#

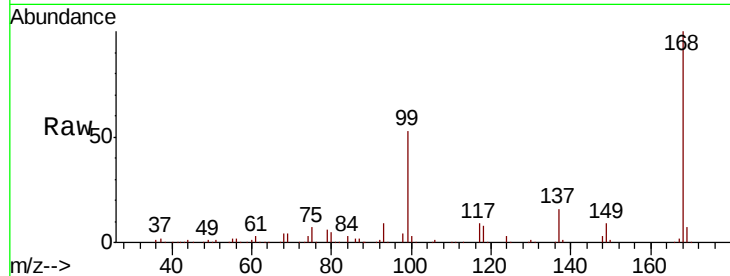

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

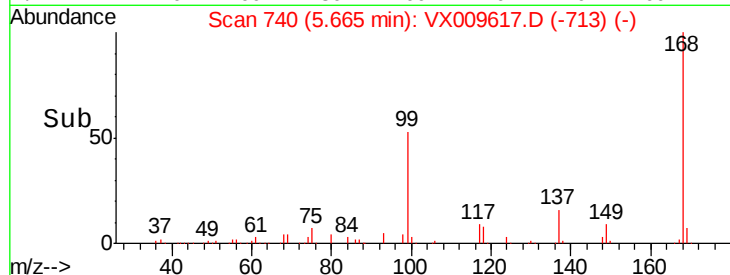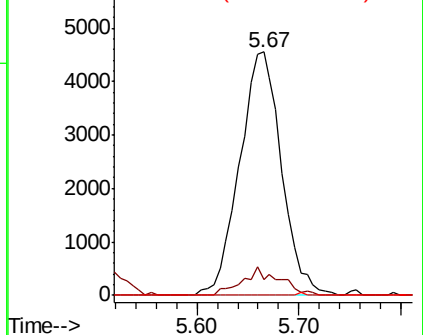

#38

Carbon Tetrachloride

Concen: 6.983 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05


Tgt Ion: 117 Resp: 15864

Ion Ratio Lower Upper

117 100

119 4.3 77.5 116.3#



121 0.0 24.7 37.1#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

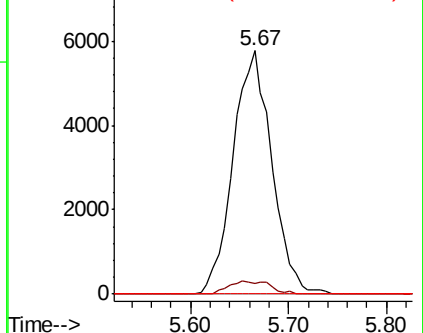

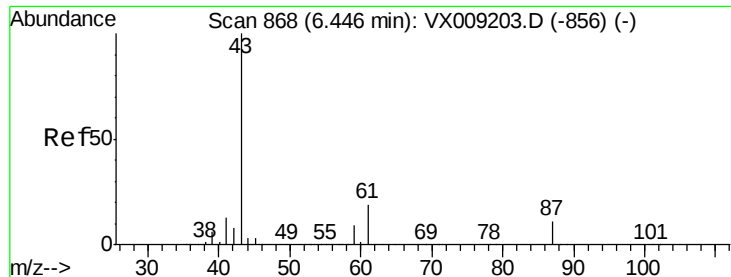

#43

Isopropyl Acetate

Concen: 2.231 ug/l

RT: 6.45 min Scan# 869

Delta R.T. 0.01 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :

EO-01-051519-B


Tot Ion: 43 Resp: 12432

Ion Ratio Lower Upper

43 100

61 19.0 15.1 22.7




87 11.3 9.0 13.6

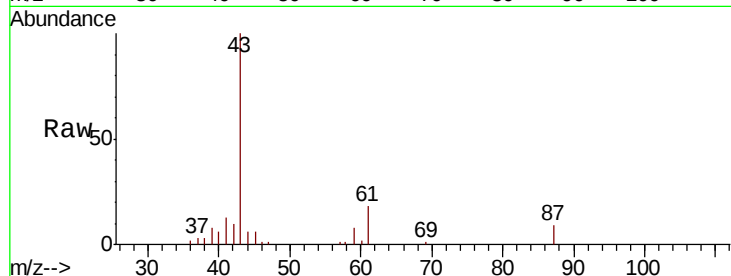

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

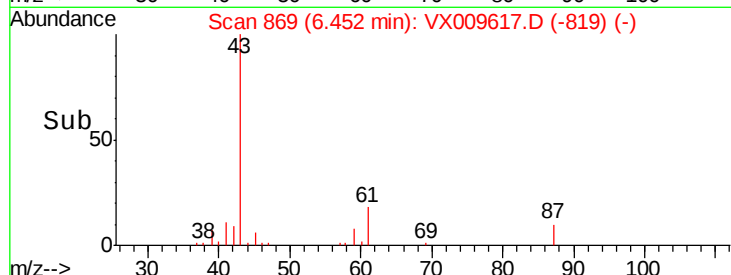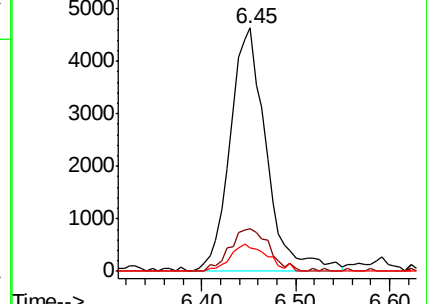

#48

Methyl methacrylate

Concen: 2.746 ug/l

RT: 7.68 min Scan# 1070

Delta R.T. -0.09 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05


Tgt Ion: 41 Resp: 7593

Ion Ratio Lower Upper

41 100

69 0.0 59.1 88.7#



39 0.0 40.4 60.6#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

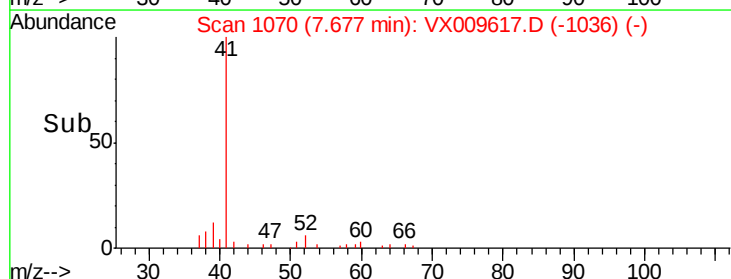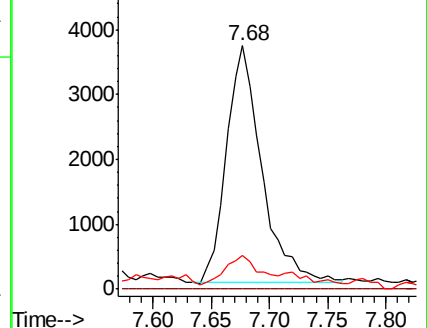



#49

1,4-Dioxane

Concen: 0.339 ug/l

RT: 7.82 min Scan# 1093

Delta R.T. 0.08 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :

EO-01-051519-B


Tot Ion: 88 Resp: 19

Ion Ratio Lower Upper

88 100

43 0.0 28.6 42.8#




58 0.0 61.7 92.5#

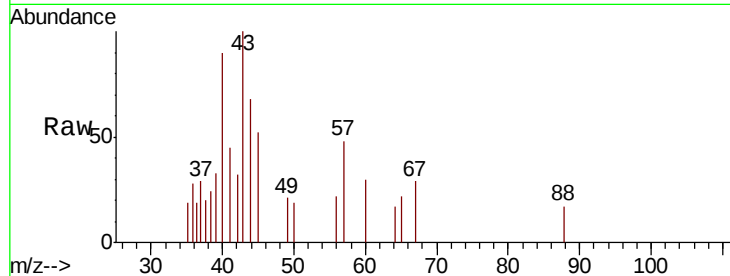

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

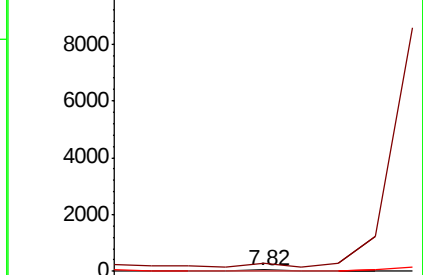

#50

Toluene-d8

Concen: 50.514 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX009617.D


Acq: 16 May 2019 19:05

Tgt Ion: 98 Resp: 344960

Ion Ratio Lower Upper



98 100


100 63.6 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

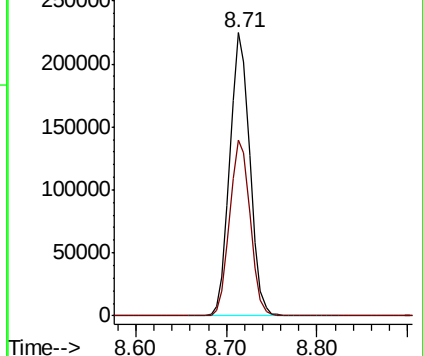

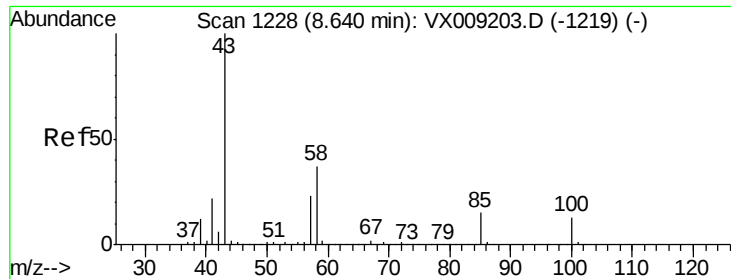

#51

4-Methyl-2-Pentanone

Concen: 23.632 ug/l

RT: 8.61 min Scan# 1223

Delta R.T. -0.03 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :


EO-01-051519-B

Tot Ion: 43 Resp: 86082

Ion Ratio Lower Upper




43 100

58 7.6 29.5 44.3#

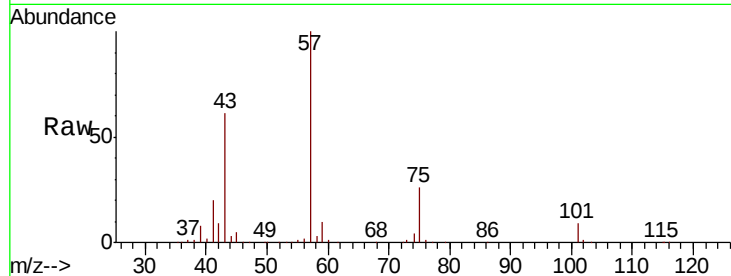

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

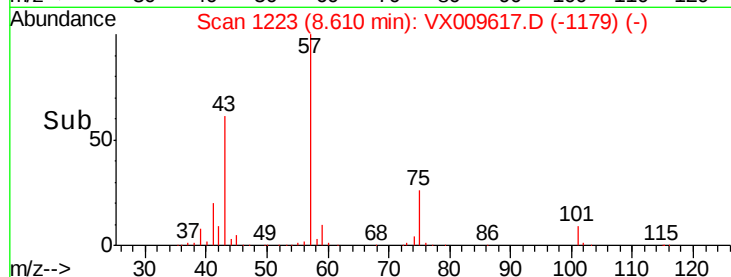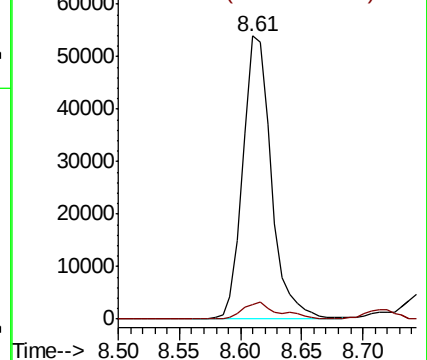

#54

cis-1,3-Dichloropropene

Concen: 11.291 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. 0.18 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05


Tgt Ion: 75 Resp: 35816

Ion Ratio Lower Upper

75 100

77 0.4 24.6 36.8#



39 29.6 40.6 60.8#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

Ion 39.00 (38.70 to 39.70): VX0

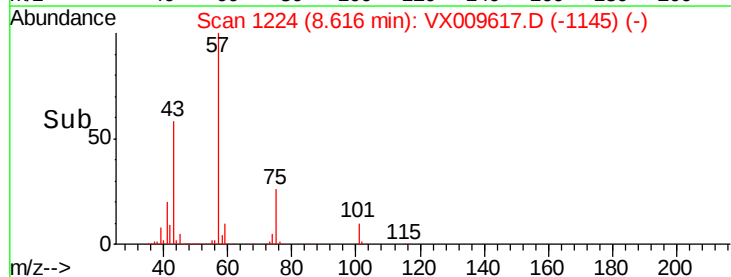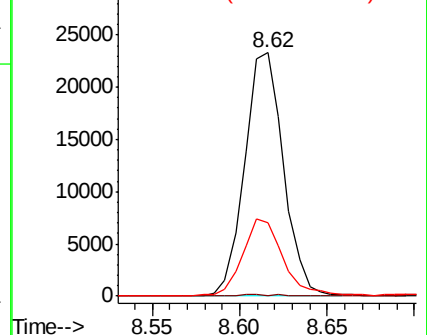



#57

1,3-Dichloropropane

Concen: 2.526 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.17 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :


EO-01-051519-B

Tot Ion: 76 Resp: 8531

Ion Ratio Lower Upper




76 100

78 0.8 25.5 38.3#

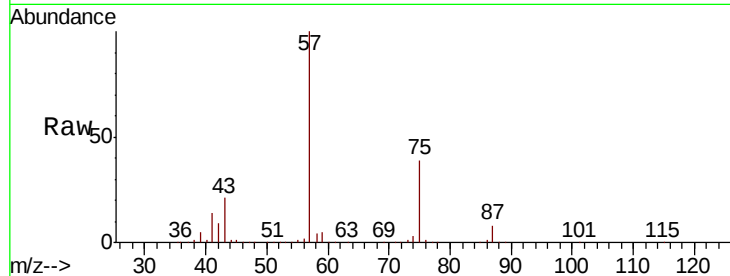

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

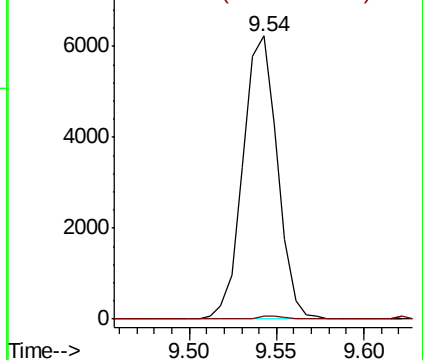

#59

2-Hexanone

Concen: 4.231 ug/l

RT: 9.44 min Scan# 1359

Delta R.T. -0.05 min

Lab File: VX009617.D


Acq: 16 May 2019 19:05

Tgt Ion: 43 Resp: 12105

Ion Ratio Lower Upper



43 100


58 0.0 25.9 77.7#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

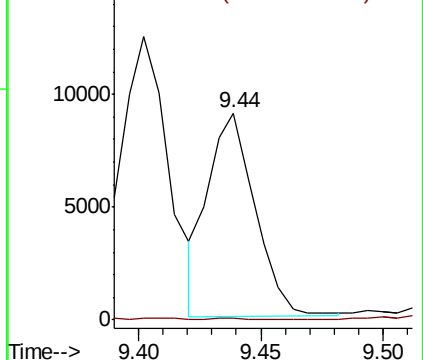



#62

4-Bromofluorobenzene

Concen: 45.347 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :

EO-01-051519-B


Tot Ion: 95 Resp: 112525

Ion Ratio Lower Upper

95 100

174 82.9 0.0 161.6




176 80.8 0.0 159.2



Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

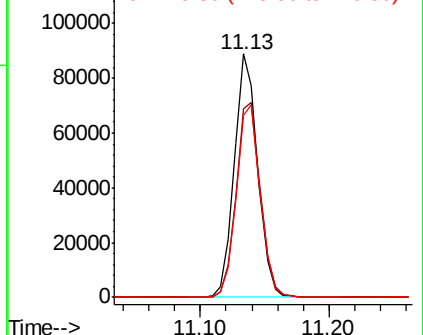

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05


Tgt Ion: 117 Resp: 242329

Ion Ratio Lower Upper

117 100

82 60.2 48.8 73.2



119 31.8 25.8 38.6




Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

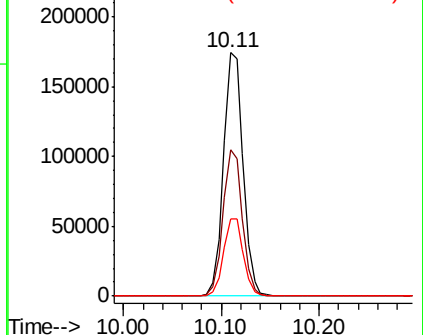

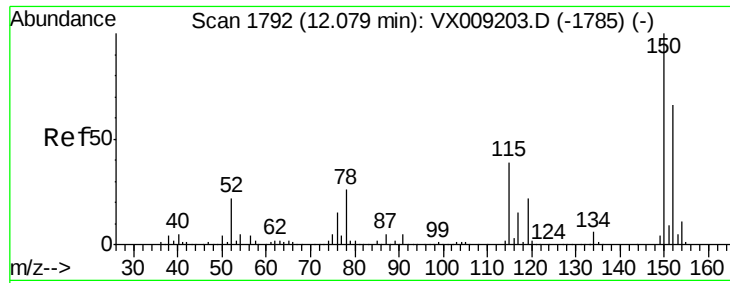

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampled :

EO-01-051519-B


Tot Ion:152 Resp: 103429

Ion Ratio Lower Upper

152 100

115 58.0 41.2 123.6




150 156.7 0.0 346.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

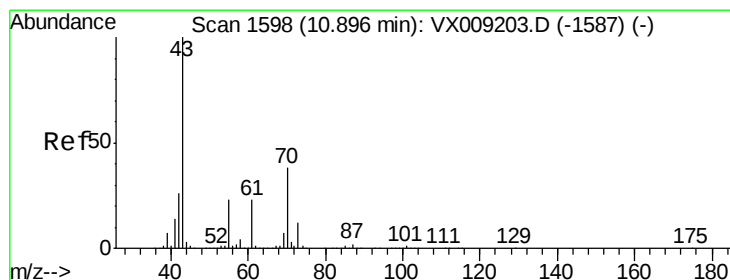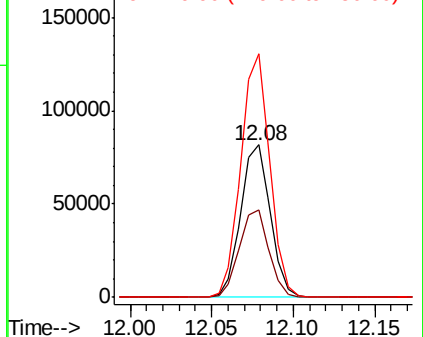

#74

N-ethyl acetate

Concen: 3.174 ug/l

RT: 10.69 min Scan# 1565

Delta R.T. -0.20 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Tgt Ion: 43 Resp: 13917


Ion Ratio Lower Upper

43 100

70 2.7 30.0 45.0#

55 4.7 17.9 26.9#

61 9.8 18.4 27.6#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0




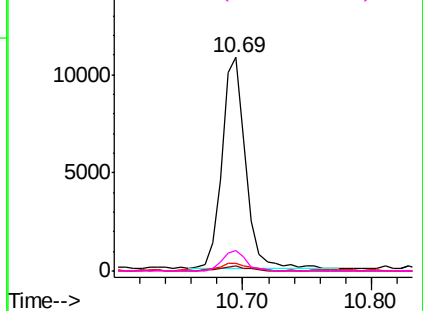




#76
 1,2,3-Trichloropropane
 Concen: 24.250 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.16 min
 Lab File: VX009617.D
 Acq: 16 May 2019 19:05




Instrument :
 MSVOA_X
 ClientSampleId :
 EO-01-051519-B


Tot Ion: 75 Resp: 58179
 Ion Ratio Lower Upper
 75 100
 77 1.4 22.1 66.1#

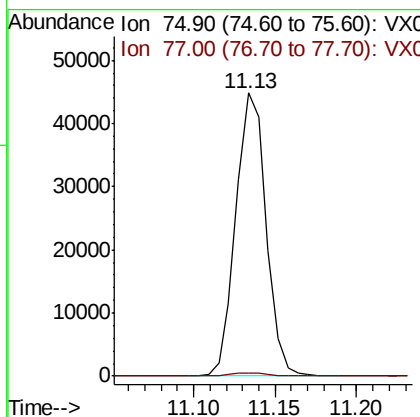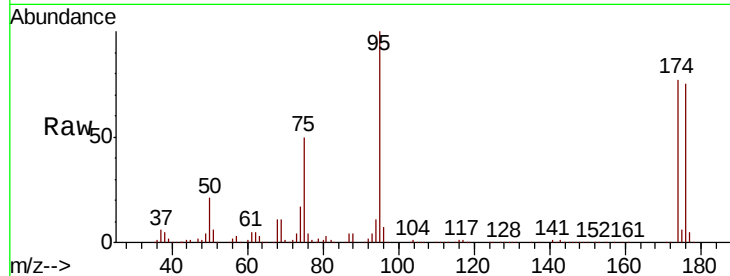

#80
 1,3,5-Trimethylbenzene
 Concen: 0.462 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. -0.00 min
 Lab File: VX009617.D
 Acq: 16 May 2019 19:05

Tgt Ion: 105 Resp: 2927
 Ion Ratio Lower Upper
 105 100
 120 46.9 24.3 72.9

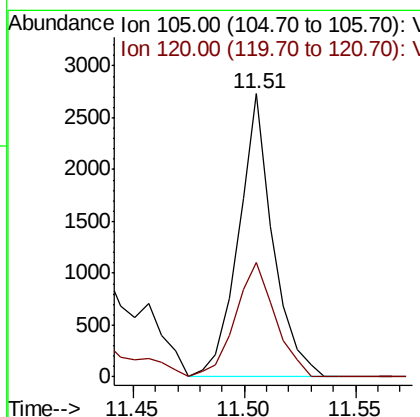



#81

trans-1,4-Dichloro-2-butene

Concen: 62.046 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX009617.D

Acq: 16 May 2019 19:05

Instrument :

MSVOA_X

ClientSampleId :

EO-01-051519-B


Tot Ion: 75 Resp: 58179

Ion Ratio Lower Upper




75 100

53 0.1 79.0 118.6#

89 0.0 34.7 52.1#

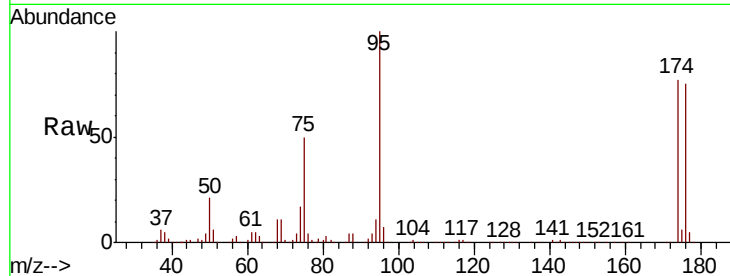

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 53.00 (52.70 to 53.70): VX0
Ion 88.90 (88.60 to 89.60): VX0

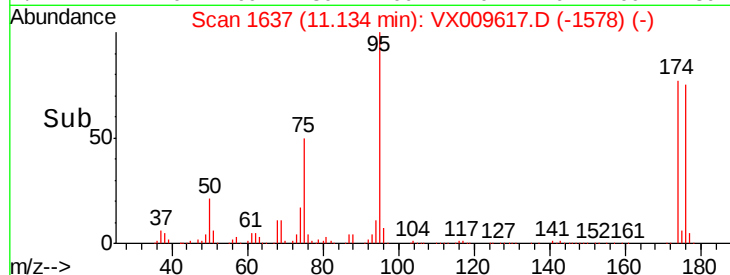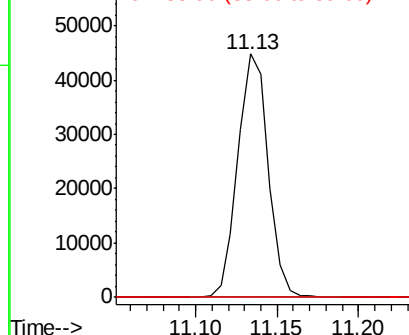

#84

1,2,4-Trimethylbenzene

Concen: 0.371 ug/l

RT: 11.80 min Scan# 1747

Delta R.T. -0.00 min

Lab File: VX009617.D


Acq: 16 May 2019 19:05

Tgt Ion: 105 Resp: 2356



Ion Ratio Lower Upper


105 100

120 47.4 22.0 66.0



Abundance Ion 105.00 (104.70 to 105.70): V
Ion 120.00 (119.70 to 120.70): V

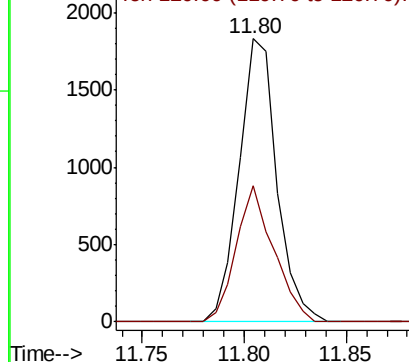


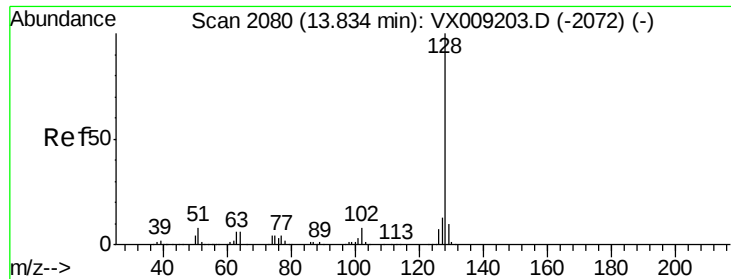

#95
Naphthalene
Concen: 1.061 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. -0.00 min
Lab File: VX009617.D
Acq: 16 May 2019 19:05

Instrument :
MSVOA_X
ClientSampleId :
EO-01-051519-B

Tot Ion	Ratio	Lower	Upper
128	100		
127	12.4	10.4	15.6
129	12.0	8.6	13.0



Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

