

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051623\
 Data File : VX035686.D
 Acq On : 16 May 2023 13:20
 Operator : JC/MD
 Sample : 02751-06DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-PRO-02-71-05082023DL

Quant Time: May 17 05:29:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	202819	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	368397	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	334865	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	150480	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	167415	47.316	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	94.640%		
35) Dibromofluoromethane	5.385	113	118984	47.891	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.780%		
50) Toluene-d8	8.647	98	443613	48.333	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.660%		
62) 4-Bromofluorobenzene	11.079	95	181348	49.072	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.140%		
Target Compounds						
						Qvalue
5) Bromomethane	1.611	94	443	0.300	ug/l	# 40
11) Tert butyl alcohol	2.940	59	625	1.001	ug/l	# 73
13) Acrolein	2.239	56	272	0.367	ug/l	# 71
15) Acrylonitrile	3.081	53	460	0.335	ug/l	# 85
16) Acetone	2.404	43	1726	1.135	ug/l	# 77
17) Carbon Disulfide	2.514	76	1585	0.291	ug/l	# 95
20) Methylene Chloride	2.788	84	892	0.324	ug/l	# 60
21) trans-1,2-Dichloroethene	3.093	96	580	0.234	ug/l	90
25) 2-Butanone	4.568	43	554	0.263	ug/l	# 51
27) cis-1,2-Dichloroethene	4.489	96	1946	0.654	ug/l	96
31) Cyclohexane	5.550	56	5825	1.303	ug/l	# 5
32) 1,1,1-Trichloroethane	5.391	97	8408	1.861	ug/l	97
36) 1,1-Dichloropropene	5.550	75	18837	4.803	ug/l	# 51
38) Carbon Tetrachloride	5.550	117	23592	6.351	ug/l	# 15
44) Trichloroethene	7.123	130	80975	29.109	ug/l	91
49) 1,4-Dioxane	7.714	88	28	2.360	ug/l	# 23
60) Dibromochloromethane	9.275	129	4546	1.753	ug/l	# 10
64) Tetrachloroethene	9.275	164	3921	1.739	ug/l	92
76) 1,2,3-Trichloropropane	11.079	75	101172	27.486	ug/l	# 34
81) trans-1,4-Dichloro-2-b...	11.079	75	101172	88.585	ug/l	# 8
82) 4-Chlorotoluene	11.457	91	2517	0.234	ug/l	90
86) p-Isopropyltoluene	12.006	119	2456	0.227	ug/l	# 69
87) 1,3-Dichlorobenzene	11.969	146	1547	0.283	ug/l	98
88) 1,4-Dichlorobenzene	11.969	146	1547	0.280	ug/l	98
89) n-Butylbenzene	12.329	91	2798	0.284	ug/l	96
91) 1,2-Dichlorobenzene	12.335	146	1125	0.210	ug/l	97
93) 1,2,4-Trichlorobenzene	13.591	180	1677	0.520	ug/l	94
94) Hexachlorobutadiene	13.725	225	751	0.587	ug/l	96
95) Naphthalene	13.780	128	3647	0.330	ug/l	96
96) 1,2,3-Trichlorobenzene	13.963	180	1588	0.501	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051623\
 Data File : VX035686.D
 Acq On : 16 May 2023 13:20
 Operator : JC/MD
 Sample : 02751-06DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-PRO-02-71-05082023DL

Quant Time: May 17 05:29:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration




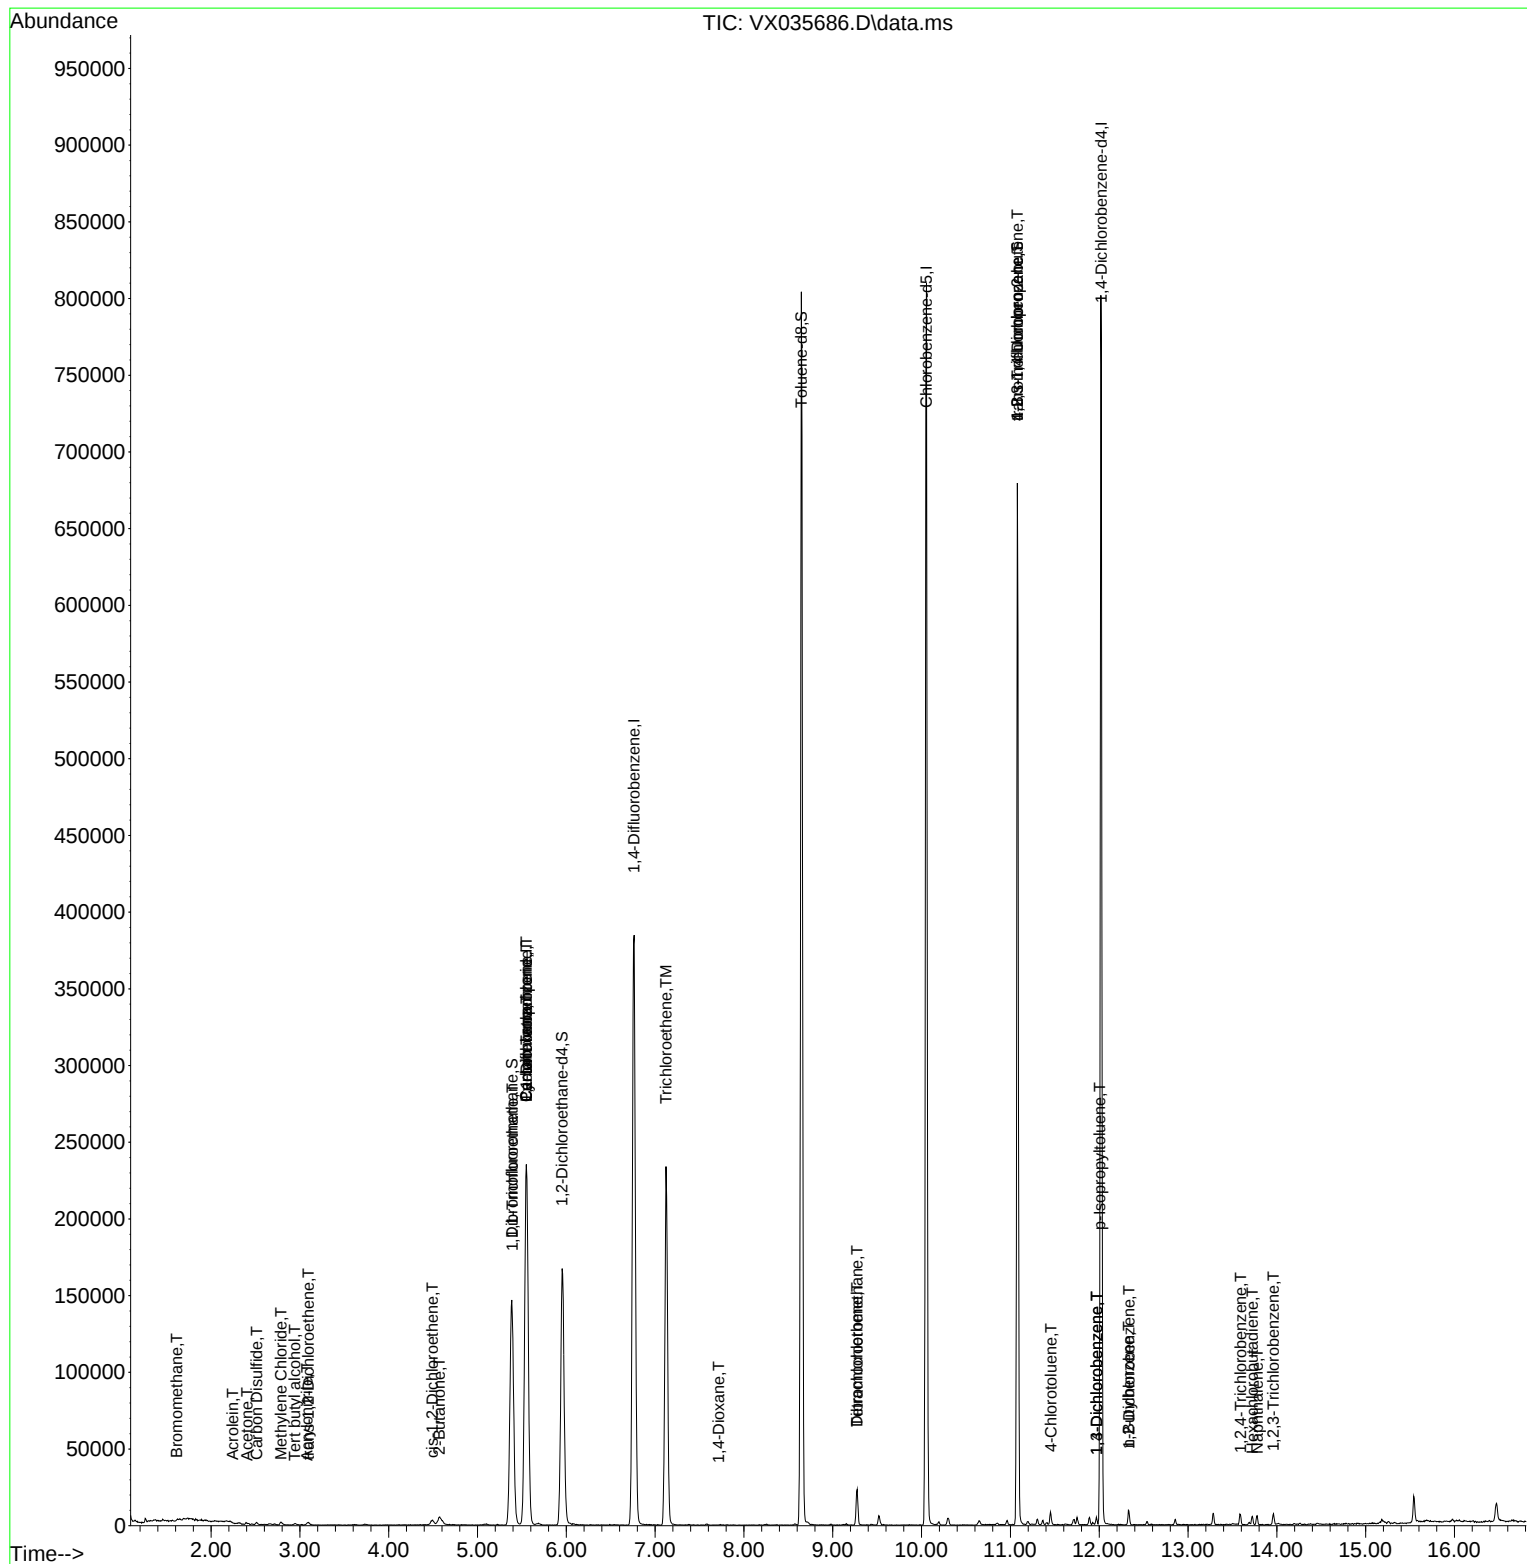




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion:168 Resp: 202819
Ion Ratio Lower Upper
168 100
99 69.5 45.7 68.5#



#5
Bromomethane
Concen: 0.300 ug/l
RT: 1.611 min Scan# 86
Delta R.T. -0.007 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 94 Resp: 443
Ion Ratio Lower Upper
94 100
96 37.3 77.0 115.6#





#11

Tert butyl alcohol

Concen: 1.001 ug/l

RT: 2.940 min Scan# 30

Delta R.T. -0.061 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Instrument :

MSVOA_X

ClientSampleId :





FSND-PRO-02-71-05082023DL

Tgt Ion: 59 Resp: 625

Ion Ratio Lower Upper

59 100

57 0.0 8.1 12.1#

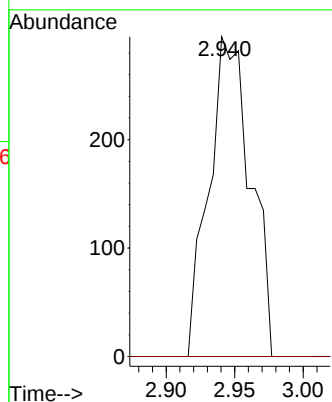

#13

Acrolein

Concen: 0.367 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX035686.D




Acq: 16 May 2023 13:20


Tgt Ion: 56 Resp: 272

Ion Ratio Lower Upper

56 100

55 94.9 56.6 85.0#


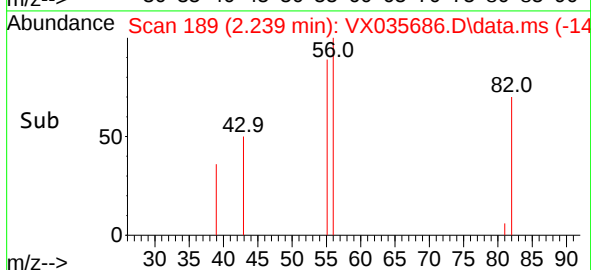






#15
Acrylonitrile
Concen: 0.335 ug/l
RT: 3.081 min Scan# 31
Delta R.T. 0.013 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion: 53 Resp: 460
Ion Ratio Lower Upper
53 100
52 71.1 66.2 99.2
51 23.7 28.3 42.5#

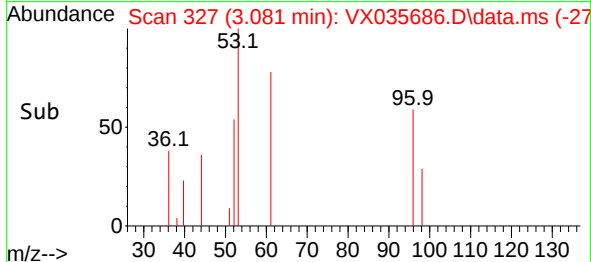

#16
Acetone
Concen: 1.135 ug/l
RT: 2.404 min Scan# 216
Delta R.T. 0.012 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 43 Resp: 1726
Ion Ratio Lower Upper
43 100
58 18.1 24.7 37.1#

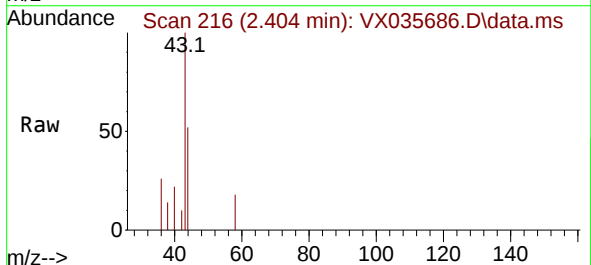



#17

Carbon Disulfide

Concen: 0.291 ug/l

RT: 2.514 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Instrument :

MSVOA_X

ClientSampleId :





FSND-PRO-02-71-05082023DL

Tgt Ion: 76 Resp: 1585

Ion Ratio Lower Upper

76 100

78 10.9 7.2 10.8#

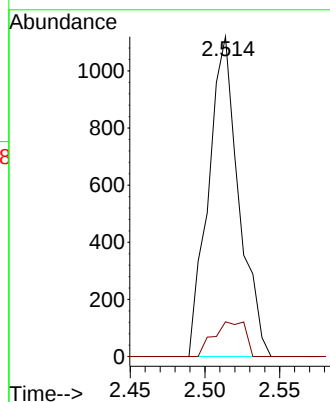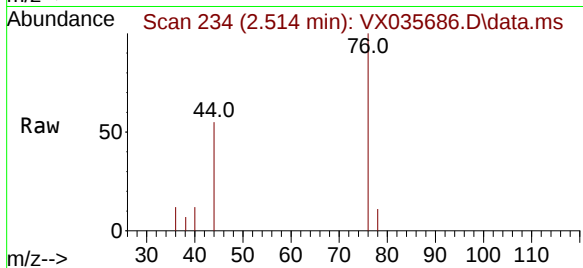

#20

Methylene Chloride

Concen: 0.324 ug/l

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Tgt Ion: 84 Resp: 892




Ion Ratio Lower Upper


84 100

49 72.3 103.8 155.8#

51 27.2 31.8 47.8#

86 37.8 51.4 77.2#


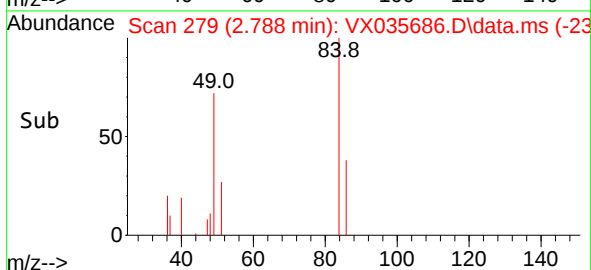
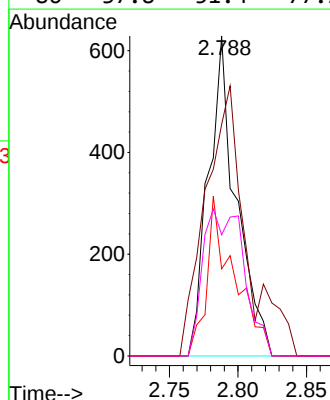
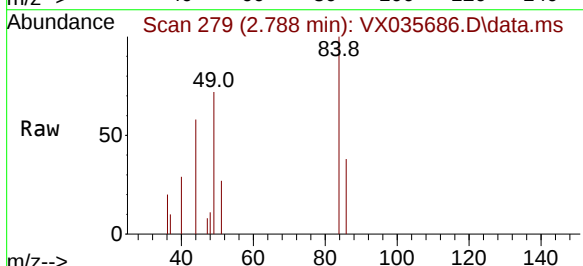




#21
trans-1,2-Dichloroethene
Concen: 0.234 ug/l
RT: 3.093 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion: 96 Resp: 580
Ion Ratio Lower Upper
96 100
61 152.6 113.0 169.6
98 55.8 52.1 78.1

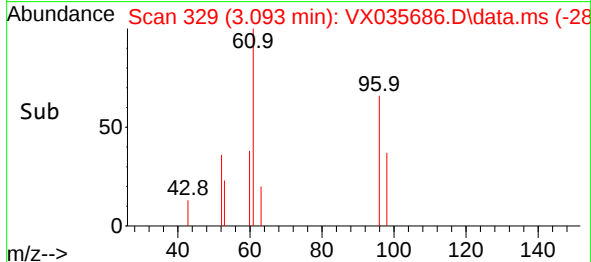

#25
2-Butanone
Concen: 0.263 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.012 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 43 Resp: 554
Ion Ratio Lower Upper
43 100
72 0.0 19.3 28.9#





#27

cis-1,2-Dichloroethene

Concen: 0.654 ug/l

RT: 4.489 min Scan# 51

Delta R.T. -0.000 min

Lab File: VX035686.D


Acq: 16 May 2023 13:20

Instrument :




MSVOA_X

ClientSampleId :

FSND-PRO-02-71-05082023DL

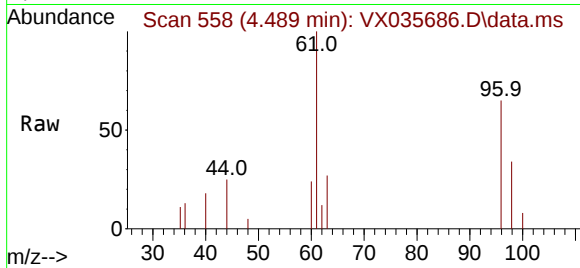

Tgt Ion:	96	Resp:	1946
Ion	Ratio	Lower	Upper
96	100		
61	145.7	0.0	300.4
98	61.6	0.0	129.0

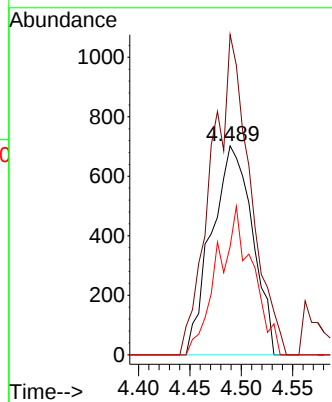

#31

Cyclohexane

Concen: 1.303 ug/l




RT: 5.550 min Scan# 732


Delta R.T. 0.079 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Tgt Ion:	56	Resp:	5825
Ion	Ratio	Lower	Upper
56	100		
69	157.1	23.7	35.5#
84	128.1	68.5	102.7#




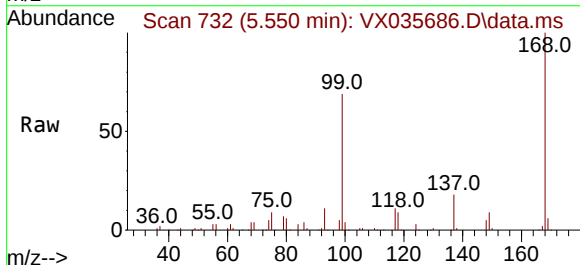




#32
1,1,1-Trichloroethane
Concen: 1.861 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion: 97 Resp: 8408
Ion Ratio Lower Upper
97 100
99 62.2 51.1 76.7
61 48.0 36.5 54.7



#33
1,2-Dichloroethane-d4
Concen: 47.316 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 65 Resp: 167415
Ion Ratio Lower Upper
65 100
67 48.9 0.0 104.0









#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion:114 Resp: 368397
Ion Ratio Lower Upper
114 100
63 23.8 0.0 42.2
88 18.4 0.0 33.2

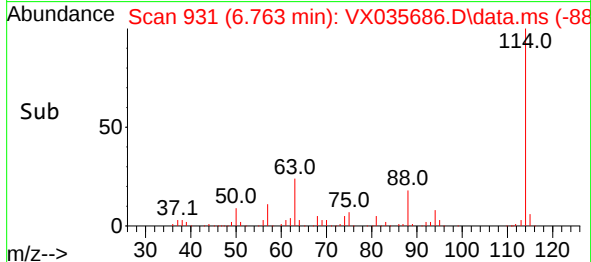

#35
Dibromofluoromethane
Concen: 47.891 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion:113 Resp: 118984
Ion Ratio Lower Upper
113 100
111 103.5 83.7 125.5
192 17.4 15.4 23.2




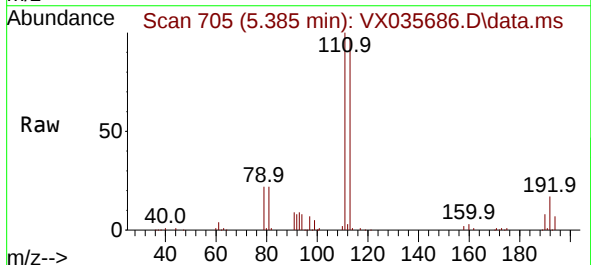




#36
 1,1-Dichloropropene
 Concen: 4.803 ug/l
 RT: 5.550 min Scan# 712
 Delta R.T. -0.140 min
 Lab File: VX035686.D
 Acq: 16 May 2023 13:20




Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-PRO-02-71-05082023DL


Tgt Ion: 75 Resp: 18837
 Ion Ratio Lower Upper
 75 100
 110 9.8 17.5 52.5#
 77 0.0 24.3 36.5#

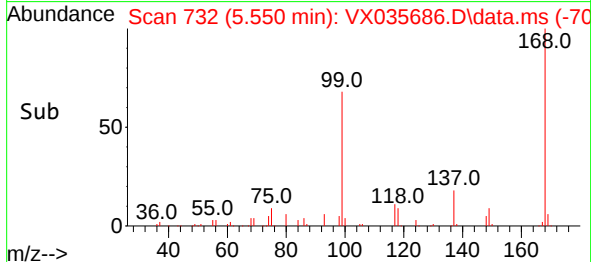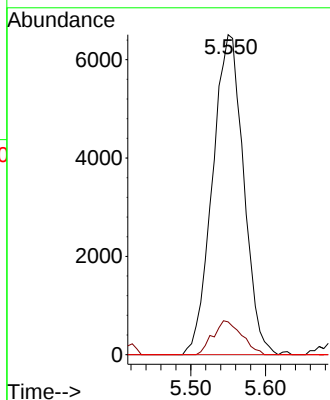

#38
 Carbon Tetrachloride
 Concen: 6.351 ug/l
 RT: 5.550 min Scan# 732
 Delta R.T. -0.128 min
 Lab File: VX035686.D
 Acq: 16 May 2023 13:20

Tgt Ion: 117 Resp: 23592
 Ion Ratio Lower Upper
 117 100
 119 4.3 76.6 114.8#
 121 0.0 23.8 35.6#


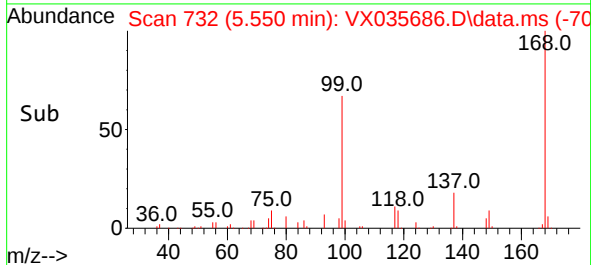
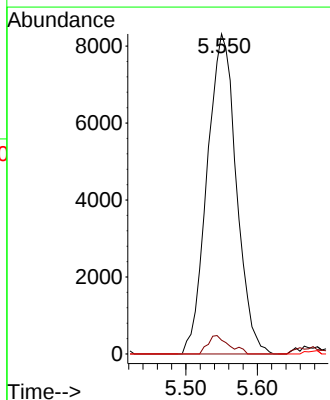





#44
Trichloroethene
Concen: 29.109 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion:130 Resp: 80975
Ion Ratio Lower Upper
130 100
95 107.9 0.0 198.4



#49
1,4-Dioxane
Concen: 2.360 ug/l
RT: 7.714 min Scan# 1087
Delta R.T. 0.006 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 88 Resp: 28
Ion Ratio Lower Upper
88 100
43 0.0 27.7 41.5#
58 0.0 56.8 85.2#


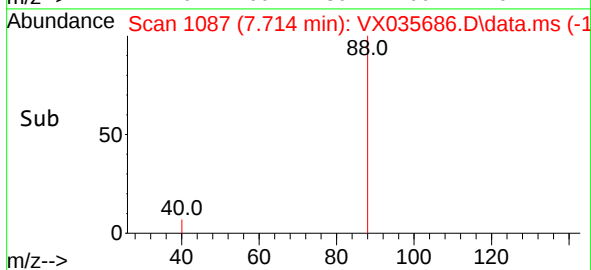






#50
Toluene-d8
Concen: 48.333 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion: 98 Resp: 443613
Ion Ratio Lower Upper
98 100
100 65.5 52.5 78.7

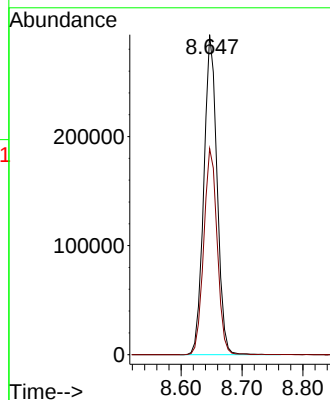

#60
Dibromochloromethane
Concen: 1.753 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.244 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 129 Resp: 4546
Ion Ratio Lower Upper
129 100
127 0.0 39.0 117.0#



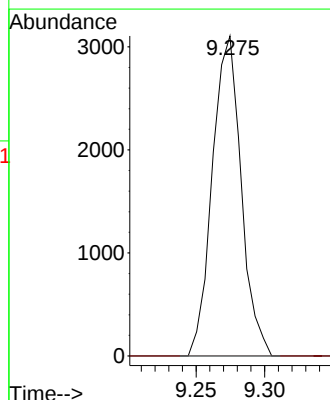





#62
4-Bromofluorobenzene
Concen: 49.072 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion: 95 Resp: 181348
Ion Ratio Lower Upper
95 100
174 65.2 0.0 147.4
176 63.7 0.0 140.6

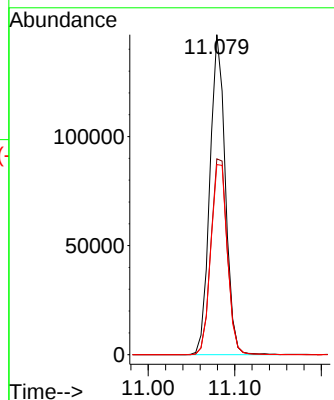

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 117 Resp: 334865
Ion Ratio Lower Upper
117 100
82 60.3 45.0 67.4
119 31.7 26.0 39.0

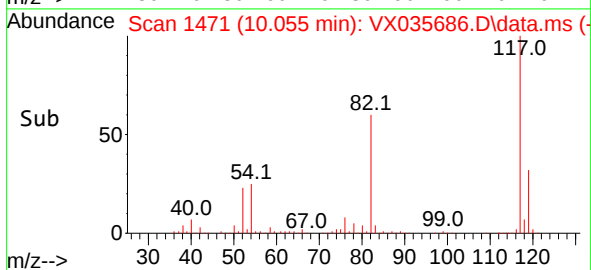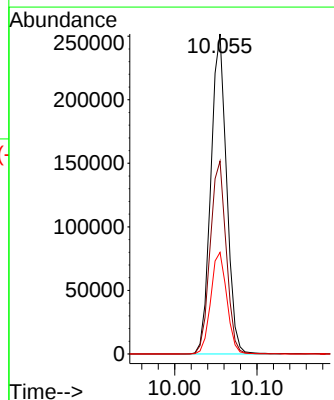



#64

Tetrachloroethene

Concen: 1.739 ug/l

RT: 9.275 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX035686.D


Acq: 16 May 2023 13:20

Instrument :

MSVOA_X

ClientSampleId :

FSND-PRO-02-71-05082023DL



Tgt Ion:164 Resp: 3921




Ion Ratio Lower Upper

164 100

166 119.1 102.7 154.1

129 108.0 75.6 113.4

131 92.5 73.7 110.5

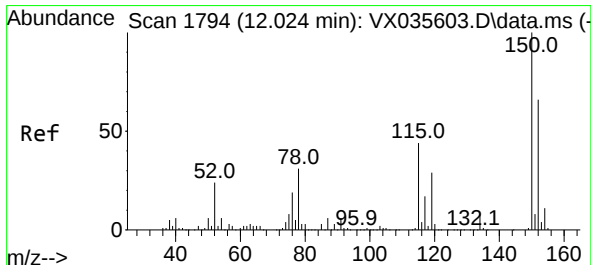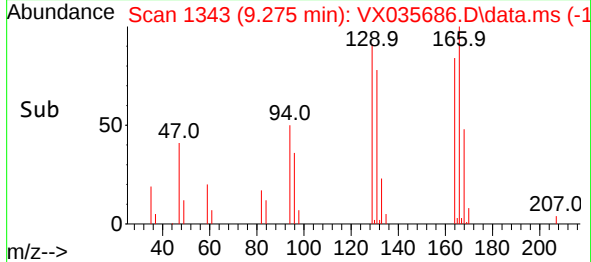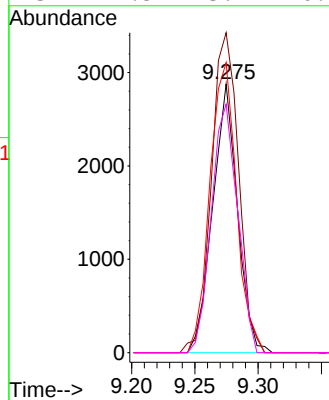

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20




Tgt Ion:152 Resp: 150480


Ion Ratio Lower Upper

152 100

115 66.0 45.0 135.0

150 161.0 0.0 352.4



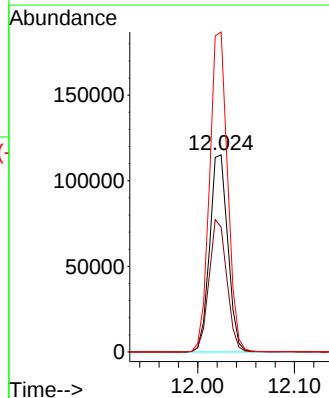
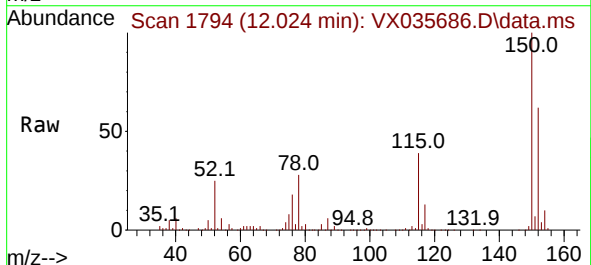




#76
1,2,3-Trichloropropane
Concen: 27.486 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20




Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-02-71-05082023DL


Tgt Ion: 75 Resp: 101172
Ion Ratio Lower Upper
75 100
77 1.1 21.6 64.8#

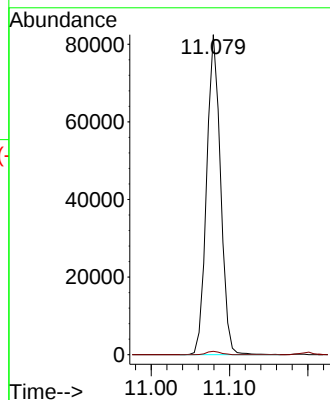

#81
trans-1,4-Dichloro-2-butene
Concen: 88.585 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX035686.D
Acq: 16 May 2023 13:20

Tgt Ion: 75 Resp: 101172
Ion Ratio Lower Upper
75 100
53 0.0 82.6 124.0#
89 0.0 36.9 55.3#

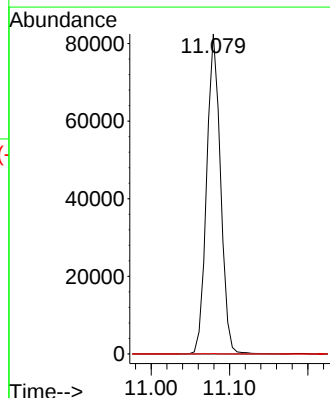



#82

4-Chlorotoluene

Concen: 0.234 ug/l

RT: 11.457 min Scan# 1701

Delta R.T. 0.006 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Instrument :

MSVOA_X

ClientSampleId :





FSND-PRO-02-71-05082023DL

Tgt Ion: 91 Resp: 2517

Ion Ratio Lower Upper

91 100

126 22.9 14.2 42.6

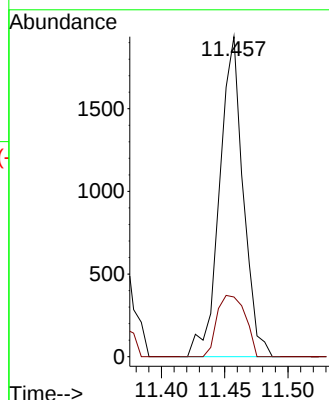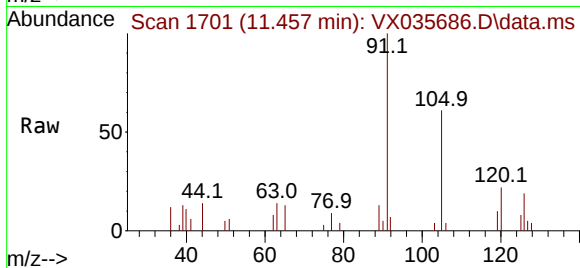

#86

p-Isopropyltoluene

Concen: 0.227 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20




Tgt Ion: 119 Resp: 2456


Ion Ratio Lower Upper

119 100

134 35.4 13.2 39.5

91 47.9 12.9 38.7#

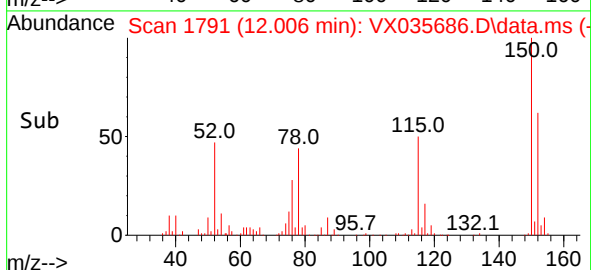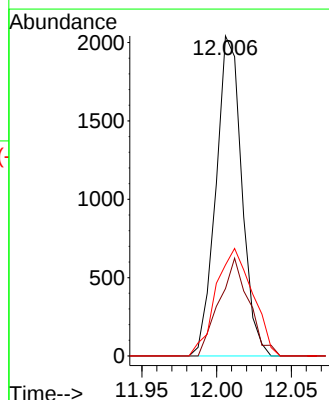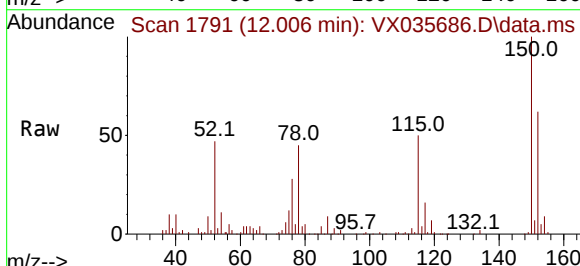



#87

1,3-Dichlorobenzene

Concen: 0.283 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Instrument :

MSVOA_X

ClientSampleId :

FSND-PRO-02-71-05082023DL





Tgt Ion:146 Resp: 1547

Ion Ratio Lower Upper

146 100

111 44.0 20.9 62.8

148 63.0 31.6 95.0



#88

1,4-Dichlorobenzene

Concen: 0.280 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.073 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20




Tgt Ion:146 Resp: 1547


Ion Ratio Lower Upper

146 100

111 44.0 20.6 61.9

148 63.0 31.8 95.4

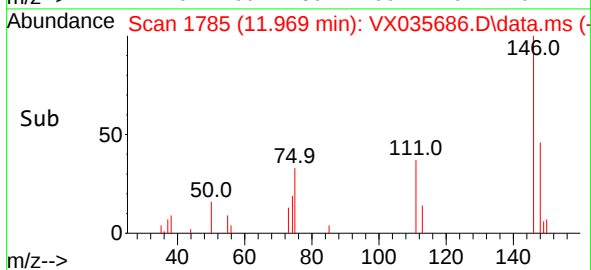



#89

n-Butylbenzene

Concen: 0.284 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Instrument :

MSVOA_X

ClientSampleId :

FSND-PRO-02-71-05082023DL





Tgt Ion: 91 Resp: 2798

Ion Ratio Lower Upper

91 100

92 52.5 27.7 83.0

134 24.3 13.0 38.9

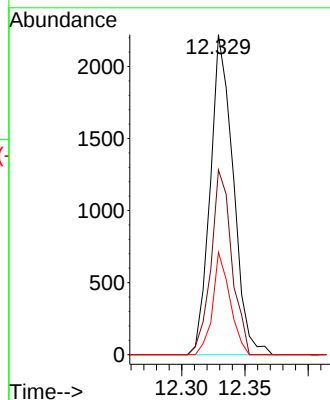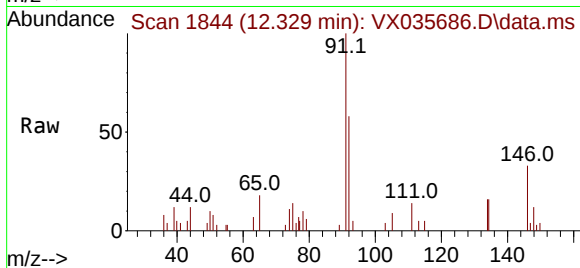

#91

1,2-Dichlorobenzene

Concen: 0.210 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20




Tgt Ion: 146 Resp: 1125


Ion Ratio Lower Upper

146 100

111 44.9 22.0 66.0

148 60.4 32.0 96.0

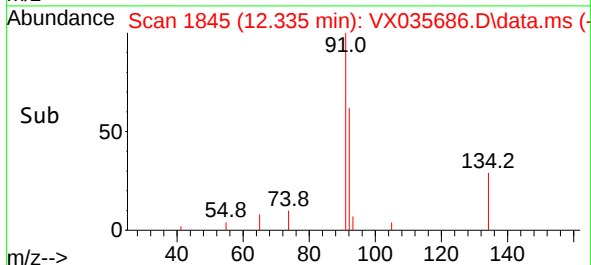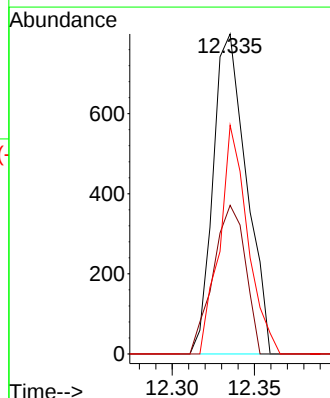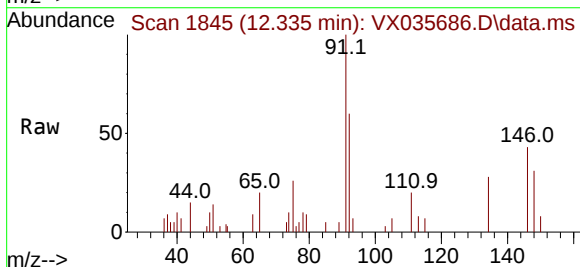



#93

1,2,4-Trichlorobenzene

Concen: 0.520 ug/l

RT: 13.591 min Scan# 2050

Delta R.T. 0.006 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Instrument :

MSVOA_X

ClientSampleId :

FSND-PRO-02-71-05082023DL





Tgt Ion:180 Resp: 1677

Ion Ratio Lower Upper

180 100

182 90.9 47.0 141.0

145 40.3 15.9 47.7

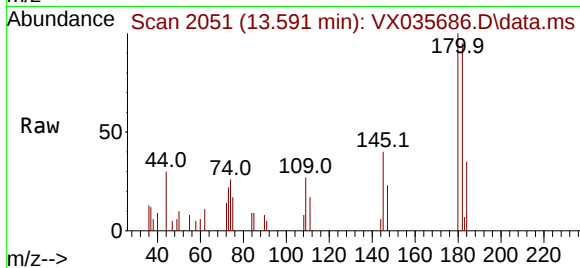

#94

Hexachlorobutadiene

Concen: 0.587 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20




Tgt Ion:225 Resp: 751


Ion Ratio Lower Upper

225 100

223 58.7 32.1 96.5

227 65.0 31.8 95.4

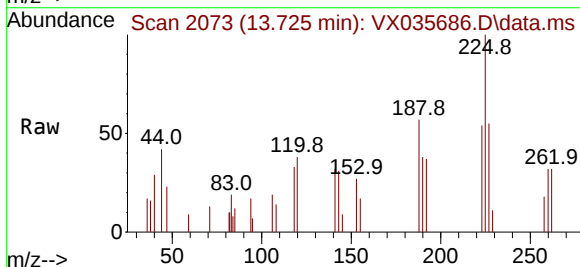

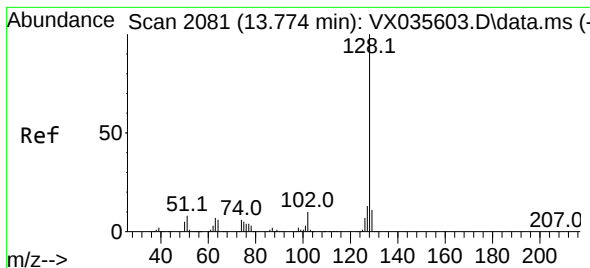

#95

Naphthalene

Concen: 0.330 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20





Instrument :

MSVOA_X

ClientSampleId :

FSND-PRO-02-71-05082023DL

Tgt Ion:128	Resp:	3647
Ion Ratio	Lower	Upper
128	100	
127	14.7	10.2 15.4
129	11.7	8.6 13.0

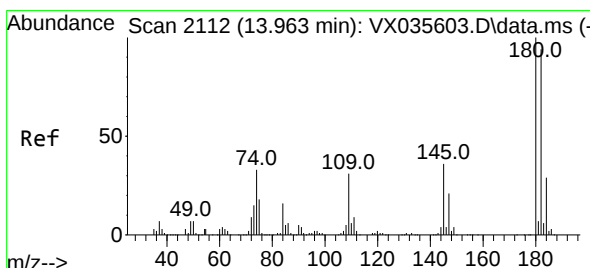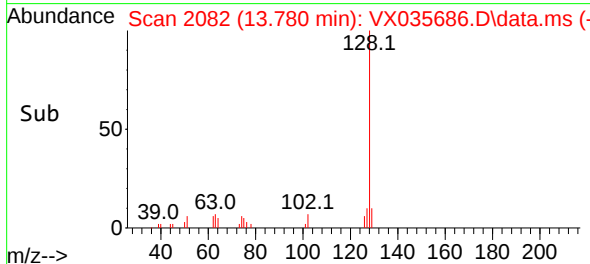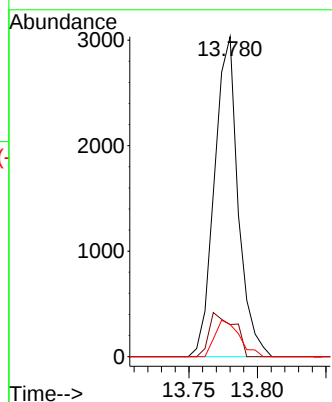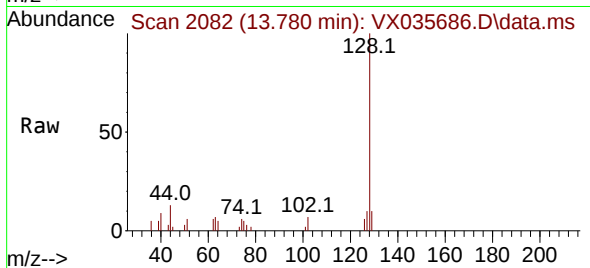

#96

1,2,3-Trichlorobenzene

Concen: 0.501 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX035686.D

Acq: 16 May 2023 13:20

Tgt Ion:180	Resp:	1588
Ion Ratio	Lower	Upper
180	100	
182	87.6	48.0 144.2
145	37.0	17.7 53.1

