

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051623\
 Data File : VX035680.D
 Acq On : 16 May 2023 10:33
 Operator : JC/MD
 Sample : VX0516MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0516MBL01

Quant Time: May 17 05:25:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	200718	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	370565	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	342681	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	161104	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	170875	48.799	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.600%
35) Dibromofluoromethane	5.385	113	122825	49.148	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.300%
50) Toluene-d8	8.647	98	454479	49.227	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.460%
62) 4-Bromofluorobenzene	11.079	95	188350	50.669	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051623\
Data File : VX035680.D
Acq On : 16 May 2023 10:33
Operator : JC/MD
Sample : VX0516MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0516MBL01

Quant Time: May 17 05:25:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260
QLast Update : Thu May 11 13:57:54 2023
Response via : Initial Calibration




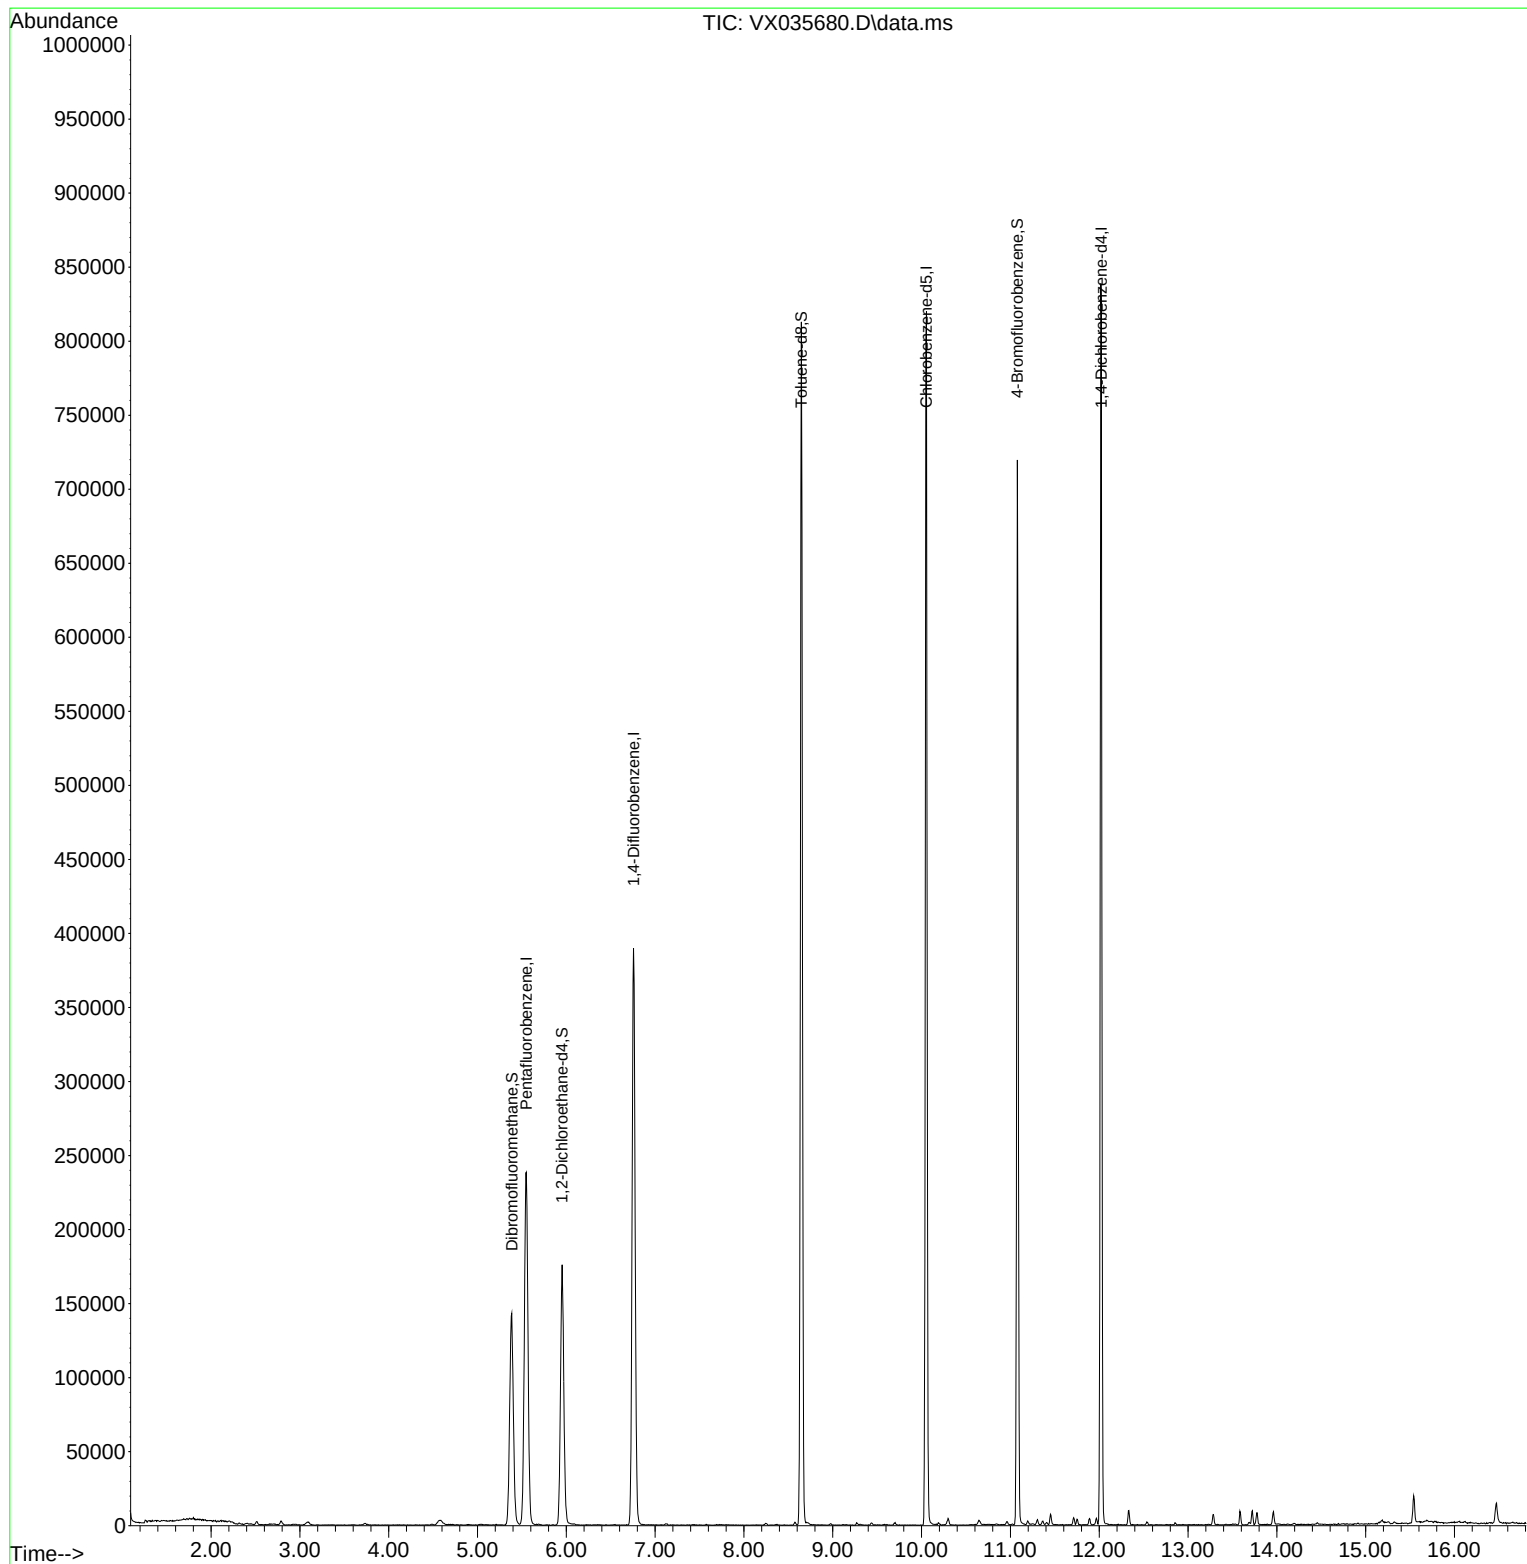


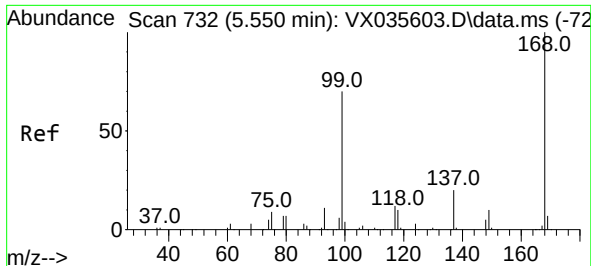

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 718
Delta R.T. -0.000 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33




Instrument :
MSVOA_X
ClientSampleId :
VX0516MBL01


Tgt Ion:168 Resp: 200718
Ion Ratio Lower Upper
168 100
99 72.0 45.7 68.5#

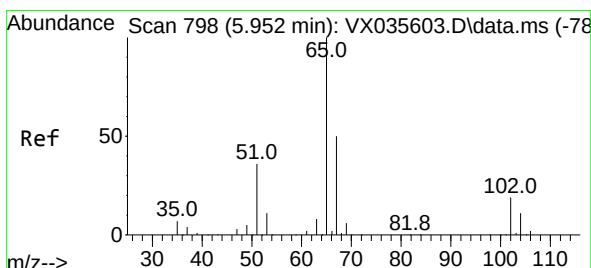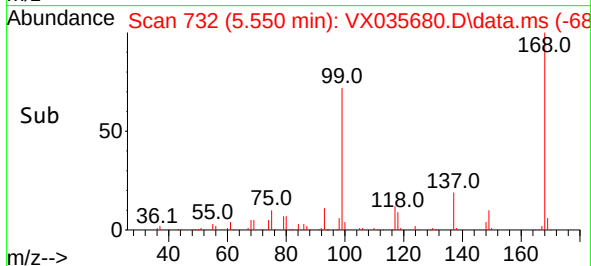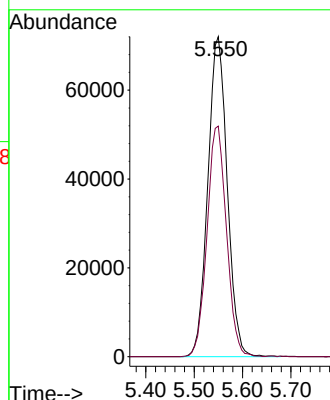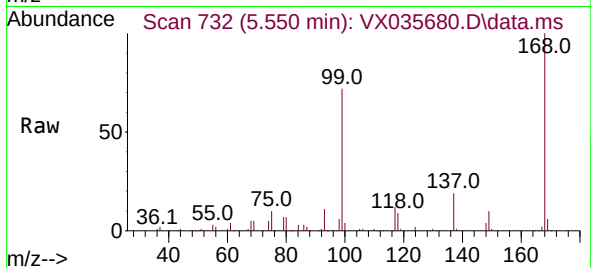

#33
1,2-Dichloroethane-d4
Concen: 48.799 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33

Tgt Ion: 65 Resp: 170875
Ion Ratio Lower Upper
65 100
67 49.7 0.0 104.0


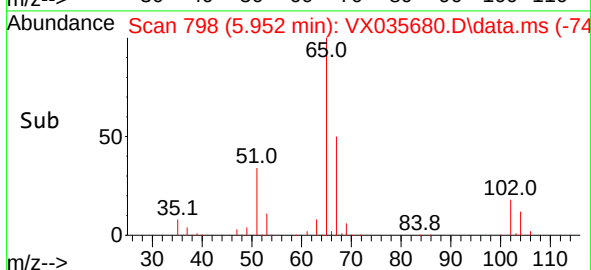
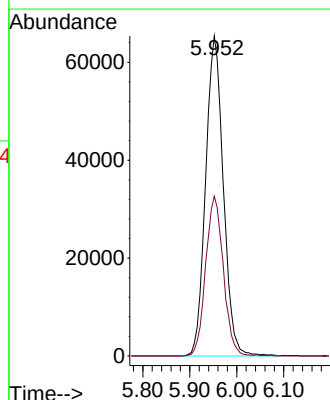
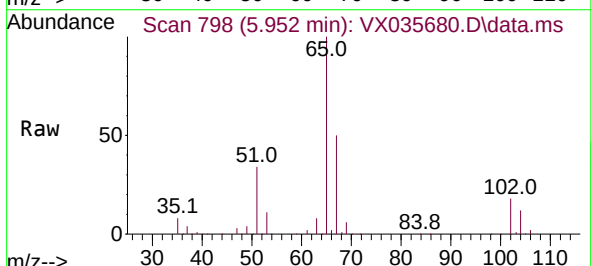


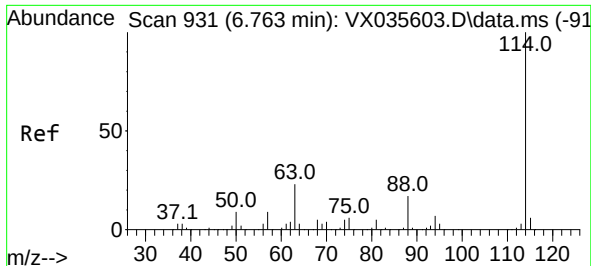

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. -0.006 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33




Instrument :
MSVOA_X
ClientSampleId :
VX0516MBL01


Tgt Ion:114 Resp: 370565
Ion Ratio Lower Upper
114 100
63 24.4 0.0 42.2
88 18.2 0.0 33.2

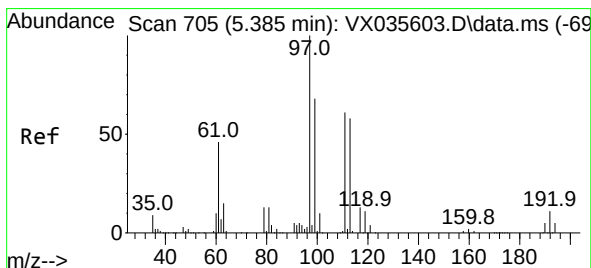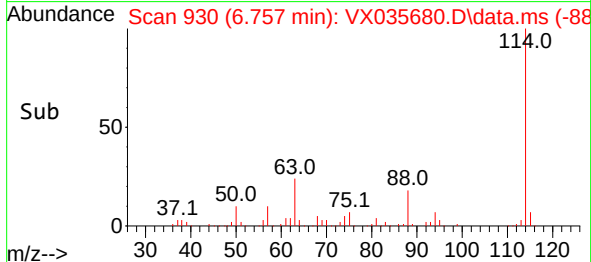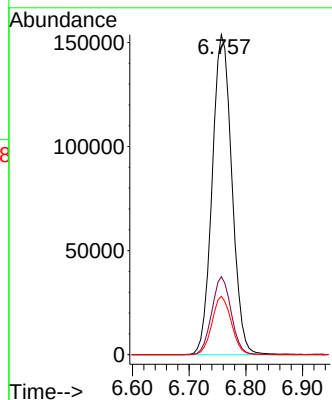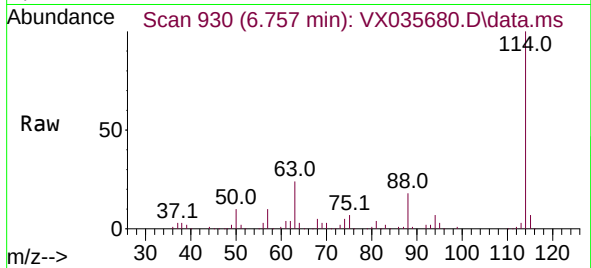

#35
Dibromofluoromethane
Concen: 49.148 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33

Tgt Ion:113 Resp: 122825
Ion Ratio Lower Upper
113 100
111 102.5 83.7 125.5
192 17.3 15.4 23.2


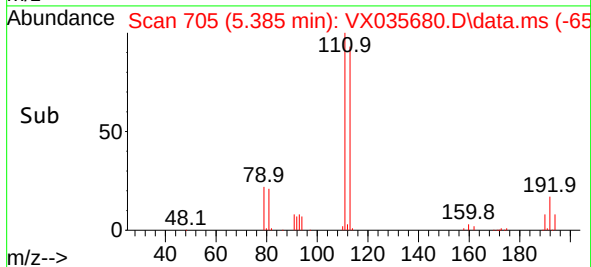
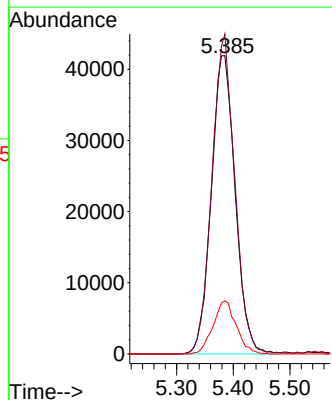
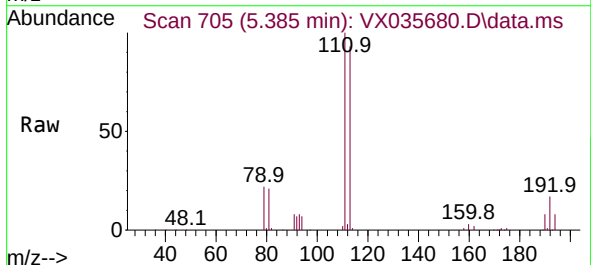


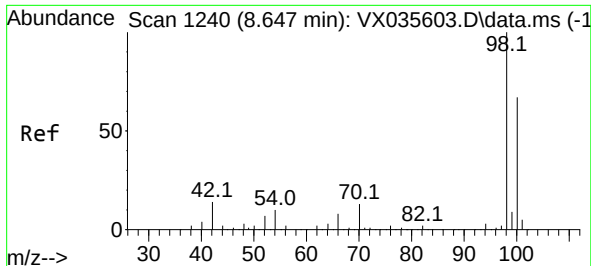

#50
Toluene-d8
Concen: 49.227 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33




Instrument :
MSVOA_X
ClientSampleId :
VX0516MBL01


Tgt Ion: 98 Resp: 454479
Ion Ratio Lower Upper
98 100
100 65.4 52.5 78.7

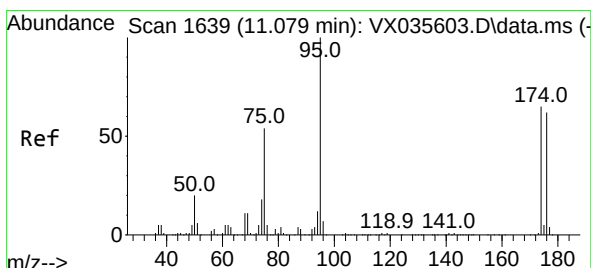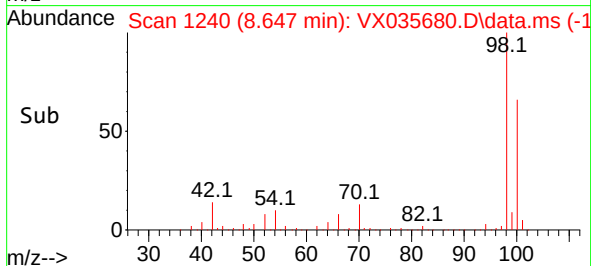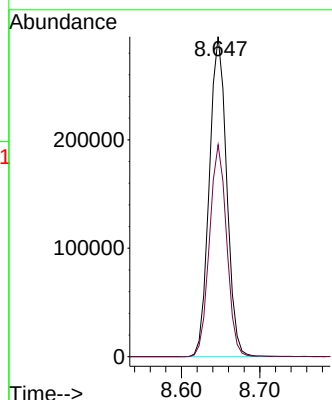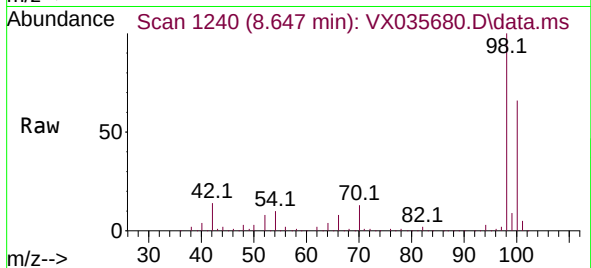

#62
4-Bromofluorobenzene
Concen: 50.669 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33

Tgt Ion: 95 Resp: 188350
Ion Ratio Lower Upper
95 100
174 67.0 0.0 147.4
176 63.7 0.0 140.6


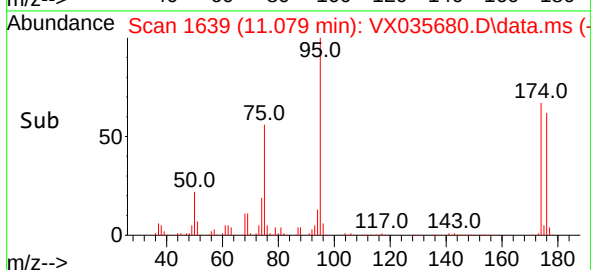
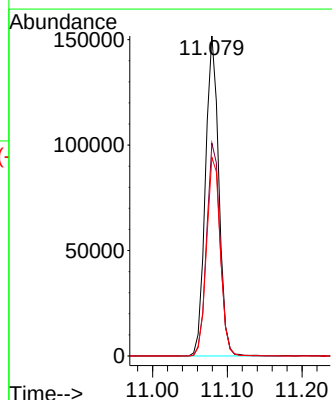
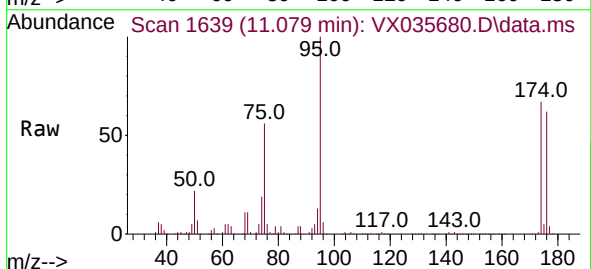


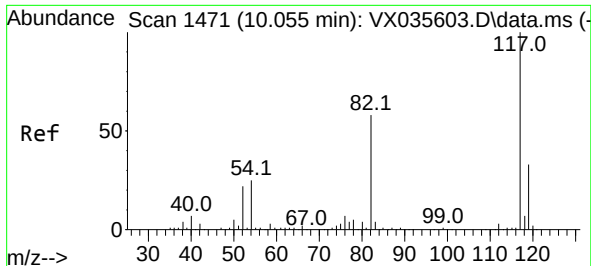

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33

Instrument :
MSVOA_X
ClientSampleId :
VX0516MBL01

Tgt Ion:117 Resp: 342681
Ion Ratio Lower Upper
117 100
82 61.7 45.0 67.4
119 33.2 26.0 39.0

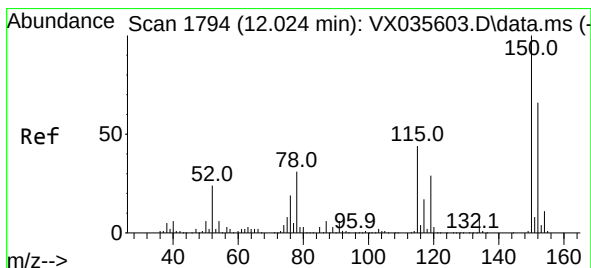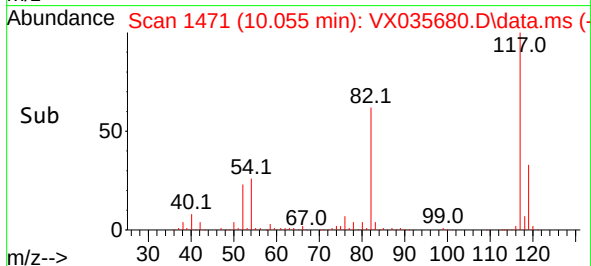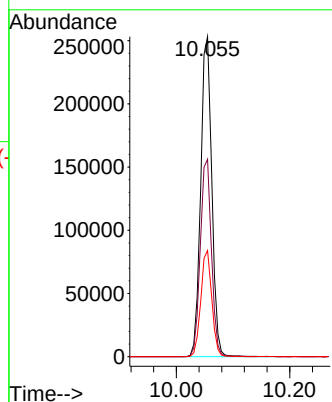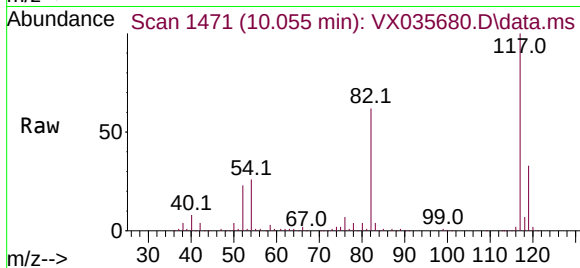

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX035680.D
Acq: 16 May 2023 10:33

Tgt Ion:152 Resp: 161104
Ion Ratio Lower Upper
152 100
115 65.4 45.0 135.0
150 157.8 0.0 352.4

