

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051623\
 Data File : VX035690.D
 Acq On : 16 May 2023 14:53
 Operator : JC/MD
 Sample : 02751-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-TB-01-05102023

Quant Time: May 17 05:30:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	180677	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	335506	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	301471	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	129956	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	154167	48.911	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.820%
35) Dibromofluoromethane	5.385	113	107256	47.403	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.800%
50) Toluene-d8	8.647	98	398746	47.704	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.400%
62) 4-Bromofluorobenzene	11.079	95	159432	47.371	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.740%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051623\
Data File : VX035690.D
Acq On : 16 May 2023 14:53
Operator : JC/MD
Sample : 02751-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-TB-01-05102023

Quant Time: May 17 05:30:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260
QLast Update : Thu May 11 13:57:54 2023
Response via : Initial Calibration




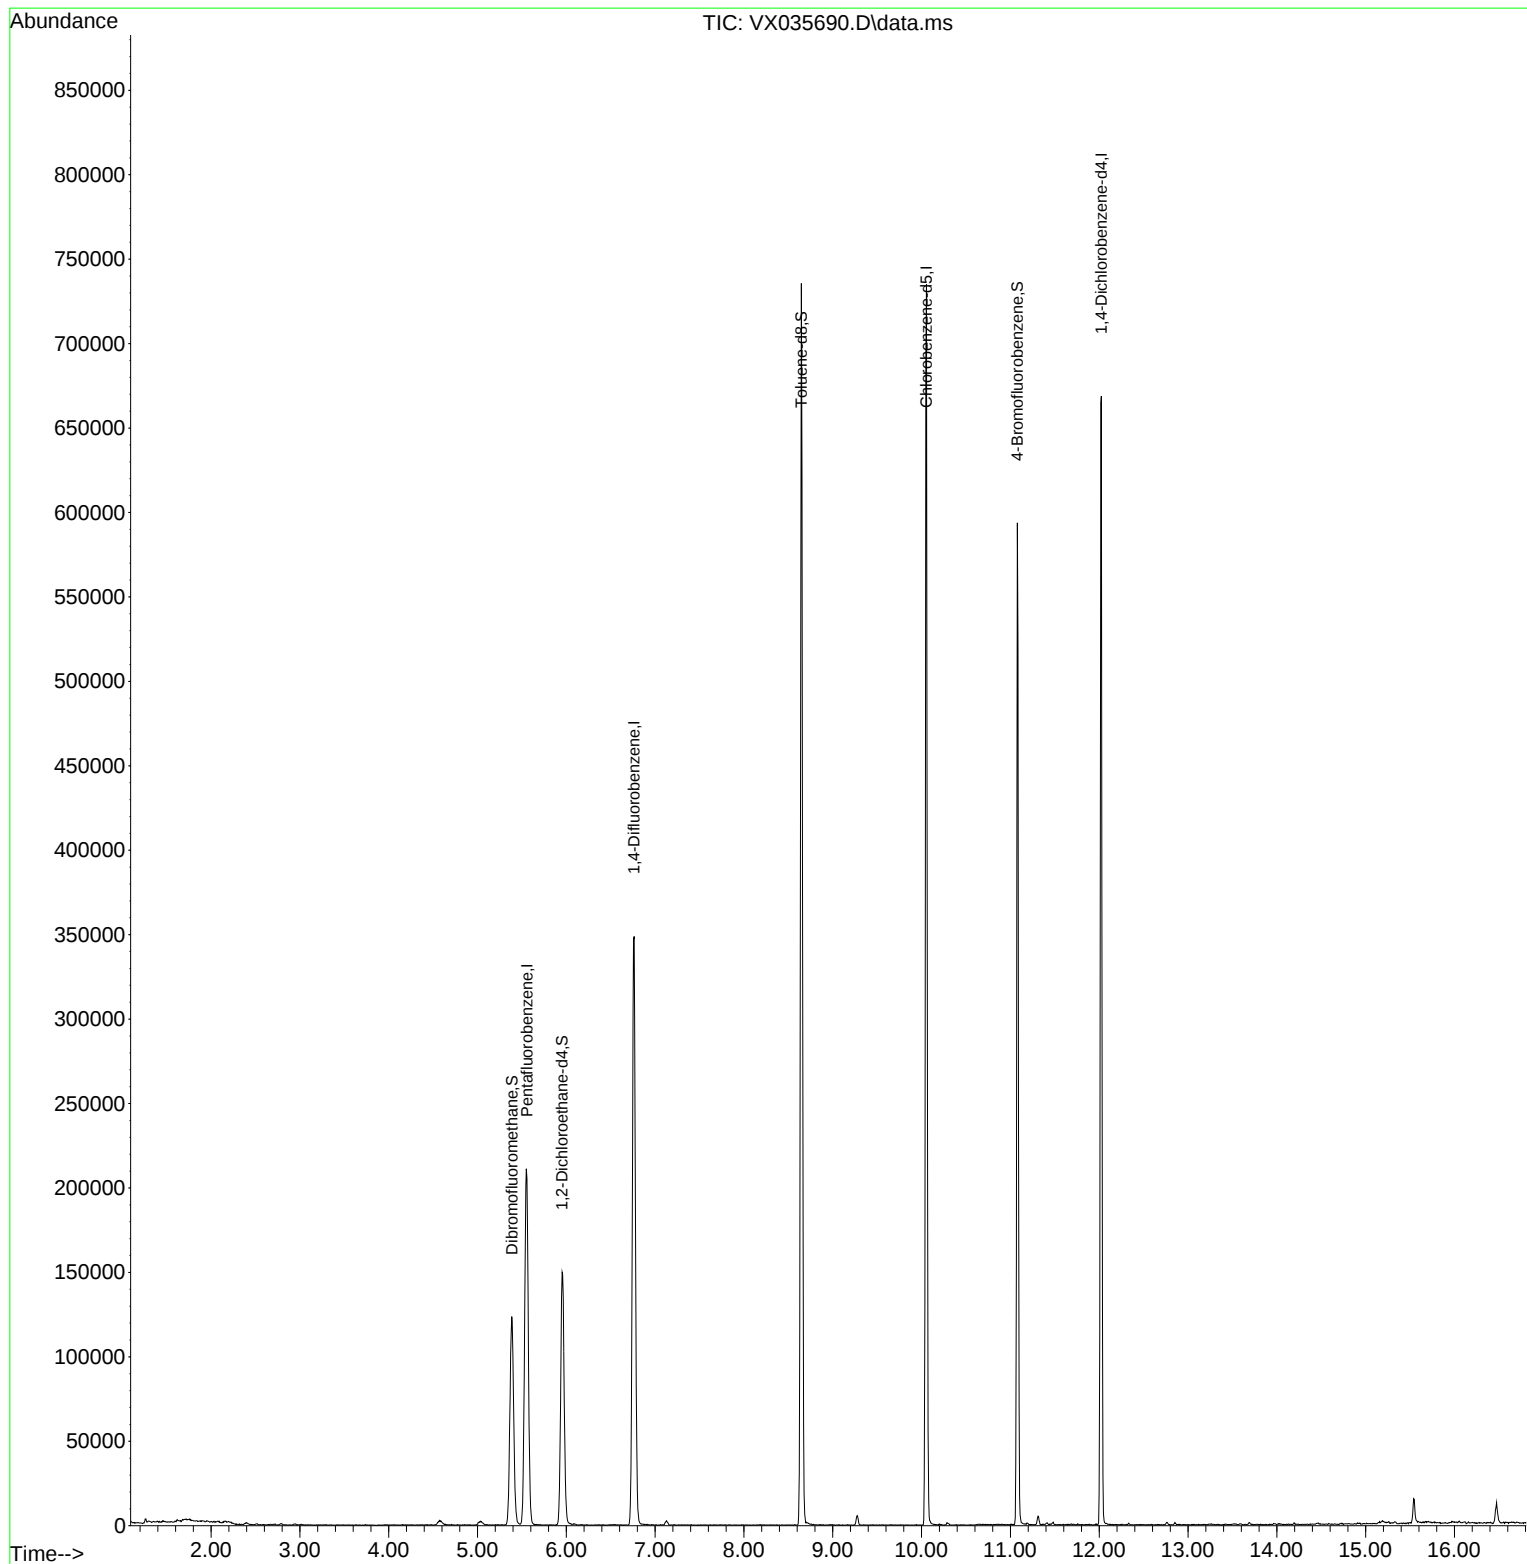


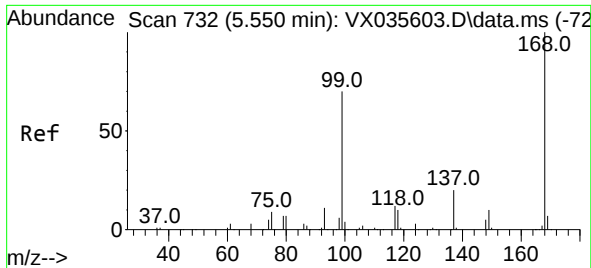

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. 0.006 min
Lab File: VX035690.D
Acq: 16 May 2023 14:53




Instrument :
MSVOA_X
ClientSampleId :
FSND-TB-01-05102023


Tgt Ion:168 Resp: 180677
Ion Ratio Lower Upper
168 100
99 67.1 45.7 68.5

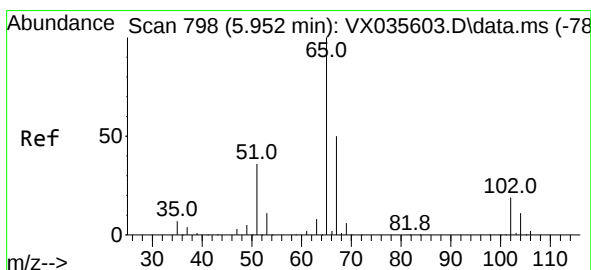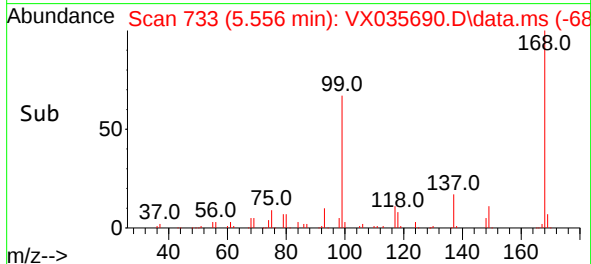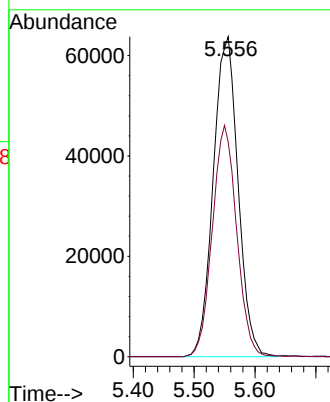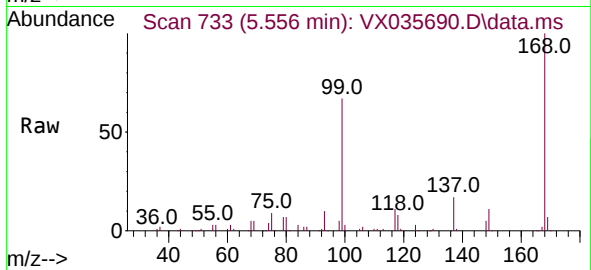

#33
1,2-Dichloroethane-d4
Concen: 48.911 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX035690.D
Acq: 16 May 2023 14:53

Tgt Ion: 65 Resp: 154167
Ion Ratio Lower Upper
65 100
67 49.6 0.0 104.0


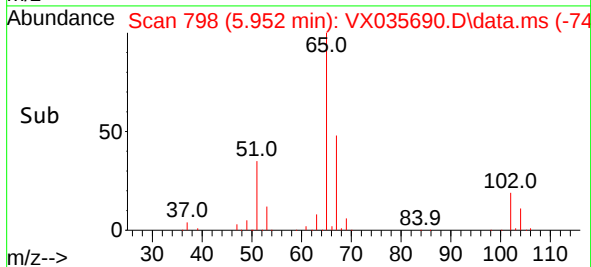
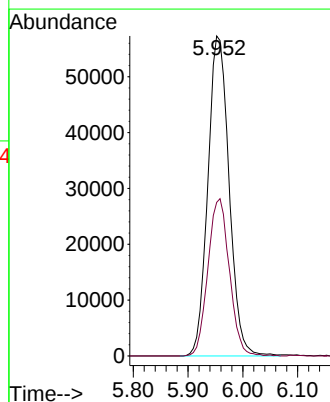
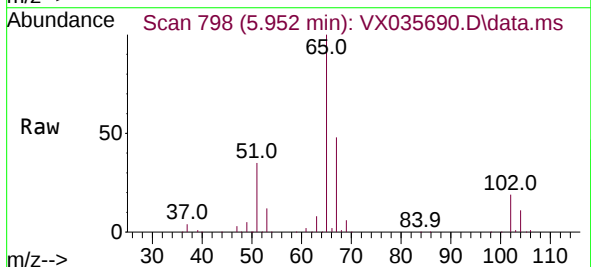


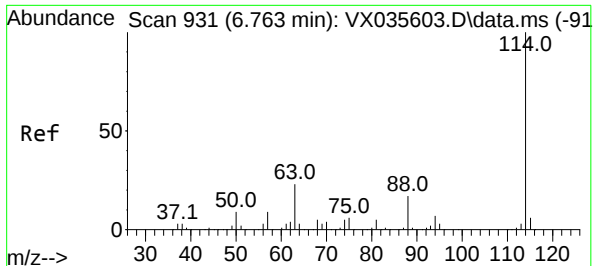

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX035690.D
Acq: 16 May 2023 14:53




Instrument :
MSVOA_X
ClientSampleId :
FSND-TB-01-05102023


Tgt Ion:114 Resp: 335506
Ion Ratio Lower Upper
114 100
63 23.5 0.0 42.2
88 17.4 0.0 33.2

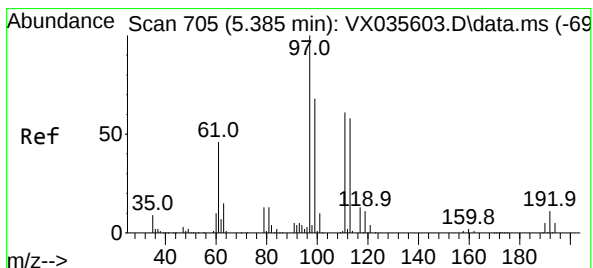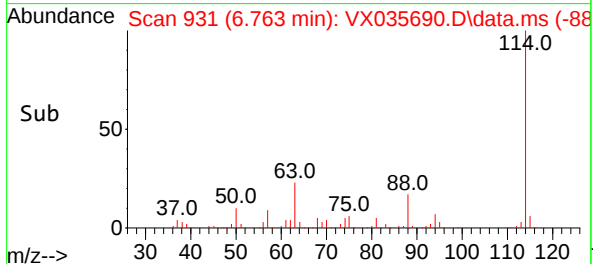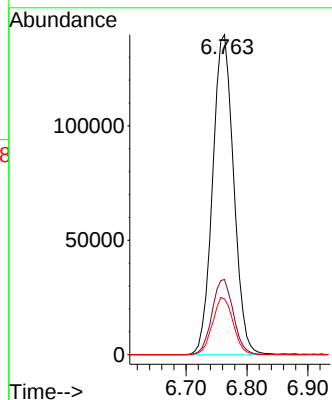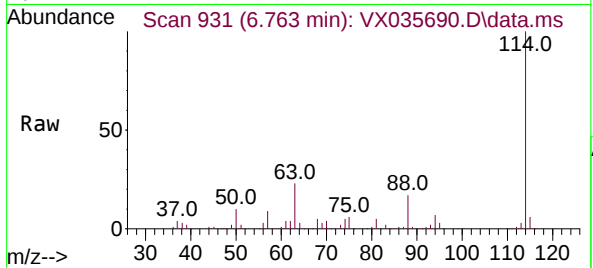

#35
Dibromofluoromethane
Concen: 47.403 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035690.D
Acq: 16 May 2023 14:53

Tgt Ion:113 Resp: 107256
Ion Ratio Lower Upper
113 100
111 104.0 83.7 125.5
192 16.9 15.4 23.2


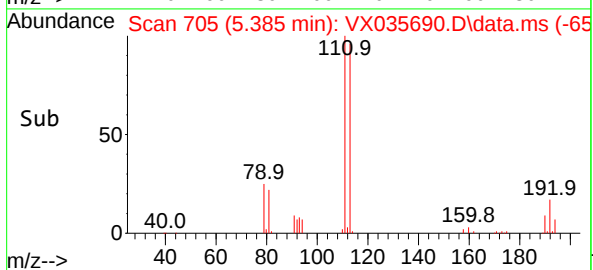
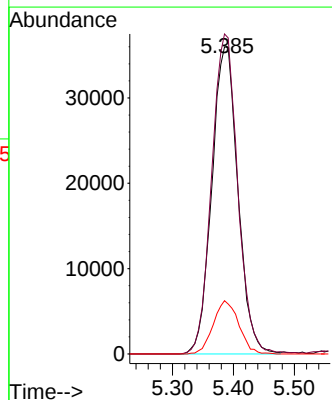
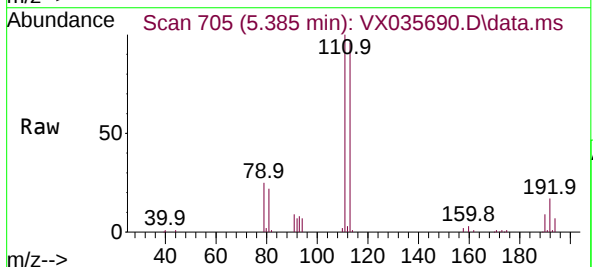


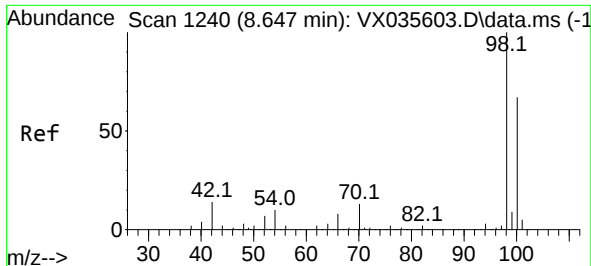

#50
Toluene-d8
Concen: 47.704 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX035690.D
Acq: 16 May 2023 14:53




Instrument :
MSVOA_X
ClientSampleId :
FSND-TB-01-05102023


Tgt Ion: 98 Resp: 398746
Ion Ratio Lower Upper
98 100
100 66.8 52.5 78.7

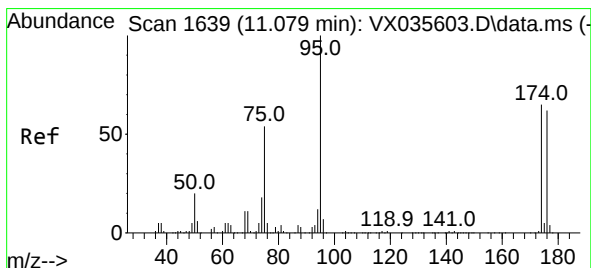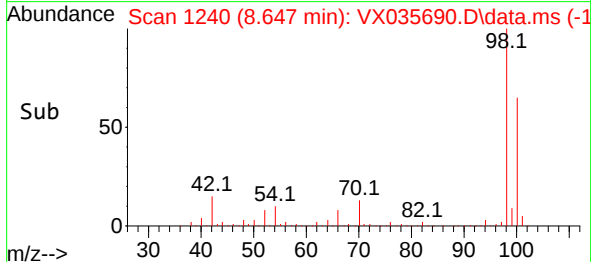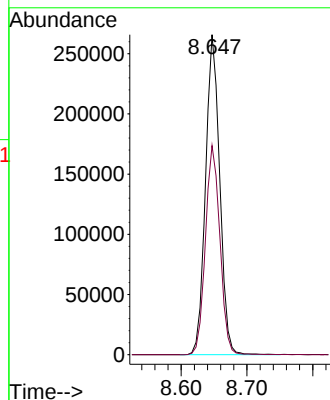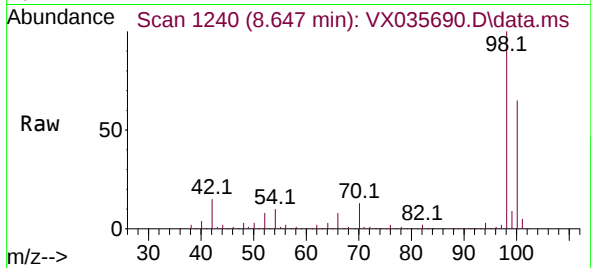

#62
4-Bromofluorobenzene
Concen: 47.371 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035690.D
Acq: 16 May 2023 14:53

Tgt Ion: 95 Resp: 159432
Ion Ratio Lower Upper
95 100
174 65.0 0.0 147.4
176 62.0 0.0 140.6

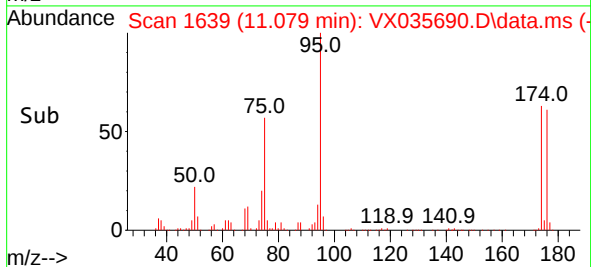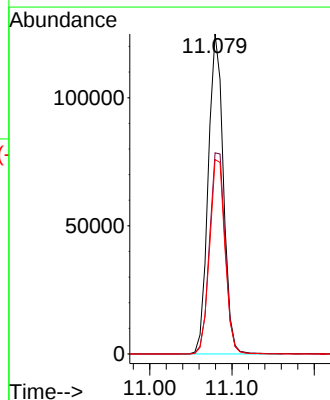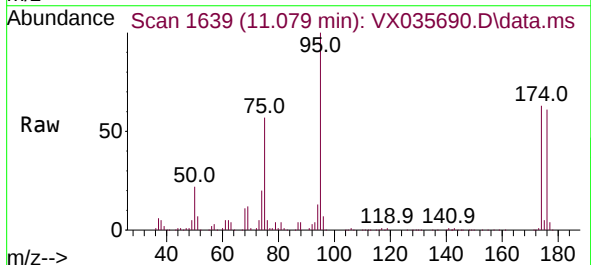

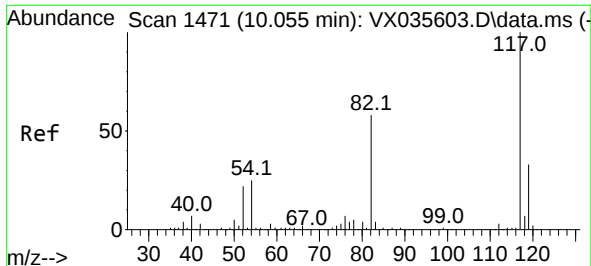

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX035690.D

Acq: 16 May 2023 14:53

Instrument :

MSVOA_X

ClientSampleId :

FSND-TB-01-05102023





Tgt Ion:117 Resp: 301471

Ion Ratio Lower Upper

117 100

82 60.4 45.0 67.4

119 32.4 26.0 39.0

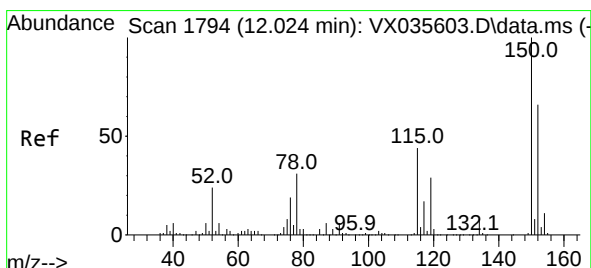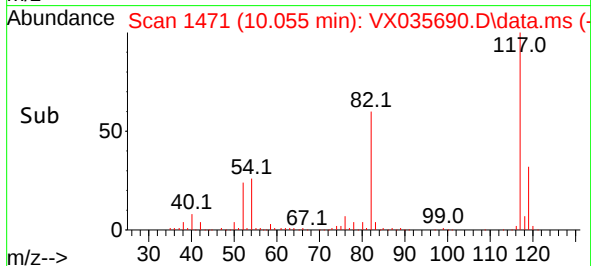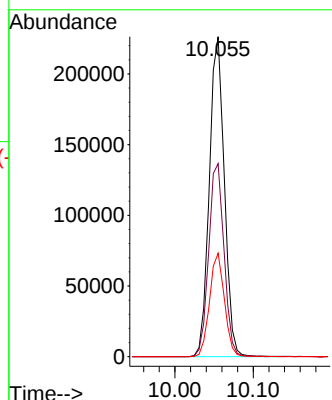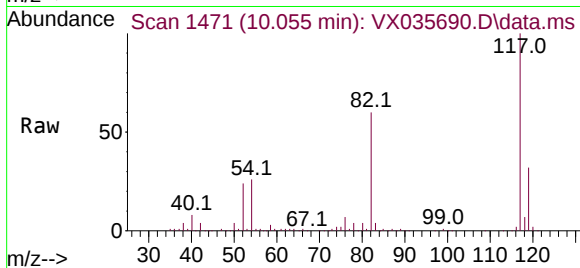

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX035690.D

Acq: 16 May 2023 14:53

Tgt Ion:152 Resp: 129956

Ion Ratio Lower Upper

152 100

115 65.6 45.0 135.0

150 155.5 0.0 352.4

