


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051624\
Data File : VX041549.D
Acq On : 16 May 2024 08:42
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051524W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu May 16 05:13:13 2024

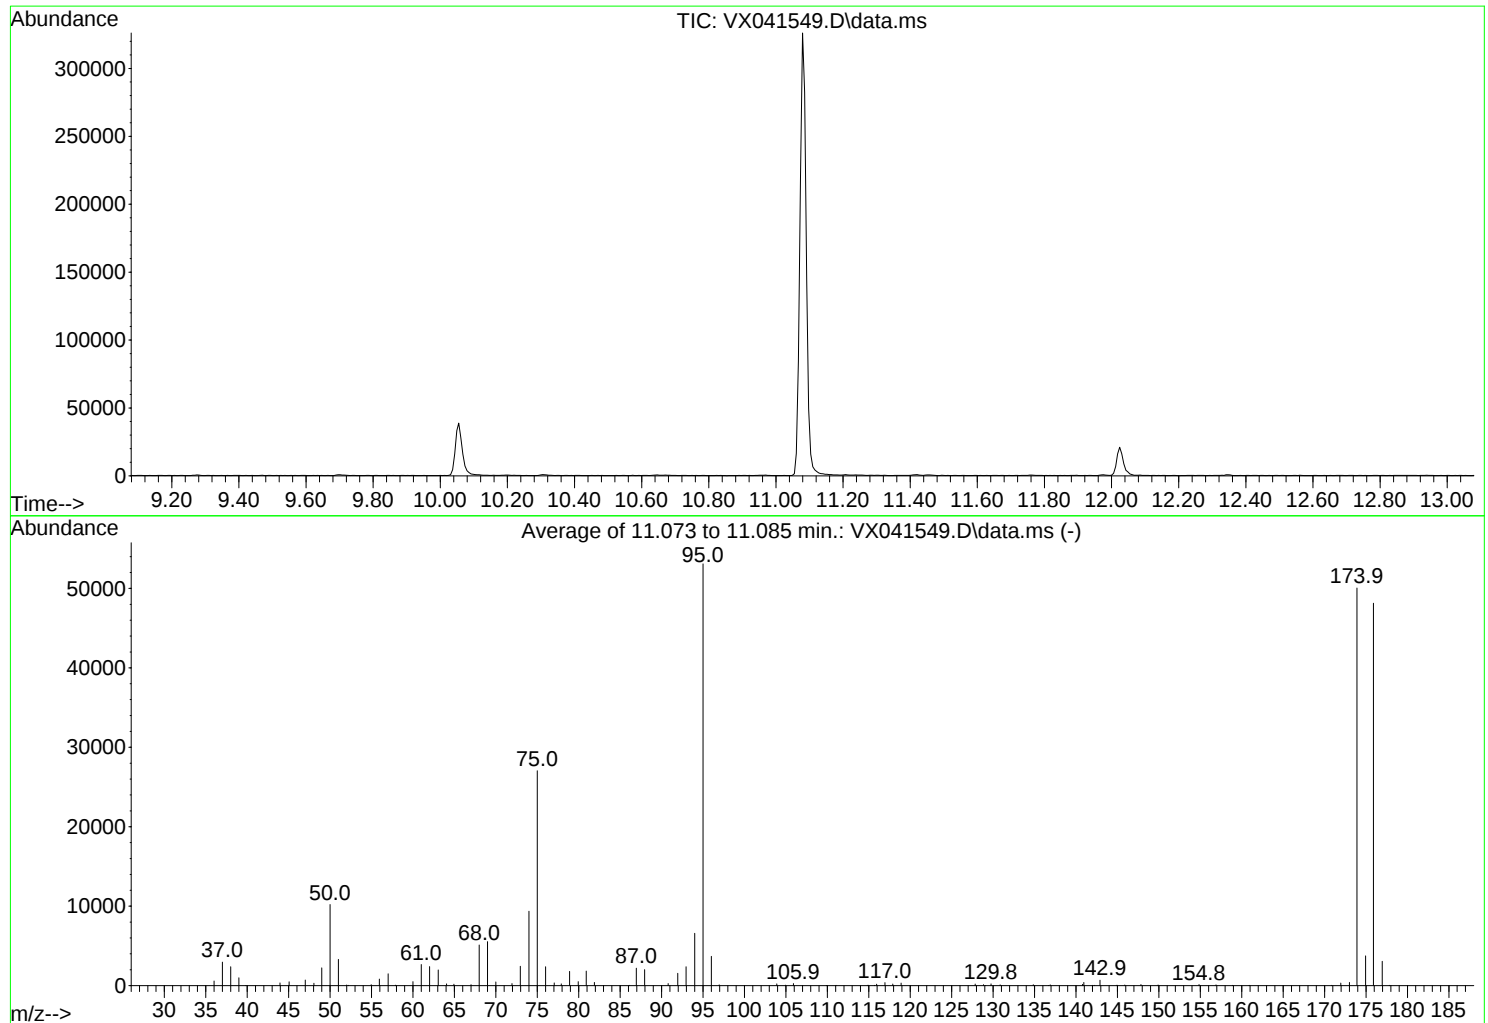

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	10220	PASS
75	95	30	60	50.9	27040	PASS
95	95	100	100	100.0	53091	PASS
96	95	5	9	7.0	3696	PASS
173	174	0.00	2	0.8	402	PASS
174	95	50	100	94.3	50051	PASS
175	174	5	9	7.5	3752	PASS
176	174	95	101	96.2	48139	PASS
177	176	5	9	6.4	3057	PASS