

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX051719\
 Data File : VX009678.D
 Acq On : 17 May 2019 21:40
 Operator : JC/SP
 Sample : K2891-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB202-GW-558-560

Quant Time: May 18 06:31:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 09 07:31:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	160258	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	256434	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	223230	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	93697	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	107897	49.32	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.64%	
35) Dibromofluoromethane	5.50	113	78446	48.66	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.32%	
50) Toluene-d8	8.71	98	319774	49.13	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.26%	
62) 4-Bromofluorobenzene	11.13	95	106195	44.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.82%	
Target Compounds						
16) Acetone	2.45	43	8905	7.581	ug/l	99
52) Toluene	8.79	92	1452	0.324	ug/l	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX051719\
Data File : VX009678.D
Acq On : 17 May 2019 21:40
Operator : JC/SP
Sample : K2891-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB202-GW-558-560

Quant Time: May 18 06:31:07 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Quant Title : SW846 8260
QLast Update : Thu May 09 07:31:15 2019
Response via : Initial Calibration

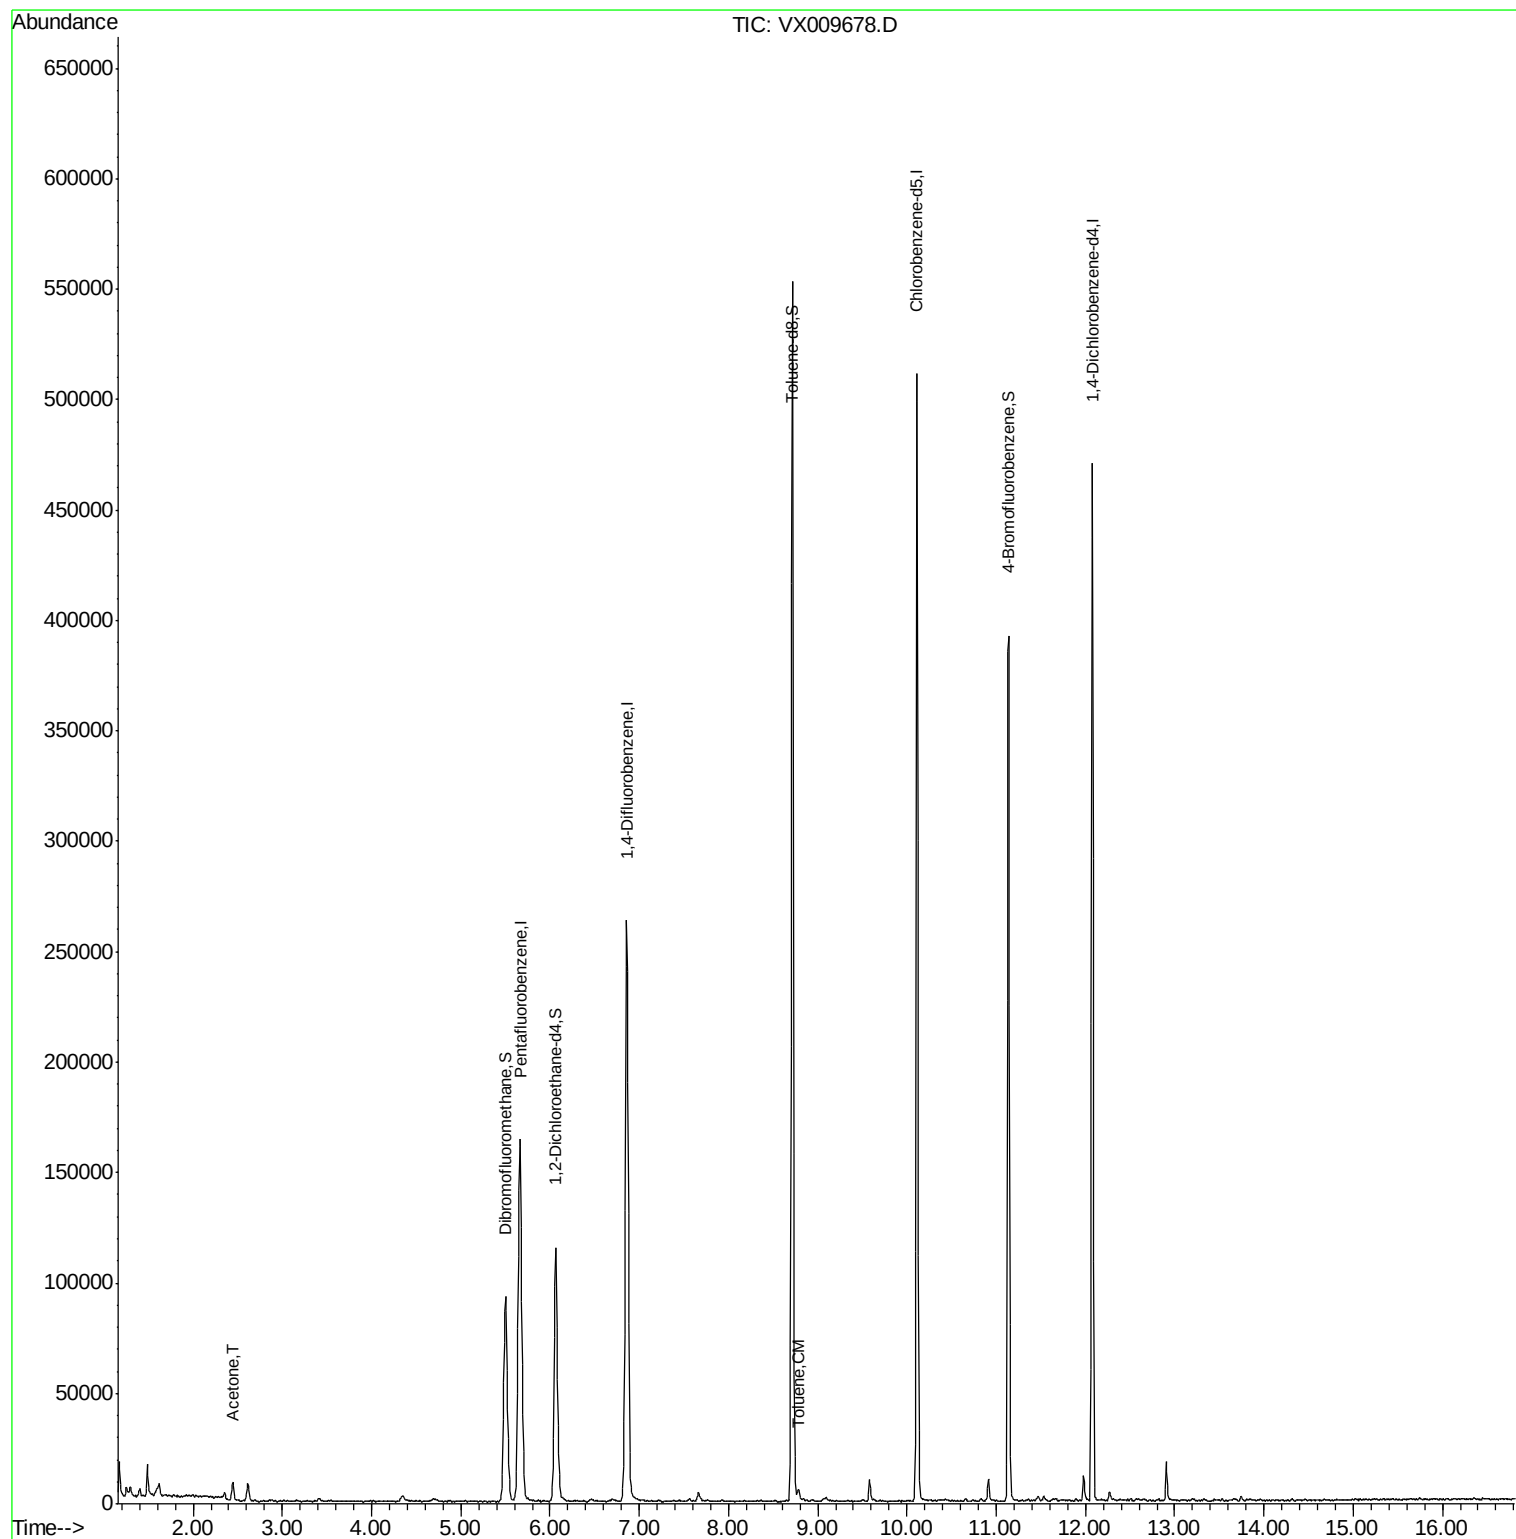

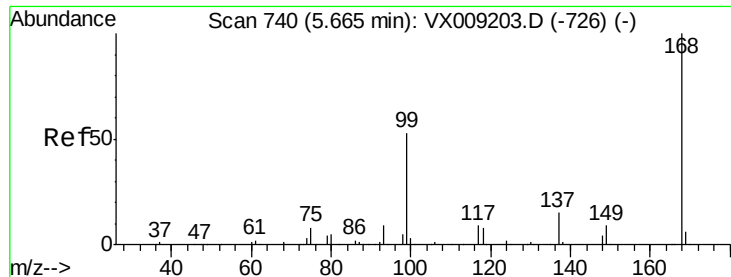

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX009678.D

Acq: 17 May 2019 21:40

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB202-GW-558-560

Tot Ion:168 Resp: 160258

Ion Ratio Lower Upper




168 100

99 54.1 42.3 63.5

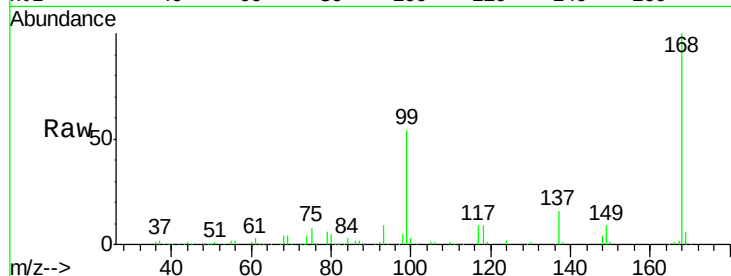

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

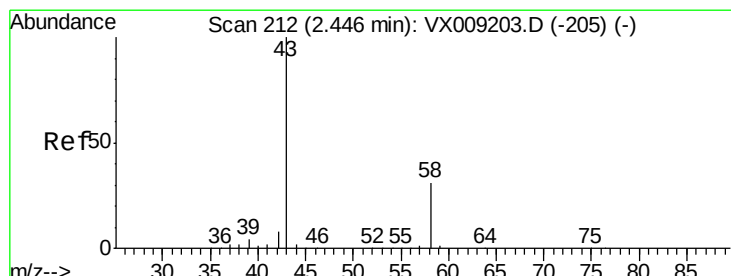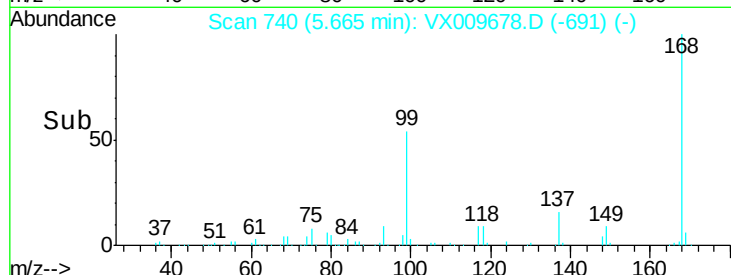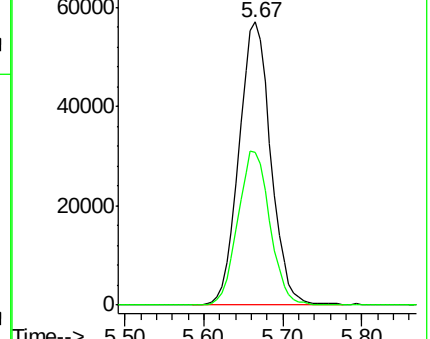

#16

Acetone

Concen: 7.581 ug/l

RT: 2.45 min Scan# 212

Delta R.T. -0.00 min

Lab File: VX009678.D


Acq: 17 May 2019 21:40

Tgt Ion: 43 Resp: 8905

Ion Ratio Lower Upper



43 100


58 30.5 24.9 37.3

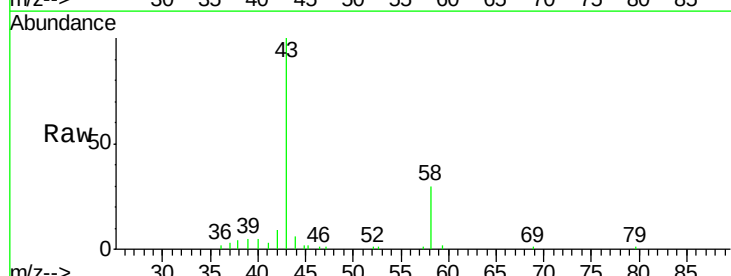

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



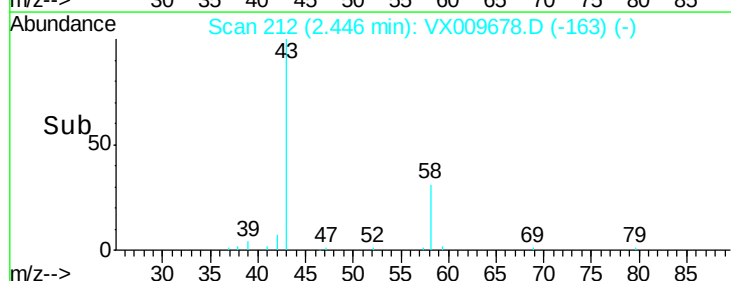
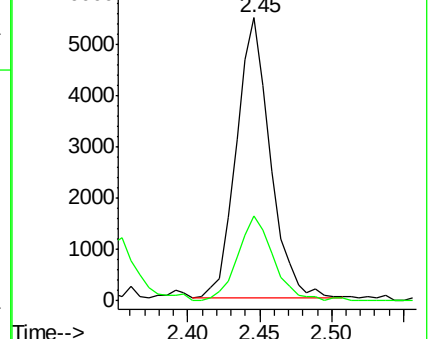


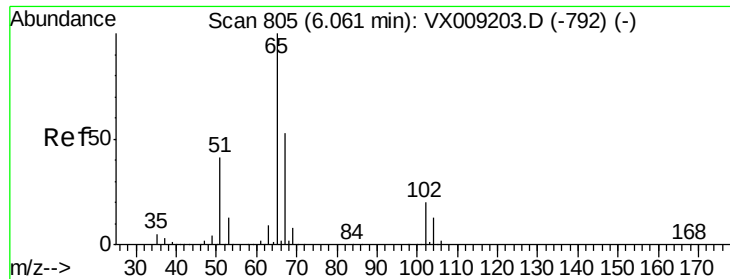

#33
 1,2-Dichloroethane-d4
 Concen: 49.320 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: VX009678.D
 Acq: 17 May 2019 21:40




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB202-GW-558-560


Tot Ion: 65 Resp: 107897
 Ion Ratio Lower Upper
 65 100
 67 53.5 0.0 106.6

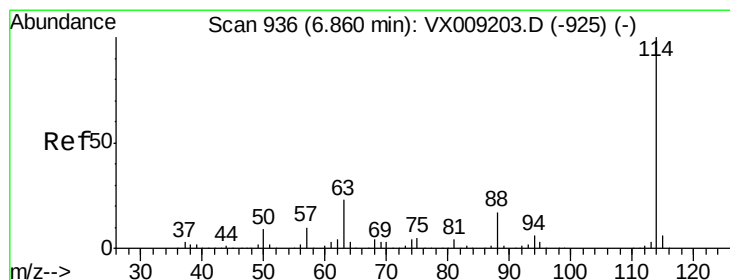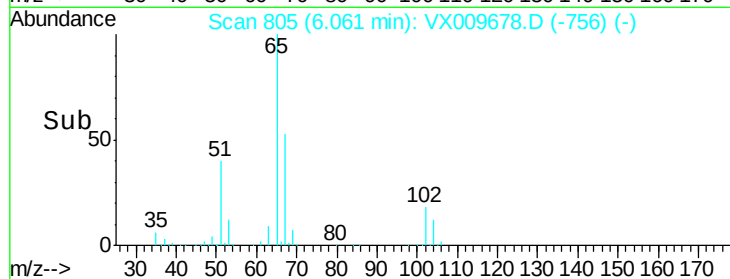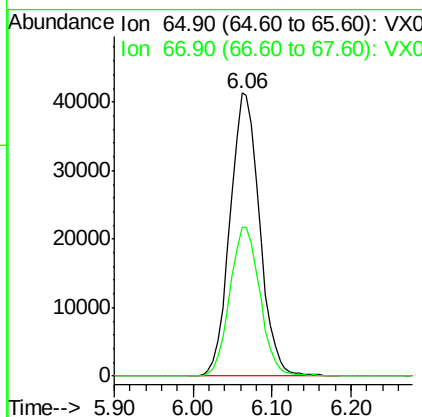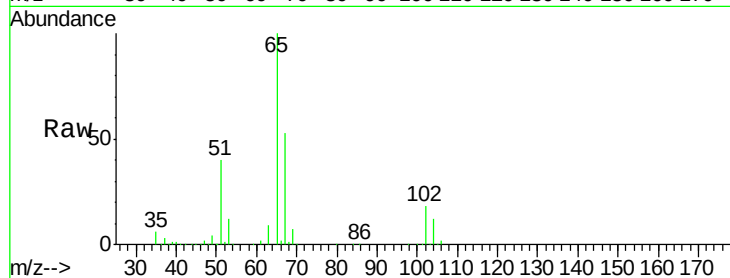

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX009678.D
 Acq: 17 May 2019 21:40

Tgt Ion: 114 Resp: 256434
 Ion Ratio Lower Upper
 114 100
 63 21.7 0.0 45.6
 88 15.1 0.0 33.2


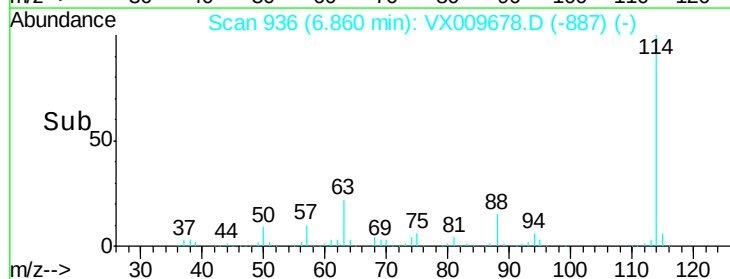
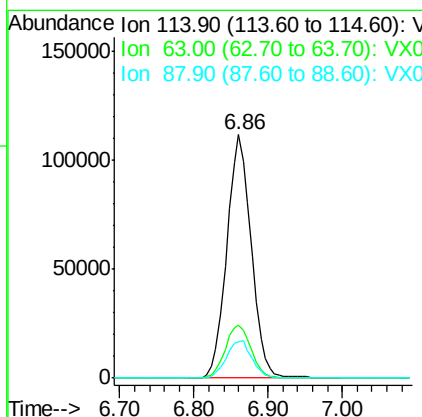
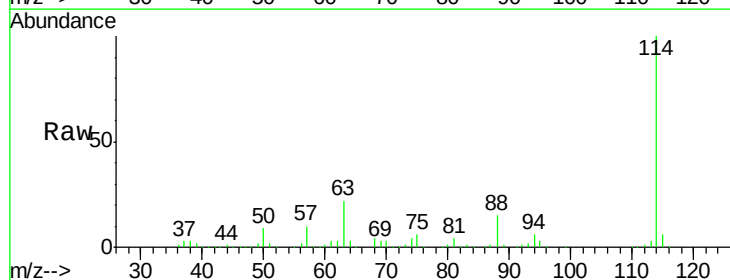


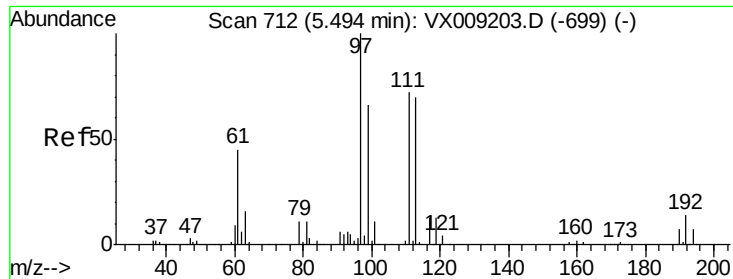

#35
 Dibromofluoromethane
 Concen: 48.662 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX009678.D
 Acq: 17 May 2019 21:40




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB202-GW-558-560


Tot Ion:113 Resp: 78446
 Ion Ratio Lower Upper
 113 100
 111 103.4 82.8 124.2
 192 21.8 17.0 25.6

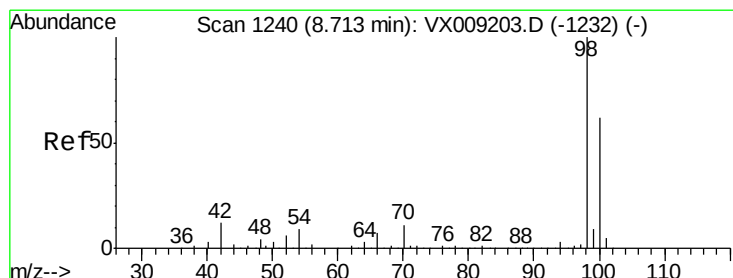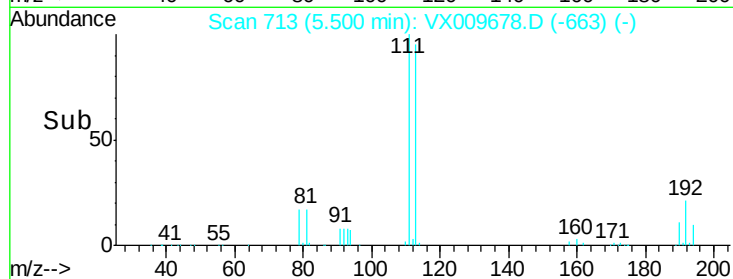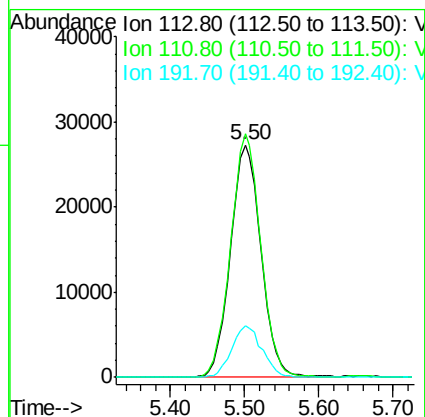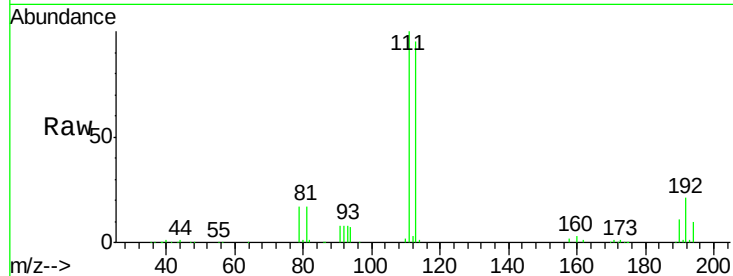

#50
 Toluene-d8
 Concen: 49.134 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. -0.00 min
 Lab File: VX009678.D
 Acq: 17 May 2019 21:40

Tgt Ion: 98 Resp: 319774
 Ion Ratio Lower Upper
 98 100
 100 64.5 51.2 76.8

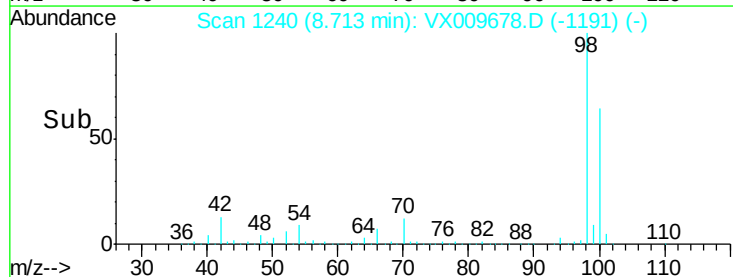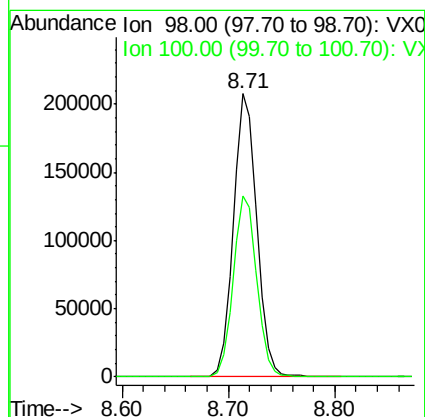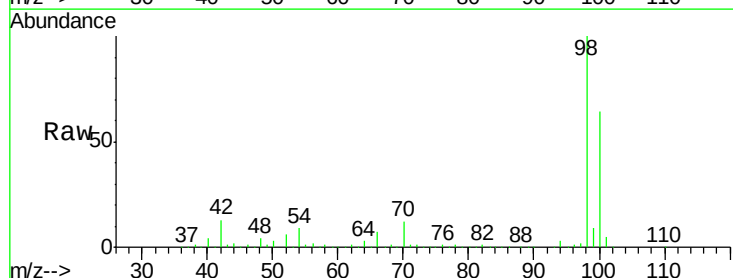

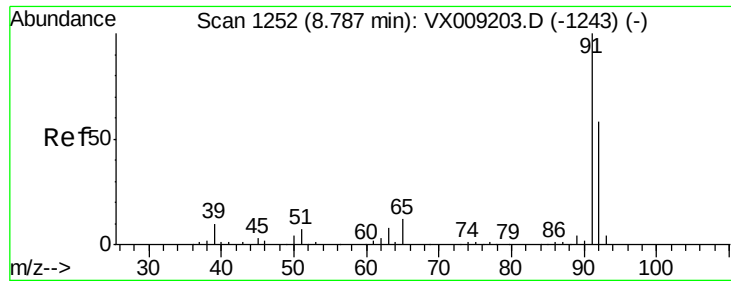

#52

Toluene

Concen: 0.324 ug/l

RT: 8.79 min Scan# 1252

Delta R.T. -0.00 min

Lab File: VX009678.D

Acq: 17 May 2019 21:40

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB202-GW-558-560

Tot Ion: 92 Resp: 1452

Ion Ratio Lower Upper




92 100

91 152.9 138.8 208.2

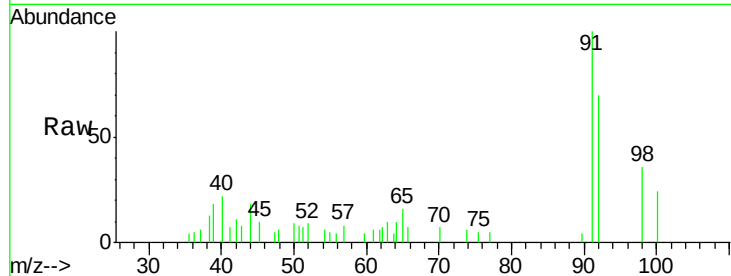

Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

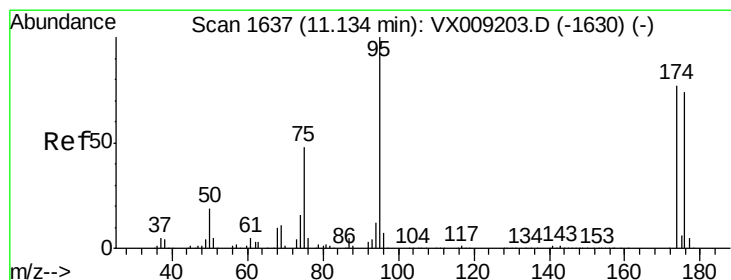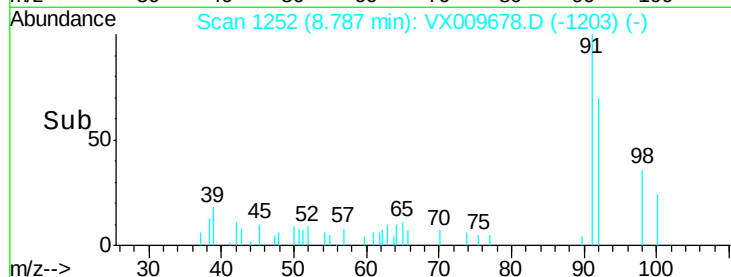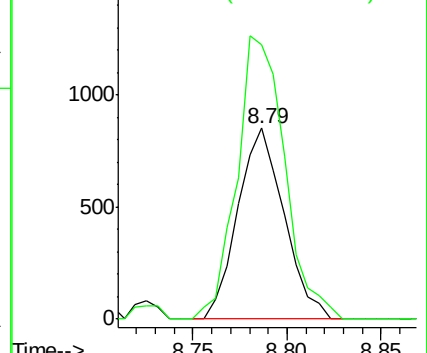

#62

4-Bromofluorobenzene

Concen: 44.906 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX009678.D

Acq: 17 May 2019 21:40


Tgt Ion: 95 Resp: 106195

Ion Ratio Lower Upper

95 100

174 81.2 0.0 161.6



176 78.5 0.0 159.2

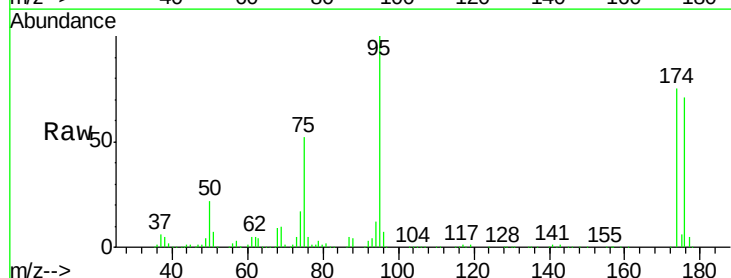


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

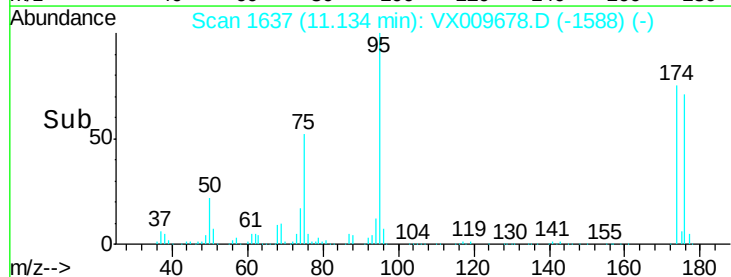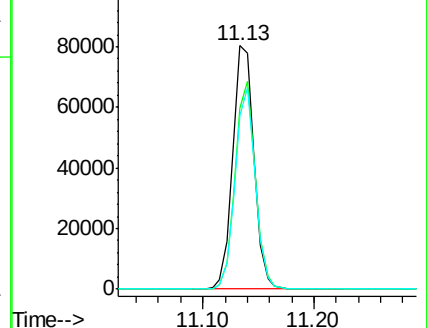


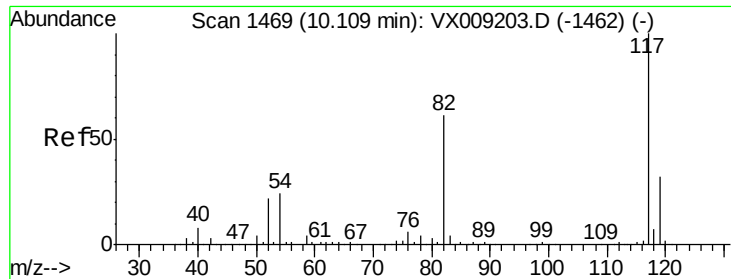




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.01 min
Lab File: VX009678.D
Acq: 17 May 2019 21:40

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB202-GW-558-560

Tot Ion:117 Resp: 223230
Ion Ratio Lower Upper
117 100
82 58.2 48.8 73.2
119 32.4 25.8 38.6

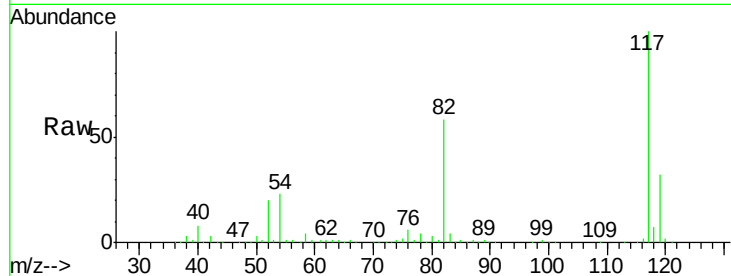


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

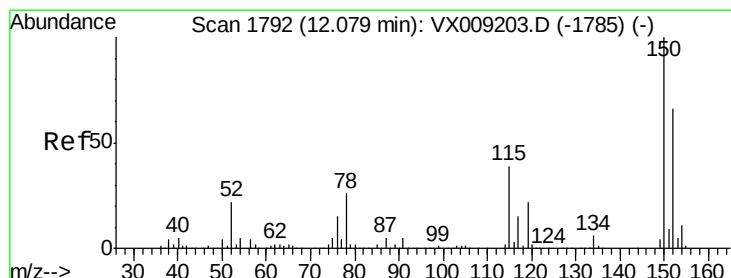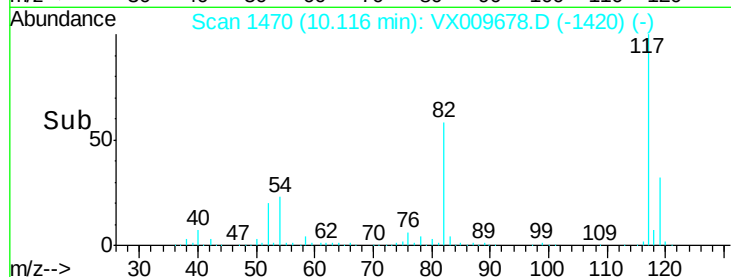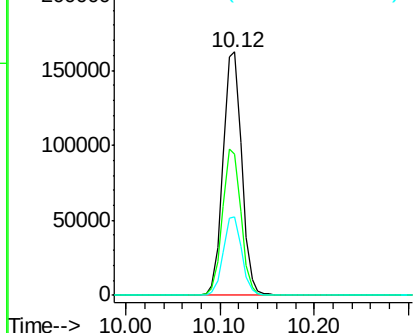

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX009678.D
Acq: 17 May 2019 21:40

Tgt Ion:152 Resp: 93697
Ion Ratio Lower Upper
152 100
115 58.9 41.2 123.6
150 159.7 0.0 346.4

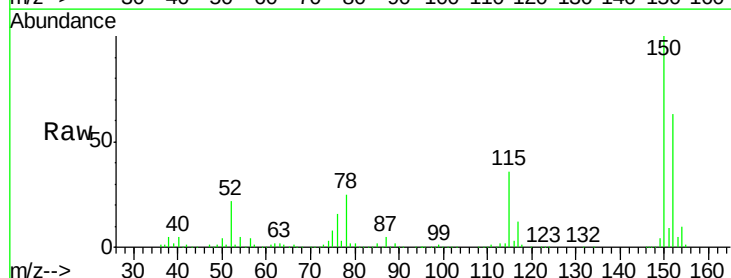

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

