


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX051719\
Data File : VX009650.D
Acq On : 17 May 2019 08:43
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X050119W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu May 02 06:46:57 2019

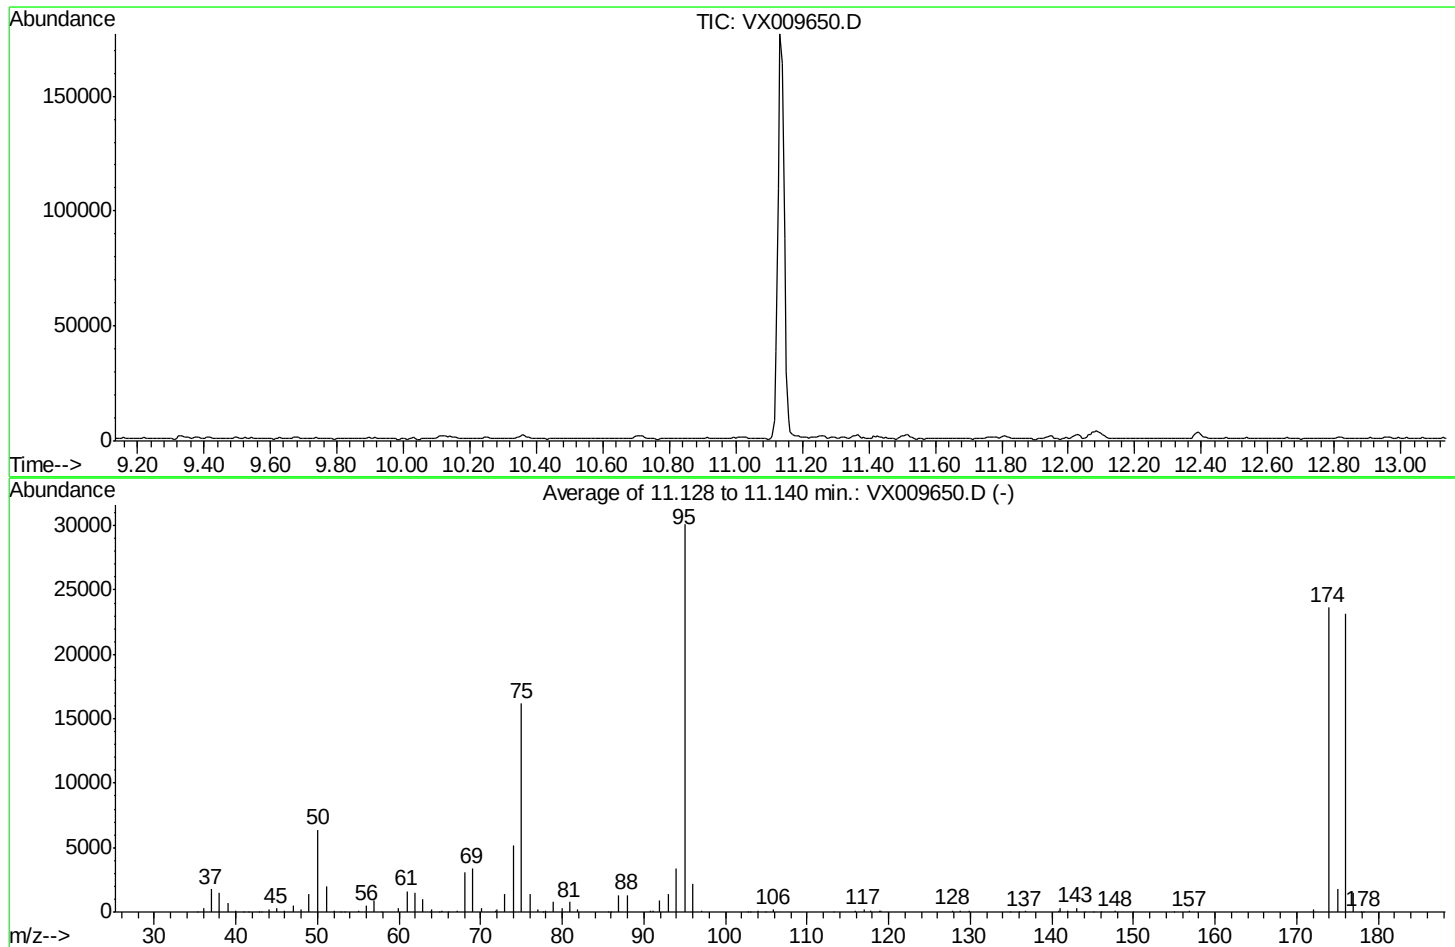

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	6360	PASS
75	95	30	60	53.7	16162	PASS
95	95	100	100	100.0	30096	PASS
96	95	5	9	7.2	2155	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.5	23638	PASS
175	174	5	9	7.7	1823	PASS
176	174	95	101	98.0	23170	PASS
177	176	5	9	6.2	1448	PASS