

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022022.D
 Acq On : 17 May 2021 10:28
 Operator : JC/MD
 Sample : VX0517WBL01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK305

Quant Time: May 18 04:18:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 18 04:17:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	78570	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	70760	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31856	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	28649	4.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.80%
7) Chloroethane-d5	1.672	69	24736	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.40%
11) 1,1-Dichloroethene-d2	2.306	63	41313	3.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.80%
20) 2-Butanone-d5	4.477	46	72113	46.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.80%
24) Chloroform-d	5.068	84	53156	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	5.964	65	27224	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
32) Benzene-d6	5.982	84	114524	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	7.312	67	33995	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	8.653	98	105500	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
43) trans-1,3-Dichloroprop...	8.951	79	13872	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	9.384	63	63716	46.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.32%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	25187	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
66) 1,2-Dichlorobenzene-d4	12.323	152	32177	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%
Target Compounds						Qvalue
16) Methylene chloride	2.794	84	1764	0.23	ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022022.D
Acq On : 17 May 2021 10:28
Operator : JC/MD
Sample : VX0517WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK305

Quant Time: May 18 04:18:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 18 04:17:19 2021
Response via : Initial Calibration

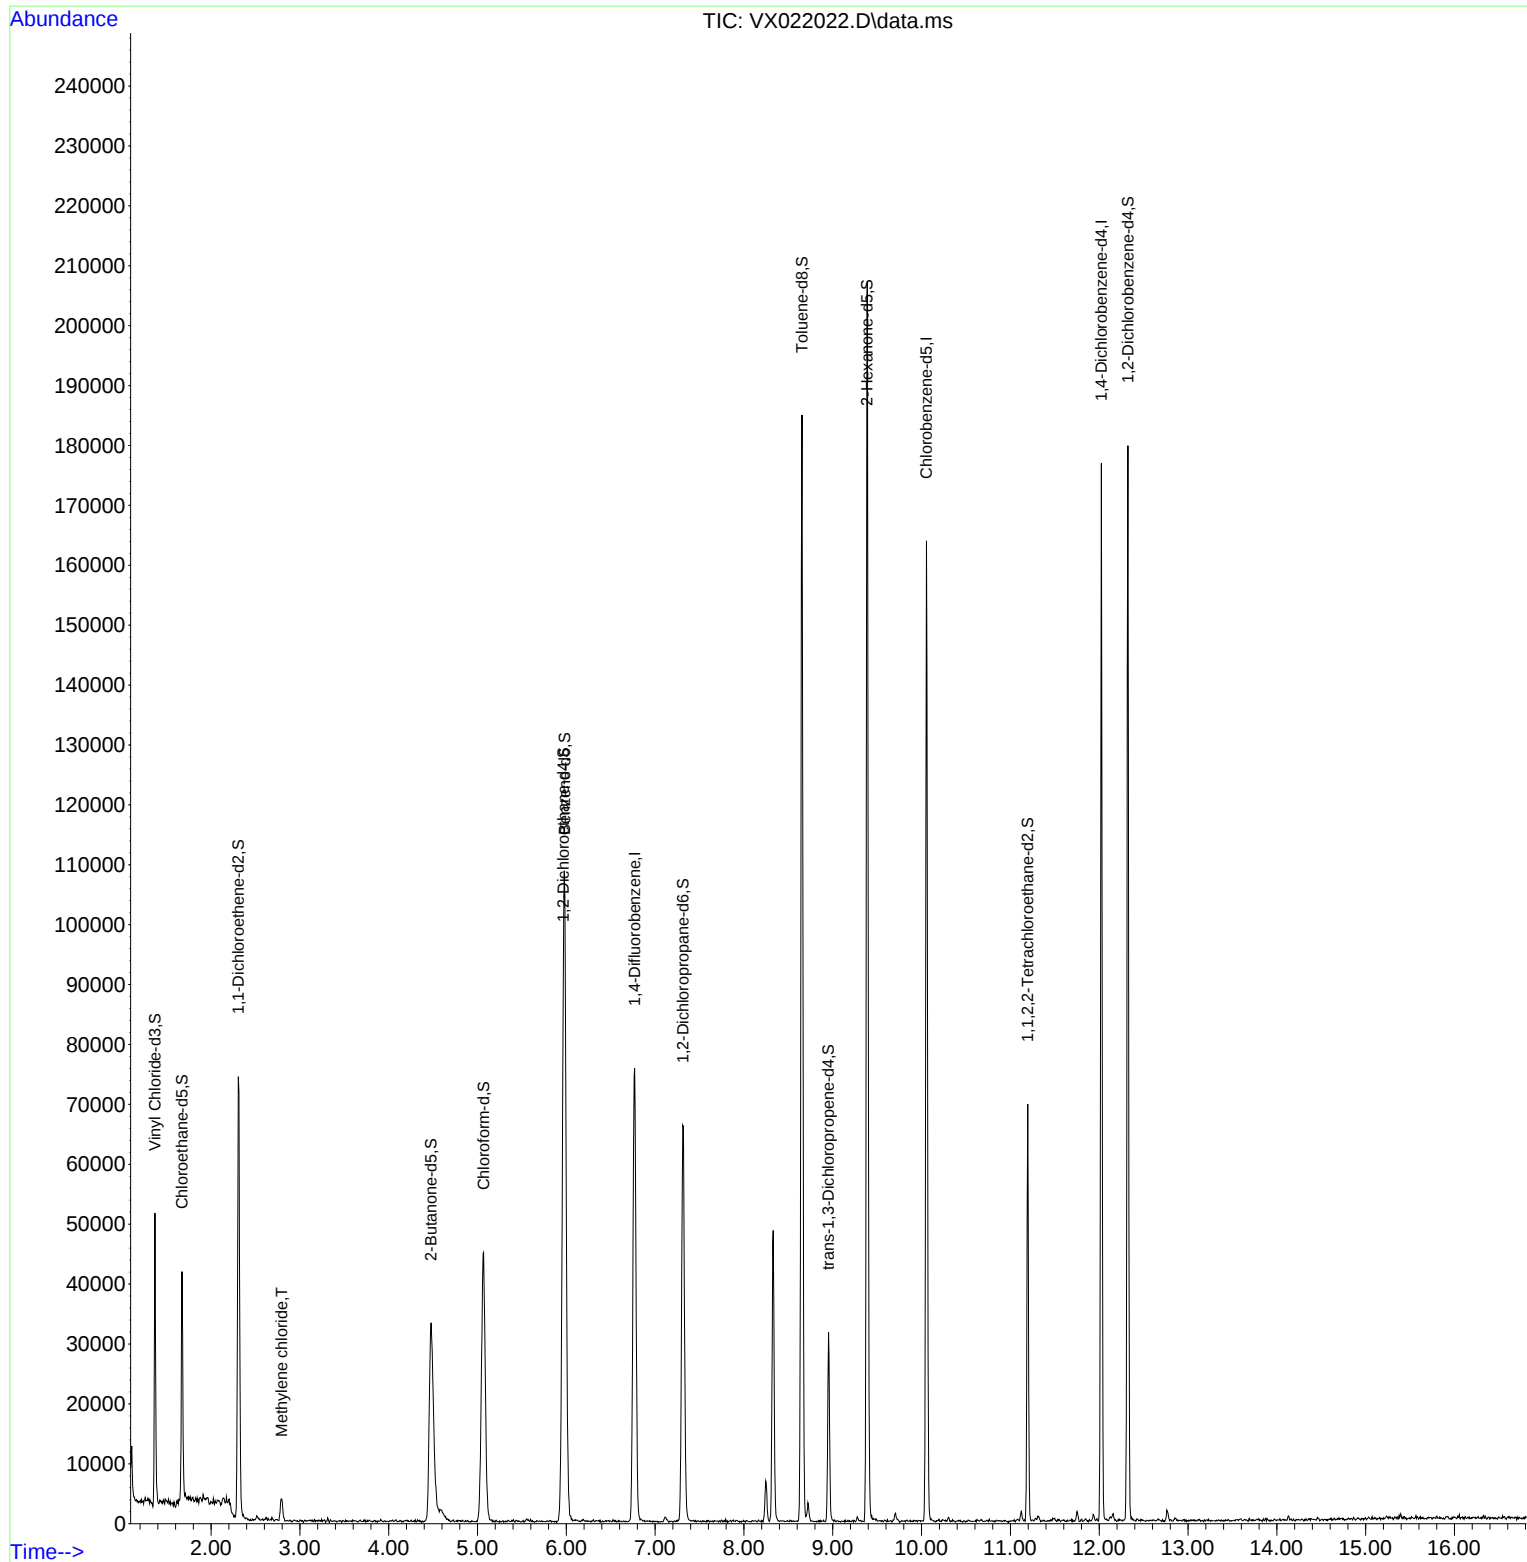

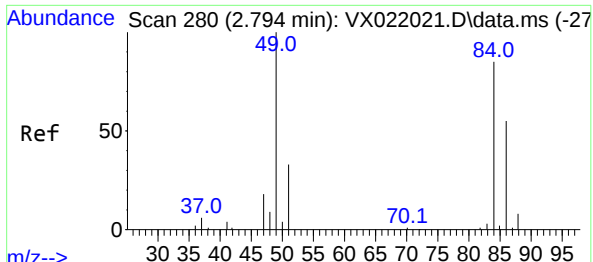

#16
Methylene chloride
Concen: 0.23 ug/L
RT: 2.794 min Scan# 280
Delta R.T. -0.000 min
Lab File: VX022022.D
Acq: 17 May 2021 10:28

Instrument :
MSVOA_X
ClientSampleId :
VBLK305

Tgt Ion: 84 Resp: 1764
Ion Ratio Lower Upper
84 100
86 39.1 46.3 86.1#
49 103.7 84.4 156.7

