

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022034.D
 Acq On : 17 May 2021 15:19
 Operator : JC/MD
 Sample : M2410-13
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: May 18 04:19:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 18 04:17:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	71478	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	63790	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	29247	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	24978	4.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.40%
7) Chloroethane-d5	1.672	69	20962	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.20%
11) 1,1-Dichloroethene-d2	2.306	63	36762	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	4.483	46	65165	46.59	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.18%
24) Chloroform-d	5.068	84	46471	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	5.964	65	26619	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.983	84	107369	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	7.318	67	31785	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	8.653	98	99071	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
43) trans-1,3-Dichloroprop...	8.952	79	13011	4.45	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.00%
46) 2-Hexanone-d5	9.391	63	57122	45.90	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.80%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	22547	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
66) 1,2-Dichlorobenzene-d4	12.323	152	30751	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.794	84	2199	0.31	ug/L	96
25) Chloroform	5.099	83	4332	0.43	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022034.D
Acq On : 17 May 2021 15:19
Operator : JC/MD
Sample : M2410-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: May 18 04:19:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 18 04:17:19 2021
Response via : Initial Calibration

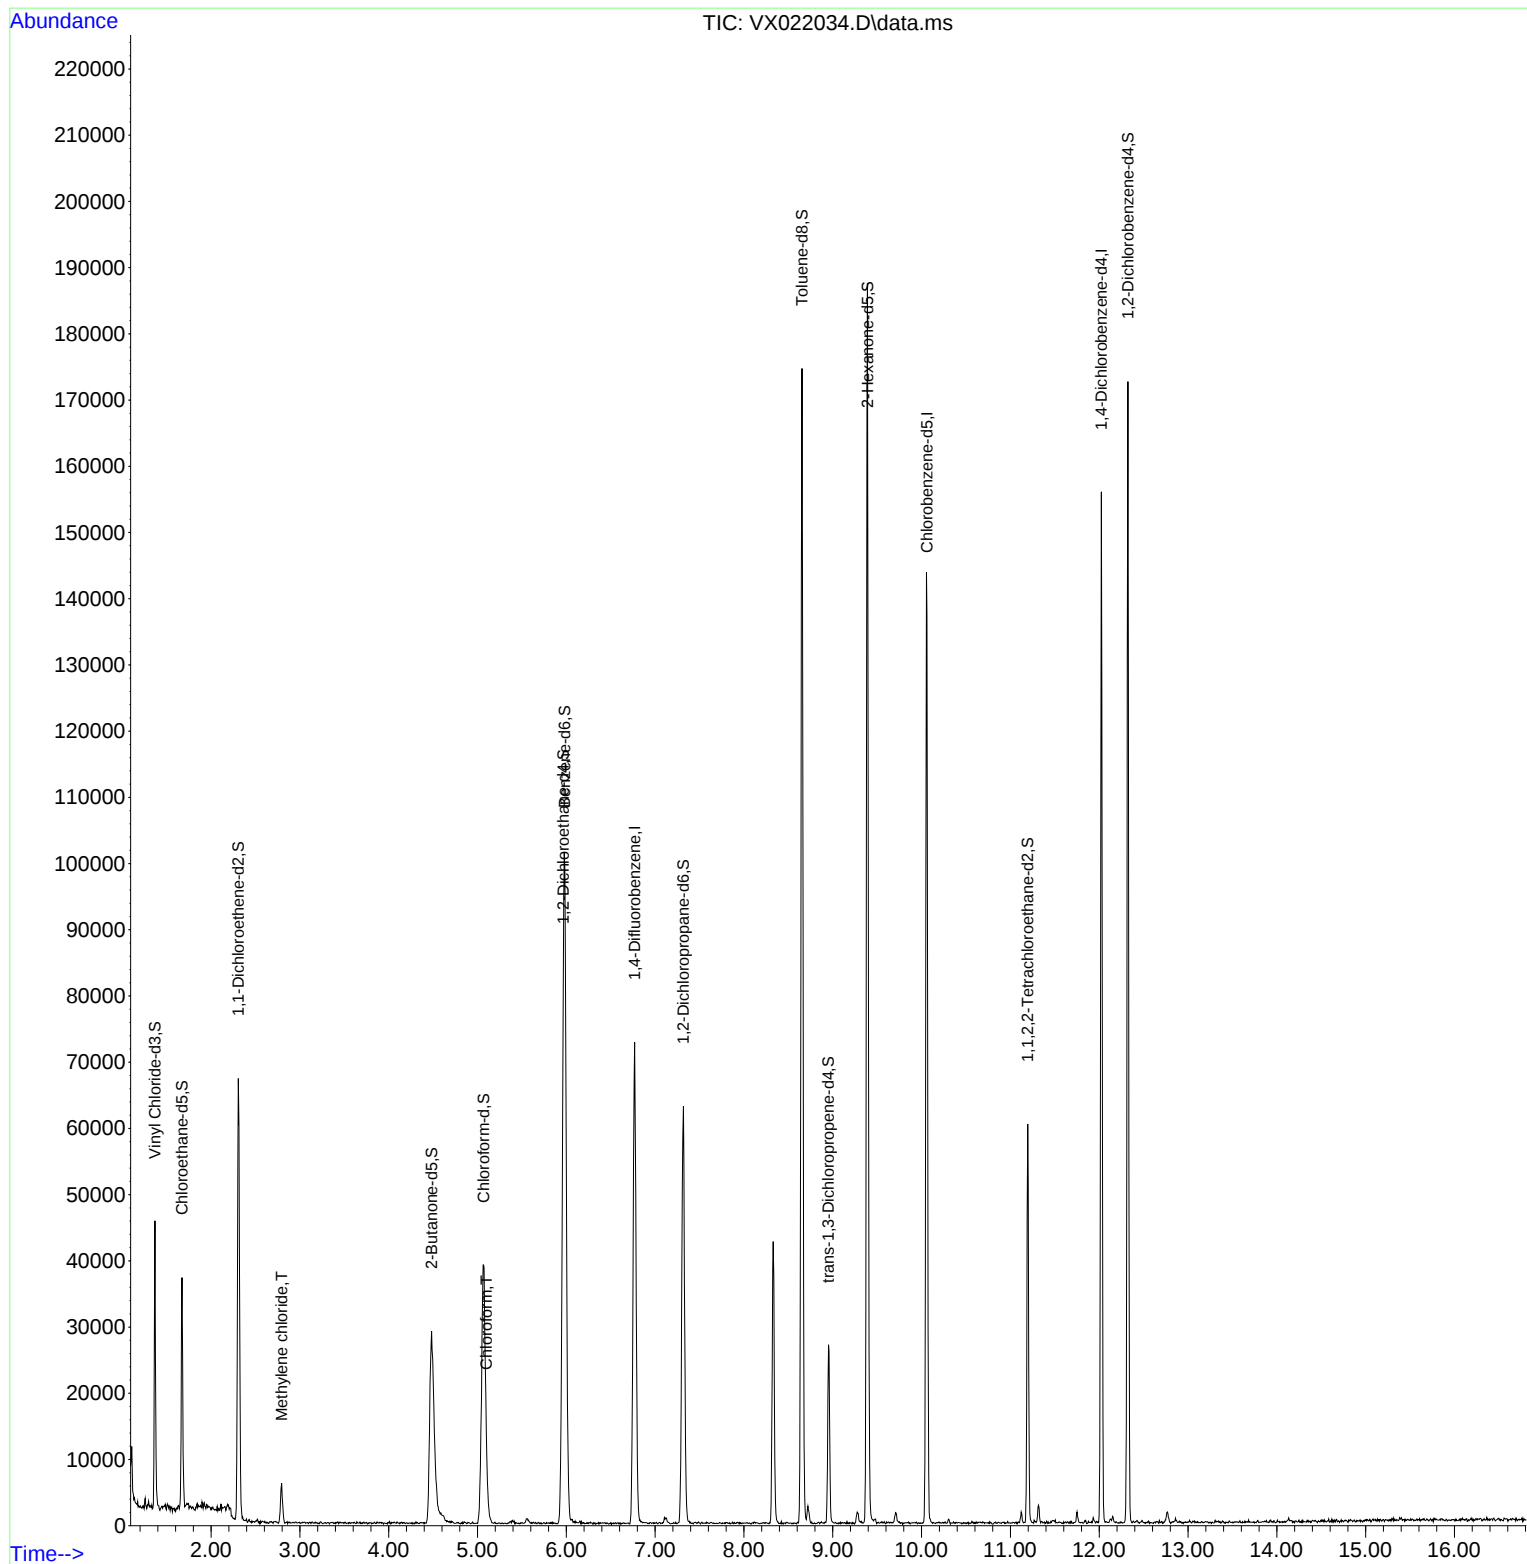




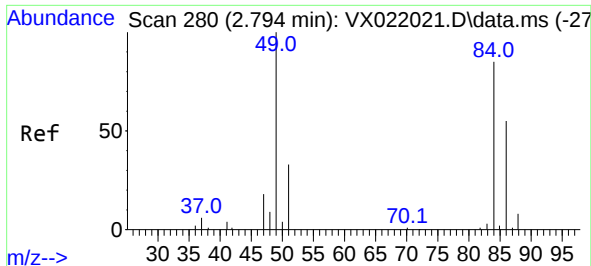


#16
Methylene chloride
Concen: 0.31 ug/L
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022034.D
Acq: 17 May 2021 15:19

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 2199

Ion	Ratio	Lower	Upper
84	100		
86	65.8	46.3	86.1
49	127.0	84.4	156.7

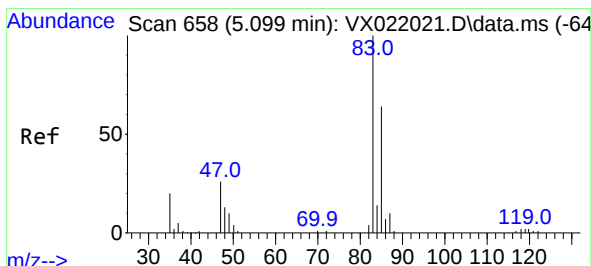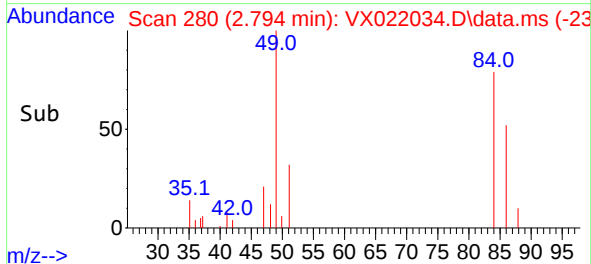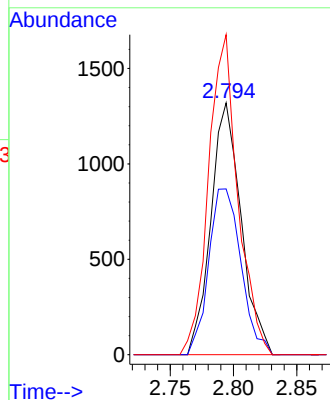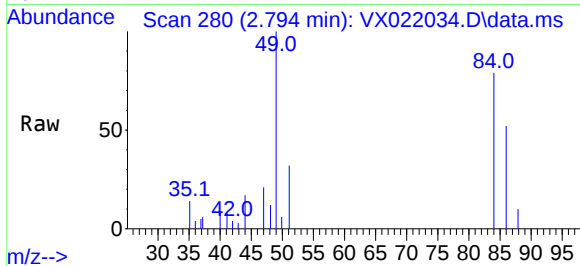

#25
Chloroform
Concen: 0.43 ug/L
RT: 5.099 min Scan# 658
Delta R.T. 0.000 min
Lab File: VX022034.D
Acq: 17 May 2021 15:19

Tgt Ion: 83 Resp: 4332

Ion	Ratio	Lower	Upper
83	100		
85	54.3	46.3	86.1

