

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022023.D
 Acq On : 17 May 2021 11:04
 Operator : JC/MD
 Sample : M2395-01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW6E0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX022023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	51	rBV	45674	44065	14.73%	1.796%
2	1.672	91	96	104	rBV	33731	44618	14.91%	1.818%
3	2.307	194	200	210	rVB	72097	107816	36.03%	4.393%
4	2.794	273	280	287	rBV2	15471	29210	9.76%	1.190%
5	3.440	381	386	395	rVB5	1698	3940	1.32%	0.161%
6	4.477	546	556	575	rBV2	26449	104047	34.77%	4.240%
7	5.068	638	653	665	rBV2	39830	128573	42.97%	5.239%
8	5.977	788	802	814	rBV2	100387	299235	100.00%	12.193%
9	6.763	922	931	943	rBV2	74925	173078	57.84%	7.052%
10	7.312	1012	1021	1033	rBV2	61470	139058	46.47%	5.666%
11	8.324	1180	1187	1198	rVB	44937	75271	25.15%	3.067%
12	8.653	1234	1241	1248	rBV	169874	269851	90.18%	10.996%
13	8.720	1248	1252	1257	rVB2	3878	6154	2.06%	0.251%
14	8.952	1284	1290	1301	rVB	29208	42891	14.33%	1.748%
15	9.391	1355	1362	1371	rBV	183787	274105	91.60%	11.169%
16	10.055	1465	1471	1481	rBV	155229	206129	68.89%	8.399%
17	10.244	1497	1502	1507	rBV	11161	14093	4.71%	0.574%
18	11.195	1653	1658	1667	rBV	60966	75133	25.11%	3.061%
19	11.317	1673	1678	1682	rVB2	2004	3097	1.03%	0.126%
20	12.024	1789	1794	1807	rVB	164773	200706	67.07%	8.178%
21	12.323	1835	1843	1850	rVB	168477	209902	70.15%	8.553%
22	12.859	1926	1931	1934	rBV2	2839	3207	1.07%	0.131%


Sum of corrected areas: 2454179

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022023.D
Acq On : 17 May 2021 11:04
Operator : JC/MD
Sample : M2395-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

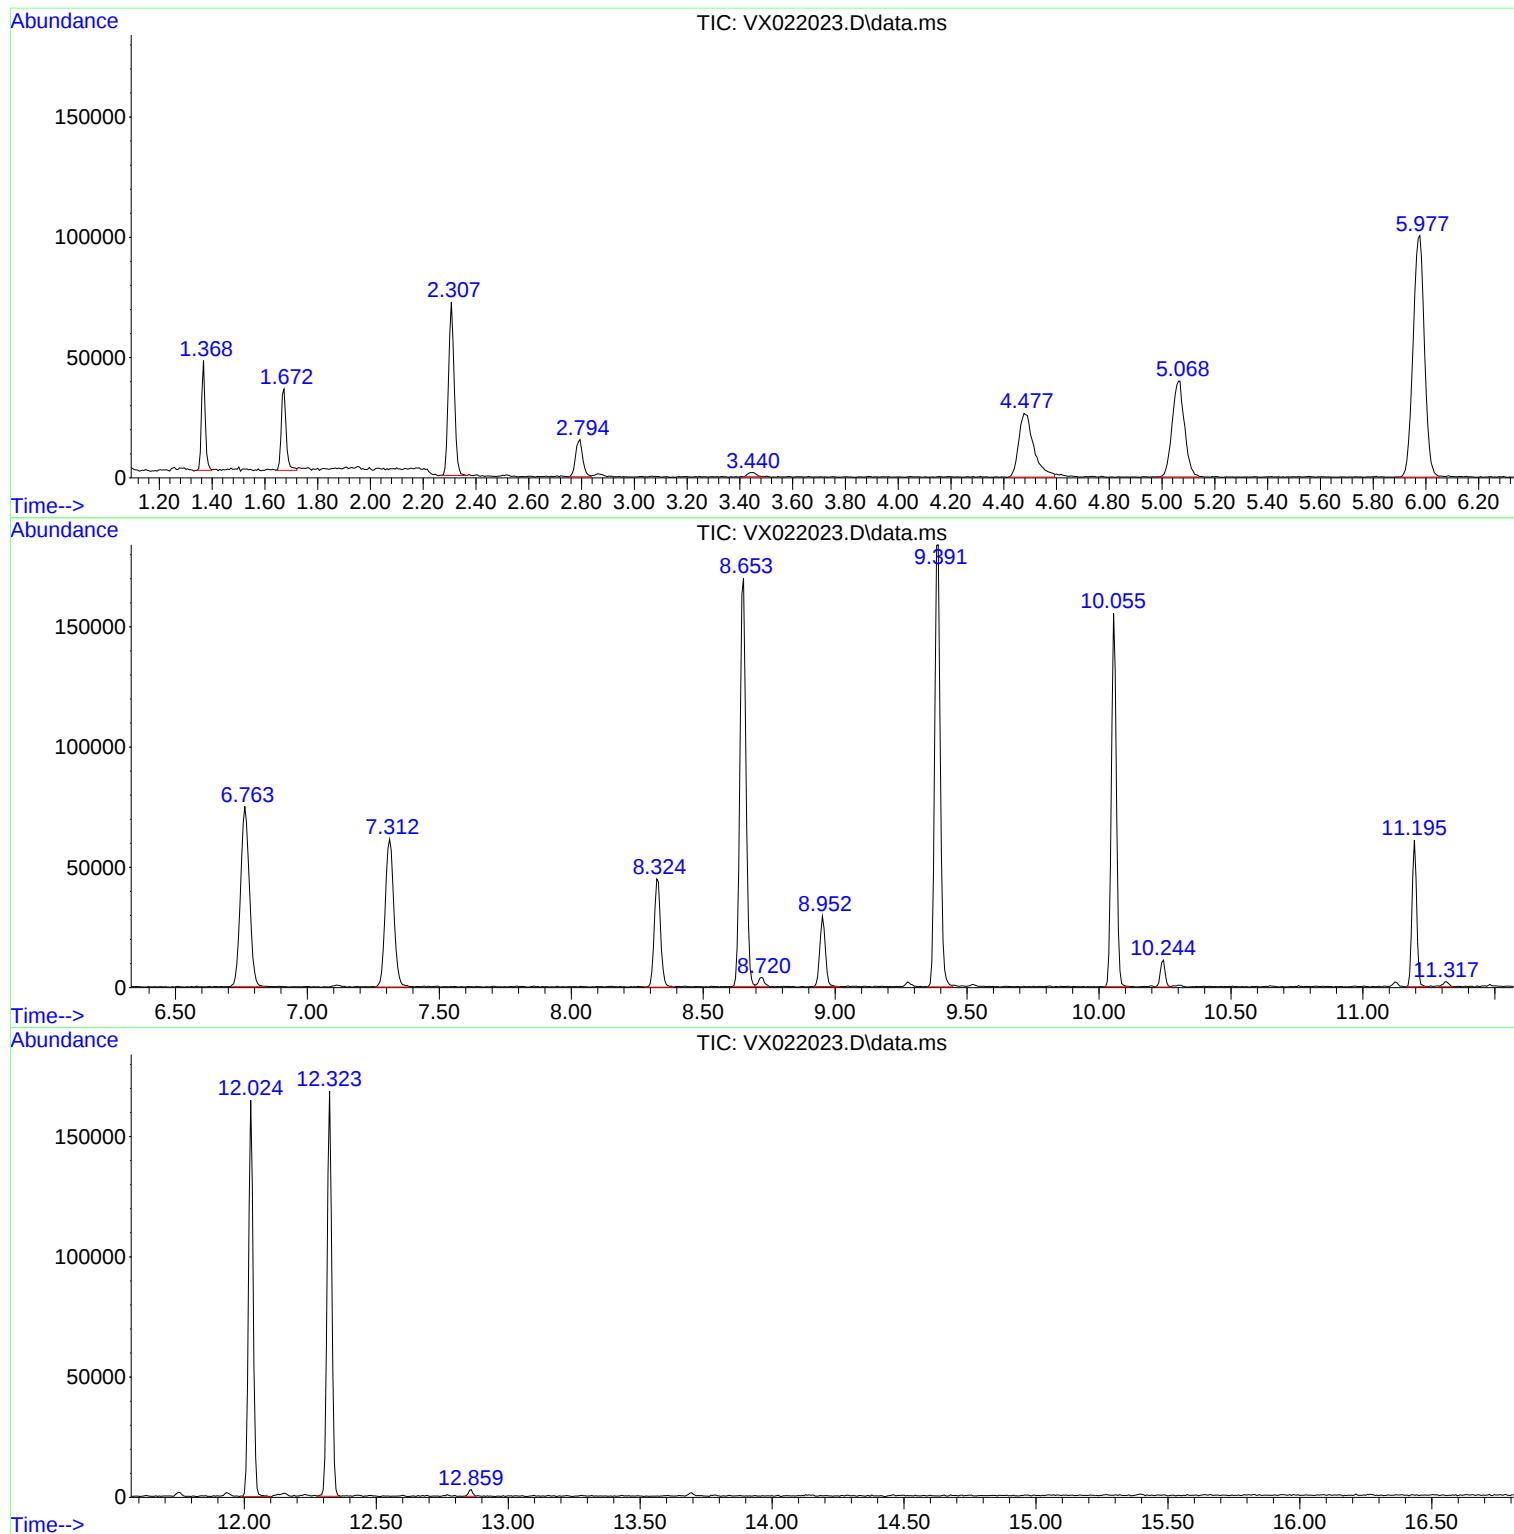

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022023.D
Acq On : 17 May 2021 11:04
Operator : JC/MD
Sample : M2395-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022023.D
Acq On : 17 May 2021 11:04
Operator : JC/MD
Sample : M2395-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW6E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
