

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022024.D
 Acq On : 17 May 2021 11:27
 Operator : JC/MD
 Sample : M2410-12
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6N7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX022024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	47031	47067	15.13%	1.783%
2	1.673	92	96	103	rBV	37554	43593	14.01%	1.651%
3	2.307	195	200	210	rVV	70558	110724	35.59%	4.195%
4	2.404	210	216	229	rVB	3730	11930	3.83%	0.452%
5	4.483	547	557	567	rBV	31367	107545	34.57%	4.074%
6	4.593	567	575	588	rVB2	14900	58883	18.93%	2.231%
7	5.062	638	652	670	rBV	43450	146392	47.05%	5.546%
8	5.977	786	802	815	rBV2	107614	311125	100.00%	11.786%
9	6.769	922	932	942	rBV	74995	178353	57.33%	6.757%
10	7.129	984	991	999	rBV4	8724	19297	6.20%	0.731%
11	7.312	1012	1021	1031	rBV	66706	145538	46.78%	5.513%
12	8.330	1181	1188	1197	rBV	44363	75391	24.23%	2.856%
13	8.653	1234	1241	1248	rBV	176400	276678	88.93%	10.482%
14	8.720	1248	1252	1263	rVB	5267	8558	2.75%	0.324%
15	8.952	1284	1290	1297	rVB	30240	43907	14.11%	1.663%
16	9.281	1339	1344	1353	rBV4	1856	3369	1.08%	0.128%
17	9.391	1356	1362	1372	rBV	199275	286952	92.23%	10.871%
18	10.055	1463	1471	1479	rBV	157327	211802	68.08%	8.024%
19	10.305	1506	1512	1518	rBV	2538	3406	1.09%	0.129%
20	11.195	1652	1658	1664	rVV	64341	78997	25.39%	2.993%
21	11.317	1674	1678	1684	rVB2	3628	4948	1.59%	0.187%
22	11.756	1743	1750	1754	rBV2	2960	3689	1.19%	0.140%
23	12.024	1789	1794	1800	rBV	172625	209971	67.49%	7.954%
24	12.232	1822	1828	1833	rBV	4442	8381	2.69%	0.318%
25	12.323	1837	1843	1849	rVB	174783	217469	69.90%	8.238%
26	13.256	1990	1996	2000	rBV2	2411	3519	1.13%	0.133%
27	14.134	2134	2140	2147	rVB	11475	15285	4.91%	0.579%
28	15.396	2342	2347	2353	rVB	4155	6907	2.22%	0.262%


Sum of corrected areas: 2639676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022024.D
Acq On : 17 May 2021 11:27
Operator : JC/MD
Sample : M2410-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

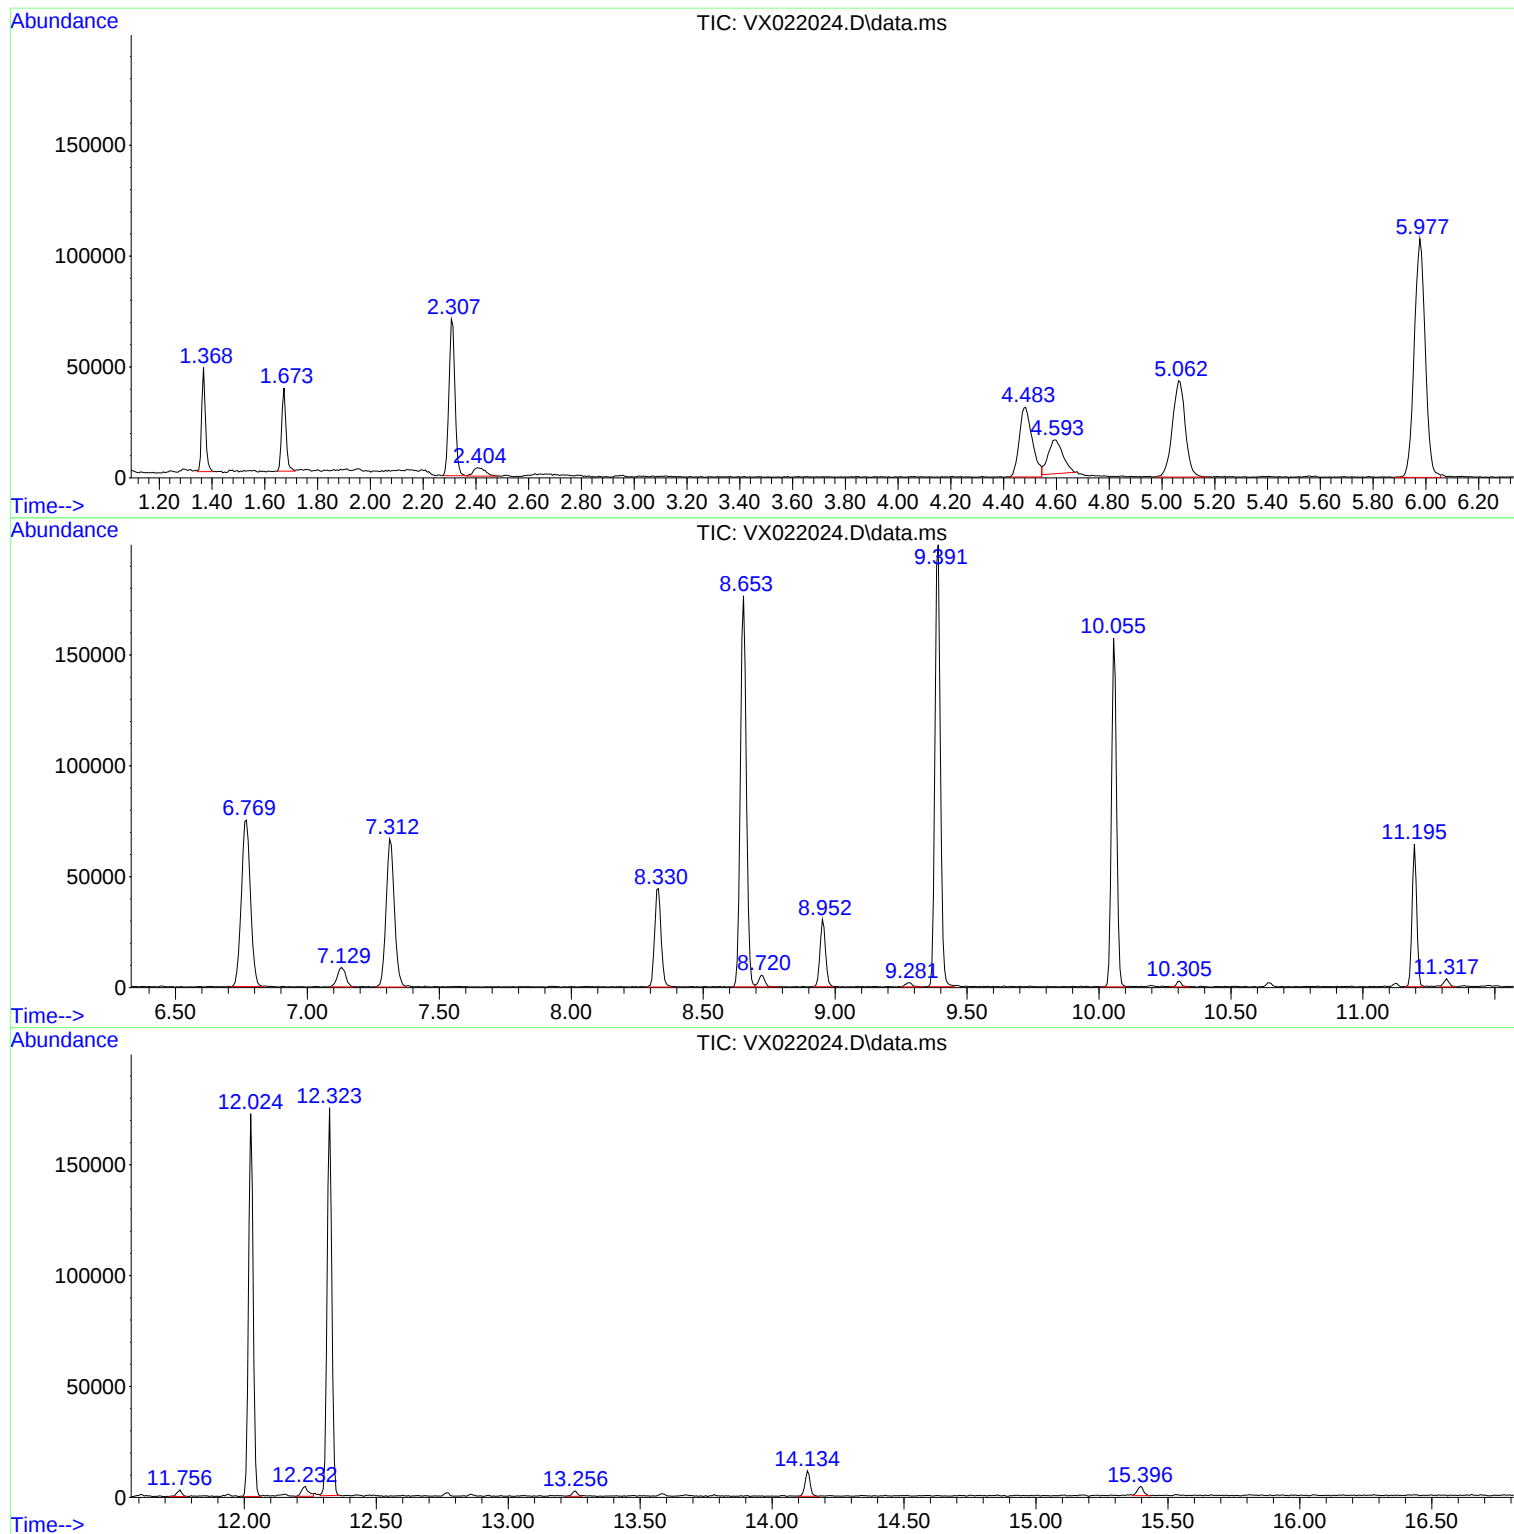

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022024.D
Acq On : 17 May 2021 11:27
Operator : JC/MD
Sample : M2410-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022024.D
Acq On : 17 May 2021 11:27
Operator : JC/MD
Sample : M2410-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
