

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022026.D
 Acq On : 17 May 2021 12:12
 Operator : JC/MD
 Sample : M2410-03DL 5X
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6M8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX022026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rBV	46981	44487	11.48%	1.544%
2	1.502	64	68	73	rVB2	7756	9822	2.53%	0.341%
3	1.672	91	96	102	rBV	37346	45879	11.83%	1.592%
4	2.306	194	200	208	rBV	65099	106181	27.39%	3.685%
5	2.788	275	279	289	rVB2	3948	7271	1.88%	0.252%
6	4.483	547	557	568	rBV	32234	106257	27.41%	3.688%
7	4.599	568	576	588	rVB2	5793	22955	5.92%	0.797%
8	5.068	642	653	668	rVB	45890	127134	32.80%	4.412%
9	5.977	791	802	814	rBV2	102607	298503	77.00%	10.360%
10	6.769	922	932	943	rBV2	77869	181930	46.93%	6.314%
11	7.135	981	992	1001	rBV	174229	387659	100.00%	13.454%
12	7.318	1014	1022	1034	rBV	63091	140671	36.29%	4.882%
13	8.330	1181	1188	1197	rBV	43936	74306	19.17%	2.579%
14	8.653	1234	1241	1249	rBV	175722	271046	69.92%	9.407%
15	8.726	1249	1253	1260	rVB3	2431	3924	1.01%	0.136%
16	8.952	1285	1290	1298	rBV	28409	42815	11.04%	1.486%
17	9.275	1337	1343	1349	rBV2	9901	14672	3.78%	0.509%
18	9.391	1356	1362	1373	rBV	198935	278719	71.90%	9.673%
19	10.055	1465	1471	1483	rBV	154774	215576	55.61%	7.482%
20	11.195	1653	1658	1665	rVB	62877	76882	19.83%	2.668%
21	12.024	1789	1794	1800	rBV	174840	210225	54.23%	7.296%
22	12.323	1836	1843	1849	rBV	166902	214358	55.30%	7.440%


Sum of corrected areas: 2881272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022026.D
Acq On : 17 May 2021 12:12
Operator : JC/MD
Sample : M2410-03DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

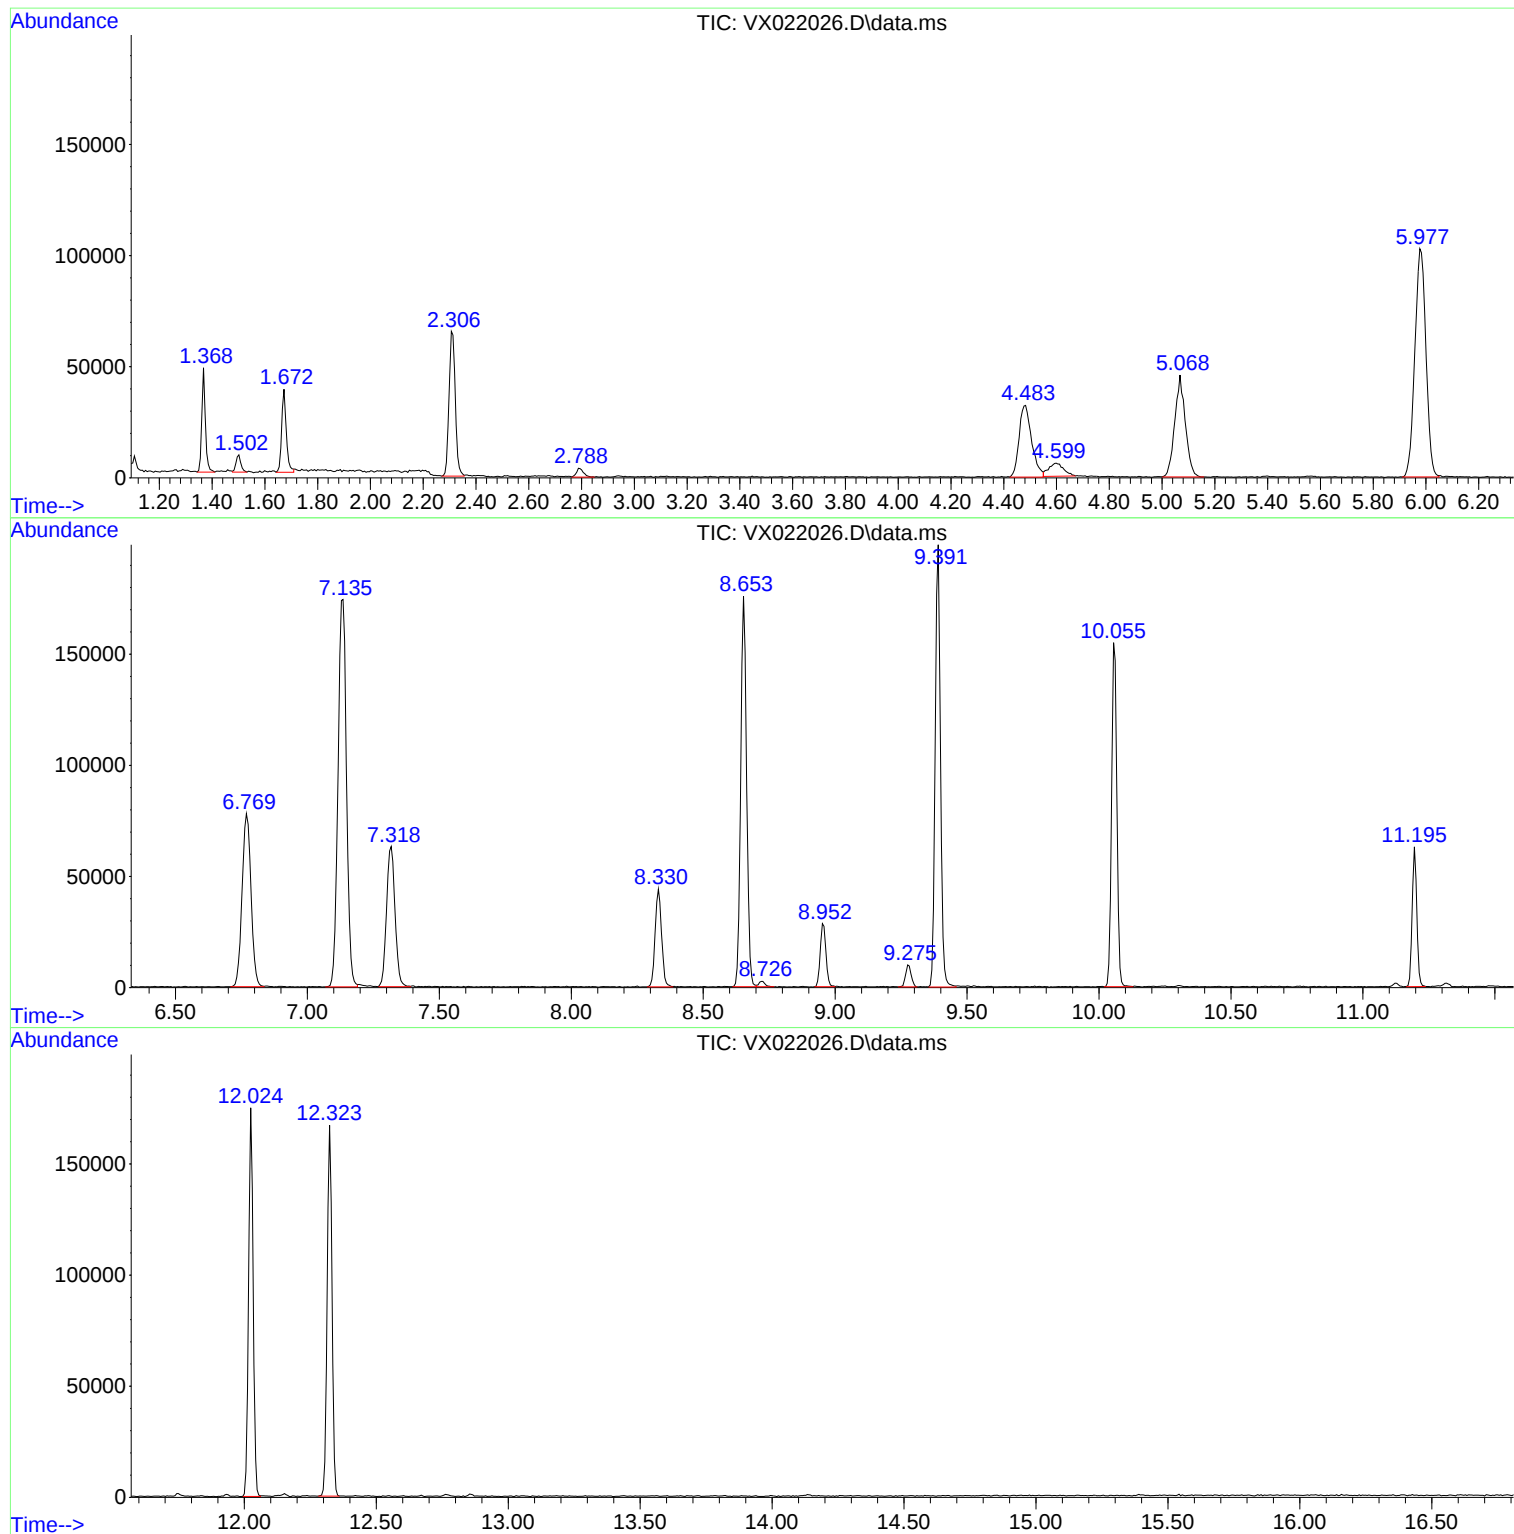

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022026.D
Acq On : 17 May 2021 12:12
Operator : JC/MD
Sample : M2410-03DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022026.D
Acq On : 17 May 2021 12:12
Operator : JC/MD
Sample : M2410-03DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
