

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022027.D
 Acq On : 17 May 2021 12:36
 Operator : JC/MD
 Sample : M2410-04DL 4X
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6M9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX022027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	42447	42836	14.40%	1.633%
2	1.672	91	96	102	rBV	36469	44115	14.83%	1.682%
3	2.209	181	184	190	rVB4	2521	4525	1.52%	0.172%
4	2.307	194	200	210	rBV	68784	107588	36.17%	4.101%
5	2.794	275	280	286	rVB3	3413	5993	2.01%	0.228%
6	4.483	544	557	570	rBV2	30244	106471	35.79%	4.059%
7	5.062	640	652	668	rVB	41568	128139	43.08%	4.885%
8	5.977	790	802	813	rBV2	102432	297475	100.00%	11.340%
9	6.769	920	932	940	rBV	71436	168996	56.81%	6.442%
10	7.129	982	991	1003	rBV2	92015	199783	67.16%	7.616%
11	7.318	1012	1022	1032	rBV	63525	142035	47.75%	5.414%
12	8.330	1180	1188	1198	rVB	45996	74081	24.90%	2.824%
13	8.653	1233	1241	1250	rBV	172691	271321	91.21%	10.343%
14	8.726	1250	1253	1260	rVB3	2200	3539	1.19%	0.135%
15	8.952	1285	1290	1300	rBV	28411	43141	14.50%	1.645%
16	9.281	1338	1344	1351	rVB2	11769	17202	5.78%	0.656%
17	9.391	1355	1362	1370	rBV	193481	276723	93.02%	10.549%
18	10.055	1466	1471	1479	rBV	147438	202785	68.17%	7.730%
19	11.195	1653	1658	1665	rVB	62604	77560	26.07%	2.957%
20	12.024	1789	1794	1800	rBV	159972	196884	66.19%	7.505%
21	12.323	1835	1843	1850	rBV	169153	212067	71.29%	8.084%




Sum of corrected areas: 2623259

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022027.D
Acq On : 17 May 2021 12:36
Operator : JC/MD
Sample : M2410-04DL 4X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

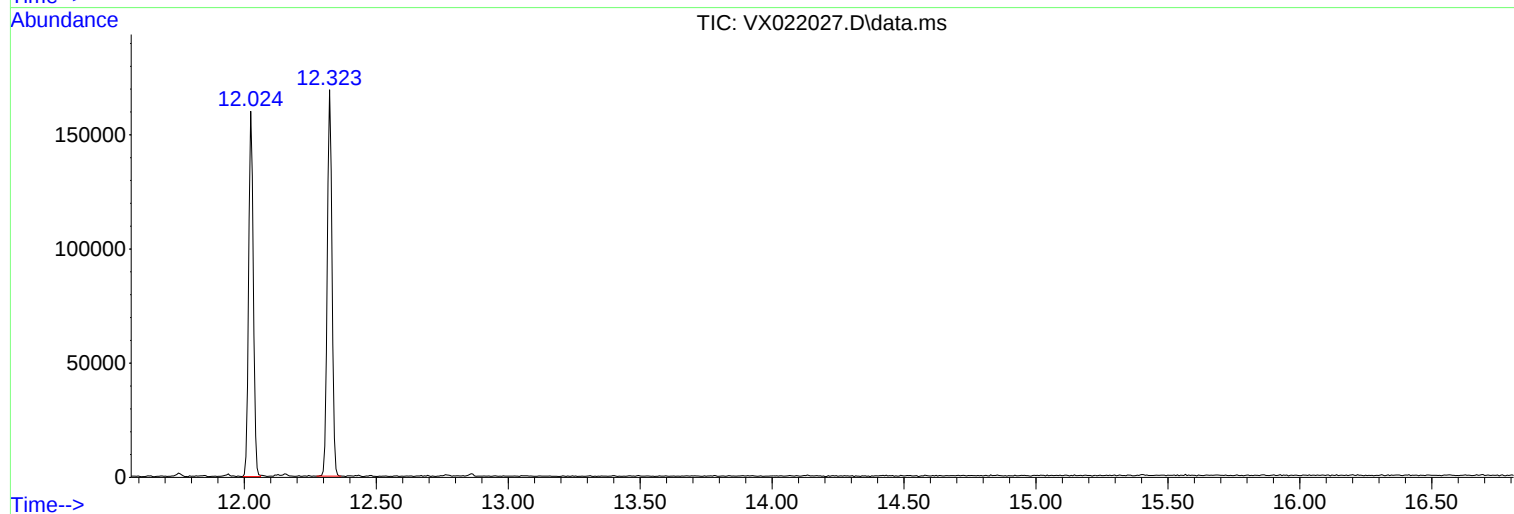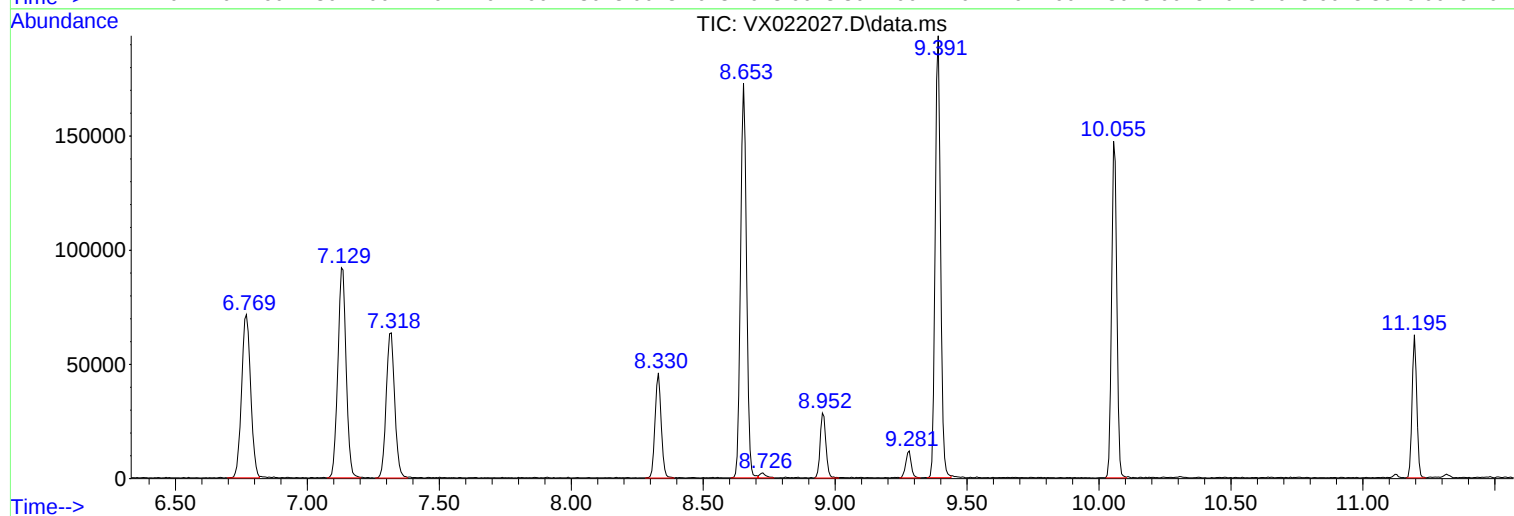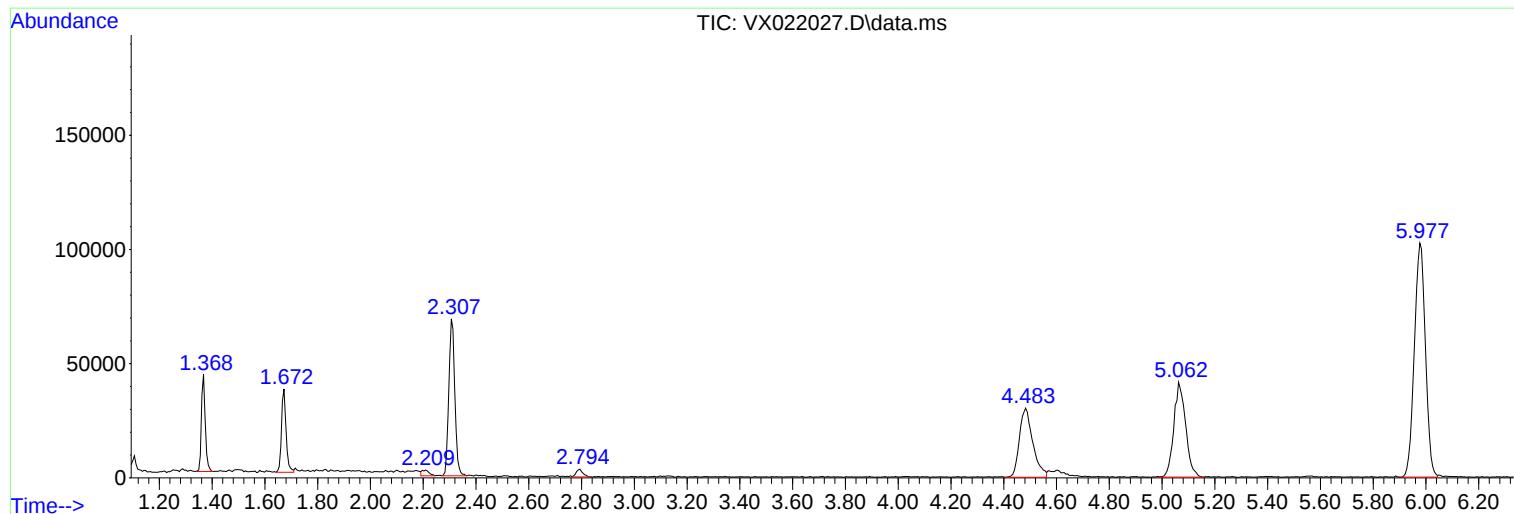

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022027.D
Acq On : 17 May 2021 12:36
Operator : JC/MD
Sample : M2410-04DL 4X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022027.D
Acq On : 17 May 2021 12:36
Operator : JC/MD
Sample : M2410-04DL 4X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6M9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
