

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022031.D
 Acq On : 17 May 2021 14:09
 Operator : JC/MD
 Sample : M2410-09DL 5X
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6N4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX022031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB	44762	43928	12.94%	1.572%
2	1.672	89	96	104	rBV	36581	46511	13.70%	1.665%
3	2.306	194	200	212	rVB	66727	105896	31.20%	3.791%
4	2.794	275	280	287	rVB3	2932	5378	1.58%	0.193%
5	3.117	326	333	343	rVB2	1915	4360	1.28%	0.156%
6	4.483	547	557	569	rBV	31929	108805	32.05%	3.895%
7	5.068	640	653	668	rBV	39919	131083	38.62%	4.692%
8	5.976	791	802	814	rBV2	103134	302166	89.02%	10.816%
9	6.769	921	932	945	rBV2	69301	170339	50.18%	6.097%
10	7.129	980	991	1003	rBV	156631	339452	100.00%	12.151%
11	7.318	1013	1022	1036	rVB	63599	141286	41.62%	5.057%
12	8.330	1181	1188	1196	rBV	45323	73479	21.65%	2.630%
13	8.653	1234	1241	1249	rBV	179635	277767	81.83%	9.943%
14	8.720	1249	1252	1259	rVB2	2983	4533	1.34%	0.162%
15	8.951	1284	1290	1297	rBV	28214	41805	12.32%	1.496%
16	9.275	1337	1343	1350	rVB2	23140	33888	9.98%	1.213%
17	9.390	1356	1362	1376	rBV	188241	274044	80.73%	9.810%
18	10.055	1466	1471	1480	rVB	140844	199116	58.66%	7.128%
19	11.195	1653	1658	1664	rBV	63802	78317	23.07%	2.803%
20	12.024	1789	1794	1802	rBV	167356	197750	58.26%	7.079%
21	12.323	1837	1843	1849	rVV	172407	213720	62.96%	7.650%


Sum of corrected areas: 2793623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022031.D
Acq On : 17 May 2021 14:09
Operator : JC/MD
Sample : M2410-09DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

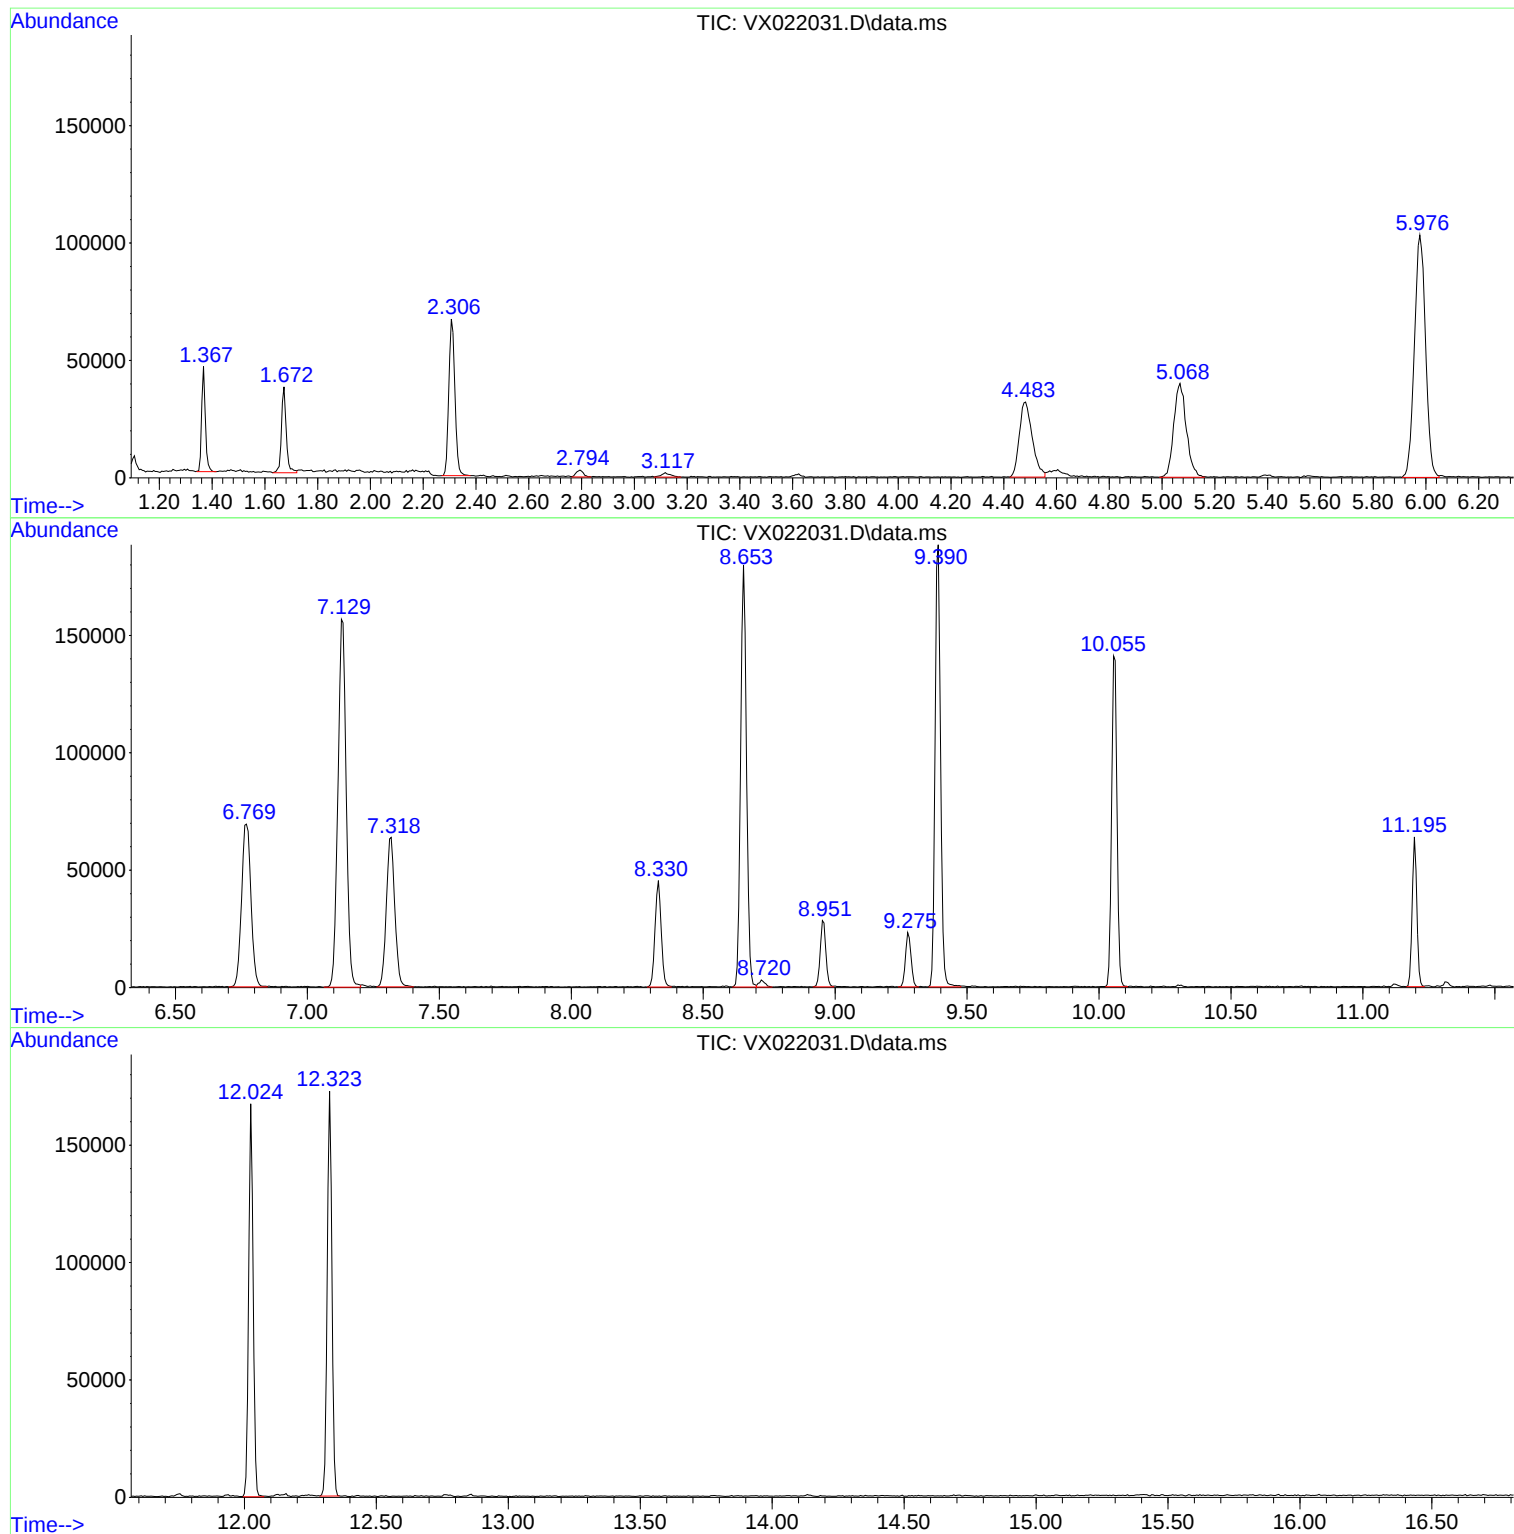

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022031.D
Acq On : 17 May 2021 14:09
Operator : JC/MD
Sample : M2410-09DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022031.D
Acq On : 17 May 2021 14:09
Operator : JC/MD
Sample : M2410-09DL 5X
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
