

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022033.D
 Acq On : 17 May 2021 14:56
 Operator : JC/MD
 Sample : M2410-11
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG6N6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX022033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	51	rBV	41574	41983	14.09%	1.697%
2	1.672	92	96	103	rVB	35897	43110	14.46%	1.742%
3	2.306	194	200	213	rBV	68380	108501	36.40%	4.385%
4	3.117	324	333	342	rBV	4897	11566	3.88%	0.467%
5	4.477	543	556	569	rBV	33095	105927	35.54%	4.281%
6	5.068	638	653	666	rBV	41442	128791	43.21%	5.205%
7	5.976	789	802	818	rBV2	102886	298042	100.00%	12.045%
8	6.769	922	932	942	rBV	72486	167841	56.31%	6.783%
9	7.129	982	991	1001	rBV	38723	84614	28.39%	3.420%
10	7.312	1013	1021	1032	rBV2	63109	138341	46.42%	5.591%
11	8.330	1179	1188	1195	rBV	44113	71259	23.91%	2.880%
12	8.653	1233	1241	1249	rBV	176690	270417	90.73%	10.929%
13	8.720	1249	1252	1258	rVB2	2561	4498	1.51%	0.182%
14	8.951	1285	1290	1298	rBV	27604	40156	13.47%	1.623%
15	9.390	1356	1362	1370	rBV	189822	270580	90.79%	10.935%
16	10.055	1466	1471	1484	rBV	148264	199631	66.98%	8.068%
17	11.195	1653	1658	1663	rBV	62449	76262	25.59%	3.082%
18	11.311	1673	1677	1684	rVB3	1994	3207	1.08%	0.130%
19	12.024	1789	1794	1801	rBV	158962	195388	65.56%	7.896%
20	12.225	1821	1827	1836	rBV3	3133	6134	2.06%	0.248%
21	12.323	1837	1843	1848	rVB	167240	208166	69.84%	8.413%




Sum of corrected areas: 2474414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022033.D
Acq On : 17 May 2021 14:56
Operator : JC/MD
Sample : M2410-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

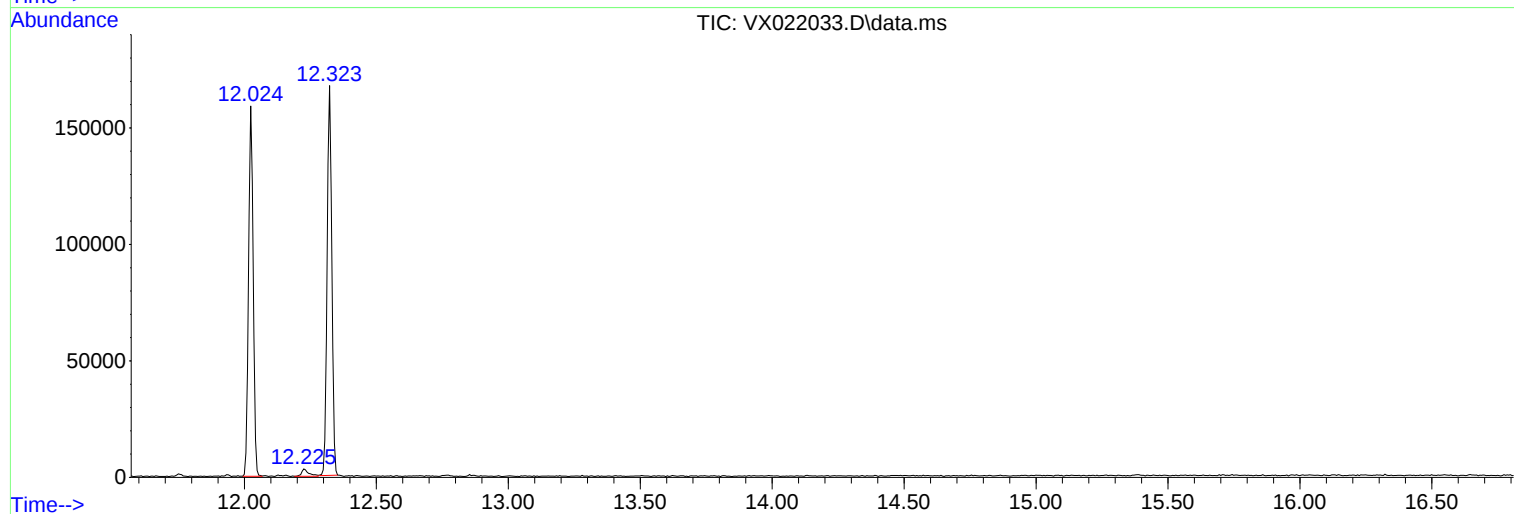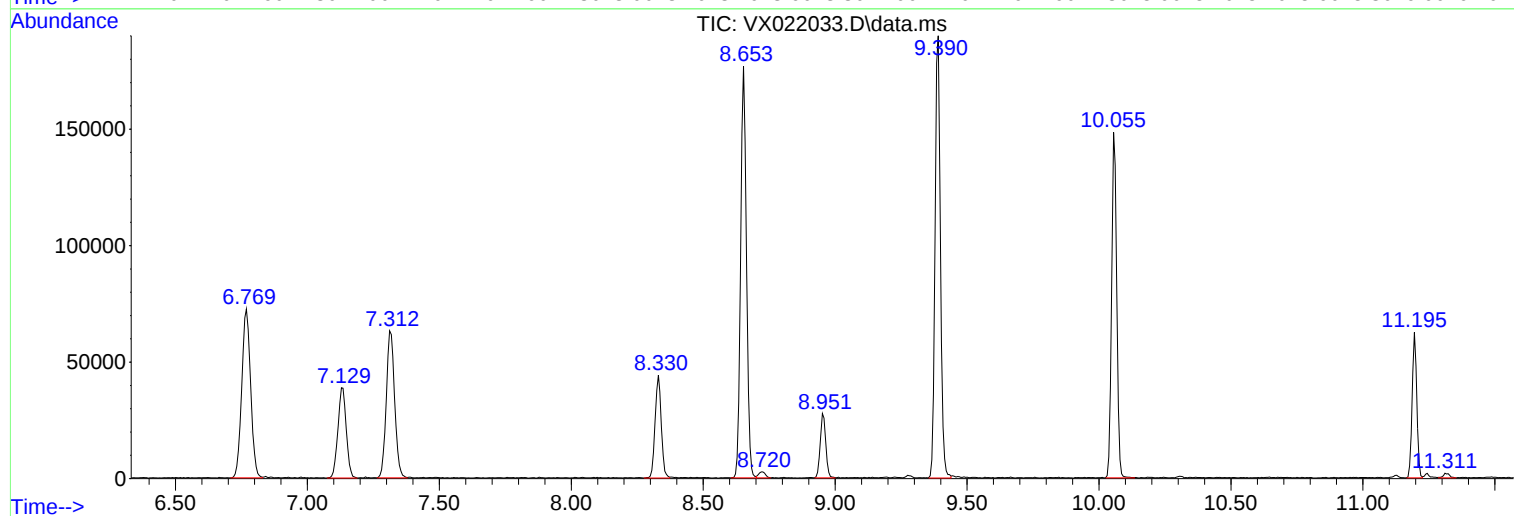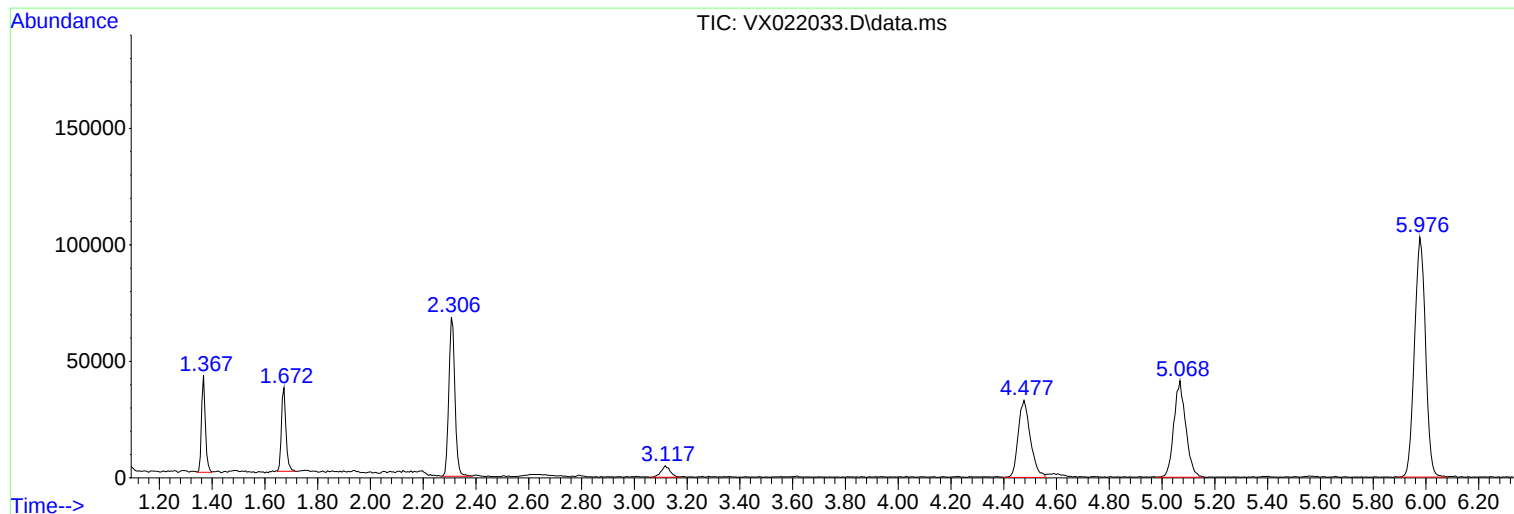

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022033.D
Acq On : 17 May 2021 14:56
Operator : JC/MD
Sample : M2410-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022033.D
Acq On : 17 May 2021 14:56
Operator : JC/MD
Sample : M2410-11
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG6N6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
