

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022034.D
 Acq On : 17 May 2021 15:19
 Operator : JC/MD
 Sample : M2410-13
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX022034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rBV	43404	42622	14.24%	1.790%
2	1.672	91	96	101	rBV	34954	41465	13.85%	1.741%
3	2.306	194	200	211	rVB	66760	104785	35.01%	4.401%
4	2.794	274	280	286	rVB2	6039	9794	3.27%	0.411%
5	4.483	547	557	573	rBV	29024	104127	34.79%	4.373%
6	5.062	642	652	669	rBV	39069	126615	42.31%	5.318%
7	5.977	789	802	814	rBV3	101328	299281	100.00%	12.570%
8	6.769	923	932	943	rBV	72748	168280	56.23%	7.068%
9	7.318	1013	1022	1032	rBV	62869	136540	45.62%	5.735%
10	8.330	1180	1188	1200	rBV	42626	71586	23.92%	3.007%
11	8.653	1234	1241	1249	rBV	174389	267936	89.53%	11.253%
12	8.720	1249	1252	1258	rVB4	2568	3922	1.31%	0.165%
13	8.952	1285	1290	1301	rVB	26934	40637	13.58%	1.707%
14	9.275	1338	1343	1349	rBV4	1812	3489	1.17%	0.147%
15	9.391	1354	1362	1373	rBV	187233	270379	90.34%	11.356%
16	10.055	1466	1471	1482	rVB	143640	199155	66.54%	8.364%
17	11.195	1653	1658	1667	rVB	60224	77758	25.98%	3.266%
18	11.317	1674	1678	1682	rVB2	2701	3720	1.24%	0.156%
19	12.024	1789	1794	1801	rVB	155693	194061	64.84%	8.150%
20	12.323	1835	1843	1851	rVB	172383	211303	70.60%	8.875%
21	12.768	1909	1916	1922	rVB5	1746	3546	1.18%	0.149%


Sum of corrected areas: 2381001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022034.D
Acq On : 17 May 2021 15:19
Operator : JC/MD
Sample : M2410-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

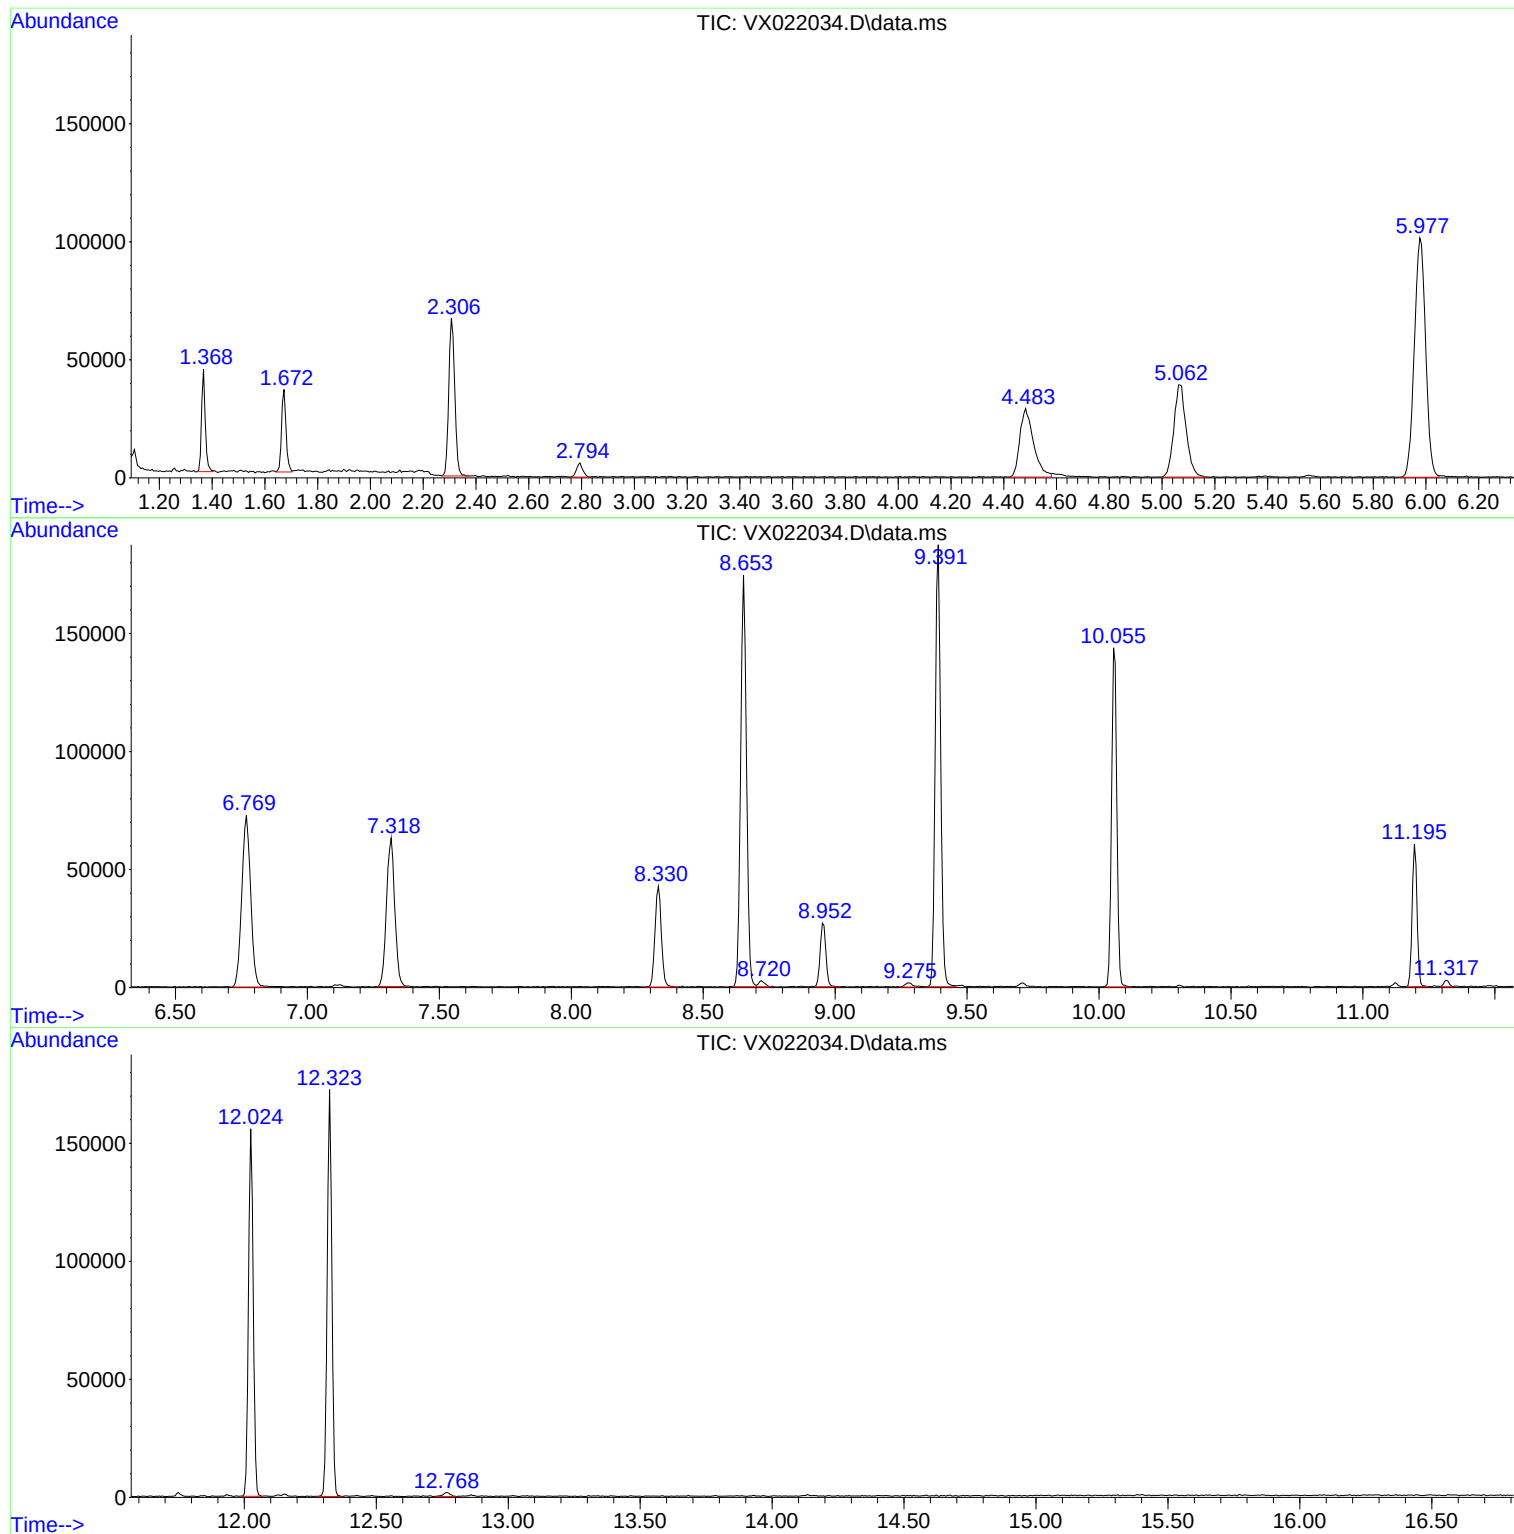

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022034.D
Acq On : 17 May 2021 15:19
Operator : JC/MD
Sample : M2410-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
Data File : VX022034.D
Acq On : 17 May 2021 15:19
Operator : JC/MD
Sample : M2410-13
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
