
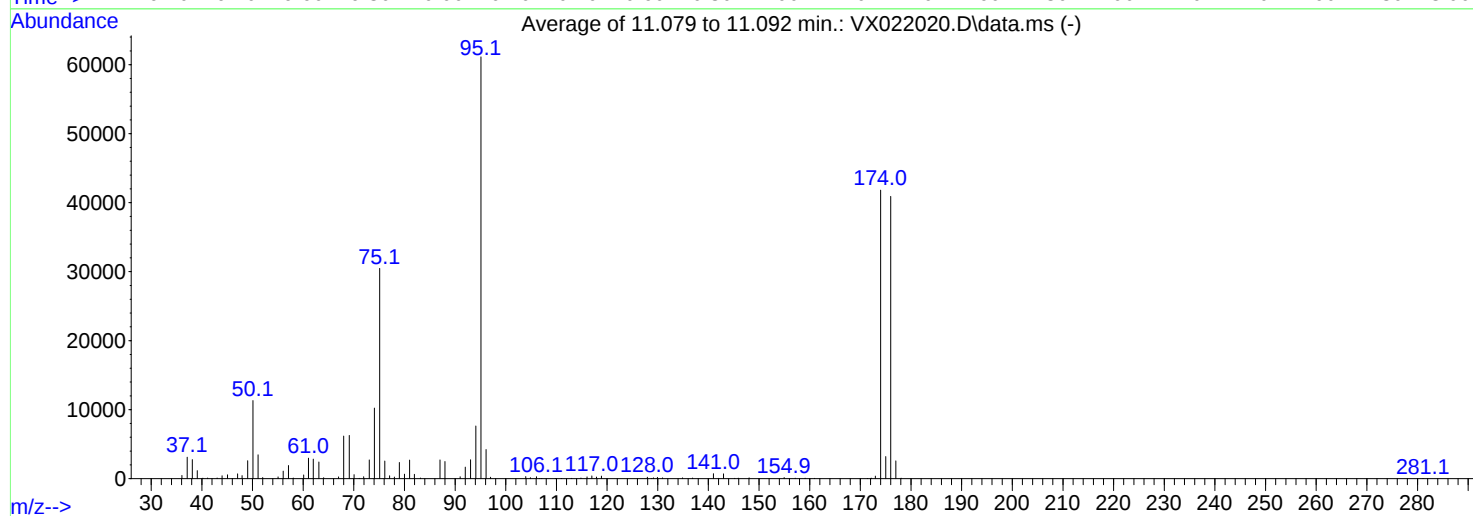


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051721\
 Data File : VX022020.D
 Acq On : 17 May 2021 08:52
 Operator : JC/MD
 Sample : BFB73
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB173

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR051021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 18 04:17:19 2021

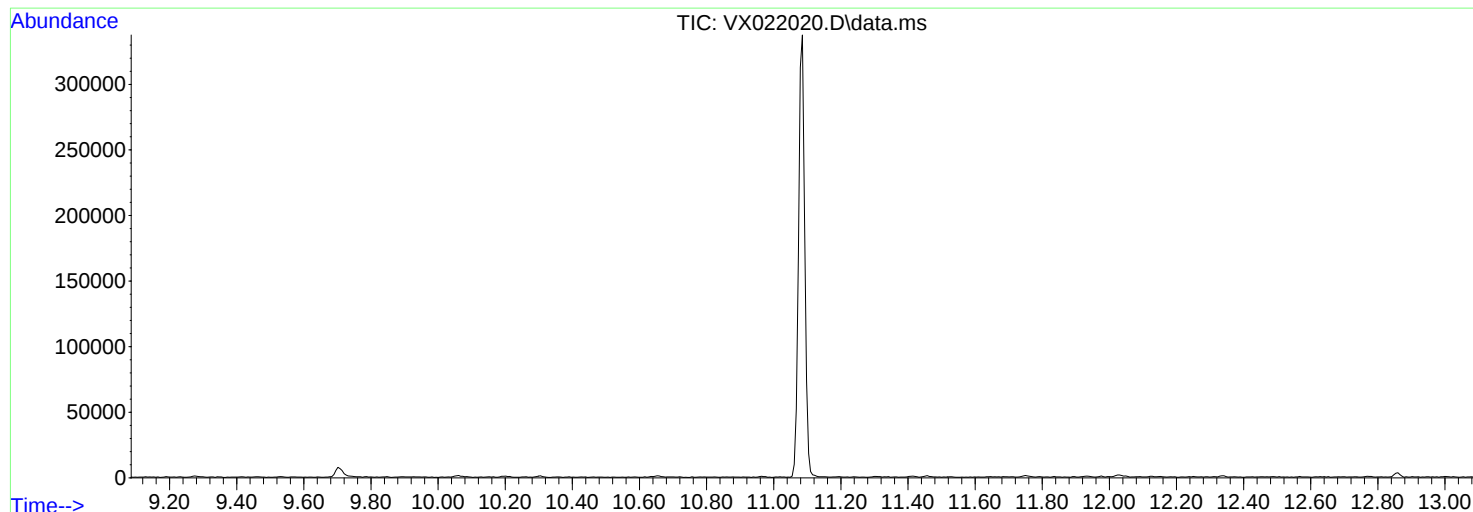

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	11328	PASS
75	95	30	80	49.8	30464	PASS
95	95	100	100	100.0	61136	PASS
96	95	5	9	6.9	4216	PASS
173	174	0.00	2	0.9	367	PASS
174	95	50	120	68.4	41821	PASS
175	174	5	9	7.7	3207	PASS
176	174	95	105	97.8	40899	PASS
177	176	5	10	6.3	2578	PASS

m/z	Abundance
40.00	118.0
44.00	330.0

Instrument :
MSVOA_X
ClientSampleId :
BFB173

m/z	Abundance
36.10	618.0
37.10	3540.0
38.10	2799.0
39.10	1373.0
40.20	103.0
41.10	97.0
42.90	103.0
44.00	733.0
45.10	773.0
47.00	766.0
48.00	420.0
49.00	3202.0
50.10	13123.0
51.10	4115.0
52.00	146.0
55.00	314.0
56.00	1146.0
57.10	2246.0
58.00	190.0
60.10	688.0
61.00	3716.0
62.00	3237.0
63.10	2783.0
64.00	152.0
67.00	247.0
68.00	7524.0
69.10	7190.0
70.00	618.0
71.10	96.0
71.90	330.0
73.10	3049.0
74.00	11847.0
75.10	35368.0
76.10	3041.0
77.00	489.0
78.10	274.0
79.00	2865.0
80.00	711.0
81.00	3168.0
81.90	741.0
83.20	136.0
87.00	3173.0
88.00	2991.0
91.00	430.0
92.00	1861.0
93.00	3141.0
94.10	8853.0
95.10	72360.0
96.10	5364.0
97.00	209.0
104.00	368.0
104.80	146.0
106.10	285.0
107.10	67.0
111.00	64.0
113.00	66.0
114.80	102.0
116.10	222.0
117.00	410.0
117.80	250.0
118.90	462.0
128.00	199.0
128.80	76.0
129.20	114.0
130.00	225.0
131.00	82.0
134.90	163.0
136.90	135.0
141.00	853.0
142.00	110.0
143.00	871.0
145.20	54.0
145.90	105.0
148.10	125.0
154.90	201.0
157.20	110.0
159.10	95.0
160.90	70.0
172.20	94.0
173.00	279.0
174.00	51080.0
175.00	4010.0
176.00	50736.0
177.00	2884.0
178.00	60.0

Instrument :
MSVOA_X
ClientSampleId :
BFB173

m/z	Abundance
36.00	484.0
37.10	3968.0
38.10	3869.0
39.10	1405.0
40.00	237.0
41.10	88.0
43.10	133.0
44.00	928.0
45.00	552.0
46.00	103.0
47.10	794.0
47.90	522.0
49.10	3152.0
50.10	14073.0
51.10	4118.0
52.00	174.0
55.10	263.0
56.10	1345.0
57.10	2181.0
58.10	125.0
60.10	698.0
61.10	3397.0
62.00	3604.0
63.10	2981.0
64.10	195.0
67.00	316.0
68.00	7011.0
69.10	7376.0
70.10	609.0
72.00	360.0
73.00	3281.0
74.10	12028.0
75.10	35792.0
76.10	3130.0
77.00	461.0
78.00	197.0
79.00	2755.0
80.00	731.0
81.00	3218.0
82.00	765.0
83.10	158.0
87.00	3087.0
88.00	2645.0
91.00	256.0
92.00	1963.0
93.00	3001.0
94.10	8247.0
95.10	68704.0
96.10	5055.0
97.00	318.0
103.90	285.0
104.90	174.0
106.00	357.0
106.70	60.0
113.00	73.0
114.80	64.0
116.00	328.0
117.00	589.0
117.90	254.0
119.00	401.0
127.90	294.0
129.10	128.0
129.90	191.0
131.00	121.0
134.90	135.0
136.80	79.0
141.00	780.0
142.10	66.0
143.00	739.0
145.90	136.0
148.00	106.0
155.00	185.0
157.10	77.0
159.10	74.0
161.00	68.0
171.40	73.0
172.00	128.0
172.90	404.0
174.00	41112.0
175.00	2914.0
176.00	38576.0
177.00	2895.0
178.00	78.0
281.10	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB173

m/z	Abundance
36.10	328.0
37.10	1839.0
38.00	1642.0
39.10	719.0
40.20	100.0
41.20	68.0
43.00	53.0
44.00	607.0
45.10	325.0
47.00	502.0
48.00	363.0
49.00	1409.0
50.10	6788.0
51.10	2144.0
52.00	167.0
55.00	170.0
56.10	762.0
57.00	1260.0
60.10	238.0
61.00	1830.0
62.00	1648.0
63.10	1511.0
64.10	104.0
67.10	177.0
68.10	4004.0
69.00	4197.0
70.00	497.0
71.00	65.0
71.90	152.0
73.00	1838.0
74.10	6797.0
75.10	20232.0
76.00	1482.0
77.10	332.0
77.90	201.0
79.00	1445.0
80.00	489.0
80.90	1660.0
81.90	365.0
87.10	1863.0
88.00	1840.0
91.00	157.0
92.00	1218.0
93.10	2088.0
94.10	5760.0
95.10	42344.0
96.10	2228.0
97.10	91.0
104.00	232.0
104.80	120.0
106.00	200.0
109.80	58.0
114.90	83.0
116.10	236.0
117.00	214.0
118.00	176.0
118.80	254.0
127.90	109.0
129.10	93.0
130.00	137.0
130.90	158.0
134.80	52.0
137.00	81.0
141.00	533.0
143.00	513.0
145.20	106.0
148.00	93.0
154.80	75.0
159.10	52.0
172.20	127.0
172.90	417.0
174.00	33272.0
175.00	2696.0
176.00	33384.0
177.00	1954.0
178.10	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB173