

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051722\
 Data File : VX028770.D
 Acq On : 17 May 2022 20:02
 Operator : JC/MD
 Sample : N2884-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31770

Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/18/2022
 Supervised By : Mahesh Dadoda 05/18/2022

Quant Time: May 18 04:55:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	303889	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	542307	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	517999	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	254829	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	206369	49.541	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.080%		
35) Dibromofluoromethane	5.385	113	180290	50.741	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	101.480%		
50) Toluene-d8	8.653	98	648508	48.411	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	96.820%		
62) 4-Bromofluorobenzene	11.079	95	296797	59.318	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	118.640%		
Target Compounds					Qvalue	
4) Vinyl Chloride	1.374	62	1240	0.307	ug/l #	81
11) Tert butyl alcohol	2.953	59	617617	713.426	ug/l #	93
16) Acetone	2.374	43	240159	134.334	ug/l	93
17) Carbon Disulfide	2.514	76	2964	0.364	ug/l	98
19) Methyl tert-butyl Ether	3.117	73	3946	0.354	ug/l #	87
25) 2-Butanone	4.556	43	147344	52.506	ug/l	98
27) cis-1,2-Dichloroethene	4.501	96	4518	1.092	ug/l	89
29) Tetrahydrofuran	4.995	42	4990m	2.736	ug/l	
31) Cyclohexane	5.477	56	8027	1.388	ug/l	97
39) Methylcyclohexane	7.385	83	9501	1.552	ug/l	93
40) Benzene	6.044	78	1590413	103.693	ug/l	100
43) Isopropyl Acetate	6.336	43	27555	3.160	ug/l #	72
51) 4-Methyl-2-Pentanone	8.574	43	61439	10.696	ug/l	91
52) Toluene	8.720	92	1112990	112.807	ug/l	98
59) 2-Hexanone	9.433	43	6639	1.488	ug/l	95
67) Ethyl Benzene	10.195	91	1564917	79.451	ug/l	99
68) m/p-Xylenes	10.299	106	619640	80.804	ug/l	98
69) o-Xylene	10.640	106	317411	42.041	ug/l	98
70) Styrene	10.659	104	551639	44.992	ug/l	97
73) Isopropylbenzene	10.964	105	69996	3.622	ug/l	100
78) n-propylbenzene	11.305	91	59380	2.656	ug/l	96
80) 1,3,5-Trimethylbenzene	11.451	105	128007	7.950	ug/l	99
83) tert-Butylbenzene	11.713	119	6042	0.388	ug/l	92
84) 1,2,4-Trimethylbenzene	11.756	105	338738	20.978	ug/l	98
85) sec-Butylbenzene	11.890	105	10188	0.530	ug/l	88
86) p-Isopropyltoluene	12.012	119	20839	1.291	ug/l	90
88) 1,4-Dichlorobenzene	12.043	146	6833m	0.735	ug/l	
94) Hexachlorobutadiene	13.731	225	826	0.400	ug/l	92
95) Naphthalene	13.780	128	2812844	155.336	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051722\
Data File : VX028770.D
Acq On : 17 May 2022 20:02
Operator : JC/MD
Sample : N2884-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
31770

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022


Quant Time: May 18 04:55:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration

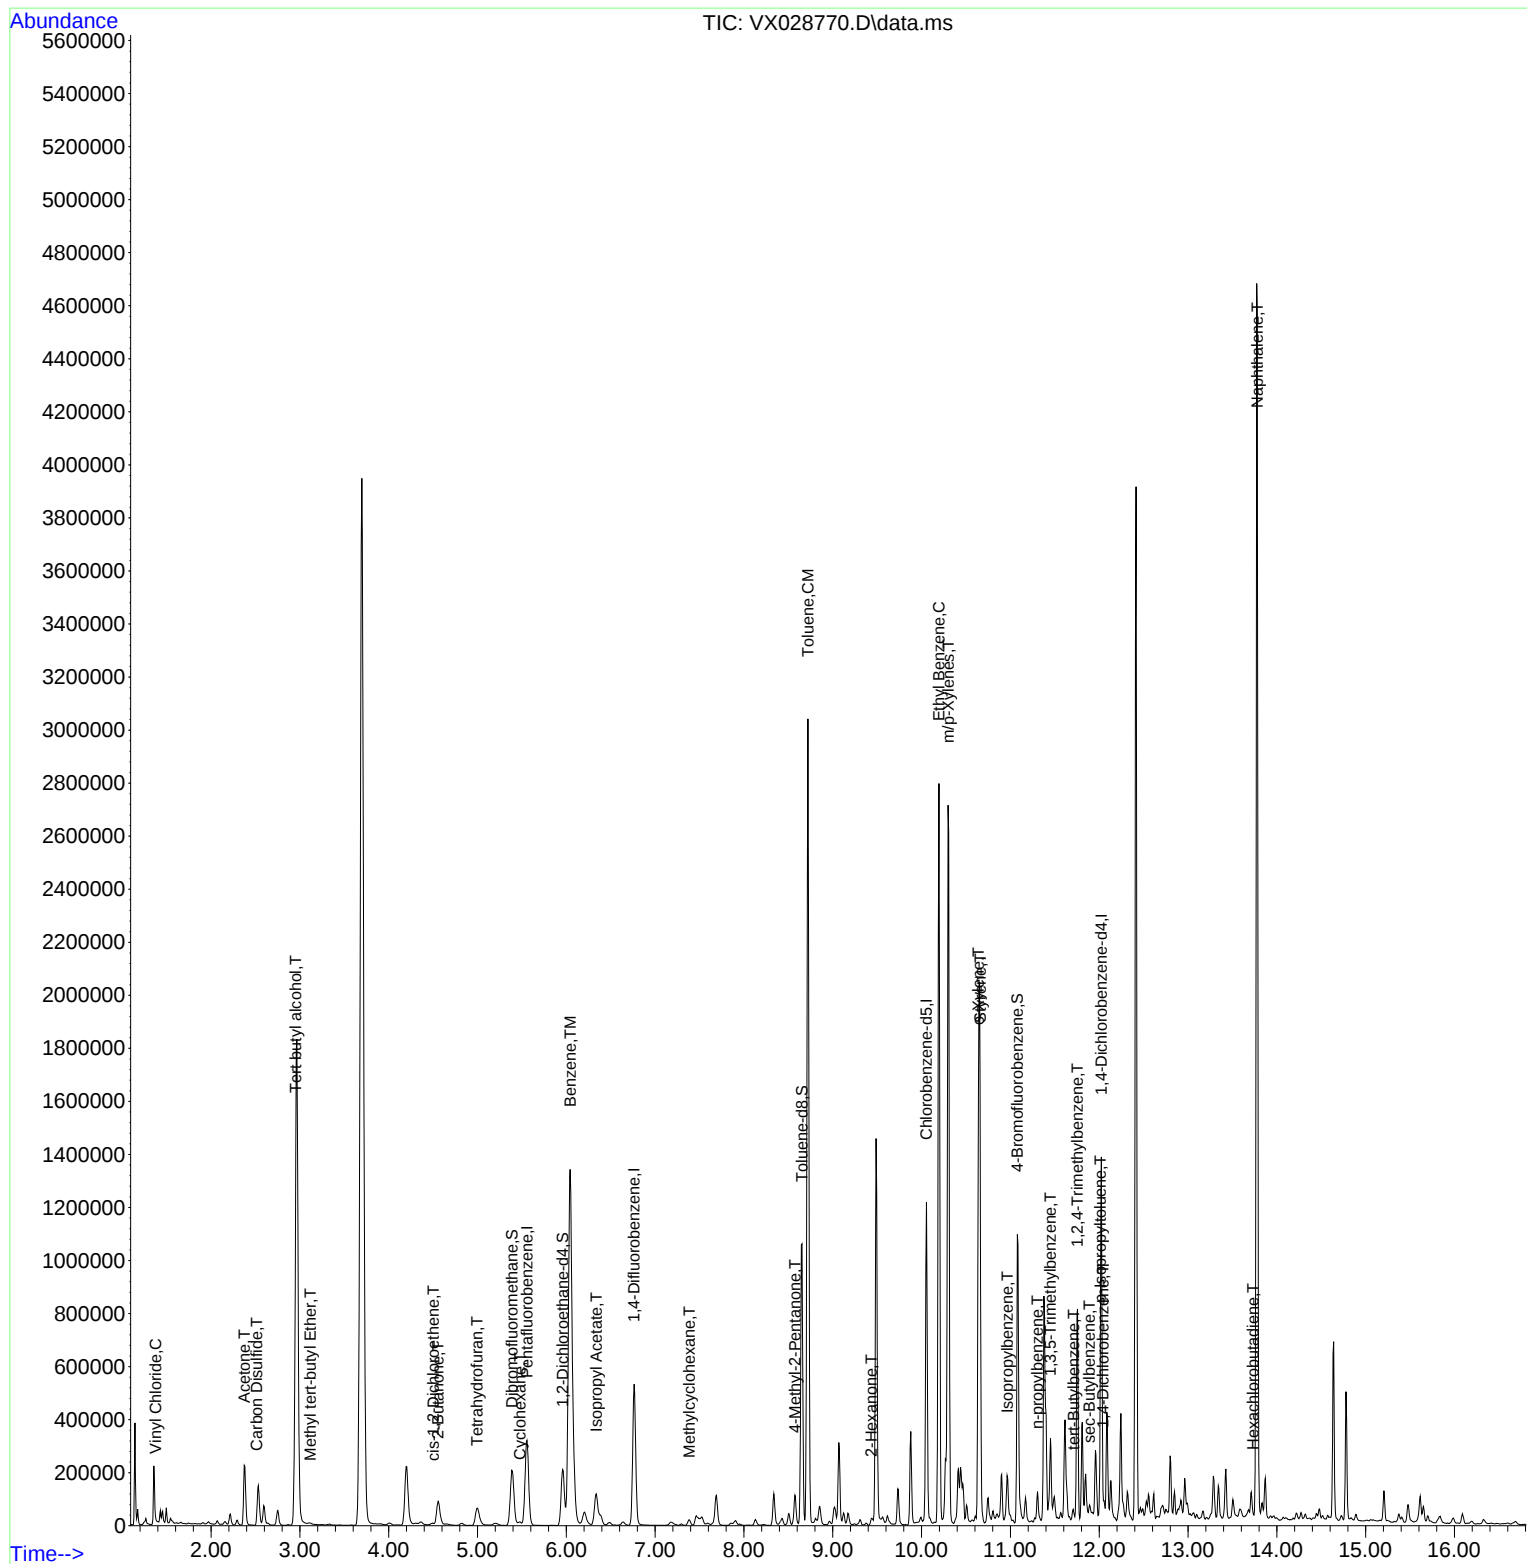



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.007 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770

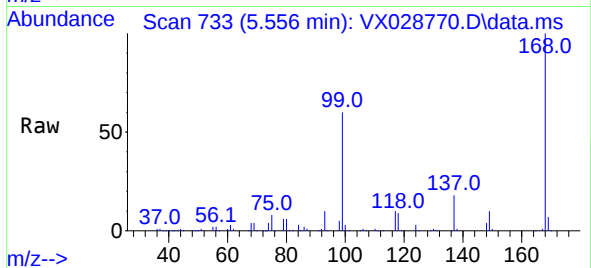

Tgt Ion:168 Resp: 303889
Ion Ratio Lower Upper
168 100
99 59.6 41.7 62.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022



#4
Vinyl Chloride
Concen: 0.307 ug/l
RT: 1.374 min Scan# 47
Delta R.T. 0.001 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Tgt Ion: 62 Resp: 1240
Ion Ratio Lower Upper
62 100
64 42.4 25.5 38.3

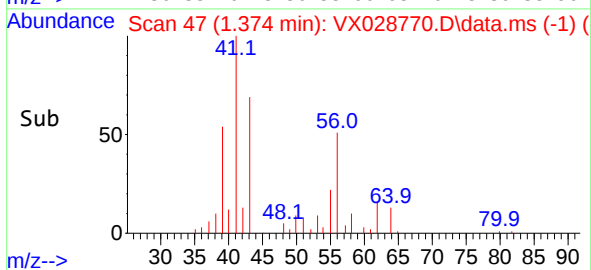



#11

Tert butyl alcohol

Concen: 713.426 ug/l

RT: 2.953 min Scan# 307

Delta R.T. -0.005 min

Lab File: VX028770.D

Acq: 17 May 2022 20:02

Instrument :

MSVOA_X

ClientSampleId :

31770

Tgt Ion: 59 Resp: 61761

Ion Ratio Lower Upper

59 100





57 12.9 8.3 12.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/18/2022

Supervised By :Mahesh Dadoda 05/18/2022

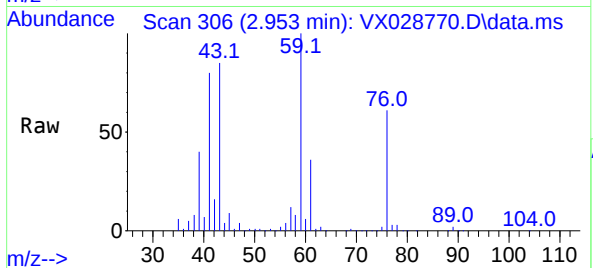

#16

Acetone

Concen: 134.334 ug/l

RT: 2.374 min Scan# 211

Delta R.T. 0.001 min

Lab File: VX028770.D




Acq: 17 May 2022 20:02


Tgt Ion: 43 Resp: 240159

Ion Ratio Lower Upper

43 100

58 31.8 28.8 43.2

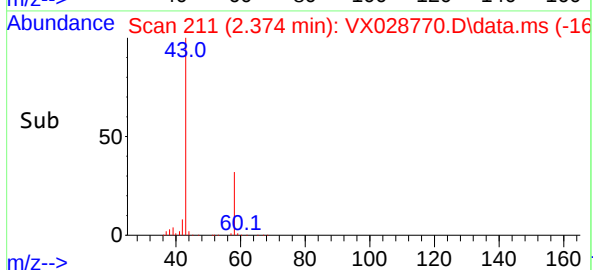







#17
Carbon Disulfide
Concen: 0.364 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.007 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Instrument :
MSVOA_X
ClientSampleId :
31770

Tgt Ion: 76 Resp: 2964
Ion Ratio Lower Upper
76 100
78 8.2 7.2 10.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

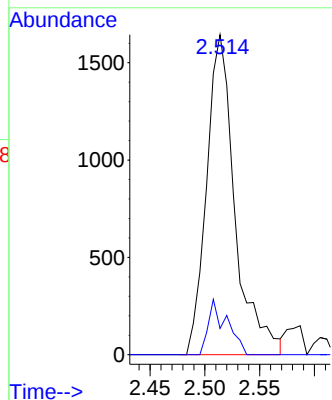

#19
Methyl tert-butyl Ether
Concen: 0.354 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.006 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02


Tgt Ion: 73 Resp: 3946
Ion Ratio Lower Upper
73 100
57 27.1 16.8 25.2#

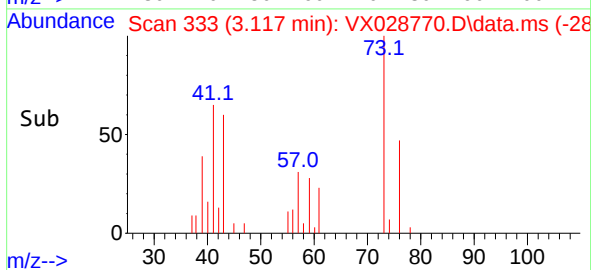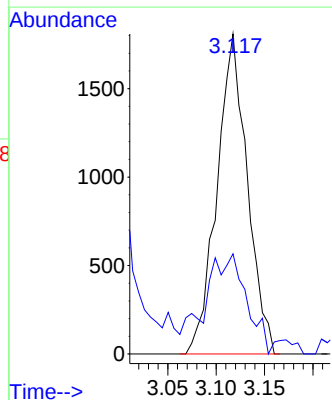



#25
2-Butanone
Concen: 52.506 ug/l
RT: 4.556 min Scan# 50
Delta R.T. 0.006 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770




Tgt Ion: 43 Resp: 147344
Ion Ratio Lower Upper
43 100
72 29.2 24.4 36.6

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022




#27
cis-1,2-Dichloroethene
Concen: 1.092 ug/l
RT: 4.501 min Scan# 560
Delta R.T. 0.012 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Tgt Ion: 96 Resp: 4518
Ion Ratio Lower Upper
96 100
61 122.3 0.0 283.8
98 64.2 0.0 129.8

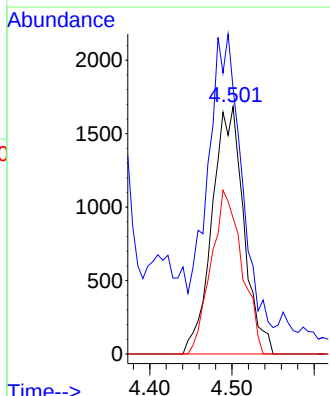



#29
Tetrahydrofuran
Concen: 2.736 ug/l m
RT: 4.995 min Scan# 641
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770

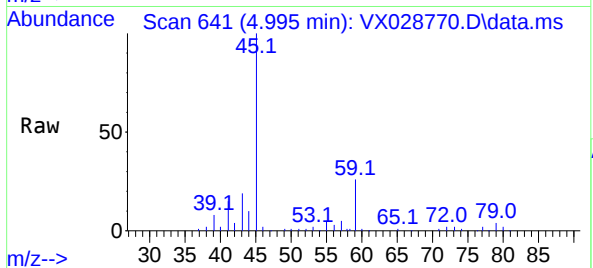


Tgt Ion: 42 Resp: 4990
Ion Ratio Lower Upper
42 100
72 33.2 44.1 66.1
71 15.8 40.5 60.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

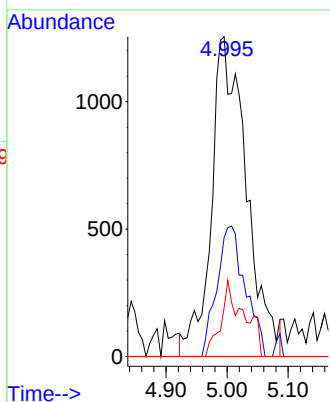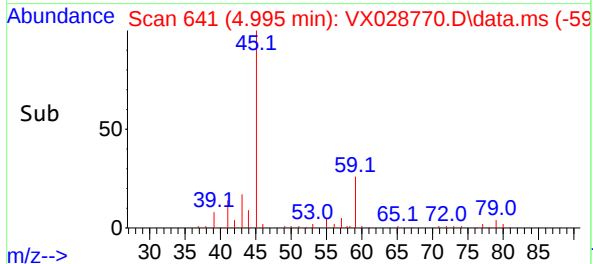


#31
Cyclohexane
Concen: 1.388 ug/l
RT: 5.477 min Scan# 720
Delta R.T. 0.013 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

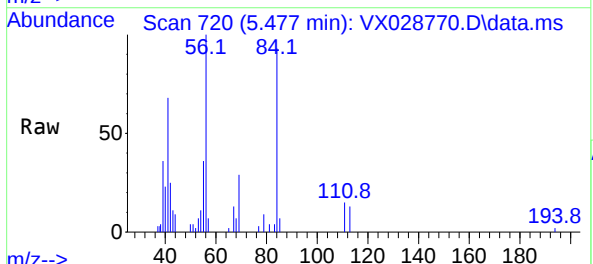

Tgt Ion: 56 Resp: 8027
Ion Ratio Lower Upper
56 100
69 29.4 26.7 40.1
84 95.6 77.2 115.8

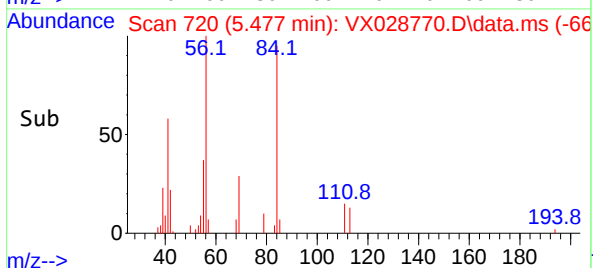



#33

1,2-Dichloroethane-d4

Concen: 49.541 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX028770.D

Acq: 17 May 2022 20:02

Instrument :

MSVOA_X

ClientSampleId :

31770

Tgt Ion: 65 Resp: 206369

Ion Ratio Lower Upper

65 100





67 51.2 0.0 107.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/18/2022

Supervised By :Mahesh Dadoda 05/18/2022

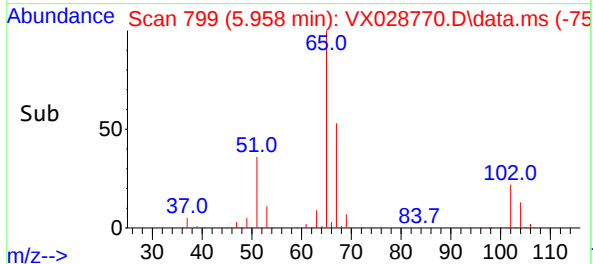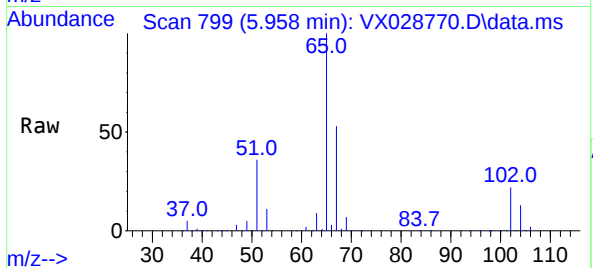

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX028770.D

Acq: 17 May 2022 20:02




Tgt Ion:114 Resp: 542307


Ion Ratio Lower Upper

114 100

63 20.4 0.0 36.8


88 16.3 0.0 32.4

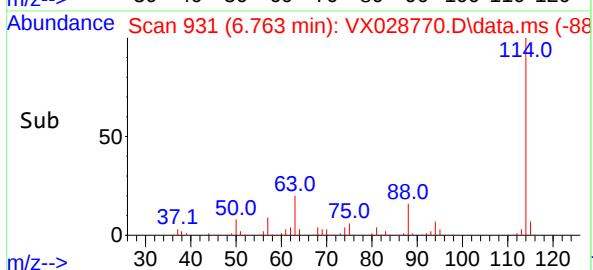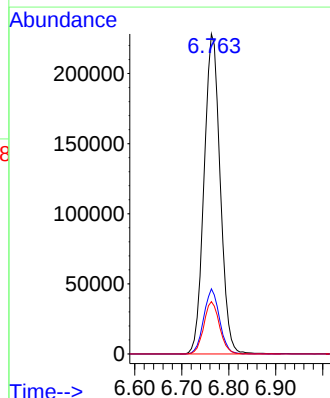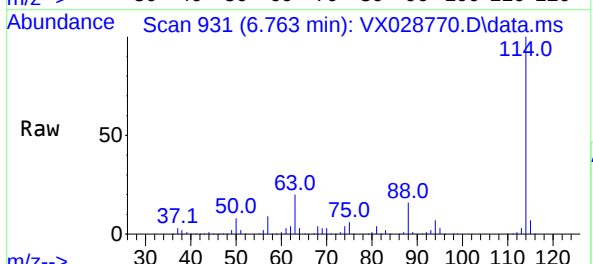

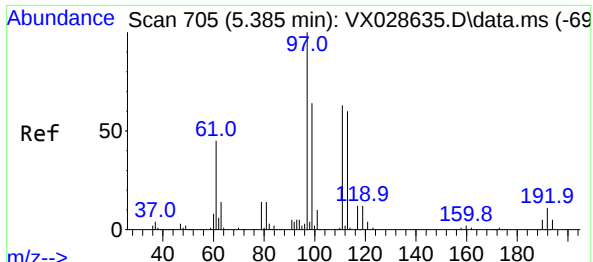

#35
Dibromofluoromethane
Concen: 50.741 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770

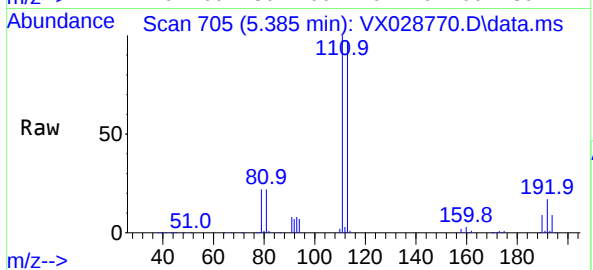


Tgt Ion: 113 Resp: 180290
Ion Ratio Lower Upper
113 100
111 102.0 82.8 124.2
192 18.5 16.9 25.3

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

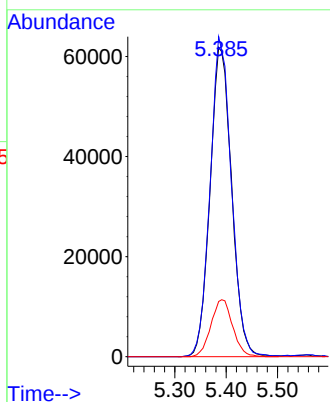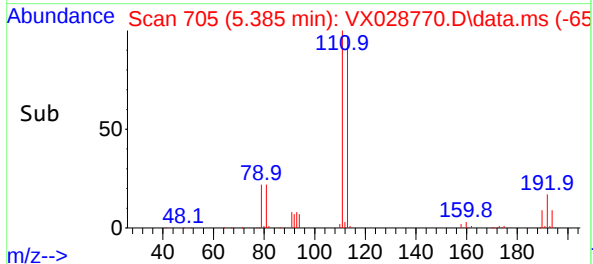


#39
Methylcyclohexane
Concen: 1.552 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.007 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

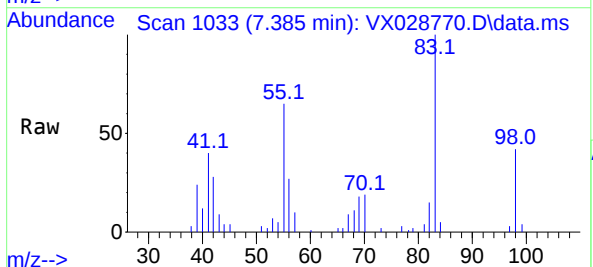

Tgt Ion: 83 Resp: 9501
Ion Ratio Lower Upper
83 100
55 62.8 54.6 81.8
98 42.1 37.4 56.2

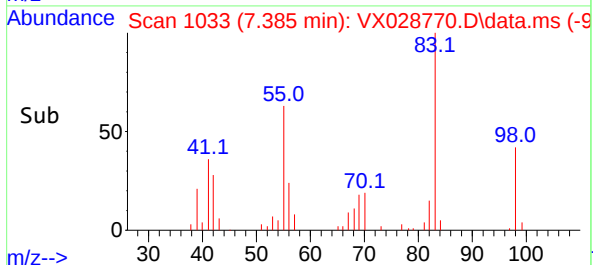







#40
Benzene
Concen: 103.693 ug/l
RT: 6.044 min Scan# 812
Delta R.T. 0.007 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Instrument :
MSVOA_X
ClientSampleId :
31770

Tgt Ion: 78 Resp: 159041
Ion Ratio Lower Upper
78 100
77 24.3 19.3 28.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

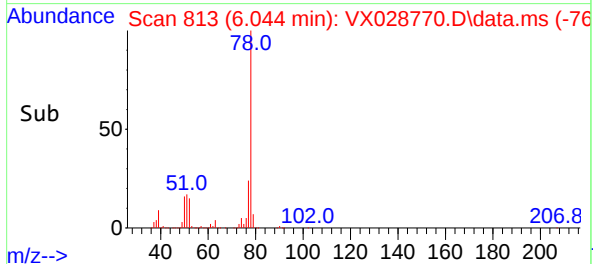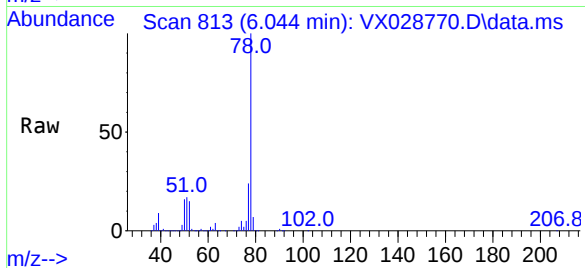

#43
Isopropyl Acetate
Concen: 3.160 ug/l
RT: 6.336 min Scan# 861
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Tgt Ion: 43 Resp: 27555
Ion Ratio Lower Upper
43 100
61 12.9 18.5 27.7#
87 0.0 13.0 19.6#

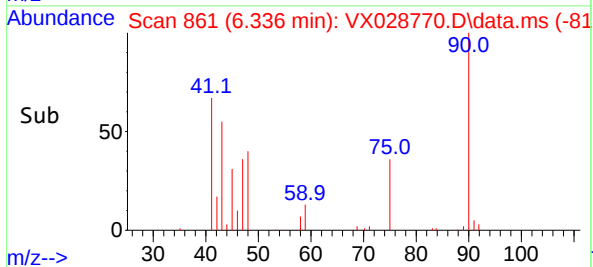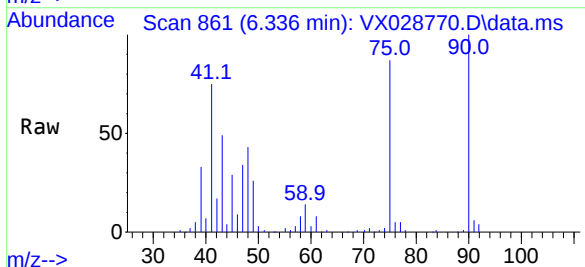







#50
Toluene-d8
Concen: 48.411 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.007 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Instrument :
MSVOA_X
ClientSampleId :
31770

Tgt Ion: 98 Resp: 648508
Ion Ratio Lower Upper
98 100
100 65.3 52.6 78.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

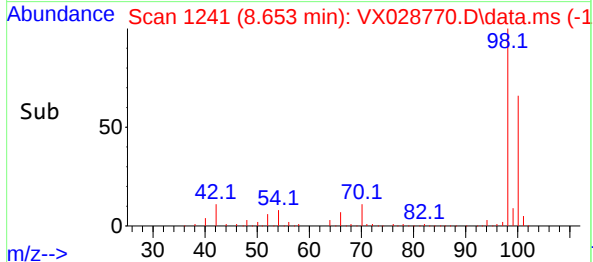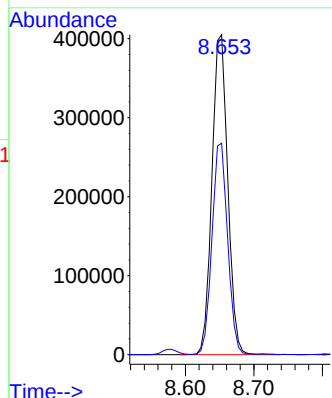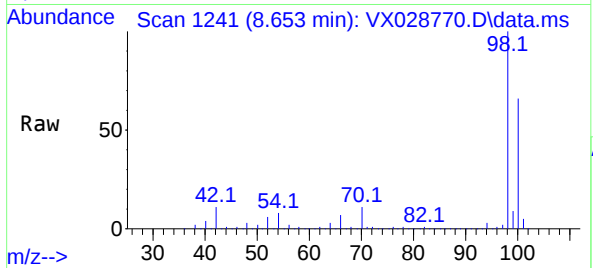

#51
4-Methyl-2-Pentanone
Concen: 10.696 ug/l
RT: 8.574 min Scan# 1228
Delta R.T. 0.001 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02


Tgt Ion: 43 Resp: 61439
Ion Ratio Lower Upper
43 100
58 39.4 36.1 54.1

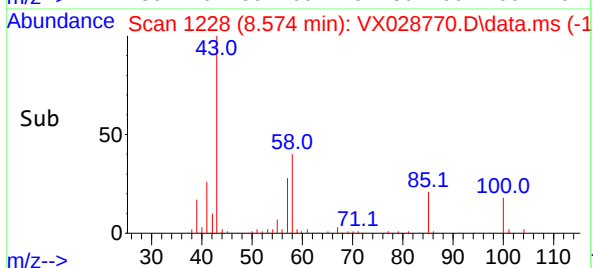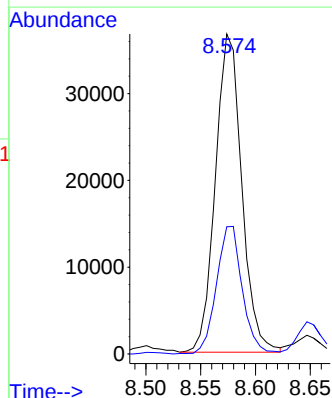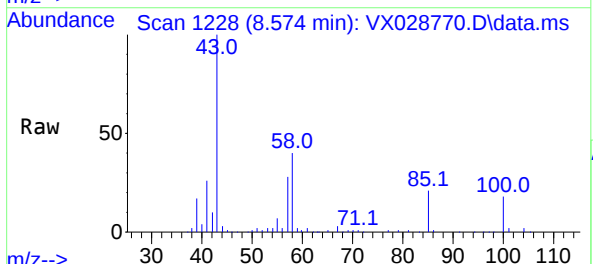



#52
Toluene
Concen: 112.807 ug/l
RT: 8.720 min Scan# 1112990
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770

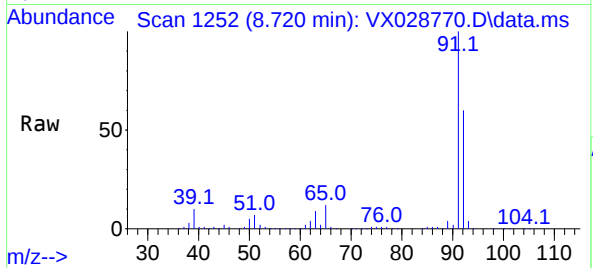

Tgt Ion: 92 Resp: 1112990
Ion Ratio Lower Upper
92 100
91 169.1 137.5 206.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

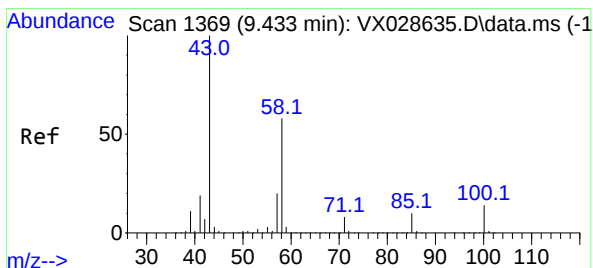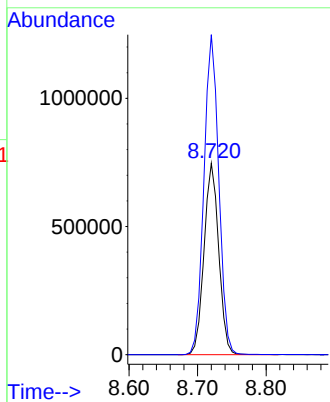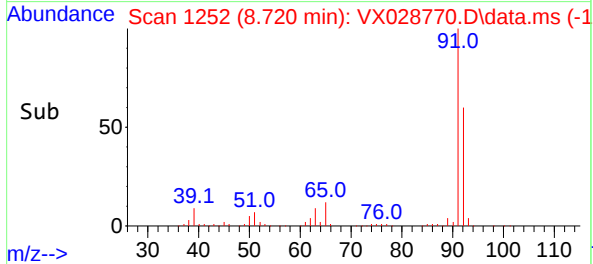

#59
2-Hexanone
Concen: 1.488 ug/l
RT: 9.433 min Scan# 1369
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Tgt Ion: 43 Resp: 6639
Ion Ratio Lower Upper
43 100
58 60.2 31.9 95.7

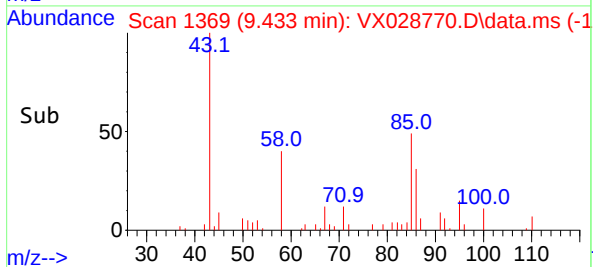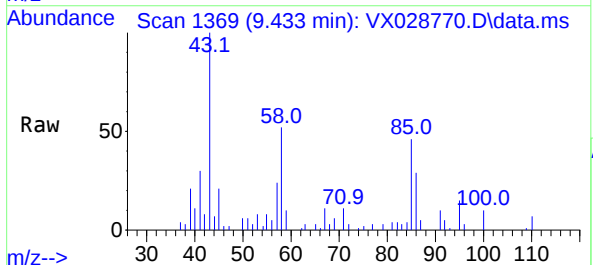







#62
4-Bromofluorobenzene
Concen: 59.318 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Instrument :
MSVOA_X
ClientSampleId :
31770

Tgt Ion: 95 Resp: 29679
Ion Ratio Lower Upper
95 100
174 75.5 0.0 163.0
176 72.9 0.0 155.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

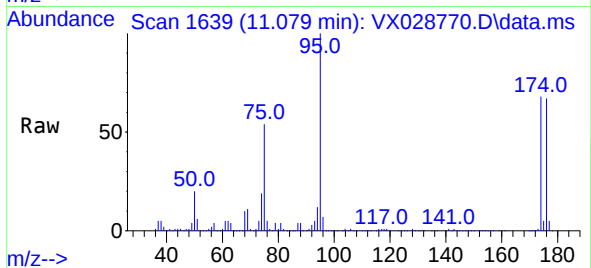

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Tgt Ion:117 Resp: 517999
Ion Ratio Lower Upper
117 100
82 56.3 41.8 62.8
119 32.5 24.8 37.2

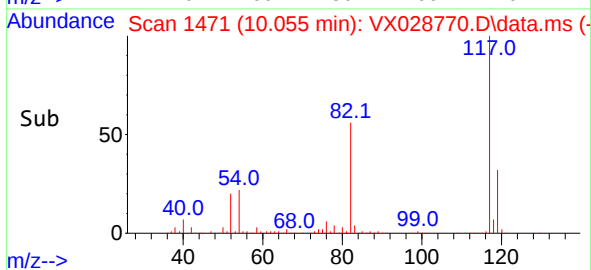



#67

Ethyl Benzene

Concen: 79.451 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX028770.D

Acq: 17 May 2022 20:02

Instrument :

MSVOA_X

ClientSampleId :

31770

Tgt Ion: 91 Resp: 156491

Ion Ratio Lower Upper

91 100





106 31.4 24.6 36.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/18/2022

Supervised By :Mahesh Dadoda 05/18/2022

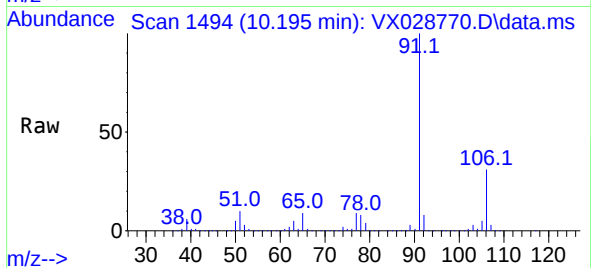

#68

m/p-Xylenes

Concen: 80.804 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.006 min

Lab File: VX028770.D




Acq: 17 May 2022 20:02


Tgt Ion:106 Resp: 619640

Ion Ratio Lower Upper

106 100

91 204.1 160.4 240.6

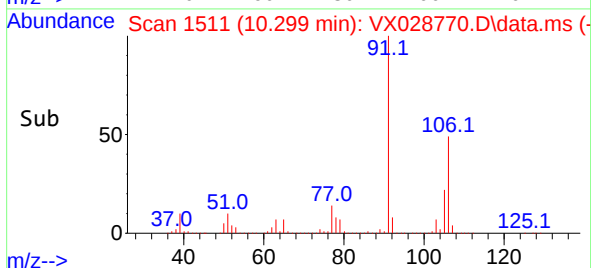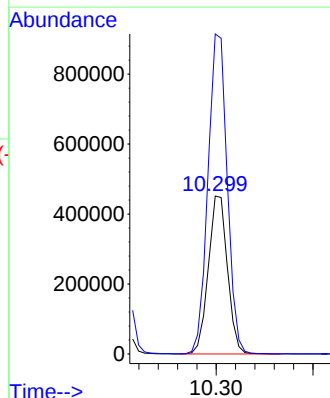







#69
o-Xylene
Concen: 42.041 ug/l
RT: 10.640 min Scan# 1568
Delta R.T. -0.006 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Instrument :
MSVOA_X
ClientSampleId :
31770

Tgt Ion:106 Resp: 31741
Ion Ratio Lower Upper
106 100
91 216.0 106.1 318.1




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

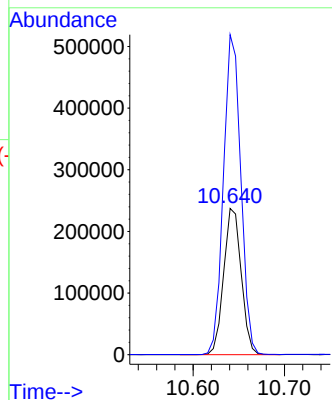

#70
Styrene
Concen: 44.992 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.001 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02


Tgt Ion:104 Resp: 551639
Ion Ratio Lower Upper
104 100
78 52.1 38.6 57.8
103 54.4 43.8 65.8

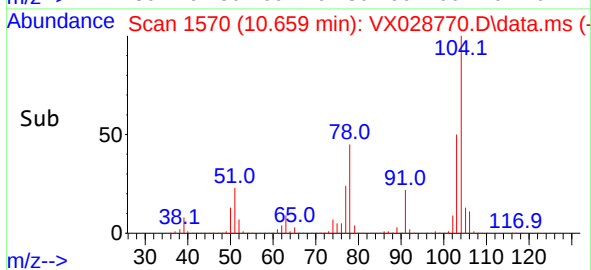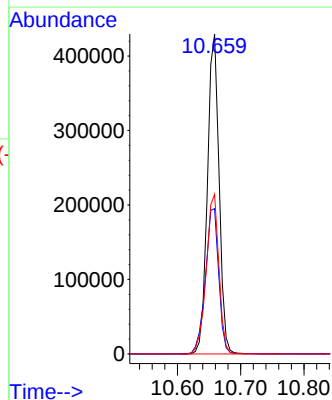



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770

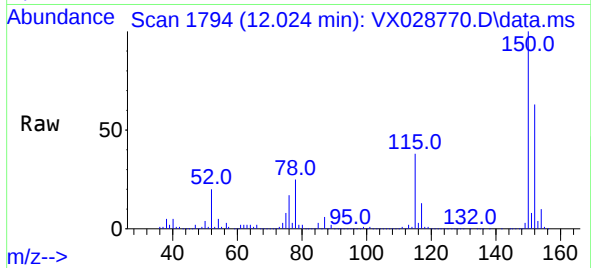


Tgt Ion:152 Resp: 254829
Ion Ratio Lower Upper
152 100
115 61.4 37.5 112.7
150 161.2 0.0 338.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

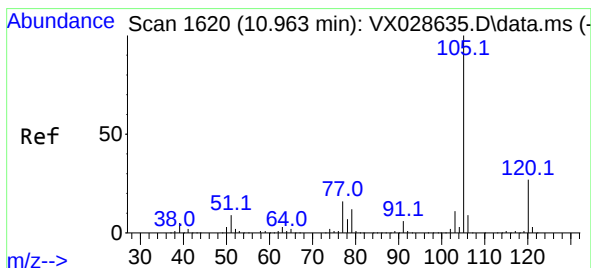


#73
Isopropylbenzene
Concen: 3.622 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

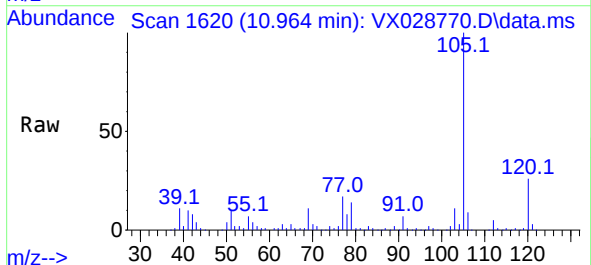

Tgt Ion:105 Resp: 69996
Ion Ratio Lower Upper
105 100
120 27.0 13.5 40.5

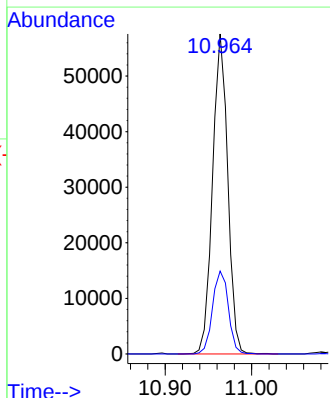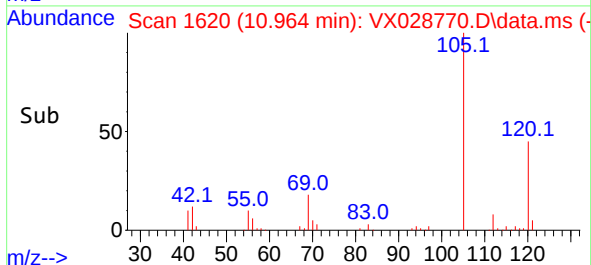







#78
n-propylbenzene
Concen: 2.656 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.001 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

Instrument :
MSVOA_X
ClientSampleId :
31770

Tgt Ion: 91 Resp: 59380
Ion Ratio Lower Upper
91 100
120 21.5 11.6 34.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

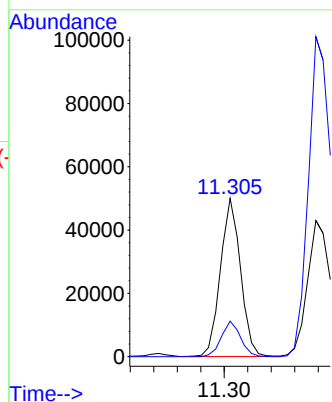

#80
1,3,5-Trimethylbenzene
Concen: 7.950 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02


Tgt Ion:105 Resp: 128007
Ion Ratio Lower Upper
105 100
120 48.2 24.3 72.9

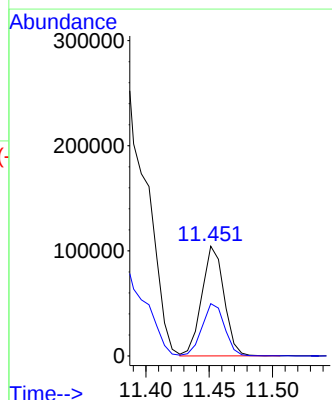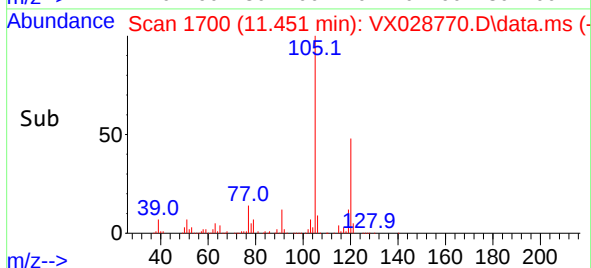



#83
tert-Butylbenzene
Concen: 0.388 ug/l
RT: 11.713 min Scan# 1170
Delta R.T. -0.006 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770

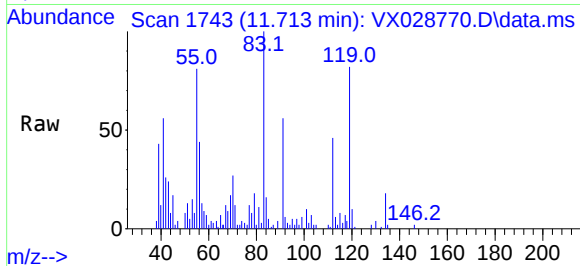


Tgt Ion:119 Resp: 604
Ion Ratio Lower Upper
119 100
91 60.3 26.9 80.6
134 20.1 11.4 34.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022




#84
1,2,4-Trimethylbenzene
Concen: 20.978 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02

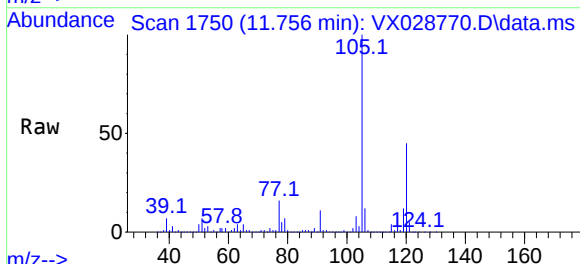

Tgt Ion:105 Resp: 338738
Ion Ratio Lower Upper
105 100
120 44.2 22.6 67.8

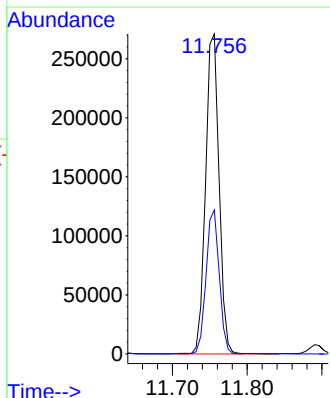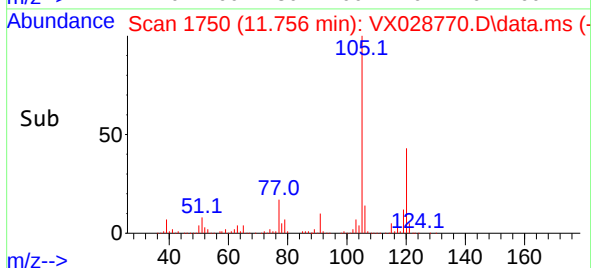







#85
 sec-Butylbenzene
 Concen: 0.530 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX028770.D
 Acq: 17 May 2022 20:02

Instrument :
 MSVOA_X
 ClientSampleId :
 31770

Tgt Ion:105 Resp: 1018
 Ion Ratio Lower Upper
 105 100
 134 14.7 10.2 30.4




Manual Integrations
 APPROVED


Reviewed By :John Carlone 05/18/2022
 Supervised By :Mahesh Dadoda 05/18/2022

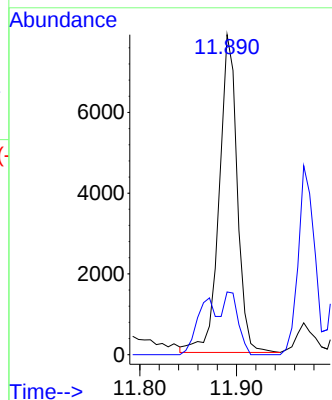

#86
 p-Isopropyltoluene
 Concen: 1.291 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX028770.D
 Acq: 17 May 2022 20:02


Tgt Ion:119 Resp: 20839
 Ion Ratio Lower Upper
 119 100
 134 29.5 13.0 39.0
 91 28.9 11.3 33.9

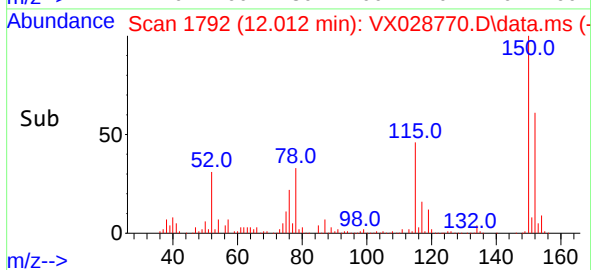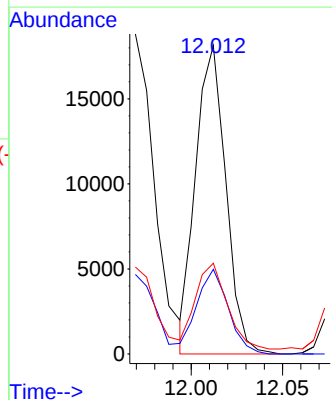



#88
1,4-Dichlorobenzene
Concen: 0.735 ug/l m
RT: 12.043 min Scan# 11
Delta R.T. 0.001 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02




Instrument :
MSVOA_X
ClientSampleId :
31770




Tgt Ion:146 Resp: 683
Ion Ratio Lower Upper
146 100
111 8.3 19.2 57.6
148 9.2 32.3 96.9

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022




#94
Hexachlorobutadiene
Concen: 0.400 ug/l
RT: 13.731 min Scan# 2074
Delta R.T. 0.006 min
Lab File: VX028770.D
Acq: 17 May 2022 20:02



Tgt Ion:225 Resp: 826
Ion Ratio Lower Upper
225 100
223 62.2 34.2 102.5
227 75.3 33.9 101.7

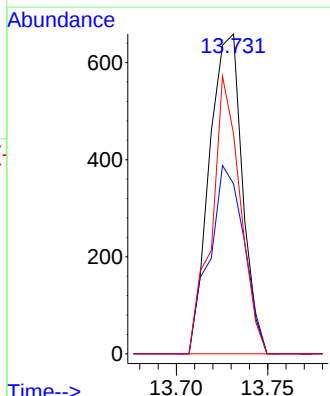

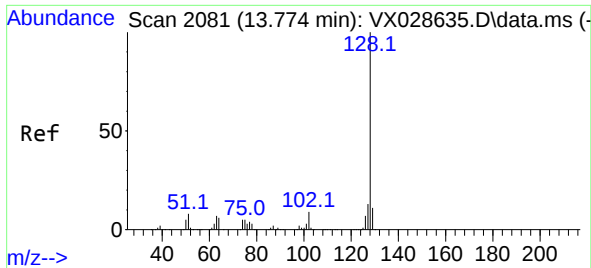

#95

Naphthalene

Concen: 155.336 ug/l

RT: 13.780 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX028770.D


Acq: 17 May 2022 20:02

Instrument :

MSVOA_X

ClientSampleId :

31770

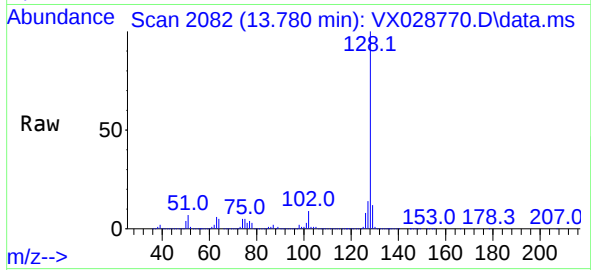

Tgt Ion:128 Resp: 281284

Ion Ratio Lower Upper

128 100

127 13.3 10.2 15.4

129 11.5 8.7 13.1

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/18/2022

Supervised By :Mahesh Dadoda 05/18/2022

