

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051722\
 Data File : VX028781.D
 Acq On : 18 May 2022 01:02
 Operator : JC/MD
 Sample : PB144875TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB144875TB

Quant Time: May 18 04:59:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	349953	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	614749	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	593669	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	282605	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	253076	52.757	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 105.520%	
35) Dibromofluoromethane	5.385	113	204044	50.660	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 101.320%	
50) Toluene-d8	8.653	98	742744	48.912	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 97.820%	
62) 4-Bromofluorobenzene	11.079	95	302453	53.325	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 106.660%	
Target Compounds						Qvalue
16) Acetone	2.380	43	30390	14.761	ug/l	93
20) Methylene Chloride	2.788	84	23777	5.505	ug/l	93
43) Isopropyl Acetate	6.348	43	31792	3.216	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051722\
Data File : VX028781.D
Acq On : 18 May 2022 01:02
Operator : JC/MD
Sample : PB144875TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB144875TB

Quant Time: May 18 04:59:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration




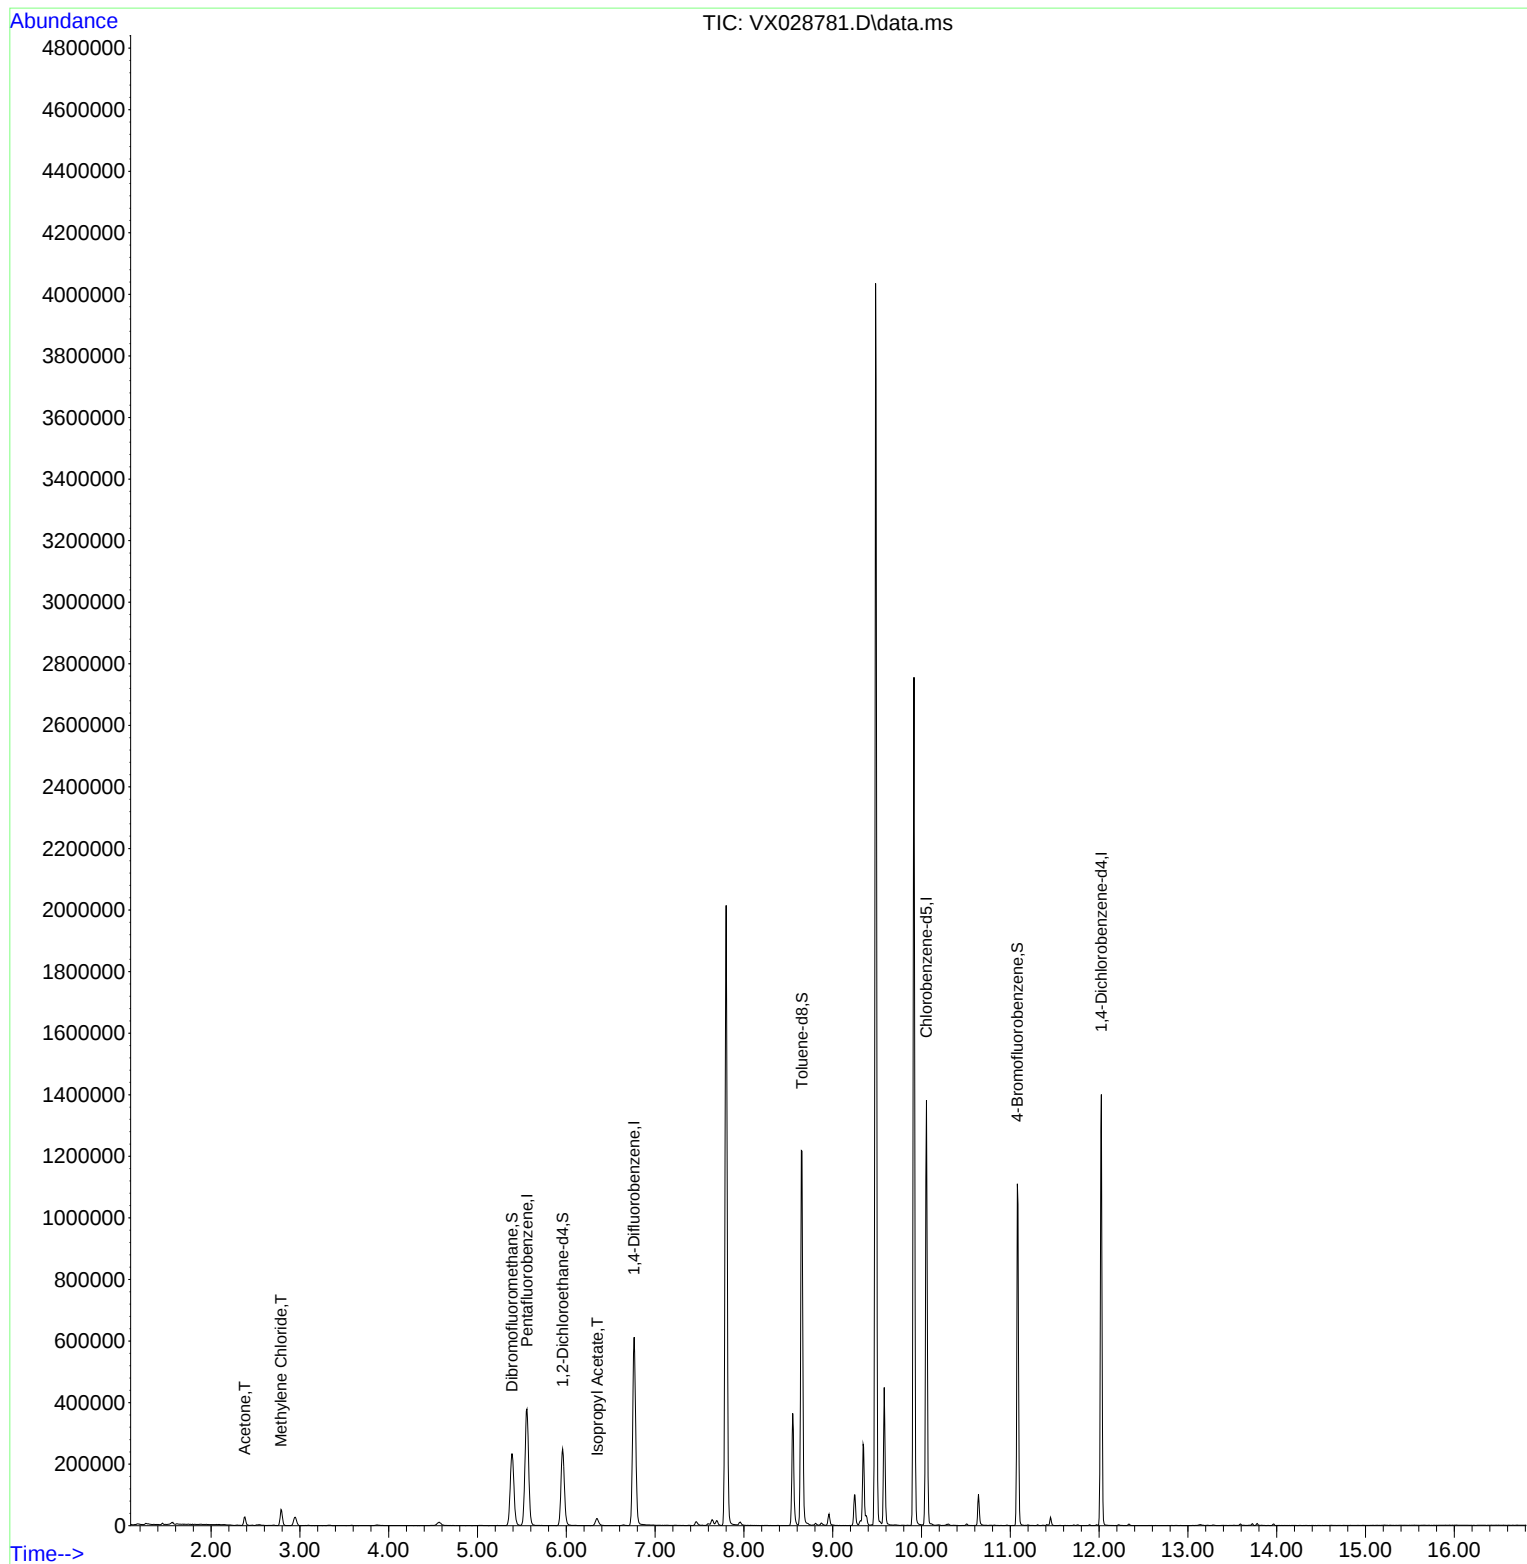


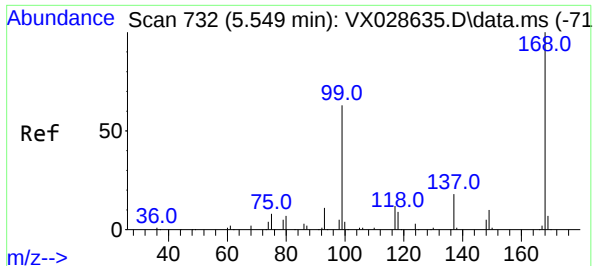

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02




Instrument :
MSVOA_X
ClientSampleId :
PB144875TB


Tgt Ion:168 Resp: 349953
Ion Ratio Lower Upper
168 100
99 62.8 41.7 62.5#

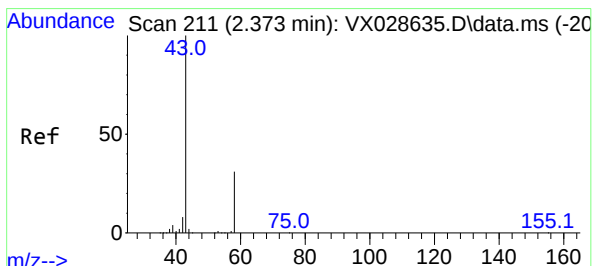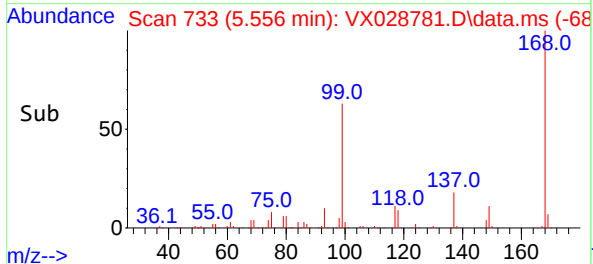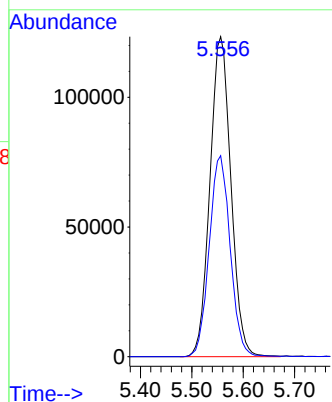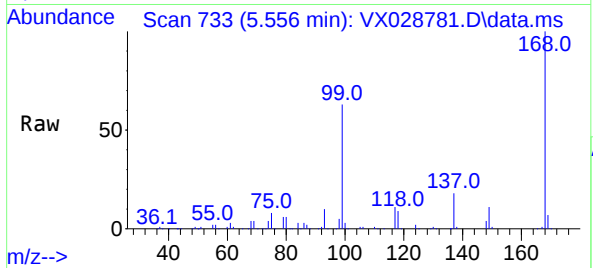

#16
Acetone
Concen: 14.761 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.007 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02

Tgt Ion: 43 Resp: 30390
Ion Ratio Lower Upper
43 100
58 32.0 28.8 43.2

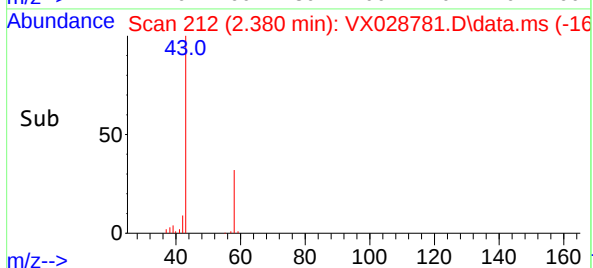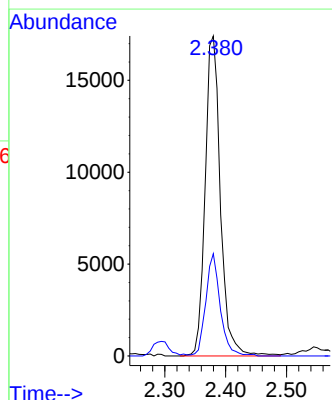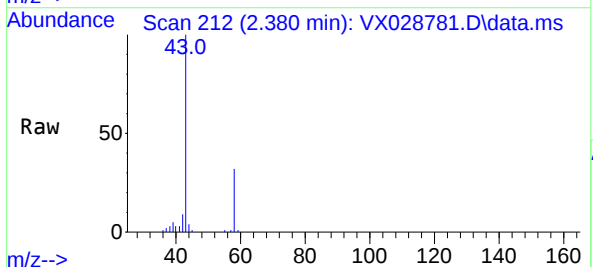




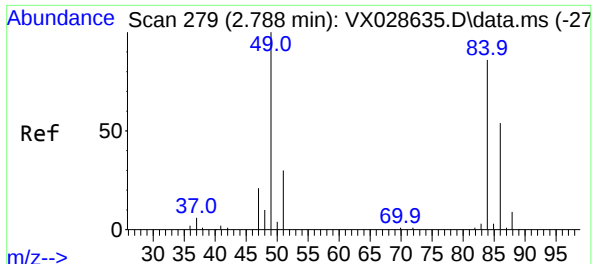


#20
Methylene Chloride
Concen: 5.505 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02

Instrument :
MSVOA_X
ClientSampleId :
PB144875TB

Tgt Ion: 84 Resp: 23777




Ion	Ratio	Lower	Upper
84	100		
49	118.2	85.5	128.3
51	37.0	26.6	39.8
86	63.3	51.5	77.3

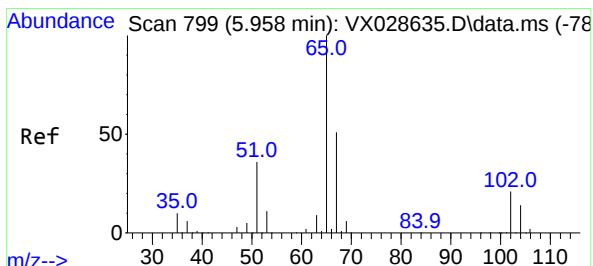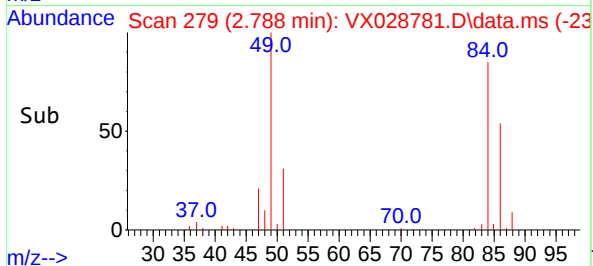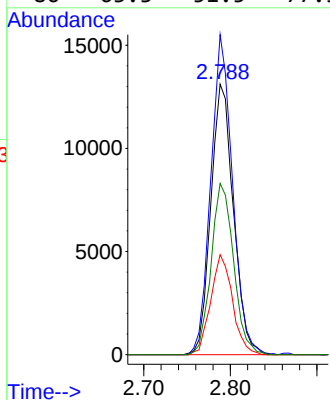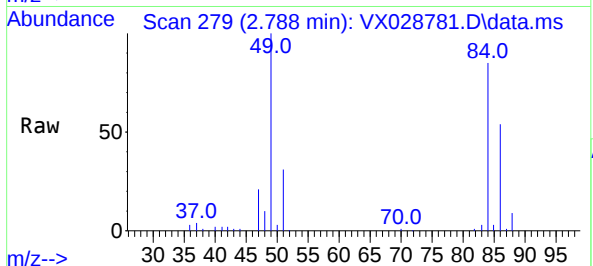


#33
1,2-Dichloroethane-d4
Concen: 52.757 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02

Tgt Ion: 65 Resp: 253076

Ion	Ratio	Lower	Upper
65	100		
67	49.7	0.0	107.4


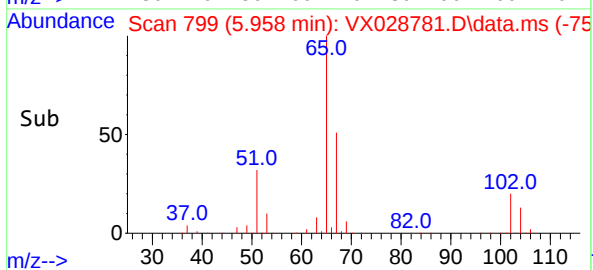
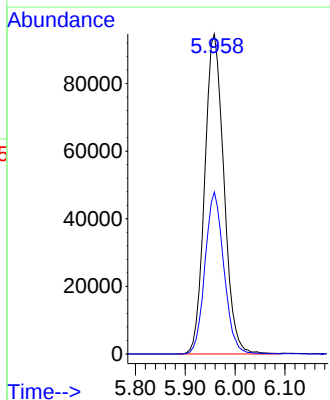
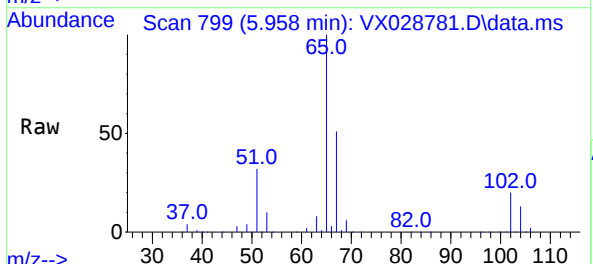


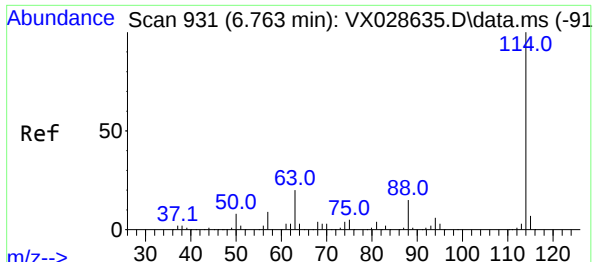

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02




Instrument :
MSVOA_X
ClientSampleId :
PB144875TB


Tgt Ion:114 Resp: 614749
Ion Ratio Lower Upper
114 100
63 20.2 0.0 36.8
88 16.5 0.0 32.4

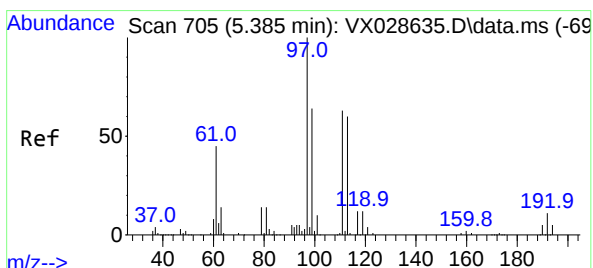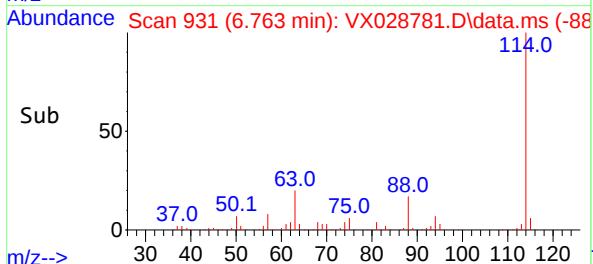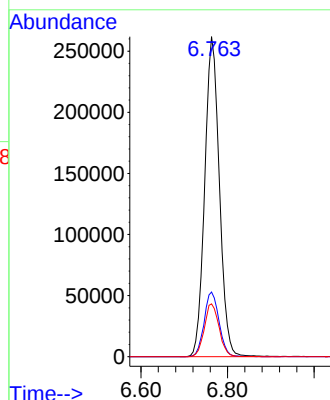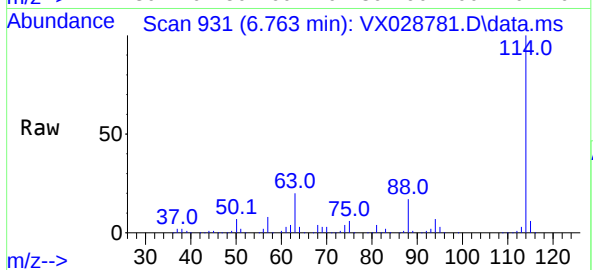

#35
Dibromofluoromethane
Concen: 50.660 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02

Tgt Ion:113 Resp: 204044
Ion Ratio Lower Upper
113 100
111 102.5 82.8 124.2
192 19.1 16.9 25.3


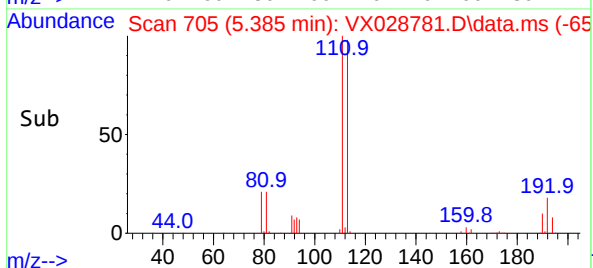
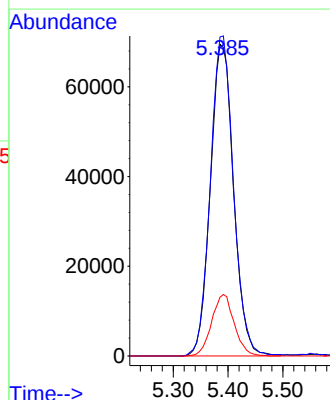
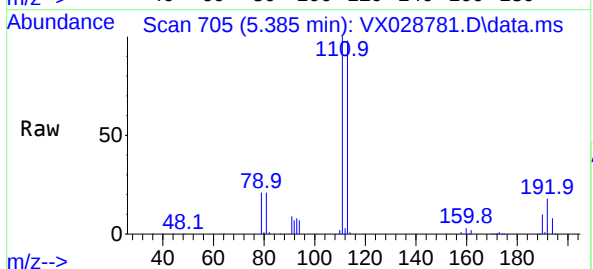


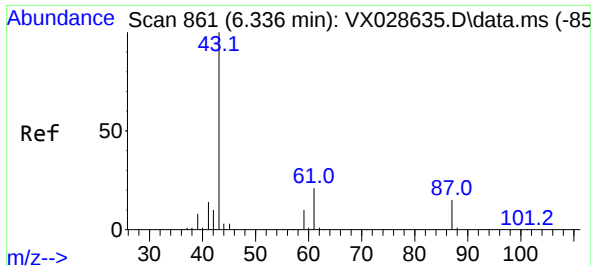

#43
Isopropyl Acetate
Concen: 3.216 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.012 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02




Instrument :
MSVOA_X
ClientSampleId :
PB144875TB


Tgt Ion: 43 Resp: 31792
Ion Ratio Lower Upper
43 100
61 20.7 18.5 27.7
87 14.6 13.0 19.6

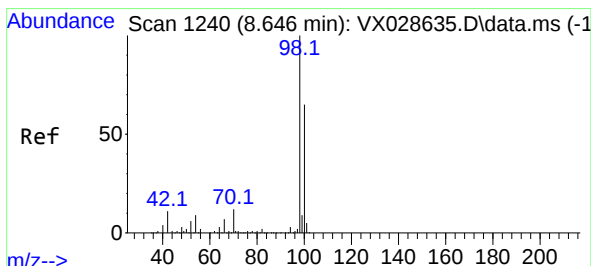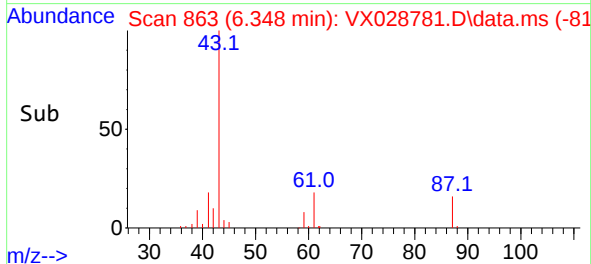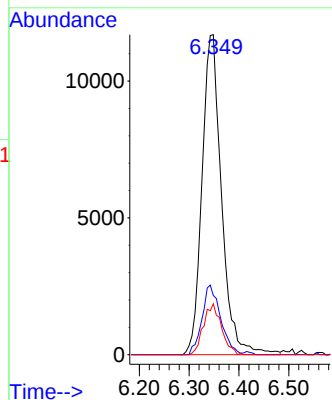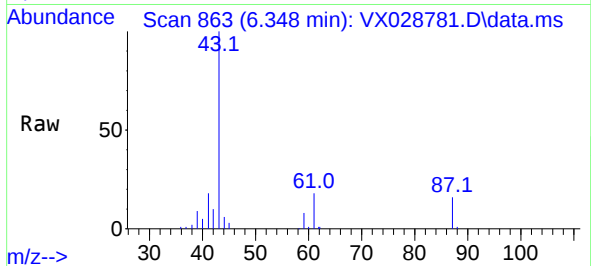

#50
Toluene-d8
Concen: 48.912 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.007 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02

Tgt Ion: 98 Resp: 742744
Ion Ratio Lower Upper
98 100
100 66.6 52.6 78.8


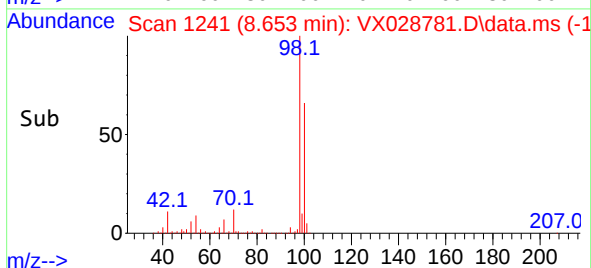
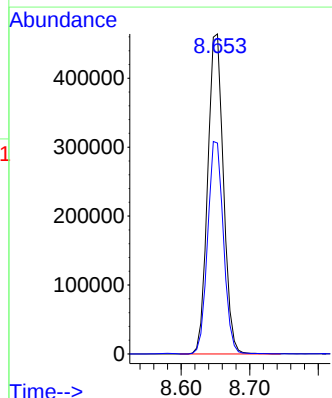
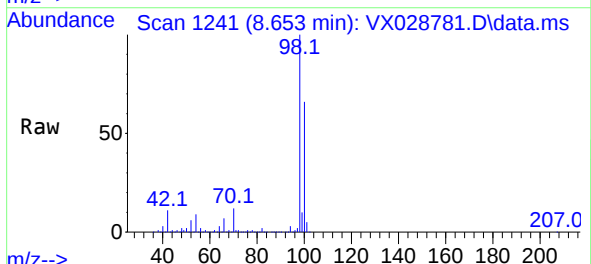


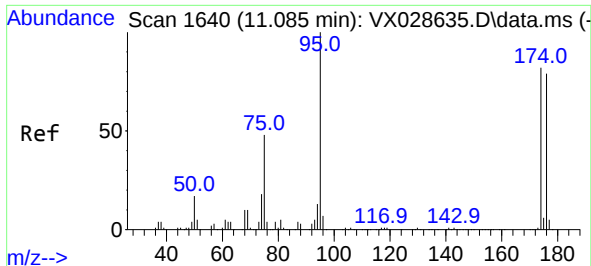

#62
4-Bromofluorobenzene
Concen: 53.325 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02




Instrument :
MSVOA_X
ClientSampleId :
PB144875TB


Tgt Ion: 95 Resp: 302453
Ion Ratio Lower Upper
95 100
174 75.1 0.0 163.0
176 71.8 0.0 155.0

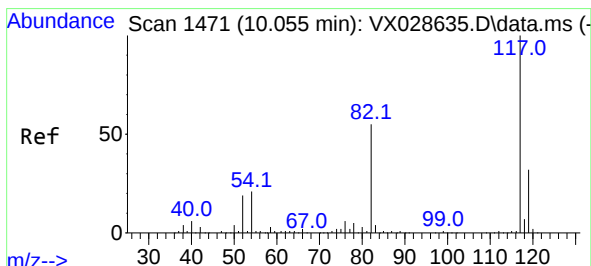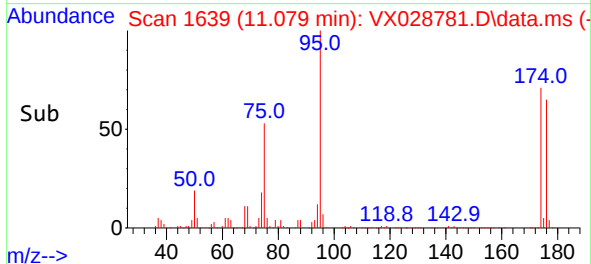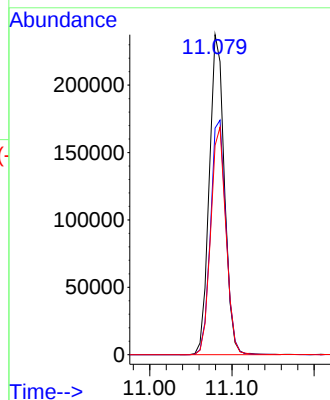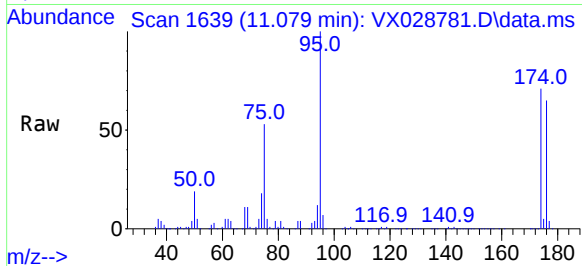

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028781.D
Acq: 18 May 2022 01:02

Tgt Ion: 117 Resp: 593669
Ion Ratio Lower Upper
117 100
82 56.8 41.8 62.8
119 32.2 24.8 37.2

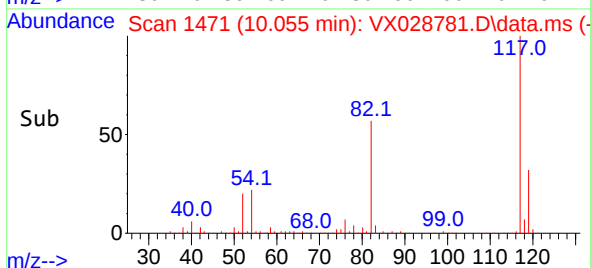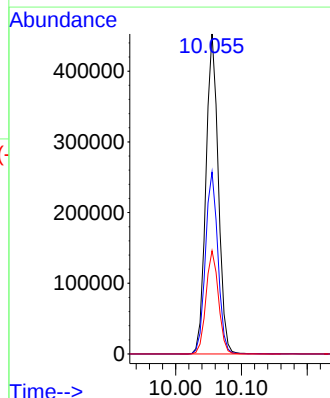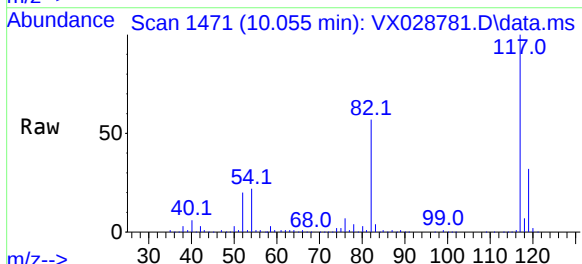

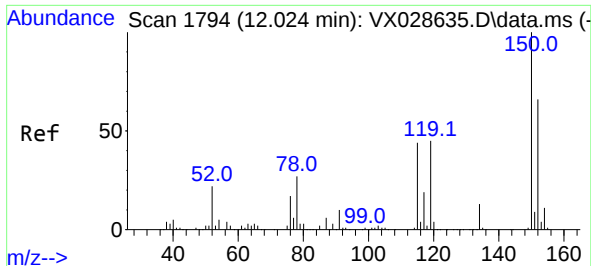

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX028781.D


Acq: 18 May 2022 01:02

Instrument :

MSVOA_X

ClientSampleId :

PB144875TB

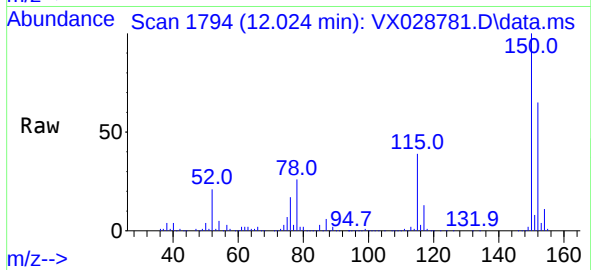

Tgt Ion:152 Resp: 282605

Ion Ratio Lower Upper

152 100

115 62.3 37.5 112.7

150 156.5 0.0 338.2

