

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051722\
 Data File : VX028789.D
 Acq On : 18 May 2022 04:09
 Operator : JC/MD
 Sample : N2879-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-4-0516

Quant Time: May 18 07:15:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	329626	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	586244	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	557758	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	263105	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	239203	52.940	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 105.880%	
35) Dibromofluoromethane	5.391	113	195085	50.790	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 101.580%	
50) Toluene-d8	8.653	98	699111	48.277	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 96.560%	
62) 4-Bromofluorobenzene	11.079	95	280686	51.894	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 103.780%	
Target Compounds						Qvalue
16) Acetone	2.380	43	34399	17.739	ug/l	92
20) Methylene Chloride	2.794	84	20473	5.032	ug/l	95
43) Isopropyl Acetate	6.348	43	24765	2.627	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051722\
Data File : VX028789.D
Acq On : 18 May 2022 04:09
Operator : JC/MD
Sample : N2879-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-4-0516

Quant Time: May 18 07:15:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration



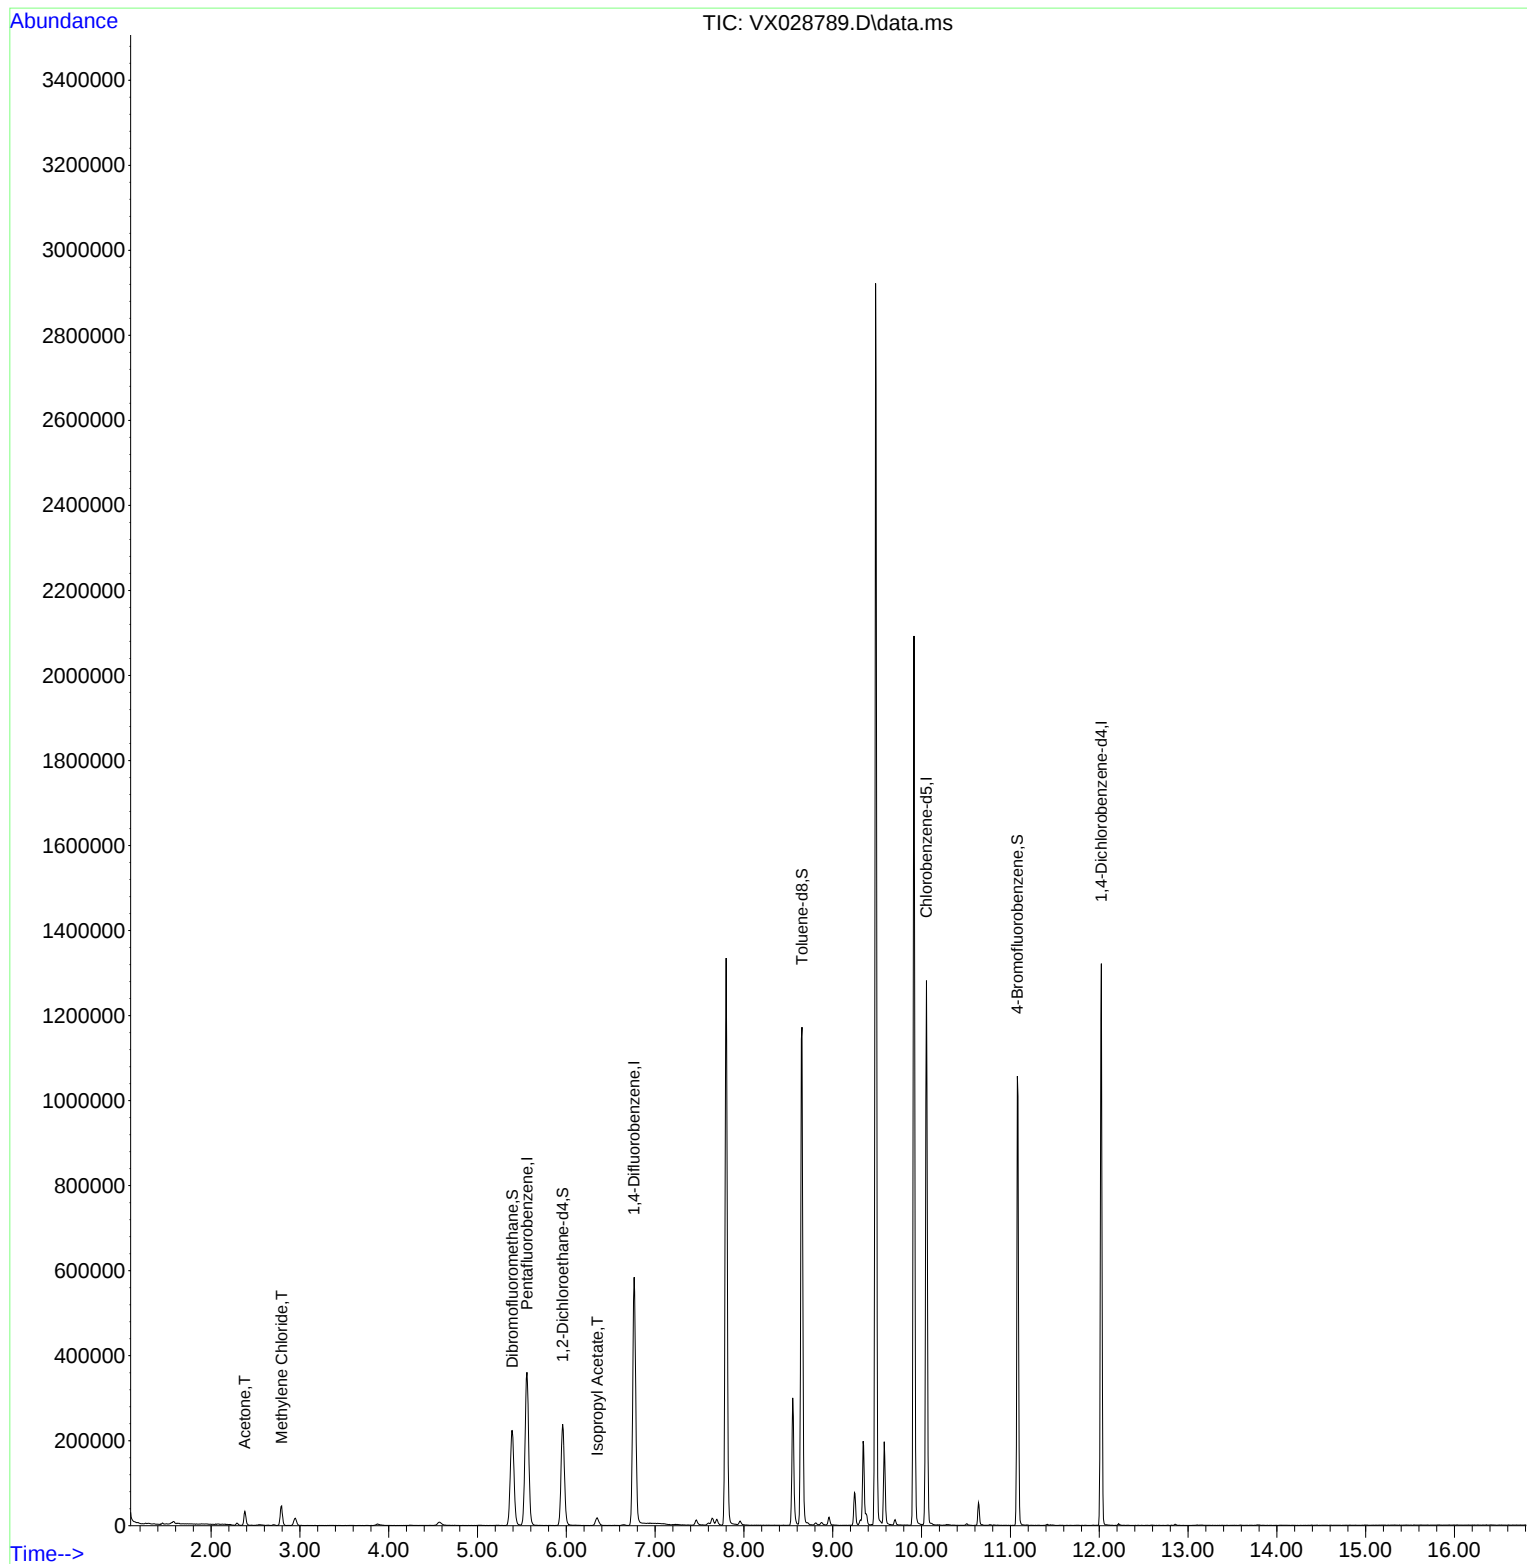


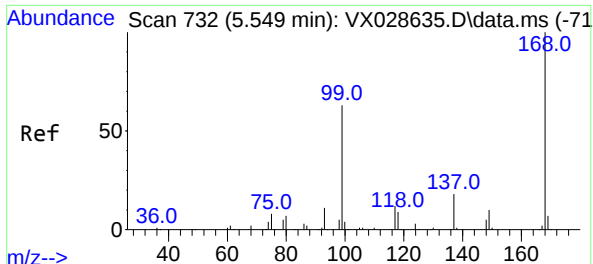

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09




Instrument :
MSVOA_X
ClientSampleId :
TP-4-0516


Tgt Ion:168 Resp: 329626
Ion Ratio Lower Upper
168 100
99 63.2 41.7 62.5#

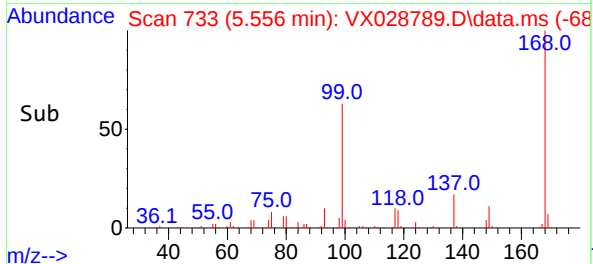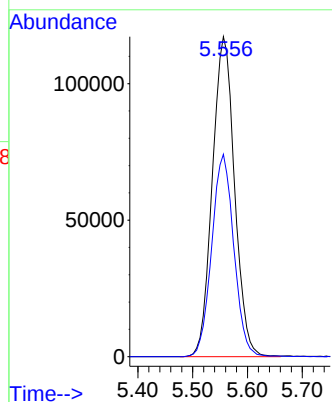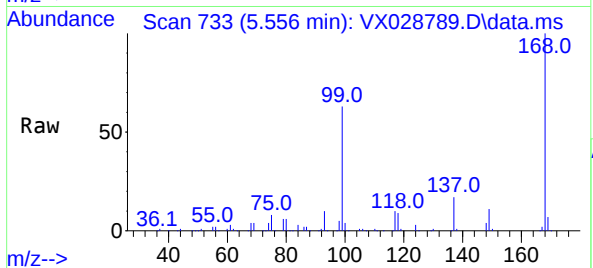

#16
Acetone
Concen: 17.739 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.007 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09

Tgt Ion: 43 Resp: 34399
Ion Ratio Lower Upper
43 100
58 31.4 28.8 43.2

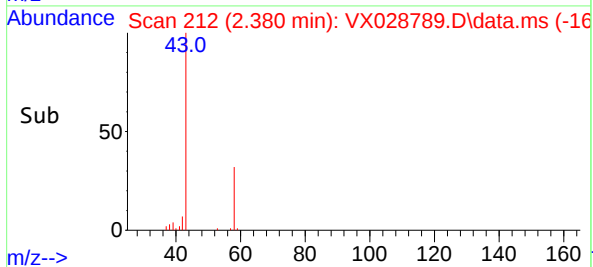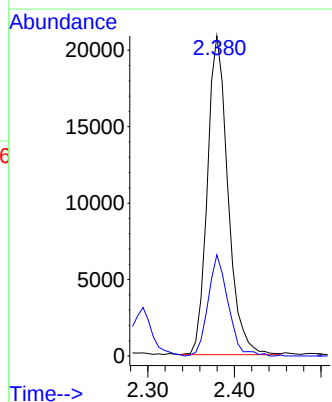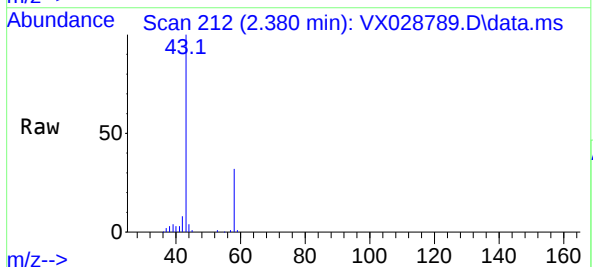




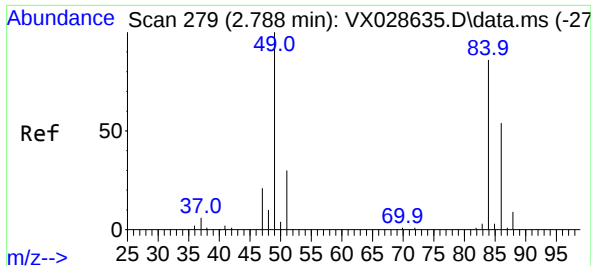


#20
Methylene Chloride
Concen: 5.032 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09

Instrument :
MSVOA_X
ClientSampleId :
TP-4-0516

Tgt Ion: 84 Resp: 20473




Ion	Ratio	Lower	Upper
84	100		
49	113.6	85.5	128.3
51	37.3	26.6	39.8
86	64.3	51.5	77.3

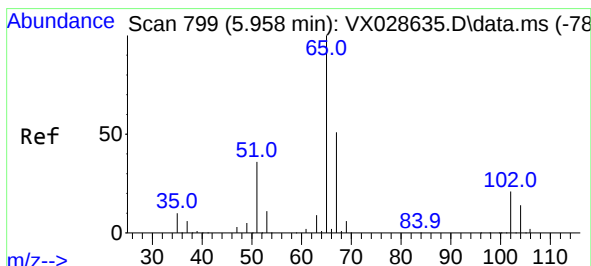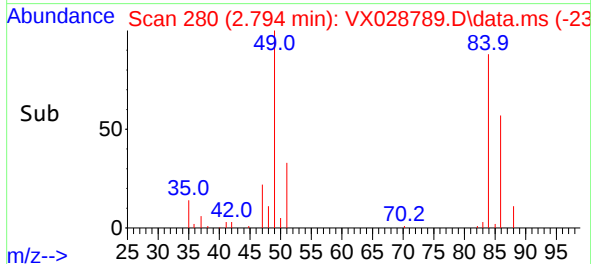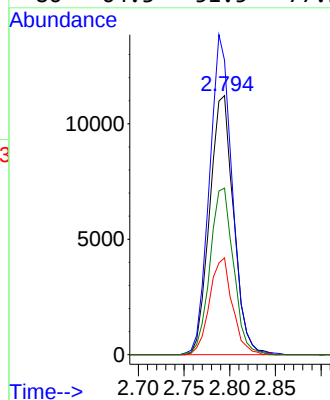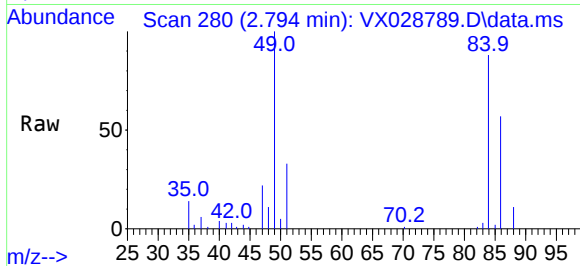


#33
1,2-Dichloroethane-d4
Concen: 52.940 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09

Tgt Ion: 65 Resp: 239203

Ion	Ratio	Lower	Upper
65	100		
67	49.6	0.0	107.4


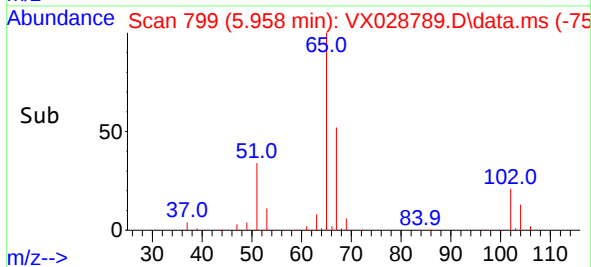
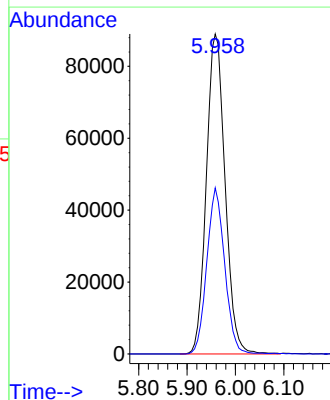
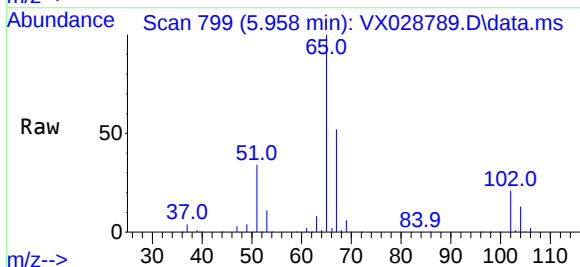


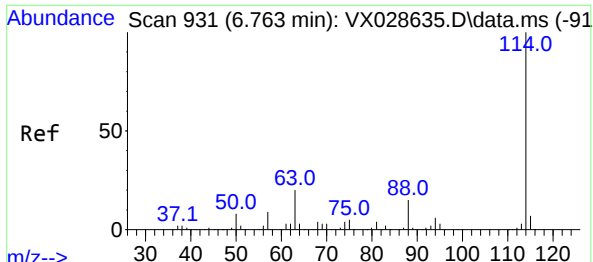

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09




Instrument :
MSVOA_X
ClientSampleId :
TP-4-0516


Tgt Ion:114 Resp: 586244
Ion Ratio Lower Upper
114 100
63 19.4 0.0 36.8
88 16.0 0.0 32.4

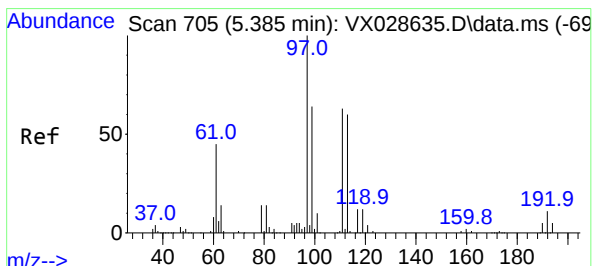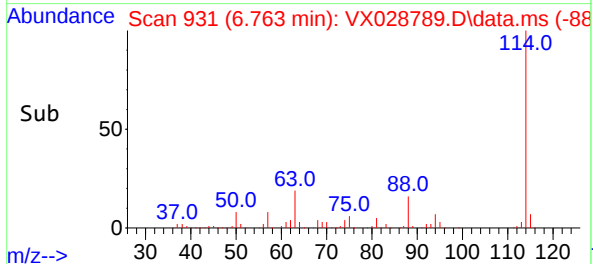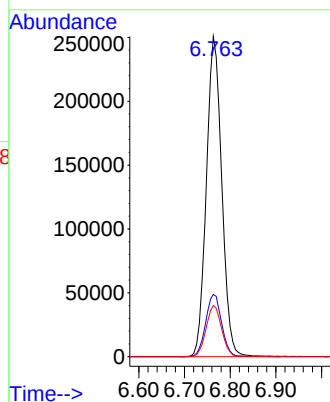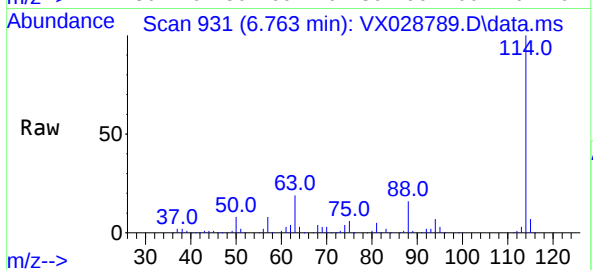

#35
Dibromofluoromethane
Concen: 50.790 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09

Tgt Ion:113 Resp: 195085
Ion Ratio Lower Upper
113 100
111 103.3 82.8 124.2
192 18.7 16.9 25.3


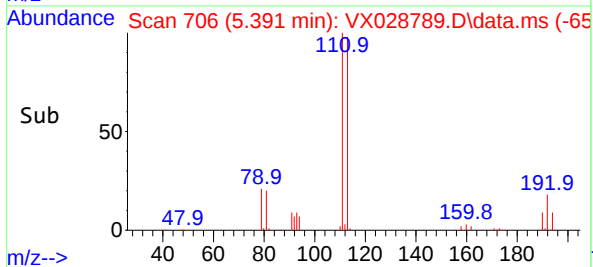
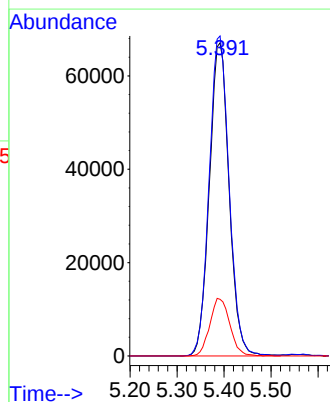
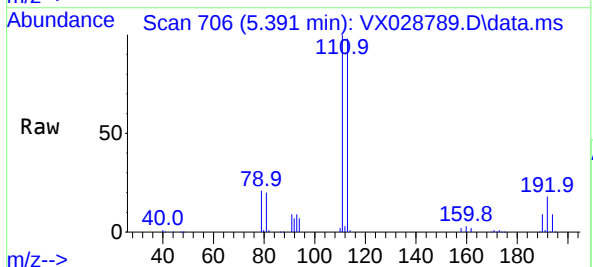


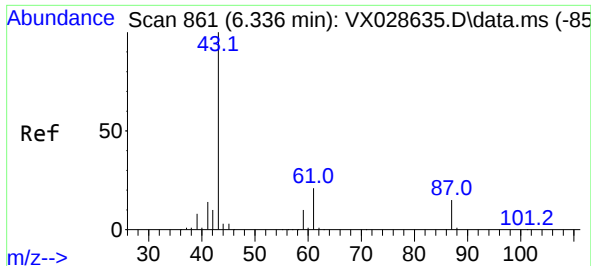

#43
Isopropyl Acetate
Concen: 2.627 ug/l
RT: 6.348 min Scan# 80
Delta R.T. 0.012 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09




Instrument :
MSVOA_X
ClientSampleId :
TP-4-0516


Tgt Ion: 43 Resp: 24765
Ion Ratio Lower Upper
43 100
61 21.2 18.5 27.7
87 15.3 13.0 19.6

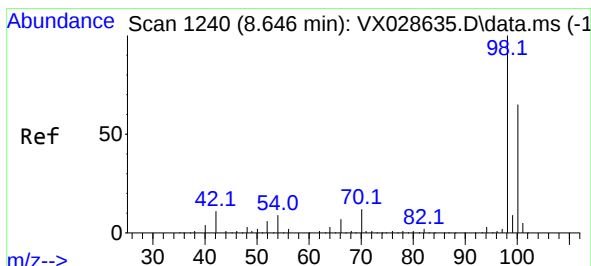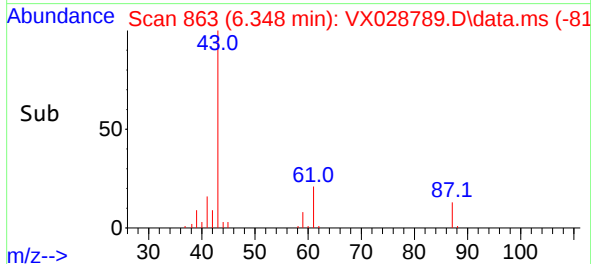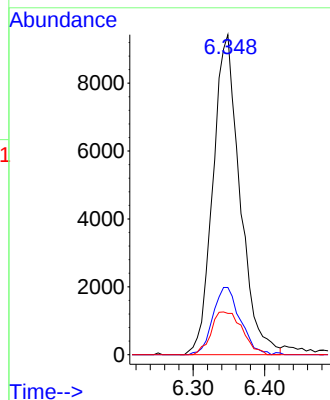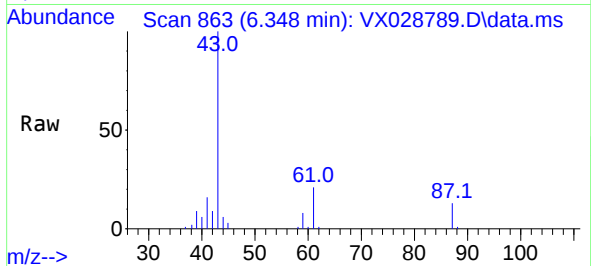

#50
Toluene-d8
Concen: 48.277 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.007 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09

Tgt Ion: 98 Resp: 699111
Ion Ratio Lower Upper
98 100
100 65.8 52.6 78.8


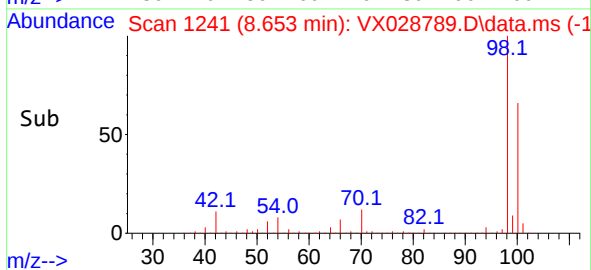
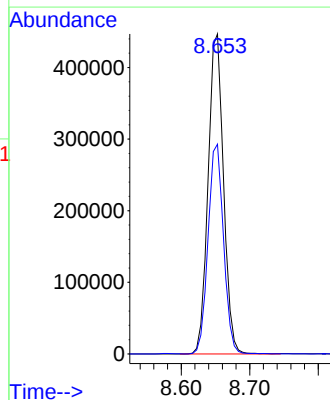
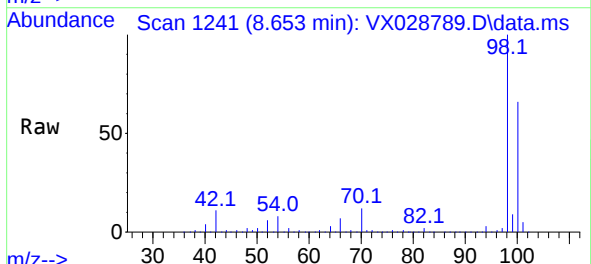


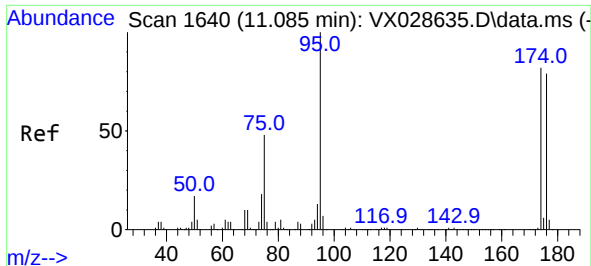

#62
4-Bromofluorobenzene
Concen: 51.894 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09




Instrument :
MSVOA_X
ClientSampleId :
TP-4-0516


Tgt Ion: 95 Resp: 280686
Ion Ratio Lower Upper
95 100
174 75.3 0.0 163.0
176 72.8 0.0 155.0

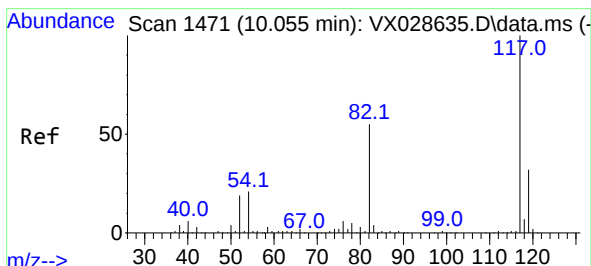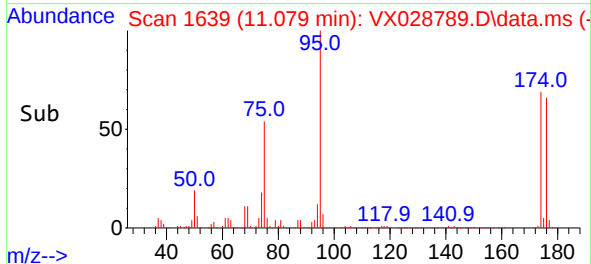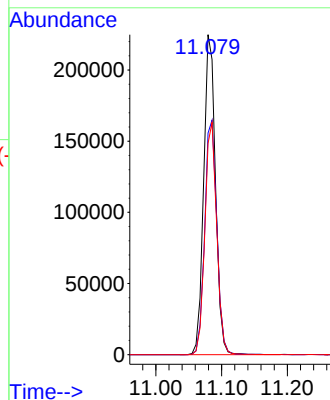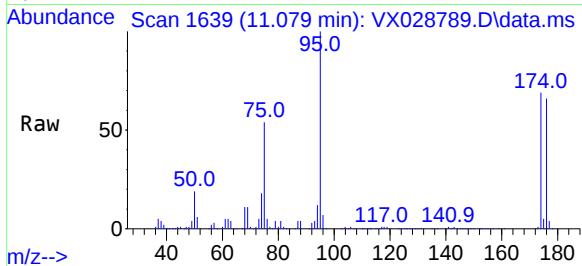

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09


Tgt Ion: 117 Resp: 557758
Ion Ratio Lower Upper
117 100
82 57.6 41.8 62.8
119 32.4 24.8 37.2

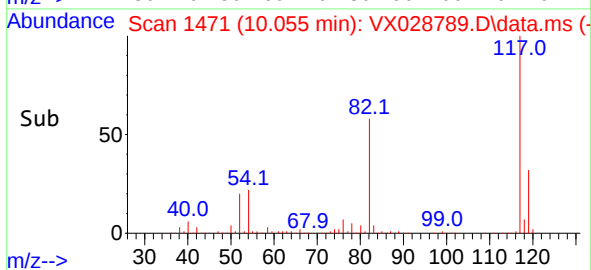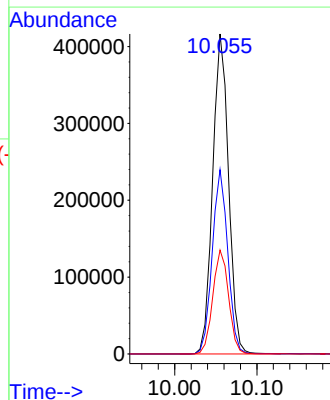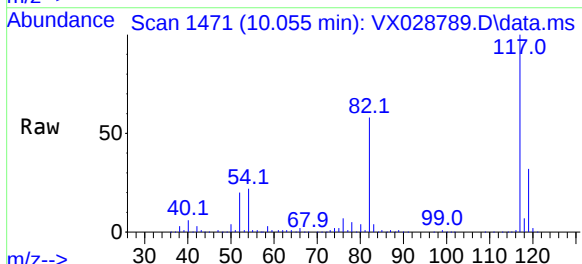

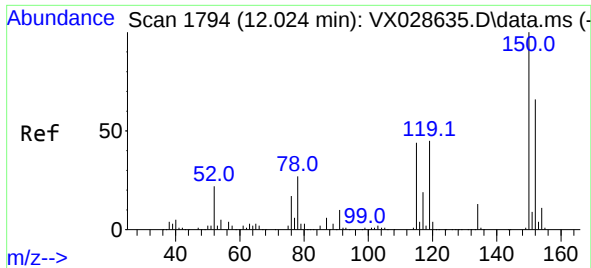

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028789.D
Acq: 18 May 2022 04:09

Instrument :
MSVOA_X
ClientSampleId :
TP-4-0516

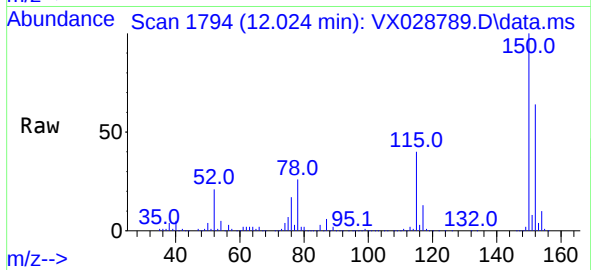

Tgt Ion:152 Resp: 263105
Ion Ratio Lower Upper
152 100
115 62.5 37.5 112.7
150 157.3 0.0 338.2

