


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051722\
Data File : VX028776.D
Acq On : 17 May 2022 22:43
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Title : SW846 8260
Last Update : Thu May 12 14:58:53 2022

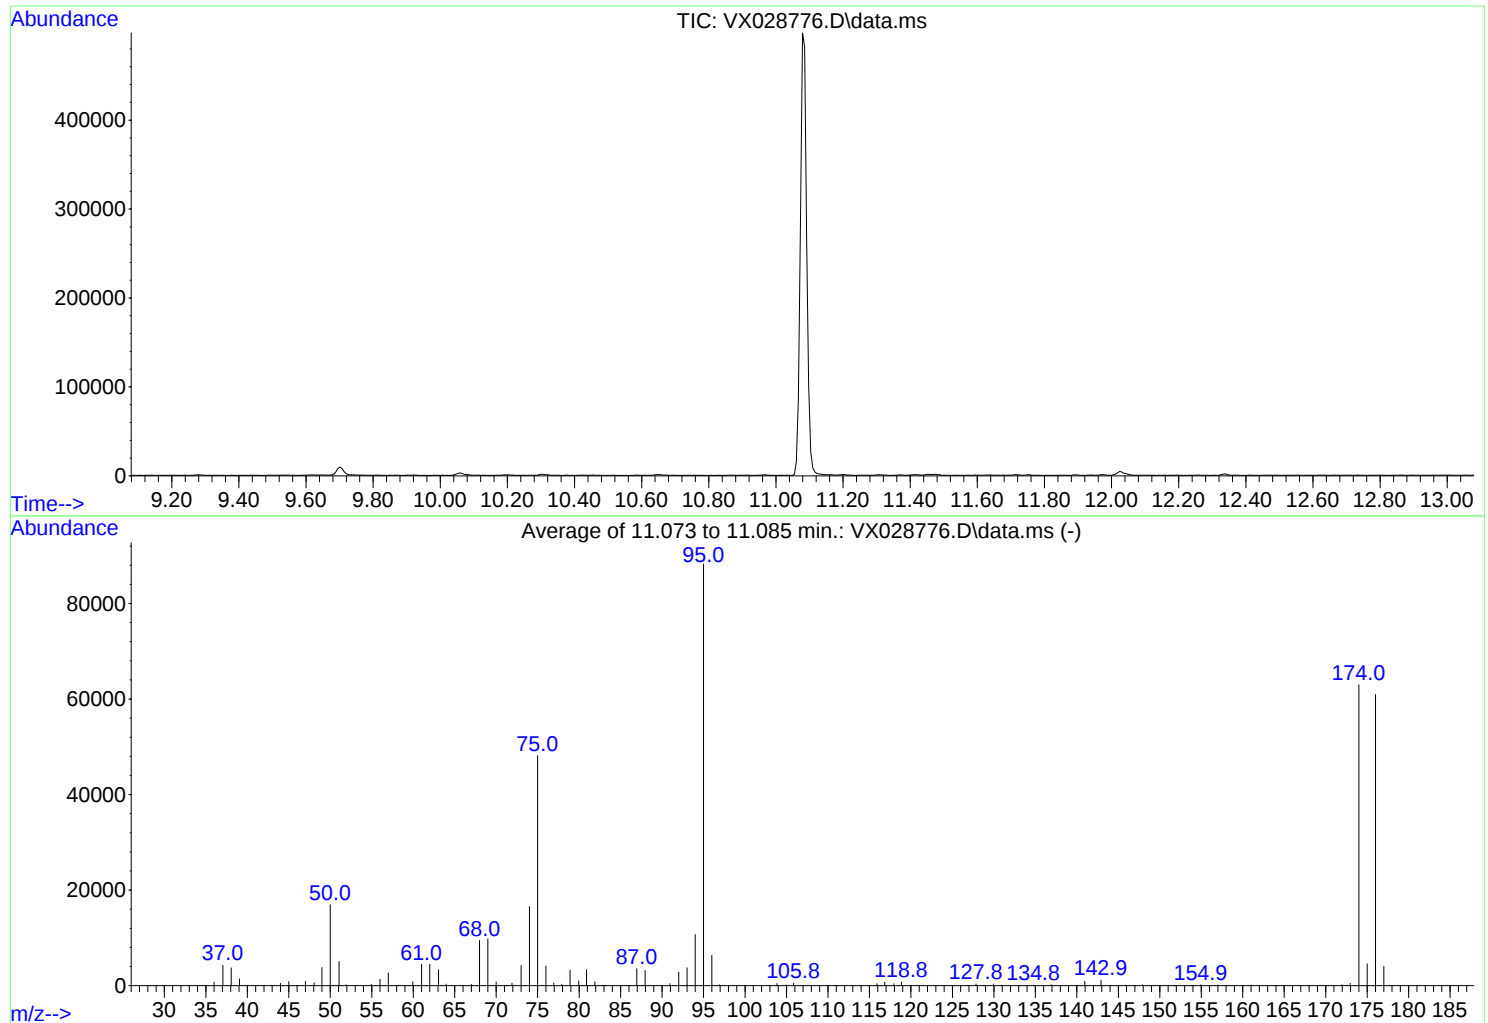

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	16950	PASS
75	95	30	60	54.5	48123	PASS
95	95	100	100	100.0	88299	PASS
96	95	5	9	7.2	6350	PASS
173	174	0.00	2	0.7	468	PASS
174	95	50	100	71.3	62984	PASS
175	174	5	9	7.2	4563	PASS
176	174	95	101	96.8	60963	PASS
177	176	5	9	6.7	4064	PASS