

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051723\
 Data File : VX035709.D
 Acq On : 17 May 2023 11:42
 Operator : JC/MD
 Sample : 02631-01RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GWOW-07B-24-29-050423

Quant Time: May 18 04:40:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 11 13:57:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	196406	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	359429	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	333216	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	146266	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	165555	48.318	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.640%
35) Dibromofluoromethane	5.385	113	117929	48.651	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.300%
50) Toluene-d8	8.647	98	437918	48.903	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.800%
62) 4-Bromofluorobenzene	11.079	95	178374	49.472	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.940%


Target Compounds				Qvalue		
2) Dichlorodifluoromethane	1.142	85	1133	0.443	ug/l	95
4) Vinyl Chloride	1.374	62	1504	0.571	ug/l	91
9) 1,1,2-Trichlorotrifluo...	2.325	101	647	0.281	ug/l #	23
11) Tert butyl alcohol	2.934	59	2097	3.469	ug/l #	73
12) 1,1-Dichloroethene	2.325	96	146655	67.051	ug/l	89
13) Acrolein	2.239	56	256	0.357	ug/l #	80
15) Acrylonitrile	3.087	53	408	0.307	ug/l #	78
16) Acetone	2.398	43	2515	1.708	ug/l	89
17) Carbon Disulfide	2.514	76	1635	0.310	ug/l #	94
20) Methylene Chloride	2.794	84	704	0.264	ug/l #	90
21) trans-1,2-Dichloroethene	3.093	96	14149	5.904	ug/l	98
24) 1,1-Dichloroethane	3.611	63	30741	6.265	ug/l	99
25) 2-Butanone	4.574	43	1957	0.960	ug/l #	85
26) 2,2-Dichloropropane	4.568	77	834	0.201	ug/l #	53
27) cis-1,2-Dichloroethene	4.489	96	141683	49.176	ug/l	95
29) Tetrahydrofuran	5.025	42	1034	0.807	ug/l #	81
30) Chloroform	5.092	83	11294	2.246	ug/l	94
31) Cyclohexane	5.550	56	5171	1.195	ug/l #	7
36) 1,1-Dichloropropene	5.550	75	18716	4.892	ug/l #	51
38) Carbon Tetrachloride	5.550	117	22767	6.281	ug/l #	15
40) Benzene	6.037	78	3328	0.311	ug/l	97
41) Methacrylonitrile	5.025	41	747	0.315	ug/l #	39
42) 1,2-Dichloroethane	6.092	62	20757	4.508	ug/l	98
44) Trichloroethene	7.129	130	142142	52.373	ug/l	94
49) 1,4-Dioxane	7.708	88	5158	70.052	ug/l #	84
76) 1,2,3-Trichloropropane	11.079	75	98956	27.659	ug/l #	34
81) trans-1,4-Dichloro-2-b...	11.079	75	98956	89.141	ug/l #	8
91) 1,2-Dichlorobenzene	12.335	146	1300	0.250	ug/l	86
93) 1,2,4-Trichlorobenzene	13.591	180	1224	0.391	ug/l	97
94) Hexachlorobutadiene	13.725	225	744	0.598	ug/l	91
95) Naphthalene	13.774	128	2965	0.276	ug/l #	94
96) 1,2,3-Trichlorobenzene	13.963	180	1152	0.374	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051723\
Data File : VX035709.D
Acq On : 17 May 2023 11:42
Operator : JC/MD
Sample : 02631-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423

Quant Time: May 18 04:40:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260
QLast Update : Thu May 11 13:57:54 2023
Response via : Initial Calibration




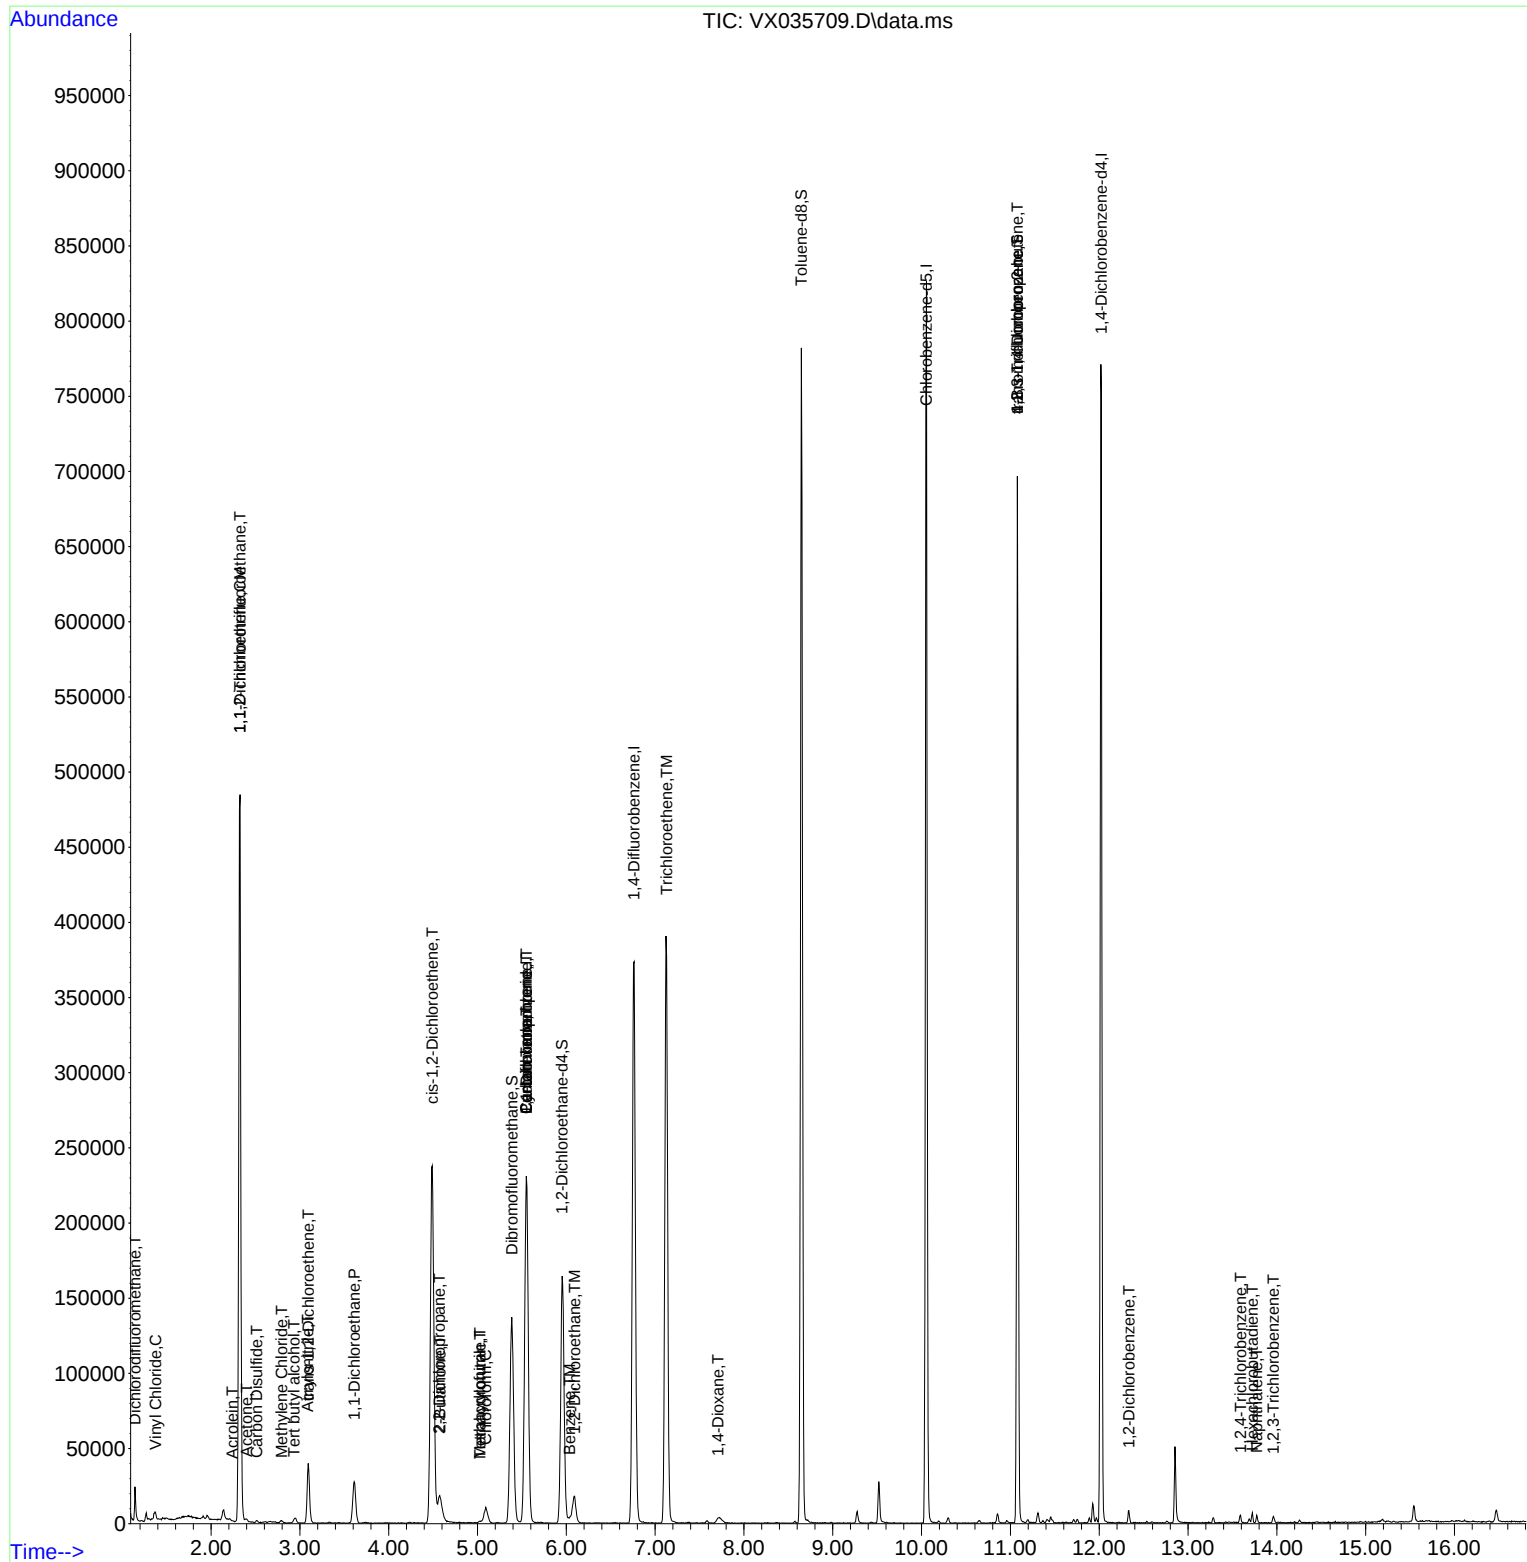


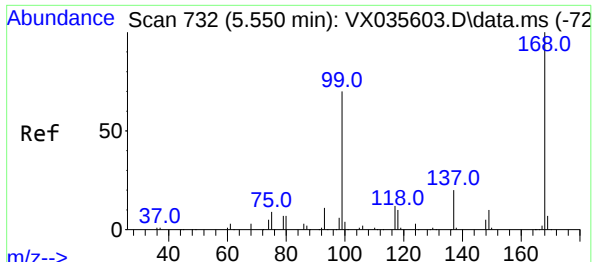

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument : MSVOA_X
ClientSampleId : GWOW-07B-24-29-050423

Tgt Ion:168 Resp: 196406
Ion Ratio Lower Upper
168 100
99 70.5 45.7 68.5#

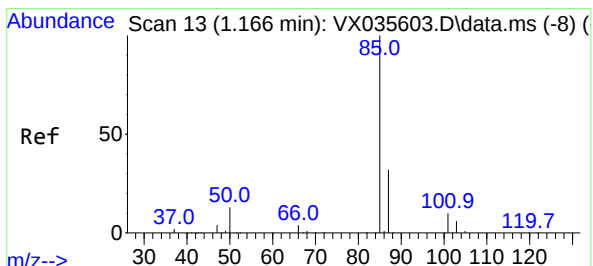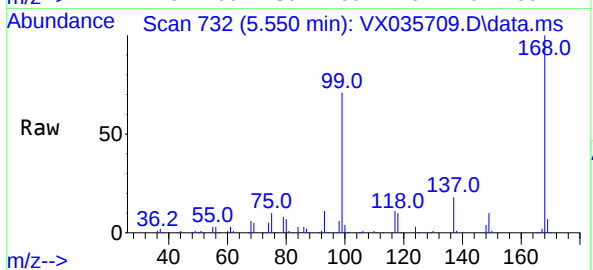


#2
Dichlorodifluoromethane
Concen: 0.443 ug/l
RT: 1.142 min Scan# 9
Delta R.T. -0.024 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 85 Resp: 1133
Ion Ratio Lower Upper
85 100
87 29.8 16.4 49.1

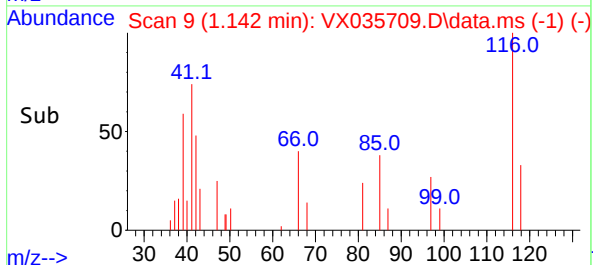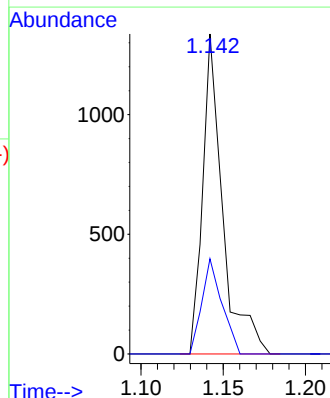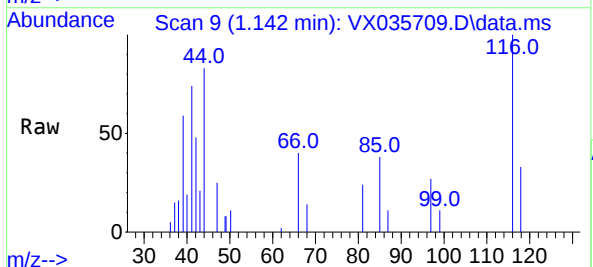





Abundance Scan 47 (1.374 min): VX035603.D\data.ms (-42)

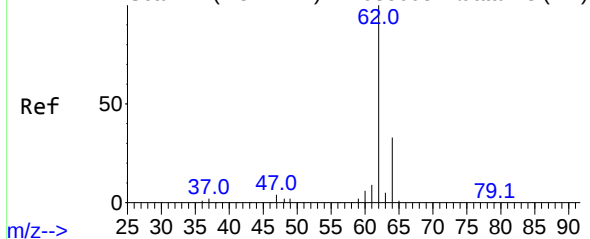

#4
Vinyl Chloride
Concen: 0.571 ug/l
RT: 1.374 min Scan# 41
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 62 Resp: 1504
Ion Ratio Lower Upper
62 100
64 28.2 26.4 39.6

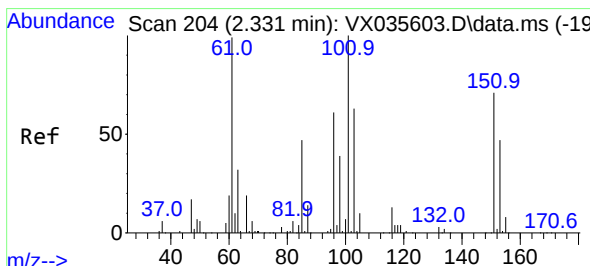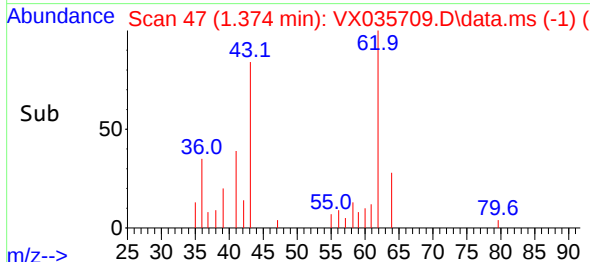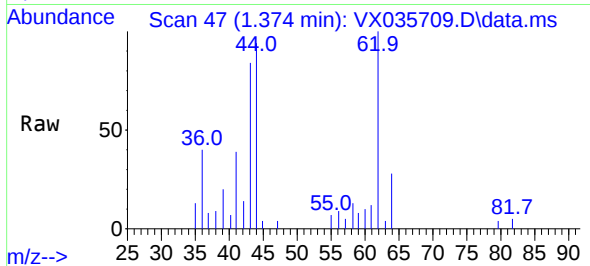

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.281 ug/l
RT: 2.325 min Scan# 203
Delta R.T. -0.006 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 101 Resp: 647
Ion Ratio Lower Upper
101 100
85 6.8 35.4 53.2#
151 0.0 60.2 90.4#

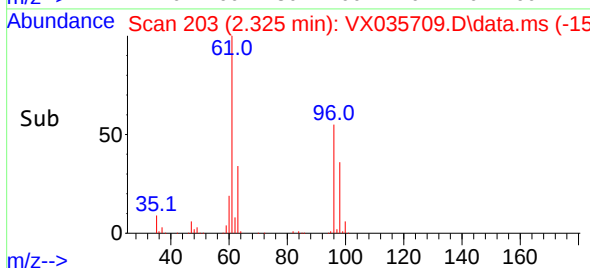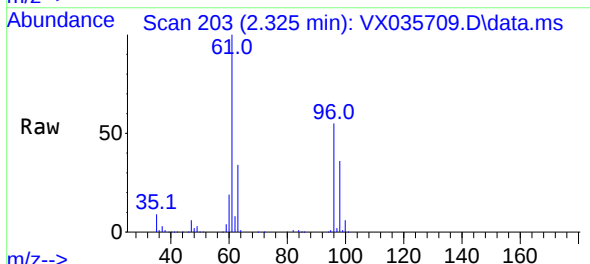



#11

Tert butyl alcohol

Concen: 3.469 ug/l

RT: 2.934 min Scan# 30

Delta R.T. -0.067 min

Lab File: VX035709.D


Acq: 17 May 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :

GWOW-07B-24-29-050423






Tgt Ion: 59 Resp: 2097

Ion Ratio Lower Upper

59 100

57 0.0 8.1 12.1#

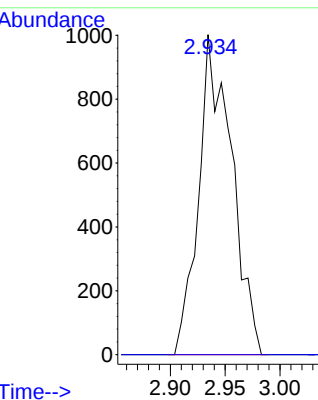

#12

1,1-Dichloroethene

Concen: 67.051 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.006 min

Lab File: VX035709.D

Acq: 17 May 2023 11:42




Tgt Ion: 96 Resp: 146655


Ion Ratio Lower Upper

96 100

61 180.8 128.8 193.2

98 65.7 51.4 77.0


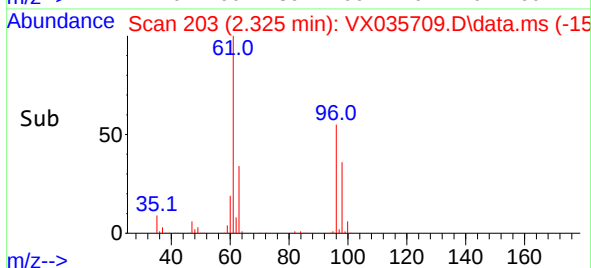
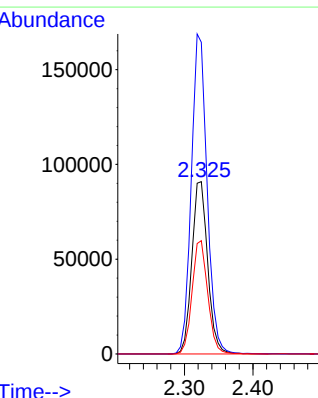





#13
Acrolein
Concen: 0.357 ug/l
RT: 2.239 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 56 Resp: 256
Ion Ratio Lower Upper
56 100
55 87.1 56.6 85.0#



#15
Acrylonitrile
Concen: 0.307 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.019 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 53 Resp: 408
Ion Ratio Lower Upper
53 100
52 77.5 66.2 99.2
51 0.0 28.3 42.5#


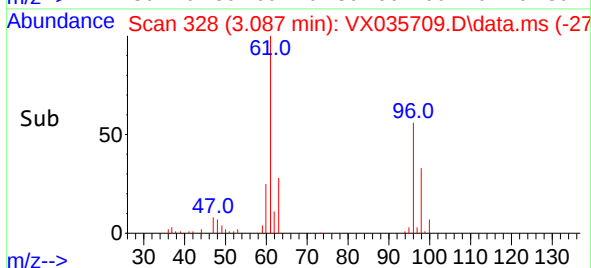
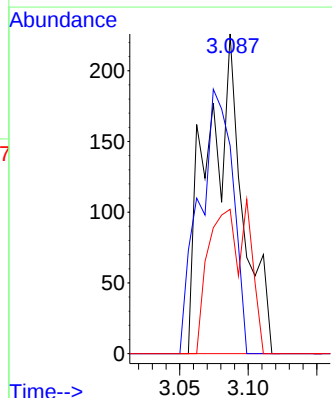





#16
Acetone
Concen: 1.708 ug/l
RT: 2.398 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 43 Resp: 2515
Ion Ratio Lower Upper
43 100
58 36.9 24.7 37.1

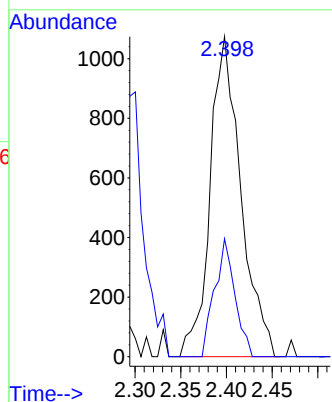

#17
Carbon Disulfide
Concen: 0.310 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 76 Resp: 1635
Ion Ratio Lower Upper
76 100
78 6.8 7.2 10.8#

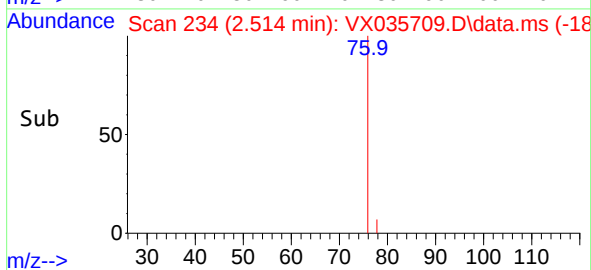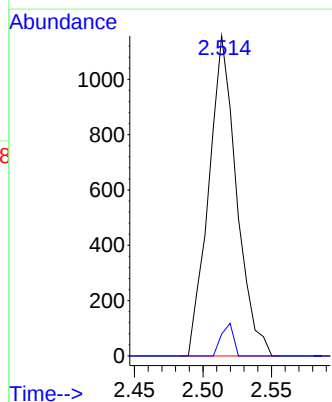







#20
Methylene Chloride
Concen: 0.264 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423

Tgt Ion: 84 Resp: 704




Ion	Ratio	Lower	Upper
84	100		
49	138.4	103.8	155.8
51	40.4	31.8	47.8
86	81.9	51.4	77.2

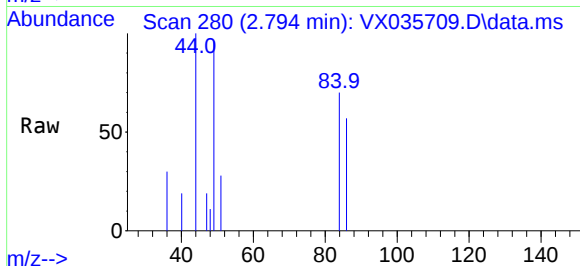


#21
trans-1,2-Dichloroethene
Concen: 5.904 ug/l
RT: 3.093 min Scan# 329
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 96 Resp: 14149

Ion	Ratio	Lower	Upper
96	100		
61	144.8	113.0	169.6
98	64.3	52.1	78.1


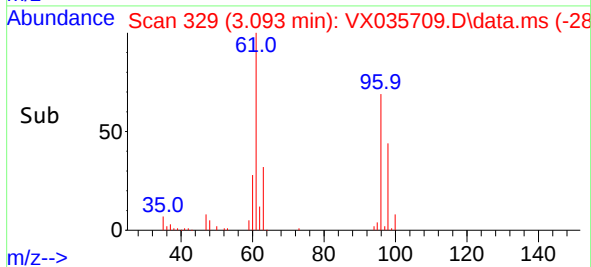

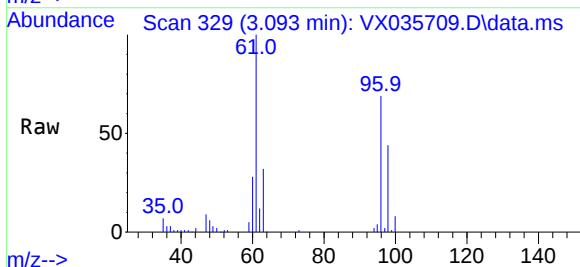




#24
1,1-Dichloroethane
Concen: 6.265 ug/l
RT: 3.611 min Scan# 414
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 63 Resp: 30741
Ion Ratio Lower Upper
63 100
98 7.3 3.8 11.2
100 5.6 2.4 7.1

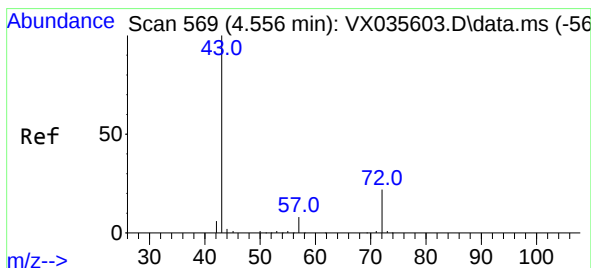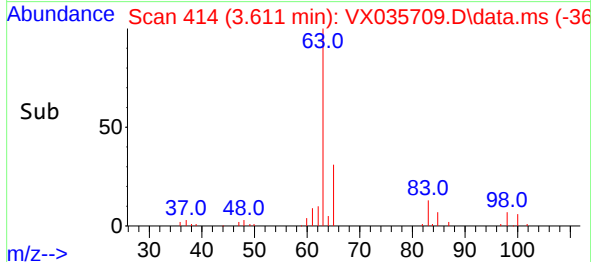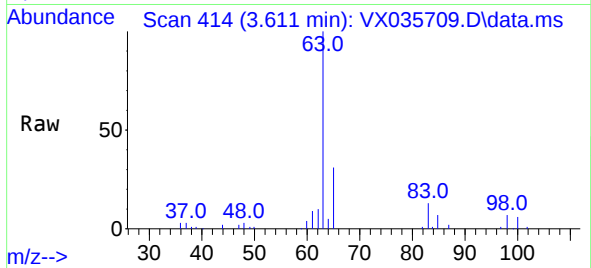

#25
2-Butanone
Concen: 0.960 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.018 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 43 Resp: 1957
Ion Ratio Lower Upper
43 100
72 16.7 19.3 28.9#


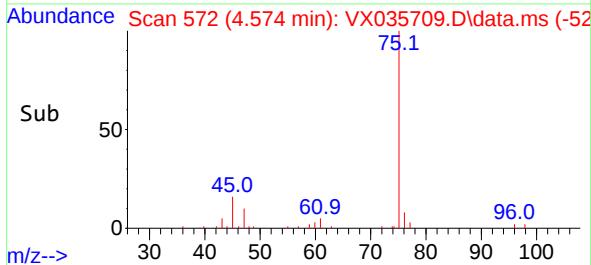

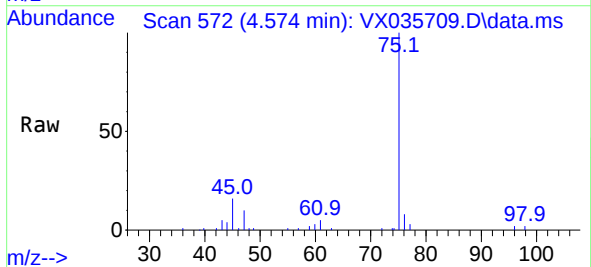




#26
2,2-Dichloropropane
Concen: 0.201 ug/l
RT: 4.568 min Scan# 51
Delta R.T. 0.091 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 77 Resp: 834
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.1#

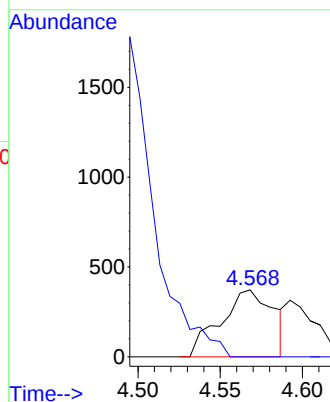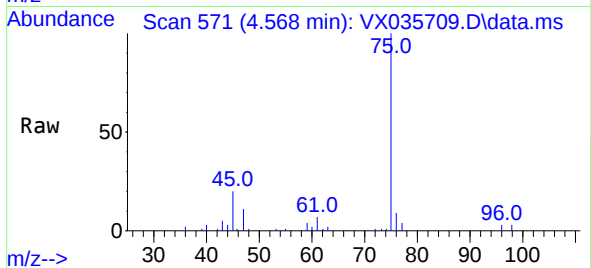

#27
cis-1,2-Dichloroethene
Concen: 49.176 ug/l
RT: 4.489 min Scan# 558
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 96 Resp: 141683
Ion Ratio Lower Upper
96 100
61 142.8 0.0 300.4
98 63.3 0.0 129.0

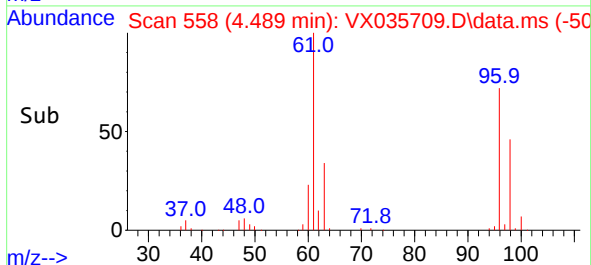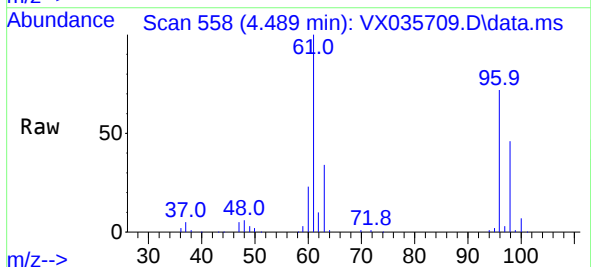



#29

Tetrahydrofuran

Concen: 0.807 ug/l

RT: 5.025 min Scan# 64

Delta R.T. 0.018 min

Lab File: VX035709.D

Acq: 17 May 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :

GWOW-07B-24-29-050423





Tgt Ion: 42 Resp: 1034

Ion Ratio Lower Upper

42 100

72 29.9 34.5 51.7#

71 28.9 32.1 48.1#

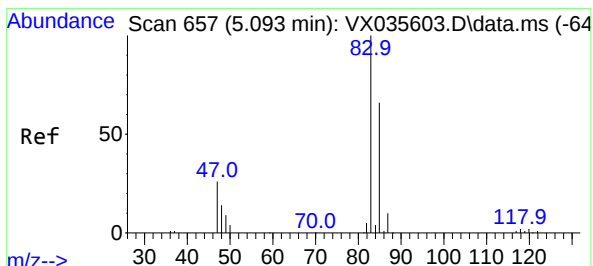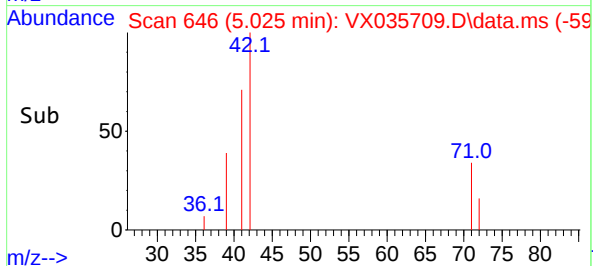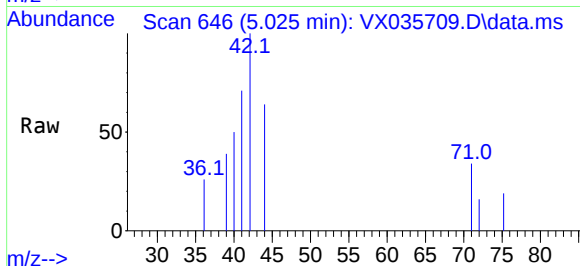

#30

Chloroform

Concen: 2.246 ug/l

RT: 5.092 min Scan# 657

Delta R.T. -0.001 min

Lab File: VX035709.D




Acq: 17 May 2023 11:42


Tgt Ion: 83 Resp: 11294

Ion Ratio Lower Upper

83 100


85 67.6 50.6 76.0

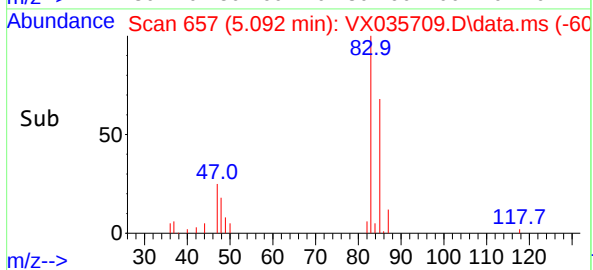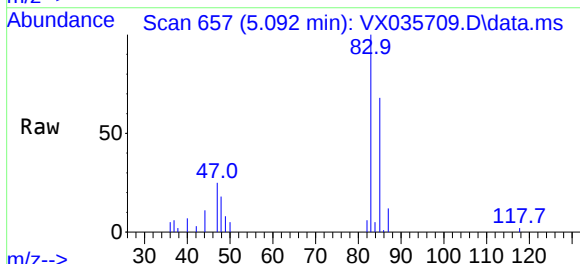






#31
Cyclohexane
Concen: 1.195 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.079 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423



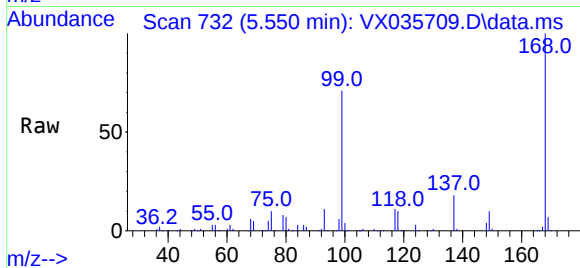



Tgt Ion: 56 Resp: 5171
Ion Ratio Lower Upper
56 100
69 193.1 23.7 35.5#
84 104.2 68.5 102.7#



#33
1,2-Dichloroethane-d4
Concen: 48.318 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 65 Resp: 165555
Ion Ratio Lower Upper
65 100
67 48.9 0.0 104.0

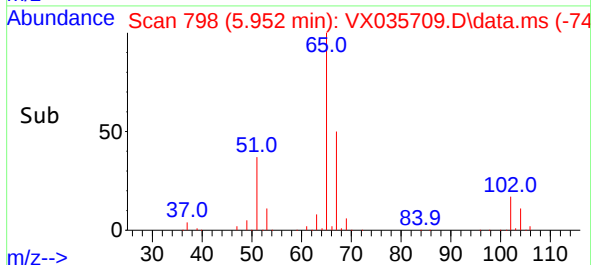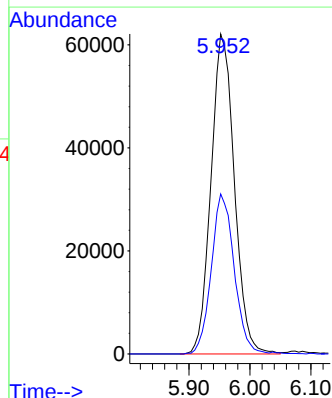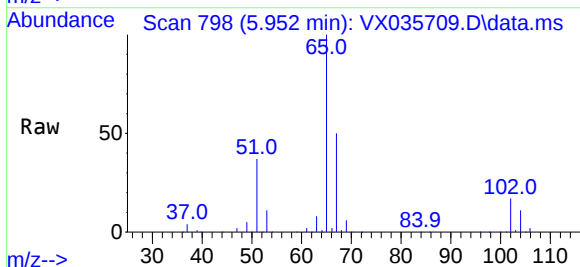



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX035709.D

Acq: 17 May 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :

GWOW-07B-24-29-050423





Tgt Ion:114 Resp: 359429

Ion Ratio Lower Upper

114 100

63 23.3 0.0 42.2

88 17.8 0.0 33.2

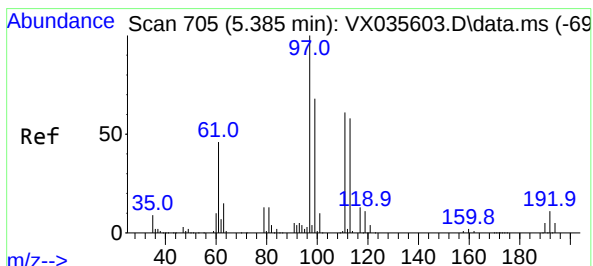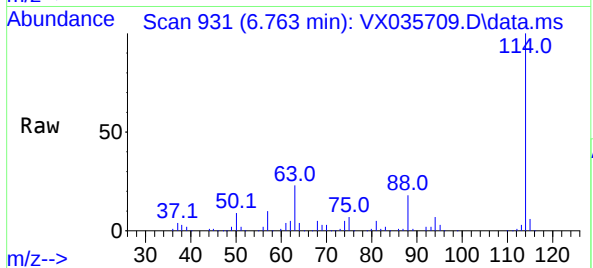

#35

Dibromofluoromethane

Concen: 48.651 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX035709.D

Acq: 17 May 2023 11:42




Tgt Ion:113 Resp: 117929


Ion Ratio Lower Upper

113 100

111 103.0 83.7 125.5

192 16.8 15.4 23.2


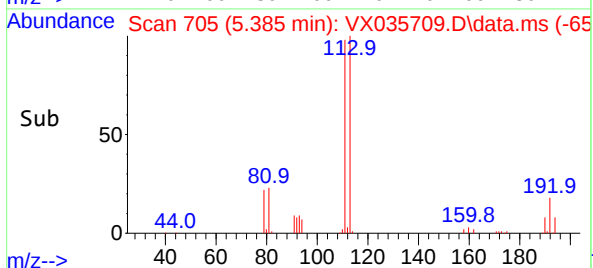
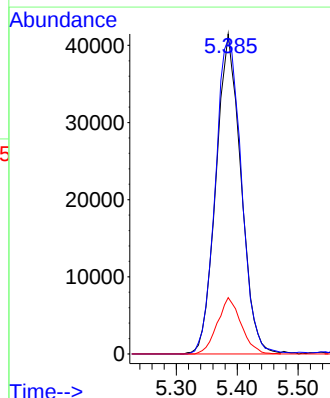



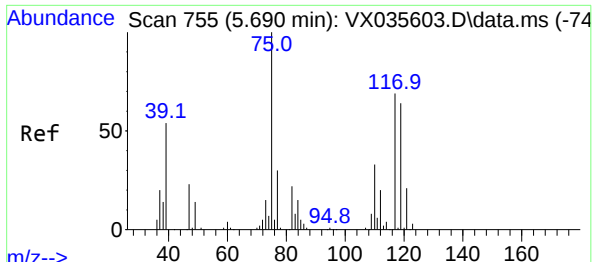

#36
1,1-Dichloropropene
Concen: 4.892 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.140 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 75 Resp: 18716
Ion Ratio Lower Upper
75 100
110 10.2 17.5 52.5#
77 0.0 24.3 36.5#

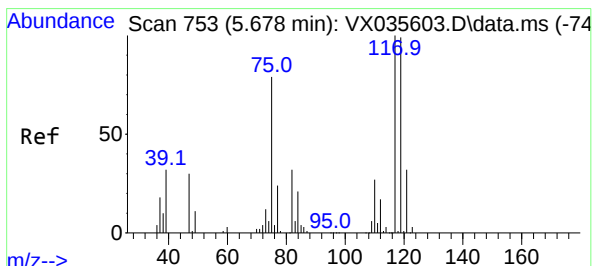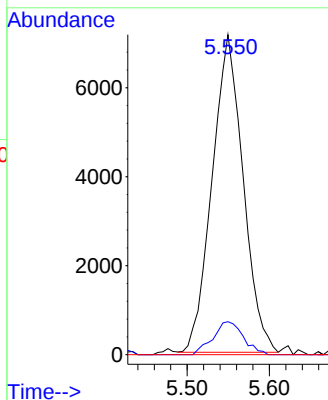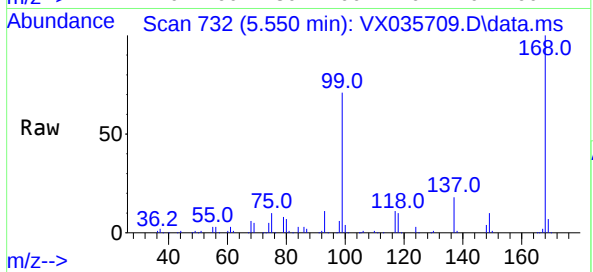

#38
Carbon Tetrachloride
Concen: 6.281 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 117 Resp: 22767
Ion Ratio Lower Upper
117 100
119 3.4 76.6 114.8#
121 0.0 23.8 35.6#


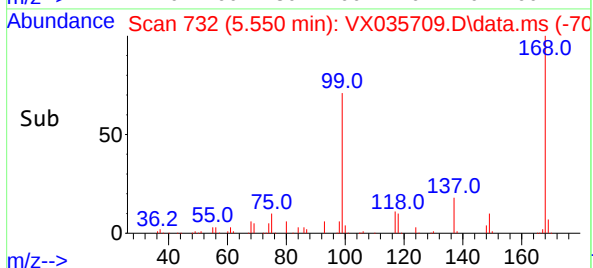
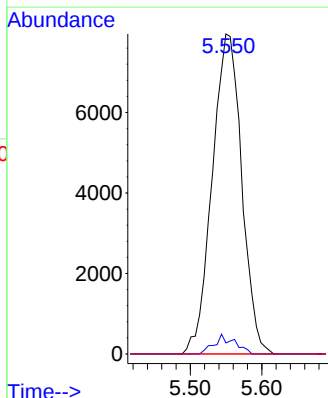
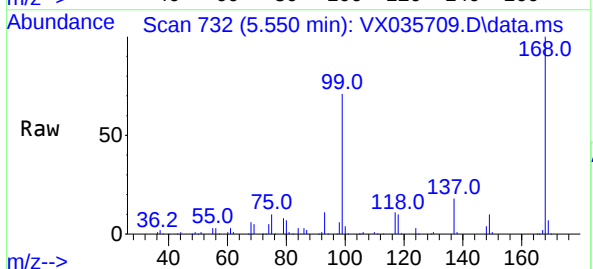


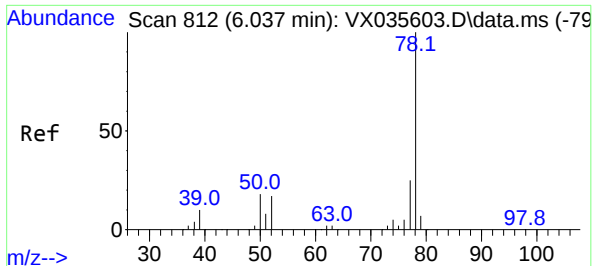

#40
Benzene
Concen: 0.311 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 78 Resp: 3328
Ion Ratio Lower Upper
78 100
77 22.0 19.0 28.4

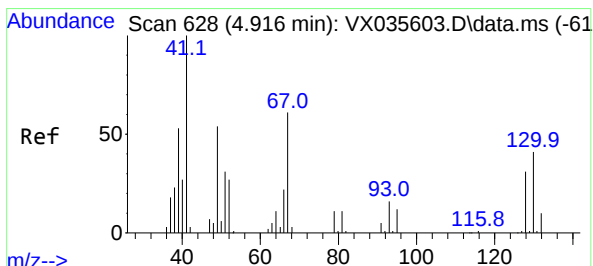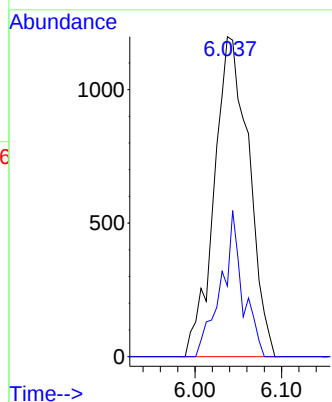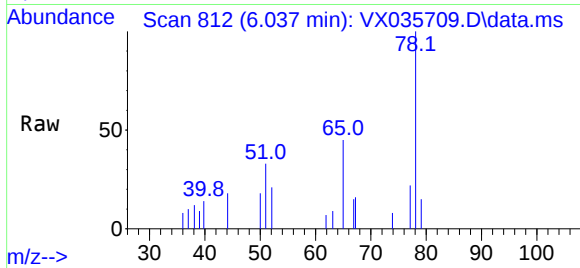

#41
Methacrylonitrile
Concen: 0.315 ug/l
RT: 5.025 min Scan# 646
Delta R.T. 0.109 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 41 Resp: 747
Ion Ratio Lower Upper
41 100
39 30.1 45.0 67.6#
67 0.0 55.6 83.4#
52 0.0 23.2 34.8#

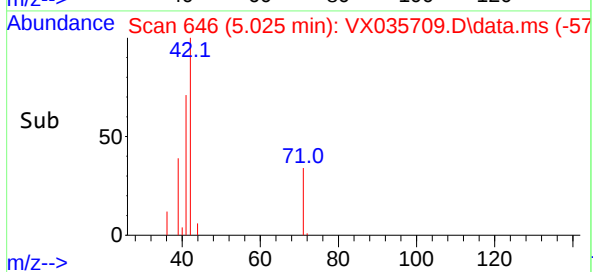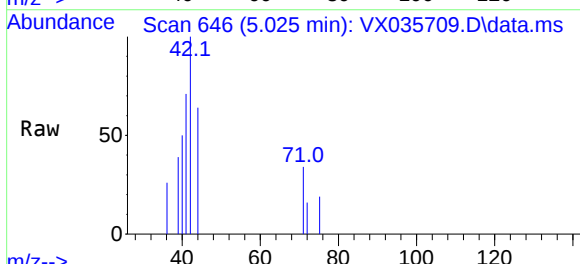



#42

1,2-Dichloroethane

Concen: 4.508 ug/l

RT: 6.092 min Scan# 81

Delta R.T. 0.006 min

Lab File: VX035709.D

Acq: 17 May 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :





GWOW-07B-24-29-050423

Tgt Ion: 62 Resp: 20757

Ion Ratio Lower Upper

62 100

98 8.2 0.0 18.0

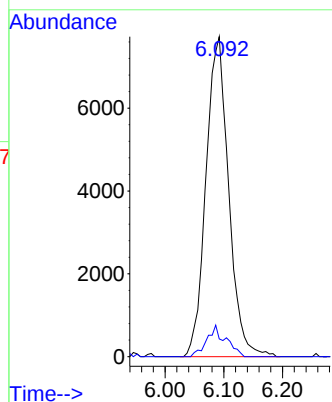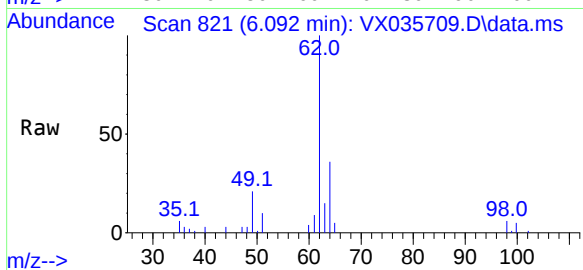

#44

Trichloroethene

Concen: 52.373 ug/l

RT: 7.129 min Scan# 991

Delta R.T. 0.006 min

Lab File: VX035709.D




Acq: 17 May 2023 11:42


Tgt Ion:130 Resp: 142142

Ion Ratio Lower Upper

130 100

95 105.4 0.0 198.4

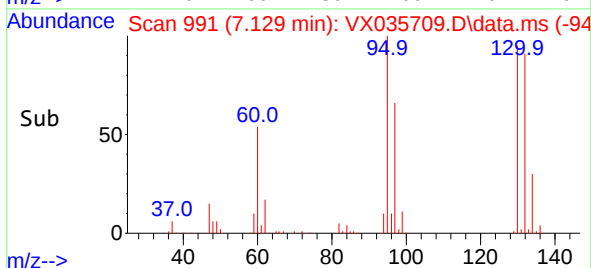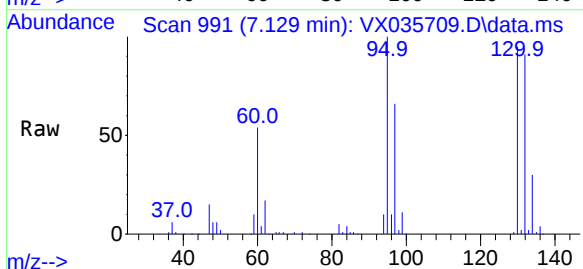



#49

1,4-Dioxane

Concen: 70.052 ug/l

RT: 7.708 min Scan# 1086

Delta R.T. -0.000 min

Lab File: VX035709.D

Acq: 17 May 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :

GWOW-07B-24-29-050423





Tgt Ion: 88 Resp: 5158

Ion Ratio Lower Upper

88 100

43 13.0 27.7 41.5#

58 75.1 56.8 85.2

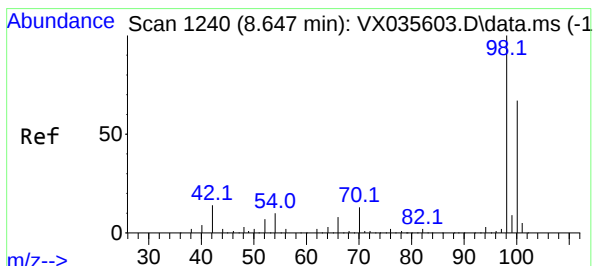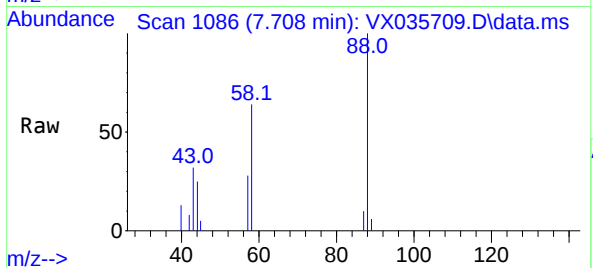

#50

Toluene-d8

Concen: 48.903 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX035709.D




Acq: 17 May 2023 11:42


Tgt Ion: 98 Resp: 437918

Ion Ratio Lower Upper

98 100

100 66.0 52.5 78.7


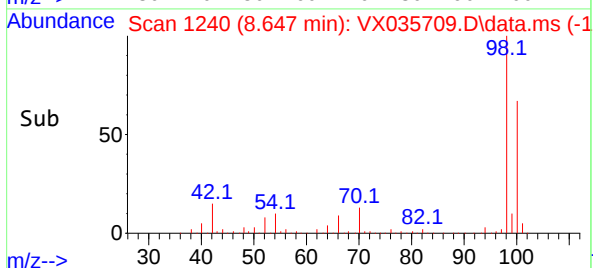






#62
4-Bromofluorobenzene
Concen: 49.472 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 95 Resp: 178374
Ion Ratio Lower Upper
95 100
174 64.1 0.0 147.4
176 62.6 0.0 140.6



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 117 Resp: 333216
Ion Ratio Lower Upper
117 100
82 58.9 45.0 67.4
119 31.6 26.0 39.0


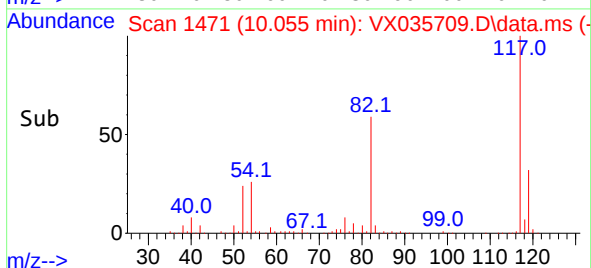
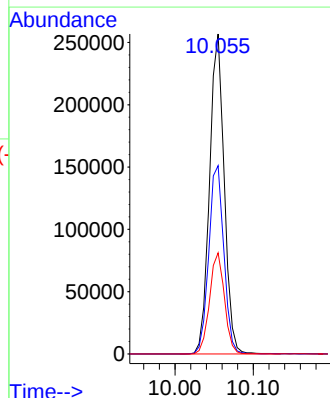





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion:152 Resp: 146266
Ion Ratio Lower Upper
152 100
115 66.1 45.0 135.0
150 158.6 0.0 352.4

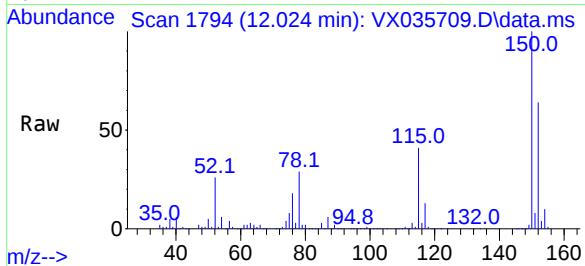

#76
1,2,3-Trichloropropane
Concen: 27.659 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion: 75 Resp: 98956
Ion Ratio Lower Upper
75 100
77 1.1 21.6 64.8#


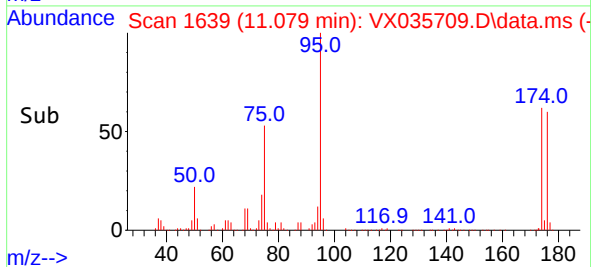

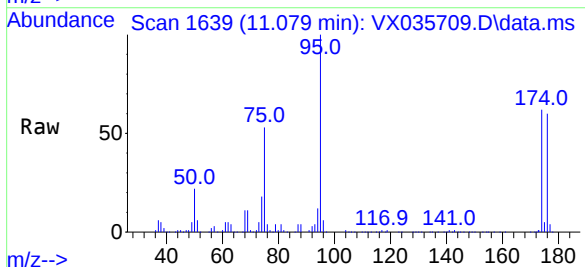




#81
trans-1,4-Dichloro-2-butene
Concen: 89.141 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion: 75 Resp: 98956
Ion Ratio Lower Upper
75 100
53 0.0 82.6 124.0#
89 0.0 36.9 55.3#

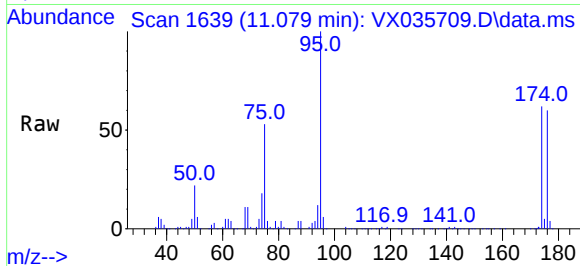

#91
1,2-Dichlorobenzene
Concen: 0.250 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion:146 Resp: 1300
Ion Ratio Lower Upper
146 100
111 37.8 22.0 66.0
148 50.1 32.0 96.0


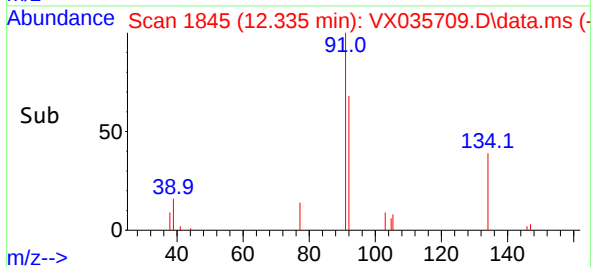

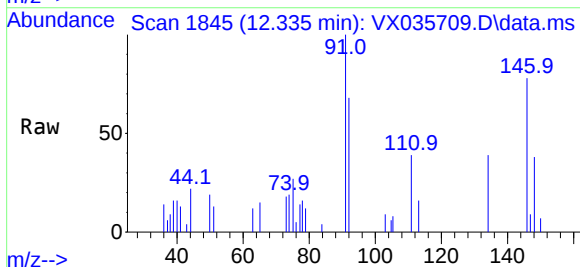




#93
1,2,4-Trichlorobenzene
Concen: 0.391 ug/l
RT: 13.591 min Scan# 2050
Delta R.T. 0.006 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423


Tgt Ion:180 Resp: 1224
Ion Ratio Lower Upper
180 100
182 92.2 47.0 141.0
145 36.3 15.9 47.7

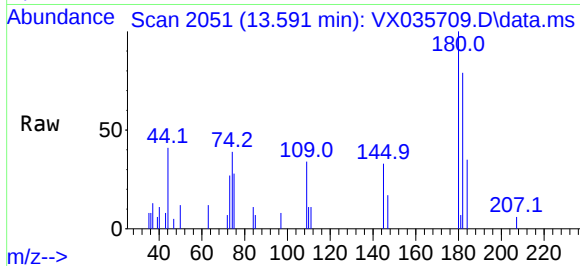

#94
Hexachlorobutadiene
Concen: 0.598 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion:225 Resp: 744
Ion Ratio Lower Upper
225 100
223 50.4 32.1 96.5
227 64.4 31.8 95.4


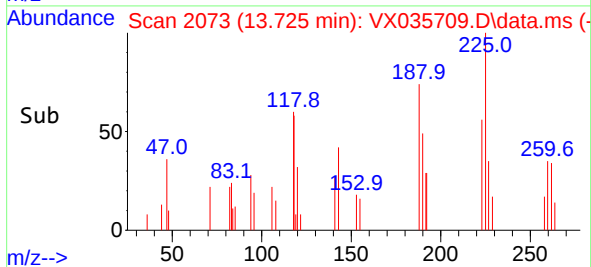

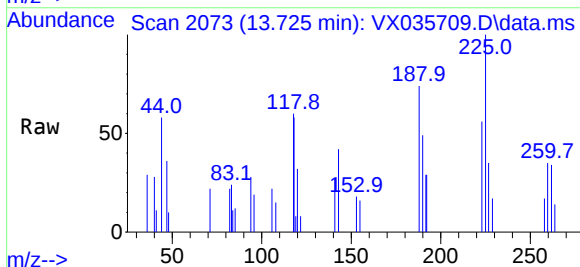




#95
Naphthalene
Concen: 0.276 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Instrument :
MSVOA_X
ClientSampleId :
GWOW-07B-24-29-050423

Tgt Ion:	128	Resp:	2965
Ion	Ratio	Lower	Upper
128	100		
127	8.9	10.2	15.4#
129	11.5	8.6	13.0

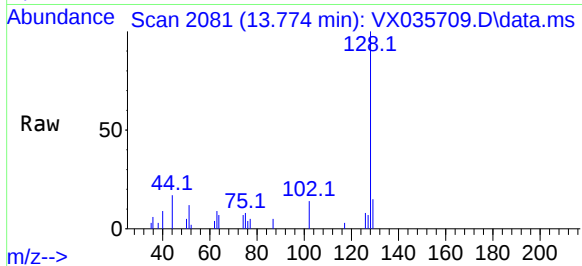

#96
1,2,3-Trichlorobenzene
Concen: 0.374 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX035709.D
Acq: 17 May 2023 11:42

Tgt Ion:	180	Resp:	1152
Ion	Ratio	Lower	Upper
180	100		
182	88.5	48.0	144.2
145	30.6	17.7	53.1

