

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051723\
 Data File : VX035720.D
 Acq On : 17 May 2023 16:00
 Operator : JC/MD
 Sample : 02794-01
 Misc : 1.15g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1927

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
 Title : SW846 8260

Signal : TIC: VX035720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.739	99	107	111	rBV8	5203	12753	1.07%	0.195%
2	2.947	296	305	312	rBV	9743	24371	2.04%	0.373%
3	5.385	695	705	718	rVB2	118929	341712	28.67%	5.223%
4	5.544	720	731	744	rVB	223279	624863	52.43%	9.551%
5	5.952	787	798	816	rBV	158736	425445	35.70%	6.503%
6	6.757	919	930	948	rBV	372924	882548	74.05%	13.490%
7	7.208	998	1004	1011	rBV4	5025	12313	1.03%	0.188%
8	8.647	1232	1240	1248	rBV	775837	1191759	100.00%	18.216%
9	10.055	1465	1471	1480	rBV	760813	1060100	88.95%	16.204%
10	11.085	1633	1640	1651	rBV	569997	807134	67.73%	12.337%
11	12.024	1788	1794	1799	rBV	753617	960832	80.62%	14.686%
12	13.853	2090	2094	2099	rVB	13838	19350	1.62%	0.296%
13	13.926	2099	2106	2110	rBV	15202	21902	1.84%	0.335%
14	13.993	2110	2117	2121	rVV4	8850	19070	1.60%	0.291%
15	14.170	2142	2146	2150	rVB2	13468	16913	1.42%	0.259%
16	14.231	2152	2156	2158	rBV2	19736	25488	2.14%	0.390%
17	14.255	2158	2160	2164	rVV2	19042	26954	2.26%	0.412%
18	14.292	2164	2166	2170	rVB2	14100	16165	1.36%	0.247%
19	14.420	2183	2187	2190	rVB2	15929	19741	1.66%	0.302%
20	15.542	2364	2371	2380	rVB5	11213	19512	1.64%	0.298%
21	16.468	2517	2523	2529	rBV5	6986	13431	1.13%	0.205%




Sum of corrected areas: 6542356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051723\
Data File : VX035720.D
Acq On : 17 May 2023 16:00
Operator : JC/MD
Sample : 02794-01
Misc : 1.15g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

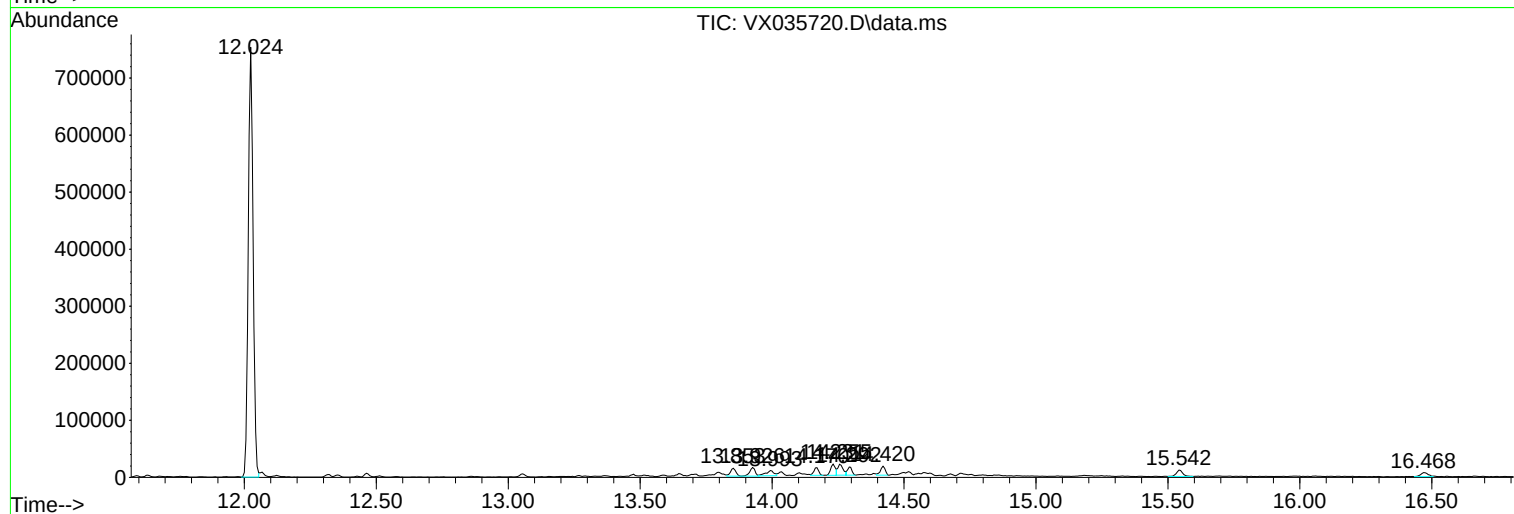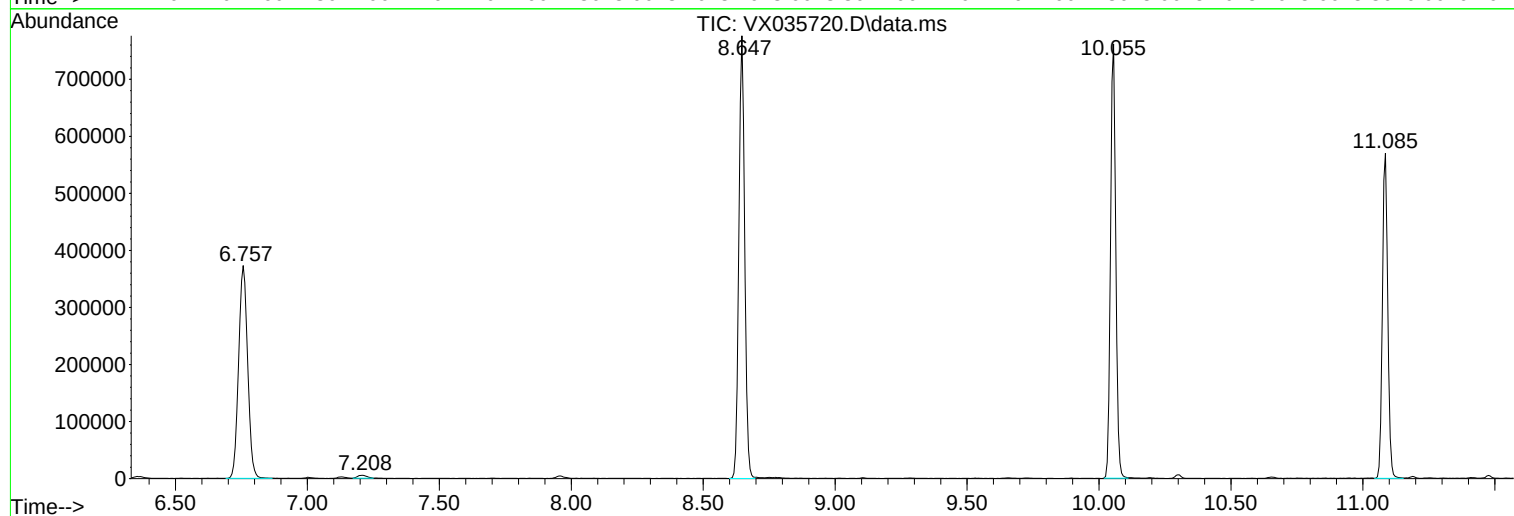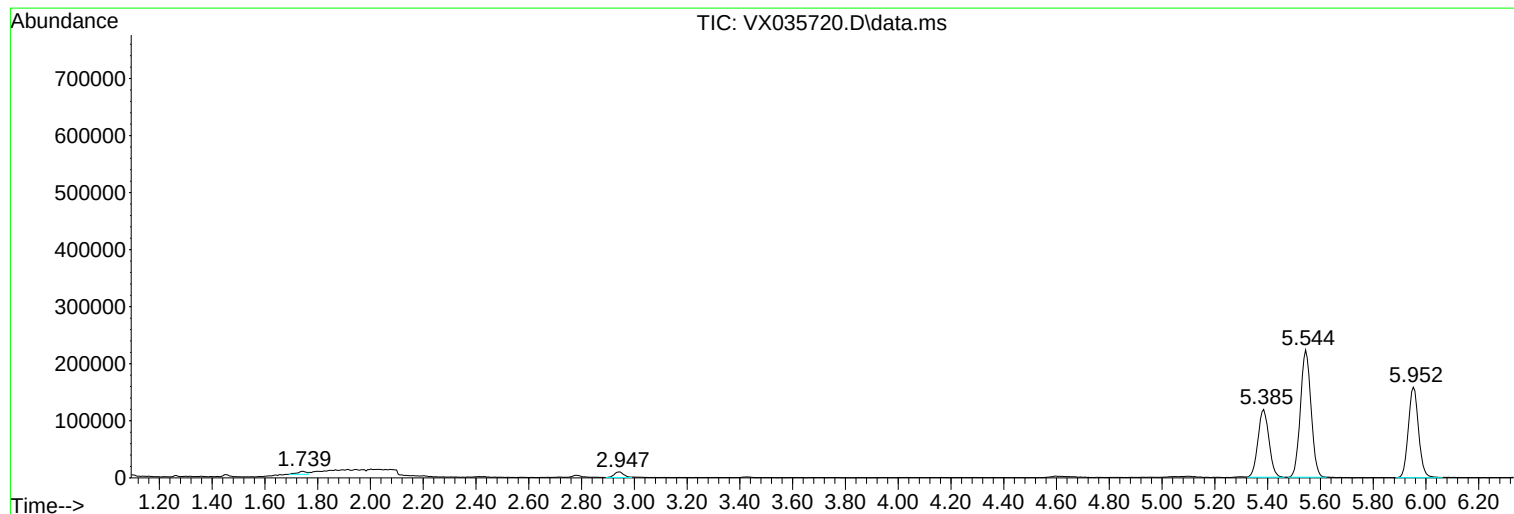

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051723\
Data File : VX035720.D
Acq On : 17 May 2023 16:00
Operator : JC/MD
Sample : 02794-01
Misc : 1.15g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051723\
Data File : VX035720.D
Acq On : 17 May 2023 16:00
Operator : JC/MD
Sample : 02794-01
Misc : 1.15g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------