

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
 Data File : VX022050.D
 Acq On : 17 May 2021 22:27
 Operator : JC/MD
 Sample : M2434-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-SB-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
 Title : SW846 8260

Signal : TIC: VX022050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.563	235	242	252	rBV3	2697	6670	1.23%	0.188%
2	3.111	326	332	345	rVB2	3759	9137	1.68%	0.257%
3	5.397	696	707	719	rBV	58551	167703	30.83%	4.716%
4	5.562	722	734	748	rVB	79965	226250	41.59%	6.362%
5	5.964	788	800	812	rBV	63534	172679	31.74%	4.856%
6	6.769	921	932	943	rBV	159776	374743	68.88%	10.538%
7	8.653	1234	1241	1251	rBV	351569	544018	100.00%	15.298%
8	10.055	1465	1471	1480	rBV	379307	520220	95.63%	14.629%
9	11.085	1634	1640	1649	rBV	327390	401949	73.89%	11.303%
10	11.890	1769	1772	1776	rVB2	4906	5695	1.05%	0.160%
11	12.024	1789	1794	1801	rBV	418533	508877	93.54%	14.310%
12	12.250	1826	1831	1835	rBV2	9667	12849	2.36%	0.361%
13	12.317	1838	1842	1848	rBV4	3776	5568	1.02%	0.157%
14	12.408	1853	1857	1862	rBV2	5084	6207	1.14%	0.175%
15	12.616	1887	1891	1894	rBV	8603	9845	1.81%	0.277%
16	12.719	1900	1908	1913	rBV5	6797	12637	2.32%	0.355%
17	12.853	1921	1930	1934	rVB4	5446	11385	2.09%	0.320%
18	12.927	1934	1942	1947	rBV3	9217	14884	2.74%	0.419%
19	13.030	1955	1959	1964	rVB4	4353	6612	1.22%	0.186%
20	13.140	1974	1977	1981	rVB2	5918	6886	1.27%	0.194%
21	13.292	1998	2002	2009	rVB3	14847	21663	3.98%	0.609%
22	13.372	2009	2015	2018	rVV3	2655	6006	1.10%	0.169%
23	13.426	2021	2024	2029	rVB3	5308	6263	1.15%	0.176%
24	13.585	2046	2050	2054	rBV4	10159	13409	2.46%	0.377%
25	13.646	2054	2060	2061	rVV3	11420	17165	3.16%	0.483%
26	13.664	2061	2063	2070	rVB3	19474	27035	4.97%	0.760%
27	13.756	2072	2078	2081	rBV2	4265	5651	1.04%	0.159%
28	13.804	2081	2086	2090	rVB5	3922	5883	1.08%	0.165%
29	13.859	2090	2095	2100	rVB	17229	21484	3.95%	0.604%
30	13.932	2100	2107	2110	rBV2	26661	37260	6.85%	1.048%
31	14.079	2126	2131	2138	rBV3	7816	11413	2.10%	0.321%
32	14.213	2148	2153	2161	rBV4	14292	28836	5.30%	0.811%
33	14.323	2168	2171	2175	rVB	14763	16581	3.05%	0.466%
34	14.378	2175	2180	2184	rVB2	18100	24745	4.55%	0.696%
35	14.481	2191	2197	2203	rBV2	36987	50385	9.26%	1.417%
36	14.615	2215	2219	2222	rVV3	13122	21520	3.96%	0.605%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
 Data File : VX022050.D
 Acq On : 17 May 2021 22:27
 Operator : JC/MD
 Sample : M2434-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-SB-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
 Title : SW846 8260

37	14.676	2226	2229	2234	rVB2	13407	17189	3.16%	0.483%
38	14.731	2234	2238	2241	rBV3	4490	5629	1.03%	0.158%
39	14.786	2241	2247	2250	rVV2	9814	16503	3.03%	0.464%
40	14.823	2250	2253	2255	rVV3	13111	17358	3.19%	0.488%
41	14.847	2255	2257	2261	rVB3	13011	15336	2.82%	0.431%
42	14.920	2261	2269	2273	rBV4	10352	15195	2.79%	0.427%
43	15.054	2283	2291	2296	rBV4	4337	7730	1.42%	0.217%
44	15.182	2304	2312	2320	rBV4	17209	35560	6.54%	1.000%
45	15.262	2320	2325	2332	rVB5	5207	9060	1.67%	0.255%
46	15.377	2340	2344	2347	rBV6	3530	5708	1.05%	0.161%
47	15.414	2347	2350	2353	rVV2	5387	6556	1.21%	0.184%
48	15.481	2357	2361	2365	rVV3	8489	12962	2.38%	0.364%
49	15.530	2365	2369	2374	rVB3	8614	13800	2.54%	0.388%
50	15.615	2379	2383	2387	rVV3	13952	22104	4.06%	0.622%
51	15.652	2387	2389	2397	rVB5	5197	8009	1.47%	0.225%
52	15.853	2418	2422	2426	rVB4	5461	7384	1.36%	0.208%


Sum of corrected areas: 3556196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
Data File : VX022050.D
Acq On : 17 May 2021 22:27
Operator : JC/MD
Sample : M2434-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-SB-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

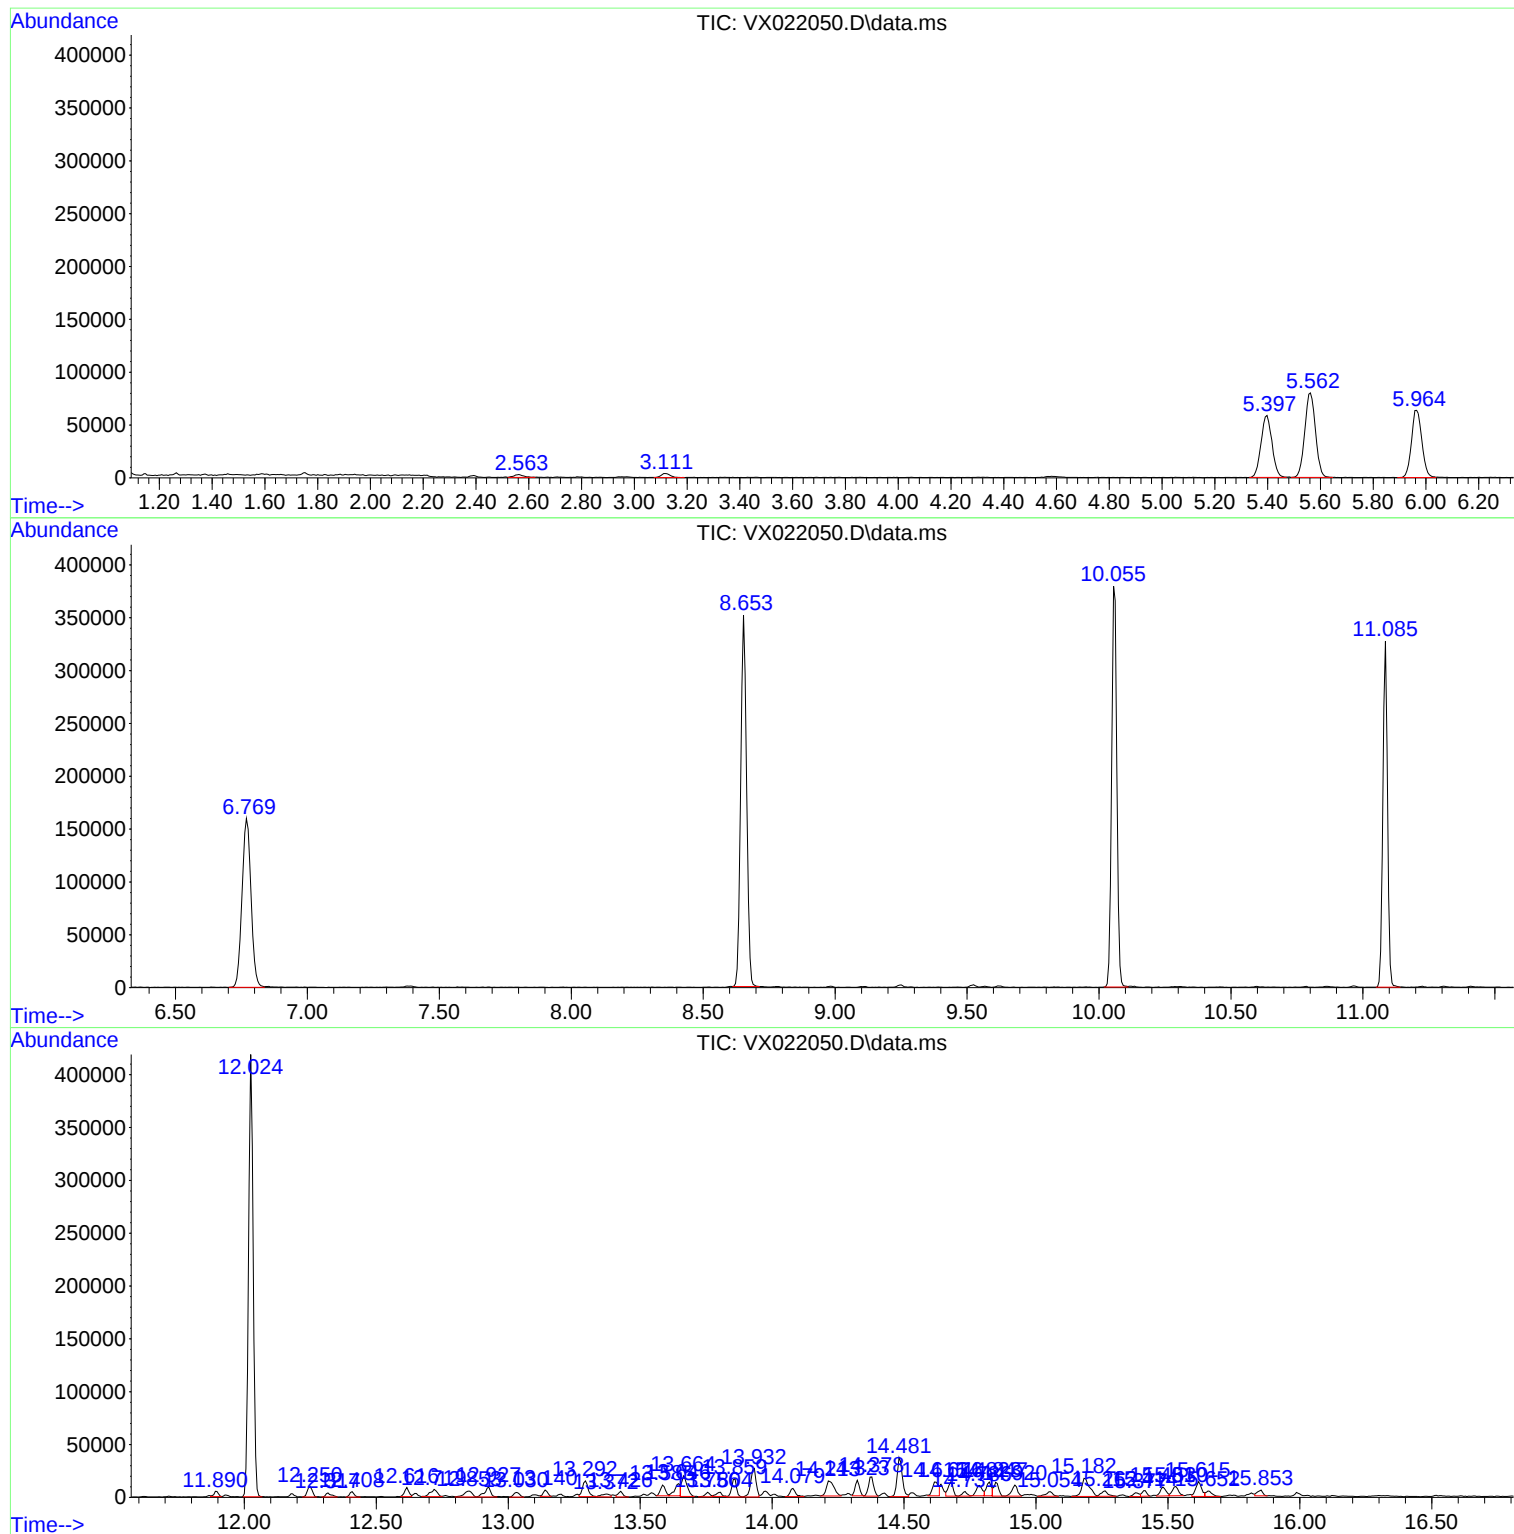

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
Data File : VX022050.D
Acq On : 17 May 2021 22:27
Operator : JC/MD
Sample : M2434-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-SB-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
Data File : VX022050.D
Acq On : 17 May 2021 22:27
Operator : JC/MD
Sample : M2434-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-SB-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
