

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
 Data File : VX022059.D
 Acq On : 18 May 2021 14:21
 Operator : JC/MD
 Sample : M2434-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-SB-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
 Title : SW846 8260

Signal : TIC: VX022059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	324	333	343	rBV3	4009	10323	1.89%	0.291%
2	5.397	694	707	723	rBV2	59966	171212	31.38%	4.828%
3	5.562	723	734	748	rVB	82826	233122	42.72%	6.574%
4	5.964	789	800	811	rBV2	63896	173666	31.83%	4.897%
5	6.769	921	932	943	rBV	157431	375777	68.87%	10.597%
6	8.653	1234	1241	1251	rVB	356445	545638	100.00%	15.387%
7	10.055	1465	1471	1481	rBV	385282	521992	95.67%	14.720%
8	11.085	1634	1640	1651	rVB	320096	401720	73.62%	11.329%
9	11.896	1769	1773	1776	rVB	5489	5912	1.08%	0.167%
10	12.024	1788	1794	1801	rBV	427404	509921	93.45%	14.380%
11	12.250	1827	1831	1836	rBV2	9371	12226	2.24%	0.345%
12	12.317	1838	1842	1849	rVB4	3524	6777	1.24%	0.191%
13	12.408	1853	1857	1860	rBV3	4633	6110	1.12%	0.172%
14	12.616	1884	1891	1894	rBV	8504	11433	2.10%	0.322%
15	12.719	1901	1908	1913	rBV6	6483	13379	2.45%	0.377%
16	12.853	1921	1930	1935	rBV5	9504	18354	3.36%	0.518%
17	12.927	1935	1942	1946	rBV2	9615	15074	2.76%	0.425%
18	13.030	1955	1959	1965	rVV4	3681	6035	1.11%	0.170%
19	13.140	1974	1977	1982	rVV2	5962	7951	1.46%	0.224%
20	13.292	1998	2002	2009	rVB3	15491	22280	4.08%	0.628%
21	13.427	2021	2024	2028	rVB3	4837	5894	1.08%	0.166%
22	13.585	2047	2050	2054	rBV2	9908	12716	2.33%	0.359%
23	13.646	2054	2060	2061	rVV2	11520	17724	3.25%	0.500%
24	13.664	2061	2063	2073	rVB2	19764	28635	5.25%	0.808%
25	13.853	2090	2094	2099	rVB2	16378	20943	3.84%	0.591%
26	13.926	2099	2106	2111	rBV2	25558	36724	6.73%	1.036%
27	13.975	2111	2114	2117	rBV2	5773	5968	1.09%	0.168%
28	14.079	2126	2131	2138	rBV	8153	10987	2.01%	0.310%
29	14.219	2148	2154	2162	rBV4	15025	30201	5.53%	0.852%
30	14.323	2167	2171	2175	rVB2	13340	17274	3.17%	0.487%
31	14.371	2175	2179	2184	rBV2	18653	24653	4.52%	0.695%
32	14.487	2192	2198	2202	rBV2	33883	48807	8.94%	1.376%
33	14.621	2215	2220	2221	rVV2	13333	18239	3.34%	0.514%
34	14.676	2225	2229	2234	rVB2	14807	19329	3.54%	0.545%
35	14.731	2234	2238	2242	rBV3	4938	5819	1.07%	0.164%
36	14.786	2242	2247	2250	rVV3	10314	16466	3.02%	0.464%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
 Data File : VX022059.D
 Acq On : 18 May 2021 14:21
 Operator : JC/MD
 Sample : M2434-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-SB-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
 Title : SW846 8260

37	14.823	2250	2253	2255	rVV2	13484	18496	3.39%	0.522%
38	14.847	2255	2257	2261	rVV3	11923	15257	2.80%	0.430%
39	14.920	2261	2269	2273	rVV3	11243	17964	3.29%	0.507%
40	15.182	2306	2312	2320	rBV3	16976	33006	6.05%	0.931%
41	15.262	2320	2325	2333	rVB5	5198	8892	1.63%	0.251%
42	15.408	2346	2349	2354	rVB2	4381	5726	1.05%	0.161%
43	15.481	2355	2361	2365	rVV4	7511	12201	2.24%	0.344%
44	15.530	2365	2369	2373	rVB3	7495	12307	2.26%	0.347%
45	15.615	2379	2383	2387	rBV	12811	18616	3.41%	0.525%
46	15.652	2387	2389	2396	rVB4	4711	7275	1.33%	0.205%
47	15.847	2417	2421	2428	rVB5	4359	7071	1.30%	0.199%


Sum of corrected areas: 3546092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
Data File : VX022059.D
Acq On : 18 May 2021 14:21
Operator : JC/MD
Sample : M2434-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-SB-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

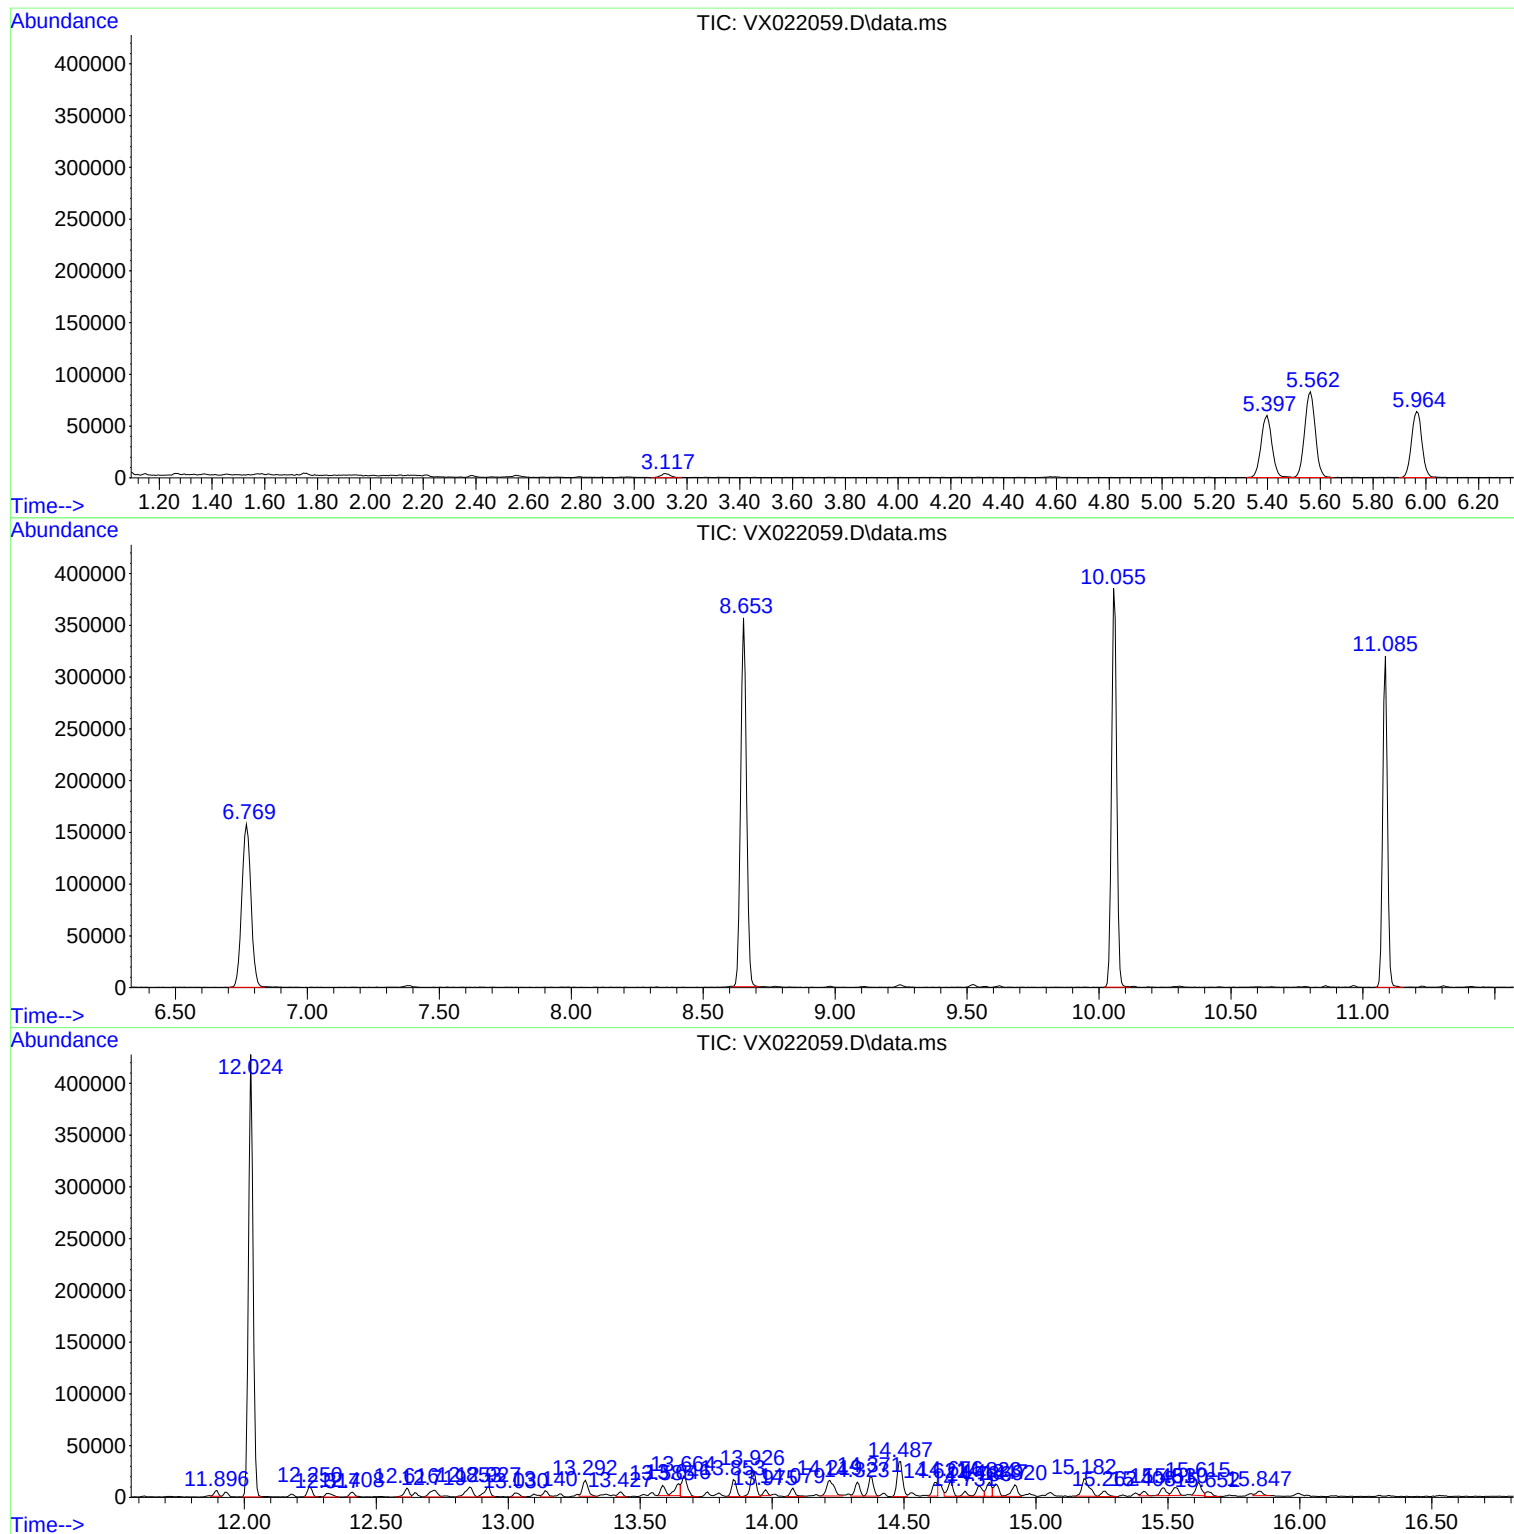

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
Data File : VX022059.D
Acq On : 18 May 2021 14:21
Operator : JC/MD
Sample : M2434-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-SB-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051821\
Data File : VX022059.D
Acq On : 18 May 2021 14:21
Operator : JC/MD
Sample : M2434-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-SB-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
