

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051822\
 Data File : VX028808.D
 Acq On : 18 May 2022 16:05
 Operator : JC/MD
 Sample : N2813-01ME
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1103ME

Quant Time: May 19 01:35:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 12 14:58:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	264427	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	448531	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	436520	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	159767	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	169722	46.824	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.640%		
35) Dibromofluoromethane	5.391	113	132203	44.987	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	89.980%		
50) Toluene-d8	8.653	98	520402	46.970	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	93.940%		
62) 4-Bromofluorobenzene	11.085	95	173357	41.891	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	83.780%		
Target Compounds					Qvalue	
16) Acetone	2.422	43	129734	83.397	ug/l	93
25) 2-Butanone	4.611	43	24189	9.906	ug/l #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051822\
Data File : VX028808.D
Acq On : 18 May 2022 16:05
Operator : JC/MD
Sample : N2813-01ME
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1103ME

Quant Time: May 19 01:35:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260
QLast Update : Thu May 12 14:58:53 2022
Response via : Initial Calibration




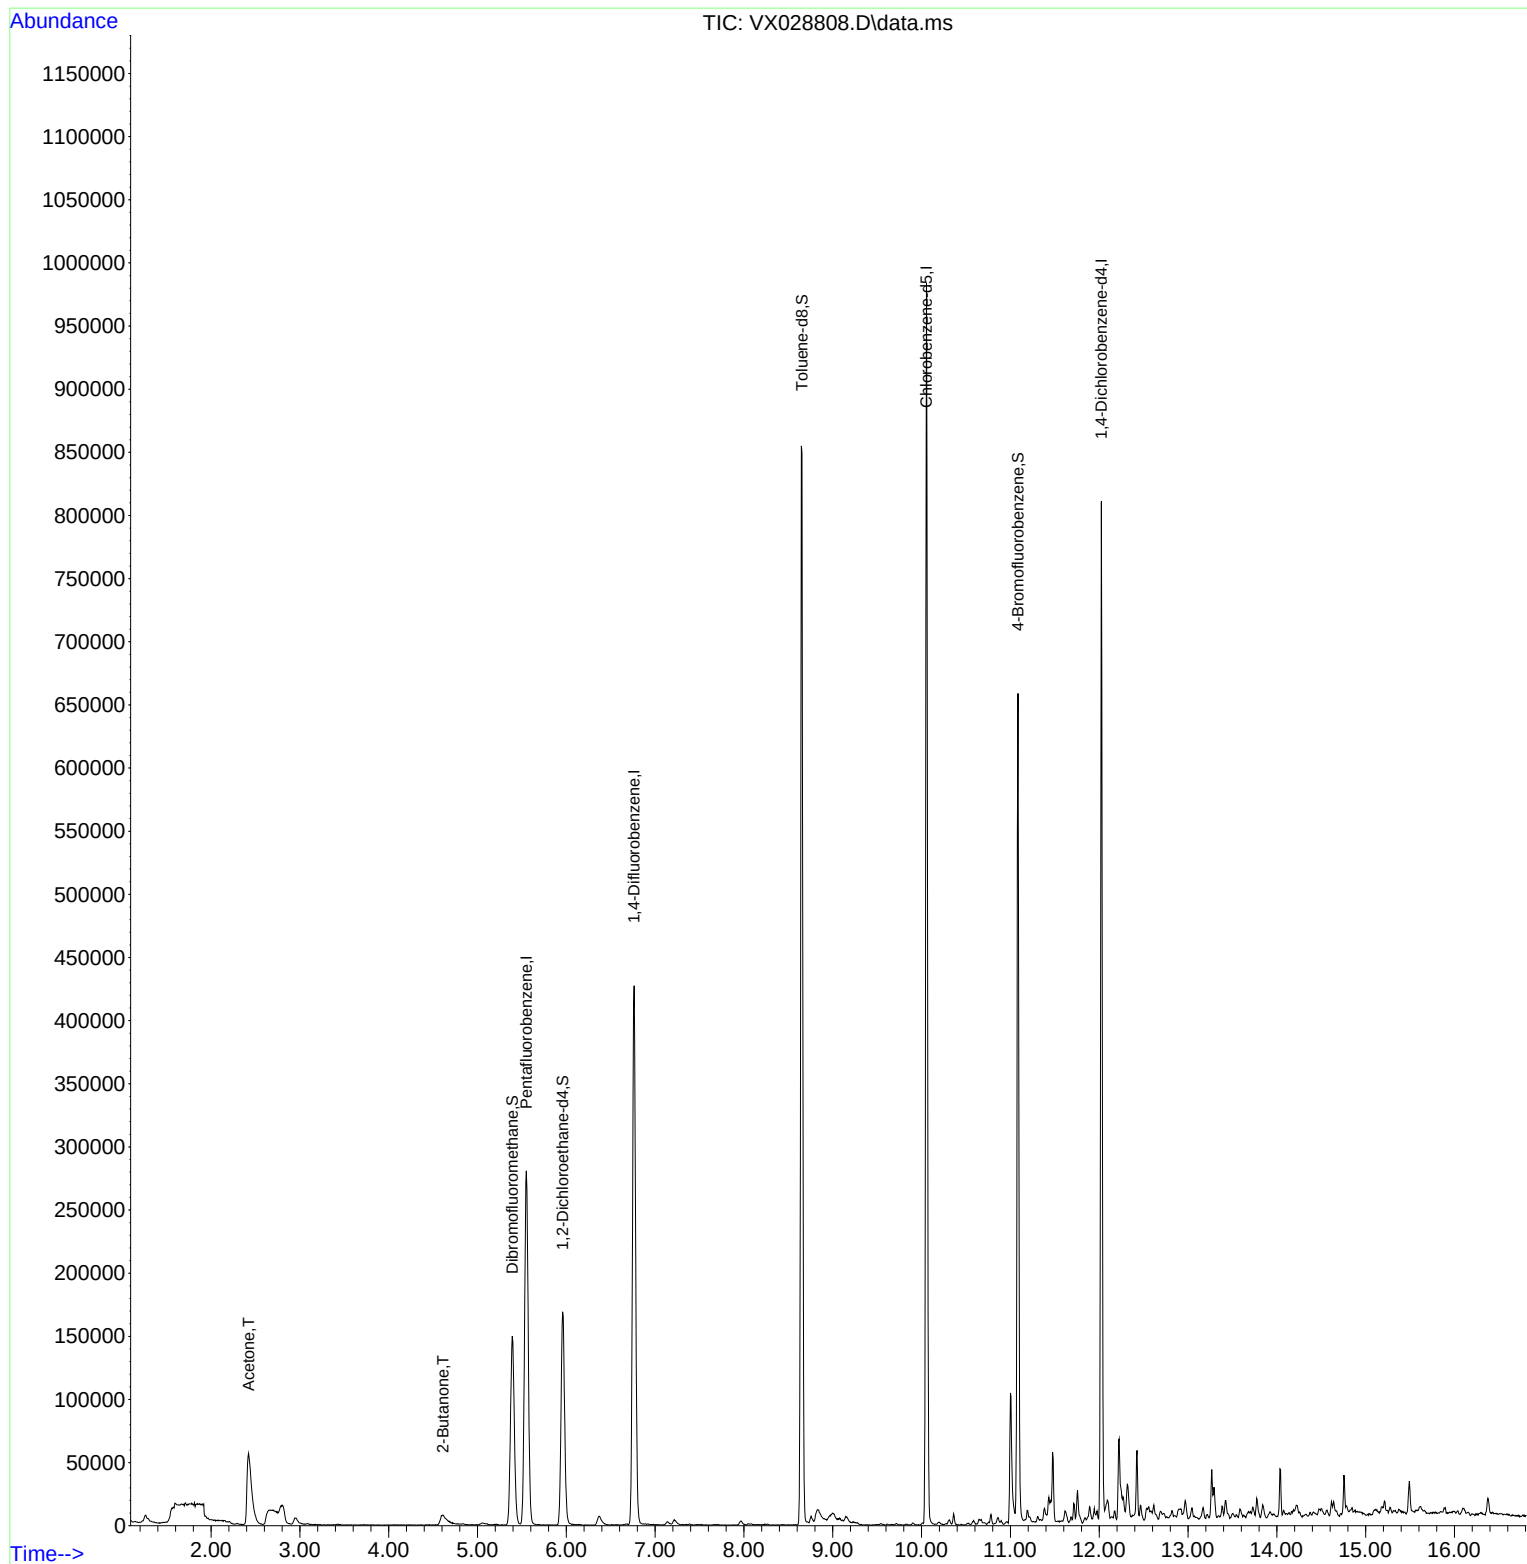


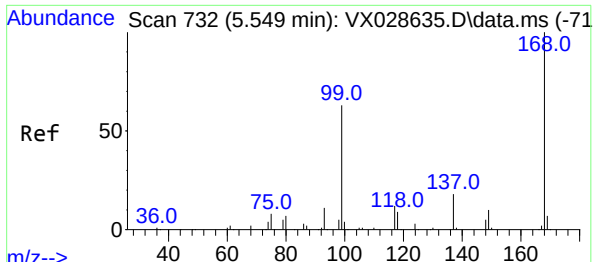

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05




Instrument :
MSVOA_X
ClientSampleId :
BUR-1103ME


Tgt Ion:168 Resp: 264427
Ion Ratio Lower Upper
168 100
99 59.4 41.7 62.5

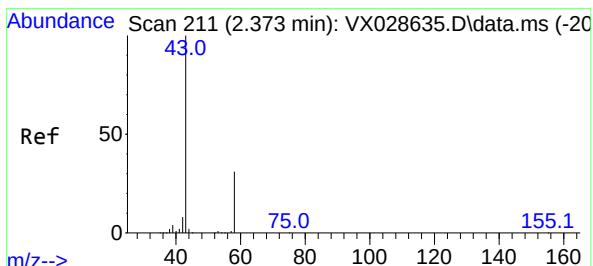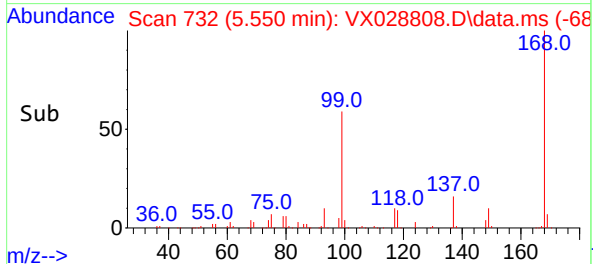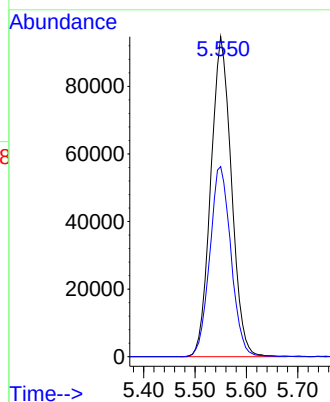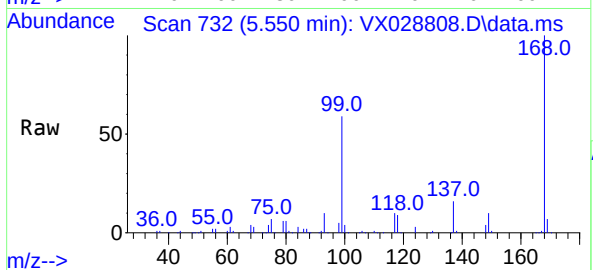

#16
Acetone
Concen: 83.397 ug/l
RT: 2.422 min Scan# 219
Delta R.T. 0.049 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05

Tgt Ion: 43 Resp: 129734
Ion Ratio Lower Upper
43 100
58 32.0 28.8 43.2


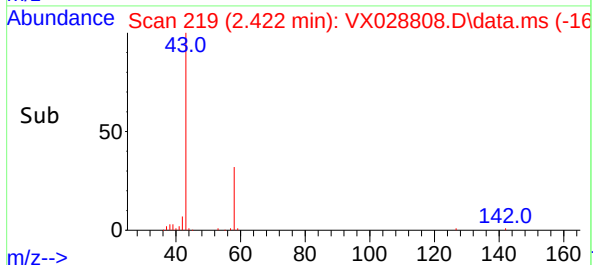
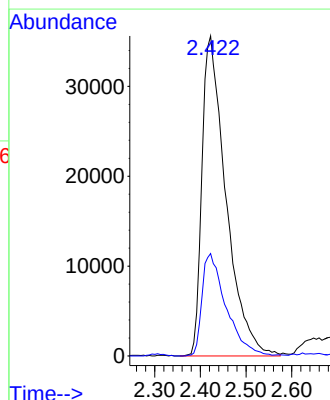
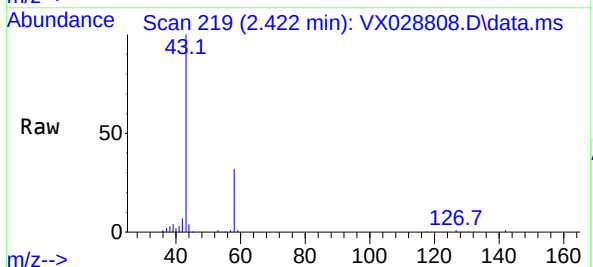


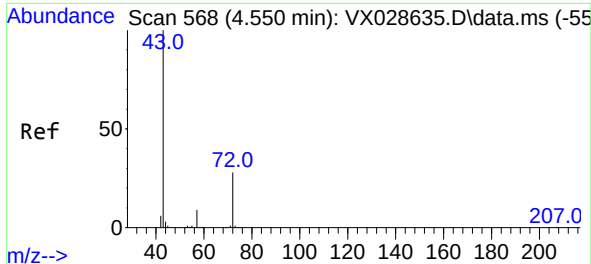

#25
2-Butanone
Concen: 9.906 ug/l
RT: 4.611 min Scan# 51
Delta R.T. 0.061 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05




Instrument :
MSVOA_X
ClientSampleId :
BUR-1103ME


Tgt Ion: 43 Resp: 24189
Ion Ratio Lower Upper
43 100
72 24.4 24.4 36.6#

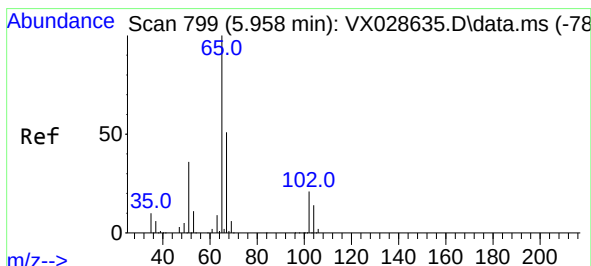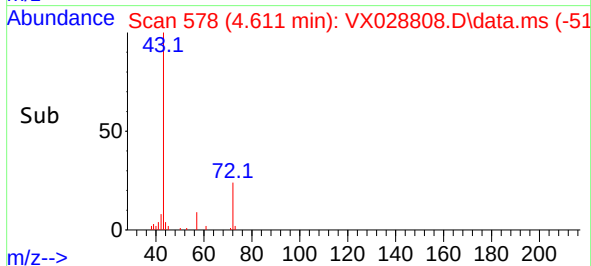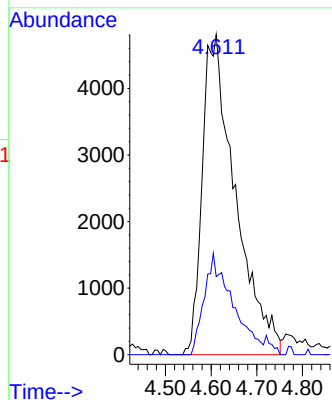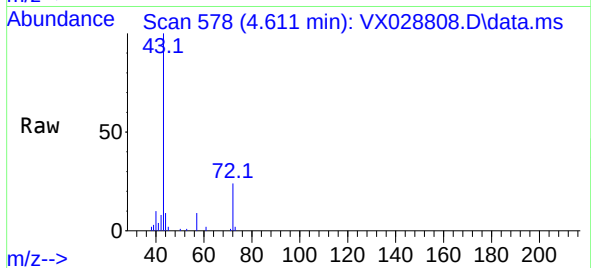

#33
1,2-Dichloroethane-d4
Concen: 46.824 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05

Tgt Ion: 65 Resp: 169722
Ion Ratio Lower Upper
65 100
67 51.0 0.0 107.4


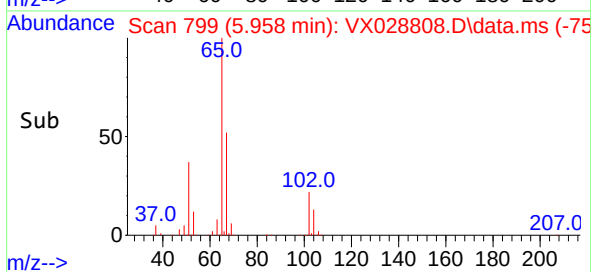
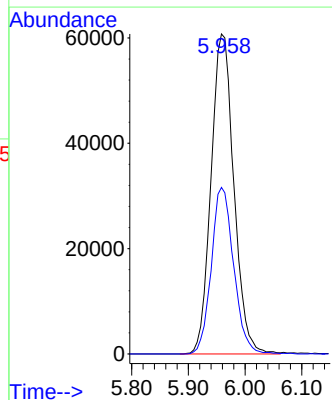
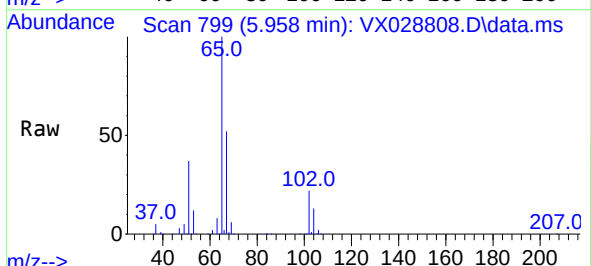


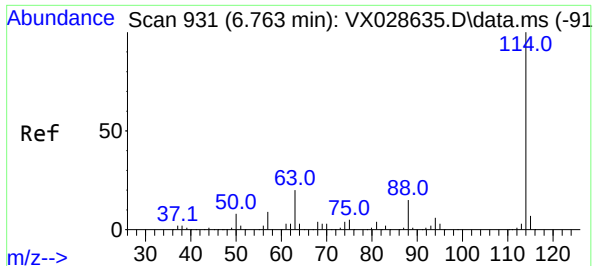

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05




Instrument :
MSVOA_X
ClientSampleId :
BUR-1103ME


Tgt Ion:114 Resp: 448531
Ion Ratio Lower Upper
114 100
63 19.8 0.0 36.8
88 16.2 0.0 32.4

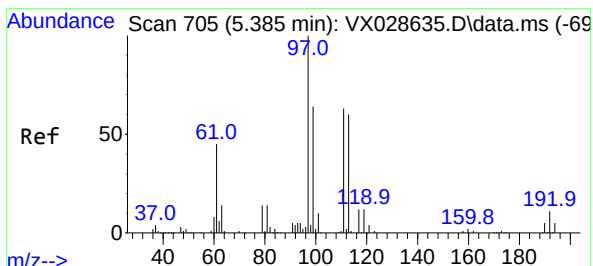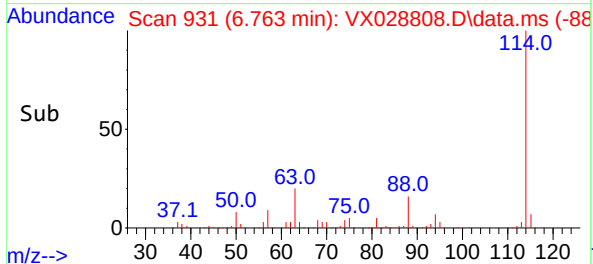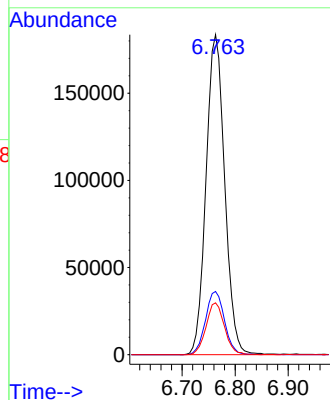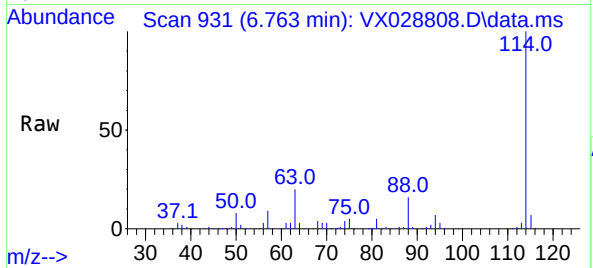

#35
Dibromofluoromethane
Concen: 44.987 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05

Tgt Ion:113 Resp: 132203
Ion Ratio Lower Upper
113 100
111 103.5 82.8 124.2
192 18.8 16.9 25.3


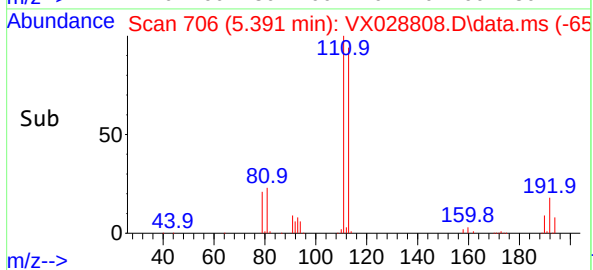
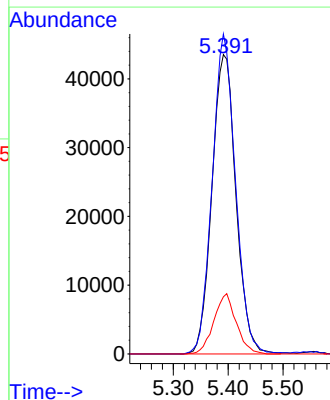
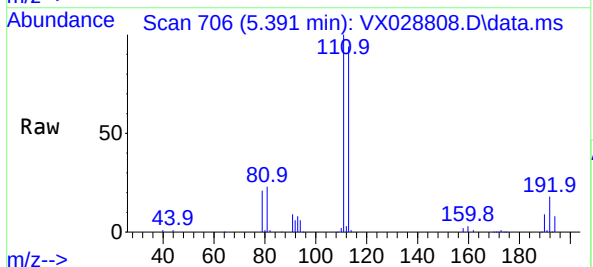


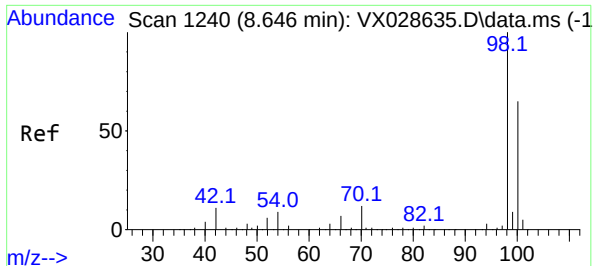

#50
Toluene-d8
Concen: 46.970 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.007 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05




Instrument :
MSVOA_X
ClientSampleId :
BUR-1103ME


Tgt Ion: 98 Resp: 520402
Ion Ratio Lower Upper
98 100
100 66.3 52.6 78.8

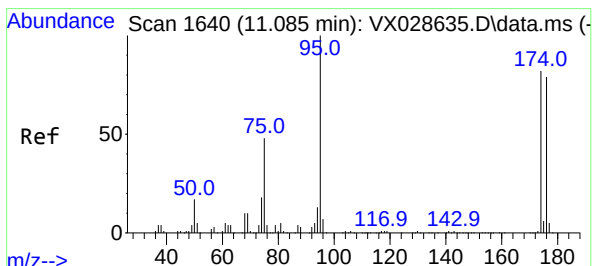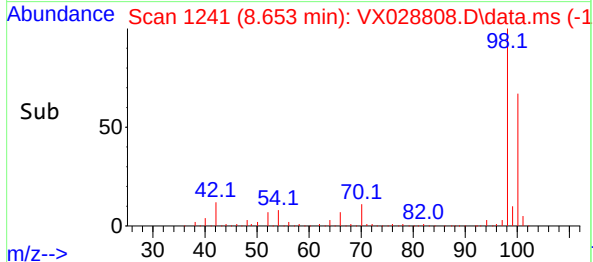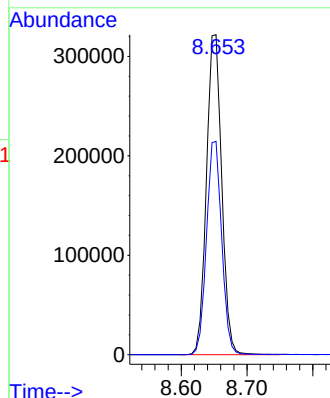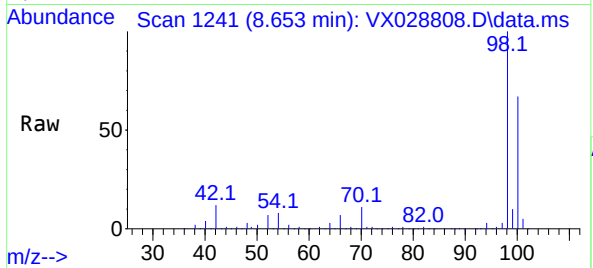

#62
4-Bromofluorobenzene
Concen: 41.891 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05

Tgt Ion: 95 Resp: 173357
Ion Ratio Lower Upper
95 100
174 76.4 0.0 163.0
176 73.0 0.0 155.0


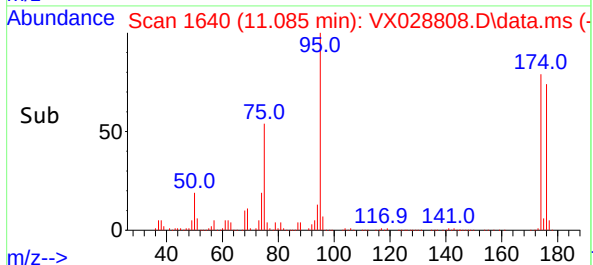
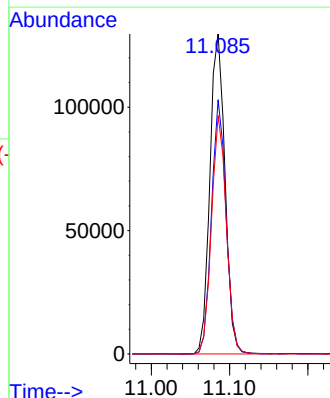
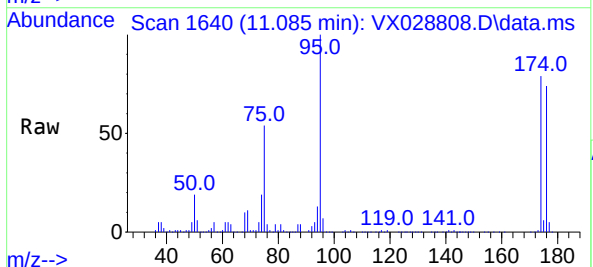


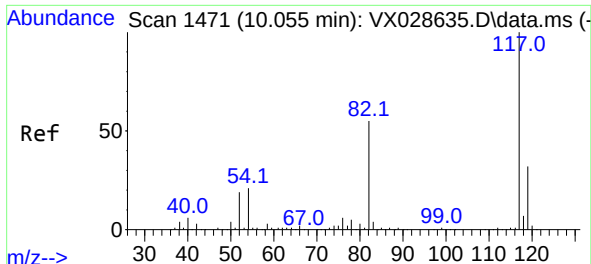

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05

Instrument :
MSVOA_X
ClientSampleId :
BUR-1103ME

Tgt Ion:117 Resp: 436520
Ion Ratio Lower Upper
117 100
82 58.5 41.8 62.8
119 32.4 24.8 37.2

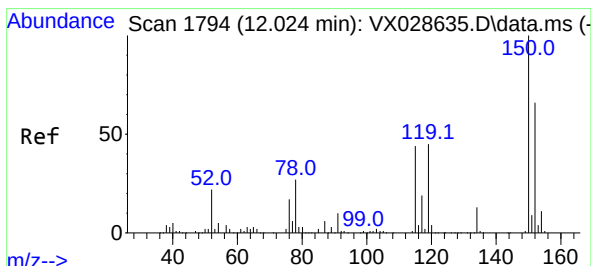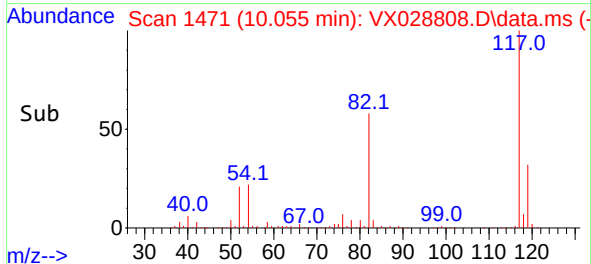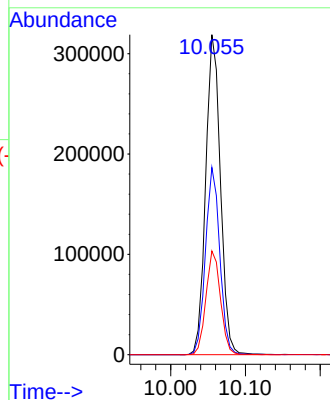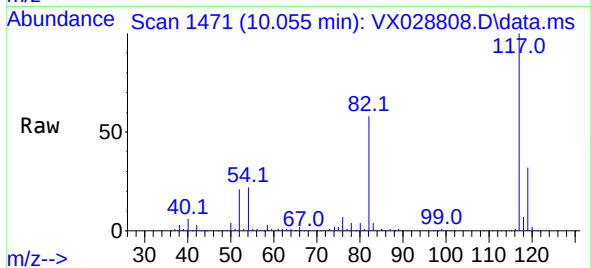

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028808.D
Acq: 18 May 2022 16:05

Tgt Ion:152 Resp: 159767
Ion Ratio Lower Upper
152 100
115 61.2 37.5 112.7
150 155.2 0.0 338.2

