

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051921\
 Data File : VX022100.D
 Acq On : 19 May 2021 20:05
 Operator : JC/MD
 Sample : VIBLK04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK04

Quant Time: May 20 04:24:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	78510	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	162079	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	138507	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	54340	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	62855	51.90	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.80%
35) Dibromofluoromethane	5.397	113	49182	47.85	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.70%
50) Toluene-d8	8.653	98	194016	49.00	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.00%
62) 4-Bromofluorobenzene	11.085	95	66595	45.51	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.02%


Target Compounds						Qvalue
3) Chloromethane	1.294	50	147	0.14	ug/l #	42
6) Chloroethane	1.953	64	26	0.04	ug/l #	43
14) Allyl chloride	2.617	41	84	0.05	ug/l #	24
15) Acrylonitrile	3.105	53	52	0.10	ug/l #	18
17) Carbon Disulfide	2.526	76	295	0.13	ug/l #	75
18) Methyl Acetate	2.703	43	137	0.10	ug/l #	47
23) Vinyl Acetate	3.745	43	42	0.01	ug/l #	68
25) 2-Butanone	4.495	43	20	0.02	ug/l #	45
37) Ethyl Acetate	4.678	43	72	0.04	ug/l #	64
39) Methylcyclohexane	7.403	83	20	0.01	ug/l #	19
41) Methacrylonitrile	4.928	41	31	0.03	ug/l #	21
43) Isopropyl Acetate	6.556	43	53	0.02	ug/l #	57
48) Methyl methacrylate	7.677	41	19	0.01	ug/l #	1
59) 2-Hexanone	9.439	43	24	0.02	ug/l #	19
67) Ethyl Benzene	10.201	91	19	0.00	ug/l #	44
68) m/p-Xylenes	10.311	106	21	0.01	ug/l #	1
70) Styrene	10.665	104	19	0.01	ug/l #	26
73) Isopropylbenzene	10.969	105	74	0.02	ug/l #	49
74) N-amyl acetate	10.969	43	52	0.02	ug/l #	38
75) 1,1,2,2-Tetrachloroethane	11.091	83	38	0.02	ug/l #	1
78) n-propylbenzene	11.299	91	158	0.03	ug/l #	53
79) 2-Chlorotoluene	11.372	91	82	0.03	ug/l #	41
82) 4-Chlorotoluene	11.463	91	102	0.03	ug/l #	61
84) 1,2,4-Trimethylbenzene	11.756	105	96	0.03	ug/l	99
85) sec-Butylbenzene	11.896	105	116	0.02	ug/l #	57
86) p-Isopropyltoluene	12.006	119	165	0.04	ug/l #	51
87) 1,3-Dichlorobenzene	11.975	146	93	0.05	ug/l #	25
88) 1,4-Dichlorobenzene	12.049	146	79	0.04	ug/l #	1
89) n-Butylbenzene	12.341	91	206	0.06	ug/l #	69
93) 1,2,4-Trichlorobenzene	13.591	180	73	0.07	ug/l #	12
95) Naphthalene	13.780	128	181	0.04	ug/l #	69
96) 1,2,3-Trichlorobenzene	13.969	180	44	0.04	ug/l #	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051921\
Data File : VX022100.D
Acq On : 19 May 2021 20:05
Operator : JC/MD
Sample : VIBLK04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK04

Quant Time: May 20 04:24:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration




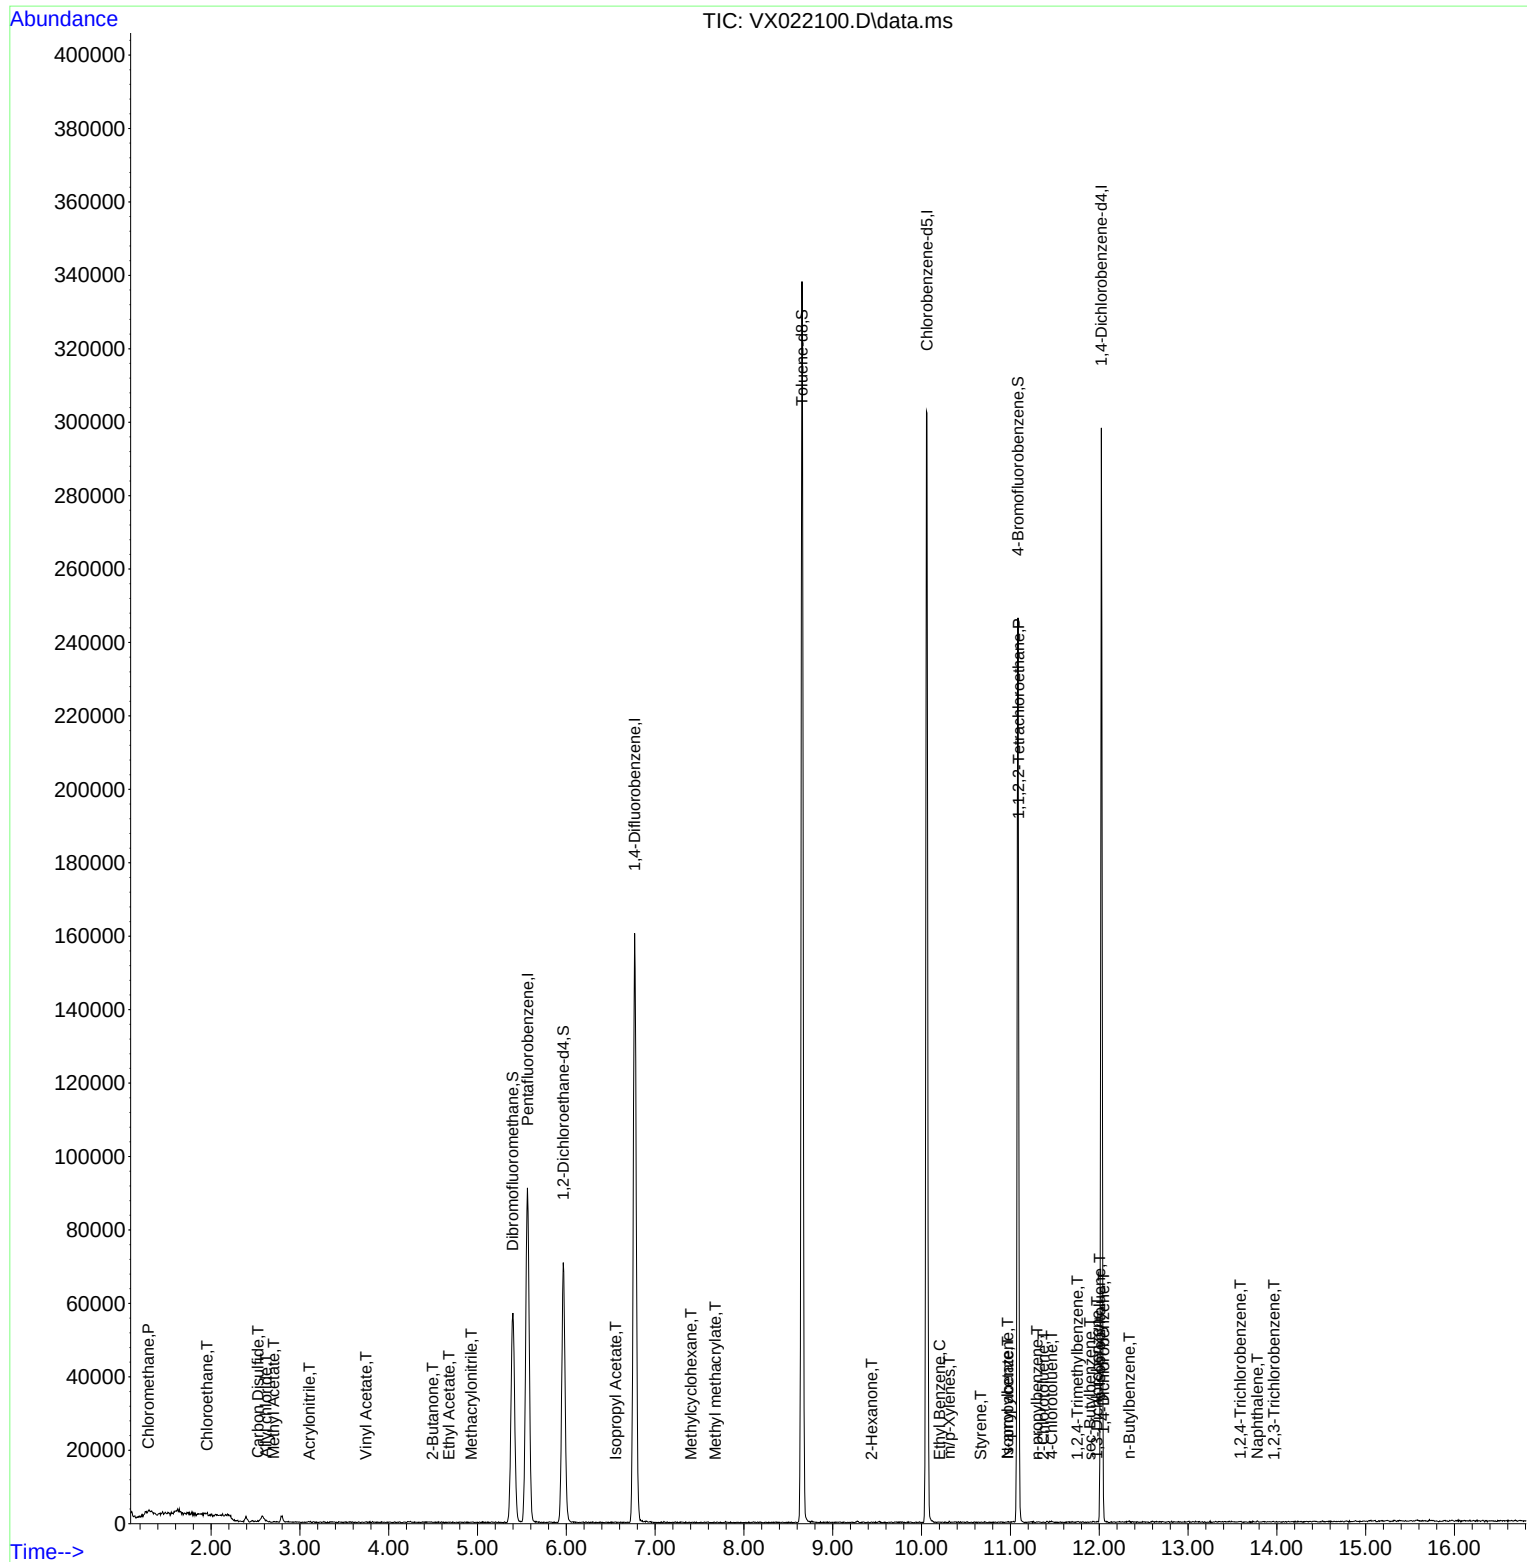




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04

Tgt Ion:168 Resp: 78510
Ion Ratio Lower Upper
168 100
99 66.9 45.8 68.6

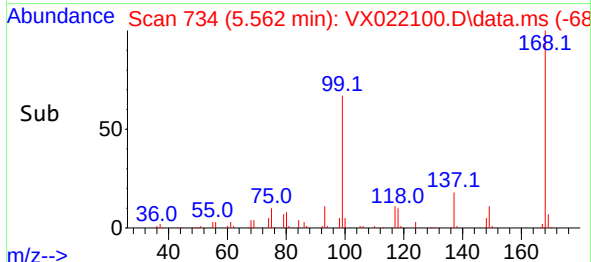


#3
Chloromethane
Concen: 0.14 ug/l
RT: 1.294 min Scan# 34
Delta R.T. -0.001 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 50 Resp: 147
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#



Abundance Scan 98 (1.685 min): VX022082.D\data.ms (-92)


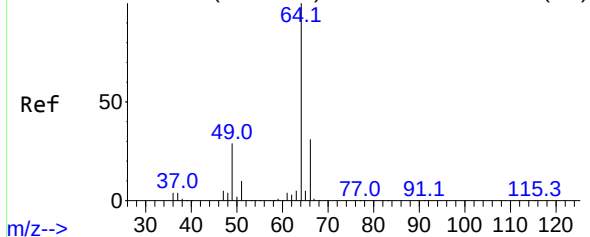


#6
Chloroethane
Concen: 0.04 ug/l
RT: 1.953 min Scan# 142
Delta R.T. 0.268 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05


Tgt Ion: 64 Resp: 26
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

Instrument :
MSVOA_X
ClientSampled :
VIBLK04


Abundance Scan 142 (1.953 min): VX022100.D\data.ms

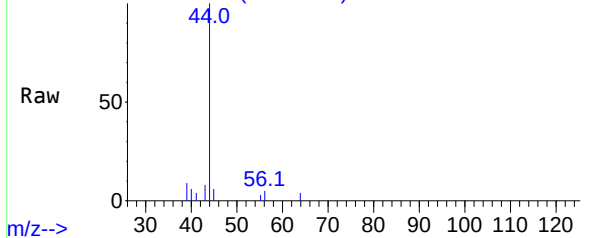

Abundance Scan 142 (1.953 min): VX022100.D\data.ms (-49)

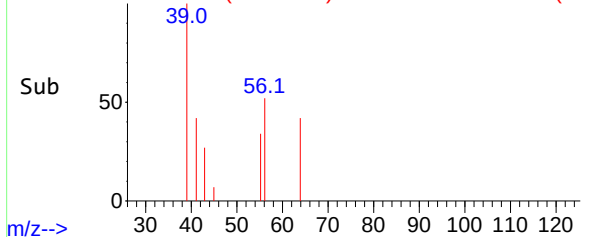



Abundance Scan 259 (2.666 min): VX022082.D\data.ms (-24)

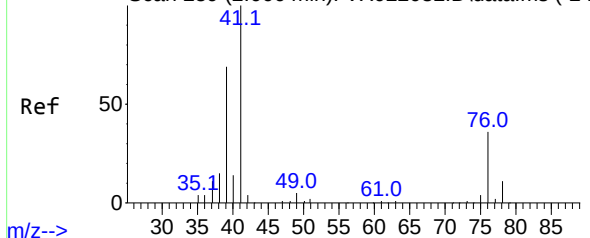


#14
Allyl chloride
Concen: 0.05 ug/l
RT: 2.617 min Scan# 251
Delta R.T. -0.049 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05


Tgt Ion: 41 Resp: 84
Ion Ratio Lower Upper
41 100
39 129.8 51.6 77.4#
76 0.0 30.5 45.7#

Abundance Scan 251 (2.617 min): VX022100.D\data.ms

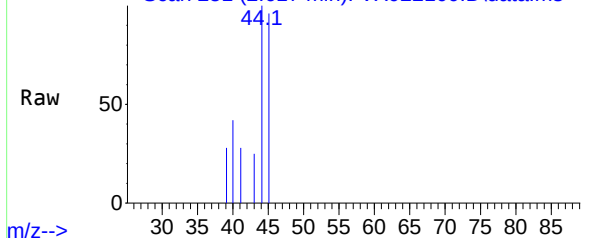

Abundance Scan 251 (2.617 min): VX022100.D\data.ms (-21)




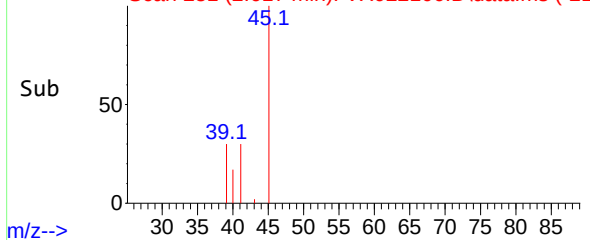




#15
Acrylonitrile
Concen: 0.10 ug/l
RT: 3.105 min Scan# 331
Delta R.T. 0.036 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion: 53 Resp: 52
Ion Ratio Lower Upper
53 100
52 0.0 65.3 97.9#
51 0.0 28.2 42.2#



#17
Carbon Disulfide
Concen: 0.13 ug/l
RT: 2.526 min Scan# 236
Delta R.T. 0.012 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 76 Resp: 295
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

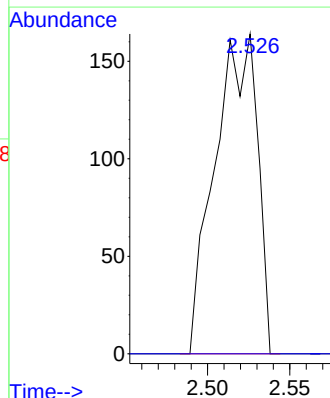



#18

Methyl Acetate

Concen: 0.10 ug/l

RT: 2.703 min Scan# 265

Delta R.T. -0.006 min

Lab File: VX022100.D





Acq: 19 May 2021 20:05

Tgt Ion: 43 Resp: 137

Ion Ratio Lower Upper

43 100

74 0.0 21.9 32.9#



#23

Vinyl Acetate

Concen: 0.01 ug/l

RT: 3.745 min Scan# 436

Delta R.T. 0.018 min

Lab File: VX022100.D




Acq: 19 May 2021 20:05


Tgt Ion: 43 Resp: 42

Ion Ratio Lower Upper

43 100

86 0.0 9.9 14.9#



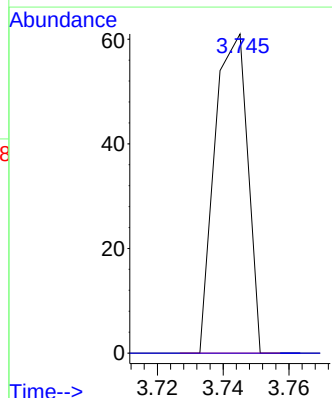





#25
2-Butanone
Concen: 0.02 ug/l
RT: 4.495 min Scan# 559
Delta R.T. -0.073 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion: 43 Resp: 20
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#

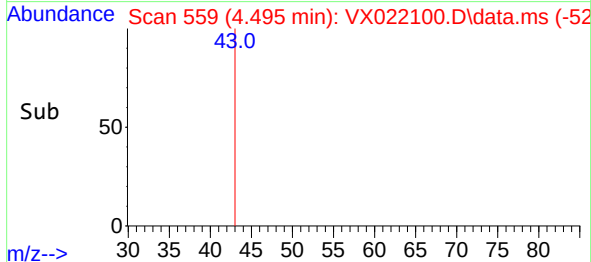

#33
1,2-Dichloroethane-d4
Concen: 51.90 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 65 Resp: 62855
Ion Ratio Lower Upper
65 100
67 52.4 0.0 105.4


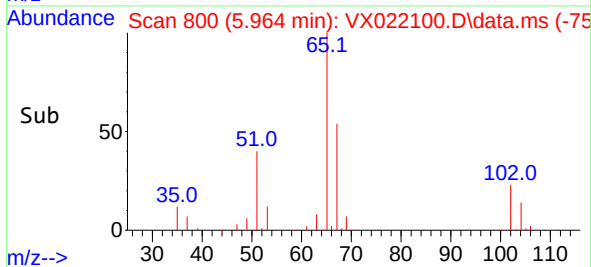

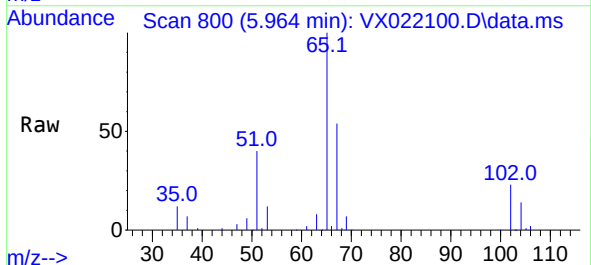


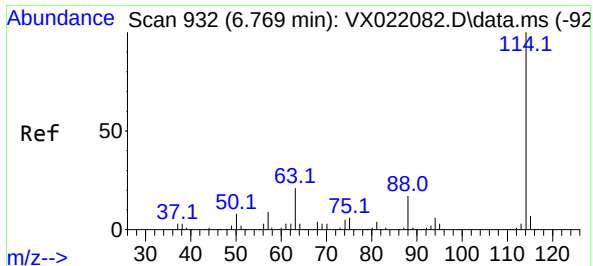

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion:114 Resp: 162079
Ion Ratio Lower Upper
114 100
63 20.8 0.0 40.8
88 16.8 0.0 32.8

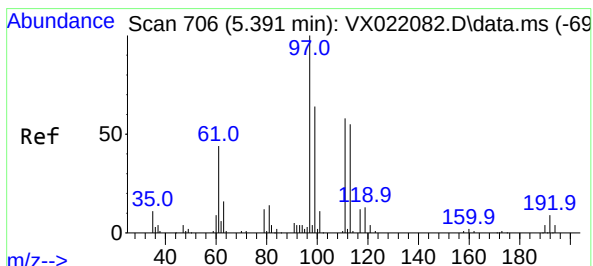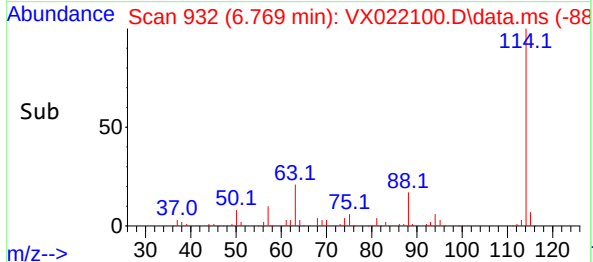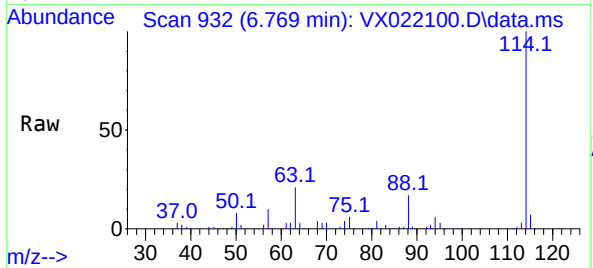

#35
Dibromofluoromethane
Concen: 47.85 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion:113 Resp: 49182
Ion Ratio Lower Upper
113 100
111 105.7 81.9 122.9
192 16.6 16.7 25.1#

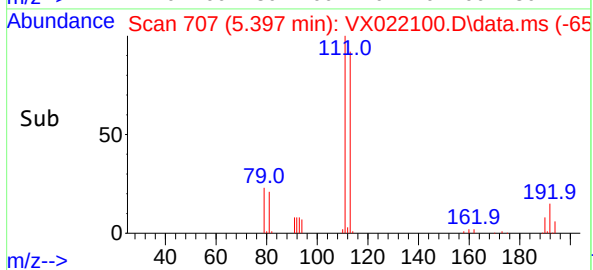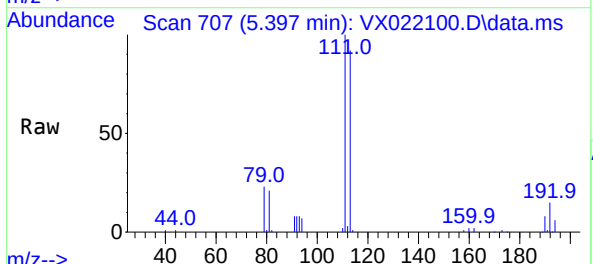

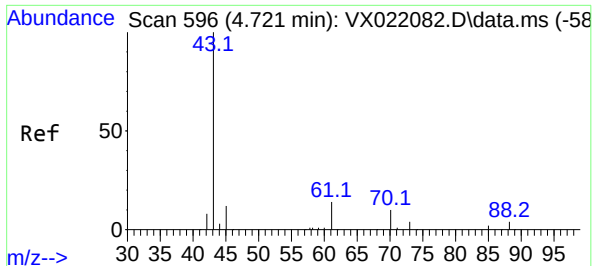

#37

Ethyl Acetate

Concen: 0.04 ug/l

RT: 4.678 min Scan# 589





Delta R.T. -0.043 min

Lab File: VX022100.D

Acq: 19 May 2021 20:05

Tgt Ion: 43	Resp: 72
Ion Ratio	Lower Upper
43 100	
61 0.0	12.8 19.2#
70 0.0	10.5 15.7#

Instrument :
MSVOA_X
ClientSampled :
VIBLK04

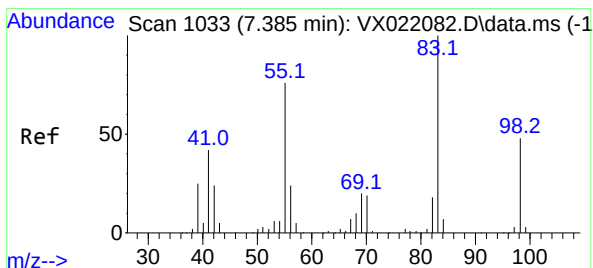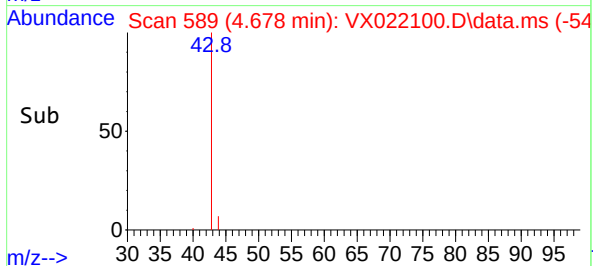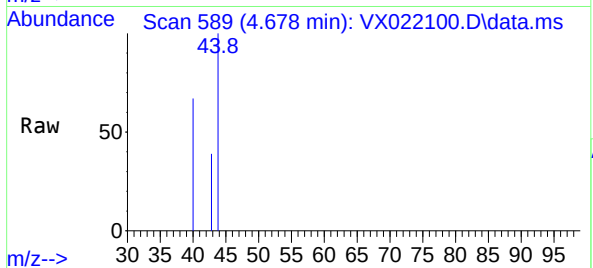

#39

Methylcyclohexane

Concen: 0.01 ug/l




RT: 7.403 min Scan# 1036


Delta R.T. 0.018 min

Lab File: VX022100.D

Acq: 19 May 2021 20:05

Tgt Ion: 83	Resp: 20
Ion Ratio	Lower Upper
83 100	
55 0.0	58.9 88.3#
98 0.0	38.1 57.1#


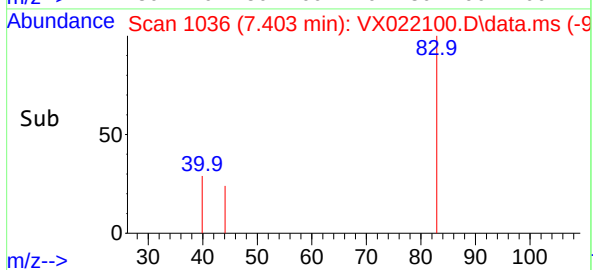

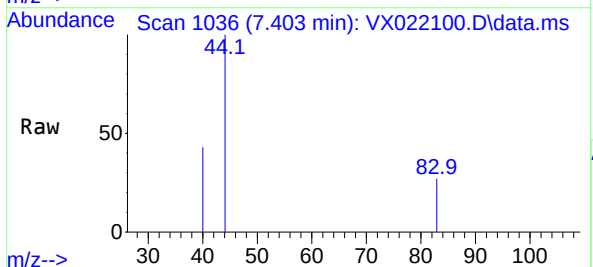


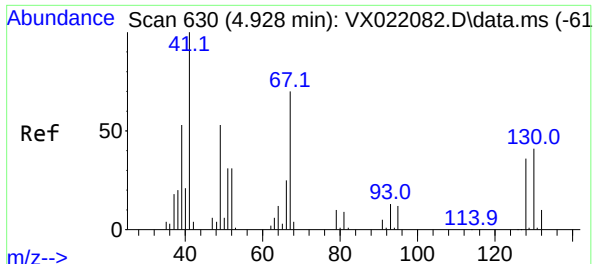

#41
Methacrylonitrile
Concen: 0.03 ug/l
RT: 4.928 min Scan# 630
Delta R.T. -0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion:	41	Resp:	31
Ion	Ratio	Lower	Upper
41	100		
39	0.0	42.5	63.7#
67	0.0	65.0	97.6#
52	0.0	25.3	37.9#

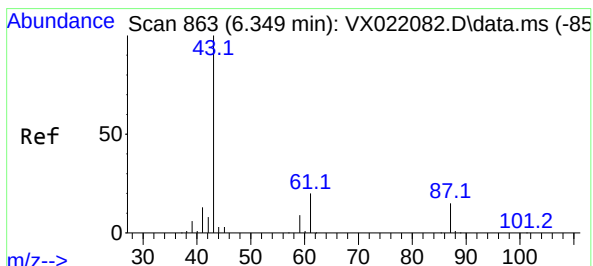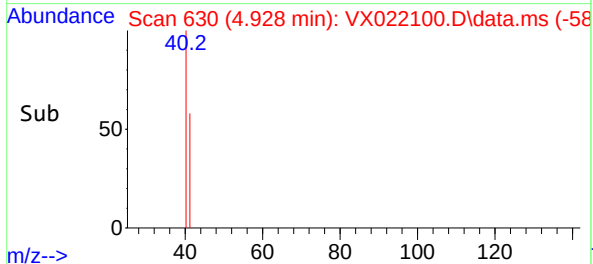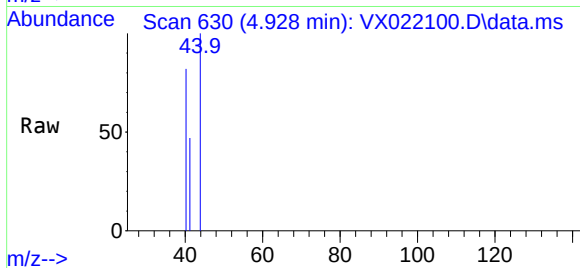

#43
Isopropyl Acetate
Concen: 0.02 ug/l
RT: 6.556 min Scan# 897
Delta R.T. 0.207 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion:	43	Resp:	53
Ion	Ratio	Lower	Upper
43	100		
61	0.0	18.2	27.4#
87	0.0	12.5	18.7#

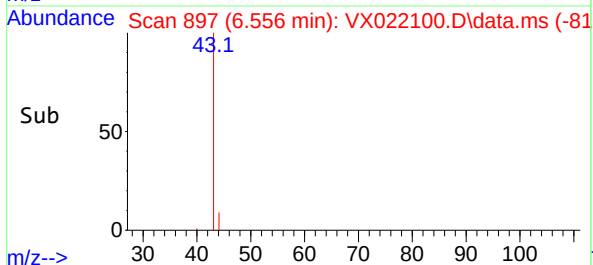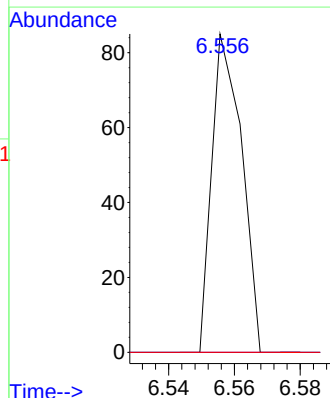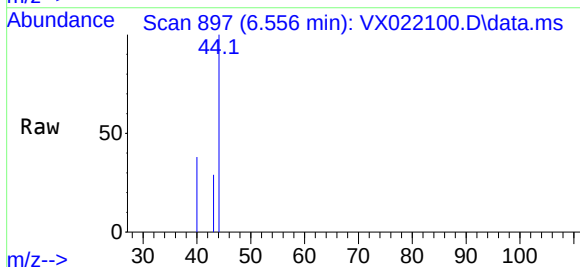

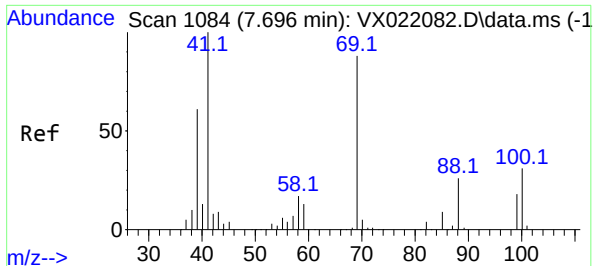

#48

Methyl methacrylate

Concen: 0.01 ug/l

RT: 7.677 min Scan# 1081

Delta R.T. -0.019 min

Lab File: VX022100.D

Acq: 19 May 2021 20:05


Tgt Ion: 41 Resp: 19

Ion Ratio Lower Upper




41 100

69 0.0 76.0 114.0#

39 421.1 44.6 67.0#

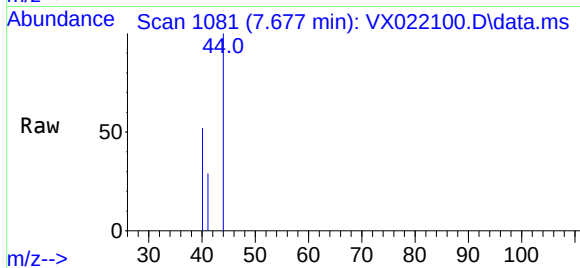

Abundance

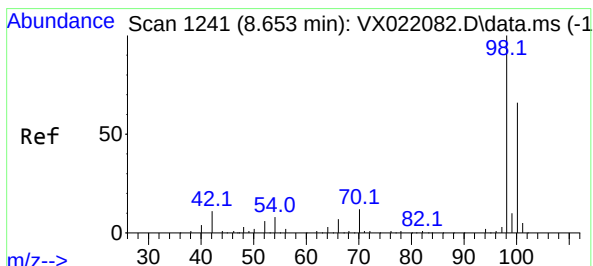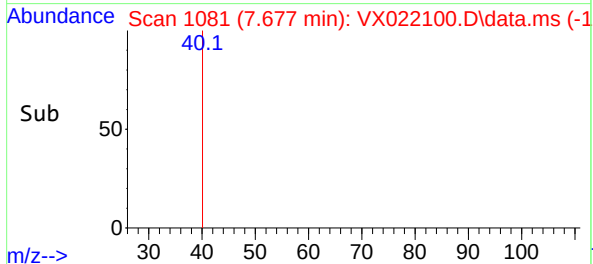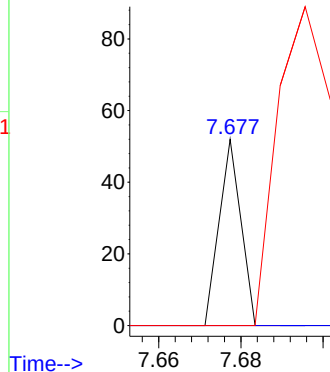

#50

Toluene-d8

Concen: 49.00 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX022100.D


Acq: 19 May 2021 20:05

Tgt Ion: 98 Resp: 194016



Ion Ratio Lower Upper

98 100

100 66.4 51.9 77.9

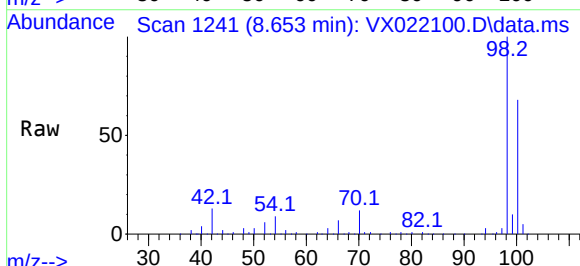

Abundance

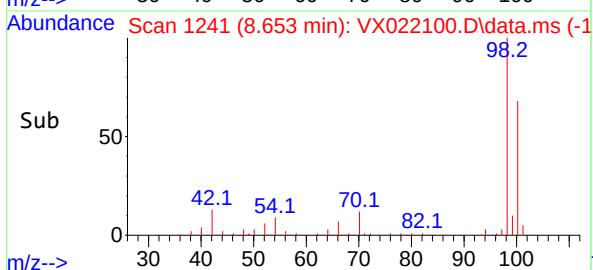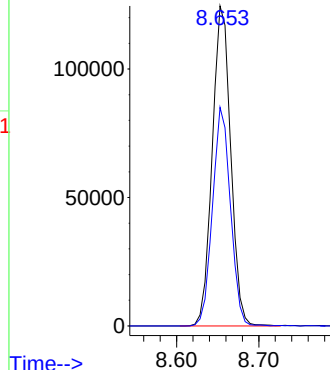


Instrument :

MSVOA_X

ClientSampleId :





VIBLK04

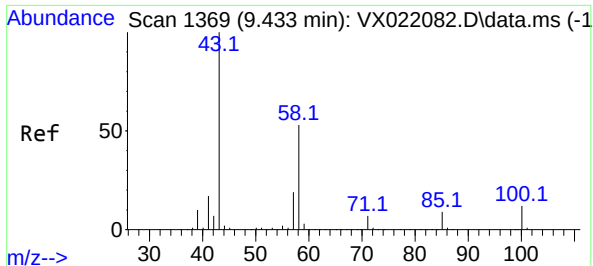

#59
2-Hexanone
Concen: 0.02 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion: 43 Resp: 24
Ion Ratio Lower Upper
43 100
58 0.0 30.9 92.8#

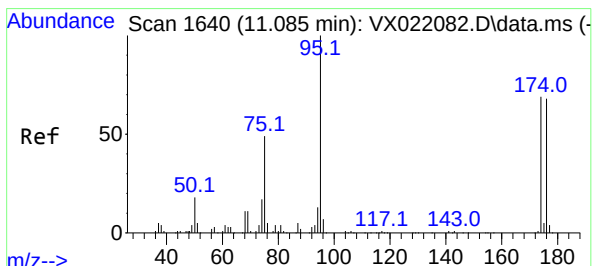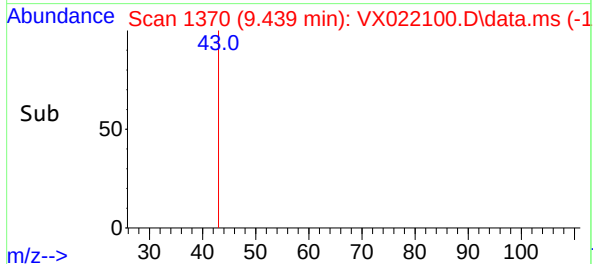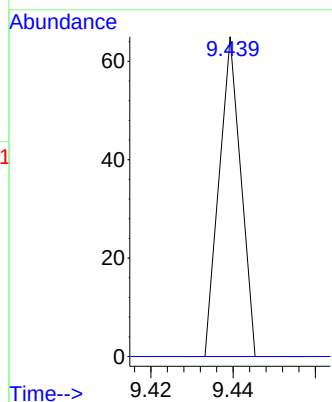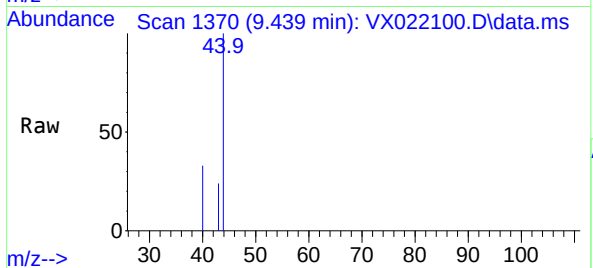

#62
4-Bromofluorobenzene
Concen: 45.51 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 95 Resp: 66595
Ion Ratio Lower Upper
95 100
174 65.4 0.0 154.6
176 64.6 0.0 155.8


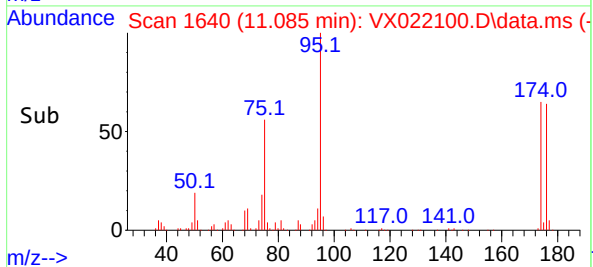
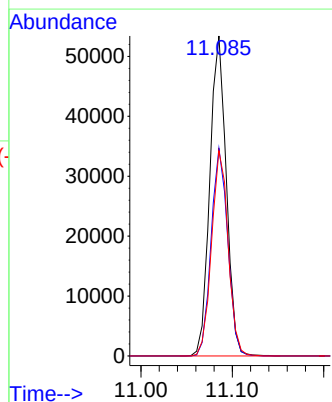
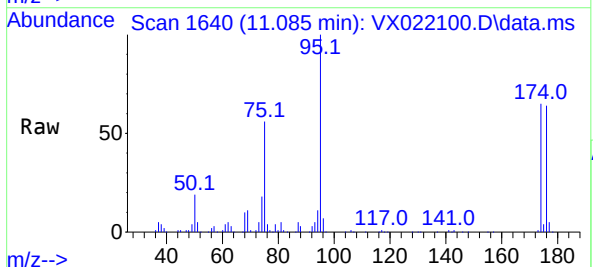




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion:117 Resp: 138507
Ion Ratio Lower Upper
117 100
82 56.1 47.4 71.2
119 31.3 26.6 39.8

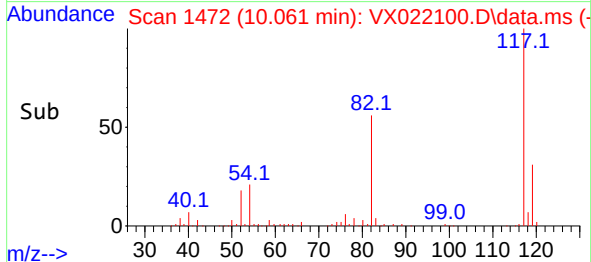

#67
Ethyl Benzene
Concen: 0.00 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 91 Resp: 19
Ion Ratio Lower Upper
91 100
106 0.0 24.6 37.0#


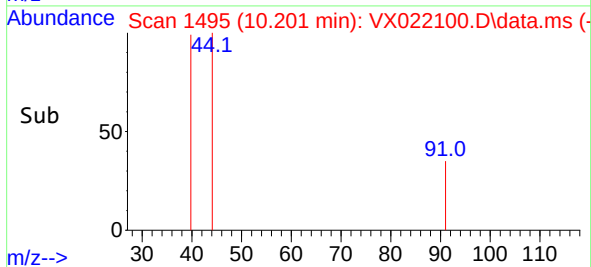

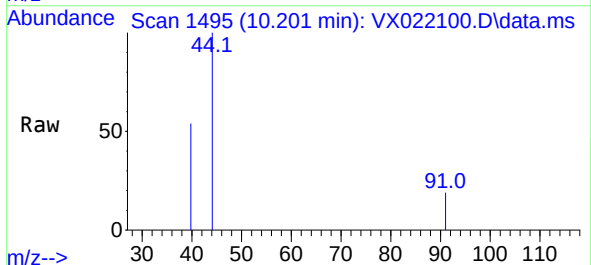




#68
m/p-Xylenes
Concen: 0.01 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampled :
VIBLK04


Tgt Ion:106 Resp: 21
Ion Ratio Lower Upper
106 100
91 757.1 162.8 244.2#

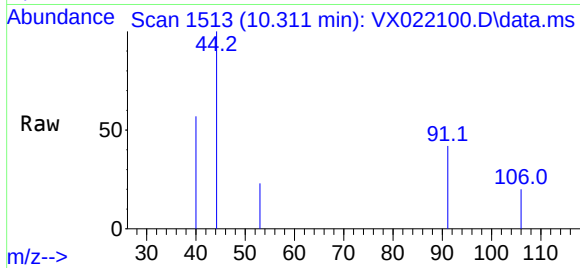

#70
Styrene
Concen: 0.01 ug/l
RT: 10.665 min Scan# 1571
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion:104 Resp: 19
Ion Ratio Lower Upper
104 100
78 0.0 40.0 60.0#
103 0.0 43.4 65.0#



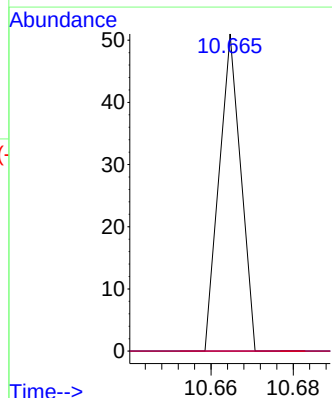
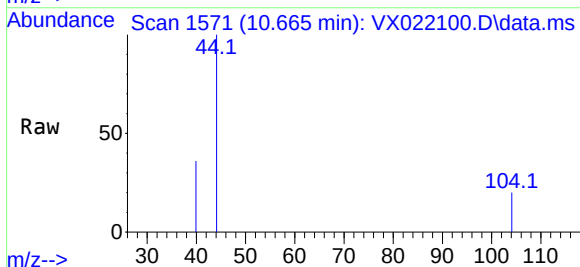




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampled :
VIBLK04


Tgt Ion:152 Resp: 54340
Ion Ratio Lower Upper
152 100
115 66.2 41.1 123.3
150 158.7 0.0 349.0

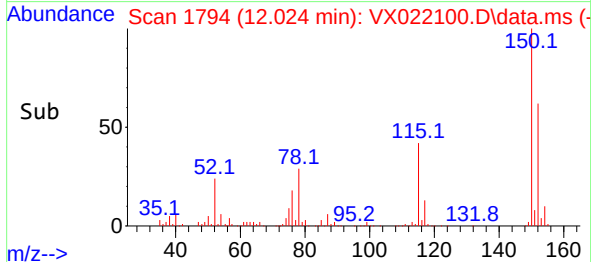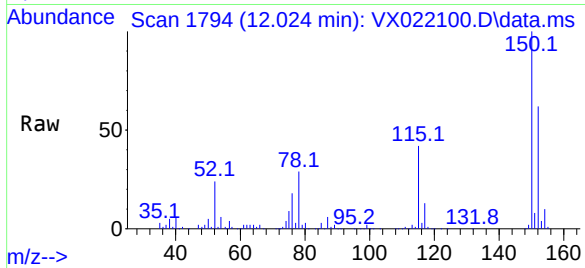

#73
Isopropylbenzene
Concen: 0.02 ug/l
RT: 10.969 min Scan# 1621
Delta R.T. 0.005 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion:105 Resp: 74
Ion Ratio Lower Upper
105 100
120 0.0 13.2 39.6#


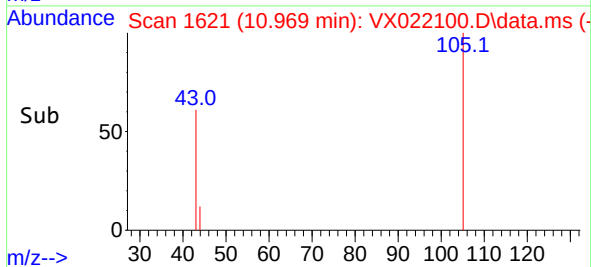

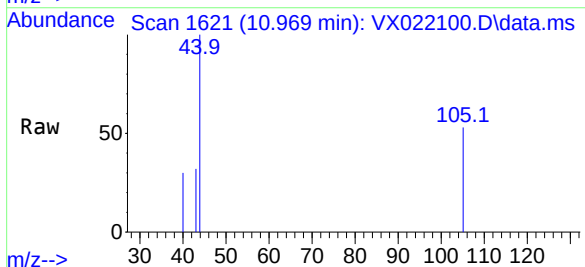




#74
N-amy1 acetate
Concen: 0.02 ug/l
RT: 10.969 min Scan# 1621
Delta R.T. 0.121 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampled :
VIBLK04


Tgt Ion: 43	Resp:	52
Ion	Ratio	Lower Upper
43	100	
70	0.0	39.0 58.6#
55	0.0	21.5 32.3#
61	0.0	22.1 33.1#

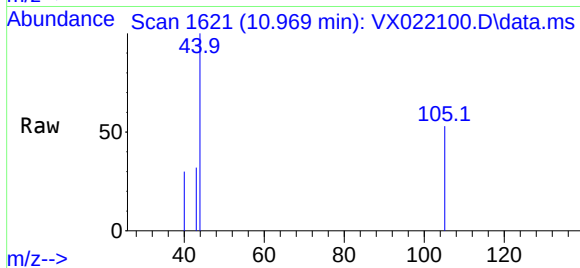

#75
1,1,2,2-Tetrachloroethane
Concen: 0.02 ug/l
RT: 11.091 min Scan# 1641
Delta R.T. -0.123 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 83	Resp:	38
Ion	Ratio	Lower Upper
83	100	
131	113.2	5.1 15.2#
85	0.0	31.8 95.4#


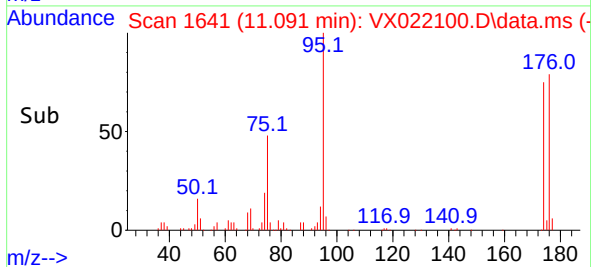

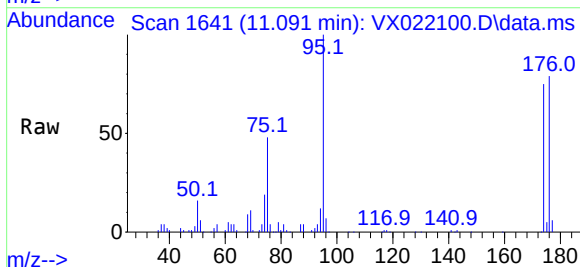




#78
n-propylbenzene
Concen: 0.03 ug/l
RT: 11.299 min Scan# 1675
Delta R.T. -0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion: 91 Resp: 158
Ion Ratio Lower Upper
91 100
120 0.0 11.5 34.5#



#79
2-Chlorotoluene
Concen: 0.03 ug/l
RT: 11.372 min Scan# 1687
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 91 Resp: 82
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


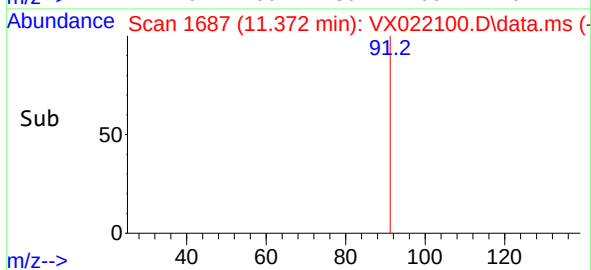

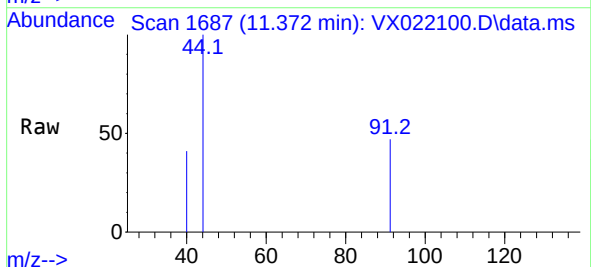




#82
4-Chlorotoluene
Concen: 0.03 ug/l
RT: 11.463 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampled :
VIBLK04


Tgt Ion: 91 Resp: 102
Ion Ratio Lower Upper
91 100
126 51.0 14.9 44.5#

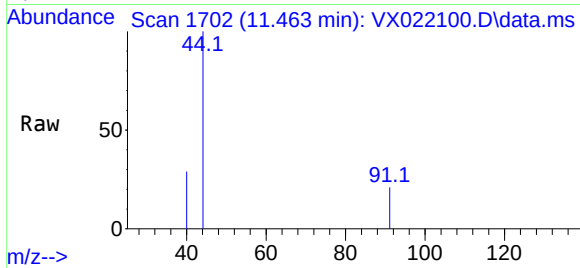

#84
1,2,4-Trimethylbenzene
Concen: 0.03 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 105 Resp: 96
Ion Ratio Lower Upper
105 100
120 45.8 22.4 67.3



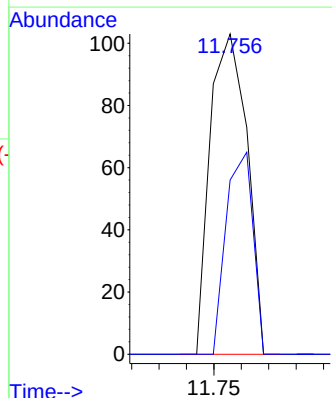
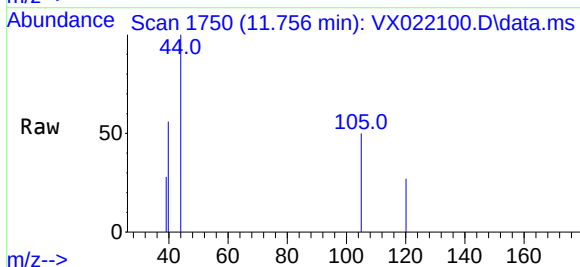




#85
sec-Butylbenzene
Concen: 0.02 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampleId :
VIBLK04


Tgt Ion:105 Resp: 116
Ion Ratio Lower Upper
105 100
134 0.0 10.0 29.8#

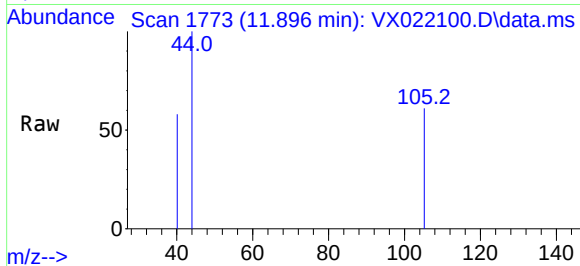

#86
p-Isopropyltoluene
Concen: 0.04 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion:119 Resp: 165
Ion Ratio Lower Upper
119 100
134 0.0 12.9 38.7#
91 0.0 11.7 35.0#


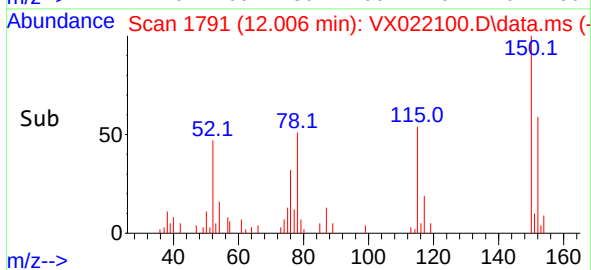

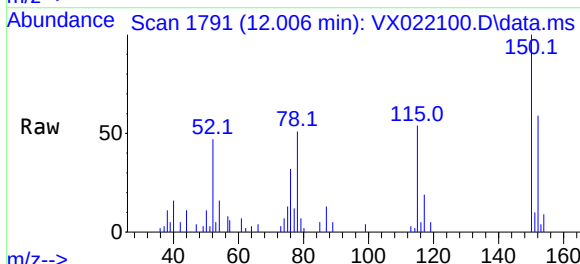




#87
1,3-Dichlorobenzene
Concen: 0.05 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.001 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampled :
VIBLK04


Tgt Ion:146 Resp: 93
Ion Ratio Lower Upper
146 100
111 0.0 20.2 60.5#
148 0.0 31.9 95.7#



#88
1,4-Dichlorobenzene
Concen: 0.04 ug/l
RT: 12.049 min Scan# 1798
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion:146 Resp: 79
Ion Ratio Lower Upper
146 100
111 1032.9 19.6 58.8#
148 574.7 31.6 95.0#


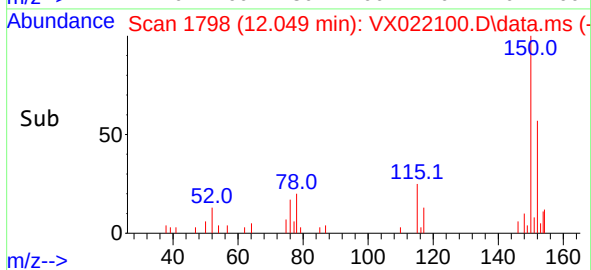






#89
n-Butylbenzene
Concen: 0.06 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05




Instrument :
MSVOA_X
ClientSampled :
VIBLK04


Tgt Ion: 91 Resp: 206
Ion Ratio Lower Upper
91 100
92 39.3 27.4 82.0
134 0.0 13.2 39.5#

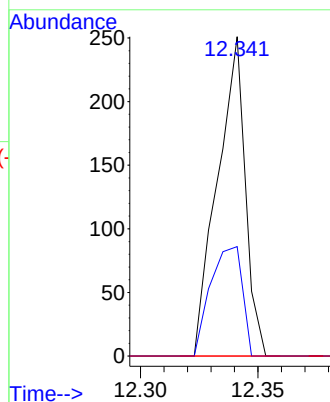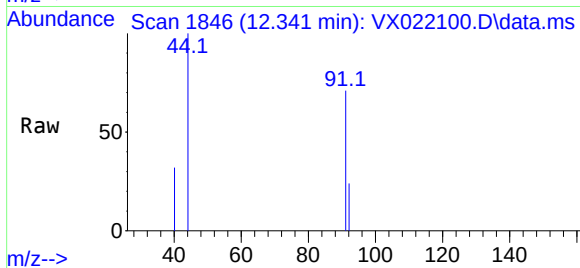

#93
1,2,4-Trichlorobenzene
Concen: 0.07 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. -0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion: 180 Resp: 73
Ion Ratio Lower Upper
180 100
182 0.0 47.7 143.1#
145 0.0 15.0 45.0#


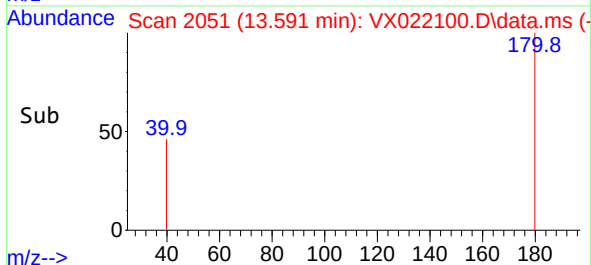

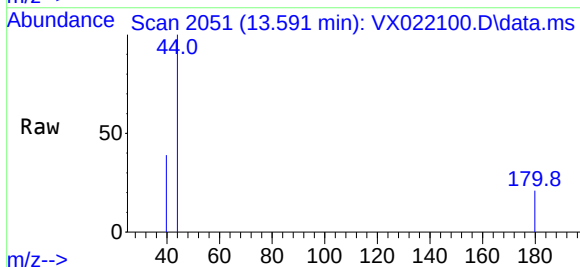




#95
Naphthalene
Concen: 0.04 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Instrument :
MSVOA_X
ClientSampleId :
VIBLK04

Tgt Ion:	128	Resp:	181
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.8	13.2#

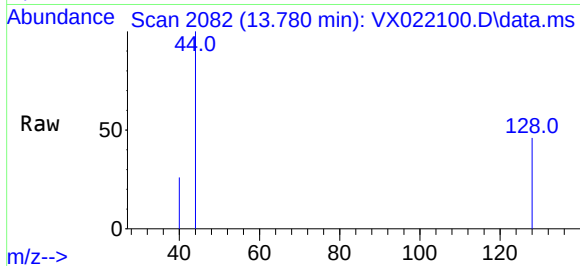

#96
1,2,3-Trichlorobenzene
Concen: 0.04 ug/l
RT: 13.969 min Scan# 2113
Delta R.T. 0.006 min
Lab File: VX022100.D
Acq: 19 May 2021 20:05

Tgt Ion:	180	Resp:	44
Ion	Ratio	Lower	Upper
180	100		
182	109.1	47.6	142.9
145	0.0	16.1	48.3#

