

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX051921\  
 Data File : VX022100.D  
 Acq On : 19 May 2021 20:05  
 Operator : JC/MD  
 Sample : M2406-04  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VIBLK04

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022100.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.397       | 694           | 707         | 719          | rBV2     | 57160          | 166528        | 31.81%          | 6.403%        |
| 2         | 5.562       | 724           | 734         | 747          | rVB      | 90969          | 253115        | 48.35%          | 9.732%        |
| 3         | 5.964       | 790           | 800         | 815          | rBV2     | 70812          | 182858        | 34.93%          | 7.031%        |
| 4         | 6.769       | 922           | 932         | 945          | rBV      | 160468         | 378912        | 72.38%          | 14.569%       |
| 5         | 8.653       | 1234          | 1241        | 1253         | rBV      | 337888         | 523510        | 100.00%         | 20.129%       |
| 6         | 10.055      | 1466          | 1471        | 1481         | rBV      | 302581         | 427412        | 81.64%          | 16.434%       |
| 7         | 11.085      | 1634          | 1640        | 1652         | rVB      | 246488         | 307248        | 58.69%          | 11.813%       |
| 8         | 12.024      | 1789          | 1794        | 1800         | rBV      | 297951         | 361256        | 69.01%          | 13.890%       |


Sum of corrected areas: 2600839

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX051921\  
Data File : VX022100.D  
Acq On : 19 May 2021 20:05  
Operator : JC/MD  
Sample : M2406-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VIBLK04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

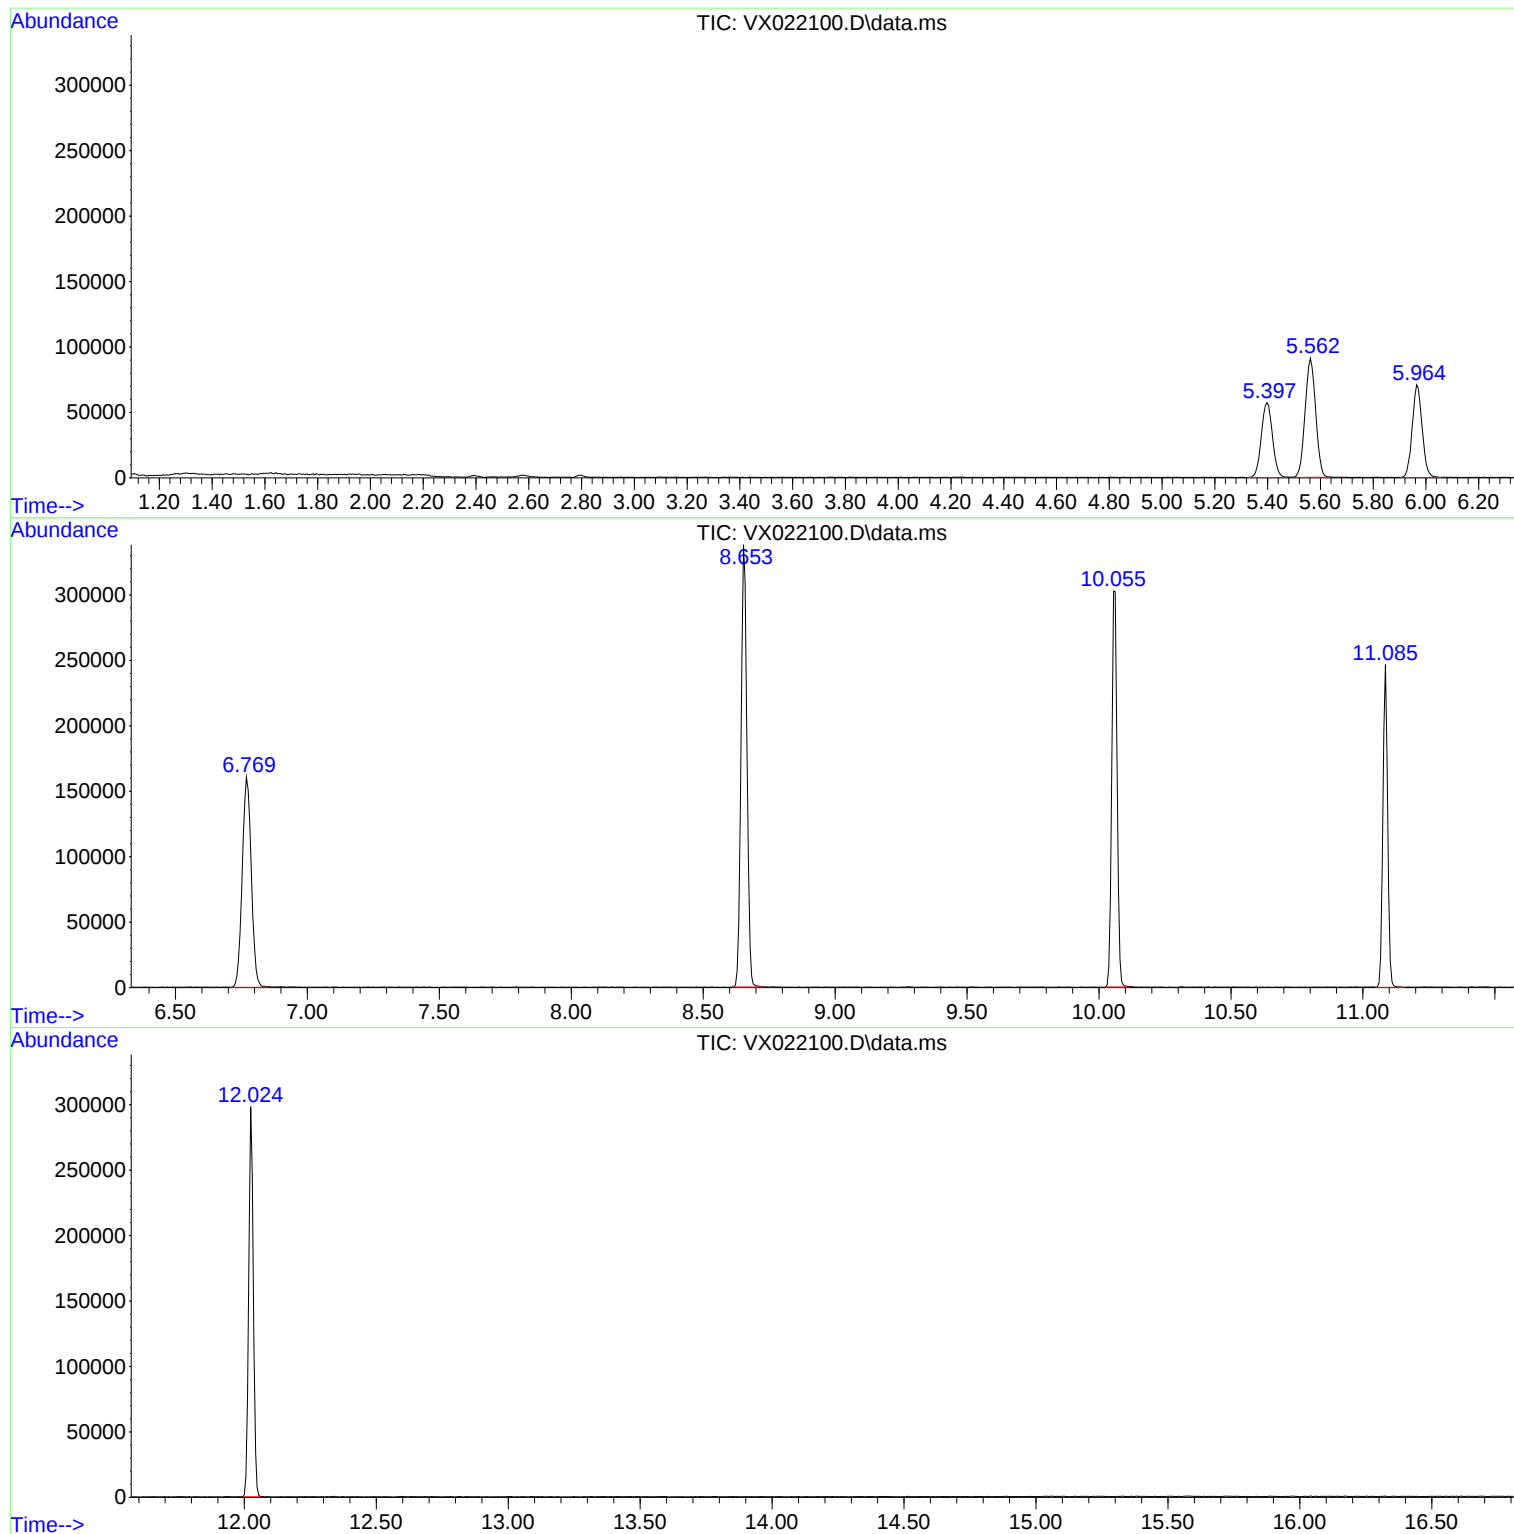

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX051921\  
Data File : VX022100.D  
Acq On : 19 May 2021 20:05  
Operator : JC/MD  
Sample : M2406-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VIBLK04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX051921\  
Data File : VX022100.D  
Acq On : 19 May 2021 20:05  
Operator : JC/MD  
Sample : M2406-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VIBLK04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----