

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
 Data File : VX028823.D
 Acq On : 19 May 2022 14:23
 Operator : JC/MD
 Sample : N2941-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 30S-20220518

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

Signal : TIC: VX028823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	42	rBV	44819	138614	8.32%	1.104%
2	2.526	229	236	248	rBV3	8312	19196	1.15%	0.153%
3	2.782	270	278	287	rBV2	13673	30961	1.86%	0.246%
4	3.105	322	331	340	rVB2	9079	21399	1.28%	0.170%
5	4.215	503	513	524	rBV3	11239	32361	1.94%	0.258%
6	5.391	695	706	722	rBV	182961	532591	31.95%	4.240%
7	5.556	722	733	756	rVB	285819	838758	50.32%	6.678%
8	5.958	789	799	816	rBV	191641	508673	30.52%	4.050%
9	6.251	836	847	859	rVB	113418	343012	20.58%	2.731%
10	6.763	920	931	946	rBV	473046	1108837	66.53%	8.828%
11	7.373	1021	1031	1040	rBV5	9040	22367	1.34%	0.178%
12	7.988	1120	1132	1143	rVB	66678	143619	8.62%	1.143%
13	8.110	1143	1152	1159	rBV	66451	130552	7.83%	1.039%
14	8.653	1227	1241	1251	rBV	952231	1545299	92.71%	12.303%
15	8.775	1256	1261	1267	rVV2	14662	23942	1.44%	0.191%
16	8.976	1289	1294	1301	rVB2	24618	39778	2.39%	0.317%
17	9.104	1306	1315	1320	rBV3	9405	17322	1.04%	0.138%
18	9.622	1394	1400	1404	rBV	24989	41083	2.46%	0.327%
19	10.055	1465	1471	1479	rBV	1258579	1666744	100.00%	13.270%
20	10.281	1503	1508	1517	rBV6	16658	37095	2.23%	0.295%
21	10.604	1546	1561	1566	rBV4	14771	39070	2.34%	0.311%
22	11.079	1634	1639	1645	rBV	874366	1113616	66.81%	8.866%
23	11.220	1658	1662	1667	rVB2	25255	33942	2.04%	0.270%
24	11.616	1718	1727	1734	rBV8	6073	16761	1.01%	0.133%
25	11.713	1734	1743	1747	rBV2	21629	33261	2.00%	0.265%
26	11.866	1760	1768	1770	rBV	39369	58348	3.50%	0.465%
27	11.890	1770	1772	1778	rVB	26902	33266	2.00%	0.265%
28	12.024	1788	1794	1800	rBV	1108271	1345434	80.72%	10.712%
29	12.177	1813	1819	1824	rVB	18917	26347	1.58%	0.210%
30	12.244	1824	1830	1834	rBV	31835	41048	2.46%	0.327%
31	12.311	1834	1841	1851	rVB7	22122	48993	2.94%	0.390%
32	12.408	1851	1857	1862	rBV	54040	71794	4.31%	0.572%
33	12.603	1880	1889	1892	rBV2	17812	28504	1.71%	0.227%
34	12.646	1892	1896	1903	rBV2	74951	133765	8.03%	1.065%
35	12.762	1912	1915	1919	rVB	29736	35731	2.14%	0.284%
36	12.817	1919	1924	1925	rVV2	50561	66059	3.96%	0.526%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
 Data File : VX028823.D
 Acq On : 19 May 2022 14:23
 Operator : JC/MD
 Sample : N2941-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 30S-20220518

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

37	12.841	1925	1928	1933	rVV	102616	128918	7.73%	1.026%
38	12.902	1933	1938	1941	rVV	52237	75257	4.52%	0.599%
39	12.933	1941	1943	1947	rVV2	21427	23870	1.43%	0.190%
40	12.988	1948	1952	1956	rVV5	12963	20388	1.22%	0.162%

41	13.036	1956	1960	1965	rVB	39042	49254	2.96%	0.392%
42	13.140	1970	1977	1982	rBV2	88497	124729	7.48%	0.993%
43	13.195	1982	1986	1990	rVB	46086	53973	3.24%	0.430%
44	13.250	1990	1995	1999	rBV	30278	44546	2.67%	0.355%
45	13.292	1999	2002	2007	rVB3	12551	18161	1.09%	0.145%

46	13.347	2007	2011	2015	rVB2	23065	28947	1.74%	0.230%
47	13.402	2015	2020	2025	rBV2	33146	57900	3.47%	0.461%
48	13.518	2035	2039	2046	rBV5	21211	44334	2.66%	0.353%
49	13.585	2046	2050	2052	rBV3	27108	38218	2.29%	0.304%
50	13.622	2052	2056	2057	rVV2	62393	81272	4.88%	0.647%

51	13.640	2057	2059	2061	rVV	76041	99164	5.95%	0.789%
52	13.664	2061	2063	2068	rVV	115892	126899	7.61%	1.010%
53	13.750	2072	2077	2081	rBV	86326	119948	7.20%	0.955%
54	13.798	2082	2085	2090	rVB2	25887	39517	2.37%	0.315%
55	13.853	2090	2094	2099	rVB2	46119	62416	3.74%	0.497%

56	13.926	2099	2106	2110	rBV2	67203	114075	6.84%	0.908%
57	13.975	2110	2114	2117	rVV2	42810	60953	3.66%	0.485%
58	14.006	2117	2119	2122	rVV	22216	25146	1.51%	0.200%
59	14.067	2126	2129	2132	rVB3	14514	16904	1.01%	0.135%
60	14.103	2132	2135	2139	rVB2	41071	43657	2.62%	0.348%

61	14.182	2141	2148	2150	rBV5	18322	31357	1.88%	0.250%
62	14.213	2150	2153	2156	rVB3	17908	19548	1.17%	0.156%
63	14.323	2167	2171	2174	rVB	40190	52562	3.15%	0.418%
64	14.371	2174	2179	2184	rVB2	34700	54590	3.28%	0.435%
65	14.420	2184	2187	2193	rVB3	12776	19020	1.14%	0.151%

66	14.487	2193	2198	2206	rBV3	53678	103671	6.22%	0.825%
67	14.585	2210	2214	2217	rBV4	14245	23806	1.43%	0.190%
68	14.676	2225	2229	2233	rBV2	42822	63232	3.79%	0.503%
69	14.725	2233	2237	2240	rVV	33639	43009	2.58%	0.342%
70	14.792	2243	2248	2252	rVV	64069	99490	5.97%	0.792%

71	14.920	2267	2269	2274	rVB5	13503	17775	1.07%	0.142%
72	14.975	2274	2278	2283	rVB7	10238	20476	1.23%	0.163%
73	15.182	2307	2312	2319	rVB3	24330	47308	2.84%	0.377%
74	15.261	2320	2325	2331	rVB6	13592	22342	1.34%	0.178%
75	15.597	2374	2380	2385	rVB	24634	37401	2.24%	0.298%

76	15.731	2396	2402	2408	rBV2	19854	38370	2.30%	0.305%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
Data File : VX028823.D
Acq On : 19 May 2022 14:23
Operator : JC/MD
Sample : N2941-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30S-20220518

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Title : SW846 8260




Sum of corrected areas: 12560545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
Data File : VX028823.D
Acq On : 19 May 2022 14:23
Operator : JC/MD
Sample : N2941-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30S-20220518

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

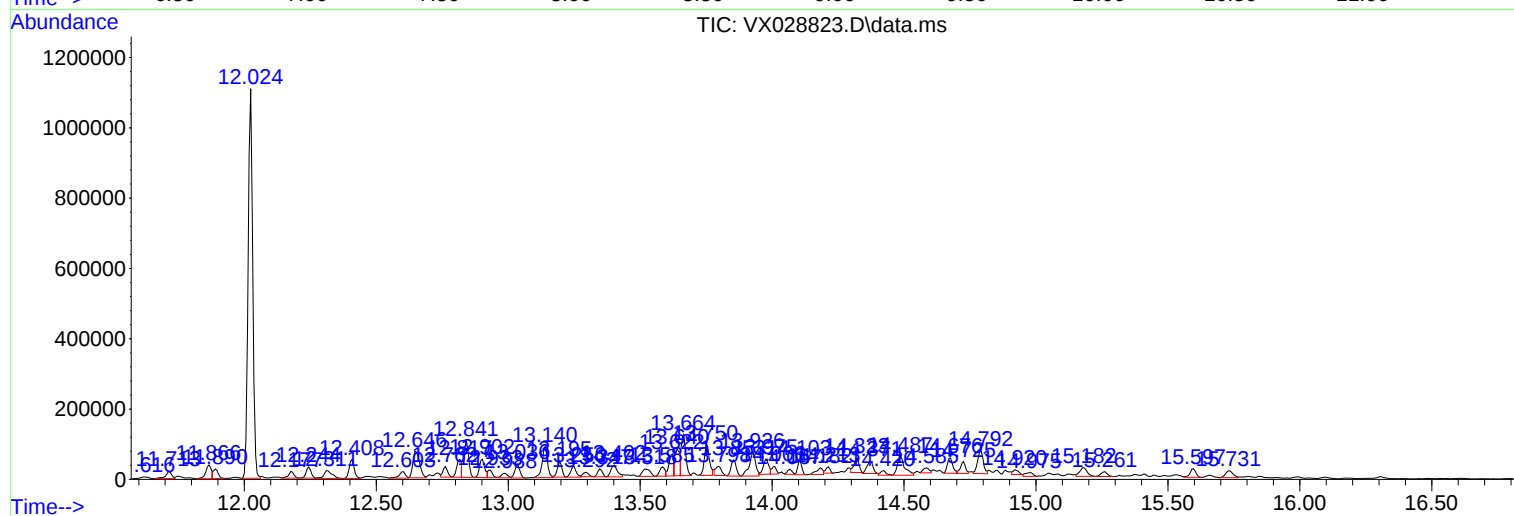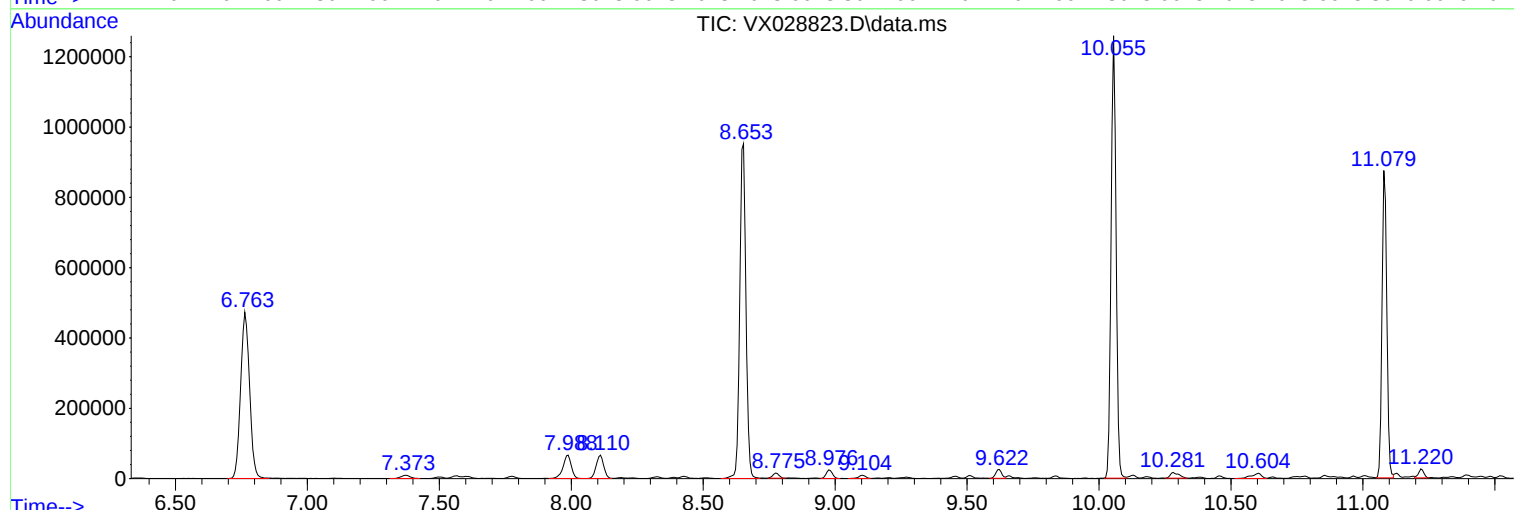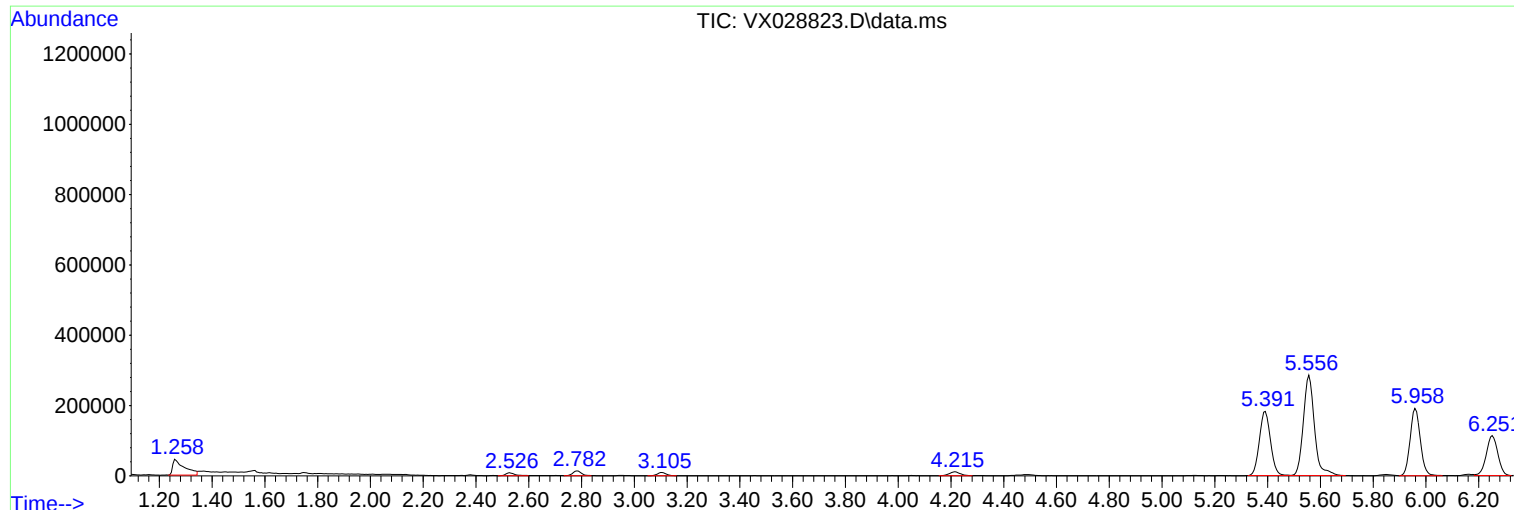

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
Data File : VX028823.D
Acq On : 19 May 2022 14:23
Operator : JC/MD
Sample : N2941-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30S-20220518

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
Data File : VX028823.D
Acq On : 19 May 2022 14:23
Operator : JC/MD
Sample : N2941-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30S-20220518

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------