

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
 Data File : VX028826.D
 Acq On : 19 May 2022 15:33
 Operator : JC/MD
 Sample : N2941-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 29S-20220518

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

Signal : TIC: VX028826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	20	27	35	rBV3	5901	15222	1.02%	0.143%
2	2.532	230	237	247	rBV	11735	23096	1.55%	0.217%
3	2.782	269	278	287	rVB3	14860	32988	2.21%	0.310%
4	4.215	503	513	524	rBV2	8858	25622	1.72%	0.241%
5	5.391	693	706	721	rBV2	178531	524225	35.14%	4.933%
6	5.556	721	733	757	rVB	279954	803189	53.84%	7.559%
7	5.958	789	799	815	rBV2	187183	499439	33.48%	4.700%
8	6.251	836	847	864	rVB	92726	278524	18.67%	2.621%
9	6.763	921	931	944	rBV	456017	1082557	72.57%	10.188%
10	7.982	1119	1131	1140	rBV	43303	93064	6.24%	0.876%
11	8.110	1144	1152	1160	rBV	47112	93542	6.27%	0.880%
12	8.653	1229	1241	1250	rBV	958420	1491797	100.00%	14.039%
13	10.055	1465	1471	1488	rBV	1049771	1375837	92.23%	12.948%
14	11.079	1634	1639	1645	rBV	817784	1062388	71.22%	9.998%
15	11.713	1734	1743	1747	rBV3	13607	21055	1.41%	0.198%
16	11.866	1762	1768	1777	rVB2	32905	56297	3.77%	0.530%
17	12.024	1788	1794	1806	rBV	1095352	1332829	89.34%	12.543%
18	12.311	1835	1841	1852	rVB	8381	23473	1.57%	0.221%
19	12.597	1882	1888	1892	rBV2	19481	28581	1.92%	0.269%
20	12.658	1892	1898	1903	rBV3	44730	72765	4.88%	0.685%
21	12.762	1912	1915	1919	rVB	25835	30803	2.06%	0.290%
22	12.817	1919	1924	1925	rBV2	49230	61685	4.13%	0.581%
23	12.841	1925	1928	1933	rVV	93627	110930	7.44%	1.044%
24	12.902	1933	1938	1940	rVV	38712	52774	3.54%	0.497%
25	12.933	1940	1943	1948	rVB2	23460	29389	1.97%	0.277%
26	13.036	1955	1960	1970	rVB	30275	40648	2.72%	0.383%
27	13.140	1970	1977	1982	rBV	31484	49662	3.33%	0.467%
28	13.195	1982	1986	1990	rVB	40575	49686	3.33%	0.468%
29	13.250	1990	1995	2001	rBV	30968	47491	3.18%	0.447%
30	13.347	2007	2011	2015	rVB2	27461	34064	2.28%	0.321%
31	13.402	2015	2020	2026	rBV2	27642	47084	3.16%	0.443%
32	13.530	2035	2041	2046	rBV4	17233	33367	2.24%	0.314%
33	13.579	2046	2049	2052	rBV3	18243	25741	1.73%	0.242%
34	13.622	2052	2056	2058	rVV2	56678	89836	6.02%	0.845%
35	13.664	2060	2063	2067	rVB	90333	110108	7.38%	1.036%
36	13.750	2072	2077	2082	rBV	110689	151248	10.14%	1.423%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
 Data File : VX028826.D
 Acq On : 19 May 2022 15:33
 Operator : JC/MD
 Sample : N2941-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 29S-20220518

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
 Title : SW846 8260

37	13.853	2090	2094	2098	rVB4	11799	19749	1.32%	0.186%
38	13.902	2098	2102	2103	rBV3	13640	14987	1.00%	0.141%
39	13.926	2103	2106	2110	rVV2	23922	32155	2.16%	0.303%
40	13.975	2110	2114	2117	rVV2	39555	55576	3.73%	0.523%
41	14.006	2117	2119	2122	rVV	16254	18629	1.25%	0.175%
42	14.067	2126	2129	2132	rVB2	13269	16061	1.08%	0.151%
43	14.103	2132	2135	2139	rBV2	26282	30212	2.03%	0.284%
44	14.292	2163	2166	2168	rBV3	13074	18380	1.23%	0.173%
45	14.323	2168	2171	2174	rVB2	22410	28385	1.90%	0.267%
46	14.371	2174	2179	2186	rVB4	26717	48125	3.23%	0.453%
47	14.487	2193	2198	2206	rBV3	29808	59354	3.98%	0.559%
48	14.585	2210	2214	2220	rVV5	14143	29692	1.99%	0.279%
49	14.676	2224	2229	2233	rBV2	39906	60456	4.05%	0.569%
50	14.725	2233	2237	2240	rVV	29635	37422	2.51%	0.352%
51	14.792	2243	2248	2252	rVB	58638	85856	5.76%	0.808%
52	15.176	2307	2311	2320	rVB7	17393	34345	2.30%	0.323%
53	15.262	2320	2325	2330	rBV3	14181	21780	1.46%	0.205%
54	15.597	2375	2380	2385	rVB2	25388	37285	2.50%	0.351%
55	15.731	2396	2402	2407	rBV2	16332	29692	1.99%	0.279%
56	16.328	2489	2500	2508	rVB2	21813	46955	3.15%	0.442%


Sum of corrected areas: 10626102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
Data File : VX028826.D
Acq On : 19 May 2022 15:33
Operator : JC/MD
Sample : N2941-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
29S-20220518

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

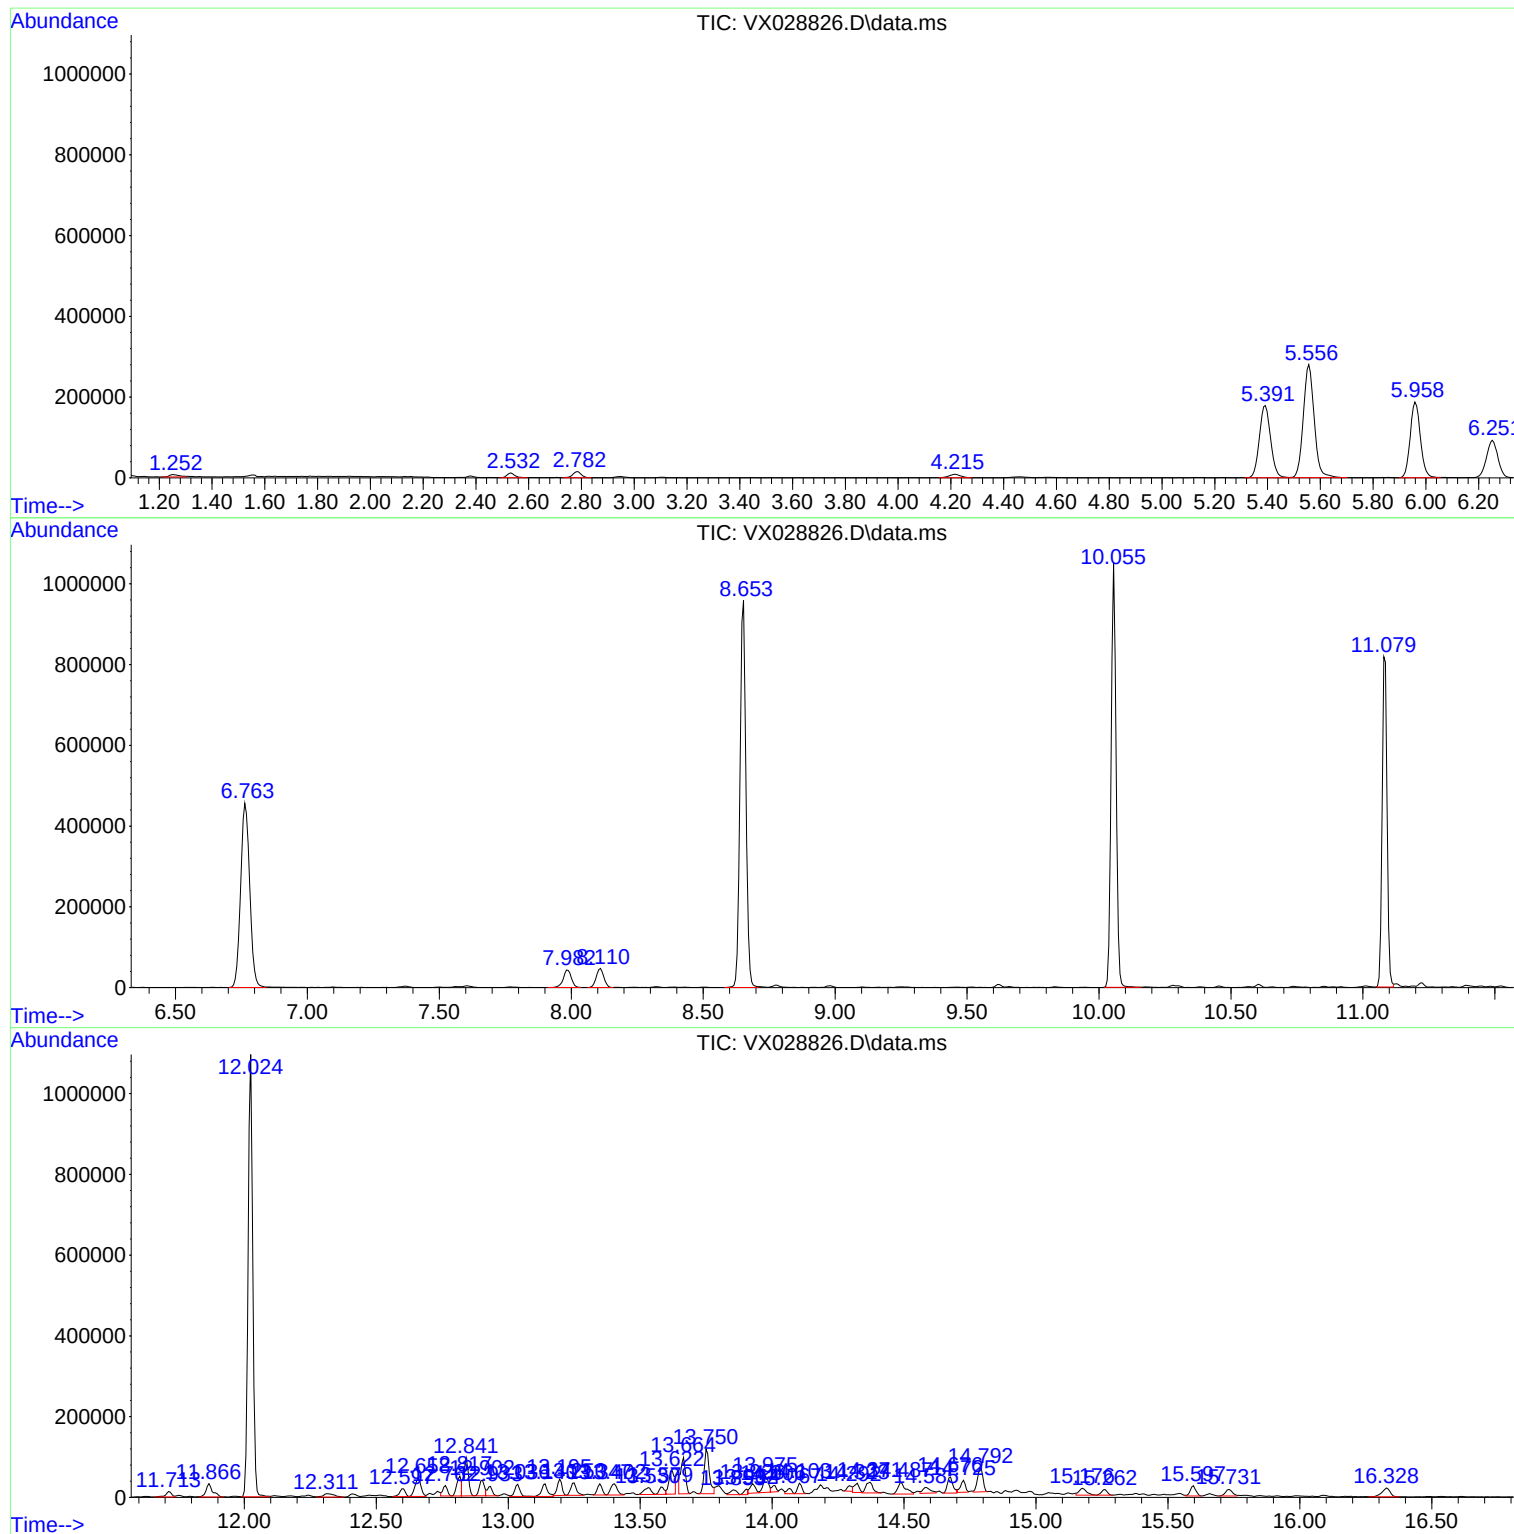

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
Data File : VX028826.D
Acq On : 19 May 2022 15:33
Operator : JC/MD
Sample : N2941-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
29S-20220518

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051922\
Data File : VX028826.D
Acq On : 19 May 2022 15:33
Operator : JC/MD
Sample : N2941-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
29S-20220518

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------