

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051923\
 Data File : VX035761.D
 Acq On : 19 May 2023 15:31
 Operator : JC/MD
 Sample : 02860-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-PRO-10-131-05152023

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M

Title : SW846 8260

Signal : TIC: VX035761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	20	rVB	45158	55344	2.85%	0.879%
2	2.294	192	198	208	rBV	26410	49526	2.55%	0.787%
3	5.385	693	705	718	rBV	88508	257080	13.23%	4.085%
4	5.550	723	732	744	rVB	159054	443458	22.82%	7.046%
5	5.958	787	799	813	rBV	118938	324237	16.69%	5.152%
6	6.763	921	931	948	rVB	250810	604636	31.12%	9.607%
7	7.123	980	990	1007	rBV	893829	1943151	100.00%	30.875%
8	7.580	1059	1065	1075	rBV2	14072	31310	1.61%	0.497%
9	8.647	1233	1240	1249	rBV	500594	787424	40.52%	12.511%
10	9.519	1377	1383	1395	rBV	67071	99427	5.12%	1.580%
11	10.055	1465	1471	1482	rBV	498814	670601	34.51%	10.655%
12	11.079	1633	1639	1650	rVB	384066	482963	24.85%	7.674%
13	12.018	1788	1793	1804	rVB	421846	544526	28.02%	8.652%




Sum of corrected areas: 6293683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051923\
Data File : VX035761.D
Acq On : 19 May 2023 15:31
Operator : JC/MD
Sample : 02860-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-10-131-05152023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

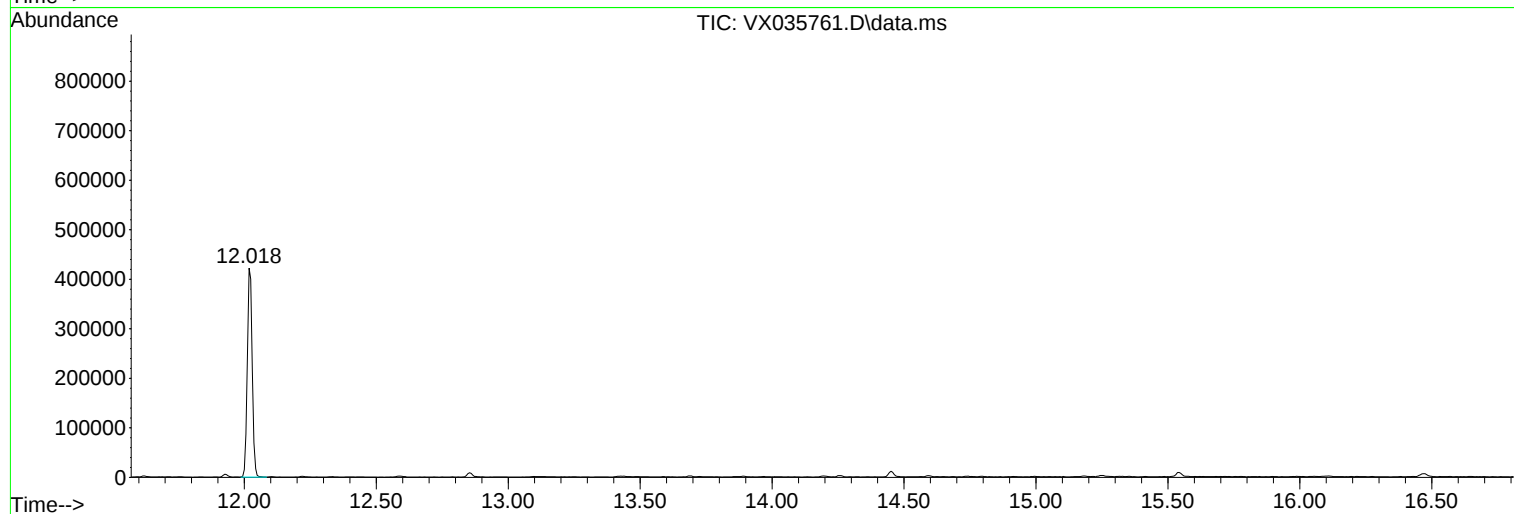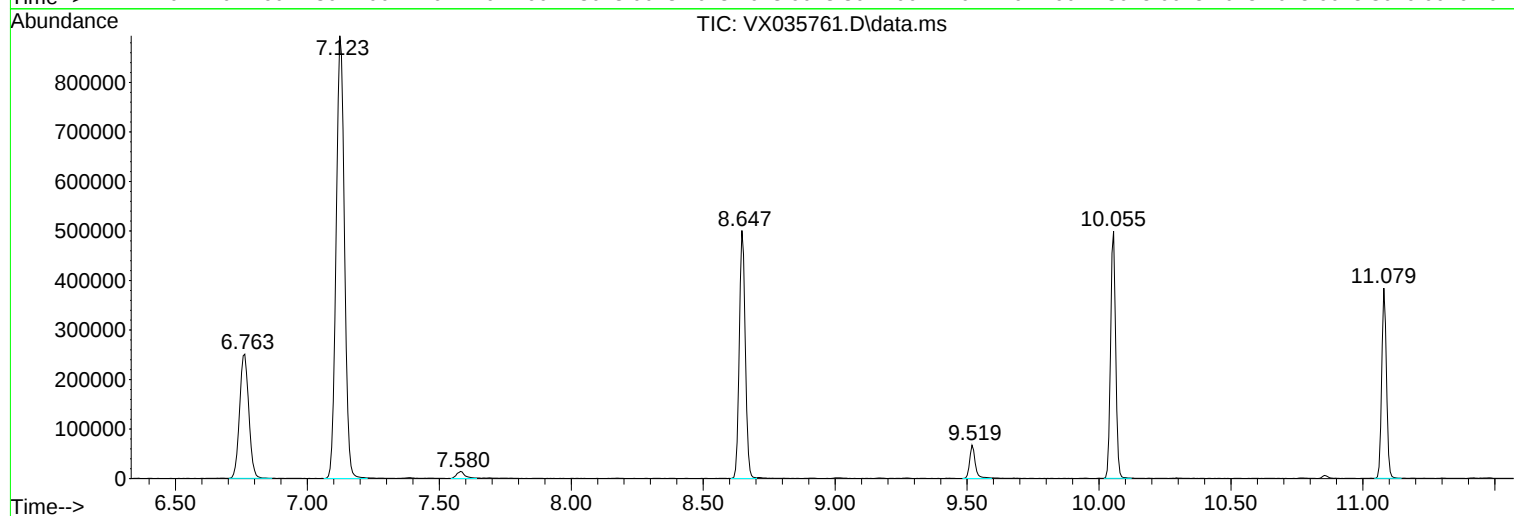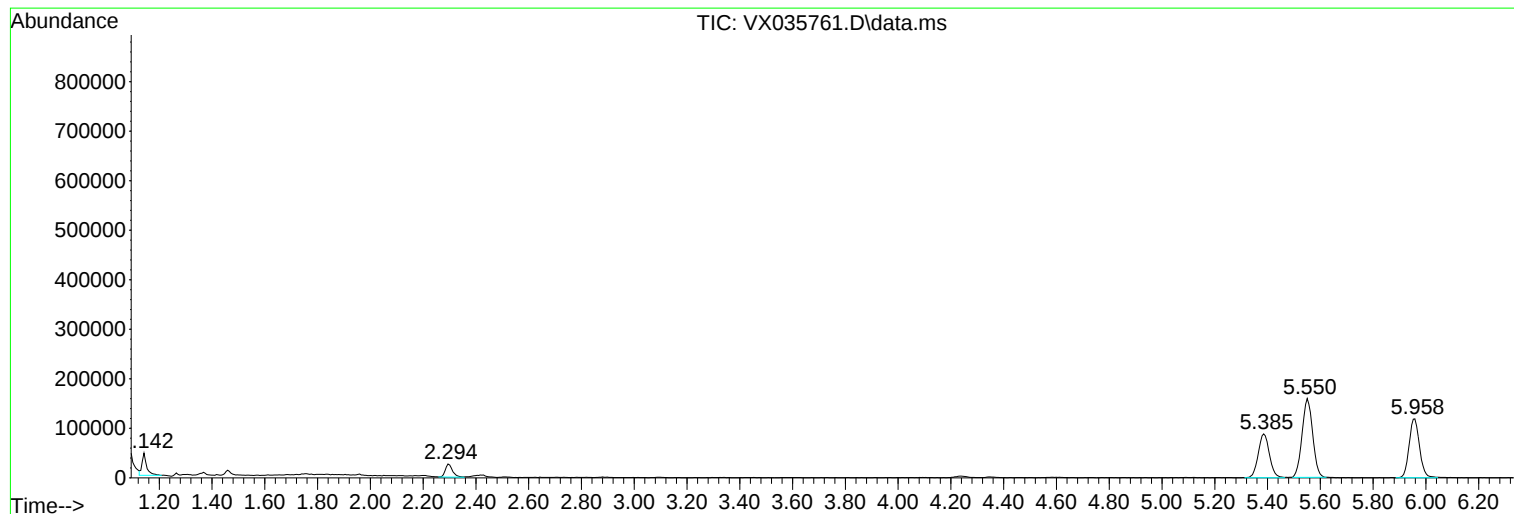

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051923\
Data File : VX035761.D
Acq On : 19 May 2023 15:31
Operator : JC/MD
Sample : 02860-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-10-131-05152023










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Hexanal Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.519	7.41 ug/l	99427	Chlorobenzene-d5	10.055

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanal	100	C6H12O	000066-25-1	72
2			2,2-Dimethyl-3-hydroxypropionald...	102	C5H10O2	000597-31-9	32
3			Butanal	72	C4H8O	000123-72-8	30
4			1-Pentene, 2-methyl-	84	C6H12	000763-29-1	25
5			Aziridine, 2-methyl-	57	C3H7N	000075-55-8	22

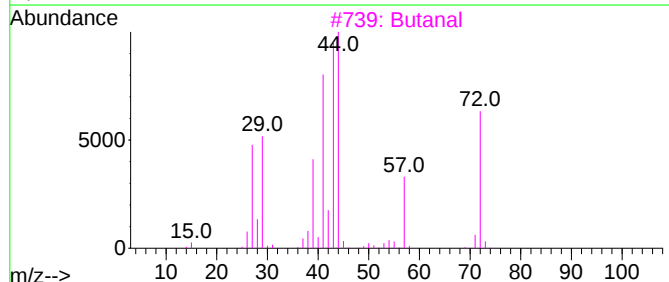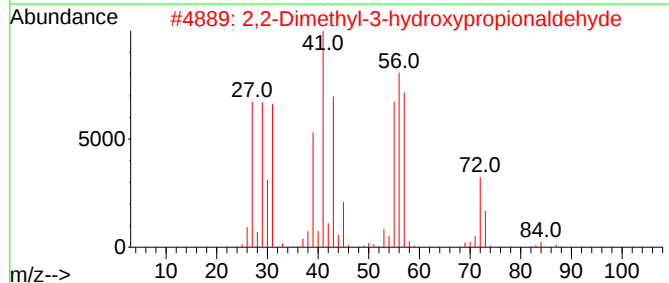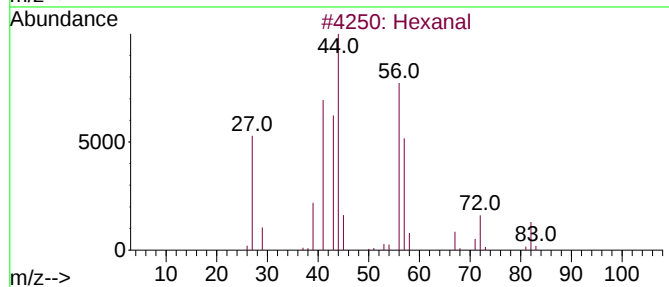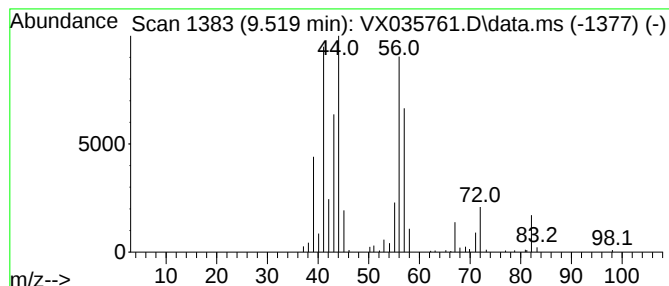

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051923\
Data File : VX035761.D
Acq On : 19 May 2023 15:31
Operator : JC/MD
Sample : 02860-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-PRO-10-131-05152023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanal	9.519	7.4	ug/l	99427	3	10.055	670601	50.0