

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051925\
 Data File : VX046272.D
 Acq On : 19 May 2025 16:58
 Operator : JC/MD
 Sample : Q2053-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3

Quant Time: May 19 23:14:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	61346	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	120549	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	113135	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	47691	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	60409	52.820	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 105.640%			
35) Dibromofluoromethane	5.385	113	44028	50.719	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.440%			
50) Toluene-d8	8.647	98	152955	50.908	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.820%			
62) 4-Bromofluorobenzene	11.079	95	58496	50.756	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 101.520%			
Target Compounds						Qvalue
3) Chloromethane	1.355	50	187	0.205	ug/l #	43
11) Tert butyl alcohol	2.977	59	1982	12.346	ug/l #	90
13) Acrolein	2.239	56	249	1.362	ug/l #	44
14) Allyl chloride	2.636	41	298	0.214	ug/l #	50
16) Acetone	2.380	43	26130	56.982	ug/l	100
17) Carbon Disulfide	2.502	76	606	0.351	ug/l #	73
18) Methyl Acetate	2.709	43	3566	3.351	ug/l	94
20) Methylene Chloride	2.788	84	11829	13.461	ug/l #	87
25) 2-Butanone	4.574	43	8059	12.105	ug/l	97
31) Cyclohexane	5.544	56	1831	1.343	ug/l #	12
36) 1,1-Dichloropropene	5.538	75	6037	5.176	ug/l #	50
37) Ethyl Acetate	4.757	43	312	0.217	ug/l #	70
38) Carbon Tetrachloride	5.550	117	7362	5.618	ug/l #	20
40) Benzene	6.038	78	5746	1.682	ug/l	93
43) Isopropyl Acetate	6.348	43	14490	6.591	ug/l	99
48) Methyl methacrylate	7.793	41	58354	51.975	ug/l #	49
49) 1,4-Dioxane	7.787	88	125	5.864	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	46691	31.997	ug/l #	47
52) Toluene	8.714	92	7707	3.679	ug/l	99
54) cis-1,3-Dichloropropene	8.549	75	17772	13.709	ug/l #	64
57) 1,3-Dichloropropane	9.482	76	1647	1.110	ug/l #	42
59) 2-Hexanone	9.378	43	10816	10.018	ug/l #	28
67) Ethyl Benzene	10.195	91	2173	0.498	ug/l	92
68) m/p-Xylenes	10.299	106	3210	2.011	ug/l	94
69) o-Xylene	10.640	106	2105	1.352	ug/l	97
70) Styrene	10.665	104	1036	0.406	ug/l #	60
74) N-amyl acetate	10.860	43	594	0.324	ug/l #	30
76) 1,2,3-Trichloropropane	11.079	75	32704	28.489	ug/l #	36
80) 1,3,5-Trimethylbenzene	11.451	105	888	0.286	ug/l	92
81) trans-1,4-Dichloro-2-b...	11.079	75	32704	92.752	ug/l #	1
84) 1,2,4-Trimethylbenzene	11.756	105	3561	1.134	ug/l	68
90) Hexachloroethane	12.603	117	115	0.206	ug/l #	19
95) Naphthalene	13.774	128	66904	20.118	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
SB-3

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051925\
Data File : VX046272.D
Acq On : 19 May 2025 16:58
Operator : JC/MD
Sample : Q2053-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-3

Quant Time: May 19 23:14:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




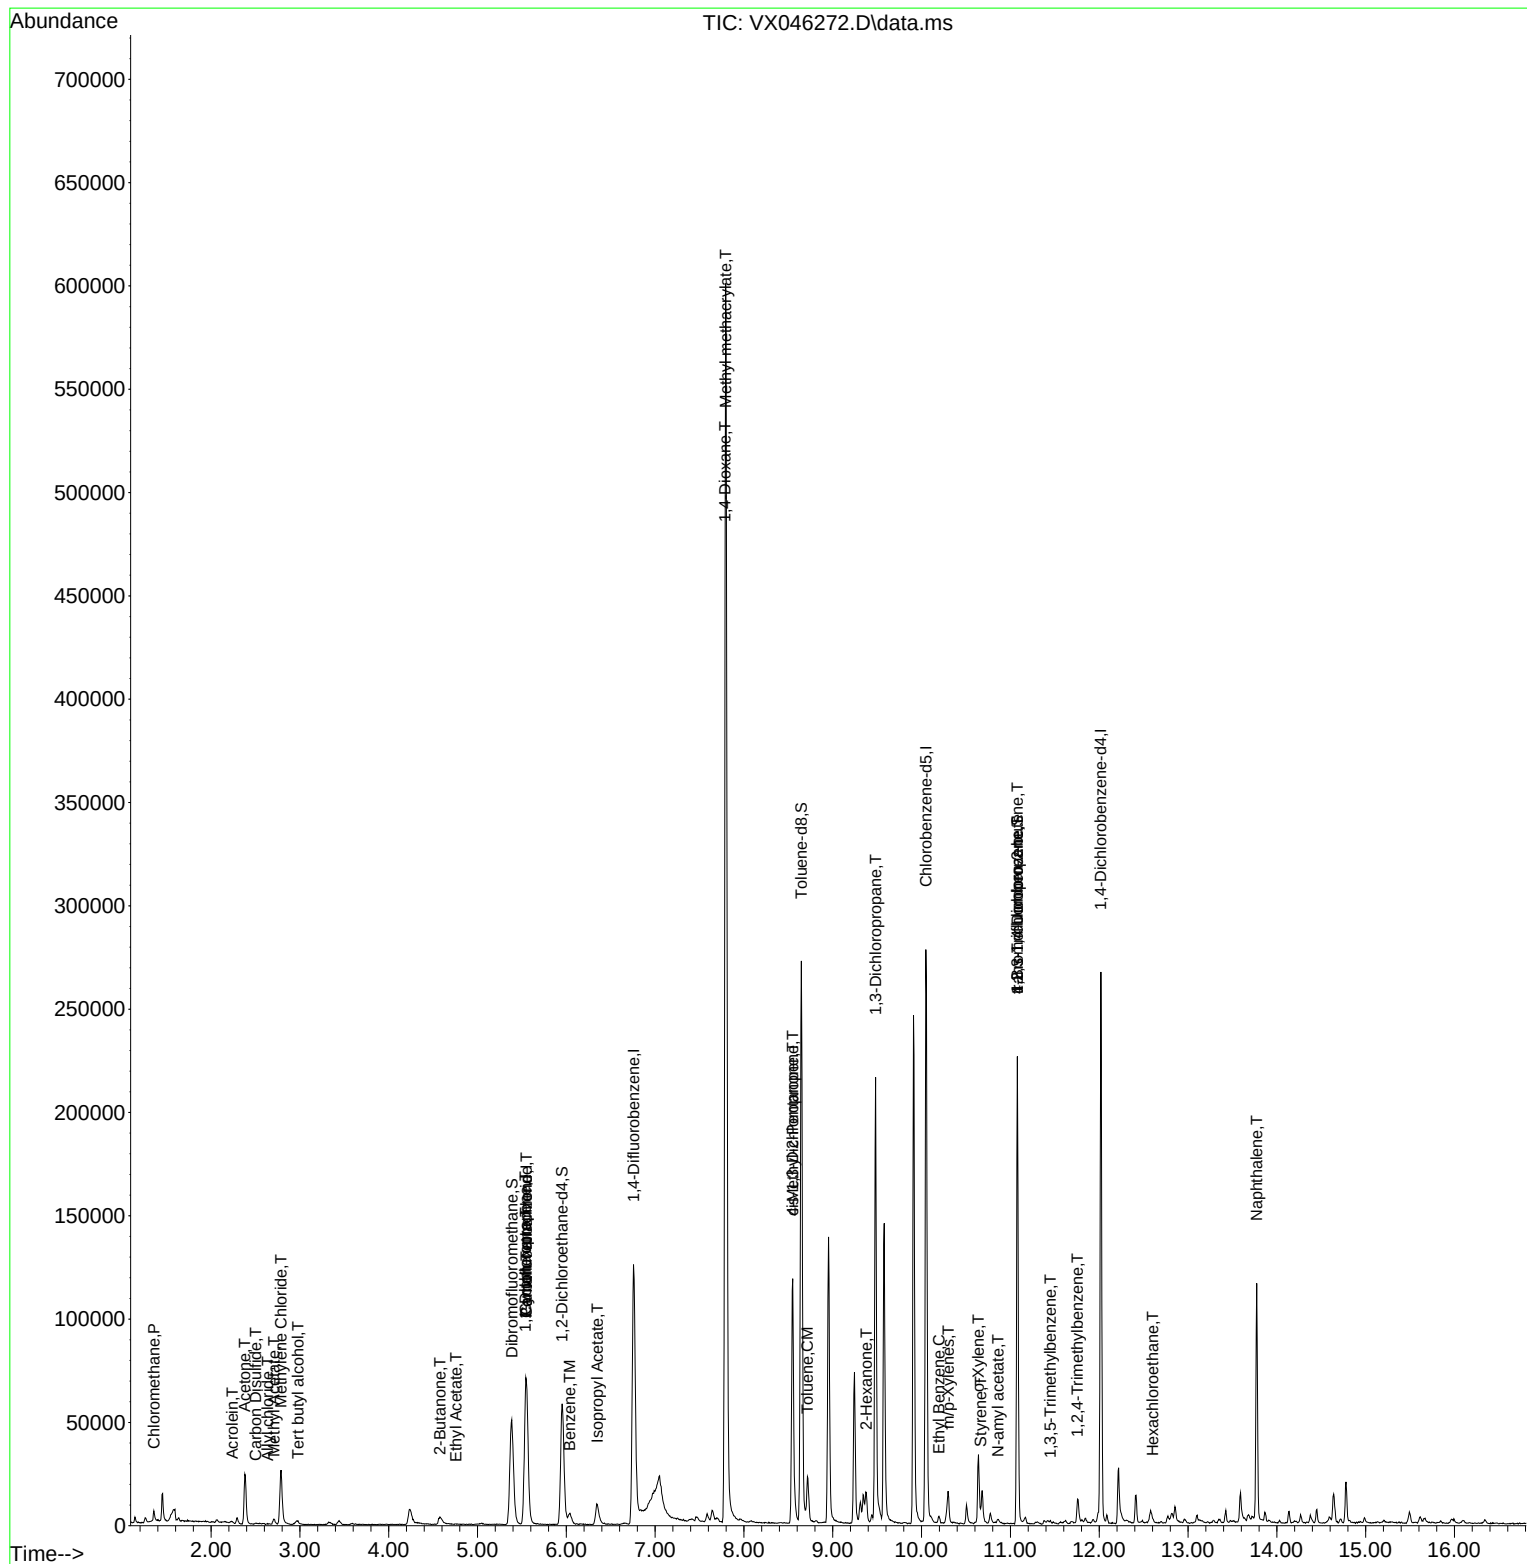




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion:168 Resp: 61346
Ion Ratio Lower Upper
168 100
99 67.0 54.9 82.3

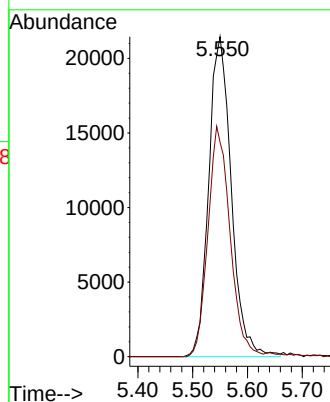

#3
Chloromethane
Concen: 0.205 ug/l
RT: 1.355 min Scan# 44
Delta R.T. 0.049 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion: 50 Resp: 187
Ion Ratio Lower Upper
50 100
52 0.0 25.4 38.2#

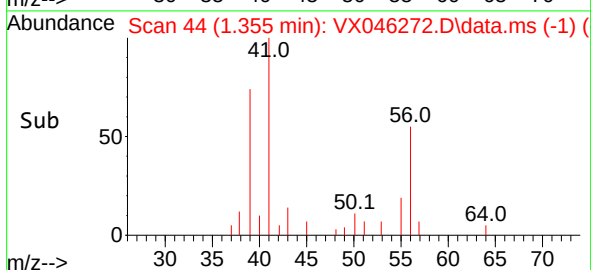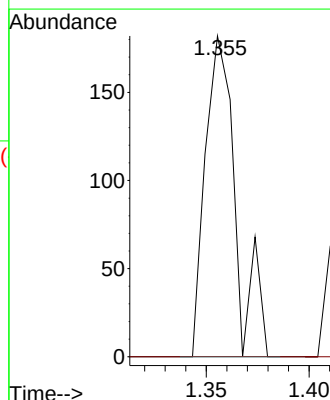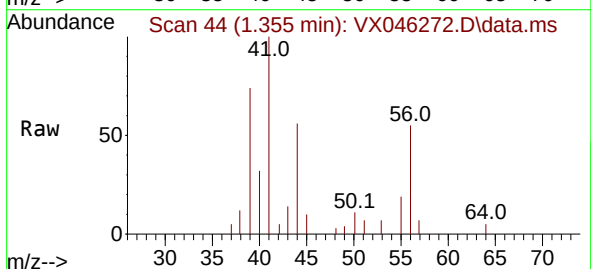



#11

Tert butyl alcohol

Concen: 12.346 ug/l

RT: 2.977 min Scan# 310

Delta R.T. -0.000 min

Lab File: VX046272.D

Acq: 19 May 2025 16:58

Instrument :

MSVOA_X

ClientSampleId :





SB-3

Tgt Ion: 59 Resp: 1982

Ion Ratio Lower Upper

59 100

57 6.8 8.6 12.8#

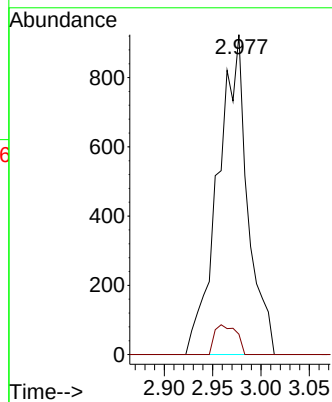

#13

Acrolein

Concen: 1.362 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.006 min

Lab File: VX046272.D




Acq: 19 May 2025 16:58


Tgt Ion: 56 Resp: 249

Ion Ratio Lower Upper

56 100

55 116.5 56.2 84.4#


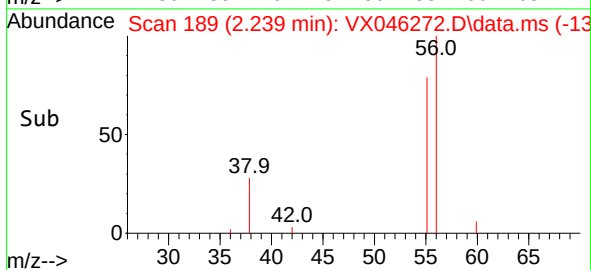






#14
 Allyl chloride
 Concen: 0.214 ug/l
 RT: 2.636 min Scan# 212
 Delta R.T. -0.018 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3


Tgt Ion: 41 Resp: 298
 Ion Ratio Lower Upper
 41 100
 39 35.2 60.6 90.8#
 76 0.0 24.9 37.3#

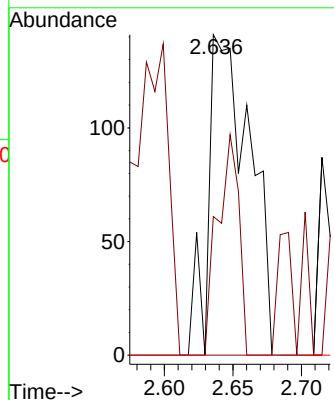

#16
 Acetone
 Concen: 56.982 ug/l
 RT: 2.380 min Scan# 212
 Delta R.T. -0.006 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58

Tgt Ion: 43 Resp: 26130
 Ion Ratio Lower Upper
 43 100
 58 26.5 21.2 31.8

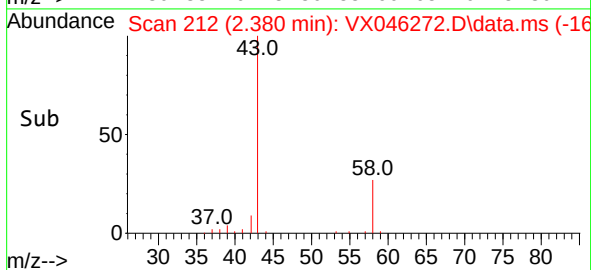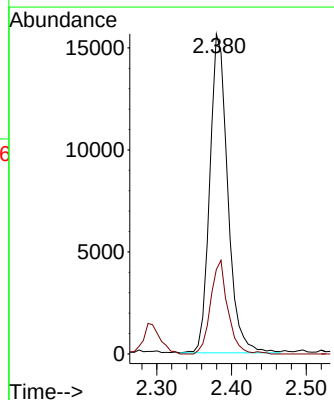



#17

Carbon Disulfide

Concen: 0.351 ug/l

RT: 2.502 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX046272.D

Acq: 19 May 2025 16:58

Instrument :

MSVOA_X

ClientSampleId :





SB-3

Tgt Ion: 76 Resp: 606

Ion Ratio Lower Upper

76 100

78 18.4 7.0 10.4#

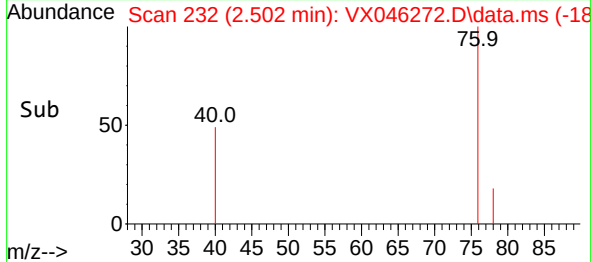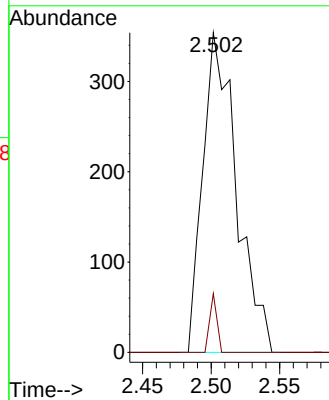

#18

Methyl Acetate

Concen: 3.351 ug/l

RT: 2.709 min Scan# 266

Delta R.T. 0.006 min

Lab File: VX046272.D




Acq: 19 May 2025 16:58


Tgt Ion: 43 Resp: 3566

Ion Ratio Lower Upper

43 100

74 18.2 16.7 25.1


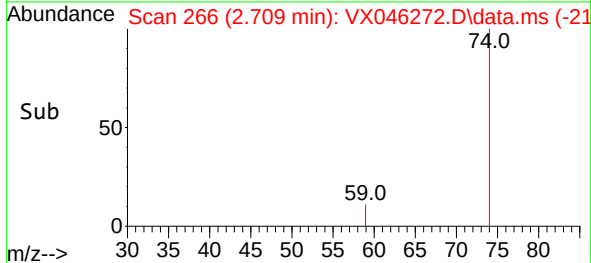
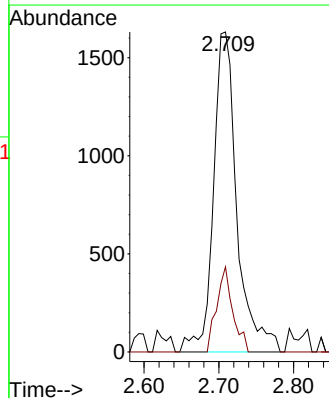





#20
Methylene Chloride
Concen: 13.461 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion:	84	Resp:	11829
Ion	Ratio	Lower	Upper
84	100		
49	127.4	113.9	170.9
51	46.0	33.5	50.3
86	53.2	53.8	80.8

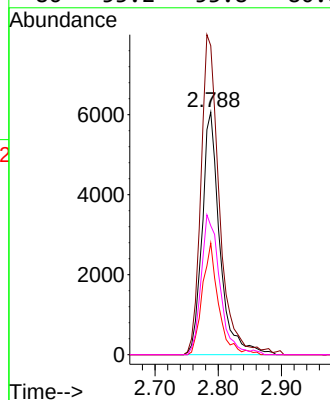

#25
2-Butanone
Concen: 12.105 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.018 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion:	43	Resp:	8059
Ion	Ratio	Lower	Upper
43	100		
72	21.4	18.4	27.6


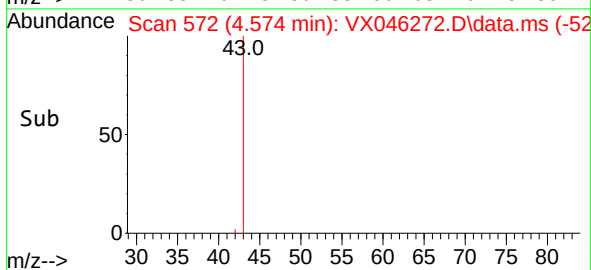
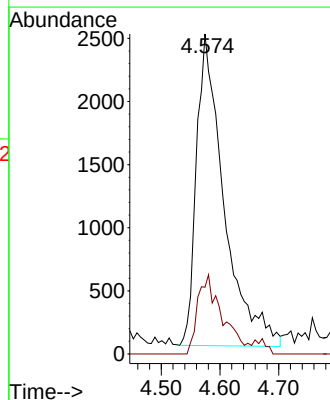





#31
Cyclohexane
Concen: 1.343 ug/l
RT: 5.544 min Scan# 718
Delta R.T. 0.079 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion: 56 Resp: 1831
Ion Ratio Lower Upper
56 100
69 175.3 24.4 36.6#
84 104.3 66.9 100.3#

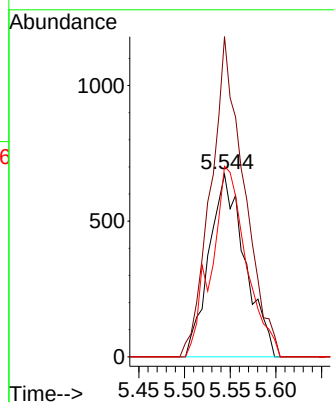

#33
1,2-Dichloroethane-d4
Concen: 52.820 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion: 65 Resp: 60409
Ion Ratio Lower Upper
65 100
67 49.3 0.0 99.0



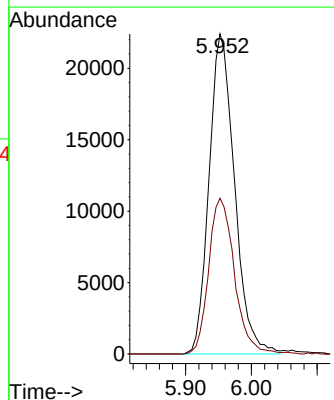
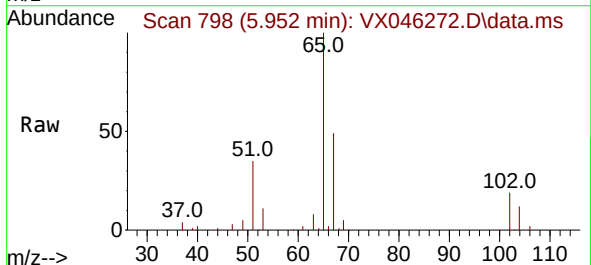




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3


Tgt Ion:114 Resp: 120549
 Ion Ratio Lower Upper
 114 100
 63 24.9 0.0 49.2
 88 16.8 0.0 33.6

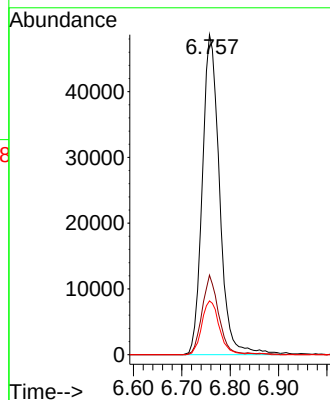

#35
 Dibromofluoromethane
 Concen: 50.719 ug/l
 RT: 5.385 min Scan# 705
 Delta R.T. 0.006 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58

Tgt Ion:113 Resp: 44028
 Ion Ratio Lower Upper
 113 100
 111 102.5 83.1 124.7
 192 16.6 13.3 19.9



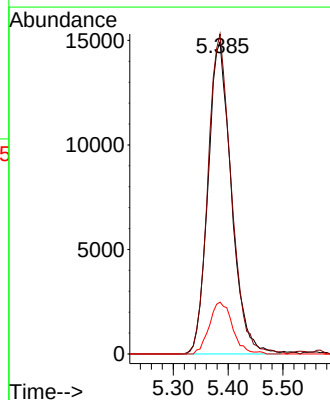





#36
1,1-Dichloropropene
Concen: 5.176 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion: 75 Resp: 6037
Ion Ratio Lower Upper
75 100
110 7.1 16.3 48.9#
77 0.0 24.3 36.5#



#37
Ethyl Acetate
Concen: 0.217 ug/l
RT: 4.757 min Scan# 602
Delta R.T. 0.043 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58


Tgt Ion: 43 Resp: 312
Ion Ratio Lower Upper
43 100
61 0.0 10.3 15.5#
70 0.0 7.9 11.9#

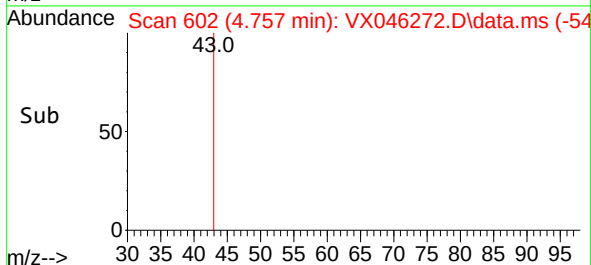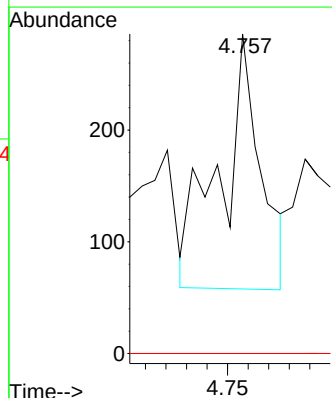






#38
Carbon Tetrachloride
Concen: 5.618 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Instrument :
MSVOA_X
ClientSampleId :
SB-3







Tgt Ion:117 Resp: 7362
Ion Ratio Lower Upper
117 100
119 8.6 75.2 112.8#
121 0.0 24.2 36.4#



#40
Benzene
Concen: 1.682 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion: 78 Resp: 5746
Ion Ratio Lower Upper
78 100
77 27.1 19.0 28.4

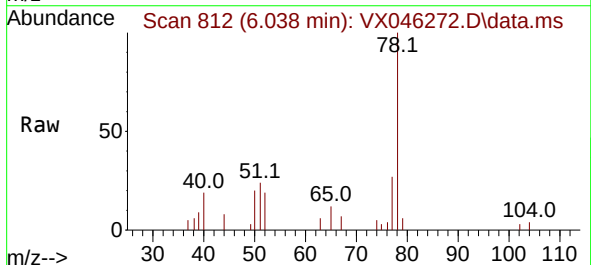



#43

Isopropyl Acetate

Concen: 6.591 ug/l

RT: 6.348 min Scan# 81

Delta R.T. 0.012 min

Lab File: VX046272.D

Acq: 19 May 2025 16:58

Instrument :

MSVOA_X

ClientSampleId :

SB-3





Tgt Ion: 43 Resp: 14490

Ion Ratio Lower Upper

43 100

61 17.6 14.3 21.5

87 11.4 9.5 14.3

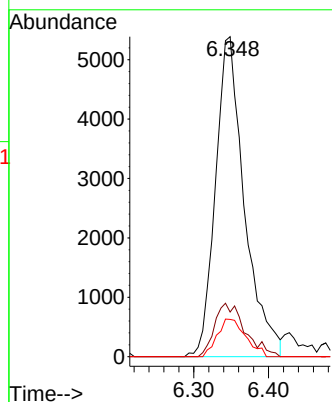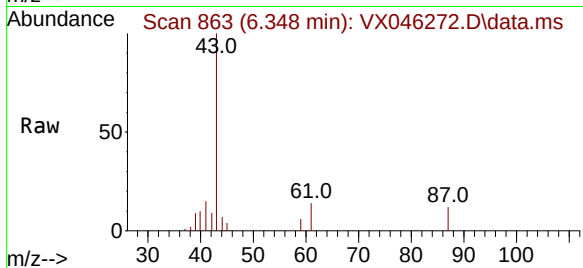

#48

Methyl methacrylate

Concen: 51.975 ug/l

RT: 7.793 min Scan# 1100

Delta R.T. 0.104 min

Lab File: VX046272.D

Acq: 19 May 2025 16:58




Tgt Ion: 41 Resp: 58354


Ion Ratio Lower Upper

41 100

69 0.2 58.5 87.7#

39 56.7 51.7 77.5


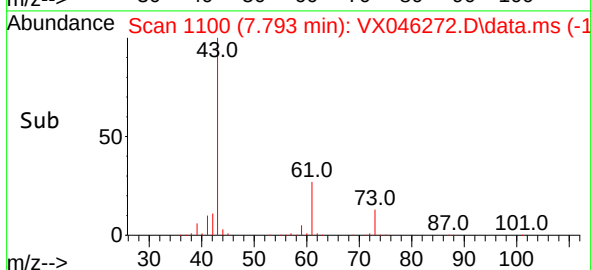

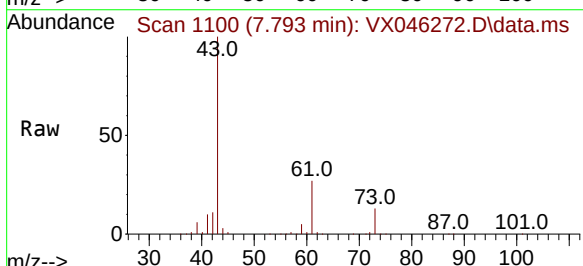




#49
1,4-Dioxane
Concen: 5.864 ug/l
RT: 7.787 min Scan# 1099
Delta R.T. 0.128 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion: 88 Resp: 125
Ion Ratio Lower Upper
88 100
43 461146.4 33.4 50.2#
58 2016.0 58.6 88.0#



#50
Toluene-d8
Concen: 50.908 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion: 98 Resp: 152955
Ion Ratio Lower Upper
98 100
100 64.5 53.5 80.3


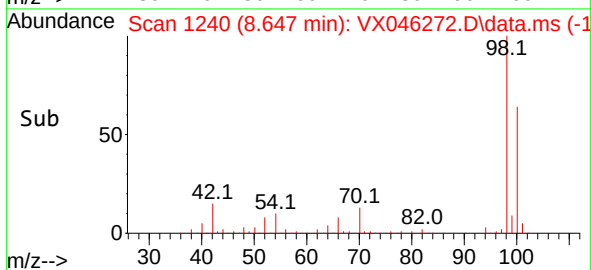






#51
4-Methyl-2-Pentanone
Concen: 31.997 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion: 43 Resp: 46691
Ion Ratio Lower Upper
43 100
58 4.8 28.9 43.3#

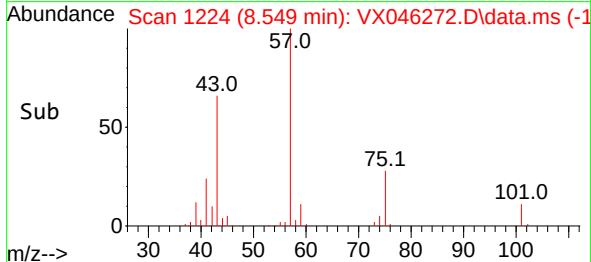

#52
Toluene
Concen: 3.679 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion: 92 Resp: 7707
Ion Ratio Lower Upper
92 100
91 171.7 136.6 205.0


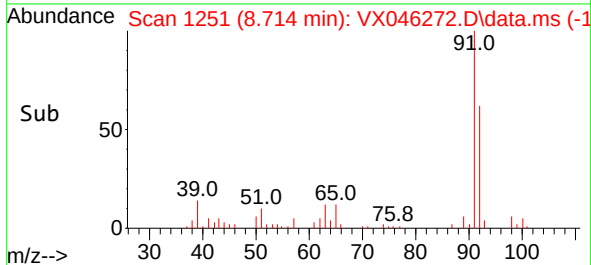




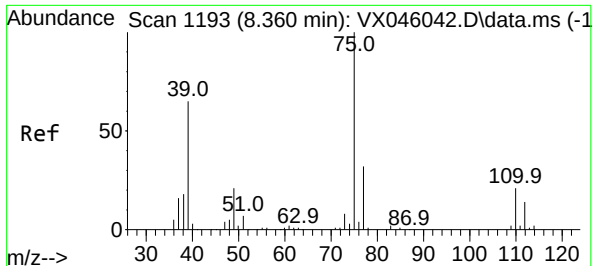

#54
 cis-1,3-Dichloropropene
 Concen: 13.709 ug/l
 RT: 8.549 min Scan# 1193
 Delta R.T. 0.189 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3


Tgt Ion: 75 Resp: 17772
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.4 38.0#
 39 44.4 52.2 78.4#

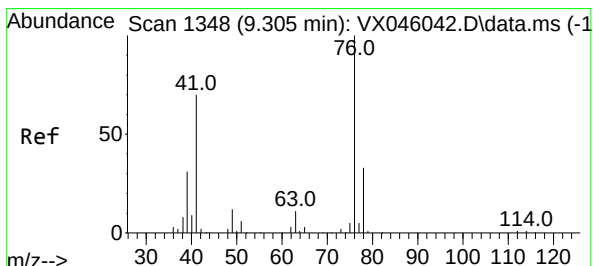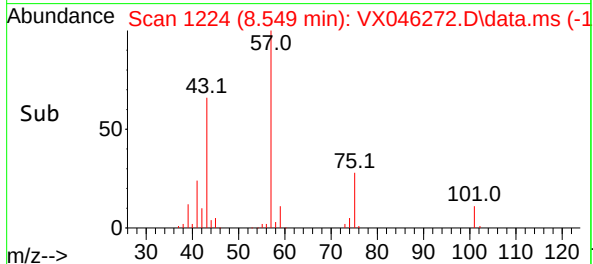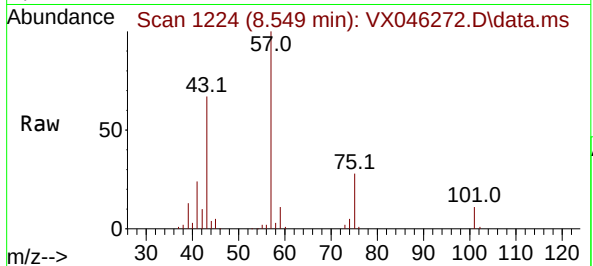

#57
 1,3-Dichloropropane
 Concen: 1.110 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.177 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58

Tgt Ion: 76 Resp: 1647
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.3 39.5#


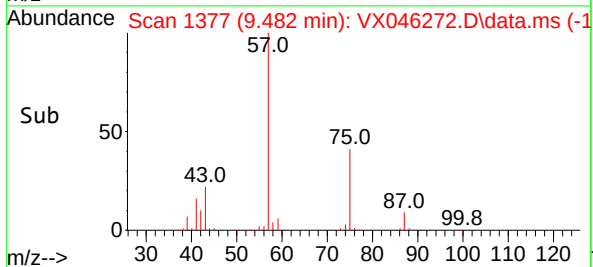

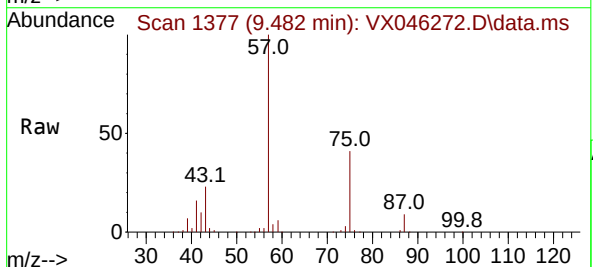




#59
2-Hexanone
Concen: 10.018 ug/l
RT: 9.378 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion: 43 Resp: 10816
Ion Ratio Lower Upper
43 100
58 0.0 24.9 74.6#

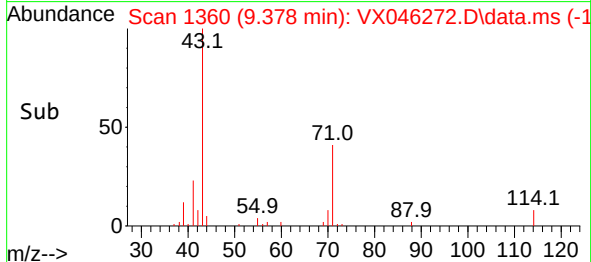

#62
4-Bromofluorobenzene
Concen: 50.756 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion: 95 Resp: 58496
Ion Ratio Lower Upper
95 100
174 66.2 0.0 135.8
176 64.4 0.0 131.4


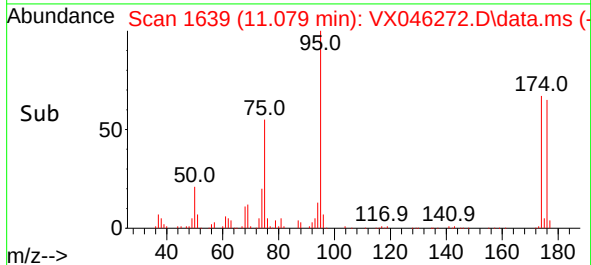






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion:117 Resp: 113135
Ion Ratio Lower Upper
117 100
82 63.2 50.6 76.0
119 31.0 25.8 38.6

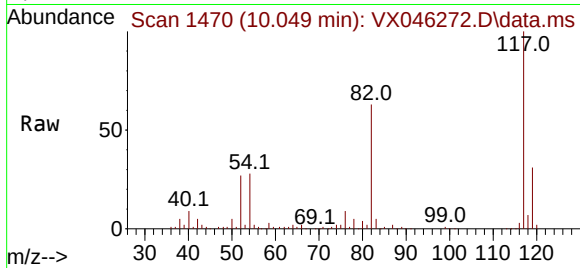

#67
Ethyl Benzene
Concen: 0.498 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion: 91 Resp: 2173
Ion Ratio Lower Upper
91 100
106 33.8 23.4 35.2



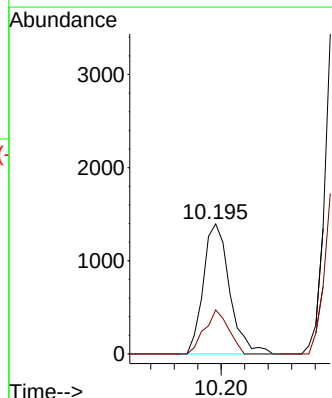
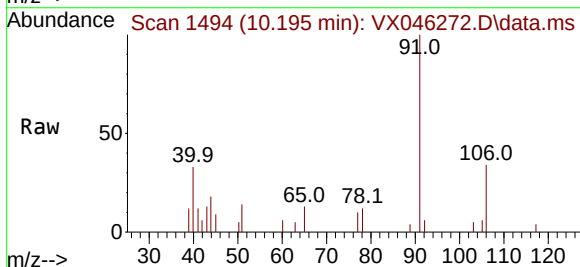




#68
m/p-Xylenes
Concen: 2.011 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58




Instrument :
MSVOA_X
ClientSampleId :
SB-3


Tgt Ion:106 Resp: 3210
Ion Ratio Lower Upper
106 100
91 205.0 171.2 256.8



#69
o-Xylene
Concen: 1.352 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Tgt Ion:106 Resp: 2105
Ion Ratio Lower Upper
106 100
91 219.8 112.7 338.1

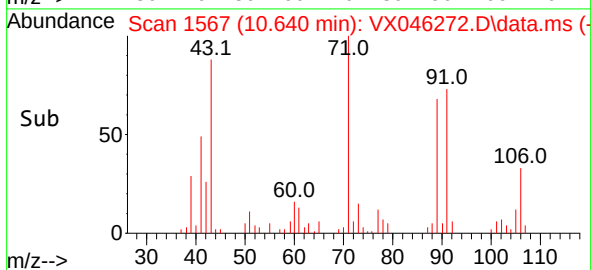



#70

Styrene

Concen: 0.406 ug/l

RT: 10.665 min Scan# 1571

Delta R.T. 0.012 min

Lab File: VX046272.D

Acq: 19 May 2025 16:58





Instrument :

MSVOA_X

ClientSampleId :

SB-3

Tgt Ion:	104	Resp:	1036
Ion Ratio	Lower	Upper	
104	100		
78	0.0	45.7	68.5#
103	53.8	43.7	65.5

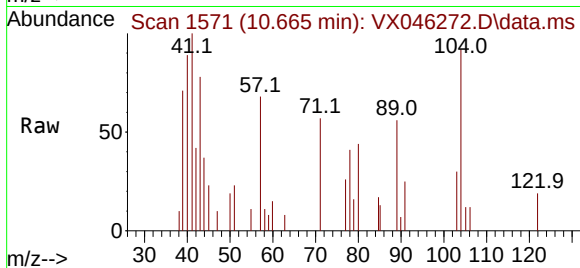

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 12.018 min Scan# 1793


Delta R.T. -0.000 min

Lab File: VX046272.D

Acq: 19 May 2025 16:58

Tgt Ion:	152	Resp:	47691
Ion Ratio	Lower	Upper	
152	100		
115	65.9	46.9	140.7
150	157.5	0.0	351.0

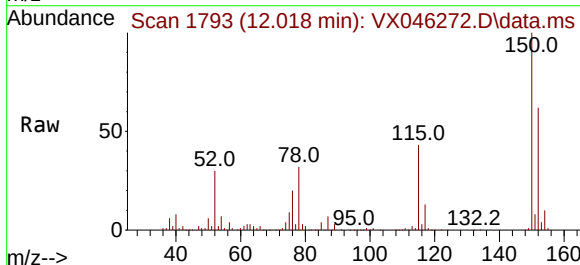

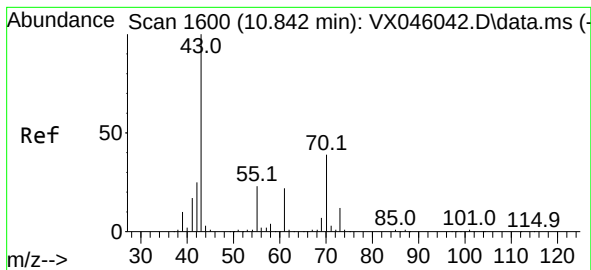

#74

N-amy1 acetate

Concen: 0.324 ug/l

RT: 10.860 min Scan# 1603

Delta R.T. 0.018 min

Lab File: VX046272.D

Acq: 19 May 2025 16:58

Instrument :

MSVOA_X

ClientSampleId :

SB-3

Tgt Ion: 43 Resp: 594





Ion Ratio Lower Upper

43 100

70 72.6 30.9 46.3#

55 79.1 18.7 28.1#

61 0.0 17.1 25.7#

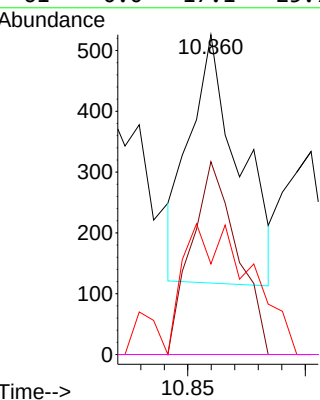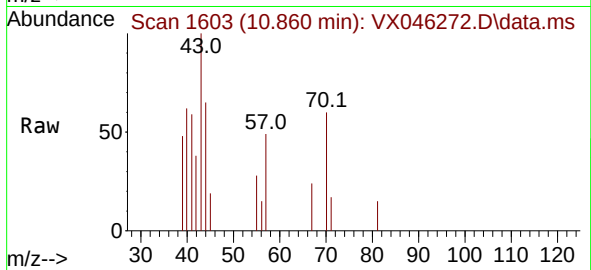

#76

1,2,3-Trichloropropane

Concen: 28.489 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX046272.D




Acq: 19 May 2025 16:58


Tgt Ion: 75 Resp: 32704

Ion Ratio Lower Upper

75 100

77 1.0 20.5 61.5#



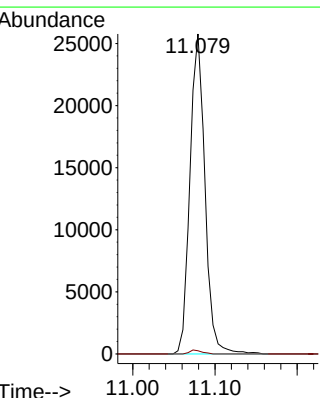





#80
 1,3,5-Trimethylbenzene
 Concen: 0.286 ug/l
 RT: 11.451 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3


Tgt Ion:105 Resp: 888
 Ion Ratio Lower Upper
 105 100
 120 40.5 23.1 69.2

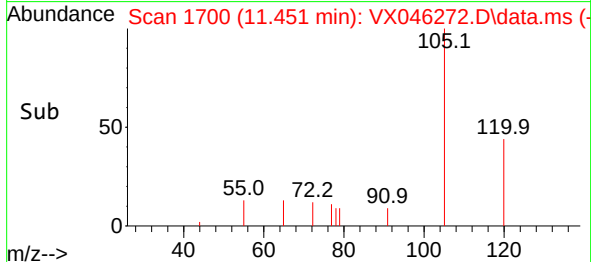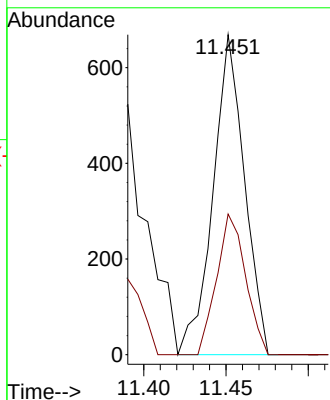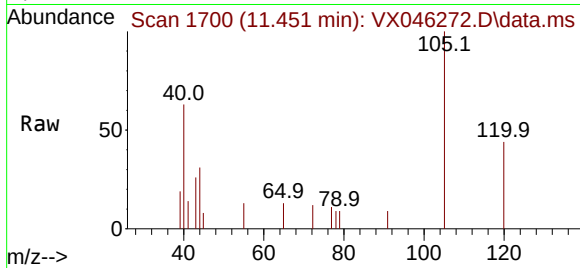

#81
 trans-1,4-Dichloro-2-butene
 Concen: 92.752 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.061 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58

Tgt Ion: 75 Resp: 32704
 Ion Ratio Lower Upper
 75 100
 53 0.0 100.5 150.7#
 89 0.0 37.0 55.6#



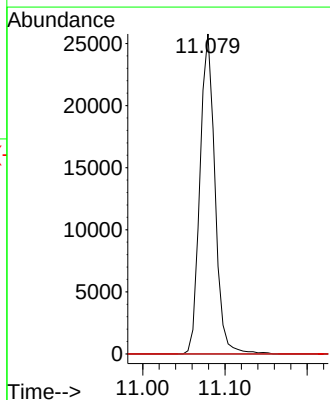
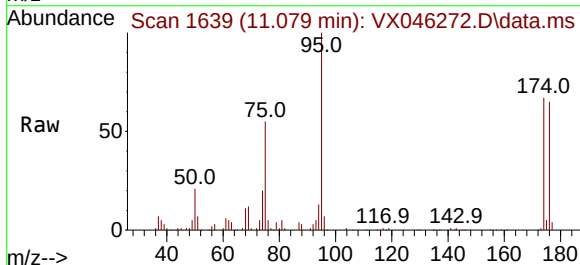




#84
 1,2,4-Trimethylbenzene
 Concen: 1.134 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-3


Tgt Ion:105 Resp: 3561
 Ion Ratio Lower Upper
 105 100
 120 22.0 21.2 63.6

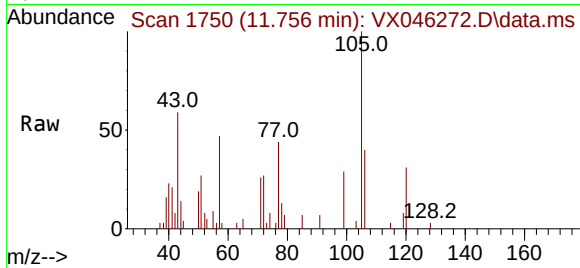

#90
 Hexachloroethane
 Concen: 0.206 ug/l
 RT: 12.603 min Scan# 1889
 Delta R.T. 0.067 min
 Lab File: VX046272.D
 Acq: 19 May 2025 16:58

Tgt Ion:117 Resp: 115
 Ion Ratio Lower Upper
 117 100
 201 0.0 31.6 94.7#

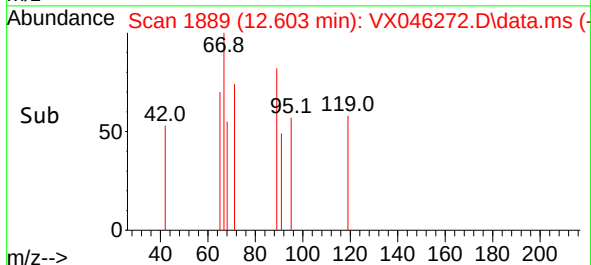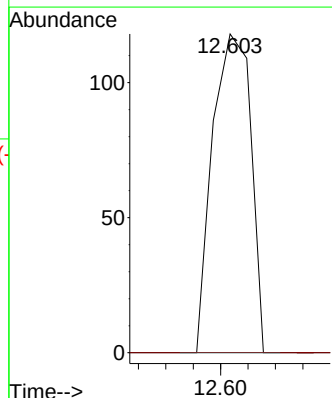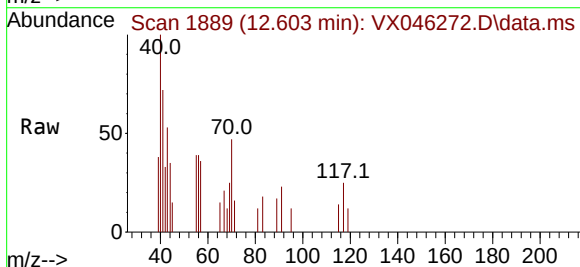



#95
Naphthalene
Concen: 20.118 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX046272.D
Acq: 19 May 2025 16:58

Instrument :
MSVOA_X
ClientSampleId :
SB-3

Tgt Ion	Ratio	Lower	Upper
128	100		
127	12.9	10.4	15.6
129	10.9	8.6	13.0

