

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051925\
 Data File : VX046277.D
 Acq On : 19 May 2025 18:55
 Operator : JC/MD
 Sample : Q2053-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-8

Quant Time: May 19 23:17:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	60568	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	124944	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	115359	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	52441	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	60983	54.006	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 108.020%			
35) Dibromofluoromethane	5.379	113	44996	50.011	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 100.020%			
50) Toluene-d8	8.647	98	154331	49.559	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 99.120%			
62) 4-Bromofluorobenzene	11.079	95	62208	52.078	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 104.160%			
Target Compounds						Qvalue
6) Chloroethane	1.642	64	143	0.320	ug/l #	44
11) Tert butyl alcohol	2.971	59	3655	23.060	ug/l	98
13) Acrolein	2.239	56	408	2.260	ug/l #	54
14) Allyl chloride	2.642	41	322	0.235	ug/l #	44
16) Acetone	2.380	43	35932	79.364	ug/l	99
17) Carbon Disulfide	2.508	76	728	0.428	ug/l #	76
18) Methyl Acetate	2.703	43	3900	3.712	ug/l	96
20) Methylene Chloride	2.788	84	9144	10.539	ug/l	93
25) 2-Butanone	4.568	43	9546	14.523	ug/l #	90
29) Tetrahydrofuran	5.038	42	451	1.095	ug/l #	47
31) Cyclohexane	5.537	56	1970	1.464	ug/l #	39
36) 1,1-Dichloropropene	5.544	75	6228	5.152	ug/l #	51
37) Ethyl Acetate	4.568	43	9442	6.322	ug/l #	70
38) Carbon Tetrachloride	5.550	117	7504	5.525	ug/l #	16
40) Benzene	6.043	78	8717	2.462	ug/l	92
41) Methacrylonitrile	5.038	41	311	0.398	ug/l #	44
43) Isopropyl Acetate	6.348	43	15630	6.860	ug/l	97
48) Methyl methacrylate	7.598	41	2814	2.418	ug/l #	40
51) 4-Methyl-2-Pentanone	8.549	43	46827	30.961	ug/l #	48
52) Toluene	8.720	92	8904	4.101	ug/l	97
54) cis-1,3-Dichloropropene	8.549	75	17735	13.199	ug/l #	59
56) Ethyl methacrylate	9.244	69	281	0.206	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	1740	1.132	ug/l #	42
59) 2-Hexanone	9.372	43	13350	11.931	ug/l #	28
67) Ethyl Benzene	10.195	91	2865	0.644	ug/l	92
68) m/p-Xylenes	10.299	106	4408	2.708	ug/l	96
69) o-Xylene	10.640	106	2899	1.827	ug/l	91
70) Styrene	10.665	104	1805	0.694	ug/l #	85
74) N-amyl acetate	10.860	43	1077	0.534	ug/l #	36
76) 1,2,3-Trichloropropane	11.079	75	34425	27.272	ug/l #	36
80) 1,3,5-Trimethylbenzene	11.457	105	1159	0.340	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	34425	88.789	ug/l #	1
84) 1,2,4-Trimethylbenzene	11.610	105	772	0.224	ug/l	80
95) Naphthalene	13.774	128	72739	19.892	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051925\
Data File : VX046277.D
Acq On : 19 May 2025 18:55
Operator : JC/MD
Sample : Q2053-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-8

Quant Time: May 19 23:17:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051925\
Data File : VX046277.D
Acq On : 19 May 2025 18:55
Operator : JC/MD
Sample : Q2053-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-8

Quant Time: May 19 23:17:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration

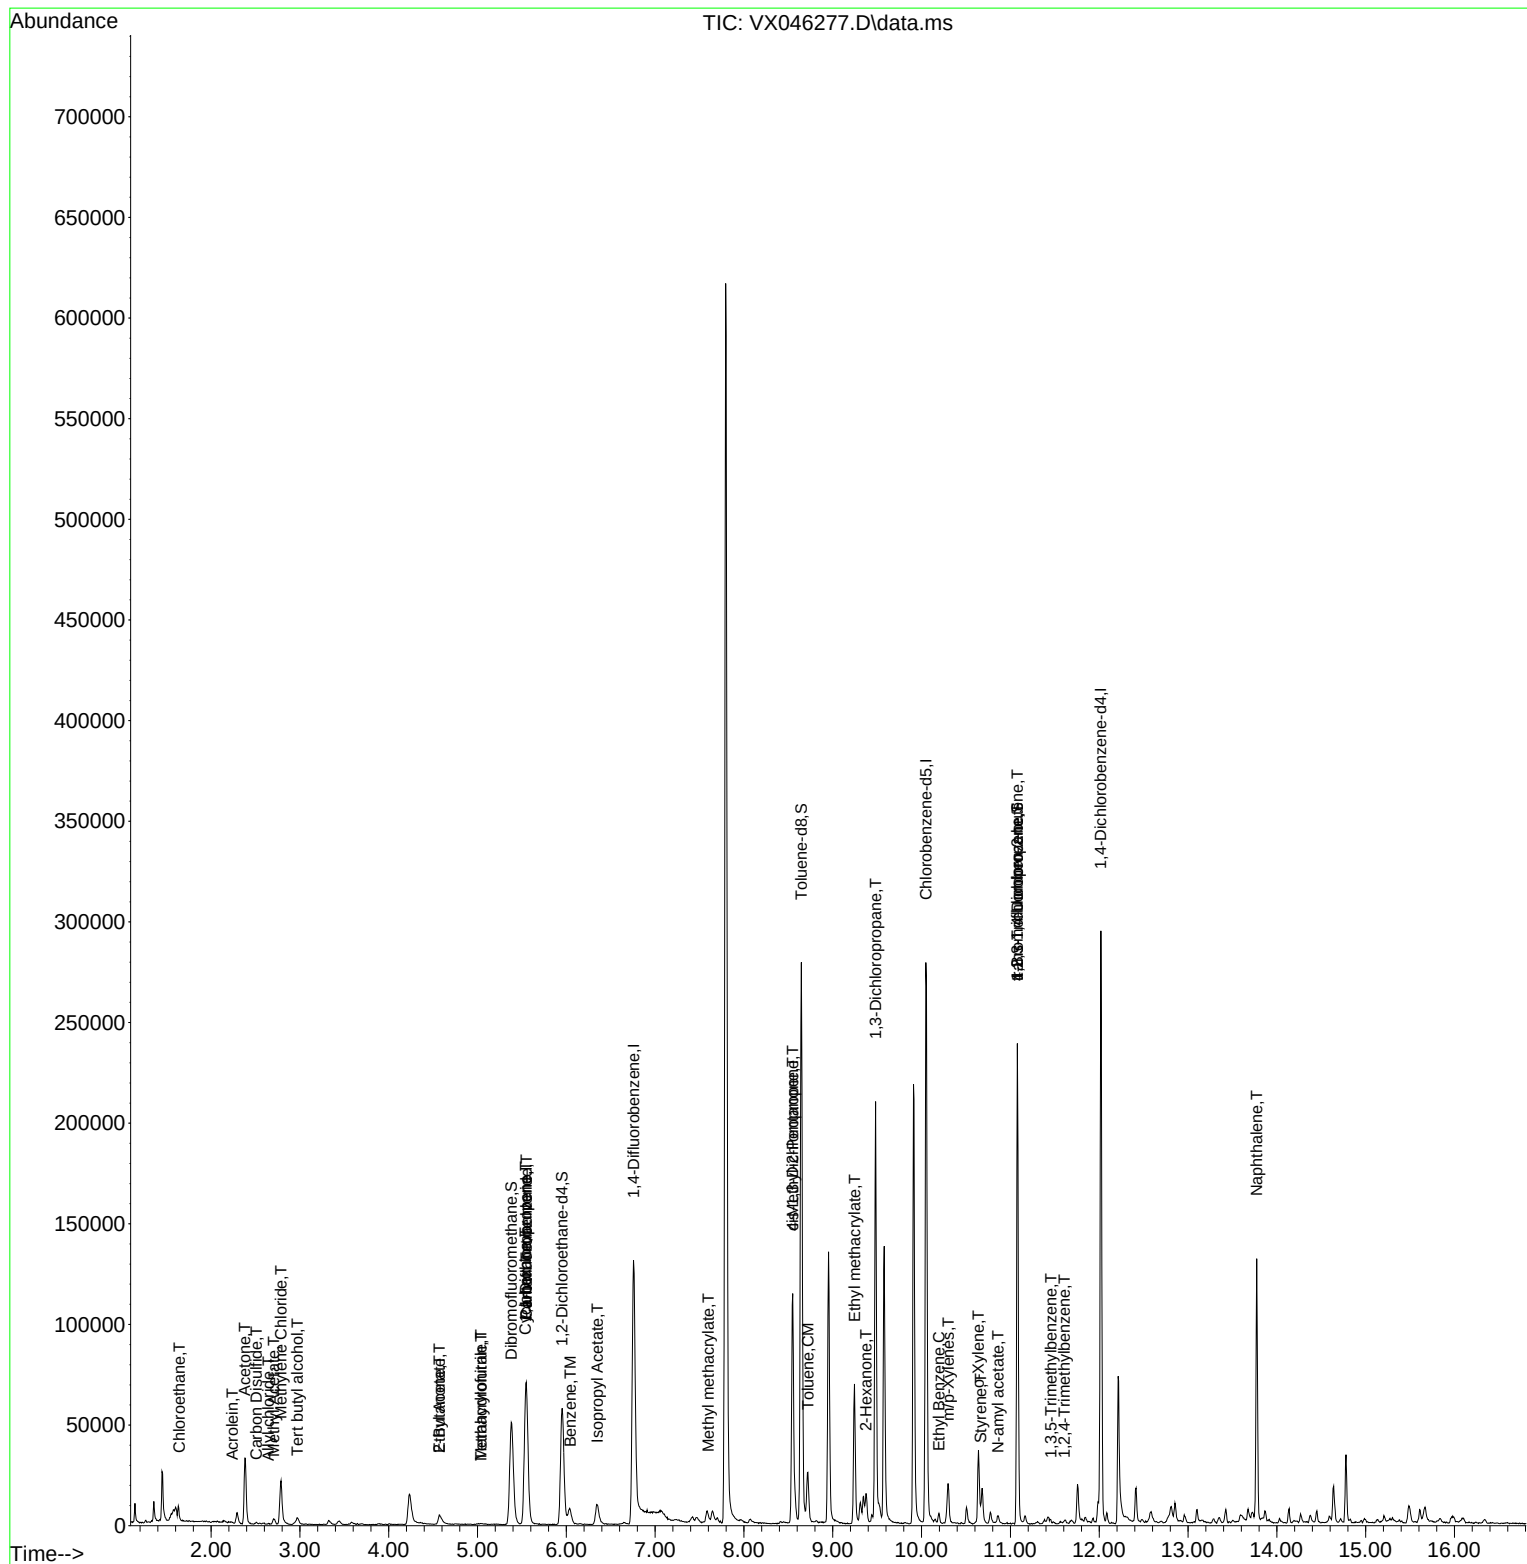



#1
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. 0.006 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55

Instrument :

MSVOA_X

ClientSampleId :





SB-8

Tgt Ion:168 Resp: 60568

Ion Ratio Lower Upper

168 100

99 71.6 54.9 82.3

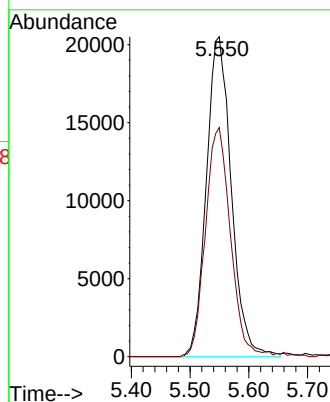

#6

Chloroethane

Concen: 0.320 ug/l

RT: 1.642 min Scan# 91

Delta R.T. -0.025 min

Lab File: VX046277.D




Acq: 19 May 2025 18:55


Tgt Ion: 64 Resp: 143

Ion Ratio Lower Upper

64 100

66 0.0 24.3 36.5#









#11
Tert butyl alcohol
Concen: 23.060 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.006 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 59 Resp: 3655
Ion Ratio Lower Upper
59 100
57 10.0 8.6 12.8

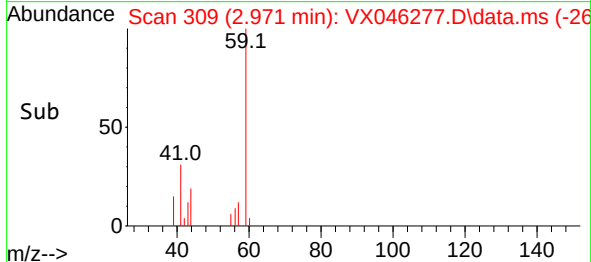

#13
Acrolein
Concen: 2.260 ug/l
RT: 2.239 min Scan# 189
Delta R.T. 0.006 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 56 Resp: 408
Ion Ratio Lower Upper
56 100
55 108.3 56.2 84.4#




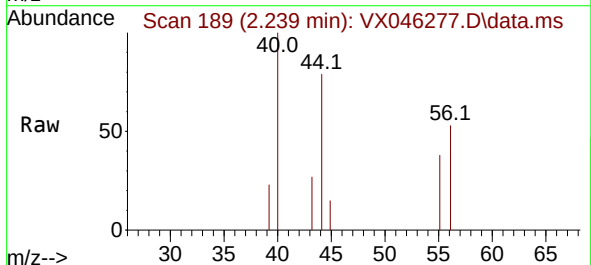




#14
 Allyl chloride
 Concen: 0.235 ug/l
 RT: 2.642 min Scan# 212
 Delta R.T. -0.012 min
 Lab File: VX046277.D
 Acq: 19 May 2025 18:55




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-8


Tgt Ion: 41 Resp: 322
 Ion Ratio Lower Upper
 41 100
 39 28.0 60.6 90.8#
 76 0.0 24.9 37.3#

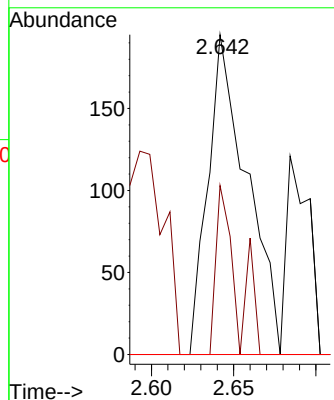

#16
 Acetone
 Concen: 79.364 ug/l
 RT: 2.380 min Scan# 212
 Delta R.T. -0.006 min
 Lab File: VX046277.D
 Acq: 19 May 2025 18:55

Tgt Ion: 43 Resp: 35932
 Ion Ratio Lower Upper
 43 100
 58 26.8 21.2 31.8



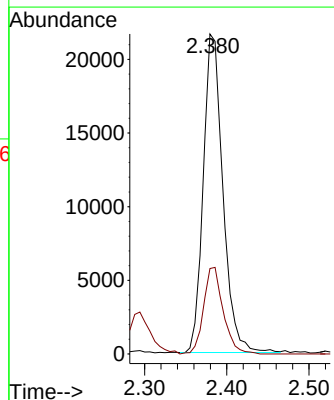





#17
Carbon Disulfide
Concen: 0.428 ug/l
RT: 2.508 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 76 Resp: 728
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#

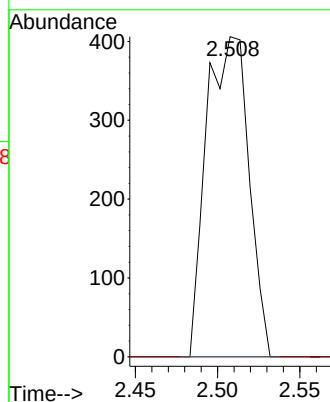

#18
Methyl Acetate
Concen: 3.712 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 43 Resp: 3900
Ion Ratio Lower Upper
43 100
74 19.0 16.7 25.1



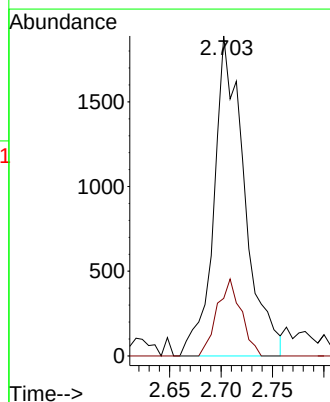





#20
Methylene Chloride
Concen: 10.539 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion:	84	Resp:	9144
Ion	Ratio	Lower	Upper
84	100		
49	130.4	113.9	170.9
51	38.9	33.5	50.3
86	64.8	53.8	80.8



#25
2-Butanone
Concen: 14.523 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.012 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion:	43	Resp:	9546
Ion	Ratio	Lower	Upper
43	100		
72	27.9	18.4	27.6#









#29
Tetrahydrofuran
Concen: 1.095 ug/l
RT: 5.038 min Scan# 642
Delta R.T. 0.036 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 42 Resp: 451
Ion Ratio Lower Upper
42 100
72 15.7 33.7 50.5#
71 0.0 31.4 47.2#



#31
Cyclohexane
Concen: 1.464 ug/l
RT: 5.537 min Scan# 730
Delta R.T. 0.073 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 56 Resp: 1970
Ion Ratio Lower Upper
56 100
69 138.3 24.4 36.6#
84 93.8 66.9 100.3





#33

1,2-Dichloroethane-d4

Concen: 54.006 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55

Instrument :

MSVOA_X

ClientSampleId :





SB-8

Tgt Ion: 65 Resp: 60983

Ion Ratio Lower Upper

65 100

67 49.8 0.0 99.0

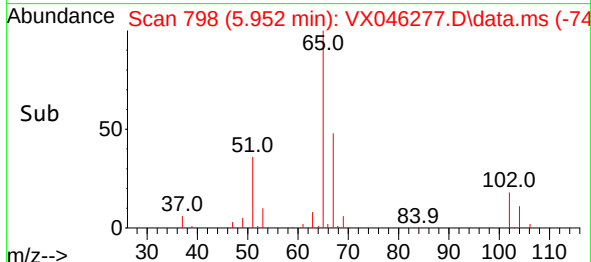

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55




Tgt Ion: 114 Resp: 124944


Ion Ratio Lower Upper

114 100

63 24.8 0.0 49.2

88 17.0 0.0 33.6









#35
Dibromofluoromethane
Concen: 50.011 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion:	113	Resp:	44996
Ion	Ratio	Lower	Upper
113	100		
111	101.6	83.1	124.7
192	16.7	13.3	19.9

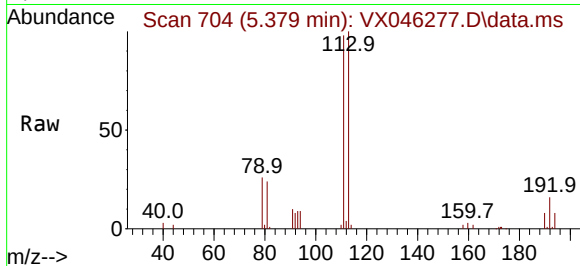

#36
1,1-Dichloropropene
Concen: 5.152 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.140 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion:	75	Resp:	6228
Ion	Ratio	Lower	Upper
75	100		
110	8.6	16.3	48.9#
77	0.0	24.3	36.5#

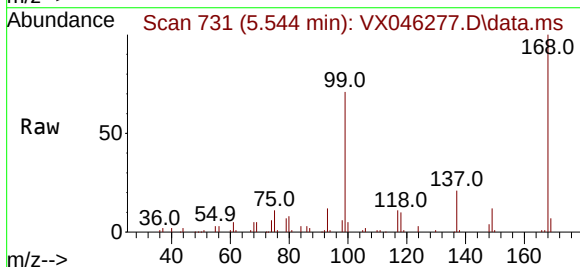



#37

Ethyl Acetate

Concen: 6.322 ug/l

RT: 4.568 min Scan# 51

Delta R.T. -0.146 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55

Instrument :

MSVOA_X

ClientSampleId :

SB-8





Tgt Ion: 43 Resp: 9442

Ion Ratio Lower Upper

43 100

61 0.0 10.3 15.5#

70 0.0 7.9 11.9#



#38

Carbon Tetrachloride

Concen: 5.525 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.122 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55




Tgt Ion: 117 Resp: 7504


Ion Ratio Lower Upper

117 100

119 4.1 75.2 112.8#

121 0.0 24.2 36.4#

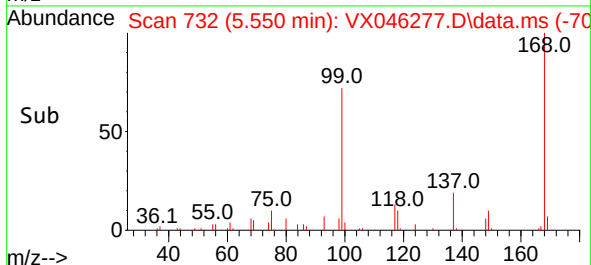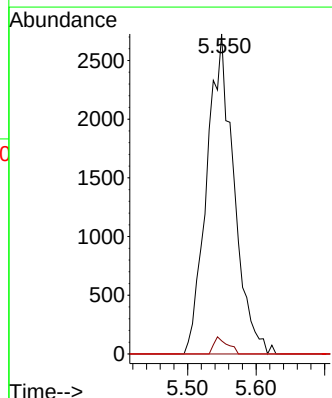



#40

Benzene

Concen: 2.462 ug/l

RT: 6.043 min Scan# 811

Delta R.T. 0.012 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55

Instrument :

MSVOA_X

ClientSampleId :





SB-8

Tgt Ion: 78 Resp: 8717

Ion Ratio Lower Upper

78 100

77 19.7 19.0 28.4

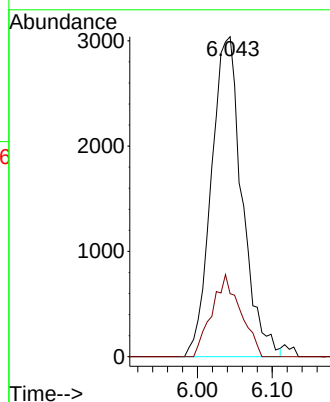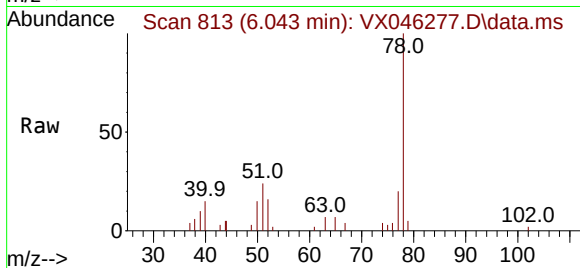

#41

Methacrylonitrile

Concen: 0.398 ug/l

RT: 5.038 min Scan# 648

Delta R.T. 0.122 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55

Tgt Ion: 41 Resp: 311




Ion Ratio Lower Upper


41 100

39 37.0 47.2 70.8#

67 0.0 50.7 76.1#

52 0.0 24.6 37.0#


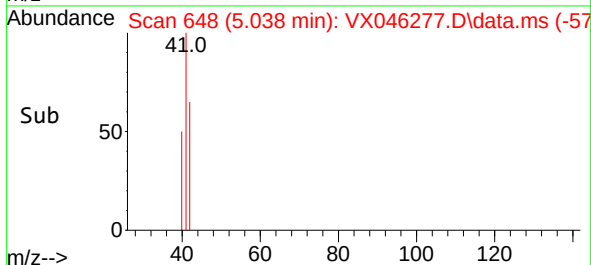
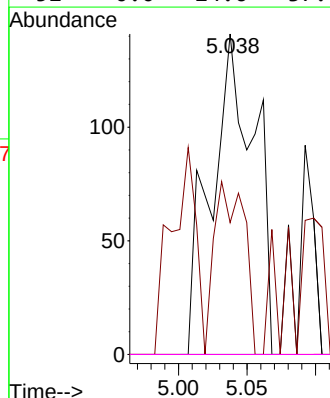
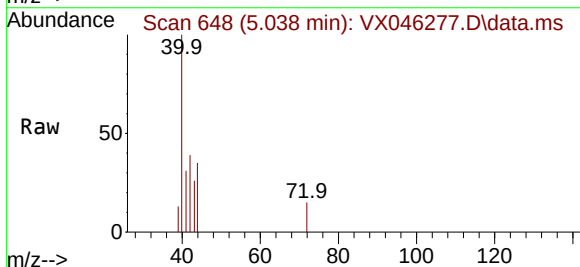




#43
Isopropyl Acetate
Concen: 6.860 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.012 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 43 Resp: 15630
Ion Ratio Lower Upper
43 100
61 17.4 14.3 21.5
87 10.1 9.5 14.3



#48
Methyl methacrylate
Concen: 2.418 ug/l
RT: 7.598 min Scan# 1068
Delta R.T. -0.092 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 41 Resp: 2814
Ion Ratio Lower Upper
41 100
69 0.0 58.5 87.7#
39 41.4 51.7 77.5#









#50
Toluene-d8
Concen: 49.559 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 98 Resp: 154331
Ion Ratio Lower Upper
98 100
100 66.5 53.5 80.3



#51
4-Methyl-2-Pentanone
Concen: 30.961 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.025 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 43 Resp: 46827
Ion Ratio Lower Upper
43 100
58 5.3 28.9 43.3#







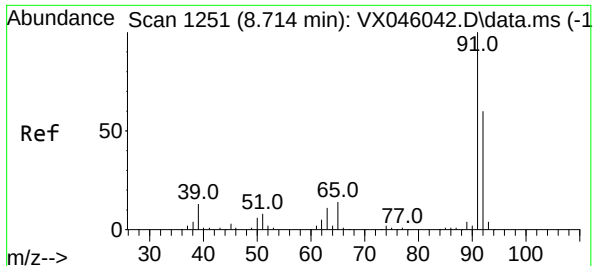

#52
Toluene
Concen: 4.101 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 92 Resp: 8904
Ion Ratio Lower Upper
92 100
91 174.9 136.6 205.0

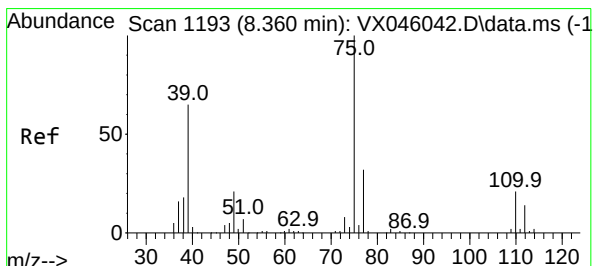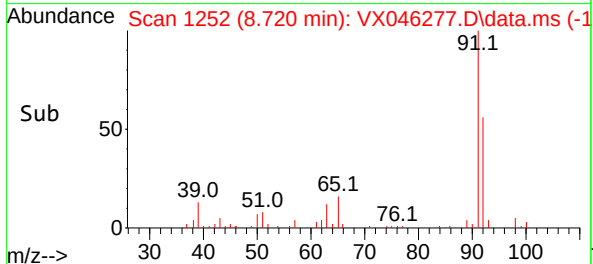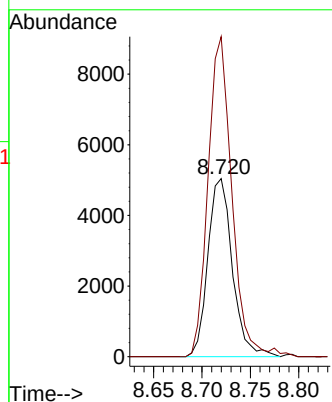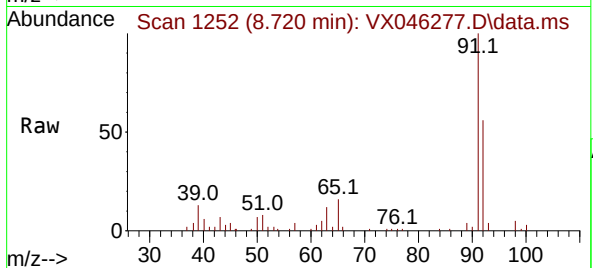

#54
cis-1,3-Dichloropropene
Concen: 13.199 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. 0.189 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 75 Resp: 17735
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#
39 38.6 52.2 78.4#

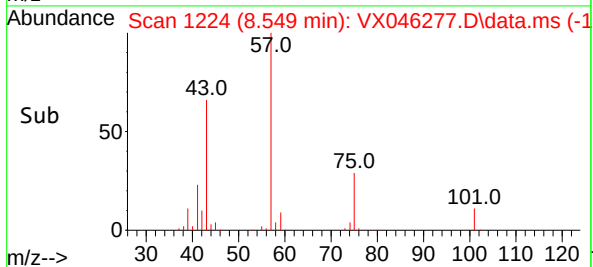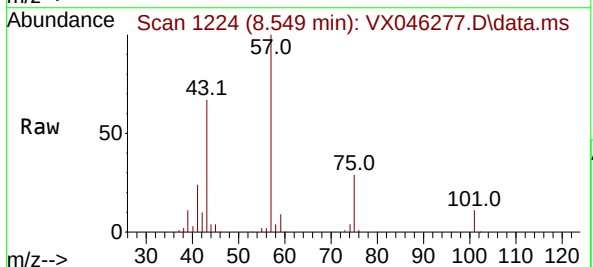

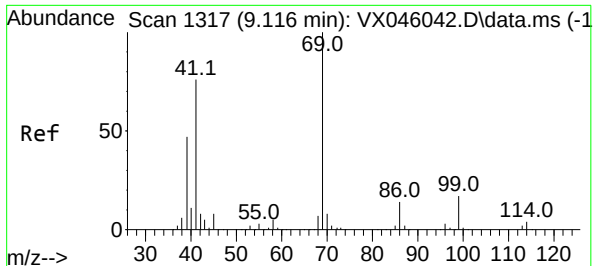

#56

Ethyl methacrylate

Concen: 0.206 ug/l

RT: 9.244 min Scan# 1338

Delta R.T. 0.128 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55





Instrument :

MSVOA_X

ClientSampleId :

SB-8

Tgt Ion:	69	Resp:	281
Ion	Ratio	Lower	Upper
69	100		
41	4399.3	60.8	91.2#
39	2085.8	39.0	58.6#

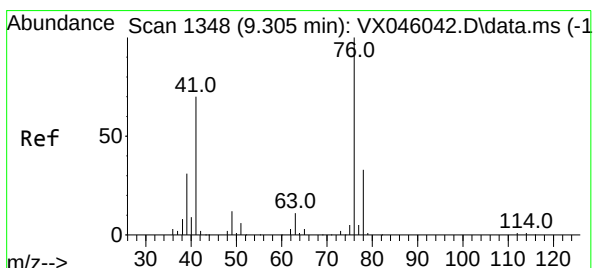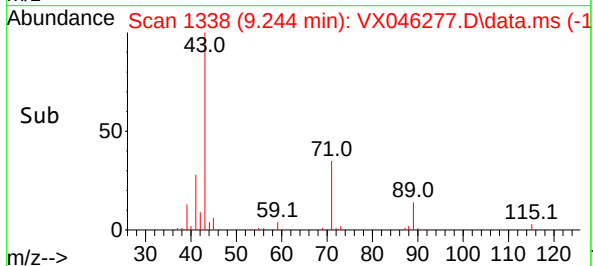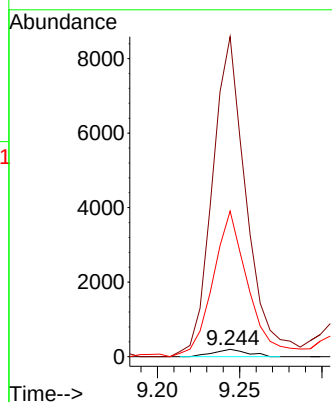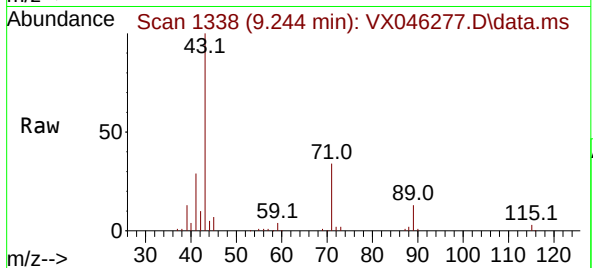

#57

1,3-Dichloropropane

Concen: 1.132 ug/l




RT: 9.482 min Scan# 1377


Delta R.T. 0.177 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55

Tgt Ion:	76	Resp:	1740
Ion	Ratio	Lower	Upper
76	100		
78	0.0	26.3	39.5#


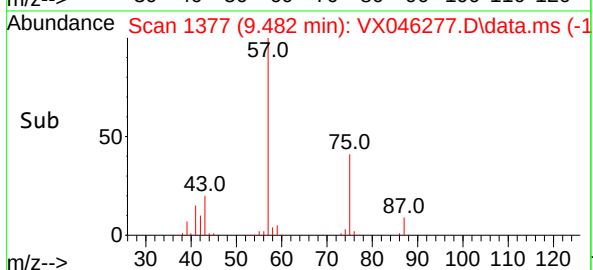

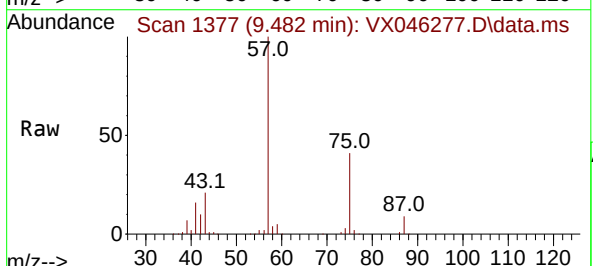




#59
2-Hexanone
Concen: 11.931 ug/l
RT: 9.372 min Scan# 11
Delta R.T. -0.055 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 43 Resp: 13350
Ion Ratio Lower Upper
43 100
58 0.0 24.9 74.6#



#62
4-Bromofluorobenzene
Concen: 52.078 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 95 Resp: 62208
Ion Ratio Lower Upper
95 100
174 66.0 0.0 135.8
176 62.3 0.0 131.4









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion:117 Resp: 115359
Ion Ratio Lower Upper
117 100
82 63.5 50.6 76.0
119 32.8 25.8 38.6

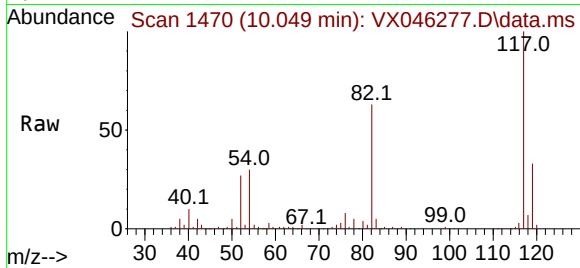

#67
Ethyl Benzene
Concen: 0.644 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 91 Resp: 2865
Ion Ratio Lower Upper
91 100
106 33.8 23.4 35.2




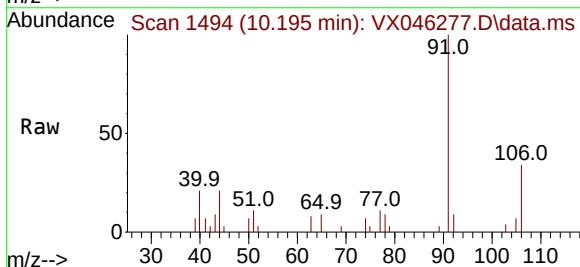




#68
m/p-Xylenes
Concen: 2.708 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion:106 Resp: 4408
Ion Ratio Lower Upper
106 100
91 207.0 171.2 256.8



#69
o-Xylene
Concen: 1.827 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion:106 Resp: 2899
Ion Ratio Lower Upper
106 100
91 240.7 112.7 338.1





#70

Styrene

Concen: 0.694 ug/l

RT: 10.665 min Scan# 1571

Delta R.T. 0.012 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55

Instrument :

MSVOA_X

ClientSampleId :

SB-8





Tgt Ion:104 Resp: 1805

Ion Ratio Lower Upper

104 100

78 74.5 45.7 68.5#

103 59.6 43.7 65.5

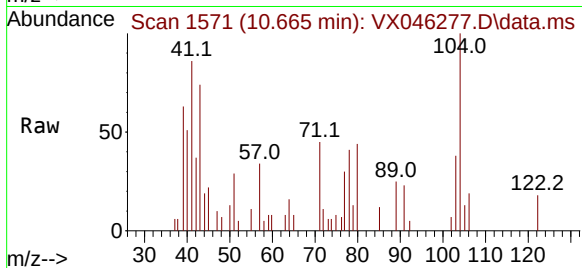

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VX046277.D

Acq: 19 May 2025 18:55




Tgt Ion:152 Resp: 52441


Ion Ratio Lower Upper

152 100

115 65.8 46.9 140.7

150 162.4 0.0 351.0




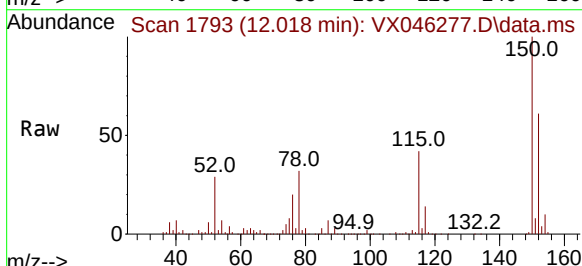




#74
N-amy1 acetate
Concen: 0.534 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.018 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion: 43 Resp: 1077
Ion Ratio Lower Upper
43 100
70 69.9 30.9 46.3#
55 72.4 18.7 28.1#
61 0.0 17.1 25.7#



#76
1,2,3-Trichloropropane
Concen: 27.272 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 75 Resp: 34425
Ion Ratio Lower Upper
75 100
77 1.0 20.5 61.5#









#80
1,3,5-Trimethylbenzene
Concen: 0.340 ug/l
RT: 11.457 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55




Instrument :
MSVOA_X
ClientSampleId :
SB-8


Tgt Ion:105 Resp: 1159
Ion Ratio Lower Upper
105 100
120 45.0 23.1 69.2

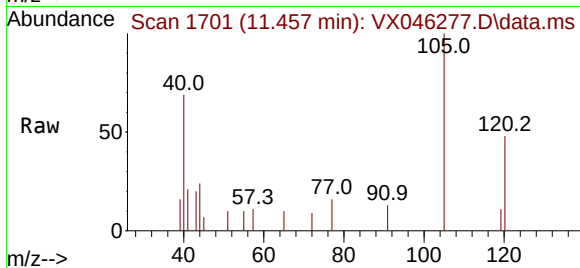

#81
trans-1,4-Dichloro-2-butene
Concen: 88.789 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046277.D
Acq: 19 May 2025 18:55

Tgt Ion: 75 Resp: 34425
Ion Ratio Lower Upper
75 100
53 0.0 100.5 150.7#
89 0.0 37.0 55.6#




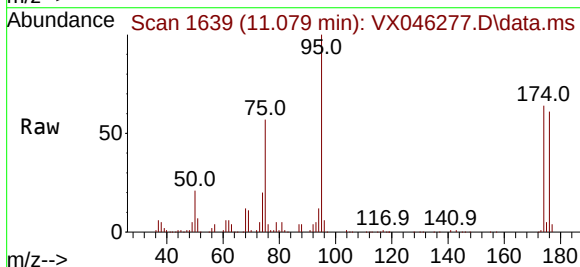




#84
 1,2,4-Trimethylbenzene
 Concen: 0.224 ug/l
 RT: 11.610 min Scan# 1726
 Delta R.T. -0.140 min
 Lab File: VX046277.D
 Acq: 19 May 2025 18:55

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-8

Tgt Ion:105 Resp: 772
 Ion Ratio Lower Upper
 105 100
 120 29.4 21.2 63.6

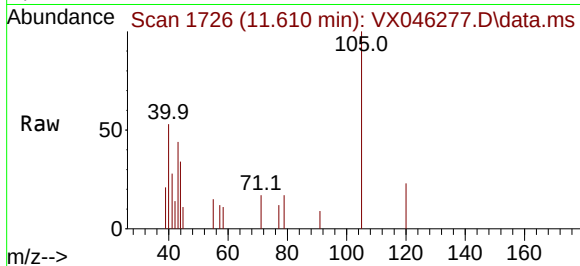

#95
 Naphthalene
 Concen: 19.892 ug/l
 RT: 13.774 min Scan# 2081
 Delta R.T. -0.000 min
 Lab File: VX046277.D
 Acq: 19 May 2025 18:55

Tgt Ion:128 Resp: 72739
 Ion Ratio Lower Upper
 128 100
 127 12.9 10.4 15.6
 129 11.2 8.6 13.0

